



US00D955245S

(12) **United States Design Patent**
Barton et al.

(10) **Patent No.:** **US D955,245 S**

(45) **Date of Patent:** **** *Jun. 21, 2022**

(54) **DIAGNOSTIC ANALYZER**

(71) Applicant: **Abbott Laboratories**, Abbott Park, IL (US)

(72) Inventors: **Christina A. Barton**, Irving, TX (US); **Sherry Sue Eckholm**, Sun Prairie, WI (US); **Vladlena Belozero**, Philadelphia, PA (US); **Ami Marie Verhalen**, Sun Prairie, WI (US); **Jesse Charles Darley**, Madison, WI (US)

(73) Assignee: **ABBOTT LABORATORIES**, Abbott Park, IL (US)

(*) Notice: This patent is subject to a terminal disclaimer.

(**) Term: **15 Years**

(21) Appl. No.: **29/716,123**

(22) Filed: **Dec. 6, 2019**

Related U.S. Application Data

(63) Continuation of application No. 29/622,464, filed on Oct. 17, 2017, now Pat. No. Des. 869,309, which is a continuation of application No. 29/549,335, filed on Dec. 21, 2015, now Pat. No. Des. 800,000, which is a continuation-in-part of application No. 29/531,578, filed on Jun. 26, 2015, now Pat. No. Des. 777,049.

(51) **LOC (13) Cl.** **10-04**

(52) **U.S. Cl.**
USPC **D10/81; D24/216**

(58) **Field of Classification Search**
USPC D10/81; D24/216, 219, 220, 232, 233, D24/234

CPC G01N 21/00; G01N 21/01; G01N 2021/0106; G01N 2201/022; G01N 2201/0221; G01N 2201/0222; G01N 2201/0224; G01N 2201/0225; G01N 2201/0227; G01N 2201/0228; G01N 2201/024; G01N 2201/0245; G01N 2021/0112-21/958

See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

D662,431 S * 6/2012 Kimura D10/81
D724,753 S * 3/2015 Gutmann D24/216
(Continued)

OTHER PUBLICATIONS

Japanese Patent Office, "Directive," issued in connection with Japanese Patent Application No. 2016-19292, dated Mar. 7, 2017, 5 pages.

(Continued)

Primary Examiner — Antoine Duval Davis

(74) *Attorney, Agent, or Firm* — McAndrews Held & Malloy, Ltd.

(57) **CLAIM**

The ornamental design for a diagnostic analyzer, as shown and described.


DESCRIPTION

The file of this patent contains at least one drawing/photograph executed in color. Copies of this patent with color drawings(s)/photograph(s) will be provided by the Office upon request and payment of the necessary fee.

FIG. 1 is a front left perspective view of a diagnostic analyzer showing our new design;
FIG. 2 is a front elevation view thereof;
FIG. 3 is a rear elevation view thereof;
FIG. 4 is a right side elevation view thereof;
FIG. 5 is a left side elevation view thereof;
FIG. 6 is a top plan view thereof; and,
FIG. 7 is a bottom plan view thereof.

The portions of the diagnostic analyzer shown in broken lines in the drawings form no part of the claimed design.

1 Claim, 6 Drawing Sheets
(2 of 6 Drawing Sheet(s) Filed in Color)

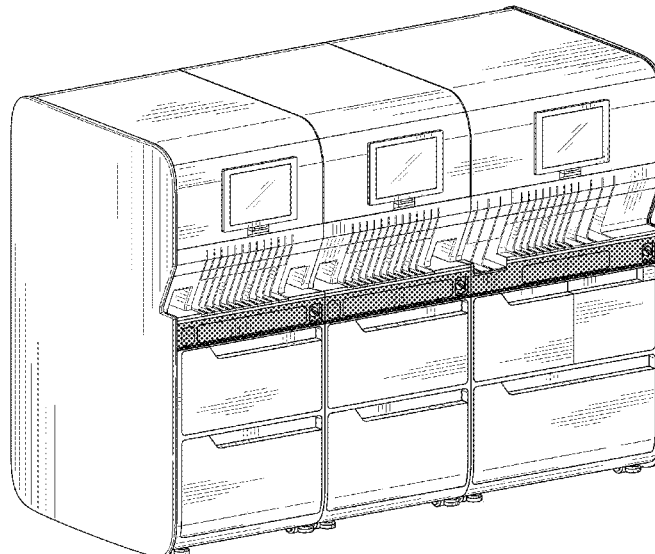

(56)

References Cited

U.S. PATENT DOCUMENTS

D773,071	S	11/2016	Hakoda	
D777,049	S	1/2017	Barton et al.	
D788,617	S	6/2017	Barton et al.	
D799,999	S	10/2017	Barton et al.	
D800,000	S	10/2017	Barton et al.	
D802,156	S *	11/2017	Barton	D24/216
D802,785	S	11/2017	Barton et al.	
9,997,266	B2	6/2018	Zhang et al.	
D824,536	S	7/2018	Barton et al.	
D825,776	S	8/2018	Quick et al.	
D828,575	S	9/2018	Ohno	
D830,210	S	10/2018	Ihara	
D838,613	S	1/2019	Barton et al.	
D840,048	S	2/2019	Barton et al.	
10,220,387	B2	3/2019	Granier et al.	

OTHER PUBLICATIONS

Japanese Patent Office, "Notice of Reason for Rejection," issued in connection with Japanese Design Application No. 2016-19293, dated Nov. 8, 2016, 3 pages.

Japanese Patent Office, "Notice of Reason for Rejection," issued in connection with Japanese Design Application No. 2016-19292, dated Nov. 8, 2016, 3 pages.

Japanese Patent Office, "Notice of Reason for Rejection," issued in connection with Japanese Design Application No. 2016-19291, dated Nov. 8, 2016, 3 pages.

State Intellectual Property Office of China, "Notice of Grant of Patent Right," issued in connection with Chinese Patent Application No. 201530555258.3, dated Oct. 20, 2016, 5 pages.

Japanese Patent Office, "Notice of Reason for Rejection," issued in connection with Japanese Design Application No. 2015-28872 dated Jun. 14, 2016, 5 pages.

Office for Harmonization in The Internal Market, "Notification of the Registration of the Community Designs," issued in connection with European Community Design Nos. 002930230-0001 through 002930230-0029, dated Mar. 17, 2016, 6 pages.

United States Patent and Trademark Office, "Notice of Allowance and Fee(s) Due," issued in connection with U.S. Appl. No. 29/531,578, dated Sep. 8, 2016, 14 pages.

United States Patent and Trademark Office, "Restriction and/or Election Requirement," issued in connection with U.S. Appl. No. 29/531,578, dated Jul. 6, 2016, 14 pages.

* cited by examiner

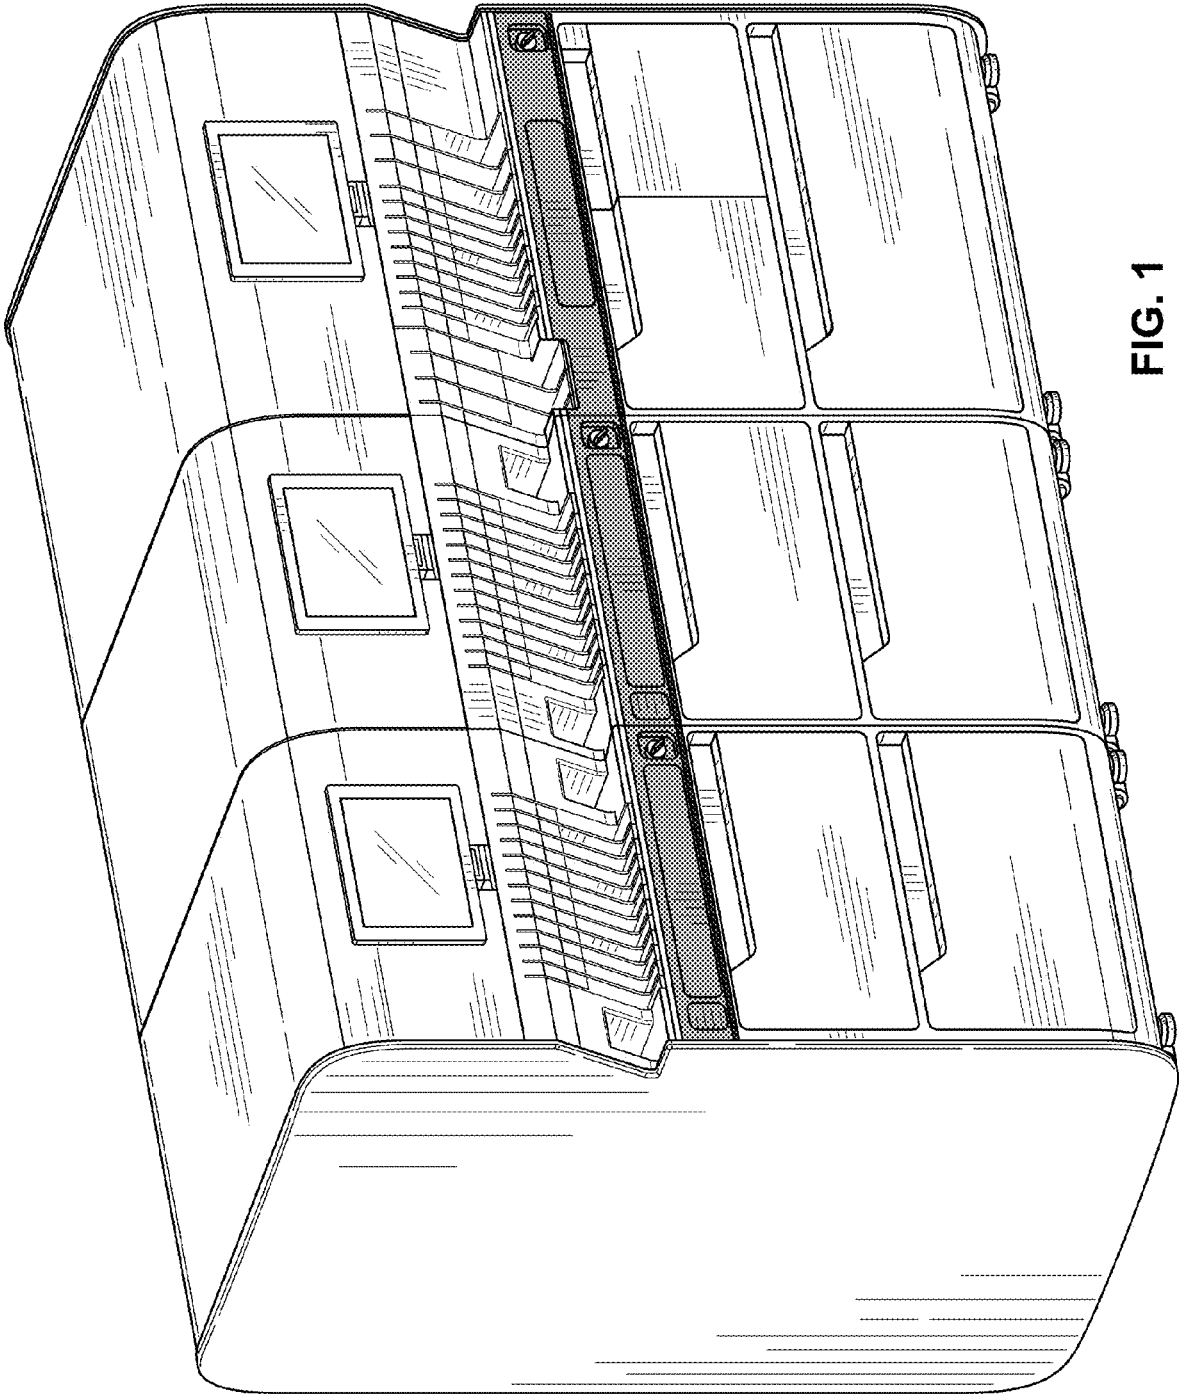


FIG. 1

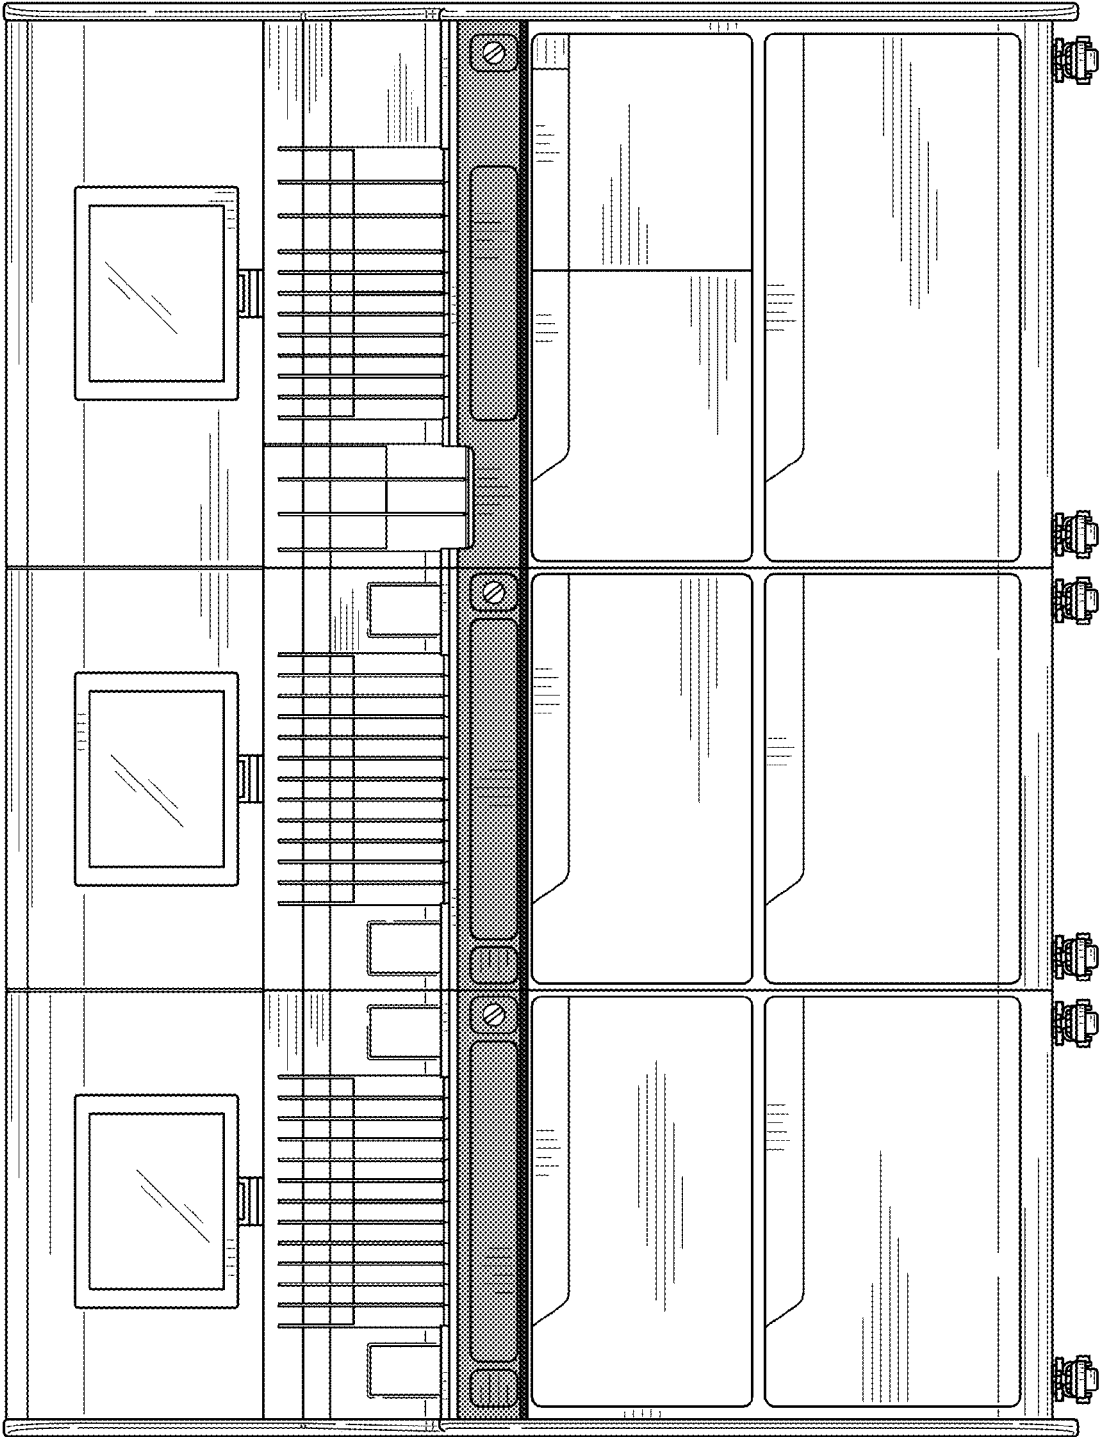


FIG. 2

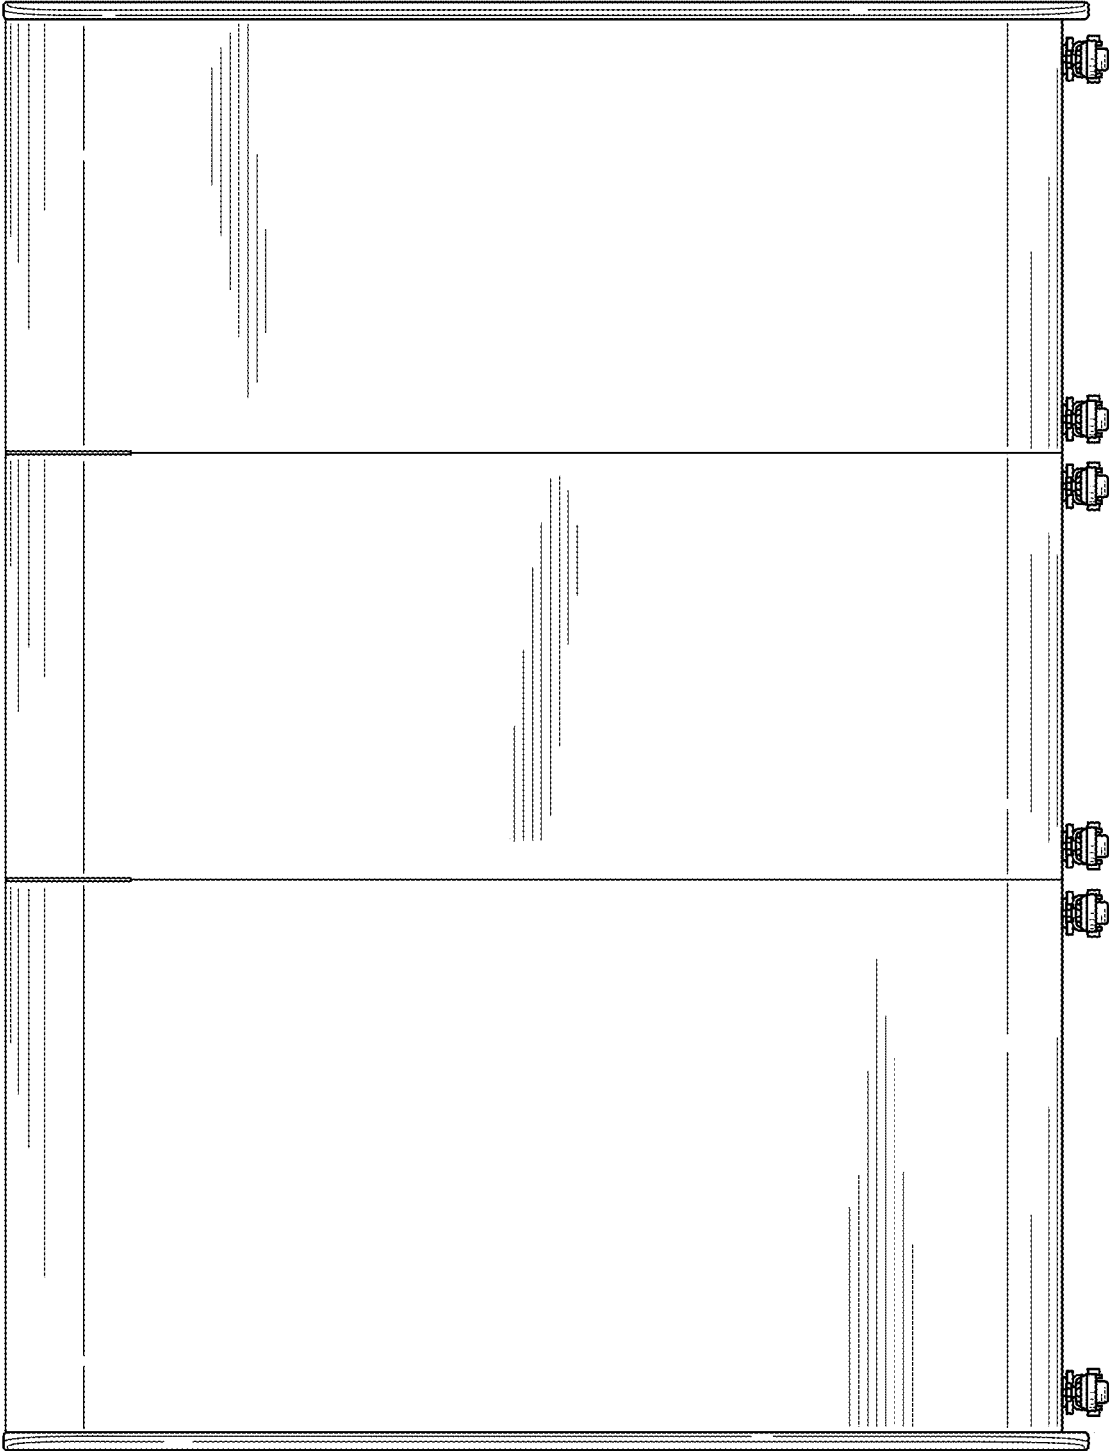


FIG. 3

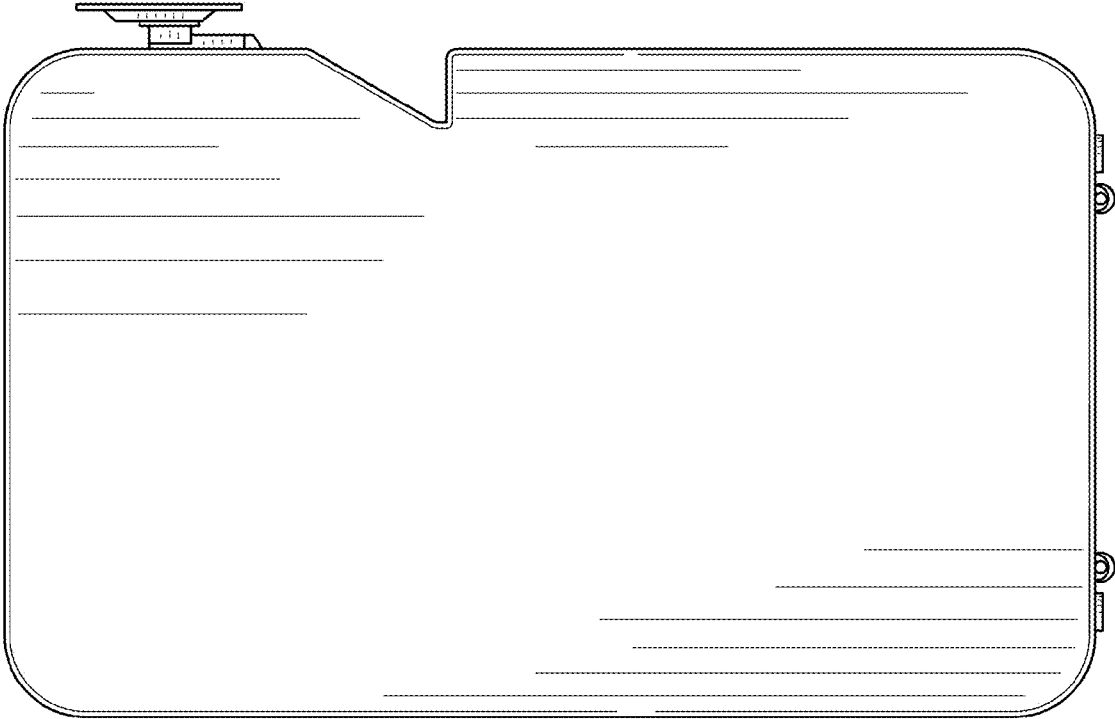


FIG. 5

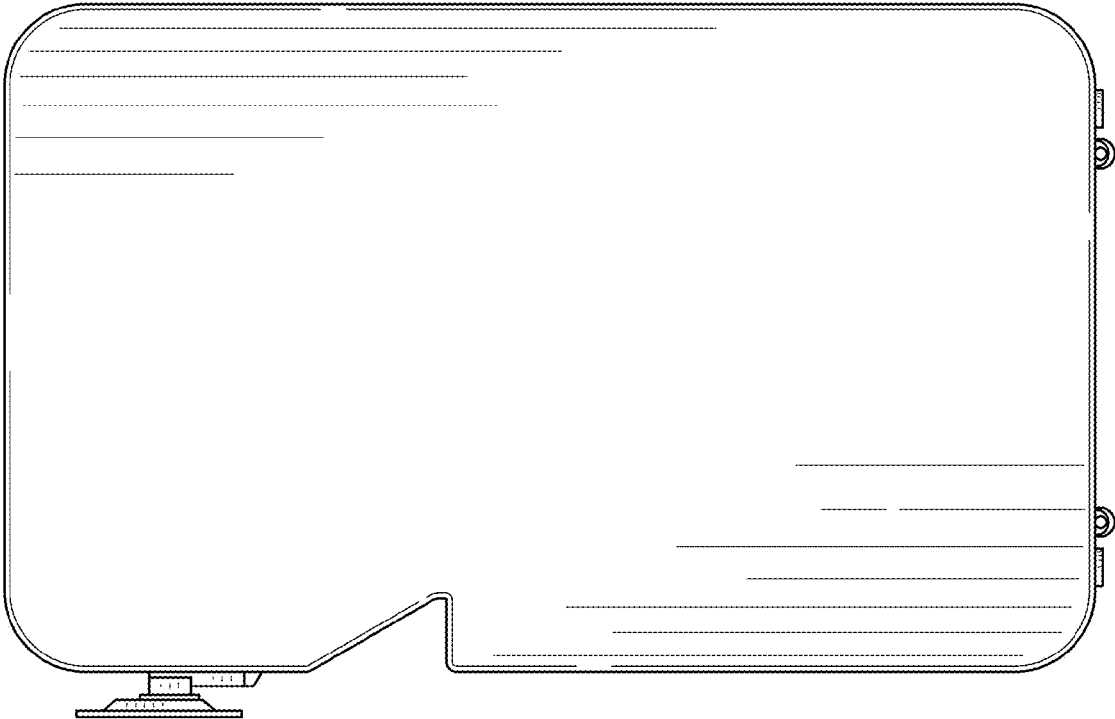


FIG. 4

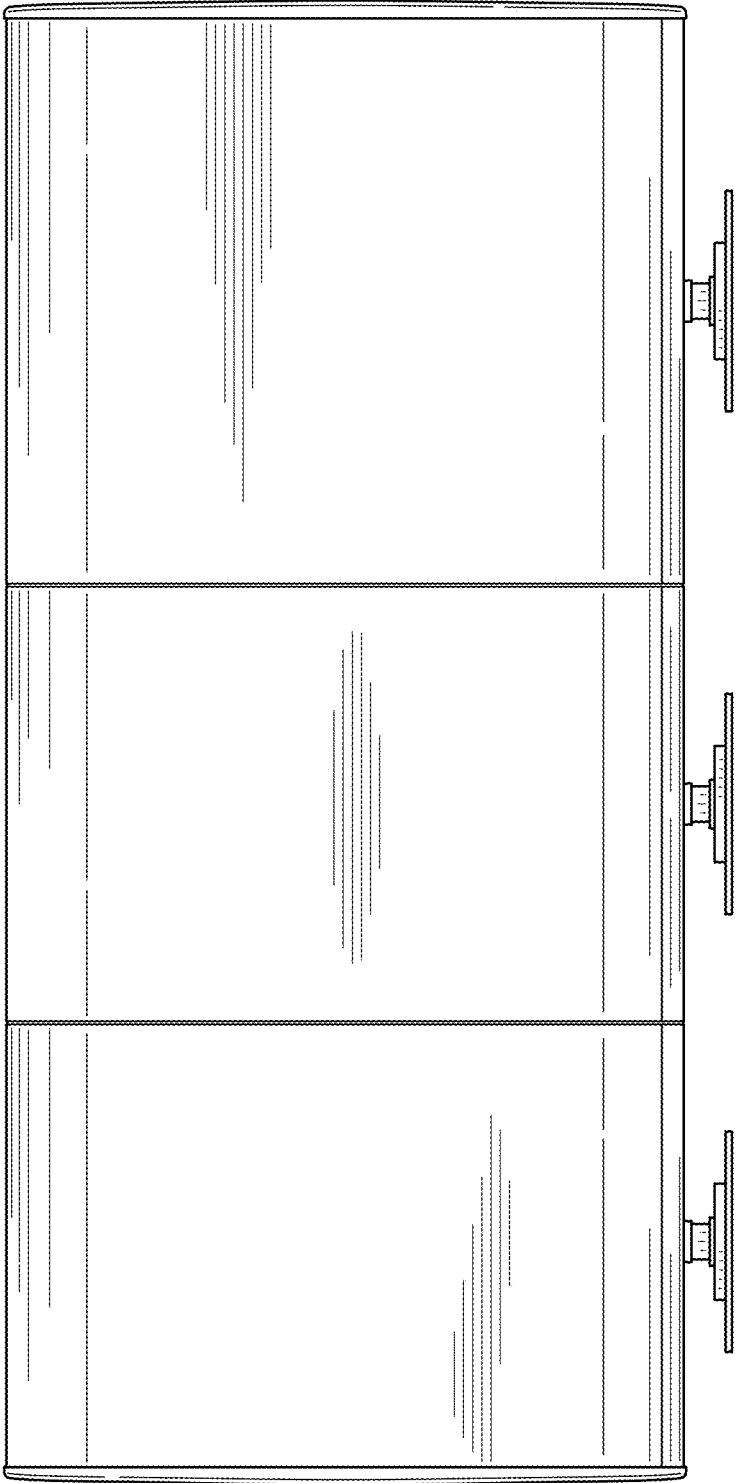


FIG. 6

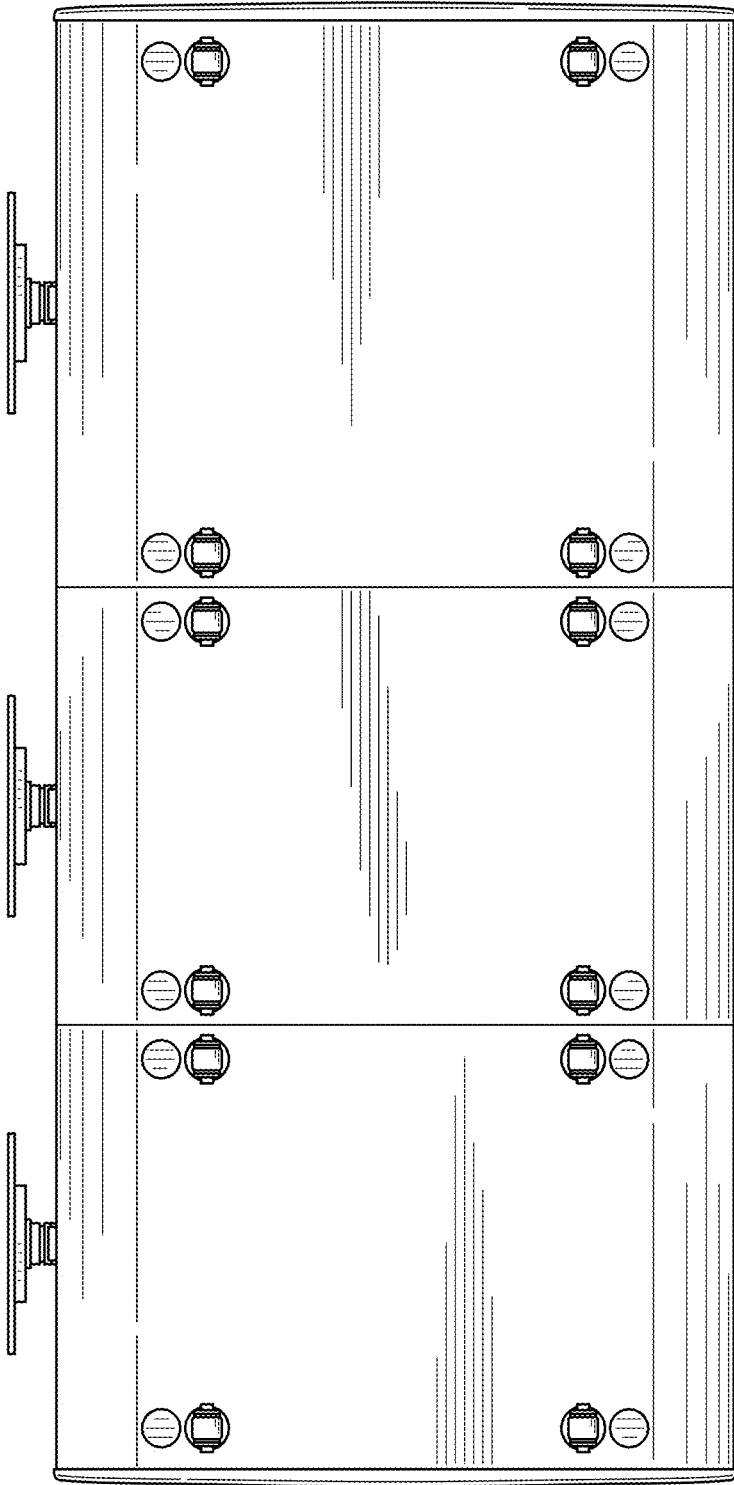


FIG. 7