



INTERNATIONAL APPLICATION PUBLISHED UNDER THE PATENT COOPERATION TREATY (PCT)

(51) International Patent Classification ⁶ : A61F 2/00, 2/06	A2	(11) International Publication Number: WO 98/27893 (43) International Publication Date: 2 July 1998 (02.07.98)
(21) International Application Number: PCT/US97/21640 (22) International Filing Date: 9 December 1997 (09.12.97) (30) Priority Data: 08/772,372 23 December 1996 (23.12.96) US (71) Applicant: PROGRAFT MEDICAL, INC. [US/US]; 2500 Faber Place, Palo Alto, CA 94303 (US). (72) Inventors: THORNTON, Troy; 130A South Park, San Francisco, CA 94107 (US). CHAN, Randy, S.; 1623 Parkview Green Circle, San Jose, CA 95131 (US). LAU, Lilip; 4500 Faber Place, Palo Alto, CA 94303 (US). (74) Agents: MARCUS, Michael, S. et al.; Morgan & Finnegan, L.L.P., 345 Park Avenue, New York, NY 10154-0053 (US).		(81) Designated States: AL, AM, AT, AU, AZ, BA, BB, BG, BR, BY, CA, CH, CN, CU, CZ, DE, DK, EE, ES, FI, GB, GE, GH, HU, IL, IS, JP, KE, KG, KP, KR, KZ, LC, LK, LR, LS, LT, LU, LV, MD, MG, MK, MN, MW, MX, NO, NZ, PL, PT, RO, RU, SD, SE, SG, SI, SK, SL, TJ, TM, TR, TT, UA, UG, UZ, VN, YU, ZW, ARIPO patent (GH, GM, KE, LS, MW, SD, SZ, UG, ZW), Eurasian patent (AM, AZ, BY, KG, KZ, MD, RU, TJ, TM), European patent (AT, BE, CH, DE, DK, ES, FI, FR, GB, GR, IE, IT, LU, MC, NL, PT, SE), OAPI patent (BF, BJ, CF, CG, CI, CM, GA, GN, ML, MR, NE, SN, TD, TG). Published <i>Without international search report and to be republished upon receipt of that report.</i>
(54) Title: KINK RESISTANT BIFURCATED PROSTHESIS		
(57) Abstract The invention relates to an endoluminal prosthesis adapted for placement at a bifurcation site within the body. The stent or stent-graft may be constructed to have segments of differing structural properties. A section of the stent-graft may be constructed to have a single-lumen tubular stent member covering a multilumen graft member. The stent-graft may comprise at least two modular components adapted for in situ assembly. An extended cylindrical interference fit may be used to seal the modular components.		

FOR THE PURPOSES OF INFORMATION ONLY

Codes used to identify States party to the PCT on the front pages of pamphlets publishing international applications under the PCT.

AL	Albania	ES	Spain	LS	Lesotho	SI	Slovenia
AM	Armenia	FI	Finland	LT	Lithuania	SK	Slovakia
AT	Austria	FR	France	LU	Luxembourg	SN	Senegal
AU	Australia	GA	Gabon	LV	Latvia	SZ	Swaziland
AZ	Azerbaijan	GB	United Kingdom	MC	Monaco	TD	Chad
BA	Bosnia and Herzegovina	GE	Georgia	MD	Republic of Moldova	TG	Togo
BB	Barbados	GH	Ghana	MG	Madagascar	TJ	Tajikistan
BE	Belgium	GN	Guinea	MK	The former Yugoslav Republic of Macedonia	TM	Turkmenistan
BF	Burkina Faso	GR	Greece			TR	Turkey
BG	Bulgaria	HU	Hungary	ML	Mali	TT	Trinidad and Tobago
BJ	Benin	IE	Ireland	MN	Mongolia	UA	Ukraine
BR	Brazil	IL	Israel	MR	Mauritania	UG	Uganda
BY	Belarus	IS	Iceland	MW	Malawi	US	United States of America
CA	Canada	IT	Italy	MX	Mexico	UZ	Uzbekistan
CF	Central African Republic	JP	Japan	NE	Niger	VN	Viet Nam
CG	Congo	KE	Kenya	NL	Netherlands	YU	Yugoslavia
CH	Switzerland	KG	Kyrgyzstan	NO	Norway	ZW	Zimbabwe
CI	Côte d'Ivoire	KP	Democratic People's Republic of Korea	NZ	New Zealand		
CM	Cameroon	KR	Republic of Korea	PL	Poland		
CN	China	KZ	Kazakstan	PT	Portugal		
CU	Cuba	LC	Saint Lucia	RO	Romania		
CZ	Czech Republic	LI	Liechtenstein	RU	Russian Federation		
DE	Germany	LK	Sri Lanka	SD	Sudan		
DK	Denmark	LR	Liberia	SE	Sweden		
EE	Estonia			SG	Singapore		

KINK RESISTANT BIFURCATED PROSTHESIS

5

TECHNICAL FIELD

This invention relates generally to implants for repairing ducts and passageways in a body. More specifically this invention relates to an implant adapted for delivery to and repair of a bifurcation site within the body. In one aspect, this invention involves a modular, kink-resistant, bifurcated stent-graft device.

10

BACKGROUND ART

Treatment or isolation of vascular aneurysms or of vessel walls which have been thickened by disease has traditionally been performed via surgical bypassing with vascular grafts. Shortcomings of this invasive procedure include the morbidity and mortality associated with major surgery, long patient recovery times, and the high incidence of repeat intervention needed due to limitations of the graft or of the procedure.

15

20

Minimally invasive alternatives involving stents or stent-grafts are generally known and widely used in certain types of treatments. Intraluminal stents, for example, are particularly useful for treatment of vascular or arterial occlusion or stenosis typically associated with vessels thickened by disease. Intraluminal stents function to mechanically hold these vessels open. In some instances, stents may be used subsequent to or as an adjunct to a balloon angioplasty procedure.

25

30

Stent-grafts, which include a graft layer either inside or outside of a stent structure, are particularly useful for the treatment of aneurysms. An aneurysm may be characterized as a sac formed by the dilatation of the wall or an artery, vein, or vessel. Typically the aneurysm is filled with fluid or clotted blood. The stent-graft

35

provides a graft layer to reestablish a flow lumen through the aneurysm as well as a stent structure to support the graft and to resist occlusion or restenosis.

5 Treatment of a bifurcation site afflicted with such defects as an occlusion, stenosis, or aneurysm is a particularly demanding application for either stents or stent-grafts. A bifurcation site is generally where a single lumen or artery (often called the trunk) splits into two lumen or arteries (often called branches), such as in a "Y" configuration. For example, one such
10 bifurcation site is found within the human body at the location where the abdominal aortic artery branches into the left and right (or ipsilateral and contralateral) iliac arteries.

15 When a defect, such as an aneurysm, is located very close to the bifurcation of a trunk lumen into two branch lumens, treatment becomes especially difficult. One reason for this difficulty is because neither the trunk lumen nor either of the branch lumens provides a
20 sufficient portion of healthy, lumen wall on both sides of the defect to which a straight section of single lumen stent or stent-graft can be secured. The stent or stent-graft must span the bifurcation site and yet allow undisturbed flow through each of the branch and trunk
25 lumens.

What is required then is a stent or stent-graft which may be secured to each of the lumen wall a sufficient distance away from the defect and yet is capable of allowing undisturbed flow into each of the branch and
30 trunk lumen. Such a configuration, at least after implantation, generally must have the same Y-shape as described for the bifurcation site. Prior to implantation, the stent or stent-graft may have a Y-shape or may have a modular construction which is assembled into
35 the desired shape as it is implanted.

5 As we shall see, deployment of implants adapted to meet these needs is also problematic in that they must be deployed and secured in three different lumen which are impossible to access from a single direction. Further, to facilitate intraluminal delivery through a body's tortuous vasculature, the implant must be capable of being compressed into a very small diameter or profile.

10 Prior devices that deal with treatment at a bifurcation site within the body generally include grafts, stents, and stent-grafts in either a single-piece or modular configuration as described below.

15 The use of tubular grafts for treating defects at bifurcation sites has been known for some time. Bifurcated grafts have been disclosed, for example, in United States Patent Nos. 3,029,819 to Starks, 3,096,560 to Liebig, 3,142,067 to Liebig, and 3,805,301 to Liebig. These grafts are typically made of woven fabric or other synthetic material and, because they have no supporting stent structure, typically involve excising the defected segment and suturing the fabric graft in place using
20 common surgical procedures.

25 A number of bifurcated graft implants have been developed which use some limited means of supporting the one-piece bifurcated graft structure. Typically such means also provide a way to hold the graft open and secure the graft to the lumen wall without the need for sutures so that the graft may be suitable for transluminal delivery via a remote site as opposed to the more invasive surgical grafting techniques as described above.

30 One such implant is disclosed in United States Patent No. 4,562,596 to Kornberg. Kornberg discloses a bifurcated aortic graft constructed for intraluminal delivery through the femoral artery. The graft consists of a tubular graft material having a plurality of
35 longitudinal supporting struts or stays equipped with

5 hooks or barbs to facilitate attachment within the desired
location of the damaged artery. The graft is equipped
with a resilient top ring for snugging the upper end of
the trunk portion against the aortic wall upon deployment.
10 The graft has a trunk portion and two legs, one of which
is shorter than the other. The graft is delivered in a
compressed state through a first branch artery with the
shorter leg folded against the longer. At some point, as
the compressed implant is advance through the first branch
15 artery, the shorter leg clears the bifurcation point and
articulates into the luminal region of a second branch
artery. The entire implant is then moved in the reverse
direction to allow the shorter leg to progress down the
second branch. The implant is then expanded to its final
shape against the lumen walls by way of a balloon.

20 Instead of longitudinal struts, other devices have
provided the necessary support and securing means for the
graft material by employing sections of stent structure at
selected locations along the graft. Typically, stent
rings may be placed at the trunk and/or branch openings of
the stent. Such stent rings are either self-expanding or
require balloon expansion.

25 United States Patent No. 5,489,295 to Piplani et al.,
for example, discloses a bifurcated graft having a main
body and legs formed of a flexible surgically implantable
material. Expandable spring attachments are secured to
the main body adjacent to the trunk opening and also to
one of the legs adjacent to the branch leg opening.
30 Delivered compressed, these expandable spring attachments
urge the openings of the graft open upon deployment and
serve as anchoring means for securing the graft to the
vessel wall. Lumen wall engagement may be enhanced by the
addition of barbs or hooks at the apices of the spring
attachments.

35 Another device involving a single-piece bifurcated

5 graft with limited supporting and securing means is disclosed in U.S. Patent Nos. 5,360,443 and 5,522,880 both to Barone et al. Barone et al. disclose a tubular aortic graft for intraluminal delivery. The graft is secured by the expansion and deformation of a thin-walled tubular member. The thin walled tubular member has a first diameter for delivery. Upon the application of an expanding force from a balloon, the member has a second expanded and deformed diameter for securing the graft to the lumen wall.

10 As with all such one-piece devices, the delivery of the graft implant is complicated by the fact that each of the trunk and two legs of the graft must be positioned into their respective lumen and then secured into place. This requires the branch legs to be compressed together for delivery through one of the lumen and requires difficult maneuvering of the branch legs to get them unfolded and untwisted into place within their respective branch lumen. This type of delivery requires the graft sections to be highly flexible so that its components may be manipulated as required and requires a larger profile. This demand for high flexibility often results in unsupported graft sections that may be subject to kinking, folding, collapse or the like.

20 Bifurcated stent devices generally suffer from even greater delivery problems because they are even less compressible and less flexible than their unsupported graft counterparts discussed above. United States Patent No. 4,994,071 to MacGregor, for example, discloses a single-piece bifurcated stent for insertion into a bifurcating vessel. The stent includes a trunk portion constructed from a series of generally parallel loops interconnected by a sequence of half-hitch connections which extend along its length. The parallel loops form a cylindrical lattice which define a flow passageway. Two

5 smaller cylindrical lattices are similarly constructed and attached to the trunk portion to form the branch flow passageways. The stent is designed to be delivered in one piece, over two guidewires (one for each branch) from the direction of the trunk vessel.

10 Another bifurcated stent example is found in United States Patent No. 5,342,387 to Summers. Summers discloses a Y-shaped bifurcated stent comprising three coil sections (a major coil section and two minor coil sections), constructed of stent wire according to specific coil patterns and joined so as to form an unobstructed support for the trunk and branched vessels. To deploy the bifurcated stent, the stent is compressed around an inflatable bifurcated balloon. The compressed
15 balloon/stent is delivered up one of the branch vessels until one of the minor coils is clear of the bifurcation juncture. Then the stent is backed down, positioning one of the minor coils in each of the branches. The stent is then expanded by the bifurcated "tri-wing" balloon and then the balloon is removed.
20

To alleviate these complicated delivery problems, some implant devices have used a modular approach. An example of a modular stent may be found in FR 2 678 508 A1. According to that disclosure, in order to provide
25 continuity at junctions, in particular at vessel bifurcations, at least two helicoidal spring elements comprised of self locking coils are used. A first element is constructed to have a first coil diameter section corresponding to the diameter of the aortic artery and a second coil diameter section corresponding to one of the
30 iliac arteries. A second element similarly has two sections, one of which corresponds to the diameter of the second iliac artery, the other equivalent to the diameter of the aortic section of the first element so that the corresponding coils of each element may be delivered
35

separately and locked together *in situ*.

Another type of modular approach involves using two separate elongated tubes delivered through each of the branch lumen. The tubes, which may consist of a tubular graft element supported by unconnected stent segments, establish the required flow lumen in each of the branch arteries, and in the trunk lumen, are forced together in such a manner as to substantially seal around the periphery. Generally, the shape of the two tubes in the trunk lumen is that of two back-to-back, semi-circular "D" shapes. United States Patent No. 5,507,769 to Marin et al and EP 0 551 179 A1 to Palmaz et al. disclose implants of the type which employ two separate tubes. Palmaz further discloses the use of an expandable tubular member which is secured to the trunk artery prior to delivery of the separate tubes. The purpose of this additional member is to help secure the two tubes to the trunk lumen.

Still another type of modular stent-graft device is disclosed in WO 95/21592 (International Application number PCT/US95/01466. In that publication, there is disclosed a modular bifurcated stent or stent-graft comprising two separate modules for delivery in a compressed state and connected together *in situ*. A first module has a proximal part adapted to engage the trunk artery, then bifurcating into a first distal portion adapted to extend into one branched artery and a female receiving opening to be positioned near the other branched artery. A male proximal portion of a second module is connected to the female receiving opening. According to the disclosure, to ensure the two modules remain connected, it is preferred that the receiving opening has a frustoconical section and the second module has a mating male frustoconical section.

Further related modular stent-graft approaches may be found for example in EP 068 6 379 A2, EP 0 696 447 A2, and United States Patent No. 5,562,724 to Vorwerk et al.

5 While these modular devices tend to offer a measure of improved delivery, continuing problems may include a certain amount of leakage around the openings of the device, leakage at the modular connection, increased compressed profiles, and not optimized flexibility, kink-resistance, and axial stiffness.

10 Further it is generally important for any stent or stent-graft to be accurately and quickly deployed so that it may be properly positioned at a desired treatment location. This is especially true with bifurcated devices using a modular approach because, when deployed, the connecting feature must be properly aligned rotationally over a branch artery.

15 From the foregoing discussion it is evident that it would be desirable to have a self-expanding stent-graft device possessing superior kink-resistance and flexibility to allow the device to follow the natural geometry of the vasculature and, at the same time, allow for sufficient axial stiffness to facilitate accurate placement, resist movement, and prevent leakage. It would be highly desirable to have such a stent or stent-graft device that also provides for a reduced compressed profile for delivery through the body's vasculature. It would be highly desirable for such a stent or stent-graft to have the capability to ensure axial and rotational alignment.

20

25

DISCLOSURE OF THE INVENTION

30 The present invention is an endoluminal prosthesis that avoids the problems and disadvantages of the prior art. The invention generally involves a construction which can be adapted for placement at a bifurcation site within a mammalian body. In one embodiment, the prosthesis is a bifurcated stent or stent-graft.

35 In another embodiment an inventive stent-graft construction may provide for at least two segments of the

stent-graft to have different structural properties from each other. The structural properties may include flexibility and axial stiffness. With such a construction, it is possible to optimize the performance characteristics for ideal delivery and at the same time enhance the device's kink resistance, its ability to maintain its deployed position, and its conformability (which is helpful to effectuate required sealing against the vessel wall). In a preferred embodiment, the axial stiffness is varied according to the presence or absence of extended strut features or the use of a tape member of varying thickness or width.

According to another embodiment of the present invention, the bifurcated stent-graft may be constructed to have a region of single lumen stent covering a multilumen graft. This construction provides for a reduced delivery profile and simplified manufacturing. In one aspect of the present invention, the stent construction is configured to cover a larger portion of periphery of the bifurcated graft.

Another embodiment of the present invention involves a modular stent-graft. A preferred embodiment includes an extended region of cylindrical overlap between the modular components to effectuate improved sealing between the components. In a preferred embodiment the modular components in the area of the cylindrical overlap are constructed to have a diametrical interference fit. In alternate embodiments, sealing is enhanced by the addition of an anchoring ring, a flap of graft material, or both. Certain sealing defects may be further avoided by the use of a scalloping construction graft material around the end openings of the stent-graft.

In yet a further embodiment, the present invention involves a method of forming a bifurcated graft member comprising the steps of heat boding a first tube section

to a second tube section such that a common septum is formed and then removing the septum to form a smooth bifurcation.

Another embodiment of the present invention involves a prosthesis anchor for securing the prosthesis to the lumen wall. The anchor may involve a pivotably coupled wire portion extending angularly from the surface of the prosthesis. In one aspect of the inventive anchor, the anchor further has a second wire portion in angular relation to the surface of the prosthesis such that displacement of the second wire toward the surface urges said first wire away from the surface and into the lumen wall.

The above is a brief description of some deficiencies in the prior art and advantages of the present invention. Other features, advantages, and embodiments of the invention will be apparent to those skilled in the art from the following description, accompanying drawings, and appended claims.

BRIEF DESCRIPTION OF THE DRAWINGS

Figure 1 is a perspective view of a mammalian implant that is restrained in a collapsed state.

Figure 2 is an end view of the restrained implant of Figure 1.

Figure 3 is a perspective view of the assembly of Figure 1 with the restraint released and the implant in an expanded state.

Figure 4A is an end view of the assembly of Figure 3.

Figure 4B is a bottom plan view of the restraining member of Figure 4A.

Figure 5A shows a restraining member retraction mechanism where the mechanism is in an unactuated state.

Figure 5B shows the mechanism of Figure 5A in an actuated state.

Figure 5C shows an alternate construction of a retraining member retraction mechanism where the mechanism is in an unactuated state.

Figure 5D shows the mechanism of Figure 5C in an actuated state.

Figure 6A is a perspective view of another embodiment of the implant in conjunction with the restraining member of Figure 1.

Figure 6B is a perspective view of a further embodiment of the implant in conjunction with the restraining member of Figure 1.

Figure 7A illustrates the restraining and coupling member of Figure 1 and the pull direction for removing the coupling member from the restraining member.

Figure 7B shows the assembly of Figure 7A with the coupling member loosened to illustrate the chain knots.

Figure 7C diagrammatically represents release of the assembly of Figure 7A or 7B as the coupling member is pulled in the direction shown.

Figures 8A, 8B, 8C, 8D, 8E and 8F diagrammatically show a procedure for loading an expandable stent-graft into a restraining member prior to endolumenal delivery.

Figure 9A diagrammatically shows delivering a restrained implant to a desired site in a mammalian body lumen with the coupling member configured as shown in Figures 7A-7C.

Figure 9B is a sectional view of Figure 9A taken along line 9B-9B.

Figure 9C shows an alternate multiple restraining member arrangement for that shown in Figure 9A.

Figure 10A diagrammatically shows partial deployment of the implant assembly illustrated in Figure 9A showing progressive expansion in a direction away from the distal end of the illustrated guidewire (i.e., toward the illustrated hub).

Figure 10B is a sectional view of Figure 10A taken along line 10B-10B.

Figure 11 A diagrammatically shows full deployment of the implant assembly illustrated in Figure 9A.

5 Figures 12A, 12B, 12C and 12D diagrammatically show deployment of a restrained implant where the coupling member configuration provides release from the middle portion of the implant outward toward the implant ends.

10 Figure 13 illustrates one coupling member configuration for deployment as shown in Figures 12A-12D.

Figure 14A is a perspective view of a bifurcated stent-graft in accordance with the principles of the present invention.

15 Figure 14B is a top plan view of the bifurcated stent-graft of Figure 14A.

Figure 14C is a cross-section view taken along section line 14C-14C depicted in Figure 14A.

20 Figure 14D is a cross-sectional view taken along section line 14D-14D depicted in Figure 14A showing an alternate embodiment.

Figure 15 is a front view of the assembled bifurcated stent-graft of Figure 14A placed at a bifurcation site within the vasculature of a body.

25 Figure 16 is a perspective break-away view showing a close-up of one construction of stent anchors according to the present invention.

Figure 17 is a perspective break-away view showing a close-up of a preferred construction of the stent anchors.

30 Figure 18 is a cross-sectional view of the stent-graft of Figure 14B taken along section line 18-18.

Figure 19 is a cross-sectional view of the stent-graft of Figure 14A taken along section line 19-19.

Figure 20 is an enlarged partial cross-sectional view of the contralateral leg connection depicted in Figure 19.

35 Figure 21 and Figure 22 are enlarged partial cross-

sectional views of alternative constructions of the receiving lumen.

Figure 23 is a partial perspective view of an alternate scalloped construction of the proximal region of the contralateral leg component.

Figures 24A and 24B are cross-sectional views taken along section line 24A-24A as shown in Figure 14A depicting a free state and a forced state respectively.

Figures 25A and 25B are cross-sectional views taken along section line 25A-25A as shown in Figure 23 depicting a free state and a forced state respectively.

Figure 26 is a front view of graft components prior to assembly.

Figures 26B and 26C are respectively the front view and top view of the assembled graft of Figure 26A.

Figure 27A is a front view of the unassembled components of an alternate construction of the graft element.

Figure 27B is a front view of the assembled graft element according to the alternative construction of Figure 27A.

Figures 28A, 28B, 28C, 28D, and 28E diagrammatically show deployment of a bifurcated stent-graft.

Figures 29A, 29B and 29C diagrammatically show deployment of a bifurcated stent-graft using an alternate delivery system.

DETAILED DESCRIPTION

The following disclosure relating to the present invention will use certain nomenclature as set forth below. The term distal, as hereinafter used, is meant to refer to locations that are furthest away from the catheter delivery hub. Proximal is meant to refer to locations that are closer to the catheter delivery hub.

Referring to the drawings in detail wherein like

numerals indicate like elements, the present invention generally involves bifurcated implants such as stents or stent-grafts for delivery to a desired site through a body's vasculature. This may involve delivery systems that can be used in conjunction with such implants. As this invention involves both bifurcated components as well as non-bifurcated components, it is worthwhile to begin by describing in detail the general prosthesis construction and preferred manner of deployment that is applicable to both straight and bifurcated stents or stent-grafts in accordance with Figures 1-13. The bifurcated prosthesis will be described with relation to Figures 14-28.

Although the invention will be described with reference to the delivery examples illustrated in the drawings, it should be understood that it can be used in conjunction with other delivery devices having constructions different than those shown.

For illustrative purposes, this invention will be described with reference to the location in the human body where the abdominal aorta bifurcates into the left and right (or ipsilateral and contralateral) iliac arteries. It should be understood, however, that the present invention may be used at many other locations within the body.

Referring to Figures 1 through 13, delivery systems for delivering implants or devices, such as stents or stent-grafts, to a desired site in mammalian vasculature are shown. Such delivery systems generally include a restraining member that is adapted and configured for surrounding at least a portion of a collapsed or compressed implant and a coupling member(s) for releasably coupling portions of the restraining member to one another to maintain the implant in its collapsed or compressed state.

5 Referring to Figures 1-4, an implant delivery system is shown. Delivery system (100), generally includes a restraining member (102), which as shown may be in the form of a sheet of material, and a coupling member (104) for releasably coupling portions of the restraining member to one another. The restraining member portions that are coupled may differ than those illustrated, but preferably are selected to maintain the implant, such as self-expanding stent-graft (106), in a collapsed or compressed state as shown in Figures 1 and 2 where the restraining member (102) is shown in the form of a tube. In the illustrative embodiment, the coupling member (104) is shown as a filament or thread-like element which prevents the restraining member (102) from rearranging to a configuration where the stent-graft (106) could expand to its expanded state.

10 The implant may be collapsed in any suitable manner for placement within the restraining member (102). For example, the implant may be folded or radially crushed before placement within the restraining member (102) as will be described in more detail below. As shown in Figures 9-11, a delivery assembly (108), which includes the restraining member (102) and the stent-graft (106), has relatively small cross-sectional dimensions which facilitate endolumenal delivery of the assembly to a site where the natural lumen diameter may be smaller than the expanded diameter of the stent-graft (106).

20 Referring to Figures 3 and 4A, the assembly (108) is shown in a deployed state after removal of the coupling member (104). The restraining member (102) may be fixedly secured to the stent-graft (106) so that the two components remain attached after expansion at the desired deployment site. The attachment between the restraining member and the implant preferably is made to prevent significant movement between the restraining member and

stent-graft after deployment which could disrupt
endovascular fluid flow. Referring to Figures 4A and 4B
multiple sutures (110) may be used to fixedly attach the
restraining member (102) to the stent-graft (106). More
5 specifically, the sutures can form loops that pass through
the restraining member and around portions of the stent as
shown in Figure 4A. It is further noted that although one
arrangement of the sutures (110) is shown in Figure 4B
other arrangements may be used.

10 Although other configurations of the restraining
member (102) can be used, a preferred configuration is a
generally rectangular one having constant width as shown
in Figure 4B. For example, in the case where the
restraining member is used in conjunction with a modular
15 bifurcated stent as will be described below, the
restraining member may have a similar rectangular
configuration as that shown in Figure 4B. Alternatively,
it may have two differently sized rectangular portions
arranged to mate with the regions of different diameter
20 (trunk and leg) or another configuration that would
maintain the implant in a collapsed stent when secured.
Returning to Figure 4B, the restraining member may be
described as having side margins (112) that extend between
the ends (114) of the member. Eyelets (116) are disposed
25 along the side margins so that the coupling member (104)
may be laced or threaded therethrough. The eyelets may be
in the form of through holes (118), which may be formed by
a uniform-diameter puncturing device or by other means
such as laser-drilling. Alternatively, the eyelets may be
30 formed by loops (120) which may be attached to the side
margins (112) or formed by other means as would be
apparent to one of ordinary skill in the art.

It is further desirable to have structural
reinforcement at the side margins (112) to minimize or
35 eliminate the possibility of the coupling member (104)

from tearing the restraining member (102) when under load. Reinforced side margins may be formed by folding a portion of the restraining member (102) over a reinforcement member (122), such as a small diameter suture, which may be heat bonded between the two layers of sheet material. With this construction, a relatively low profile bead of material along the side margins (112) prevents or minimizes the possibility of tear propagation and, thus, accidental uncoupling of the restraining member (102). The small diameter suture (122) may comprise ePTFE, for example.

As the restraining member (102) constrains a collapsed self-expanding stent-graft, for example, forces resulting from stored spring energy in the collapsed stent-graft (106) will be acting on the restraining member (102) when it is configured for delivery. Thus, the restraining member (102) may comprise a material which is creep resistant and can withstand required loads without stretching over time. The restraining member (102) may comprise, for example, ePTFE, which is believed to provide suitable creep resistance, flexibility, and biocompatibility in a thin sheet form which can be heat bonded. Other materials also may be used including polyethers such as polyethylene terephthalate (DACRON® or MYLAR®) or polyaramids such as KEVLAR®.

The thread-like coupling member (104) may also comprise ePTFE. Sutures of polyethers such as polyethylene terephthalate (DACRON® or MYLAR® or polyaramids such as KEVLAR® or metal wire comprising nitinol, stainless steel or gold may also be used for the coupling member (104). The coupling member (104) may simply extend to form a remote pull line as will be discussed below. Alternatively, a metallic pull line, such as one comprising stainless steel may be coupled to a nonmetallic coupling member (104) such as one comprising

ePTFE. The coupling may be made by folding the end of the metallic pull line back upon itself to form an eyelet and threading the coupling member therethrough and securing it to the eyelet with a knot.

5 It is further noted that the width of the restraining member, when in a flat orientation as shown in Figure 4A, preferably is less than the diameter of the implant. Typically the restraining member width will be less than about 40mm (typically about 25-40mm when the device is
10 sized for thoracic aorta applications), and typically less than about 15mm in other applications where the lumen is smaller. The sheet of material preferably has a thickness less than .010 inch (0.254mm) and more preferably less than .005 inch (0.127mm). In addition, the length of the
15 restraining member preferably is less than or equal to that of the implant.

Additionally, a retraction assembly may be provided to retract the restraining member during expansion of the implant, so that the length of the restraining member is
20 maintained to be about equal to or less than that of the implant. The expandable portion of the implant may undergo minor amounts of shortening along the axial direction due to the expansion thereof in the radial direction, which may lead to an overlap of the restraining
25 member at the ends of the implant, but for the use of some type of retraction assembly in these situations. The retraction assembly minimizes or eliminates the risk of the restraining member extending beyond the implant and interfering with any channel formed by the implant, or any
30 fluid flowing therethrough after expansion.

Referring to Figures 5A-5D, retraction assemblies or mechanisms are shown. In Figure 5A, a retraction assembly (340) is shown including a biocompatible filament (342), which includes a portion that is stitched, tied or
35 otherwise fixed to the restraining member (102), as shown

at an attachment point (348), adjacent to one end of the
restraining member. Filament (342) is passed underneath
the members forming the first or end helical turn of the
stent (126) and looped under or otherwise slidably secured
to a portion of the second, third or another helical turn
other than the first helical turn such as an apex or bend
portion (344) in a second turn. The other end portion of
filament (342) is further fixed, by tying or other means,
to a portion of the stent that is circumferentially spaced
from the attachment point (348) or the apex or bend
portion (344), for example, such as an apex or bend
portion (346) of the same helical turn. Preferably, the
filament (342) is looped through an apex portion (344) of
the second helical turn and tied to an apex portion (346)
which is adjacent to the apex portion (344) as shown in
Figure 5A.

Figure 5A shows the stent in the compressed state.
Upon expansion of the stent, as mentioned above, the
members of the stent expand to effect the radial expansion
of the stent, as shown in Figure 5B. Because the distance
between apex portions (344) and (346) becomes greater upon
expansion of the stent, and because the filament (342) is
relatively unyieldable and inelastic, the distance between
the attachment point (344) and the apex portion (348)
necessarily decreases. The result is that the end of
the restraining member (102) is retracted with respect to
the stent (126), as shown in Figure 5B. Thus, the
retraction along the longitudinal axis of the restraining
member is driven by the expanding distance between
adjacent apexes in this embodiment. Although only one
retraction mechanism is shown at one end of the
restraining member, another similarly configured and
arranged retraction mechanism may be used at the other end
of the restraining member.

Figures 5C and 5D show another embodiment for a

5 retraction assembly. The views of this assembly (as are
those shown in Figures 5A and 5B) are taken from a
location between the generally cylindrical graft and stent
looking radially outward. In contrast to that shown above
10 where one end portion of a filament is secured to the
restraining member and another to a portion of the stent
that circumferentially moves during stent expansion, the
other end of the filament is secured to a portion of a
stent that moves generally parallel to the longitudinal
15 axis of the stent (axially) as the stent expands. In this
embodiment, at least one apex portion (364) of an end
helix of the stent member (126') (which differs from stent
(126) in that it includes eyelets or loops which may be
formed as shown in the drawings) is made shorter than the
20 majority of apex portions (366). However, the apex
portions may be otherwise configured such as those shown
in Figures 4A and 4B. A filament (362) is tied or
otherwise fixed at one end to apex portion (364), and at
the other end, to one end portion of the restraining
25 member (102). As shown in Figure 5D, upon radial
expansion of the stent, inwardly positioned apex portion
(364) retracts to a greater extent in the longitudinal or
axial direction than the full height apex portions (366)
which are shown in the last or most outwardly positioned
30 turn of the stent. This relative greater retraction
directly translates through filament (362) such that the
end of the restraining member (102) is retracted relative
to apex portions (366). As described above, another
similarly constructed retraction mechanism may be provided
at the other end of the restraining member.

Returning to Figure 1, one stent-graft construction
that may be used in conjunction with the delivery systems
disclosed herein is shown. Stent-graft (106) generally
includes a thin-walled tube or graft member (124), a stent
35 member (126), which can be a self-expanding stent, and a

5 ribbon or tape member (128) for coupling the stent (126)
and graft (124) members together. The stent (126) and
graft (124) members may be heat bonded together, thus
sealing in portions of the stent member (126) that are
between the tape member (128) and the graft member (124).
The mechanical properties of the stent-graft (128) may be
customized, for example, through materials selection, by
varying the structural pattern of the stent member,
varying the thickness of the tape (128) and graft (124)
10 members, and varying the pattern with which the tape
member contacts the stent and graft members.

As shown in Figure 1A, the tape member (128) may
cover only a portion of the stent member (126) as it
follows the helical turns of the undulating stent member.
15 With this construction, regions of the stent member do not
interface with the tape member when the stent-graft is in
an uncompressed state, for example. This is believed to
advantageously reduce shear stresses between the stent
member (126) and the tape member (128) when the stent-
20 graft undergoes bending or compression, thereby reducing
the risk of tearing the graft (124) or tape (128) members
or causing delamination between the stent (126) and graft
(124) members.

The tape member (128) also preferably has a generally
25 broad or flat surface for interfacing with the stent (126)
and graft (124) members as compared to filament or thread-
like structures such as sutures. This increases potential
bonding surface area between the tape member (128) and the
graft member (124) to enhance the structural integrity of
30 the stent-graft. The increased bonding surface area also
facilitates minimizing the thickness of the tape member
(128). It has been found that a tape member in the form
of a generally flat ribbon as shown in the drawings
provides desired results.

35 Tape members having widths of 0.025, 0.050 and 0.075

inches applied to a stent member having a peak-to-peak undulation amplitude of about 0.075 inch are believed to provide suitable results. However, it has been found that as the tape member band width increases, the stent-graft flexibility generally is diminished. It is believed that a tape member width of about one-fourth to three-fourths the amplitude of the stent member undulations, measured peak-to-peak, may be preferred (may be more preferably about one-third to two-thirds that amplitude) to optimize flexibility. It also has been found that by positioning one of the lateral margins of the tape member adjacent to the apexes, the tape member width may be reduced without significantly sacrificing apex securement. Varying the width of the tape member (e.g., varying width of the tape along the length of the stent graft) can also result in the adjustment of other structural properties. Increasing the width can also potentially increase the radial stiffness and the burst pressure and decrease the porosity of the device. Increasing band width can also diminish graft member wrinkling between coupling member turns.

The tape member (or separate pieces thereof) also may surround the terminal end portions of the stent-graft to secure the terminal portions of the graft member to the stent member.

Figures 6A and 6B illustrate further stent-graft constructions that may be used with the delivery systems described herein. Referring to Figure 6A, stent-graft (200) is the same as stent-graft (106) with the exception that stent-graft (200) includes a filament that couples stent undulations in adjacent turns. Filament (202) is laced or interwoven between undulations of the stent member and acquires a helical configuration (i.e., it forms a secondary helix) in being laced as such. Such a configuration is disclosed in PCT publication No. WO 95/26695 (International Application No. PCT/US95/04000)

the entirety of which is hereby incorporated herein by reference. The stent-graft (300) shown in Figure 6B is the same as that shown in Figure 6A with the exception that the filament (302) is interwoven between undulations in the same helical turn of the stent member.

The filaments (202, 302) are of the same construction and may be of any appropriate filamentary material which is blood compatible or biocompatible and sufficiently flexible to allow the stent to flex and not deform the stent upon folding. Although the linkage may be a single or multiple strand wire (platinum, platinum/tungsten, gold, palladium, tantalum, stainless steel, etc.), much preferred is the use of polymeric biocompatible filaments. The flexible link may be tied-off at either end of the stent-graft (100), for example, by wrapping its end portion around the stent and tying it off at the point at the beginning of the last turn as would be apparent to one of ordinary skill.

A percutaneously delivered stent-graft must expand from a reduced diameter, necessary for delivery, to a larger deployed diameter. The diameters of these devices obviously vary with the size of the body lumen into which they are placed. For instance, the stents typically may range in size from 2.0mm in diameter (for neurological applications) to 40mm in diameter (for placement in the aorta). A range of about 2.0mm to 6.5mm (perhaps to 10.0mm) is believed to be desirable. Typically, expansion ratios of 2:1 or more are required. These stents are capable of expansion ratios of up to 5:1 for larger diameter stents. Typical expansion ratios, for instance, typically are in the range of about 2:1 to about 4:1. The thickness of the stent materials obviously varies with the size (or diameter) of the stent and the ultimate required yield strength of the folded stent. These values are further dependent upon the selected materials of

5 construction. Wire used in these variations are typically
of stronger alloys, e.g., nitinol and stronger spring
stainless steels, and have diameters of about 0.002 inches
to 0.005 inches. For the larger stents, the appropriate
diameter for the stent wire may be somewhat larger, e.g.,
10 0.005 to 0.020 inches. For flat stock metallic stents,
thicknesses of about 0.002 inches to 0.005 inches is
usually sufficient. For the larger stents, the
appropriate thickness for the stent flat stock may be
10 somewhat thicker, e.g., 0.005 to 0.020 inches.

The following example is provided for purposes of
illustrating a preferred method of manufacturing a stent-
graft as shown in Figure 3. It should be noted, however,
that this example is not intended to be limiting. The
15 stent member wire is helically wound around a mandrel
having pins positioned thereon so that the helical
structure and undulations can be formed simultaneously.
While still on the mandrel, the stent member is heated to
about 460°F for about 20 minutes so that it retains its
20 shape. Wire sizes and materials may vary widely depending
on the application. The following is an example
construction for a stent-graft designed to accommodate a
6mm diameter vessel lumen. The stent member comprises a
nitinol wire (50.8 atomic % Ni) having a diameter of about
25 0.007 inches. In this example case, the wire is formed to
have sinusoidal undulations, each having an amplitude
measured peak-to-peak of about 0.100 inch and the helix is
formed with a pitch of about 10 windings per inch. The
inner diameter of the helix (when unconstrained) is about
30 6.8mm. (The filament when used as shown in Figures 6A and
6B may have a diameter of about 0.006 inch.)

In this example, the graft member is porous expanded
polytetrafluorethylene (PTFE), while the tape member is
expanded PTFE coated with FEP. The tape member is in the
35 form of a flat ribbon (as shown in the illustrative

embodiments) that is positioned around the stent and graft member as shown in Figure 3. The side of the tape member or ribbon that is FEP coated faces the graft member to secure it to the graft member. The intermediate stent-graft construction is heated to allow the materials of the tape and graft member to merge and self-bind as will be described in more detail below.

The FEP-coated porous expanded PTFE film used to form the tape member preferably is made by a process which comprises the steps of:

(a) contacting a porous PTFE film with another layer which is preferably a film of FEP or alternatively of another thermoplastic polymer;

(b) heating the composition obtained in step (a) to a temperature above the melting point of the thermoplastic polymer;

(c) stretching the heated composition of step (b) while maintaining the temperature above the melting point of the thermoplastic polymer; and

(d) cooling the product of step (c).

In addition to FEP, other thermoplastic polymers including thermoplastic fluoropolymers may also be used to make this coated film. The adhesive coating on the porous expanded PTFE film may be either continuous (non-porous) or discontinuous (porous) depending primarily on the amount and rate of stretching, the temperature during stretching, and the thickness of the adhesive prior to stretching.

In constructing this example, the thin wall expanded PTFE graft was of about 0.1mm (0.004 in) thickness and had a density of about 0.5g/cc. The microstructure of the porous expanded PTFE contained fibrils of about 25 micron length. A 3cm length of this graft material was placed on a mandrel the same diameter as the inner diameter of the graft. The nitinol stent member having about a 3cm length

was then carefully fitted over the center of the thin wall graft.

5 The stent-member was then provided with a tape coupling member comprised of the FEP coated film as described above. The tape member was helically wrapped around the exterior surface of the stent-member as shown in Figure 3. The tape member was oriented so that its FEP-coated side faced inward and contacted the exterior surface of the stent-member. This tape surface was
10 exposed to the outward facing surface of the thin wall graft member exposed through the openings in the stent member. The uniaxially-oriented fibrils of the microstructure of the helically-wrapped ribbon were helically-oriented about the exterior stent surface.

15 The mandrel assembly was placed into an oven set at 315°C for a period of 15 minutes after which the film-wrapped mandrel was removed from the oven and allowed to cool. Following cooling to approximately ambient temperature, the mandrel was removed from the resultant
20 stent-graft. The amount of heat applied was adequate to melt the FEP-coating on the porous expanded PTFE film and thereby cause the graft and coupling members to adhere to each other. Thus, the graft member was adhesively bonded to the inner surface of the helically-wrapped tape member
25 through the openings between the adjacent wires of the stent member. The combined thickness of the luminal and exterior coverings (graft and tape members) and the stent member was about 0.4mm.

30 Although the delivery systems have been described with reference to the stent-graft examples illustrated in the drawings, it should be understood that it can be used in conjunction with other devices, stents or stent-grafts having constructions different than those shown. For example, delivery systems described herein may be used in
35 conjunction with bifurcated stents or stent-grafts as will

be described in detail below. In addition, although a self-expanding stent-graft has been described, balloon expanding stent-grafts also may be used in conjunction with the delivery systems described herein. These stent-grafts require a balloon to expand them into their expanded state as opposed to the spring energy stored in a collapsed self-expanding stent.

Referring to Figures 7A-C, one slip knot configuration that may be used in conjunction with the thread-like coupling member (104) will be described. The restraining member (102) is shown without an implant positioned therein for purposes of simplification. Figure 7A illustrates the slip knot in a prerelease or predeployment state. The series of knots are generally flush with the restraining member (102) surface and add very little profile to the construct which is preferred during implant delivery. Figure 7B shows the assembly of Figure 7A with the thread-like coupling member (104) loosened to illustrate how the chain knots (130) may be formed. Figure 7C diagrammatically represents release of the assembly of Figure 7A or 7B. The illustrated stitch is releasable by pulling one end of the line that results in releasing of the cylindrical or tubular restraining member and then deployment of the device. This particular stitch is called a chain stitch and may be created with a single needle and a single line. A chain stitch is a series of loops or slip knots that are looped through one another such that one slip knot prevents the next slip knot from releasing. When the line is pulled to release a slip knot, the following slip knot is then released and that releases the next slip knot. This process continues during pulling of the line until the entire line is pulled out of the restraining member.

Referring to Figures 7A-C, as the unknotted portion or the lead (132) of the thread-like coupling member (104)

is pulled, such as in the direction shown by reference arrow (134), each consecutive chain knot (132) releases the next adjacent one. In the preferred embodiment, the chain knots (130) of the coupling member (104) are arranged to progressively release the collapsed implant in a direction away from the distal portion of the delivery catheter as shown in Figure 10A and as will be discussed in detail below.

Referring to Figures 8A through 8F, a method for making an assembly comprising a restraining member with a collapsed or compressed implant therein is shown for purposes of example. Figure 8A shows the restraining member (102) with its side margins releasably coupled to one another and its left end dilated by a tapered mechanical dilator (402). A small funnel (404) is then inserted into the restraining member (102) as shown in Figures 8B and 8C. The small funnel (404) and restraining member (102) are then mounted onto a pulling frame (410), and a large funnel (406) is fitted into the small funnel (404) as shown in Figure 8D. Traction or pull lines (408), which have been sutured to one end of the stent-graft, (106) are pulled through the large funnel (406), small funnel (404), and restraining member (102) with a tapered mandrel (416). As shown in Figures 8F, the pull lines (408) are fastened to a tie down post (412) located on a tension screw (414) and then are pulled by the tension screw (414). The stent-graft (106) is then pulled and collapsed sequentially through the large (406) and small (404) funnels, and then into the restraining member (102). Once the stent-graft (106) has been radially collapsed into the restraining member (102), which has its side margins coupled together, the pull lines (408) can be removed. The mandrel (416) may be inserted into the restrained implant to facilitate introduction of another component. In the preferred embodiment, a multilumen

catheter (136) (Figures 9-11) is introduced through the center of the compressed stent-graft (106) and is used to deliver the radially restrained stent-graft to the desired endolumenal site.

5 It also is noted that the funnels may be chilled to facilitate compression of the stent when the stent is made of nitinol. That is, when the stent is made of nitinol, the funnels may be chilled below 0°C or below the transition temperature (M_f) where nitinol is in its
10 martensitic state. In addition, the stent-graft could be folded first and then reduced in profile by pulling through the funnel and into the restraining member. Cooling may be accomplished by spray soaking the stent-graft with chilled gas such as tetrafluroethane. Micro-
15 Dust™ dry circuit duster manufactured by MicroCare Corporation (Conn) provides suitable results. The spray canister preferably is held upside down to discharge the fluid as a liquid onto the stent-graft.

20 A method of deploying an implant will be described with reference to Figures 9-11. In general, an implant may be delivered percutaneously with the delivery systems described herein, typically through the vasculature, after having been assembled in the reduced diameter form (see e.g. Figure 1). At the desired delivery site, the implant
25 may be released from the restraining member, thus allowing the implant to expand or be expanded against the lumen wall at the delivery site. Although other devices including stents or stent-grafts may be used, such as balloon expandable stents, the following example will be
30 made with reference to a selfexpanding stent-graft, which has the ability to fully expand itself into its final predetermined geometry when unconstrained. More particularly, the following example will be made using a delivery system as shown in Figures 1 and 7A-C and a
35 stent-graft construction as shown in Figure 3.

stent-graft construction as shown in Figure 3.

Referring to Figures 9A and 9B, an implant delivery assembly including a collapsed stent-graft (106) that is confined within a restraining member (102) and, which surrounds a distal portion of the delivery catheter (136), is shown. The attending physician will select a device having an appropriate size. Typically, the stent-graft will be selected to have an expanded diameter of up to about 20% greater than the diameter of the lumen at the desired deployment site.

The delivery catheter preferably is a multilumen catheter. The proximal portion of the catheter (136) is coupled to a hub (140), which includes a guidewire port (142) for a guidewire (142), and a deployment knob (144), which is coupled to the lead (132) of the thread-like coupling member (104). Accordingly, when the knob (144) is retracted, the restraining member (102) is released so that the stent-graft may expand. The hub (140) also may include a flushing port (146) as is conventional in the art. The stent-graft (106) is held axially in place prior to deployment by a proximal barrier (148) and distal barrier (150) which are positioned around delivery catheter (136) adjacent to the proximal and distal portions, respectively, of the restrained stent-graft. The proximal and distal barriers (148, 150) may be fixedly secured to the multilumen catheter (136) to restrict any axial movement of the restrained stent-graft. The barriers preferably are positioned to abut against the stent-graft or restraining member. The lead (132) of the coupling member (104) is passed through an aperture (152) in the proximal barrier (148) which is fluidly coupled to a lumen in the delivery catheter (136) so that the coupling member lead (132) can be coupled to the deployment knob (144). Figures 9A and 9B show advancement of the catheter (136) and the restrained implant through a

vessel (154) toward a desired site. Referring to Figures 10A and 10B, once the restrained stent-graft reaches the desired site (156), the deployment knob (144) is retracted so that the stent-graft progressively expands as shown in the drawings as the coupling member (104) is removed from the restraining member. The coupling member preferably is arranged to facilitate stent-graft expansion in a direction from the distal to proximal ends of the stent-graft (i.e., in a direction from the catheter tip to the catheter hub). Figures 11A and 11B show the stent-graft (106) and restraining member (102) in their final implantation position after the coupling member and catheter have been removed therefrom. In another embodiment, multiple restraining members may be used as shown in Figure 9C. When the multiple coupling members (104) are released simultaneously implant deployment time may be reduced.

A method for deploying a balloon expandable stent-graft may be the same as that described above, with the exception that after the coupling member (104) has been retracted from the eyelets (116), the balloon, which may be positioned inside the stent-graft prior to delivery, is inflated to expand the stent-graft (106) and then deflated for removal through the catheter (136).

According to further embodiments, multidirectional coupling member release or multiple coupling members may be used. These configurations may facilitate more rapid deployment of the implant than when a single unidirectional coupling member is used. Figures 12A - 12D diagrammatically show multidirectional deployment of a restrained implant where a coupling member arrangement is provided to release the implant from its middle portion, preferably its axial center, outward toward the implant ends. Although a particular coupling member configuration is not shown in these diagrammatic representations, one

suitable coupling configuration is shown in Figure 13 where the leads (132) may be passed through the aperture (152) and coupled to the deployment knob (144) as shown in Figure 9A and described above.

5 Referring to Figure 12A, the restrained stent-graft, which is positioned on the distal end portion of delivery catheter (136), is advanced through a vessel (154) for deployment in an aneurysm (158). The axial midpoint of the restraining member (102) preferably is positioned at
10 the center of the aneurysmal sac. As the coupling member arrangement unlacing propagates from middle of the construct toward the proximal and distal ends of the restraining member (102) and the stent-graft (106), the stent-graft (106) progressively expands from its axial
15 midportion toward its ends as shown in Figures 12B and 12C. This may be accomplished by pulling the leads (132) shown in Figure 13 simultaneously when the arrangement in that figure is used. The stent-graft size is selected so that when the restraining member is fully released and the
20 stent-graft fully deployed as shown in Figure 12D, the proximal and distal portions of the stent-graft are positioned against the proximal and distal necks of the aneurysm. The delivery catheter may then be retracted.

As is apparent from the drawings, this embodiment
25 advantageously allows fluid flow through the aneurysmal sac to remain substantially unobstructed during the release of the restraining member. For example, the stent-graft ends are still constrained at the deployment time shown in Figure 12C where the aneurysm neck regions
30 are shown minimally obstructed. In addition, this simultaneous, multidirectional release of the restraining member advantageously reduces the time in which fluid flow in the vessel may disturb the implant position as it is deployed as compared to a single directional release
35 mechanism such as that shown in Figures 9-11.

Referring to Figure 13, a multiple coupling member configuration is shown. The illustrated arrangement includes two lacing configurations (150) and (152). Except for the placement of the lead (132) of thread-like coupling member (104), configuration (152) is the mirror image of configuration (150). Accordingly, description of only one of the configurations will be made for purposes of simplification. Referring to the lacing configuration (152), configuration (152) is the same as that shown in Figures 7A-C with the exception that configuration (152) further includes two additional slip knots, generally designated with reference numeral (504), and tuck or loop arrangement (506). The additional slip knots are not interwoven in the restraining member and provide a delay mechanism for release of the coupling member, as is apparent from the drawings, when the lead (132) is pulled in the direction of the arrow (134). Thus, inadvertent pulling of the lead (132) will not immediately begin to release the coupling member from the restraining member. The tuck arrangement simply involves tucking the slack from lead (132) under stitches at various intervals as shown so that the additional slip knots (504) may be pulled out of the way for delivery. In addition, the tuck or loop arrangement (506) provides an additional delay mechanism for release of the slip knots.

Bifurcated Stent or Stent-Graft.

The following describes a modular bifurcated stent-graft constructed [or treating a bifurcation site within a mammalian body. The stent-graft components generally comprise a flexible graft member attached to a wire stent member using a tape member according to the principles discussed at length above. Preferably the stent-graft components are designed for compressed delivery and are self-expanding, in the manner described above.

5 The modular stent-graft of Figures 14A through 14D generally has two principal components; a main body (700) and a contralateral leg (730) each generally having a graft member attached to a stent member according to the description above. The main body (700) generally has a number of sections which have distinct overall constructions. A distal trunk section (708) has a single lumen structure beginning at a distal end (702) of the main body (700) and continuing until a bifurcation point
10 (728). The bifurcation point (728) is the location within the prosthesis where the single lumen of the distal trunk section (708) bifurcates into internal two flow lumen.

15 An intermediate section (710) begins at the bifurcation point (728) and continues to the receiving hole (704). In the intermediate section (710), the stent-graft has an internal graft structure which is bifurcated into two lumen surrounded by a generally tubular, single-lumen stent structure. Finally, a proximal section (712) is a single lumen structure for both the stent member and
20 the graft member and includes an ipsilateral leg (726) which terminates at an ipsilateral leg hole (706).

25 The graft member of the intermediate section (710) bifurcates the single lumen distal trunk section (708) into the ipsilateral leg (726) and an internal female receiving lumen (703). The receiving lumen (703) terminates at a receiving hole (704). The receiving hole (704) and receiving lumen (703) accommodate delivery and attachment of the contralateral leg component (730). Preferably, the graft material at the distal end (734) of
30 the contralateral leg component (730) is scalloped as shown more clearly in Figure 23 discussed below.

35 The receiving hole (704) is supported by a wire structure around a substantial portion of its periphery so that the receiving hole (704) is held open after deployment. In a preferred embodiment the wire structure

that supports the receiving hole (704) is an independent wire ring (714).

5 The independent wire ring (714) is located in the general area of the receiving hole (704) in the intermediate section (710). The independent wire ring (714) ensures that the graft material at the receiving hole (704) is supported in an open position to receive the distal end (734) of the contralateral leg (730). In absence of such support, the receiving hole (704) may not reliably open after delivery of the main body component (700) because within the intermediate section (710) the bifurcated graft member in the area of the receiving lumen (703) does not have full stent support on its interior periphery. This may be better seen in Figure 18 which shows the absence of any internal stent support of the interior graft periphery (785) in the area of the receiving lumen (703).

10 The independent wire ring (714) may be comprised of the same materials as the other stent-graft sections discussed above and is preferably self-expanding. In a preferred embodiment, the independent wire ring comprises a single turn of an undulating wire stent material surrounded by at least one layer of tape which is heat bonded to the receiving hole (704). Alternatively, the independent wire ring (714) could be formed as the last turn of the main body (700).

15 A radiopaque marker may be used to make the receiving hole (704) visible during implantation. Such a marker may include a radiopaque wire adjacent to the independent wire ring (714). Such markers make it easier to see the location of the receiving hole (704) after deployment of the main body (700) within the mammalian body.

20 This construction of the intermediate stent section (710) as seen in cross-section in Figure 14C is characterized by a single-lumen stent member and

bifurcated graft member and offers both a smaller compressed profile as well as simplified manufacturing over constructions which have discreet stented leg features. The compressed profile is determined largely by the physical amount of stent and graft material present in a given section. This construction eliminates the stent material that would normally support the inside periphery of the bifurcated graft section resulting in less stent material to compress in that region. As the main body component (700) is compressed for delivery as discussed above, the compressed profile is significantly smaller than would be a structure that had a section of bifurcated stent over the section of bifurcated graft.

Even though bifurcated flow is supported, manufacturing is simplified because there is no bifurcated stent section. Winding a bifurcated stent section in one piece, for example, is a more complex process. Likewise, winding separate cylindrical stent structures and connecting them to form a bifurcated stent structure is complicated and ultimately may be less reliable. The intermediate section (710) allows the entire stent member that covers the main body component (700) to be made from a single undulating wire arranged in multiple helical turns. The result is a bifurcated stent-graft device which is simple to manufacture, easily compressible and which expands reliably upon deployment.

An alternate construction of the intermediate stent section (710), is shown in Figure 14D. The intermediate stent section (710) has a shape characterized by the indented regions (727). The shape could generally be described as a 'figure-8', except that the area between the bifurcated graft member remains unsupported at its centermost region. This construction is still a single lumen stent construction and therefore maintains much of the benefits of reduced profile and simplified

5 manufacturability while providing the bifurcated graft member with increased support around a greater portion of its perimeter. Further, indented portions (727) have less of a tendency to spring outward upon application of external forces.

10 As mentioned above, the main body component (700) and the contralateral leg component (730) are adapted for delivery in a compressed state to a bifurcation site within a body. For this purpose the main body component (700) is preferably equipped with a restraining member (722) constructed as described above. Likewise, the contralateral leg component (730) has an attached restraining member (732). These restraining members are typically sutured to the graft material at intervals down their length.

15 Figure 15 shows an assembled bifurcated stent-graft (740) after deployment at a bifurcation site within a bifurcated body vessel afflicted with an aneurysm (758). Although not intended to be so limited to any particular location, the inventive prosthesis is shown at the location where the abdominal aortic artery (752) bifurcates into the left iliac artery (756) and the right iliac artery (754). So that the various features of the inventive implant are more clearly shown, the restraining member is not shown in Figure 15.

20 The assembled bifurcated stent-graft (740) is comprised of the main body component (700) and the contralateral leg component (730). The distal end (734) of the contralateral leg component (730) has been inserted into the receiving leg hole (704) and the female receiving lumen (703) of the main body component (700).

25 For best results in deploying any stent or stent-graft of these types it is essential that they have the appropriate structural properties such as axial stiffness, flexibility and kink-resistance. With complicated

structures, such as those required for treating a bifurcated site, it is increasingly difficult to obtain the desired structural properties because optimizing one may negatively effect the other.

5 For instance, optimizing the global axial stiffness of a stent or stent-graft will necessarily make the device significantly less flexible and consequently impair its resistance to kinking and lessen its ability to conform to the natural bends of curves the body's vasculature.
10 Conversely a device that has high flexibility with little axial stiffness is difficult to properly deploy and does not aid in anchoring the device in the desired location.

15 With these constraints in mind, it has been discovered that having a bifurcated stent-graft which has segments constructed with varying structural properties offers improved deployability, is less susceptible to kinking, and favorably tends to maintain its desired position after deployment while allowing sufficient flexibility to accommodate movement by the body. The
20 exact structural properties desired may depend on the location where the prosthesis is to be deployed.

For these reasons, it is preferable that the bifurcated stent or stent-graft be constructed with at least two segments having structural properties different
25 from one another. For example, in Figure 14A, a length of the distal section (708) and the intermediate section (710) may be constructed with a higher axial stiffness for improved deployment and positional stability while the proximal section (712) may be constructed to have higher
30 flexibility to accommodate the geometry of the iliac artery.

It may be further desirable to have a number of segments that have different structural properties. Accordingly, the main body component (700) and the
35 contralateral leg component (730) of the assembled stent-

graft (740) have segments constructed with structural properties different from adjacent segments. In one preferred embodiment shown in Figure 15, the main body component (700) has four different segments constructed with different structural properties. The distal segment (742) is constructed to have higher axial stiffness than the more flexible proximally adjacent segment (744). The proximal section (748) is constructed to have a higher flexibility than that of its distally adjacent segment (746). Likewise the contralateral leg component (730) has an axially stiffer distal segment (750) and a more flexible proximal segment (749).

There are a number of ways to alter the structural properties of stent or stent-graft components. One way of selectively altering the structural properties of a stent-graft segment is to use a tape member for that segment that has different physical dimensions. Such a tape member is discussed above with reference to the tape member (128) of Figure 1. For example the tape member width, thickness or spacing may be increased, from the preferred dimensions discussed above, in a segment where it is desirable to have increased or decreased stiffness. For example, the use of wider tape wound with closer spacing will increase the stiffness in that area.

Another way of selectively altering the structural properties of a stent or stent-graft segment is shown in Figures 14A and 15. Extended struts (718) and (719) may be used to increase the axial stiffness of a stent-graft segment. Extended struts are formed by extending an apex on one turn of the undulating wire until it contacts an apex on an adjacent turn. This contact between an extended strut and the apex of an adjacent stent turn provides an added amount of axial stiffness. In a preferred embodiment, a layer of tape (not shown) is applied around the device in a helical pattern that covers

each of the apexes of the extended struts. This additional layer of taping keeps the strut pairs together.

Referring to Figure 14A, a first helical stent turn (720) and a second helical stent turn (721) have a generally undulating shape having apexes. An extended strut (718) of the stent turn (720) is formed having its apex near or in contact with the apex of the stent turn (721) directly below. The extended strut (719) is similarly formed by extending an apex of the stent turn (721) directly down to contact the apex in the turn below. This pattern is continued, each time spacing the extended strut over one undulation. This results in a helical pattern of extended struts down the length of the device. Of course, the extended struts may be arranged in patterns other than the helical configuration described.

A number of these patterns may be employed in any one segment or the extended strut pattern may be used in other segments to increase axial stiffness. Preferably the distally adjacent segment (746) on the main body component (700) and the axially stiff distal segment (750) on the contralateral leg component are constructed with extended struts as shown.

Another important aspect of the present invention is achieving a secure position against the walls of the vessel lumen so that the deployed position is maintained and so that there is no leakage of luminal flow. Referring now to Figure 15, the distal end (702) is sized to properly fit the inside diameter of the target artery, in this case the abdominal aortic artery. Typically the prosthesis is designed to have an unconstrained diameter slightly larger than the inside of the target vessel.

The ipsilateral and contralateral legs of the assembled bifurcated stent-graft (740) are typically the same size at their distal ends (around 13 mm for example) regardless of the size of the distal end (702) and undergo

5 tapered sections (724) and (738) that taper to a diameter which corresponds approximately to the internal diameter of the iliac arteries. These tapered sections (724) and (738) are preferable to abrupt changes in diameter as they tend to produce superior flow dynamics.

10 After deployment, the assembled bifurcated stent-graft (740) must establish sufficient contact with the healthy vessel lumen on each side of the aneurysm (758) so that the device does not migrate or dislodge when subjected to the relatively high fluid pressures and flow rates encountered in such a major artery, especially when the body again becomes mobile after recovery. Further, sufficient contact must be made so that there is no leakage at the distal end (702), the ipsilateral leg hole (706) or the proximal end (736) of the contralateral leg.

15 Anchoring or staying features that allow the stent or stent-graft exterior to anchor itself to the vessel lumen wall may be provided to help the device seal to the vessel wall and maintain its deployed position. For example, anchors (716) as seen in Figures 14A and 15 are provided on the main body component (700) and could also be provided on the contralateral leg component (730). Preferably the top stent portion (717) is directed angularly outward. This flared stent portion works to force the anchors (716) into the vessel wall as the top stent portion (717) expands under force into radial interference with the vessel wall upon deployment.

20 A preferred construction for an anchor (716) is shown in Figure 17. This construction involves extending two wires from the upper stent turn (762) under an apex of an adjacent lower stent turn (764). The two ends of stent wires (760 and 761) are then bent out and away from the graft material (768). Extended struts (771) are formed adjacent to each anchor in the manner described above except the extended struts extend under the adjacent lower

25

30

35

5 stent turn (764) down to a third stent turn (765). This extended strut arrangement provides support for the anchors (716) and provides for low stresses in the wires (760 and 761) under the application of bending forces encountered as the prosthesis expands into the vessel wall. The extended struts (771) minimize the localized deformation of the stent-graft structure in the area of the anchors by providing broader support.

10 Another construction of the anchors (716') are shown in Figure 16. An anchor (716') is formed in the same manner except the ends of the anchor remain connected in a 'U-shape' configuration as shown. An anchor (716') may be formed at any location on the stent-graft. Most preferably, the anchors are formed in an evenly spaced pattern around the top stent portion (717) (Figure 14A).

15 It should be apparent that the anchors as described above are not limited in use to the stent-graft combination shown in the figures but indeed could be used in any non-bifurcated or stent only construction that require similar functionality.

20 Sealing at the vessel wall may also be enhanced by the alternate construction shown in Figure 17 by way of a sealing mechanism. A sealing mechanism can be used with any type of implant, including any of the implants discussed above. For purposes of illustration, the sealing mechanism is shown with reference to the bifurcated implant of Figure 14 and comprises seal member (772) as seen in detail in Figures 16 and 17. The sealing mechanism described below can be used with any of the implants discussed above.

25 One preferred construction for seal member (772) in the variations shown in Figures 16 and 17 may be similar to the preferred construction for the tape member used in constructing the stent-graft tubular member, as is provided in reference to Figure 1A and Figure 3 above.

5 In general, a thin walled ePTFE tape is used for seal member (722) similarly as that for tape member (128), shown variously in the previous figures. The tape used for seal member (722) is adhered to the outer surface of the stent-graft, including over tape member (128), described previously for bonding the stent and graft members. Seal member (722) has an inner surface constructed of a similar material for either the outer surface of the tape member (128) or the outer surface of the graft-member (124), depending upon which surface the seal member is desirably adhered.

10 First cuff end (767) is bonded to the stent-graft outer surface and second cuff end (769) is not, in order to form the unadhered flange to function as a one-way valve against peri-stent-graft flow. Seal member (722) may be selectively adhered along its length in this manner by providing a variable inner surface to the seal member such that, upon heating, only the surface in the region of first cuff end (767) bonds to the outer surface of the stent-graft. For example, the inner surface of seal member (722) may have an FEP liner in the region of first cuff end (767) but not in the region of second cuff end (769). In this case, upon contacting an outer surface of the stent-graft that has a uniform FEP outer surface, only first cuff end (767) may be heat secured thereon.

20 Alternatively, seal member (722) may have a uniform inner surface, such as constructed of FEP, and a variable outer surface, such as with a selective portion of FEP, may be provided either on the tape member (128) or on the graft member (124) in the region where the heat bonding of seal member (722) is desired. Still further, seal member (722) may have a uniform surface and may be positioned over tape member (128) and graft member (124) so that variability between the outer surfaces of tape member (128) and graft member (124) causes a selective bonding

with the first cuff end (767) over one of those surfaces.

Further to the construction of seal member (722), the particular wall thickness of the tape which may be used for this component should desirably be as thin as possible to functionally provide the flange-one-way-valve function for that member. This is because, since seal member (722) is over the outer surface of the other stent and graft components of the stent-graft, seal member (722) is believed to be the profile-limiting feature of the overall assembly. Therefore, in a particular design, seal member (722) may desirably be a thinner wall than for the tape member used to construct the stent-graft described in reference to Figures 1 and 3.

Further referring to the particular constructions and related methods just described for adhering seal member (722) to the outer surface of the underlying stent-graft, it should be apparent to one of ordinary skill in the art that the desired construction and heat securing technique for seal member (722) is premised upon the theory that, where one polymer meets a like polymer (such as FEP meeting FEP), heating under proper conditions will allow for a selected heat bond. The present invention, however, should not be construed as limited to these particularly described conditions, but instead should be considered to more broadly encompass any suitable means for securing a seal member to the outer surface of a given tubular member, as would be apparent to one of ordinary skill, and as is provided previously with reference to Figure 1.

Further there is a plurality of circumferential strut spaces between the struts of the stent member. It is believed that these spaces may provide a path for leakage flow around the outer surface of the graft member and along the outside of the stent-graft. Second cuff end (769), however, captures such leakage flow beneath its flange, which can not propagate along the outer surface of

the stent-graft because first cuff end (767) is secured to the outer surface of that stent-graft. In other words, flow over the stent-graft and into an aneurysm is occluded.

5 Furthermore, when apex strut (716) is anchored into the wall of abdominal aortic artery as shown in Figure 15, it has been observed that the portion of main body component (700) at and adjacent to the apex strut (716) may be forced away from the artery wall. This action
10 causes a separation between the outer surface of main body (700) and the artery wall, which separation is believed to create a leakage flow path. The flange of seal member (772) captures that flow and occludes it from propagating into the aneurysm (758).

15 In addition to maintaining a good contact with the vessel lumen walls, the components of the stent-graft must make sufficient contact with each other such that the separate modules stay attached and do not leak at their engagement interface. The inventive stent-graft shown in
20 Figure 18 illustrates several important features designed to effectuate a leak-free and positionally stable seal at the interface between the receiving lumen (703) of the main body component (700) and contralateral leg component (730).

25 Figure 18 shows a partial cross-section of the assembled stent-graft. The contralateral leg component (730) has been inserted into the receiving lumen (703) of the main body component (700). This cross-sectional view shows clearly that the main body component (700) includes
30 a main body graft member (780) and a main body stent member (782). The contralateral leg component (730) includes a contralateral graft member (784) and a contralateral stent member (786).

35 At the interface between the contralateral leg component (730) and the receiving lumen (703), the

assembly provides for an extending sealing region (790). Preferably the extended sealing region (790) consists of a generally cylindrical interfering friction fit between the outside diameter of the contralateral leg component (730) and the inside diameter of the receiving lumen (703). That is, the natural or resting outside diameter of the self expanding contralateral leg component (730) would be larger than the natural inside diameter of the receiving lumen (703). Thus the forces created by the interference act to seal the two components and also serve to resist movement of the two components.

The type of generally cylindrical extended sealing region just described has many advantages. First, it allows for the stent and graft structures in the extended sealing region (790) to be constructed of relatively simple generally cylindrical elements that are easily manufactured. Because the extended sealing region (790) extends over a large length it necessarily has a large surface area to effectuate sealing between the components. This larger sealing area typically provides that multiple turns of the stent structures will be engaged in an interfering and thus scaling relationship.

In one preferred embodiment, the extended sealing region has a length in excess of one-half of the diameter of the receiving lumen (703), more preferably the length is greater than the diameter of the receiving lumen (703), and most preferably the length is more than 2 times the diameter of the receiving lumen (703).

Because the manufacturing tolerances of the simplified shapes are easily controlled and because the engagement of the extended sealing region (790) is quite large, a highly reliable joint is formed between the modular components. Even so it may be desirable to create one or more localized zones of increased interference to increase the sealing capability and positional stability.

Localized zones of interference may be created in a number of ways. In a preferred embodiment, an annular ring of decreased diameter is formed within the receiving lumen. Such a localized decreased diameter causes a greater interference with the outside diameter of the contralateral leg component in a localized area while the remainder of the engagement with the receiving lumen is subject to the general interference friction fit described above.

One way of creating a localized decreased diameter is illustrated in Figure 20 which shows a partial cross-section of the extended sealing region (790). A zone of reduced diameter (799) is created by placing an anchoring ring (798) between the graft member (780) and the stent member (782) of the receiving lumen (703). The anchoring ring may be made from any polymeric or wire material, preferably a material that will not inhibit the receiving lumen from self-expanding to an open position. Most preferably the material is a suture material, typically ePTFE.

Alternately, localized zones of decreased diameter may be created as shown in Figures 21 and 22 by folding a portion of the graft member (780) back up into the receiving lumen (703). In Figure 21, the zone of reduced diameter (806) is formed by creating a folded flap (808) of the graft material (780) around an anchoring ring (802). The flap is heat bonded in place roughly at a location (804) as shown. In Figure 22, the zone of reduced diameter (809) is formed of flap (808) and heat bonded roughly at a location (807) in a similar manner but without any anchoring ring. The localized interference using these methods tends to cover a larger area and the flap (808) provides a more flexible member to seal against the outside diameter of the contralateral leg component (730).

5 One further aspect of ensuring a good seal between
the stent-graft components involves the use of a scalloped
stent-graft construction at the distal end of the
contralateral leg component (810). To create this
scalloped construction, the graft material between the
apexes of the stent member is removed on the last turn of
the stent. For example scallop (812) may be formed by
removing (or cutting and folding under) the graft material
from between a first apex (814) and an adjacent apex
10 (816).

The advantage of using a scalloped arrangement are
illustrated in Figures 24A through 25B. Figure 24A shows
a cross-section of the fully expanded contralateral leg
component (730) having an unscalloped construction. A
15 first apex (822) and an adjacent apex (824) have
continuous graft material (784) in the area between them.
When the apex (822) and the adjacent apex (824) are forced
together in the directions of the arrows (820), the graft
material (784) forms a buckle or wrinkle (818) which is a
20 potential leak path or is a potential site for
thrombogenic material to build up as seen in Figure 24B.
The scalloped construction shown in Figures 25A and 25B,
on the other hand, have no graft material between the
first apex (814) and the adjacent apex (816) and therefore
25 when forced together do not form a graft material wrinkle.

The wrinkle (818), mentioned above may also be formed
when the stent-graft is not allowed to expand to its
complete diameter. For instance it is quite common that
the receiving lumen or vessel wall internal diameter is
30 smaller than the fully expanded stent-graft outer
diameter. This being the case, it should be clear that
the scalloped construction may alternately be used at any
of the terminal openings of the main body component or the
contralateral leg component. Preferably, the distal end
35 (702) of the main body component (700) also has this

scalloped construction as shown in Figures 14A and 14B.

In the previous discussion we have referred generally to a stent-graft that includes a graft member. While the construction of such straight stent grafts are discussed at length above, the construction of a bifurcated graft member is illustrated in Figures 26, 27A and 27B. A bifurcated graft member suitable for construction of the main body component (700) discussed above is generally formed of two graft members: the ipsilateral tapered graft (840) and the contralateral tapered graft (842). The separate contralateral leg graft component (844) is a straight or tapered section and may be formed according to the principles discussed in the first section above.

The ipsilateral tapered graft (840) has three sections which are separated by tapers. A top section (846), a middle section (848), and a bottom section (850). The body component graft (854) is formed by heat bonding the top section (846) of ipsilateral tapered graft (840) to the top section (847) of contralateral tapered graft (842). This heat bonding forms a common septum (856) which in a preferred embodiment is subsequently cut away to produce a smooth bifurcation (858). Cutting away the septum material prevents fluid flow disturbance or blockage that could result from deviation of the septum. Such deviation is caused by the fluid pressure and is aggravated if the stent-graft is radially compressed in a manner which causes the septum to become loose or no longer taut.

In another embodiment, a graft section may be constructed in the manner illustrated in Figures 27A and 27B. According to this embodiment, the body component graft (867) is constructed from two pieces. A tubular graft section (860) is bent into a 'U-shape'. A top hole (864) is formed by notching the top of the 'U-shape'. Upper graft section (862) is placed over the top hole

(864) of tubular graft section (860). The two pieces are bonded together at the bonding interface (866). Preferably, the two graft pieces are heat bonded while supported by interior mandrels (not shown) to obtain the desired shape and smooth interior. However, upper graft section (862) may be attached to the tubular graft section (860) at the bond interface (866) in any manner that provides a sufficiently leak free seal. For example the components may be sutured together or adhesive bonded.

In use, the modular bifurcated stent-graft is typically delivered percutaneously through the vasculature of the body. Preferably the prosthesis is delivered by way of a restraining member as described in detail above. Figures 28A through 28E diagrammatically illustrate deployment of a bifurcated stent-graft with a restraining member (902) using a percutaneous catheter assembly. Referring to Figure 28A, a multilumen catheter assembly (928) has been inserted to a selected site within a body lumen. The main body component (700) of a bifurcated stent-graft is held in a compressed state about a guidewire (926) and a guidewire lumen (929) by a restraining member (902) and a coupling member (906). The collapsed main body component (700) is held axially in place prior to deployment by a distal barrier (930) and a proximal barrier (932). The distal (930) and proximal (932) barriers are typically affixed to the guidewire lumen (929). The coupling member (906) extends through the eyelets (920) of the restraining member (902) forming chain knots and into the multilumen catheter (928).

Figure 28A shows advancement of the multilumen catheter (928) with the distally located main body component (700) and the restraining member (902) into implantation position, typically at the bifurcation of a major vessel. During deployment it is critical that the surgeon align the main body component (700) so that the

5 ipsilateral leg (726) will extend down one branch of the bifurcated vessel, and so the receiving hole (704) and the receiving lumen (703) will be lined up with the other branch of the bifurcated vessel so as to receive the contralateral leg component (730).

10 One way of facilitating this alignment is to provide radiopaque markers so that the surgeon may readily determine the rotational position of the main body component (700) prior to deployment or release from the restraining member (902). In a preferred embodiment, a long marker (934) is located on the contralateral side of the compressed assembly and a shorter marker (936) is placed on the ipsilateral side. Preferably these markers are placed on the stent prior to compression but may
15 alternatively be part of the restraining member. Having one marker of a different length allows the surgeon to identify the orientation of both the ipsilateral leg and the receiving lumen relative to the bifurcated vessel.

20 Once the assembly is properly aligned and positioned for implantation, the coupling member (906) is pulled and the restraining member (902) begins to release the implant, typically at the distal end first. In the preferred embodiment, the restraining member (902) is located down the side as shown because it is less likely
25 to interfere with deployment of the receiving lumen (703).

30 Figure 28B shows the main body component (700) radially expanding as the coupling member (906) is retracted through the eyelets (920) of the restraining member (902) and into the catheter assembly (928). In the preferred embodiment, the restraining member (902) has been fixedly attached to the main body component (700) with a number of sutures along the length of the main body component to prevent any relative longitudinal movement
35 between the implanted prosthesis and the restraining member (902). The restraining member may optionally

employ a retracting or pull-down mechanism as described at length above.

Figure 28C shows the main body component (700) and the restraining member (902) in final implantation position at the vessel bifurcation after the guidewire (926) and the catheter assembly (928) have been retracted.

Figure 28D shows the contralateral leg component (730) being delivered to the contralateral receiving hole using a restraining member (942). The procedure for positioning and releasing the contralateral leg component (730) is the same as that described above for implantation of a generally cylindrical stent-graft except that certain radiopaque markers may be employed to ensure its proper position relative to the bifurcation point (728) of main body component (700).

Radiopaque markers may be located, for example, to indicate the position of the receiving hole (704), the distal end (734) of the contralateral leg component (730), and the bifurcation point (728) of the main body component (700). These markers serve to indicate the position of the contralateral leg component as it enters the receiving hole (704) and its ultimate position relative to the receiving lumen (703) which begins at bifurcation point (728). In a preferred embodiment illustrated in Figure 19, the radiopaque wires (794) may be heat bonded or imbedded into the graft material (780) around the periphery of the receiving lumen. Such radiopaque wires could be used in other places such as the contralateral leg component lumen, the ipsilateral leg lumen or the lumen at the distal end of the main body component (700).

Figure 28E shows the assembled bifurcated stent-graft in its final implantation state with the contralateral leg component expanded into and engaged with the receiving lumen of the main body component (700).

Figures 29A through 29D diagrammatically show the

5 same stent or stent-graft components being deployed except
that the restraining member (902) is released from the
center out towards as the coupling member (906) is
retracted. This may provide more accurate placement
relative to the bifurcation point of the vessel instead of
relative to the distal end as with end release.

10 While this invention has been described with
reference to illustrative embodiments, this description is
not intended to be construed in a limiting sense. Various
modifications and combinations of the illustrative
embodiments, as well as other embodiments of the invention
will be apparent to persons skilled in the art upon
reference to the description. It is therefore intended
15 that the appended claims encompass any such modifications
or embodiments.

CLAIMS

1. An implantable endoluminal prosthesis adapted for placement at a bifurcation site within a body, said device having at least two segments, at least one of said segments having structural properties different from another of said segments.
- 5 2. The endoluminal prosthesis of claim 1 wherein said device comprises a main body component and a contralateral leg component.
3. The endoluminal prosthesis of claim 1 wherein at least one of said components has a segment having an axial stiffness that is higher than adjacent segments.
- 10 4. The endoluminal prosthesis of claim 3 wherein said segment of higher axial stiffness comprises at least one extended strut.
5. The endoluminal prosthesis claim 1 wherein said device further comprises:
- a stent member having an outer surface;
 - 15 a generally tubular graft member;
 - a tape member covering only a portion of said outer surface of said stent member and securing the stent member and graft member to one another, said tape member having a different width in at least one of said segments.
6. A stent-graft component comprising:
- 20 a graft member having a single-lumen graft section and a bifurcated graft section, said bifurcated graft section having two separate lumen;
- a single lumen stent section secured to at least a portion of the periphery of said graft section, said single lumen stent section extending over at least a portion of said bifurcated graft section.
- 25 7. The stent-graft of claim 6 wherein greater than 180 degrees of the periphery of each of said two separate lumen are contacted by said distal stent section.
8. The stent-graft of claim 6 wherein at least one of said separate lumen terminates distally at a leg hole and said stent-graft further comprises a ring for support of said leg hole.
- 30 9. The stent-graft of claim 8 wherein said ring comprises an undulating wire.

10. The stent-graft of claim 8 wherein said stent-graft further comprises a radiopaque wire around the outside diameter of said leg hole.

11. The stent-graft of claim 10 wherein said separate lumen are a contralateral leg lumen having a receiving hole and a ipsilateral leg lumen having an ipsilateral leg hole, said independent wire ring being secured at or near said receiving hole.

12. The stent-graft of claim 8 wherein said stent member further comprises at least one anchor for securing said stent-graft to a vessel wall.

13. The stent-graft of claim 12 wherein said anchor comprises a stent apex bent at an angle to an outer surface of said graft.

14. The stent-graft of claim 12 wherein said anchor comprises at least one wire segment bent at an angle to an outer surface of said graft.

15. A stent-graft section comprising:
a generally tubular stent member section having an inner surface and an outer surface;
a multilumen graft section secured to at least one of said inner and outer surfaces of said tubular stent member.

16. The stent-graft section of claim 15 wherein said graft section is bifurcated into two lumen and is attached to said inner surface.

17. The stent-graft section of claim 16 wherein said two lumen are secured to each other by at least one suture.

18. A stent section comprising a wire structure having undulations, said undulations characterized by an alternating series of upper apexes and lower apexes, said wire structure arranged in a helical configuration having at least a first turn and a second turn, said first turn having at least one lower apex which extends to substantially meet a lower apex of said second turn.

19. The stent section of 18 wherein said upper and lower apexes of said of said first turn are in-phase with said apexes of said second turn.

20. The stent section of 18 wherein said stent section comprises multiple turns, each one of said multiple turns having at least one lower apex which extends to substantially meet a lower apex of an adjacent turn.

21. The stent section of 20 wherein the extended apex of each turn is spaced one undulation from the extended apex of a successive turn.

22. The stent section of 18 further comprising a graft member attached to said wire structure.

5 23. A modular prosthesis adapted for placement at a bifurcation site within a body, said prosthesis comprising:

a main body component having an extended cylindrical female receiving portion; and

10 a leg component having a mating cylindrical male portion, adapted for attachment to said extended cylindrical female receiving portion.

24. The modular prosthesis of claim 23 wherein said male portion is attached within said female portion by an interference fit.

25. The modular prosthesis of claim 24 wherein cylindrical male portion has a first diameter and said cylindrical female portion has a diameter smaller than said first diameter.

26. The modular prosthesis of claim 24 wherein said female receiving portion further comprises a zone of decreased diameter in the vicinity of an anchoring ring, said anchoring ring being attached to said female receiving portion.

20 27. The modular prosthesis of claim 24 wherein said female receiving portion further comprises an internal folded flap of graft material, said flap creating a zone of reduce diameter within the female receiving portion.

28. The modular prosthesis of claim 27 wherein said flap further includes an anchoring ring.

25 29. A self-expanding stent-graft device comprising a stent member and a graft member, said stent member having a terminating end in the form of a turn of an undulating wire; said graft component being attached to said stent component, said graft component having a scalloped shape at an end which corresponds to the shape of said stent end.

30 30. A method of forming a bifurcated graft member comprising the steps of:

heat bonding a first tube section to a second tube section such that a common septum is formed and removing said septum to form a smooth bifurcation.

PAGE 44 MISSING UPON FILING

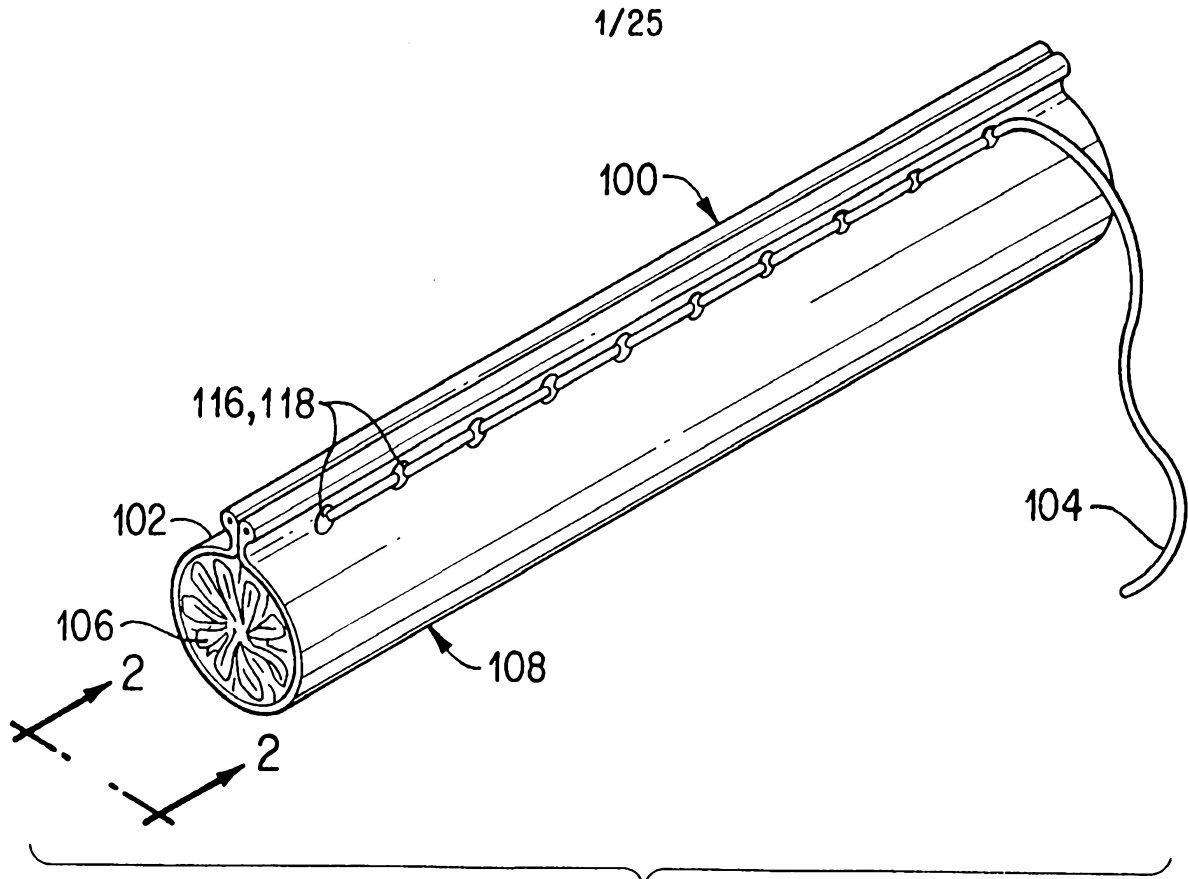


FIG. 1

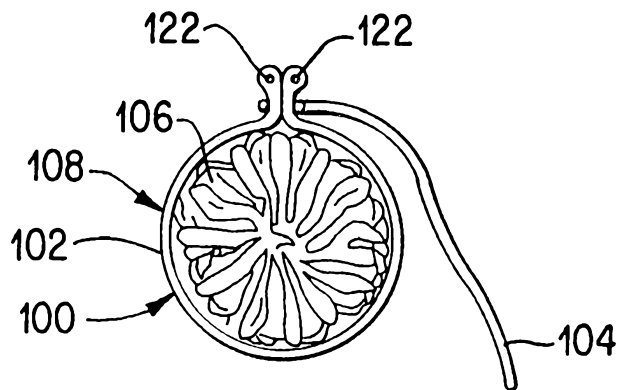


FIG. 2

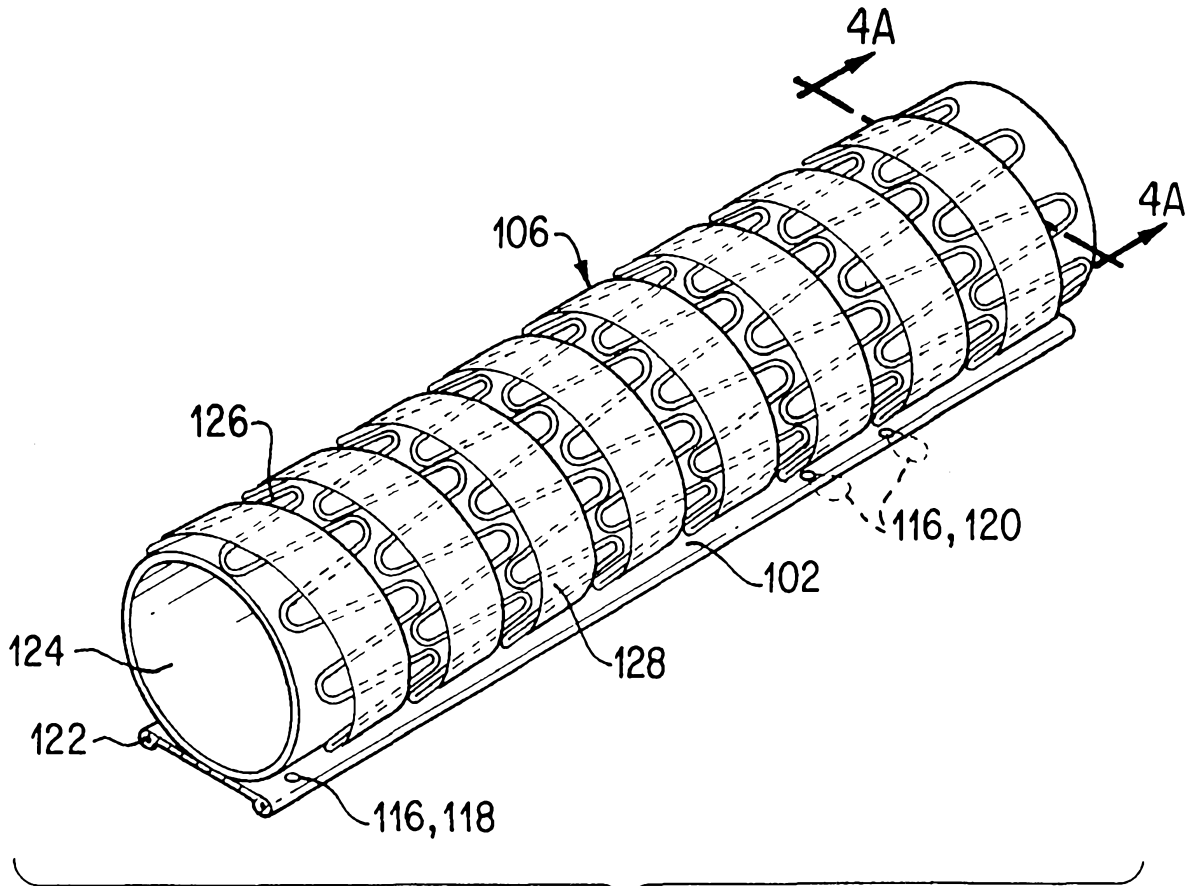


FIG. 3

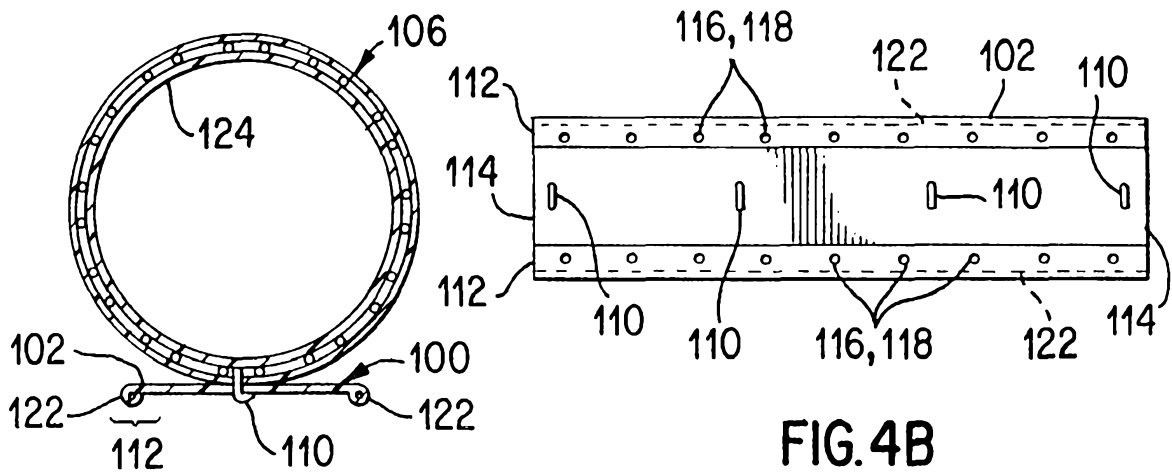


FIG. 4A

FIG. 4B

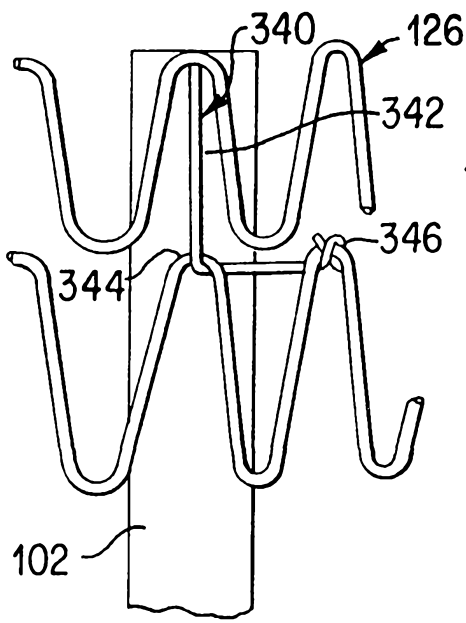


FIG. 5A

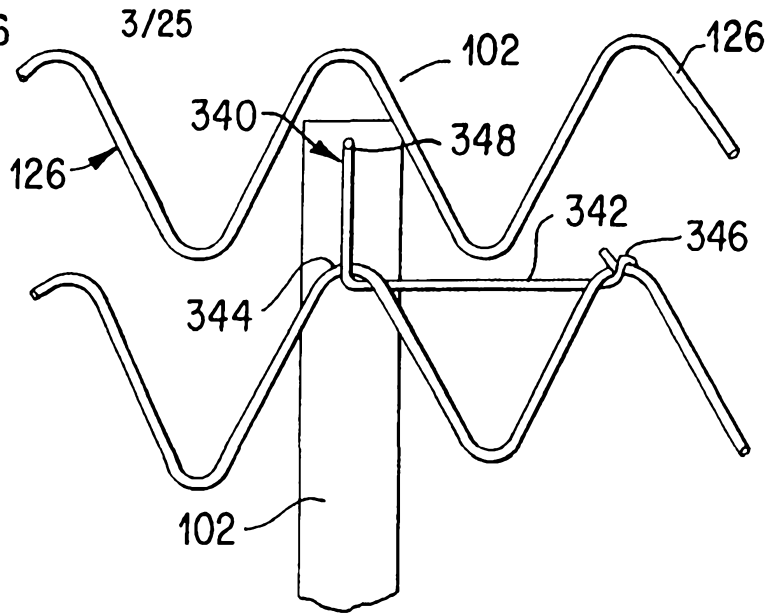


FIG. 5B

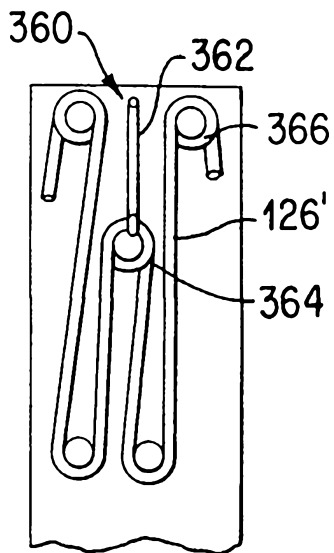


FIG. 5C

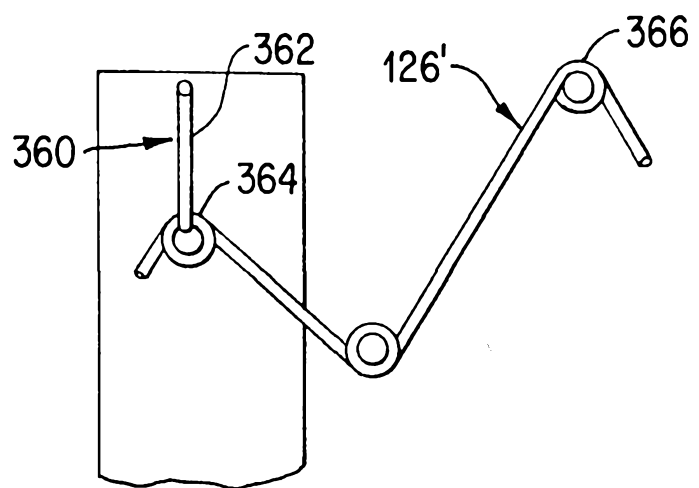


FIG. 5D

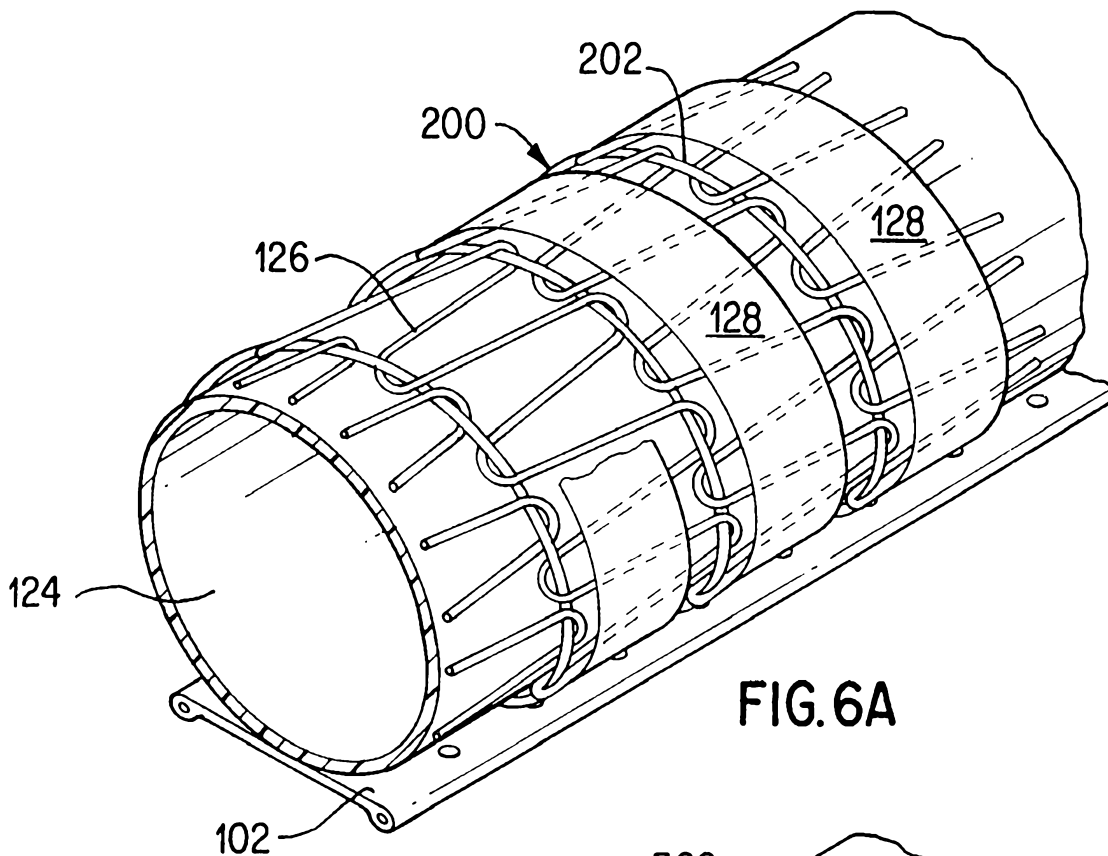


FIG. 6A

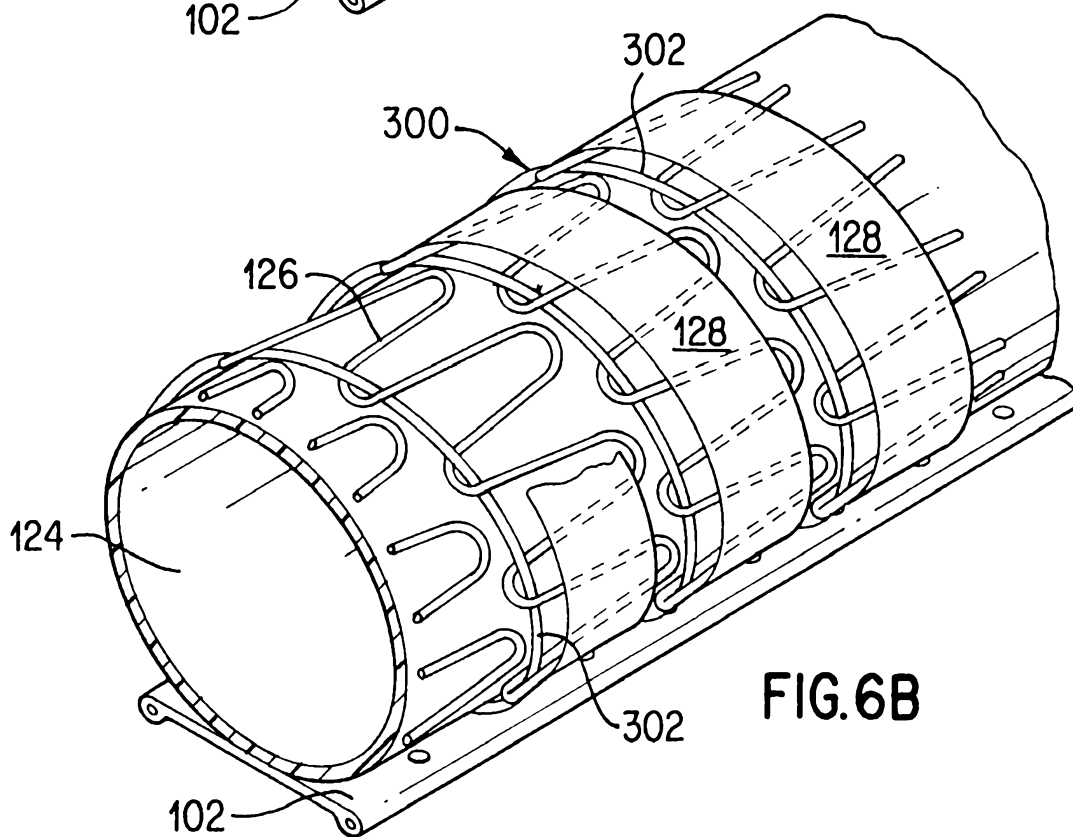


FIG. 6B

5/25

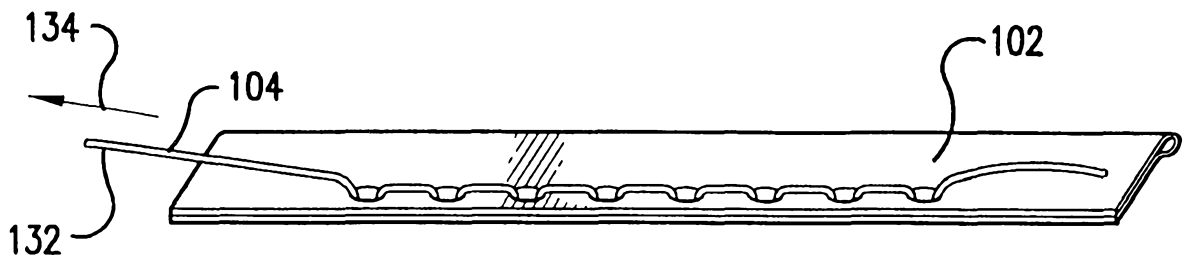


FIG. 7A

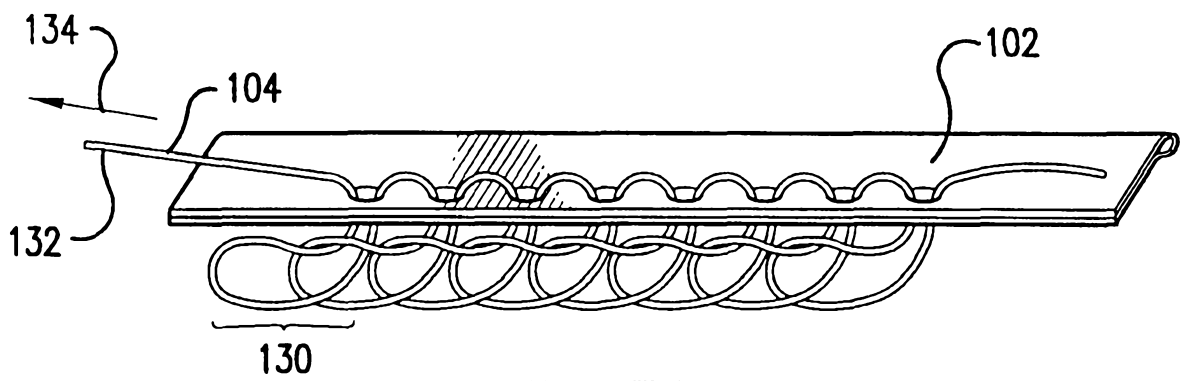


FIG. 7B

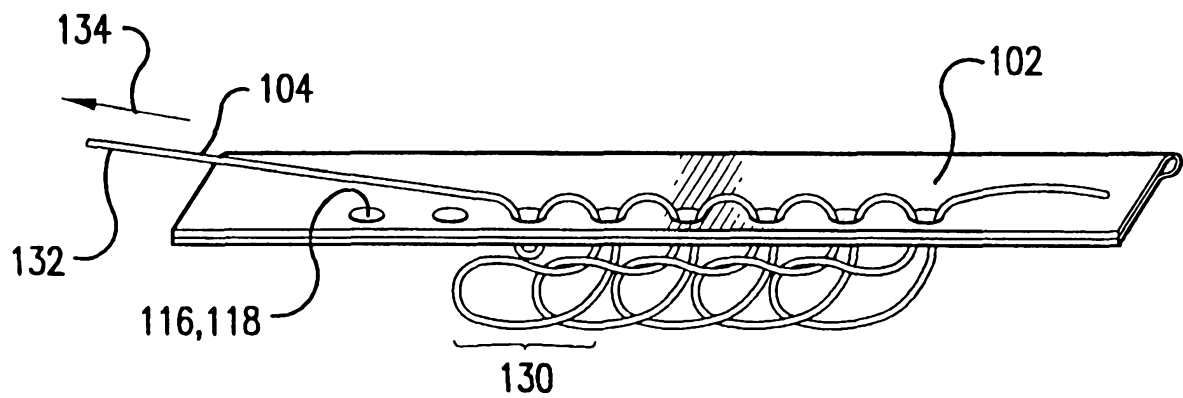


FIG. 7C

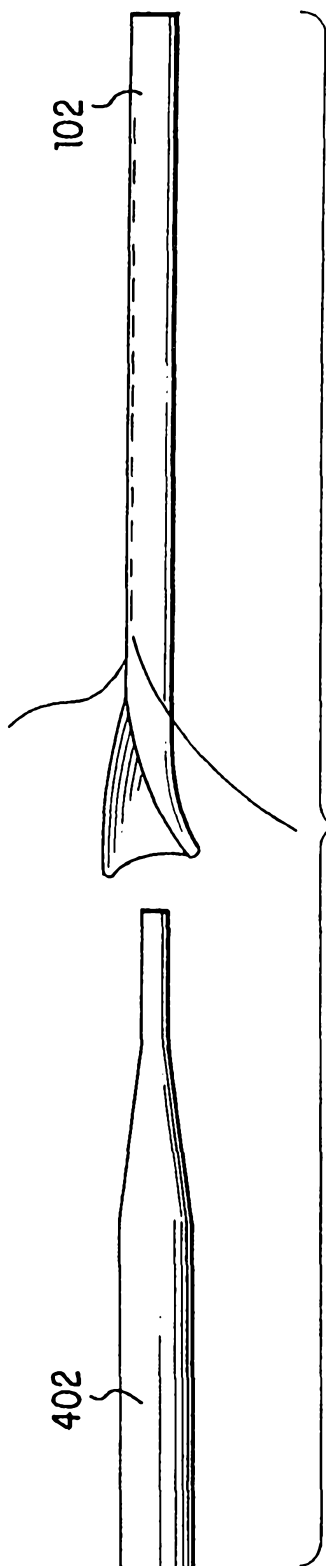


FIG. 8A

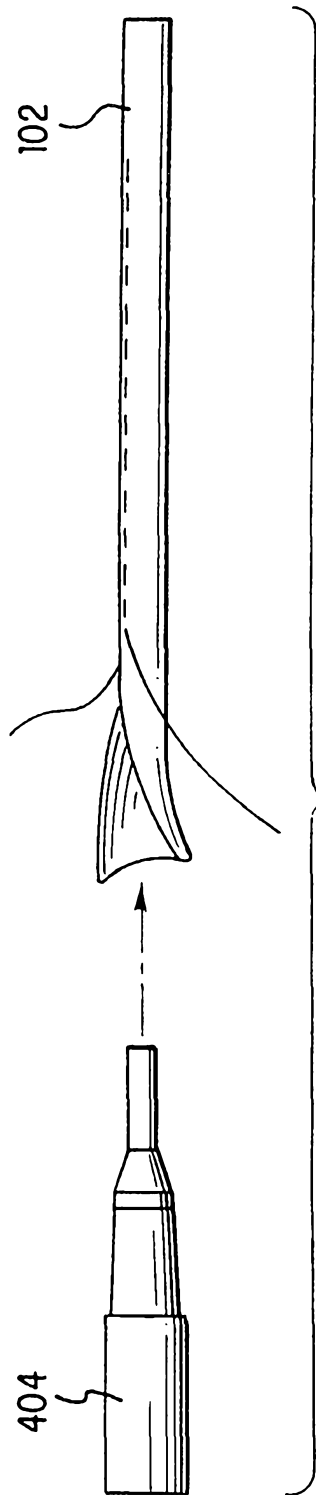


FIG. 8B

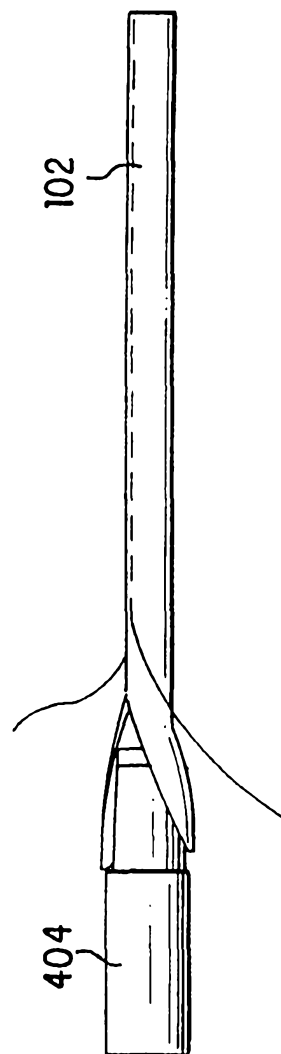


FIG. 8C

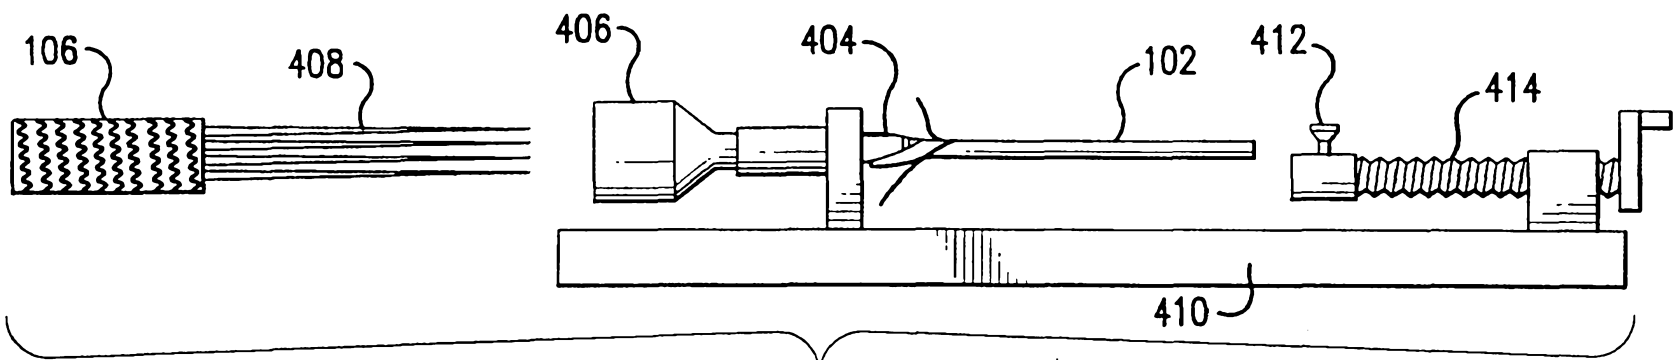


FIG. 8D

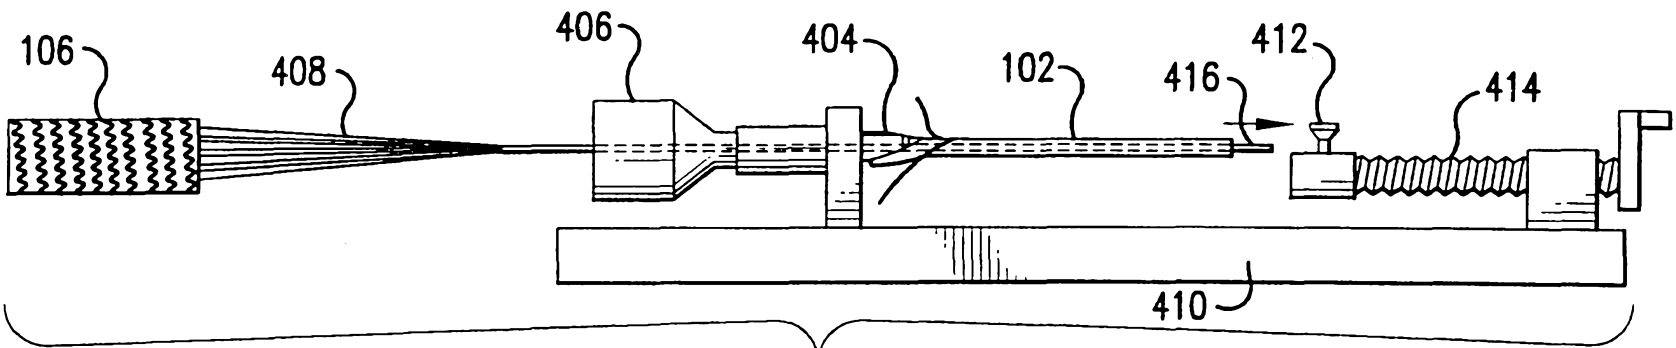


FIG. 8E

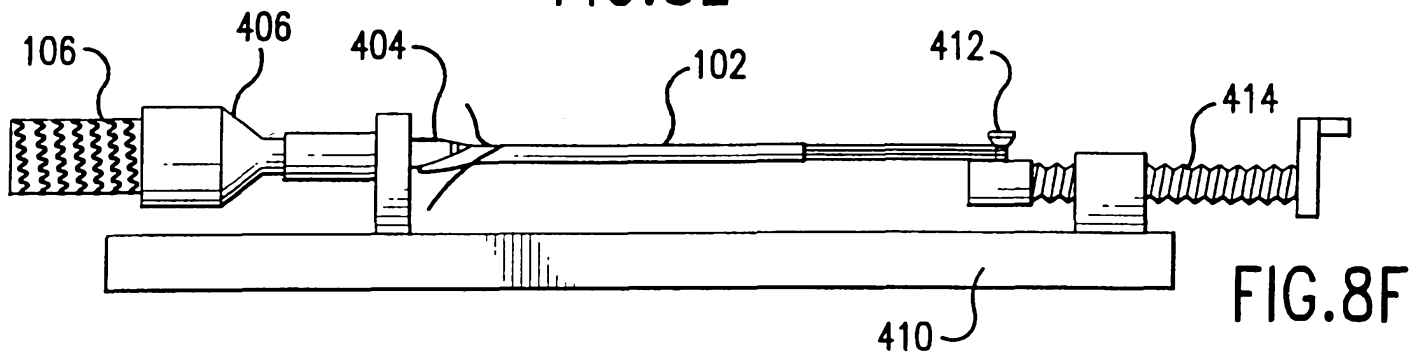
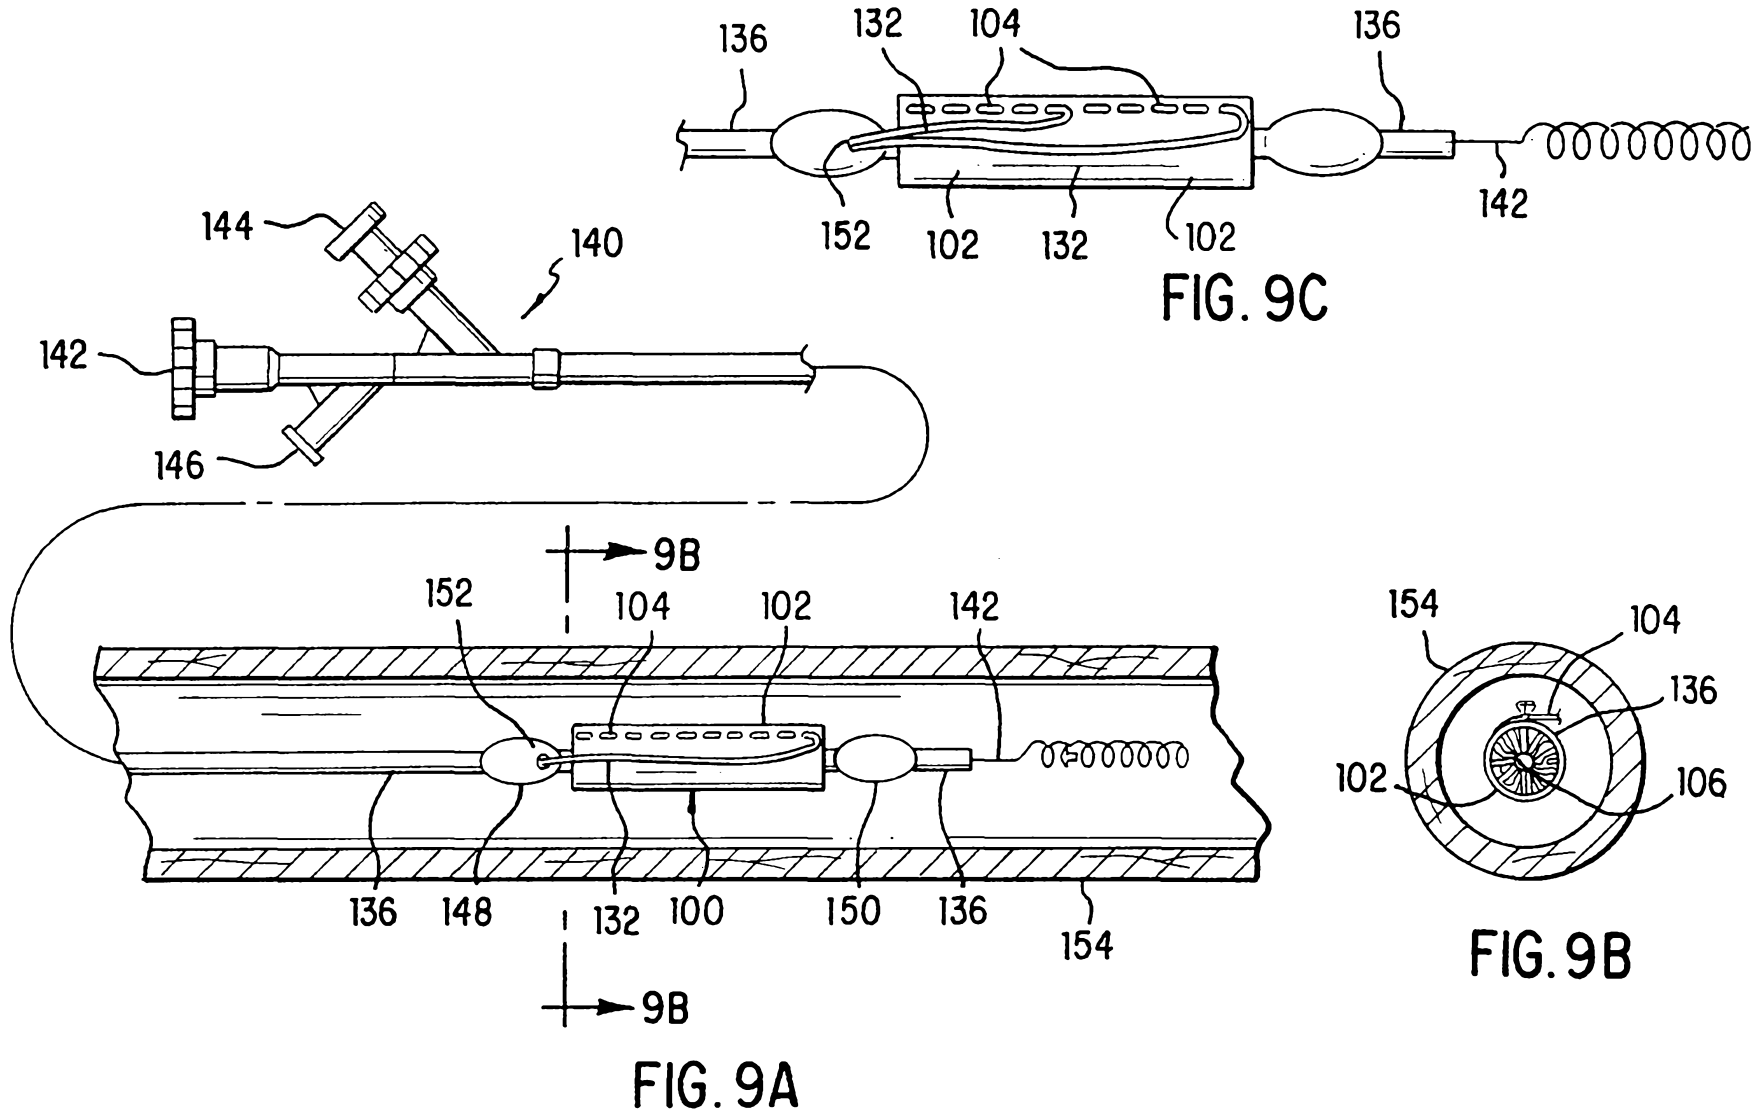


FIG. 8F



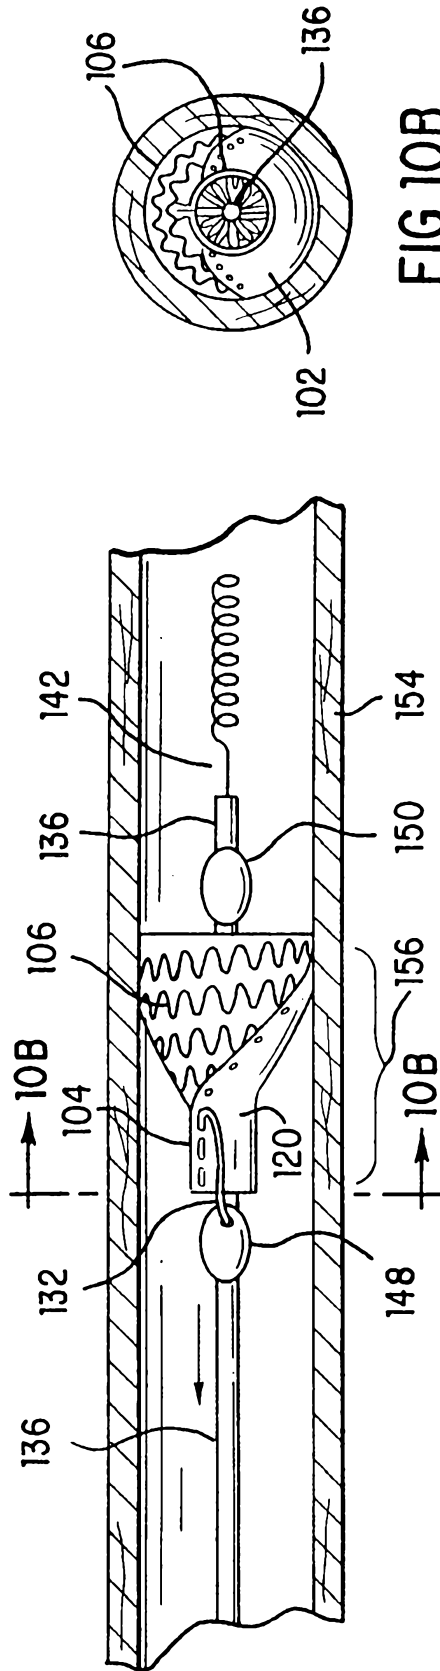


FIG. 10B

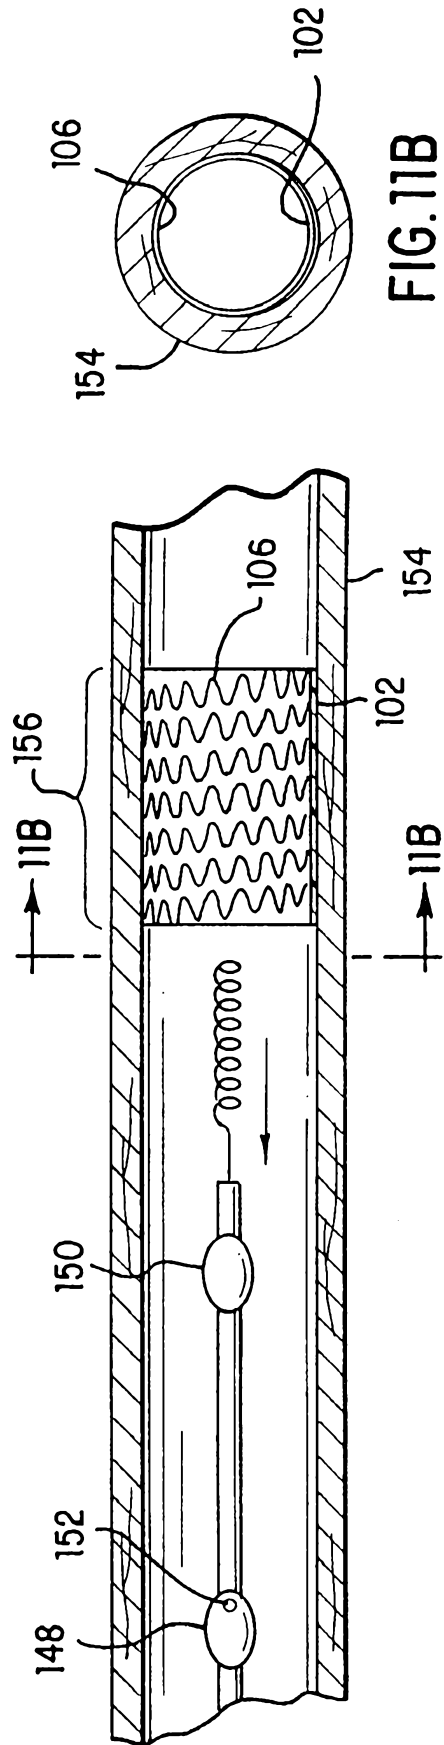


FIG. 11B

FIG. 11A

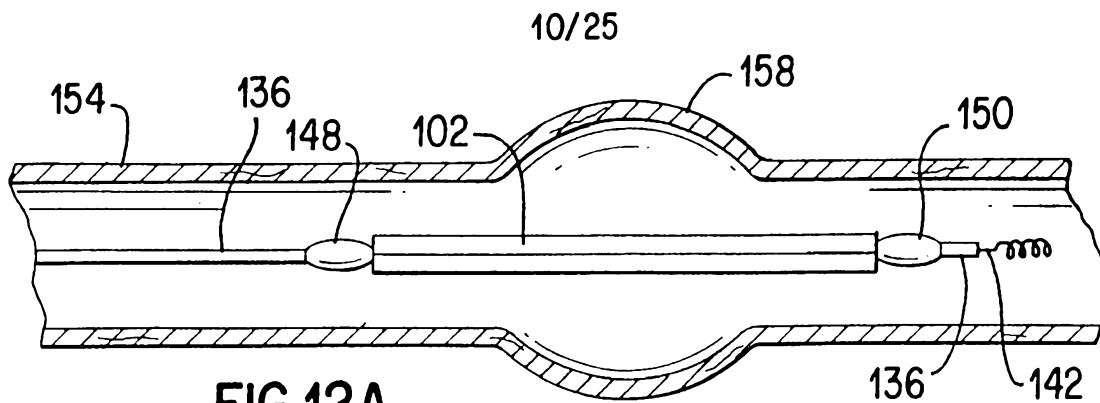


FIG. 12A

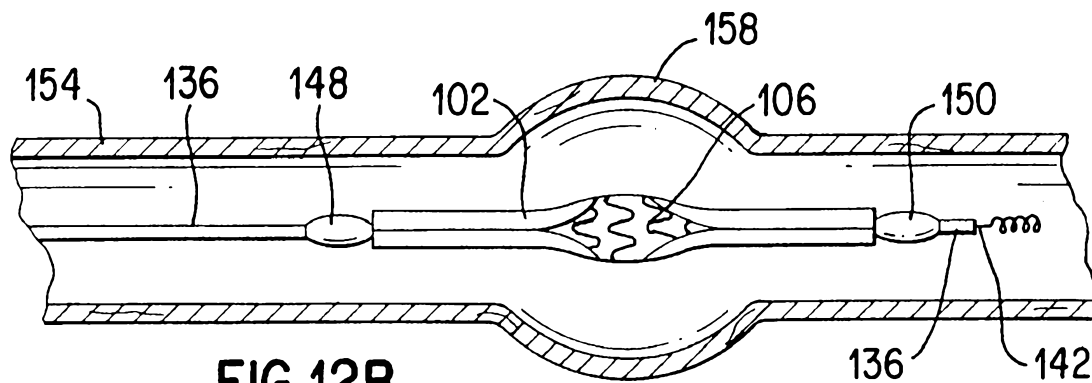


FIG. 12B

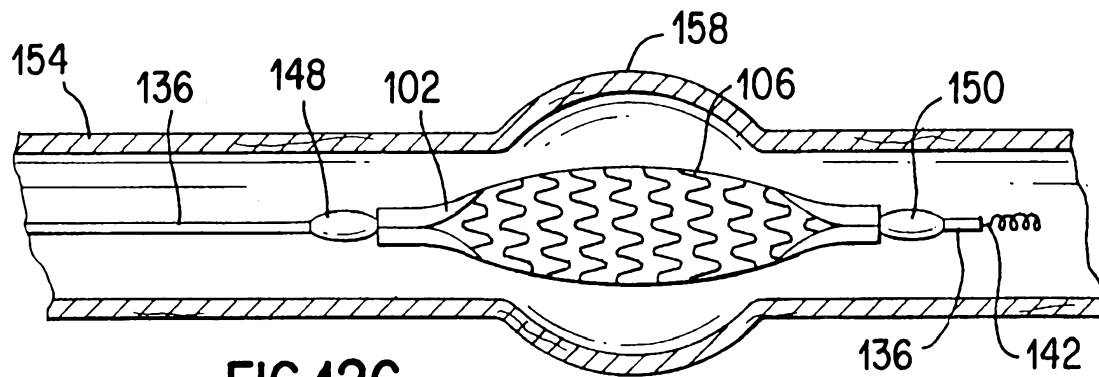


FIG. 12C

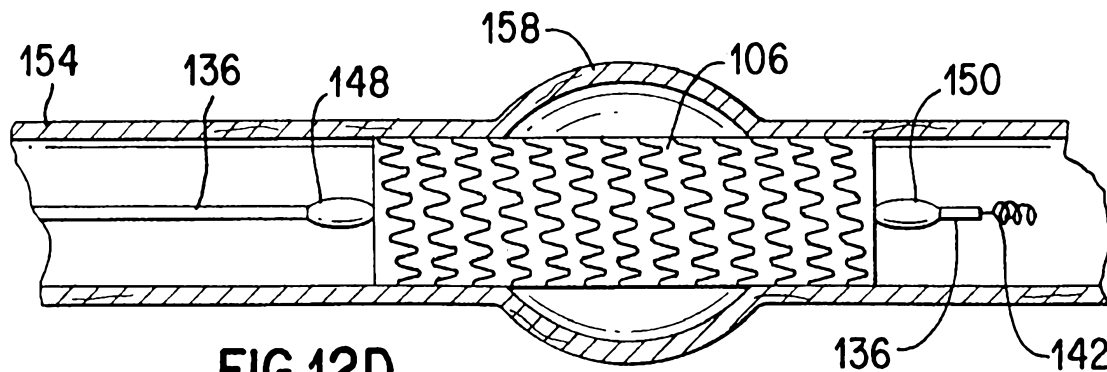


FIG. 12D

11/25

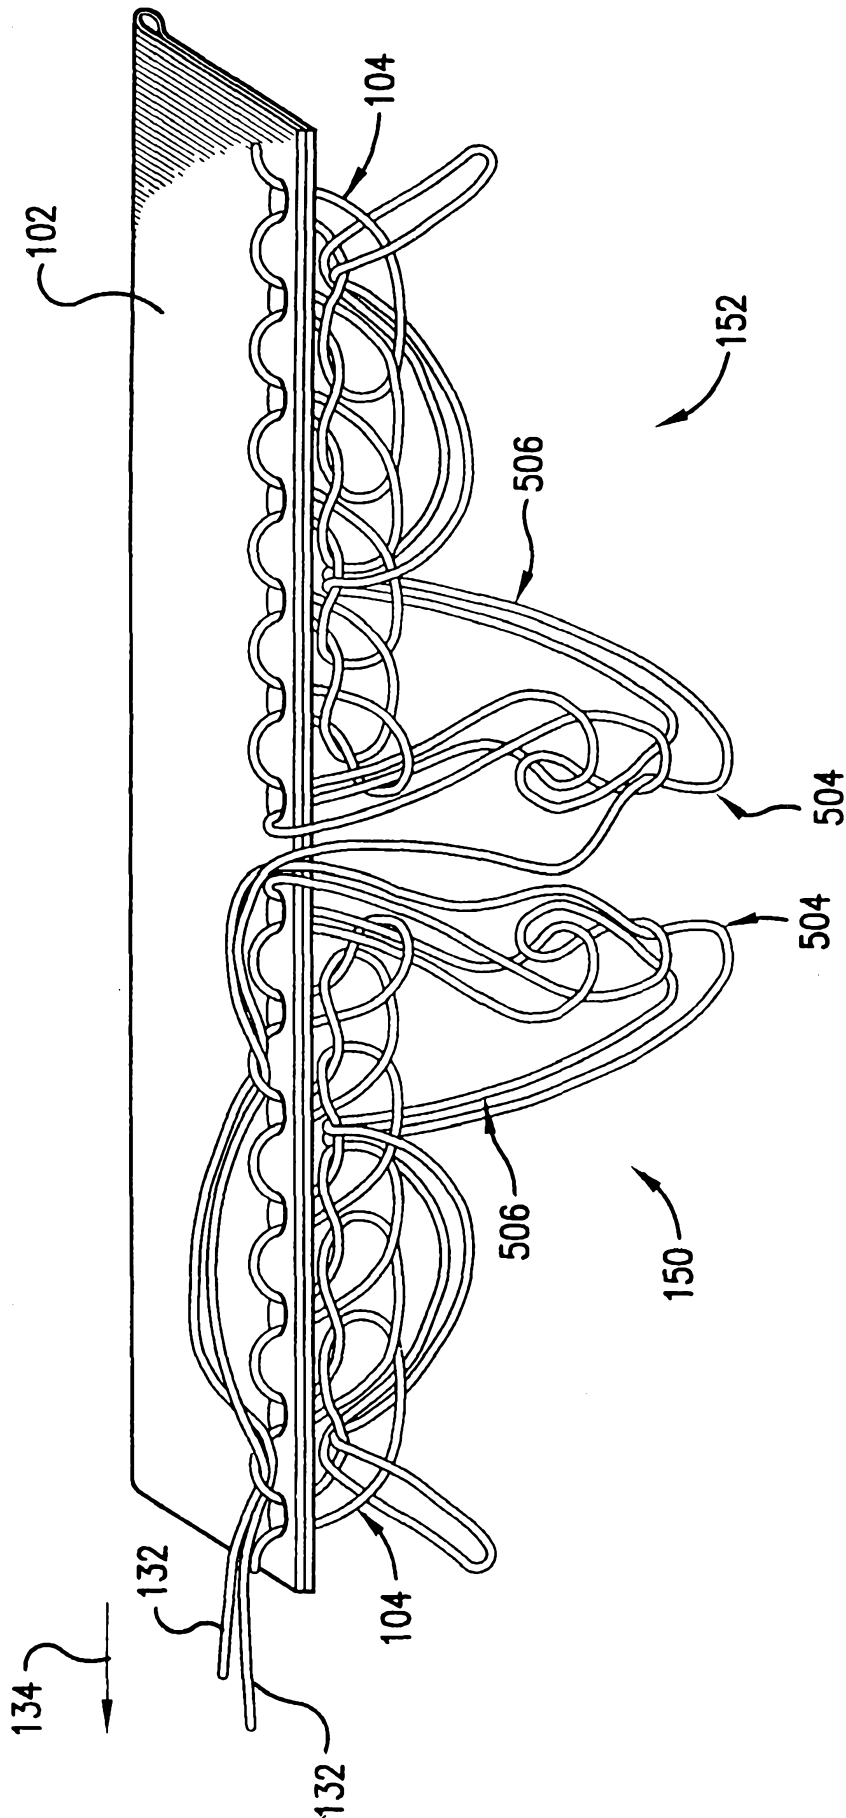
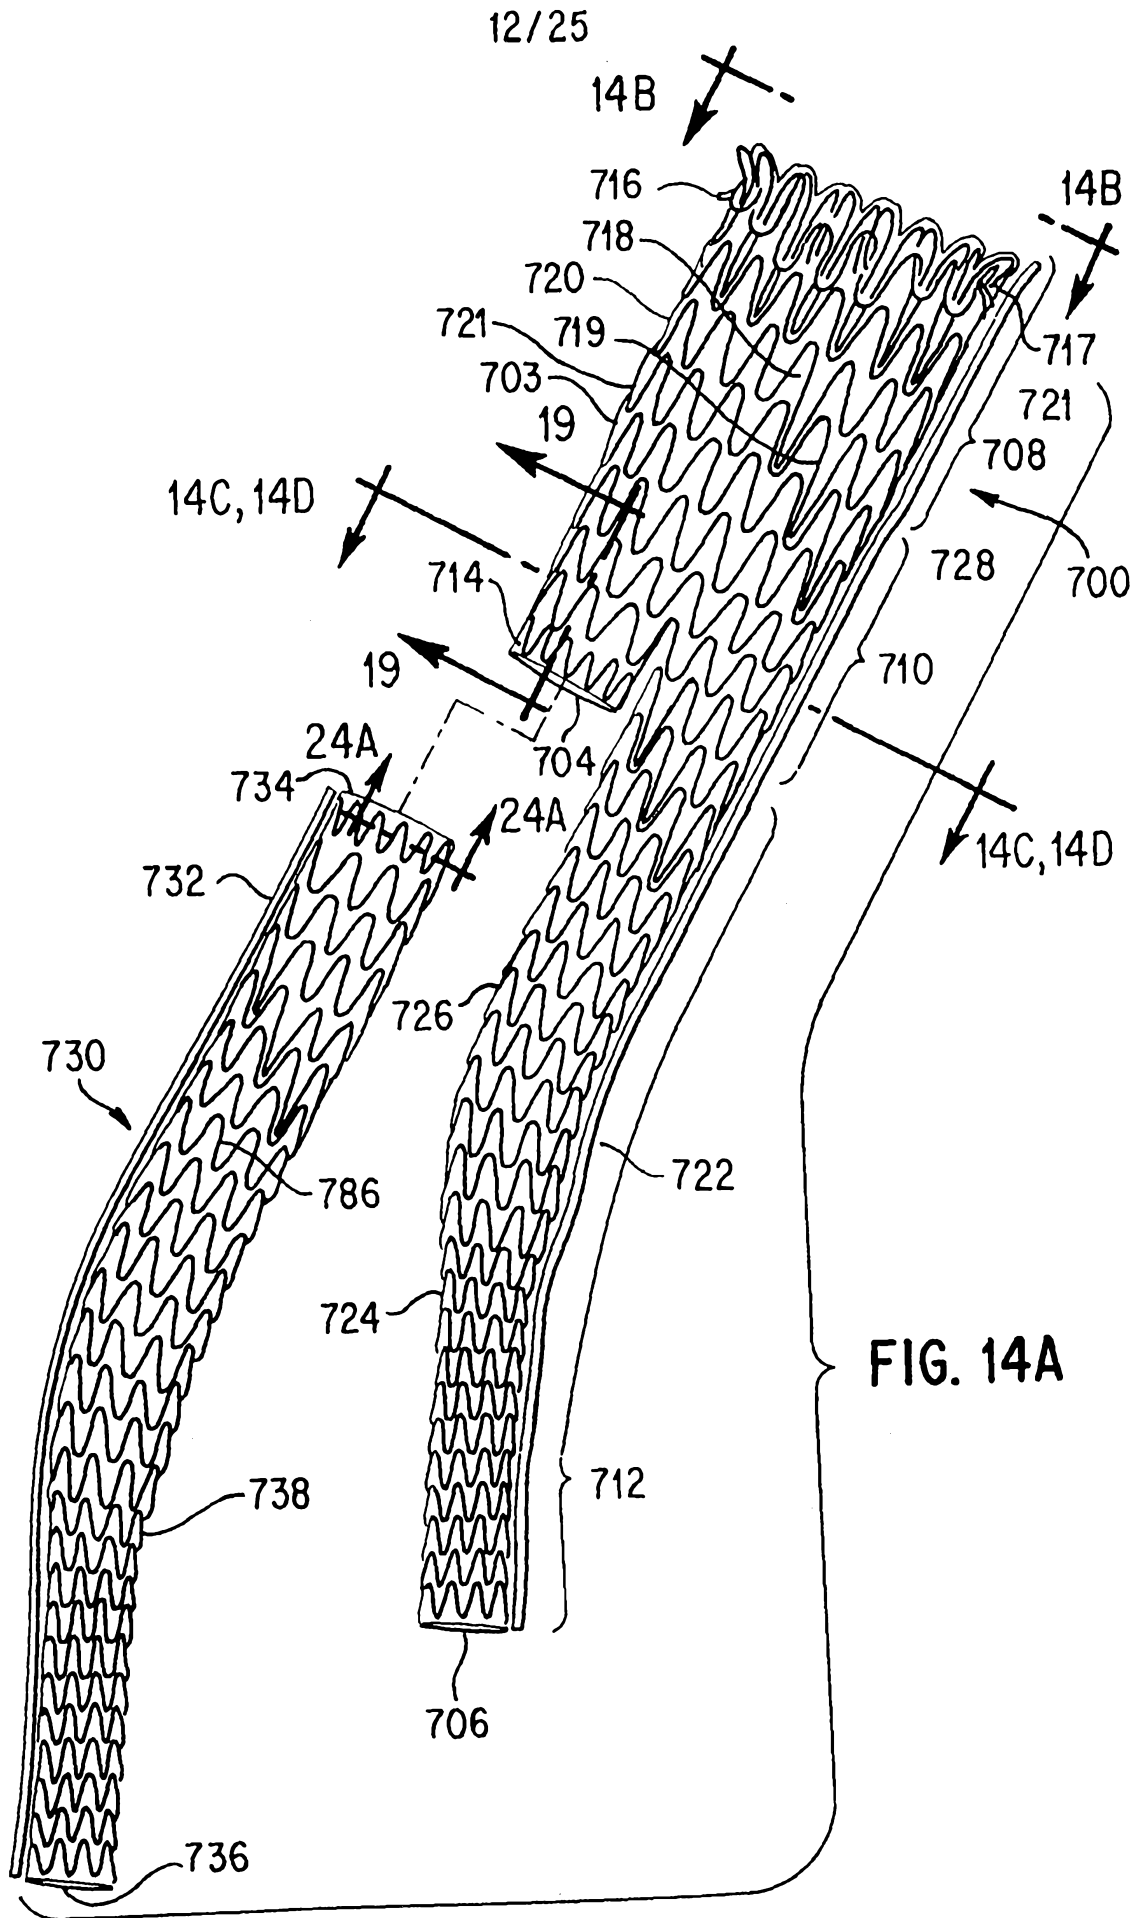


FIG.13



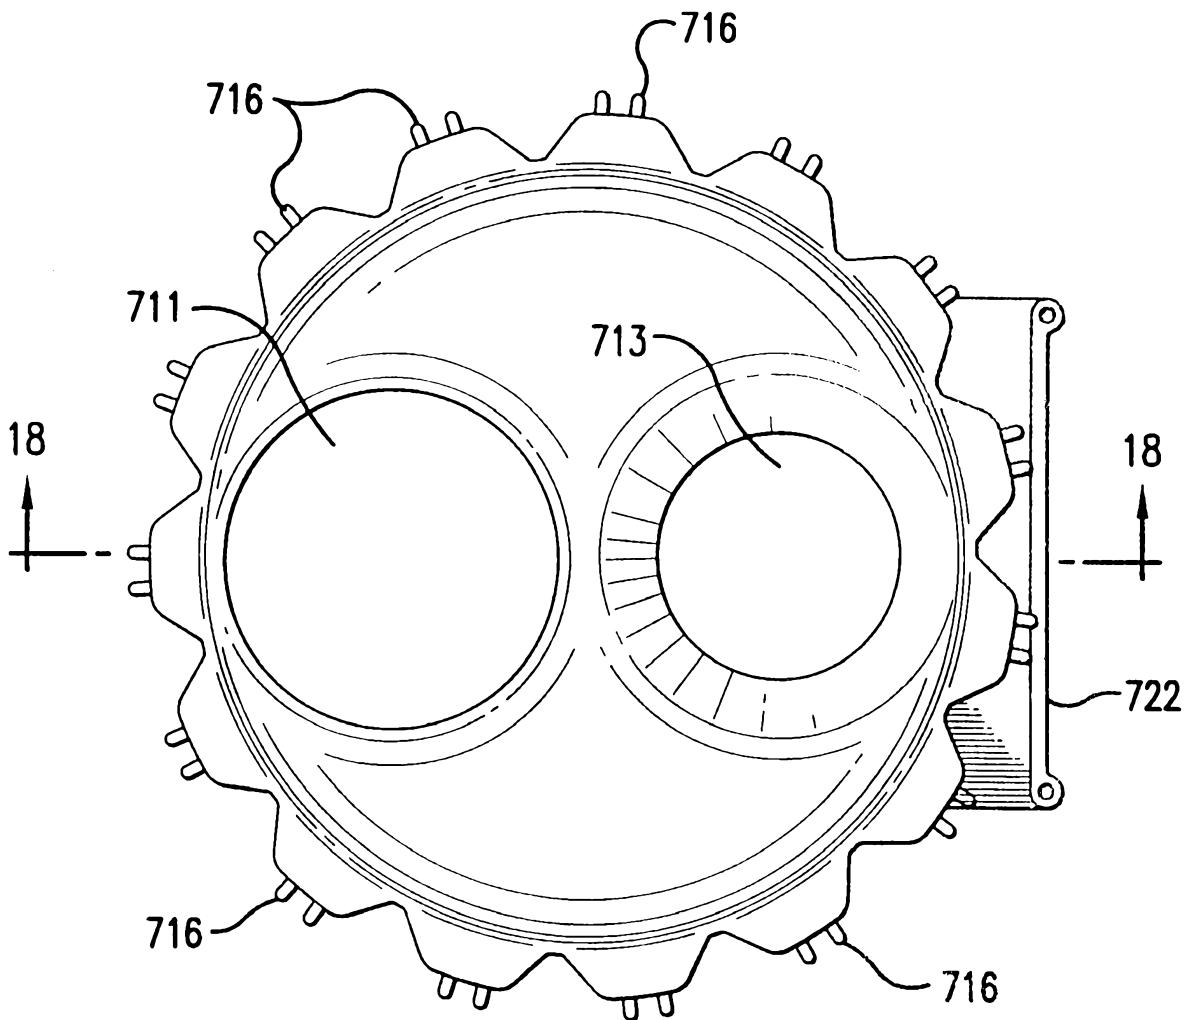


FIG.14B

14/25

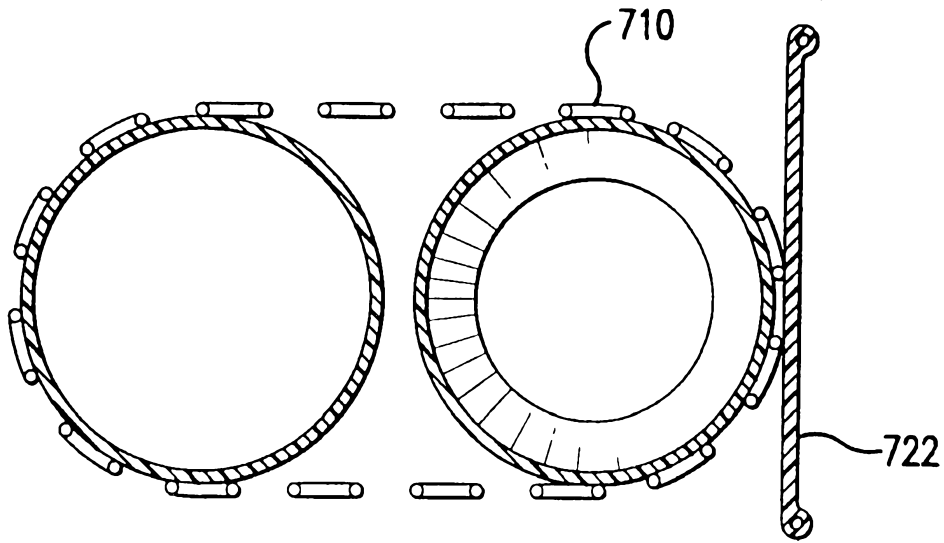


FIG. 14C


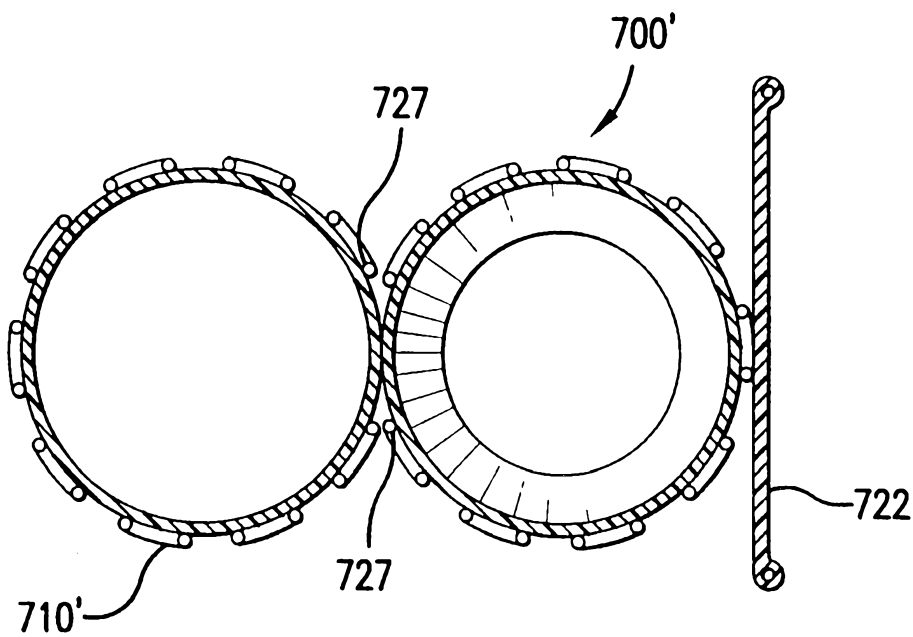


FIG. 14D

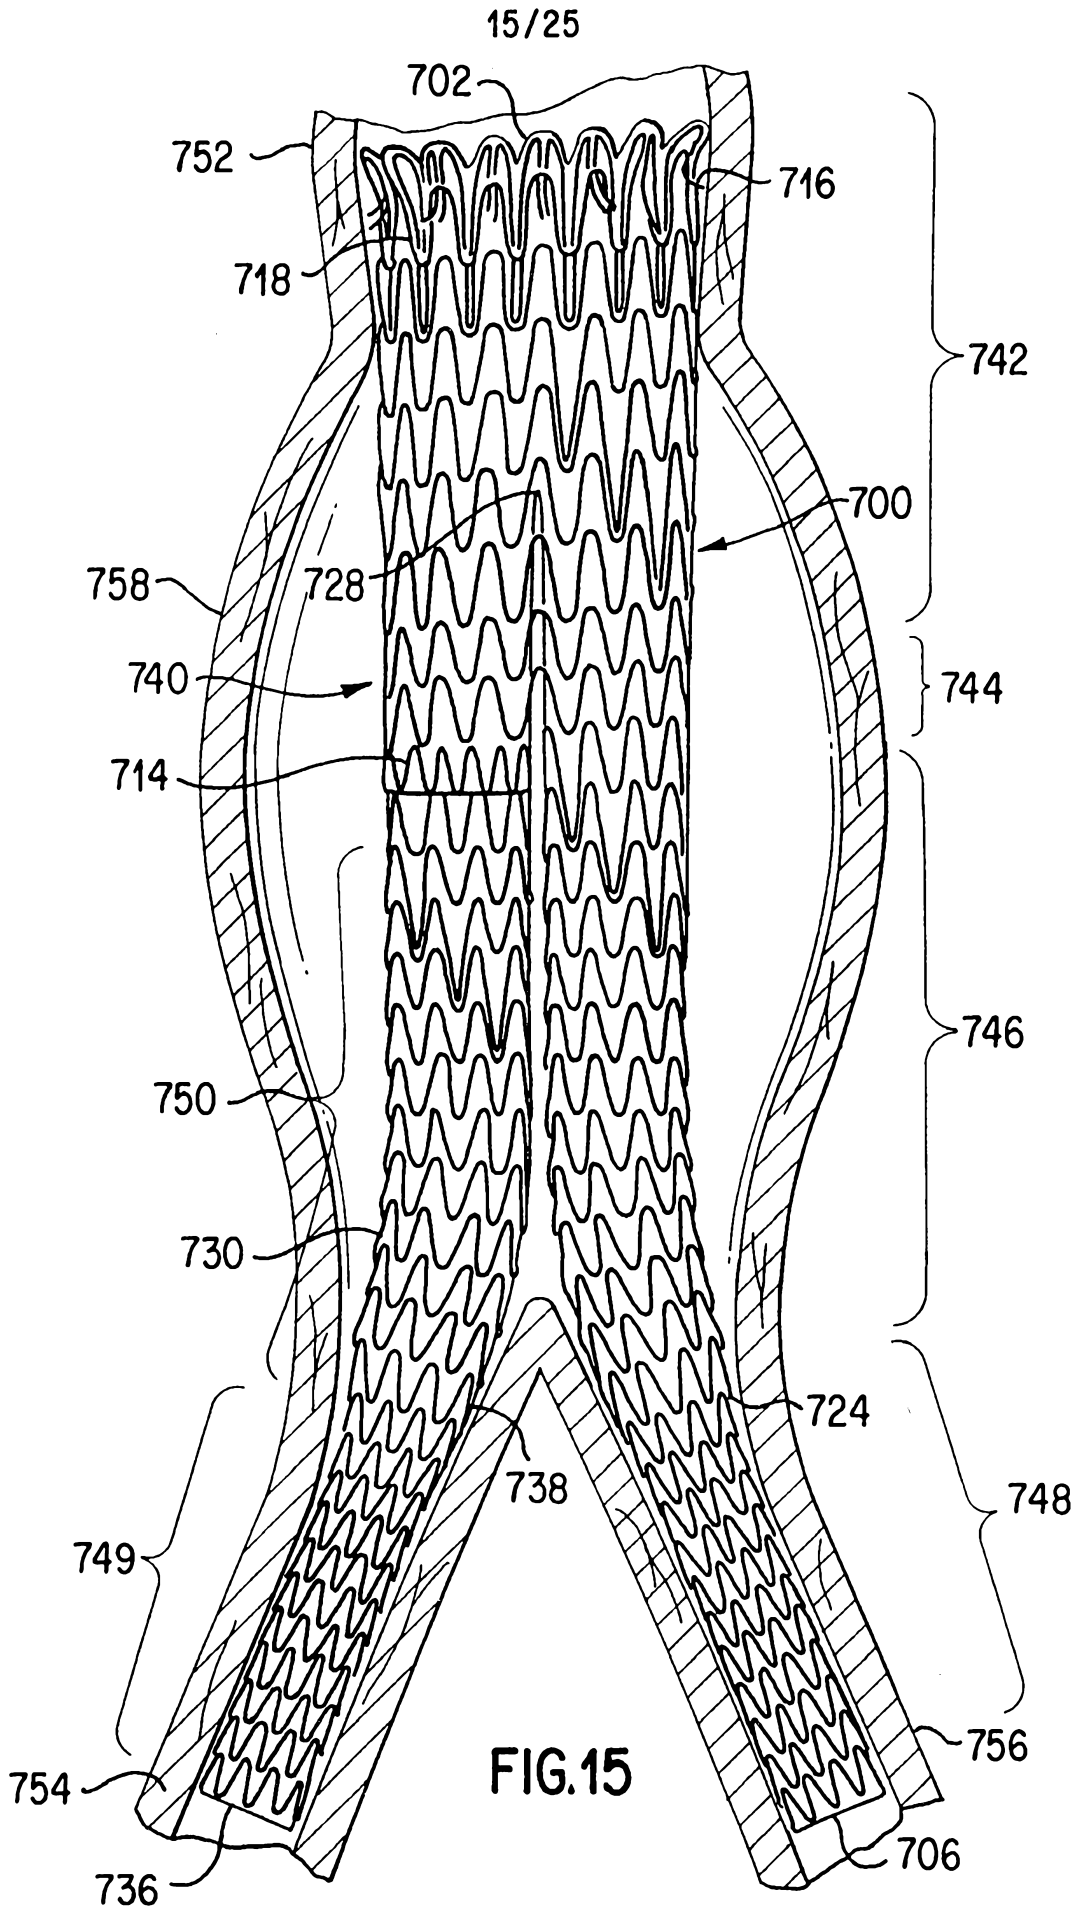

SUBSTITUTE SHEET (rule 26)

16/25

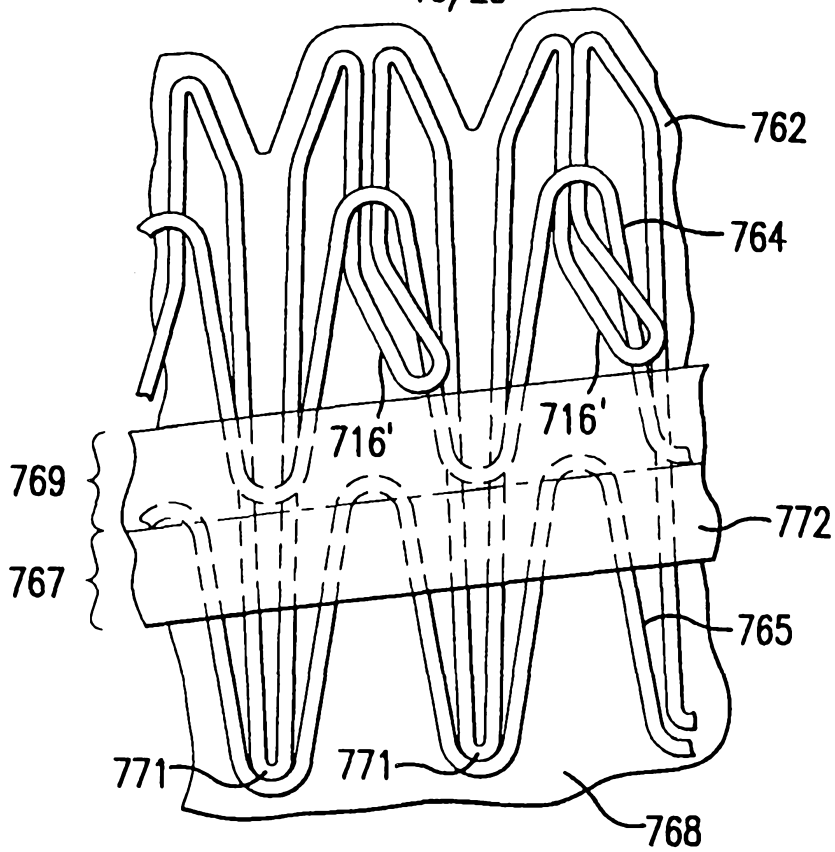


FIG. 16

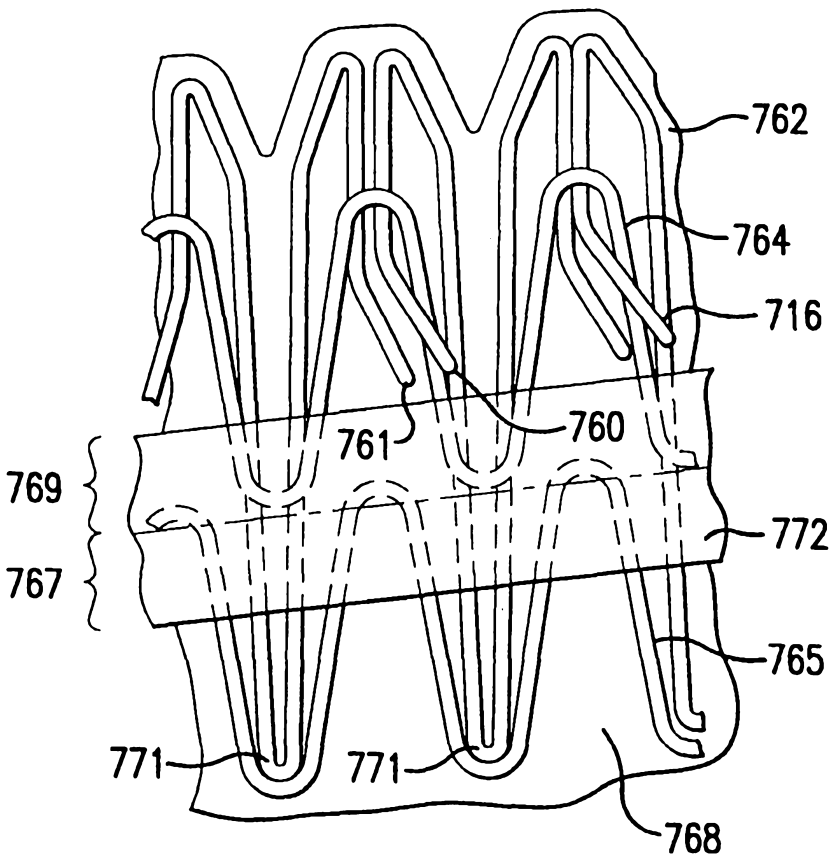


FIG. 17

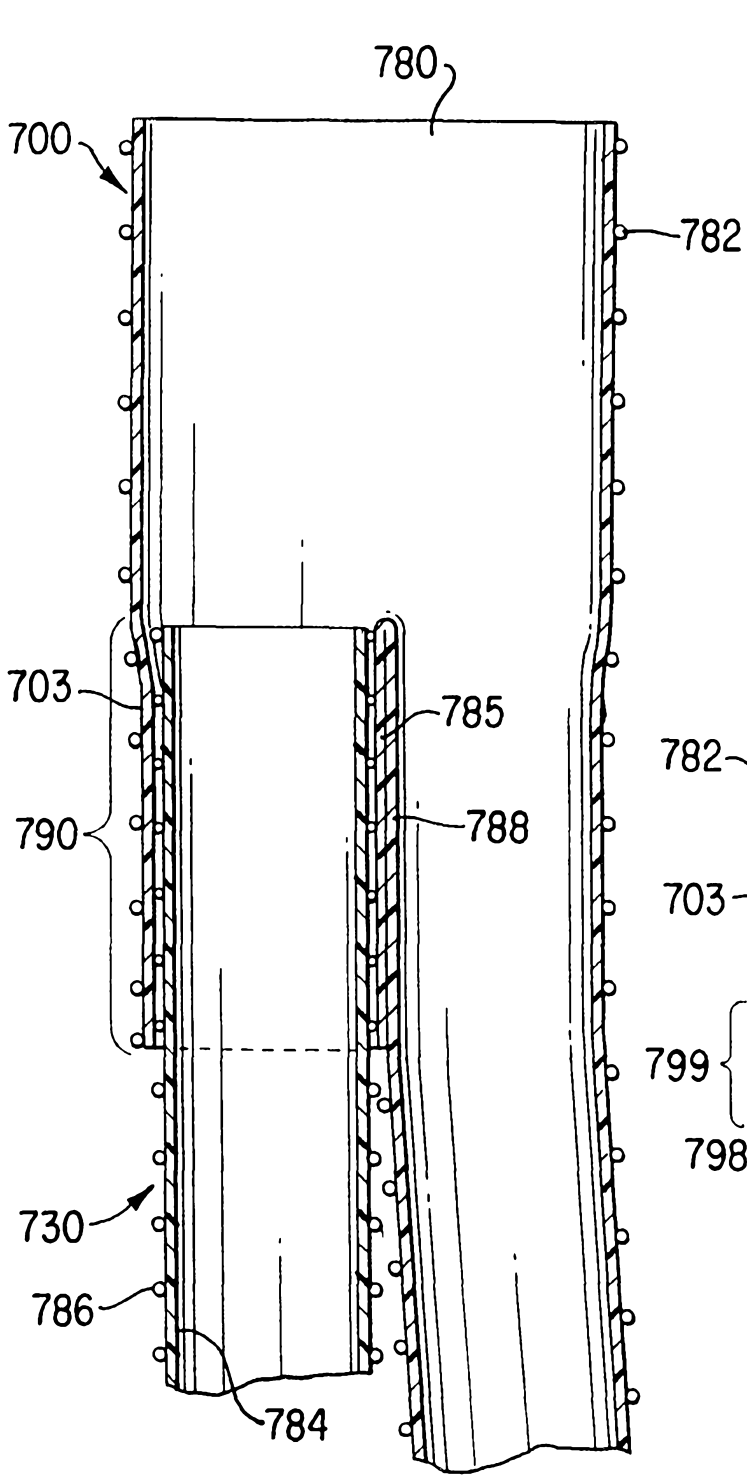


FIG. 18

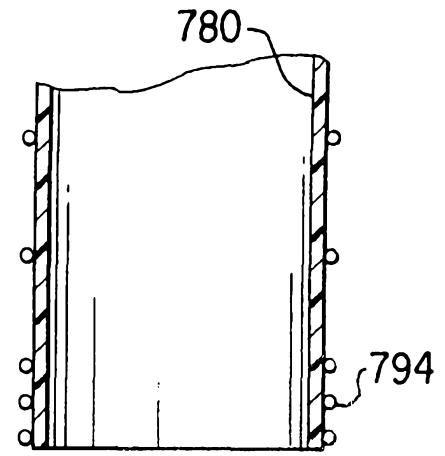


FIG. 19

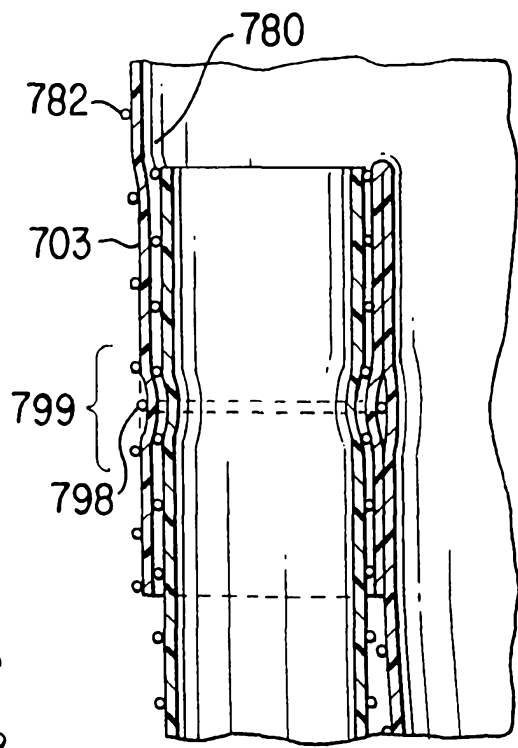


FIG. 20

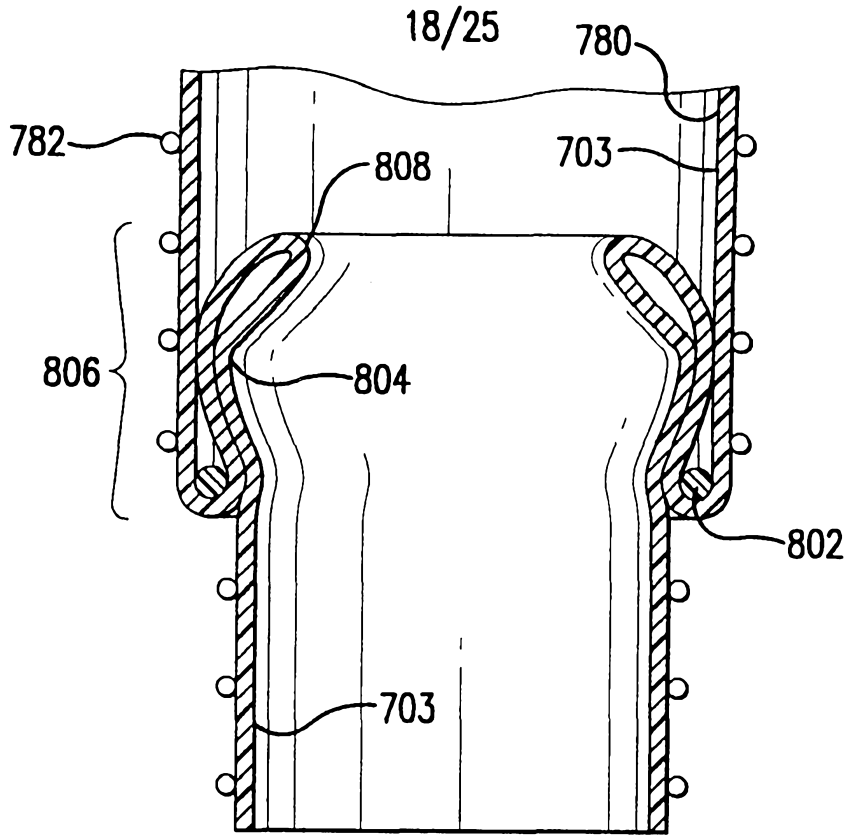


FIG. 21

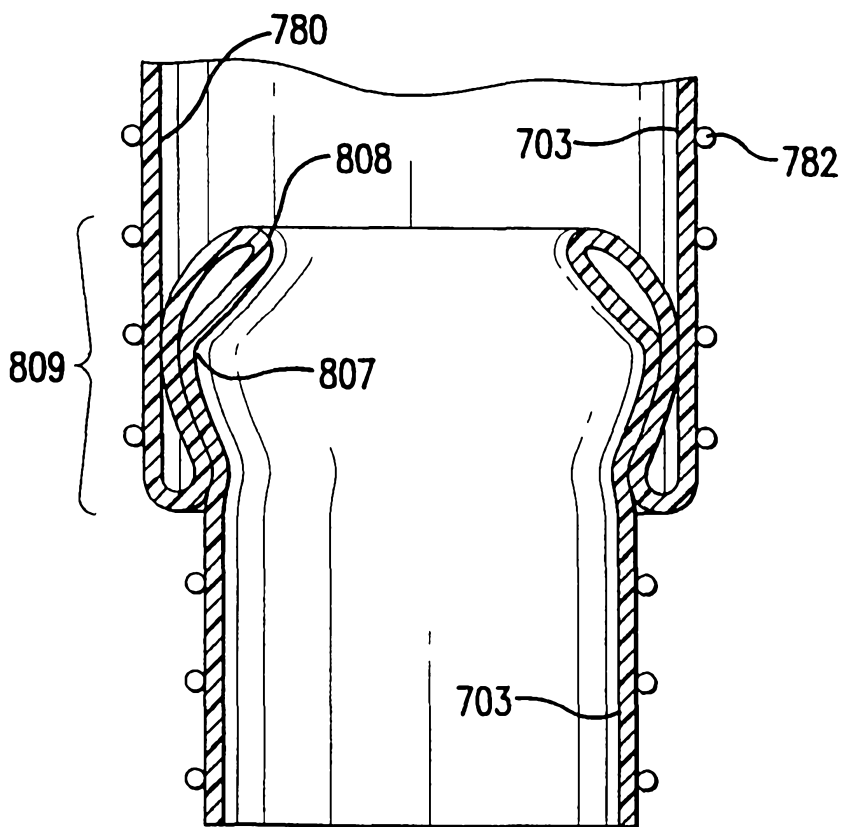


FIG. 22

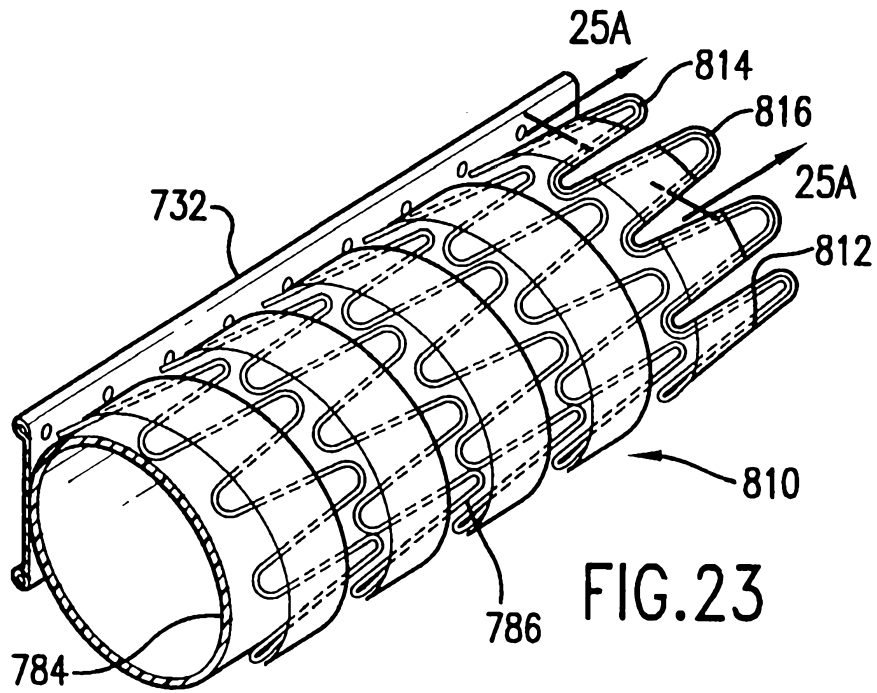


FIG. 23

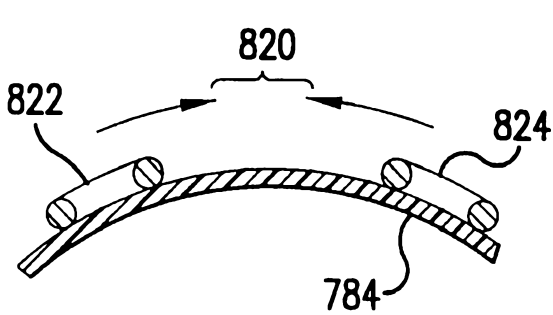


FIG. 24A

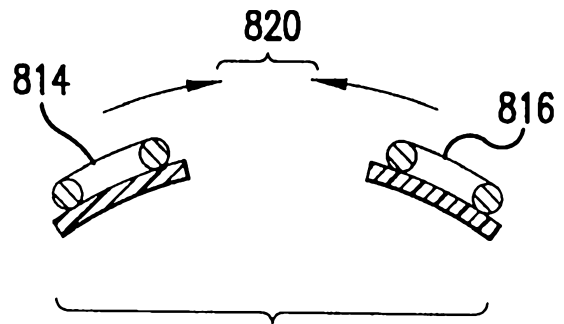


FIG. 25A

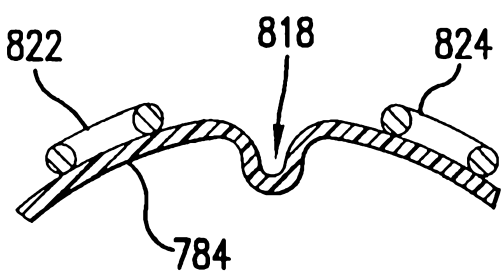


FIG. 24B

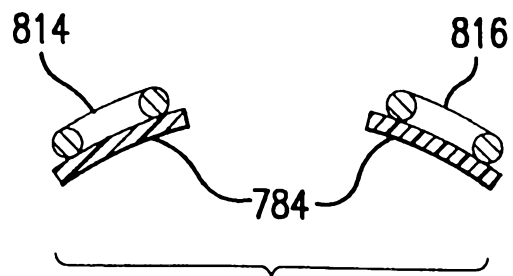


FIG. 25B

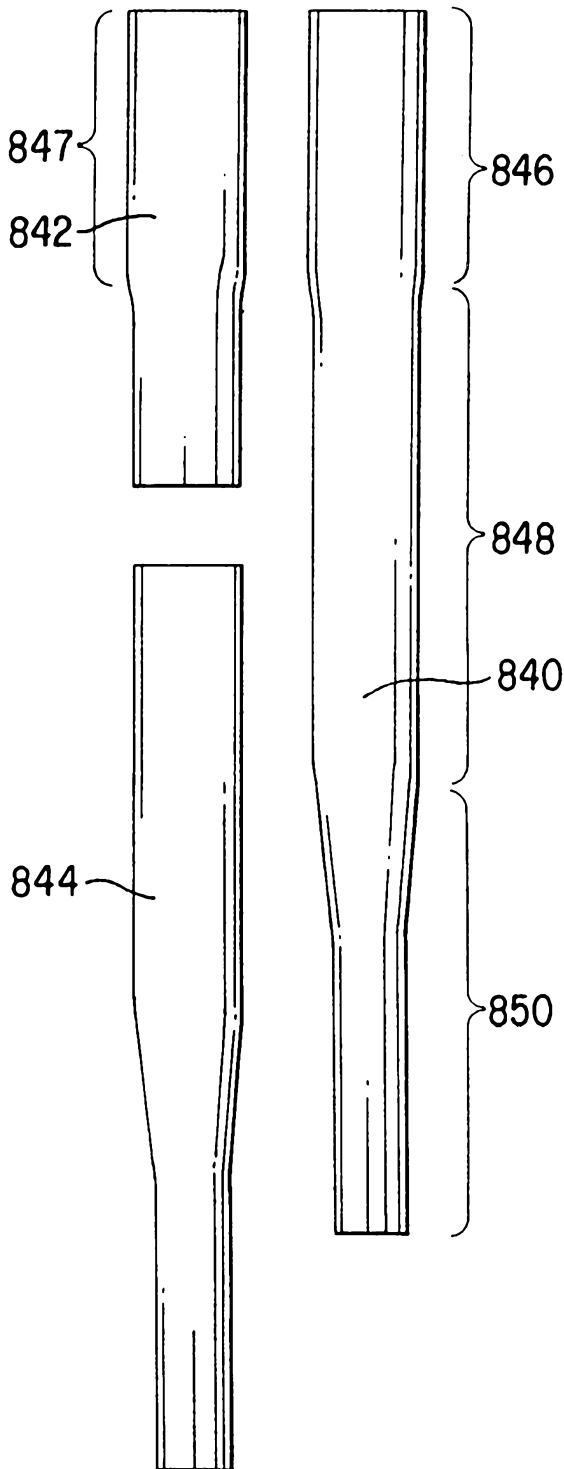


FIG. 26A

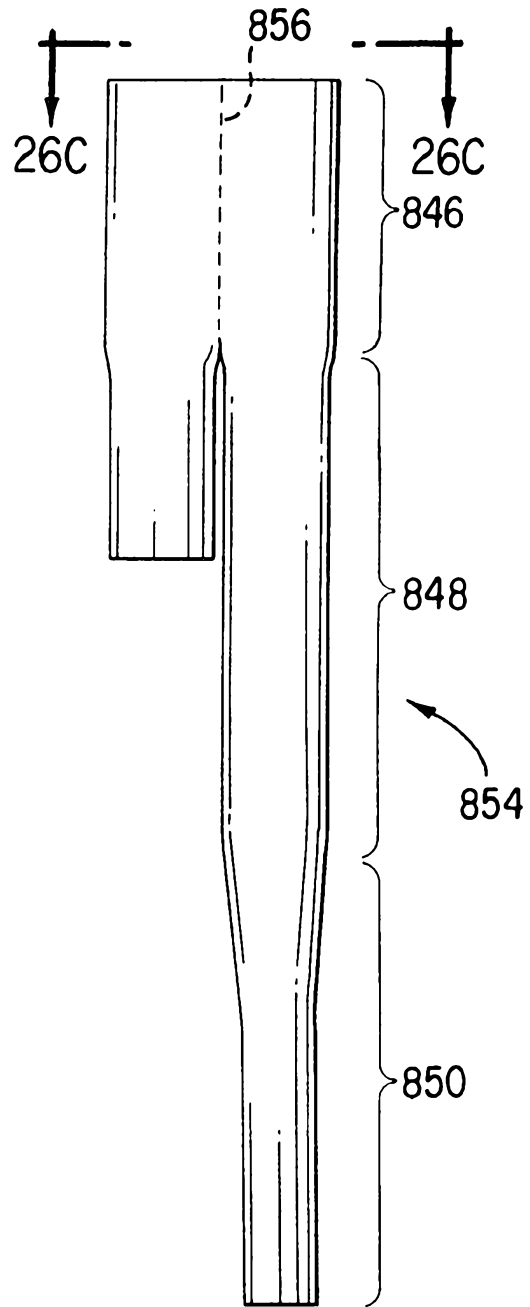


FIG. 26B

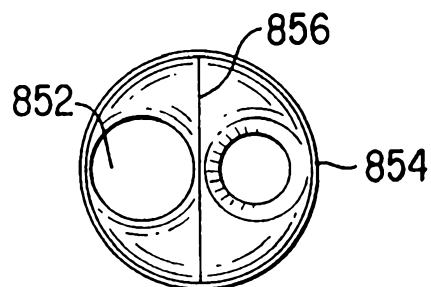


FIG. 26C

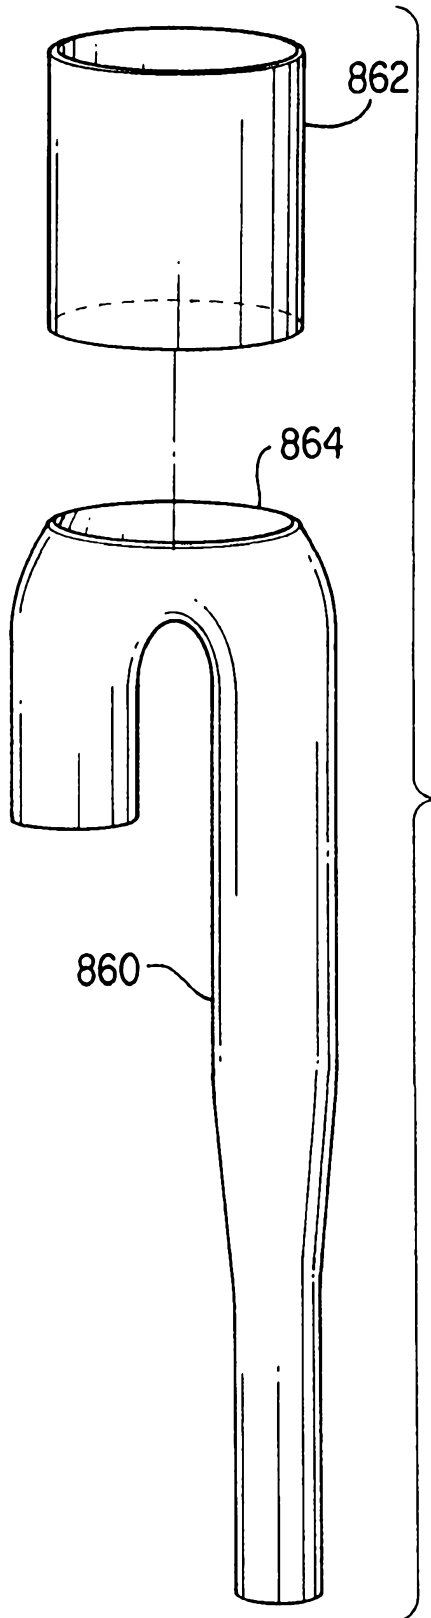


FIG. 27A

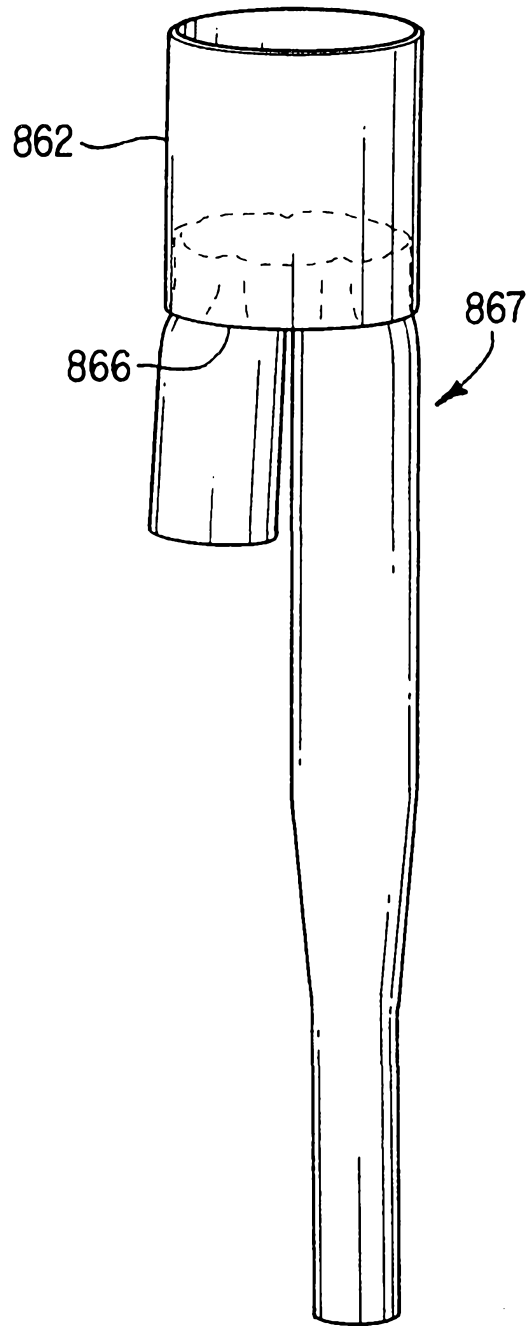


FIG. 27B

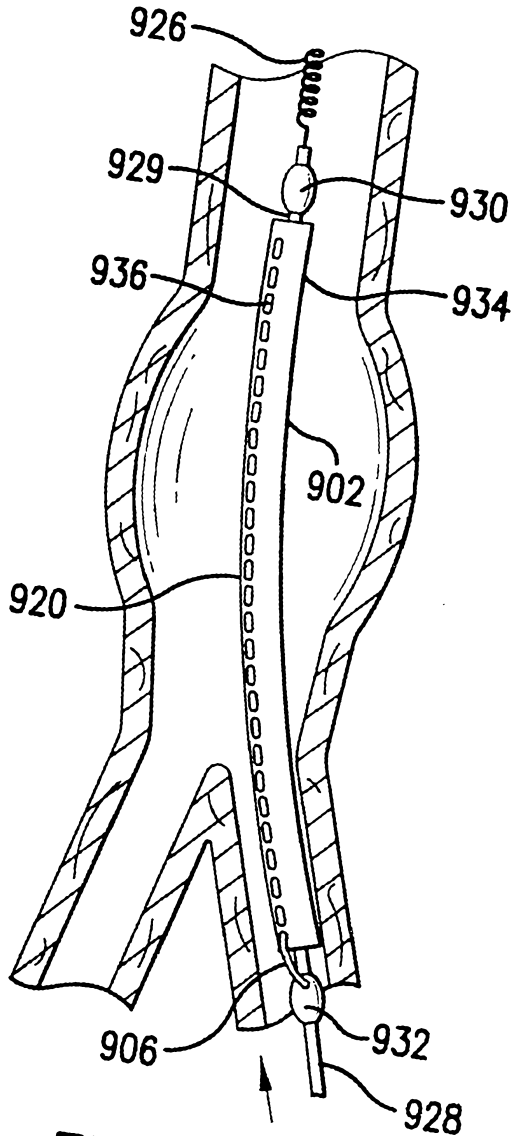


FIG. 28A

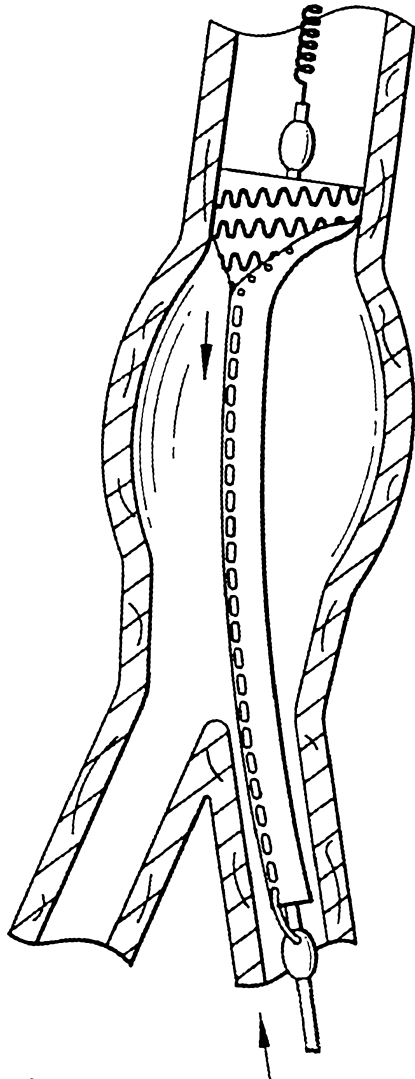


FIG. 28B

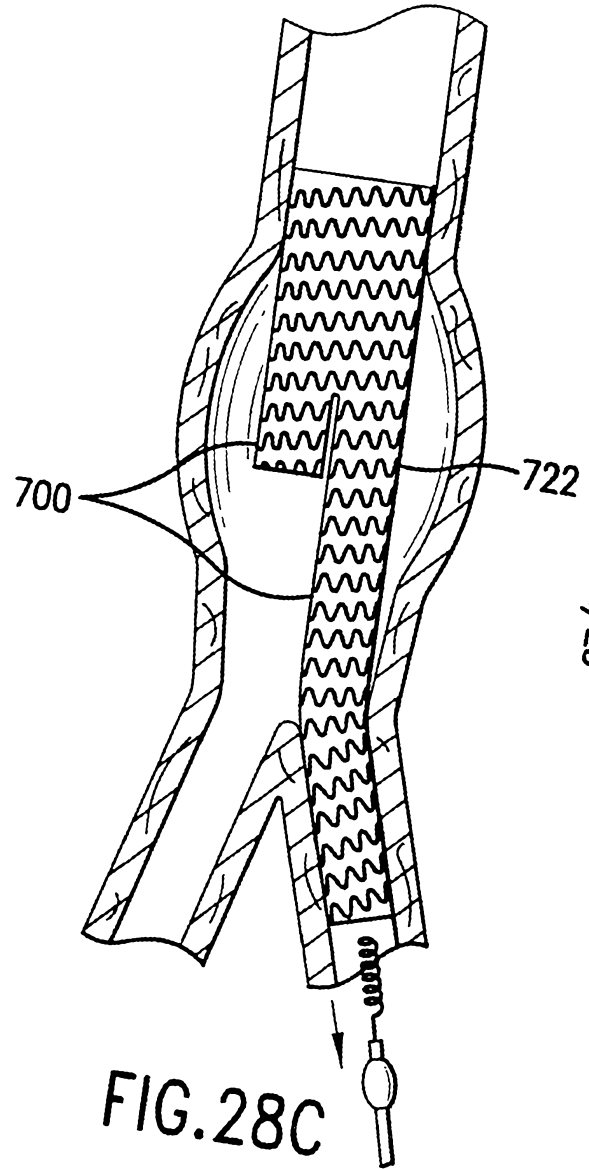


FIG. 28C

22/25

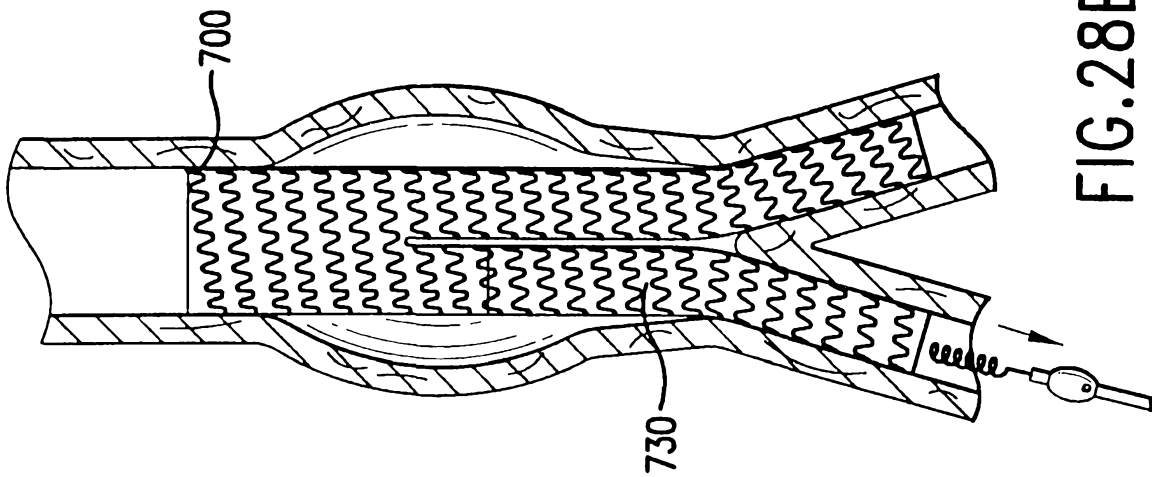


FIG. 28E

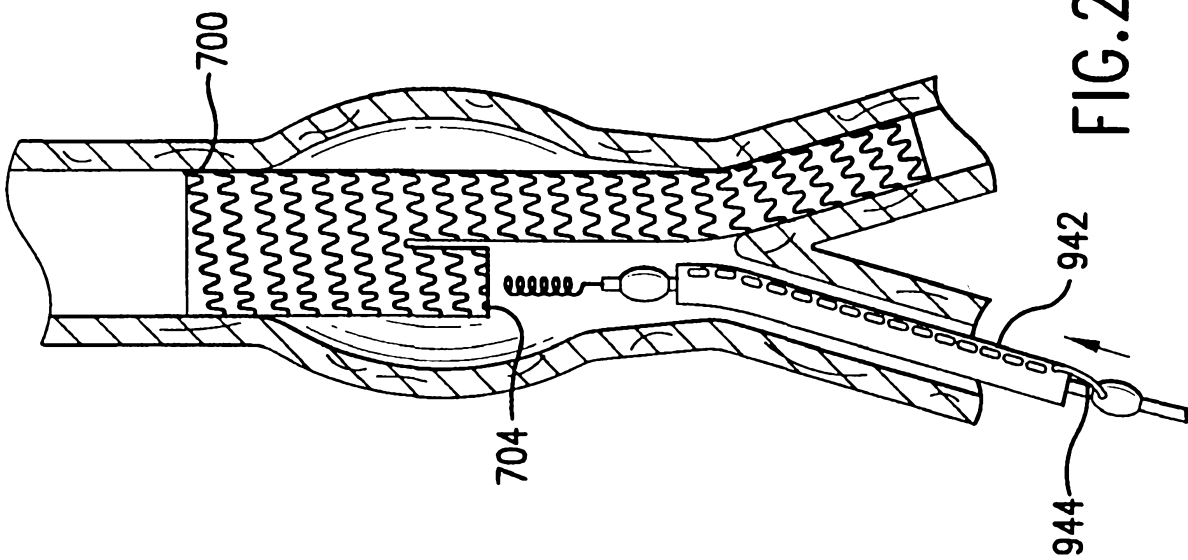


FIG. 28D

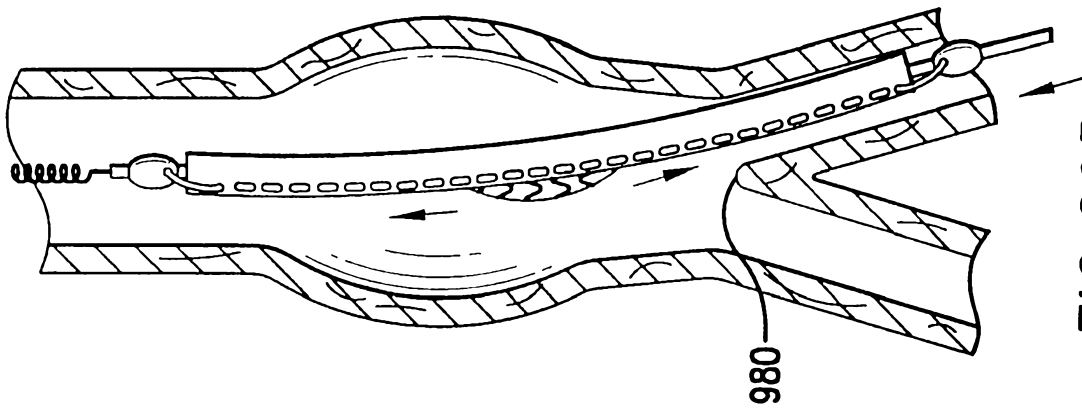


FIG. 29B

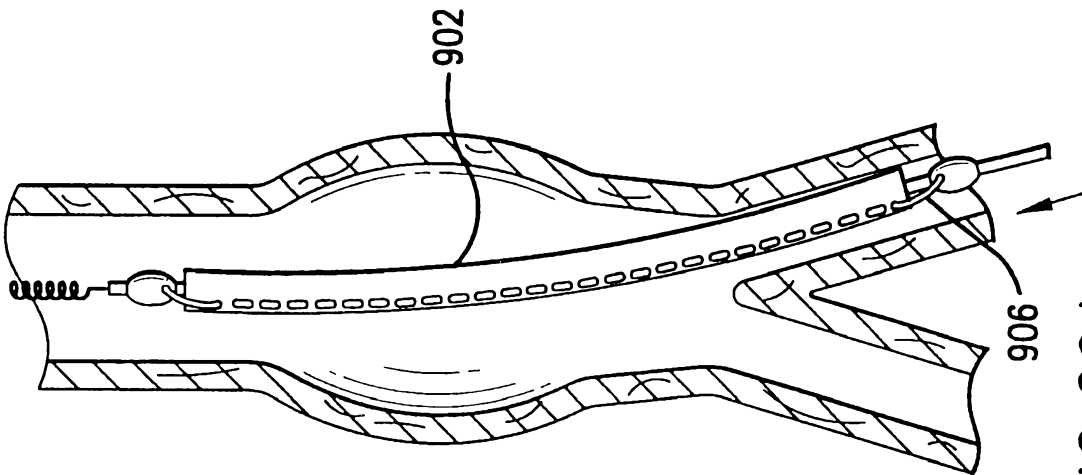


FIG. 29A

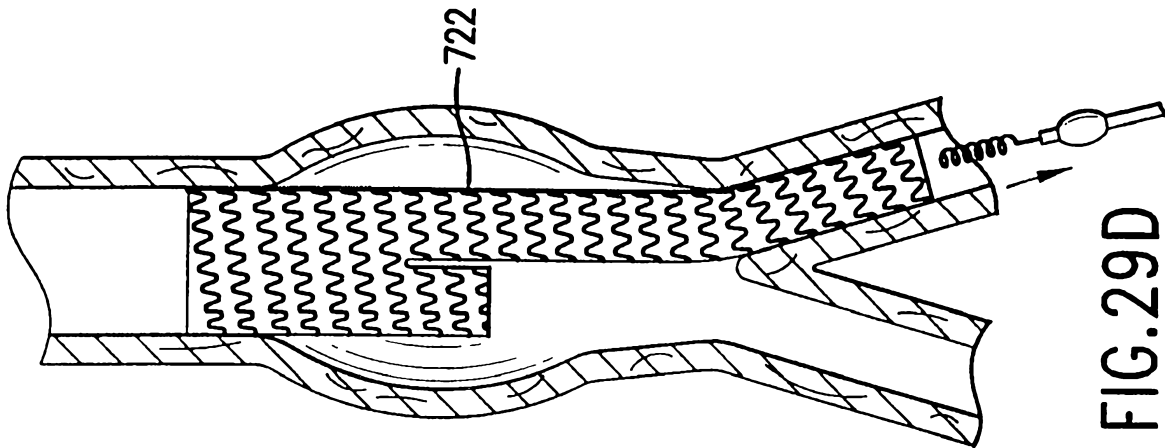


FIG. 29D

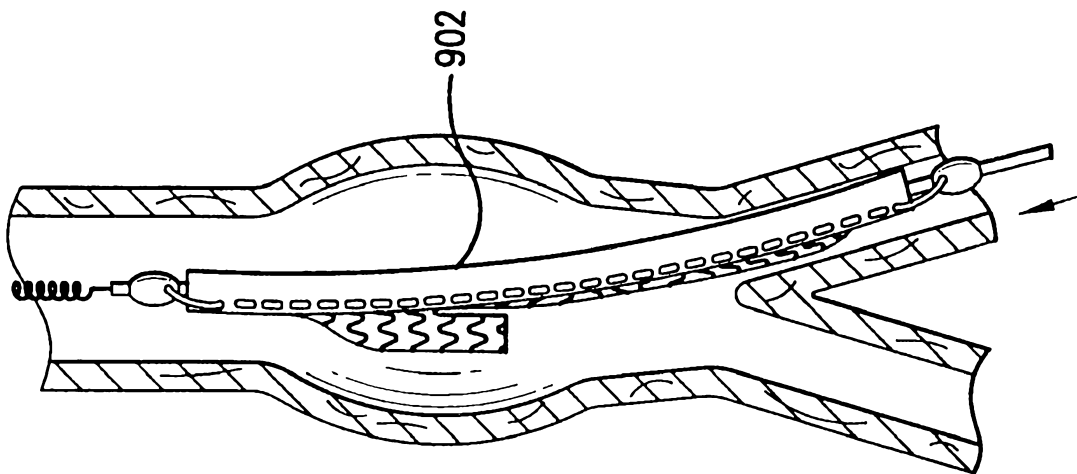


FIG. 29C