




(86) Date de dépôt PCT/PCT Filing Date: 2003/07/16
 (87) Date publication PCT/PCT Publication Date: 2004/01/22
 (85) Entrée phase nationale/National Entry: 2005/01/14
 (86) N° demande PCT/PCT Application No.: US 2003/021964
 (87) N° publication PCT/PCT Publication No.: 2004/006775
 (30) Priorité/Priority: 2002/07/17 (10/196,561) US

(51) Cl.Int.⁷/Int.Cl.⁷ A61B 8/14
 (71) Demandeur/Applicant:
VERMON, FR
 (72) Inventeurs/Inventors:
FLESCHE, AIME, FR;
LACAZE, ELISABETH, FR;
NGUYEN-DINH, AN, FR;
AUCLAIR, PHILIPPE, FR;
DUFAY, REMI, FR;
MAUCHAMP, PASCAL, FR
 (74) Agent: ADE & COMPANY

(54) Titre : RESEAU DE TRANSDUCTEURS ULTRASONORES UTILISE PAR UN CATHETER
 (54) Title: ULTRASOUND ARRAY TRANSDUCER FOR CATHETER USE

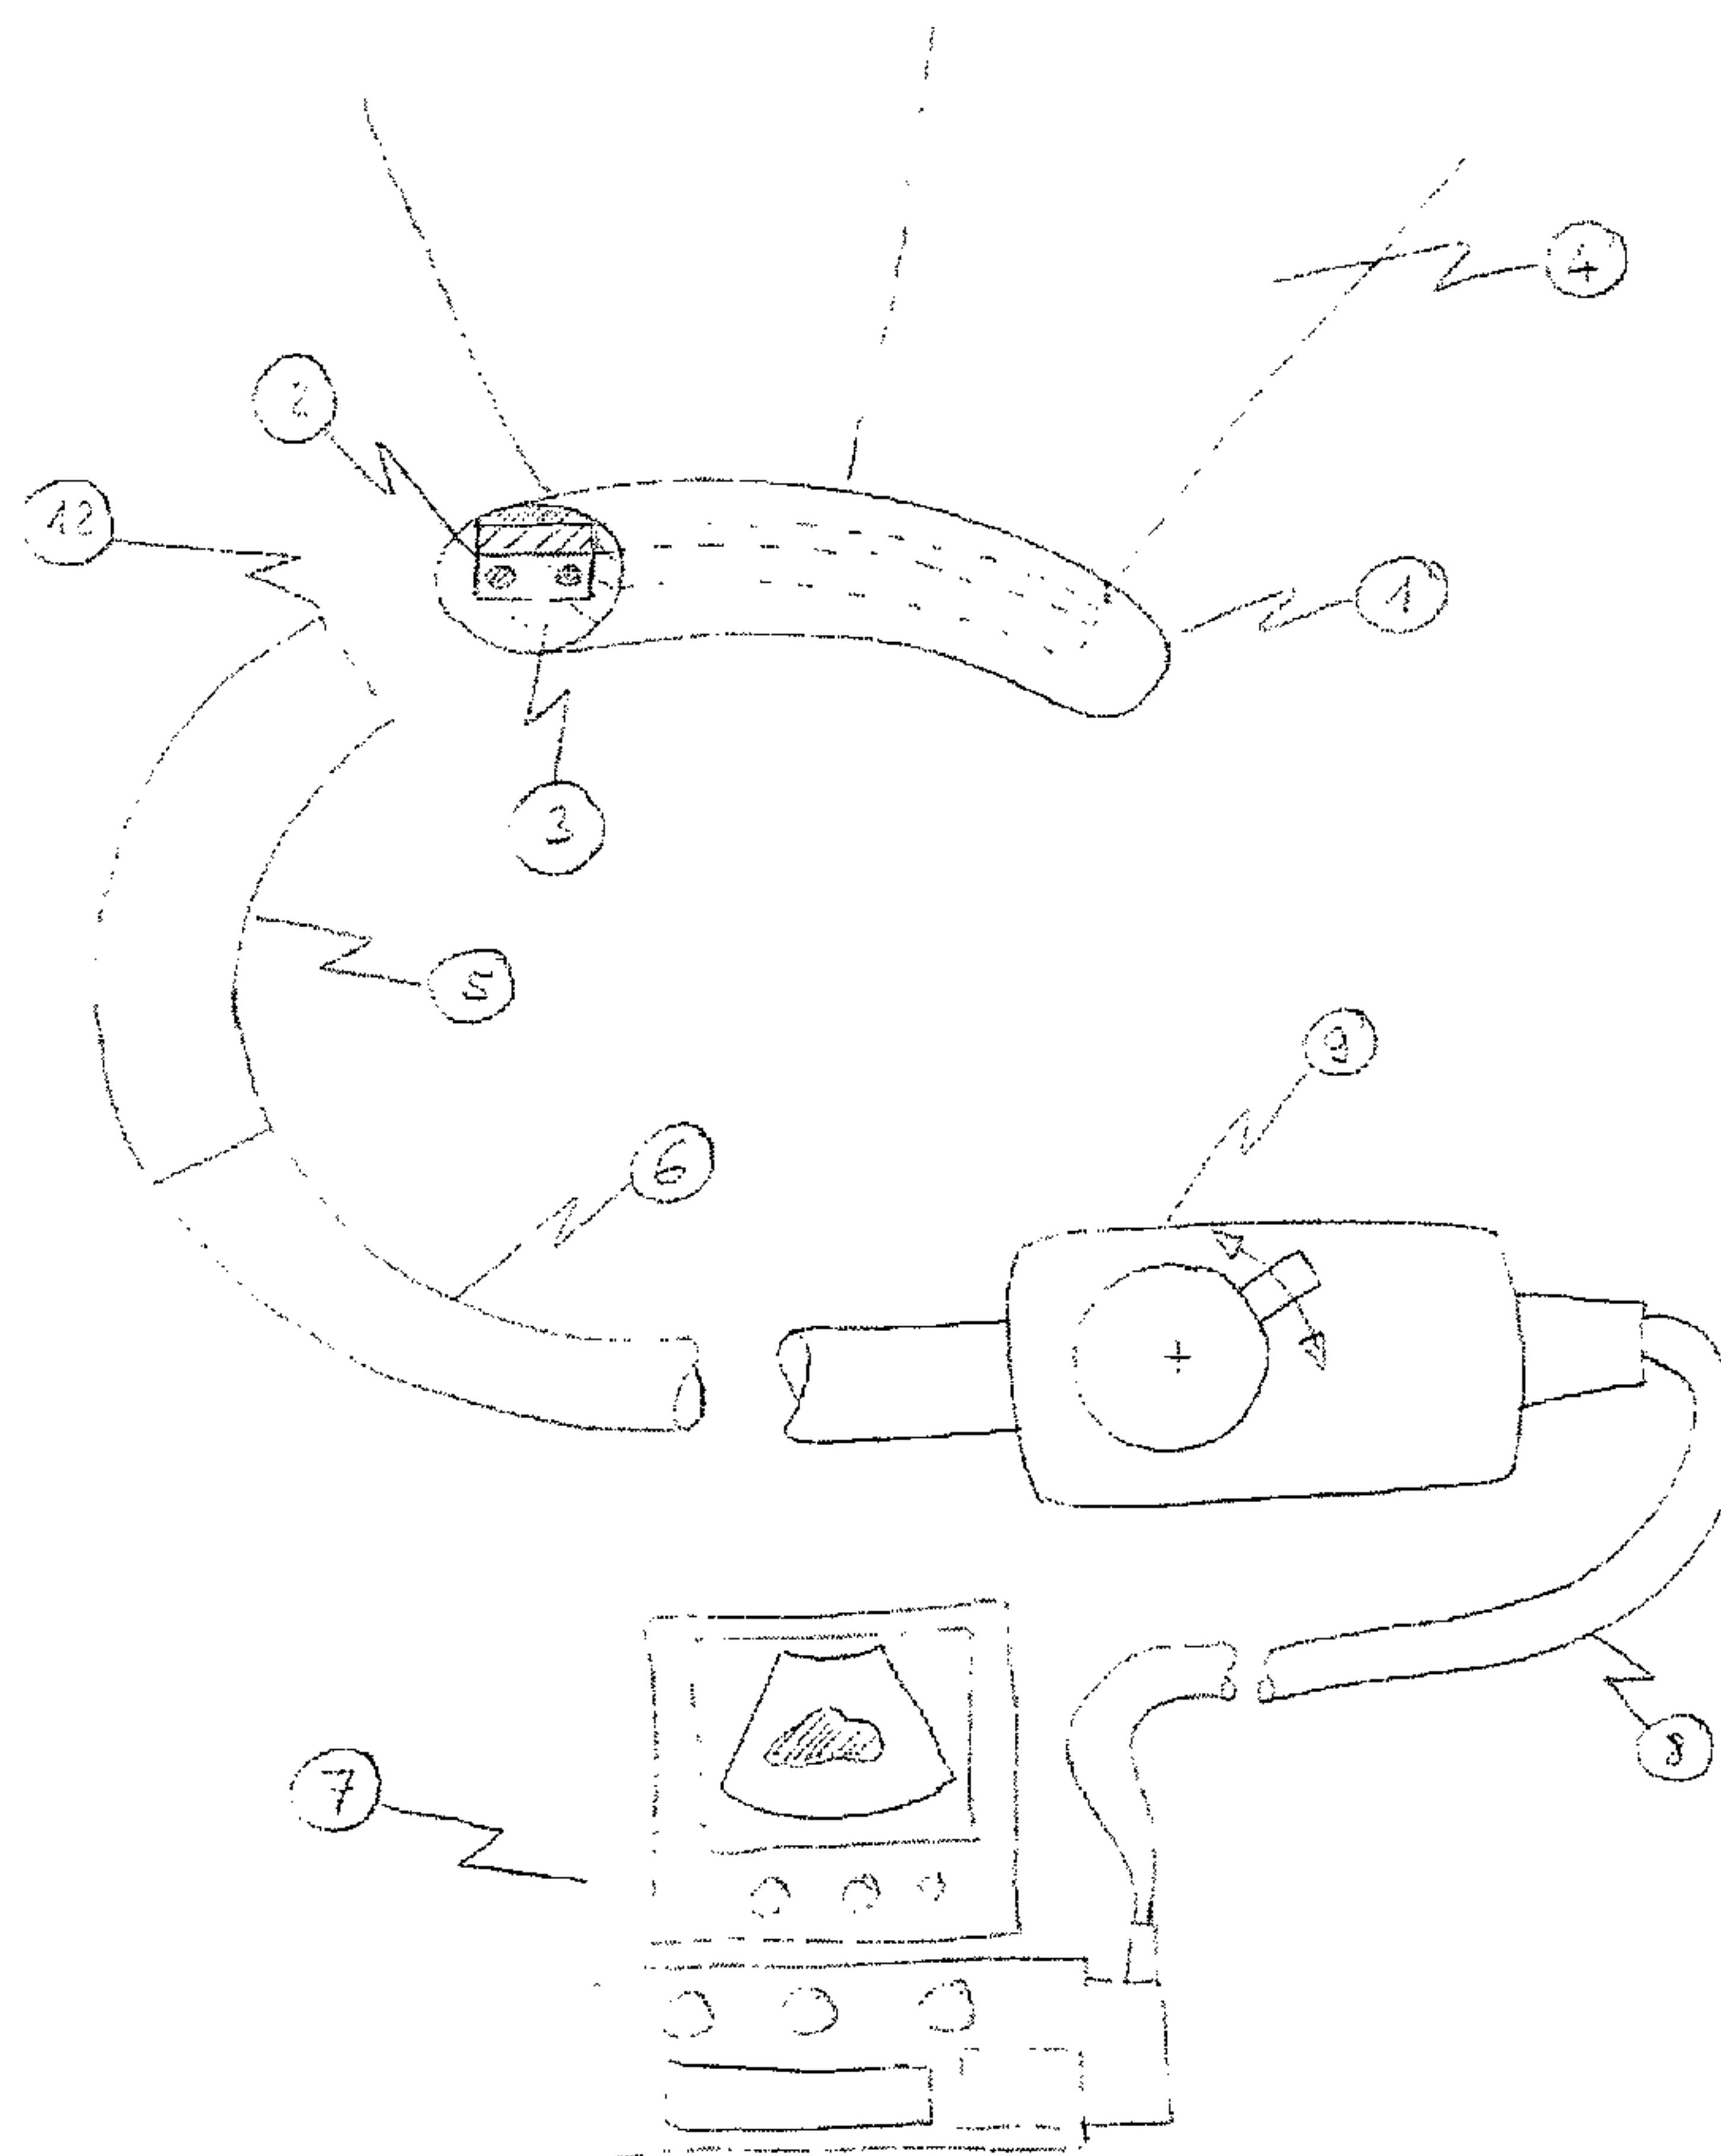

(57) Abrégé/Abstract:

A catheter-based ultrasonic transducer array (2) is provided which includes a piezoelectric member (22) sandwiched between matching layers (23) and a backing member (21). A flexible stiffening element or elements is embedded in the backing member.

(57) **Abrégé(suite)/Abstract(continued):**

The element (10a, 10b) is opaque to radio frequencies and integrated along the azimuthal axis of the array (2) so as to enable a user to view the element in an image of the array derived from the array (2) output and thus determine the angular position of the array (2). A flexible interconnection assembly (11) provides an electrical connection between the electrodes of the piezoelectric member (22) and external cabling. Different methods are provided for adding a surrounding protective cover (3) to the array (2).

(12) INTERNATIONAL APPLICATION PUBLISHED UNDER THE PATENT COOPERATION TREATY (PCT)

(19) World Intellectual Property
Organization
International Bureau



(43) International Publication Date
22 January 2004 (22.01.2004)


PCT

(10) International Publication Number
WO 2004/006775 A1

- (51) International Patent Classification⁷: **A61B 8/14**
- (21) International Application Number: PCT/US2003/021964
- (22) International Filing Date: 16 July 2003 (16.07.2003)
- (25) Filing Language: English
- (26) Publication Language: English
- (30) Priority Data:
10/196,561 17 July 2002 (17.07.2002) US
- (71) Applicant: **VERMON** [FR/FR]; 180 Rue General Renault, BP 3813, 37038 Tours Cedex 1 (FR).
- (71) Applicant (for MG only): **HUNT, Ross, F. Jr.** [US/US]; Larson & Taylor, PLC, 1199 North Fairfax Street, Suite 900, Alexandria, VA 22314 (US).
- (72) Inventors: **FLESCH, Aimé**; 97 Bis Avenue Général Leclerc, 78570 Andrésy (FR). **LACAZE, Elisabeth**; Appart 2, 22 Rue G. Doumergue, 31170 Tournefeuille (FR). **NGUYEN-DINH, An**; 15 Rue Vaussouvin, 37190 Valleres (FR). **AUCLAIR, Philippe**; 66 Rue du Pavillon, 37100 Tours (FR). **DUFAIT, Rémi**; 12 Passage George Sand, 37000 Tours (FR). **MAUCHAMP, Pascal**; 12 Rue J. Joinville, 37230 Fondettes (FR).
- (74) Agent: **HUNT, Ross, F., Jr.**; Larson & Taylor, 1199 North Fairfax Street, Suite 900, Alexandria, VA 22314 (US).
- (81) Designated States (*national*): AE, AG, AL, AM, AT, AU, AZ, BA, BB, BG, BR, BY, BZ, CA, CH, CN, CO, CR, CU, CZ, DE, DK, DM, DZ, EC, EE, ES, FI, GB, GD, GE, GH, GM, HR, HU, ID, IL, IN, IS, JP, KE, KG, KP, KR, KZ, LC, LK, LR, LS, LT, LU, LV, MA, MD, MG, MK, MN, MW, MX, MZ, NI, NO, NZ, OM, PG, PH, PL, PT, RO, RU, SC, SD, SE, SG, SK, SL, SY, TJ, TM, TN, TR, TT, TZ, UA, UG, UZ, VC, VN, YU, ZA, ZM, ZW.

[Continued on next page]

(54) Title: ULTRASOUND ARRAY TRANSDUCER FOR CATHETER USE

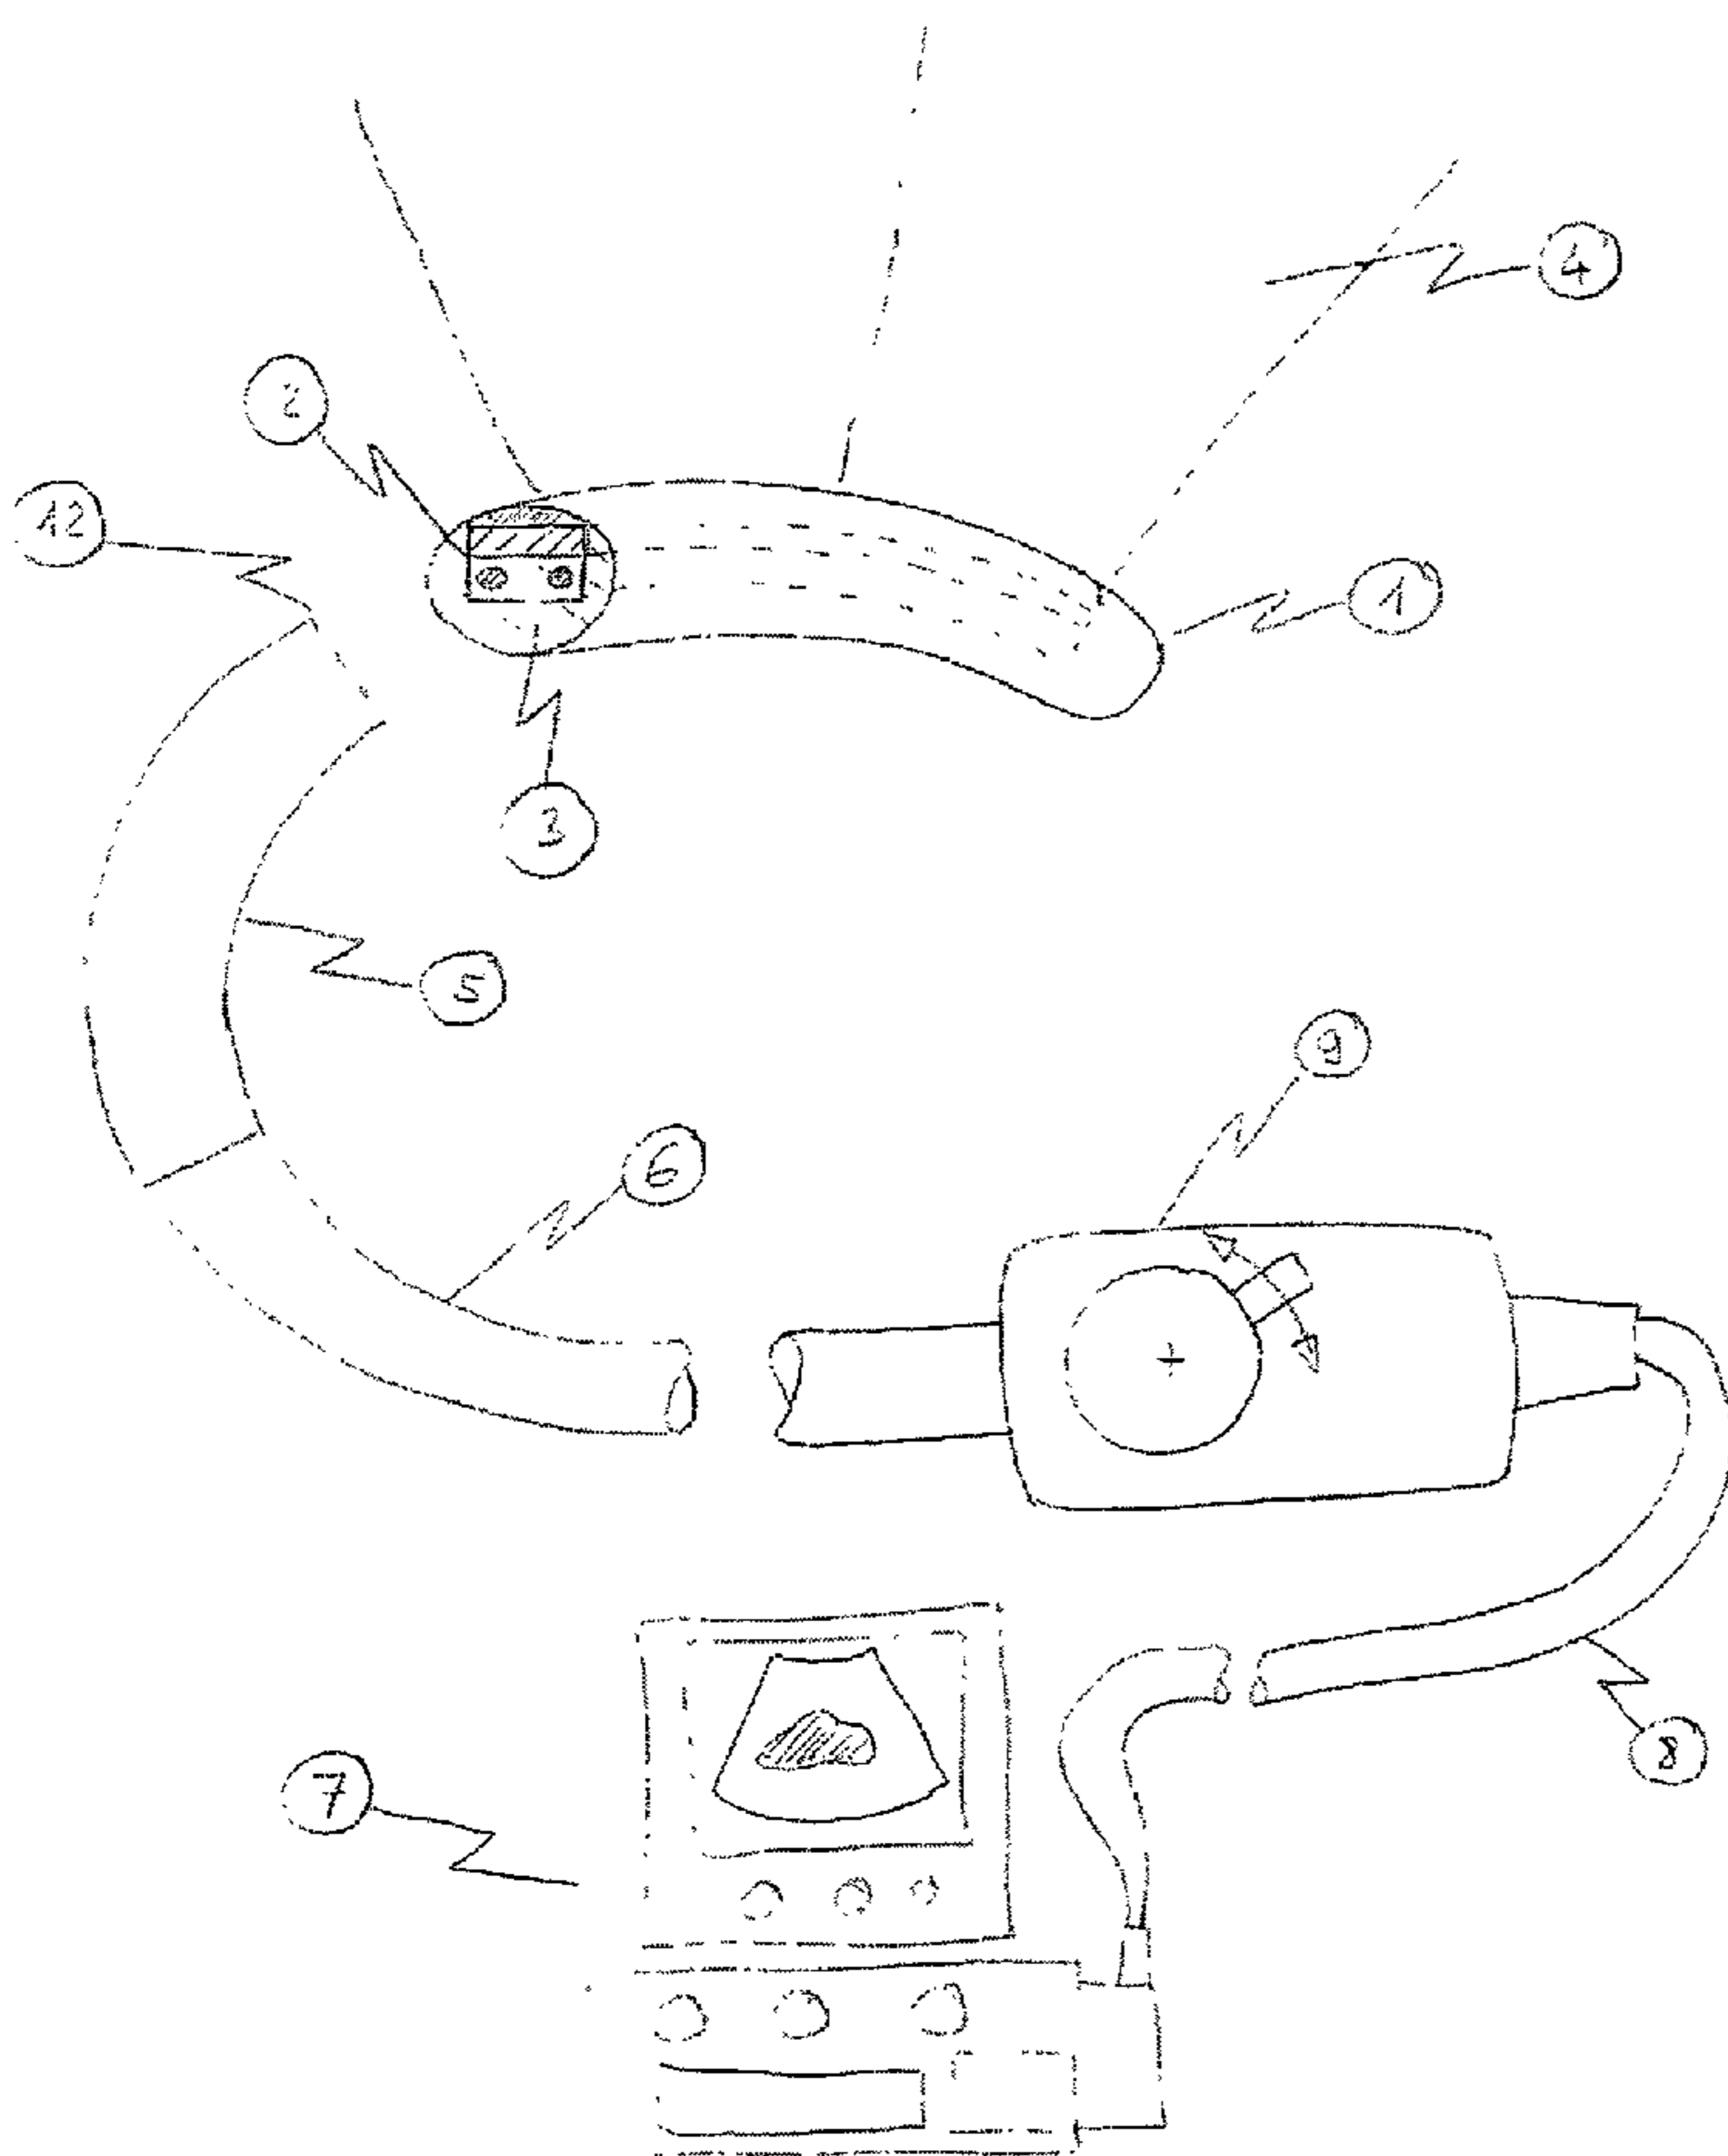

(57) Abstract: A catheter-based ultrasonic transducer array (2) is provided which includes a piezoelectric member (22) sandwiched between matching layers (23) and a backing member (21). A flexible stiffening element or elements is embedded in the backing member. The element (10a, 10b) is opaque to radio frequencies and integrated along the azimuthal axis of the array (2) so as to enable a user to view the element in an image of the array derived from the array (2) output and thus determine the angular position of the array (2). A flexible interconnection assembly (11) provides an electrical connection between the electrodes of the piezoelectric member (22) and external cabling. Different methods are provided for adding a surrounding protective cover (3) to the array (2).

WO 2004/006775 A1

WO 2004/006775 A1

(84) Designated States (regional): ARIPO patent (GH, GM, KE, LS, MW, MZ, SD, SL, SZ, TZ, UG, ZM, ZW), Eurasian patent (AM, AZ, BY, KG, KZ, MD, RU, TJ, TM), European patent (AT, BE, BG, CH, CY, CZ, DE, DK, EE, ES, FI, FR, GB, GR, HU, IE, IT, LU, MC, NL, PT, RO, SE, SI, SK, TR), OAPI patent (BF, BJ, CF, CG, CI, CM, GA, GN, GQ, GW, ML, MR, NE, SN, TD, TG).

Published:

— *with international search report*

For two-letter codes and other abbreviations, refer to the "Guidance Notes on Codes and Abbreviations" appearing at the beginning of each regular issue of the PCT Gazette.

ULTRASOUND ARRAY TRANSDUCER FOR CATHETER USE

Background of the invention

1. Field of the Invention

5 The invention relates to an ultrasonic linear array transducer for utilization in catheter instruments and to methods of manufacturing curved linear array transducers for catheter-mounted applications so as to comply with acoustic and surgical specifications relating to such products.

10

2. Related Art

Intraluminal catheter-mounted ultrasonic transducers of several different kinds and forms have been widely discussed in the literature. Usually, the transducing device is attached at, or in the vicinity of, the tip end of the catheter, and wave radiation is then directed outwardly from the catheter either in a transverse radial mode, longitudinal radial mode, forwardly directed mode, circular radial mode or a combination thereof. The catheter instrument is basically comprised of an elongated tube having, at one end thereof, an insertion tip wherein the transducer is mounted and terminated at the other end by a handle wherein are gathered the bending controls for the instrument. Catheters designed for use in cardiac examinations commonly have a diameter ranging from 3 to 10 French catheter scale, meaning that the external diameter of the inserting tube does not exceed a value of, respectively, 1 to 3.3 mm. The tube is approximately of 1 to 2 meters long and is connected to the imaging transducer of the system by a flexible coupler which is capable of causing bending of the transducer tip in two or four directions.

30 An example of an imaging catheter is disclosed by US Patent No. 3,938,502 to Bom, wherein the catheter is a circular radially

emitting device. The elements of the transducer array are disposed around the catheter circumference to form a circular scanning image. Such product is particularly well suited to arterial applications and more specifically, to examining for arteriosclerosis in plaque wherein a
5 sectional view of the artery is required.

In US Patent No. 4,605,009 to Pourcelot, there is disclosed an endoscope probe for imaging an internal wall of human body. In order to widen the angle of view of the instrument, a curved linear array transducer is associated with optical visualization means. Assembly
10 of the transducer includes the provision of a wire interconnection between the transducer piezoelectric member and a rigid printed circuit board (PCB) located at the bottom side of the transducer, and soldering of coaxial cables to the PCB to complete the interconnection. Such a construction is voluminous and prohibitive of
15 any miniaturization of transducer for implementation thereof in intraluminal probes.

Another endoscopic ultrasonic instrument of interest is disclosed in US Patent No. 5,291,893 to Slayton wherein a linear array transducer is provided at the distal end of an endoscope or
20 catheter. The transducer array is mounted in a tip housing that is capable of rotating around its longitudinal axis thereby providing rotation of the scanning plane without moving the catheter. However, the transducer array construction method includes the provision of an interconnection PCB located beneath the transducer assembly where
25 coaxial cables and piezoelectric contact wires are soldered. Making the interconnection in this way wastes the considerable space behind the array so miniaturization of transducer tip diameter is difficult and the result unreliable. Furthermore, the rotation of the transducer tip with regard to the rest of the catheter requires a dynamic seal at the
30 junction between the two moving parts. This junction is a collection

site for dust accumulation and biological contamination so the device can not be reused in surgical operations. Further, with regard to the manufacturing cost of the device, there is no corresponding disposable diagnostic instrument available on the market.

5 PCT Patent WO92/03972 to Crowley relates to an imaging system combined with an insonifier for detecting the position and orientation of the associated catheter device. The insonifier utilizes ultrasound with a frequency that can be detected by the catheter sensor. The energy transferred between the insonifier and the
10 catheter is maximized when the two devices face each other, so that by identifying the orientation of one of the devices, the position of either can be determined. Because the frequency of transmit energy from the insonifier should be at least in the bandwidth of catheter device, the separation distance between the two devices is limited.
15 The external insonifier, when used as described in the patent, is difficult to control and in actual practice, the alignment of the insonifier relative to the catheter remains approximate.

In PCT Patent WO98/33430 to Curley, there is disclosed a catheter-mounted transducer array for ultrasonic imaging. The
20 transducer includes an end portion surrounding the array and providing a speed of sound therein greater than or equal to 1250ms^{-1} . The transducer azimuth axis is parallel to the longitudinal axis of the catheter and is molded or sheathed to have an elongated cylindrical tip portion having the same proportions as those of the catheter. The
25 Curley patent discloses two alternative methods of making surrounding material for the array transducer, viz., a molding method and a pre-formed thermoplastic material. The surrounding material is characterized by its cylindrical cross-section without regard to the elevation focus of the array. Accordingly, the speed of sound in the
30 surrounding material must be close to that of the propagation medium

so as not to modify the focus of transducer. Otherwise, no details as to the placement of the transducer in molding method are provided. The pre-formed sheathing method provides for the assembly of the transducer array into the pre-formed sheath using a glass tube
5 associated with a mandrel and subsequent heating to eliminate air gaps between the transducer array and the polymer sheath. One of the important drawbacks of this method concerns the difficulty of the insertion of the transducer array into the polymer sheath without causing damage to the array due to pressure exerted thereon.

10 Further, the heat applied to the polymer sheath to shrink the sheath onto the array will inherently transfer heat to the transducer array and this heat can depolarize the piezoelectric structure thereof. Another aspect of the Curley patent that is not clearly described concerns the angular orientation of the array in the case where the polymer sheath
15 is provided with an acoustic window which is designed with a particular radius (concave or convex). It is evident, that with this arrangement, the position of the elevation plane of the array with regard to the geometry of lens is of critical importance.

20 Summary of the Invention

In accordance with the invention, there is provided a novel method for making ultrasonic imaging transducer arrays for catheter use which enables implementation of curved or linear array shapes as well as provides for detection of the array orientation by a radio-
25 opacity method described below. The method of the invention is also compatible with low cost fabrication requirements and thus finds application in the high volume disposable catheter market.

According to one aspect of the invention, a linear ultrasonic array transducer assembly is provided for intraluminal catheter use
30 wherein a curved linear ultrasonic transducer array is mounted at or

on the distal end of an elongated catheter so as to provide expanded viewing of an organ to be imaged.

Another aspect of the invention concerns the provision of an ultrasonic transducer array construction which provides optimized
5 acoustic performance as well as compact sizing so as to be compatible with conventional vascular insertion techniques. The associated transducer comprises a sandwich of a piezoelectric member, backing block or member, matching layer, focusing lens and bonded interconnection means.

10 A further aspect of the invention concerns the flexibility of the transducer array. The flexibility provided enables the transducer array to bend slightly in order to facilitate insertion thereon when embodied as a curved linear array. The transducer array then recovers its initial shape once arriving at the desired site.

15 Yet another aspect of the invention concerns the integration of stiffening dorsal elements or "sticks" that provide elasticity to the transducer array during an insertion operation as well as other advantages.

20 Still another aspect of the invention concerns the provision of dorsal elements or "sticks" which are opaque to radio frequencies and can be viewed during the imaging process so as to enable the examiner to detect the orientation of the transducer array during placement and use thereof.

25 An additional aspect of the invention concerns the provision of a polymer sheath or covering over the transducer array. In one preferred method of this aspect or embodiment, the molding of the polymer sheath is omitted and the transducer array is inserted into the tube of the catheter. The tube terminates in a flexible portion at which the array is located. Expansion of a flexible array receiving portion of
30 the tube is provided in order to facilitate insertion of the transducer

array into this flexible tube portion without excessive constraining forces being exerted thereon.

Further features and advantages of the present invention will be set forth in, or apparent from, the detailed description of preferred
5 embodiments thereof which follows.

Brief Description of the Drawings

Figure 1 is a schematic plan view of an ultrasonic catheter system including a perspective view, partially in cross section, of a
10 curved linear transducer array of the catheter system;

Figure 2 is a perspective view, partially in cross section, of a linear transducer array for catheter use;

Figure 3 is a more detailed cross sectional view of the transducer array of the catheter system of Figures 1 and 2;

15 Figure 4 is a perspective view of the transducer array of Figure 3, as equipped with a flexible interconnection assembly;

Figure 5 is a front view of the flexible interconnection assembly of Figure 4, in accordance with a preferred embodiment;

20 Figure 6 is a perspective view of a preferred method of folding the flexible interconnection assembly of Figures 4 and 5 so as to achieve a compact device;

Figure 7 is a perspective view of a step in a method of pre-formed fabrication of the dorsal element reinforced backing device of
25 the array of Figure 3;

Figure 8 is a perspective view of a tooling apparatus or molding tool for molding of the transducer tip of Figure 3;

Figure 9 is a cross sectional view of the molding tool of Figure 8, as equipped with flat lateral "cheeks" for a lens molding operation;

Figure 10 is a cross sectional view of the molding tool of Figure 8, as equipped with "dig cheeks" for a protective cover molding operation.;

5 Figures 11(a) to 11(c) are top plan views used in explanation of a method for detecting the position of a curved array transducer in the body of a patient through the use of angiography visualization;

Figures 12(a) to 12(e) are top plan views (angiographic views) of a transducer tip as equipped in accordance with a further embodiment so as to enable angular position detection;

10 Figures 13(a) to 13(e) are top plan views (angiographic views) of a transducer tip as equipped in accordance with yet another embodiment so as to enable angular position detection;

Figures 14(a) and 14(b) are perspective views of a profiled protective tube or protective cover showing a transducer assembly inserted therein and showing tube and assembly prior to such insertion, respectively;

Figure 15 is a perspective view of a step in a molding operation for the transducer end-tip; and

20 Figure 16 is a perspective view of an inserting tool for the protective cover assembly, in accordance with a further embodiment.

Detailed Description of the Preferred Embodiments

Referring to Figure 1, there is shown an ultrasonic transducer array 2 for catheter applications. The transducer array is particularly designed to match the diameter of the cardiac 9-10 French catheter scale (FCS). However, the device can be adapted for use with other diameters, even a 1 mm catheter (FCS 3).

In accordance with common practice, an imaging cardiac catheter is generally comprised of a flexible tube or tubing 6 of about 30 1-2 meters in length. Tube 6 is terminated by a transducer tip 1 which

is attached to the distal end of the tube **6** by the intermediate of a bendable coupler **5**, although coupler **5** is optional. Unlike the bendable couplers designed for reusable endoscopes, bendable couplers for catheters are of a very simple design to strictly limit the features thereof to the essential functionality, viz., bending. In most cases, the bendable coupler **5** would simply comprise a flexible tube portion equipped with one or two pairs of command cables which are adapted to slide along lumens disposed on the periphery of the flexible tube portion. This sliding action of one of the command cables will result in bending of the tube portion on the side thereon where the corresponding cable is located.

At the distal extremity of the bendable coupler **5**, a transducer tip **1** is mounted. The interconnection means for the associated imaging transducer **2** pass through the central hollow space within the bendable coupler **5** so as to extend to the main tube of catheter and are then connected to an external coaxial cable **8** adapted to be plugged into an imaging system **7**. All of the interconnection means for the external cables and command cables are commonly gathered together in a handle **9** of the probe device which is usually a separation point between disposable and reusable parts of the device. A more specific description of endoscope constructions of this type can be found, for example, in US Patent No. 5,681,263 to Flesch.

Figures 1 and 2 respectively show curved and linear array transducer shapes suited for catheter applications. However, the description of a preferred embodiment here will focus on the curved array ultrasonic transducer shown in Figure 1. The transducer tip **1** is preferably of an elongated shape with a curvature in the azimuthal plan of the transducer **2**. Because the transducer array **2** is driven by electronic phase shift beamformer (not shown) and is based on the

curvature of the emitting surface, the insonified paths will define a sector angle indicated at **4** which represents the scanning area of the probe.

Referring to Figure 2, in a similar manner, the scanning area **4**
5 of the probe of Figure 2 is generally in the shape of a rectangular section as shown in solid lines. However, sophisticated electronic beamformer techniques can be used to produce a sector shape scanning area **41**, even if a linear array is used, by steering the acoustic beam with a predetermined angle when arriving at the
10 extremity of array. It is noted that the image quality is somewhat deteriorated in this area but the user is still provided with specific features that only a curved or phased array can provide.

Returning to Figure 1, the catheter assembly also comprises a shoulder portion **12** which is designed to interfit with the associated
15 mounting part located at the distal end of bendable coupler **5**.

As will be understood by those skilled in the art, the term transducer array is used here to designate all types of transducer arrays that comprise elementary transducers aligned in one direction in azimuth, and thus this term includes linear, curved and phased
20 arrays.

Figure 3 shows a cross sectional view of a transducer tip according to a preferred embodiment. As illustrated, the transducer assembly **2** is disposed in the top portion of the transducer tip **1** and comprises a piezoelectric member **22** sandwiched between one or
25 more matching layers **23** and a backing member **21**. The front face of the transducer **2** is preferably covered by an acoustic focusing lens **13** which is advantageously made of an elastomeric rubber providing a sound velocity therein lower than that of the propagation medium, such as the silicon rubbers TSE 3331 from GE Silicones, NY, USA.
30 The backing member **21** includes a set of parallel spring elements or

sticks **10** that are disposed alongside each other and located at or near the rear or bottom side of the backing member **21**.

A flexible printed circuit **11** is bonded to the rear electrode (not shown) of the piezoelectric member **22** through connecting portion as described below and folded to assume a longitudinal shape as shown
5 in Figure 4.

The transducer assembly **2** is embedded in a protective covering or molding **3** which is made of a suitable resin or polymer material and which is of a circular cross section to match the diameter
10 of the catheter. Polymers that are compatible with the use thereof as the embedding molding **3** may be selected from the group consisting of polyurethanes, silicones, and polyether block amides resins (such as Pebax, Registered Trademark) and flexible epoxies. The molding method of mounting transducer assembly **2** is desirable in order to
15 obtain a reliable and cosmetically finished device. However, other methods for obtaining an embedded transducer tip include, for example, a bonding of a finished transducer assembly into a pre-formed protective tip cover.

To provide a better understanding of the method of
20 manufacturing of an imaging catheter transducer tip according to the preferred embodiment of the invention, reference will now be made to Figures 4 to 10. The method of manufacturing disclosed herein is particularly adapted to a small cross section transducer array and affords low cost fabrication.

In the embodiment shown in Figures 4, 5 and 6, a particular
25 aspect of the management of the flexible circuit **11** is provided. The flexible circuit **11**, which is shown in planar shape in Figure 5, is preferably of a single face design wherein conductive traces **113** are plated on a polyamide film of a thickness of 5 to 25 μ m. The opposite
30 face or surface of the film can be covered by a metal sheet or layer

(not shown) in order to control the characteristic impedance of the conductive traces **113**. Further, this metal layer provides interference protection with respect to electrical signals travelling through the conductive traces **113**.

5 In this embodiment, the flexible circuit **11** is of a rectangular shape and has a first top or upper portion **110** which includes regularly spaced traces **113** having a pitch equal to that of the array of transducer. The conductive traces **113** of this first portion **110** are free of a cover layer or protective layer. The width of the portion **110**
10 is equal to or smaller than that of the transducer elevation.

 A second portion **111** of the flexible circuit **11** is located at the middle area of the circuit **11** and may be protected by cover layer if desired. The rest of the flexible circuit **11** constitutes a third portion **112** of the circuit **11**. The third portion **112** of circuit **11** is divided
15 longitudinally into strips **112a** to **112d** of equivalent length. It is noted that although four strips are illustrated, there is no limitation on the number of strips comprising the third portion **112**. In general, the number of strips is governed by the ratio of length to elevation of the array. The strips **112a** to **112d** are obtained by spaced cuts through
20 the third portion **112** of the flexible circuit **11**. The cutting operation is advantageously performed by laser cutting or by a die-cutting process. The distal extremities of strips **112a** to **112d** are terminated in non-protected, metal plated traces in a manner such as to receive, or to be assembled to, optionally provided extending cables.

25 In an alternative embodiment of flexible circuit **11**, the flexible circuit **11** is provided with a single central portion **110**, surrounded by opposed portions corresponding to portions **111** which are, in turn terminated by portions corresponding to portions **112** at which strips **112a** to **112d** are defined.

Figure 6 is a perspective view of the flexible circuit **11** after being partially folded prior to being assembled to the transducer assembly (not shown in Figure 6). Although for clarity of the illustration, the transducer assembly is not shown in Figure 6, it will be understood that the folding of the circuit **11** illustrated creates a generally rectangular void formed by the portions **110** and **111** of the flexible circuit **11** in which the transducer assembly is received. Figure 6 shows the first portion **110** positioned so as to be bonded to the rear surface of the piezoelectric member of the transducer assembly, and folded perpendicularly to the portion **111**. Portion **112** is then folded the same way with regard to the portion **111** so as to be in parallel with the portion **110**. Strip **112a** is then folded at an angle of 45 degrees with respect to the orientation of traces **113** (not shown in Figure 6) so the strip **112a** is disposed along the azimuthal axis of the array. Next, the second strip **112b** is similarly folded so as to be superimposed on first strip **112a** and so on. At the completion of this operation, the transducer assembly will exhibit a longitudinal shape wherein the flexible circuit **11** occupies a minimum of space and is properly arranged on the rear face of transducer as shown in Figure 4.

Referring again to Figures 1 and 3, as previously described, the piezoelectric member **22** is sandwiched between backing member **21** and matching layer **23**. The piezoelectric member **22** can be a PZT ceramic, a relaxor based single crystal or a composite comprising a blend of piezoelectric and passive materials. The piezoelectric member **22** has electrodes (not shown) plated on its major opposite surfaces and one of the electrodes is divided into a plurality of individual electrodes corresponding to the transducer elements. For interference protection reasons, it is desirable to direct the ground electrode of the piezoelectric member **22** toward the propagation

medium so that the spaced electrodes are positioned at the rear face of the transducer and then bonded to the flexible circuit 11. The bonding operation between the piezoelectric 22 and the flexible circuit 11 is carried out under pressure to avoid the formation of excessive leftover adhesive. This method also maintains the flexibility of the transducer assembly. Adhesives or glues of the families of epoxies or urethanes are suitable candidates for this operation.

To ensure maximizing of the transducer energy transfer function, the front face of the piezoelectric member 22 must be matched to the propagation medium through the addition of one or more matching layers 23 (as described above in connection with Figure 3) having a suitable thickness defined by the following relation: $t = \lambda/4$. Another method for optimizing transmission lines employs a transformer as described by B. Bramham "A convenient transformer for matching coaxial lines" in Electronic Engineering (January, 1961) and D. Emerson in QST (1997). Further, the acoustic impedance of such a device is determined with respect to either standard transmission lines or using a polynomial formula proposed by Desilets. In accordance with the usual requirements, when two matching layers are employed, the first matching layer has an impedance higher than that of the second layer assembled thereto so as to be disposed outermost of the transducer assembly. Methods for manufacturing and designing matching layers are widely described in the literature and are disclosed, for example, in Kino "Acoustic Waves" or Anderson "Acoustic Transducer." Matching layers are advantageously obtained by the molding or mechanical grinding of resins or polymers. The piezoelectric 22 is then pressure bonded to the matching layer or layers 23 and the flexible circuit 11 to form an intermediate transducer assembly.

The backing member **21** of the transducer assembly **2**, according to a preferred embodiment thereof, comprises a stiffening or reinforcing arrangement provided by a pair of parallel elongated elements or "sticks" **10** embedded in the thickness of backing member **21**. As indicated above, Figure 3 shows a cross sectional view of the transducer assembly **2** wherein the parallel elements **10** are located symmetrically with regard to the central longitudinal axis of the transducer. The parallel elements **10** are also referred to as "dorsal stiffening sticks."

Referring to Figure 7, a step in a preferred method of manufacturing of the backing member **21** is shown. As illustrated, a rectangular shaped mold **14** is provided having two sets of openings **15a** and **15b**. The diameters of the openings **15a** and **15b** correspond to the diameters of the stiffening elements **10a** and **10b**. Stiffening elements or sticks **10a** and **10b** are preferably made of a spring material in order to provide flexibility to the backing member **21** if the latter is subjected to flexional forces but capable of recovering the initial shape or curvature thereof after removal of the force. Alloys such as NivaFlex® or Stainless steels (PrEN 10270-3) are suitable for this application.

It will be appreciated that in curved transducer array constructions, the mold for backing member **14** is curved as well, and the stiffening elements **10a** and **10b** will have the same curvature.

As shown in Figure 7, resin **210** is poured from a pourer **P** into the mold **14** and hardening thereof ensues. In a "slim line" transducer construction according to the present invention, the backing material for backing member **21** is preferably selected from particle-filled attenuating resins such as Eccogel from Emerson&Cumings, and soft polyurethanes. Methods for obtaining highly attenuating materials are well known in the art and particles such as air filled plastic bubbles or

air bubbles are used to provide the backing material with strong backscattering of incident wave propagation. Additionally, in case of linear or phased array transducers, the stiffening element backing member **21** can be made from a single long base member and
5 individual backing members obtained by cutting the base member to desired lengths.

Figures 8 and 9 depict a tooling apparatus for molding the transducer tip. Once the transducer assembly operation is complete, the transducer assembly **2** is disposed in a molding tool or mold **19**.
10 The mold **19** includes a dorsal carrier or member **16** which is designed to have a curvature corresponding to the curvature of the transducer assembly **2**, if the assembly is curved. The dorsal carrier **16** is bounded at each extremity by plates **18a** and **18b** which are secured to the dorsal carrier **16** by a screw system, i.e., a plurality of
15 screws. Care must be taken with respect to the geometry of the plate-dorsal carrier assembly in order to provide placement of the tooling apparatus within precise tolerances.

In this embodiment, the molding tool **19** is completed by adding two flat lateral cheeks or side members **17c** and **17d** to allow the
20 molding of the focusing lens **13** described above in connection with Figure 3. Because the carrier **16** has the same width as the transducer assembly, there should be no occurrence of excessive lens resin.

Once the lens material is cured, the lateral cheeks or side
25 members **17c** and **17d** are then removed from tool **19** and will be replaced by further side mold members or "dig cheeks" **17a** and **17b** as shown in Figure 10. As illustrated, cheeks **17a** and **17b** of Figure 10 form a cylindrical hollow section with circular opening when cheeks **17a** and **17b** are coupled together. The hollow space formed is then
30 filled with resin to obtain the protective cover **3** for the transducer **2**,

and thus, in doing so, determining the final diameter of the transducer tip **1**. It is to be noted that the resin material used for lens **13** normally differs from that of protective cover **3**. However, in a case where there is no particular specification with respect to transducer focus,
5 the same resin can be used for both and so that only the step described in connection with Figure 10 need be performed.

Another aspect of the cardiac catheter provided in accordance with the preferred embodiment of the invention concerns the ability to detect the orientation of the imaging transducer array **2** once inserted
10 into an organ of the patient being treated. In practice, the catheter device is tracked and monitored using angiography X-ray imaging. During the insertion and use, the user is able to visualize the catheter tip in the body of the patient under X-ray ionization. However, when the transducer is of a linear elongate shape as opposed to a linear
15 curved shape, no information is provided regarding the angular position of the transducer scanning plane, so that manual searching by the user of the image is required. When the transducer tip **1** is of a curved shape as shown, e.g., in Figure 1, the X-ray images can provide a user with information regarding the transducer orientation
20 by comparing the curvature of the transducer tip **1** with the images obtained. This is shown in Figures 11(a) to 11(c). For example, if the image is of a linear appearance as shown in Figure 11(b), this means that that transducer scanning plane is aligned with ionizing source. On the other hand, an image having maximum curvature is obtained
25 when the transducer scanning plane is rotated by 90° with respect to the ionizing source. Of course, the direction of the aligned scanning plane (0°) can only be specifically identified with rotation of the probe so that, for example, a left rotation of the catheter accompanied with appearance of a left convexity (-90°) as shown in Figure 11(a) (i.e., a
30 leftward facing convex curvature as viewed in the drawings) indicates

that the front surface of the transducer is facing the ionizing source (oriented toward the ionizing source), whereas in the case of a left concavity (+90°) as shown in Figure 11(c), the transducer is facing away from, and emitting in the same direction as, the ionizing source.

5 An alternative method for detecting the angular position of transducer tip is based on observation of the dorsal sticks or elements **10a**, **10b** embedded in the backing member **21** of the transducer assembly **2**. Referring to Figures 12(a) to 12(e), in this embodiment, the transducer tip is provided with dorsal elements **10a** and **10b** of
10 unequal length. As illustrated, element **10a** is shorter than element **10b** so that each cardinal (90°, 180°) angular position of the transducer array **2** can be recognized by observation of the appearance of the two elements **10a**, **10b**. Figures 12(a) to 12(e) show the relative positioning of the elements **10a**, **10b** for angular
15 orientations of -180°, -90°, 0°, +90° and +180°, respectively. With this approach, a precise angular position adjustment can be facilitated.

 Yet another method for determining or recognizing the angular position of the transducer tip is implemented with a set of dorsal elements **10a**, **10b** which are of same length but are of different
20 diameters as shown in Figures 13(a) to 13(e). More specifically, in this embodiment, the set of elements or sticks comprises a first stick **10a** having a first diameter and a second stick **10b** having a second diameter significantly larger than the first diameter. When the transducer tip **1** is facing the ionizing source (0°), the two diameters
25 are clearly distinguishable from the monitoring images and, moreover, at each cardinal position of the tip (90°, 180°), a particular image is obtained which differs from the others as shown in Figures 13(a) to 13(e), for the angles -180°, -90°, 0°, +90° and +180°, respectively. Accordingly, angular position can be determined in basically the same
30 manner as previously described. Similarly, a hollow element or stick

can be used, together with a standard element or stick, or a twisted stick together with a standard stick, can be also used, to provide similar positional information.

In a second embodiment of the invention, the basic transducer assembly remains unchanged. However, in order to reduce manufacturing cost of the device, the protective cover molding operation described above is omitted and replaced by the use of a pre-formed hollow tube having a hollow or internal cross section which corresponds to the cross section of the transducer assembly. In Figures 14(a) and 14(b), a portion of such a pre-formed profiled tube **20** is shown. Tube **20** can be obtained by cutting the tube from a continuously extruded or injection molded base tube. Suitable materials for tube **20** include materials selected from the group consisting of elastomeric rubbers such as Pebax, PU and the like. It is desirable to select materials having a sound velocity similar than that of biologic tissue in order to not disturb the focal geometry of the transducer. However, where there is a significant sound velocity difference, suitable compensation can be provided by adjustment of the radius of curvature of the lens **13**.

The portion of tube **20** used to form cover **3**, is cut to a length equal to that of the transducer assembly **2**. As the base tube is obtained from extrusion molding process, the dimensions of a hollow section **23** are made to be somewhat smaller than those of the transducer assembly **2** so that once assembled together, the tube **20** will slightly bear on the external surface of assembly **2** so as to assure that perfect contact is provided between the covering tube **20** and the external surface of the transducer member **2**.

As shown in Figure 16, the insertion operation wherein transducer assembly **2** is inserted into tube **20** is advantageously achieved using a vacuum cylinder **25** that causes expanding of the

diameter of tube **20** in such proportion as to permit the transducer assembly **2** to be inserted into tube **20** without the generation of excessive friction. As illustrated, the vacuum cylinder **25** is constructed with an internal volume **26** which communicates with a vacuum pump **VP** via an input conduit **28**. The internal surface **251** of cylinder **25** is provided with a plurality of randomly distributed through holes **29** (shown in dashed lines) and cylinder **25** preferably has a diameter of 5% greater to that of the profiled tube **20**. The cylinder **25** is closed at its two extremities by two end plates or lids (not shown) which thus define a central hollow space slightly smaller than the diameter of the profiled tube **20**. In operation, the profiled tube **20** is placed in the cylinder **25** and the lids (not shown) are mounted at the extremities of cylinder, vacuum is then provided to the cylinder **25** from pump **VP** and the external surface of the profiled tube **20** is drawn outwardly so as to contact the surface **251**. The hollow section or opening **23** of tube **20** is inherently caused to expand in size so that the transducer assembly **2** can then be inserted therein. Prior to inserting the transducer assembly **2**, an adhesive, such as a suitable glue, is applied, preferably to the entire surface of the transducer assembly **2**, in order to provide an air gap free assembly.

Figure 15 shows an end-tip molding operation where the transducer tip **1** is placed into mold **22** which has a hemispherically shaped opening **30** therein. Liquid resin **21** is injected into the opening **24** to fill the space between the transducer assembly **2** and the mold **22** to form the tip extremity of the transducer probe. This tip molding method is more suitable for high quantity production where the fabrication of profiled tube is contemplated. It is important to note that this method of making transducer protection cover is only feasible when applied to a transducer assembly with a perfectly constant cross section. Otherwise, the final product will exhibit an irregular external

surface due to the constant thickness and flexibility of the protective cover portion.

Although the invention has been described above in relation to preferred embodiments thereof, it will be understood by those skilled in the art that variations and modifications can be effected in these
5 preferred embodiments without departing from the scope and spirit of the invention.

What is Claimed:

1. A catheter-based ultrasonic transducer array assembly, said assembly comprising:
 - 5 at least one matching layer;
 - a backing member;
 - a piezoelectric member having electrodes and being sandwiched between the at least one matching layer and the backing member;
 - 10 at least one stiffening element embedded in the backing member;
 - flexible interconnection means for providing connection between the electrodes of the piezoelectric member and at least one external cable; and
 - 15 a surrounding protective cover.
2. A transducer array assembly as claimed in claim 1 further comprising a focusing lens attached to the front face of the at least one matching layer.
- 20 3. A transducer array assembly as claimed in claim 1 wherein said at least one stiffening element comprises a pair of elongate elements disposed in said by side relation.
- 25 4. A transducer array assembly as claimed in claim 3 wherein said stiffening elements are of different lengths.
5. A transducer array assembly as claimed in claim 3 wherein said stiffening elements are of different thicknesses.

6. A catheter-based ultrasonic transducer array comprising a transducer including at least one element opaque to radio frequencies and integrated along the azimuthal axis of the transducer to enable a user to view the element in an image of the transducer derived from the transducer output and thus determine the angular position of the transducer.
7. A transducer array assembly as claimed in claim 5 wherein said at least element comprises a pair of elongate elements disposed in said by side relation.
8. A transducer array assembly as claimed in claim 6 wherein said elements are of different lengths.
9. A transducer array assembly as claimed in claim 6 wherein said elements are of different thicknesses.
10. A method for providing a protective cover for an ultrasonic transducer having a predetermined cross section so as to form a transducer tip, said method comprising:
- providing an elastomeric tube having internal hollow space therein of a cross section corresponding to the cross section of the transducer;
 - inserting the transducer into the hollow space of the tube to form a transducer tip; and
 - molding one end of the transducer tip using a flexible resin so as to obtain a smooth tip extremity.
11. A method for making a compact size catheter based ultrasonic transducer array, said method comprising the steps of:

laminating at least one matching layer to a front face of a piezoelectric member having front and rear electrodes;

assembling a flexible circuit to the rear electrodes of the piezoelectric member;

5 assembling a backing member to a rear face of the piezoelectric member;

folding the flexible circuit along a lateral side of the backing member; and

10 folding strips of the flexible circuit in a manner so as to provide superposition of the strips on a rear surface of the backing member.

12. A method for making an ultrasonic transducer array, said method comprising the steps of:

15 providing a mold including at least one longitudinally extending stiffening element;

pouring a resin into the mold to form a backing member having the at least one stiffening element embedded therein; and

20 assembling the backing member to a piezoelectric element and at least one matching layer to form a transducer array wherein said piezoelectric member is sandwiched between said at least one matching layer and said backing member.

13. A method as claimed in claim 12 further comprising using shaped molding members to form a lens on a distal surface of said at least one matching layer.

14. A method as claimed in claim 12 further comprising using shaped molding members with matching hemicylindrical cut out portions to mold a cylindrical resin covering for said transducer array.

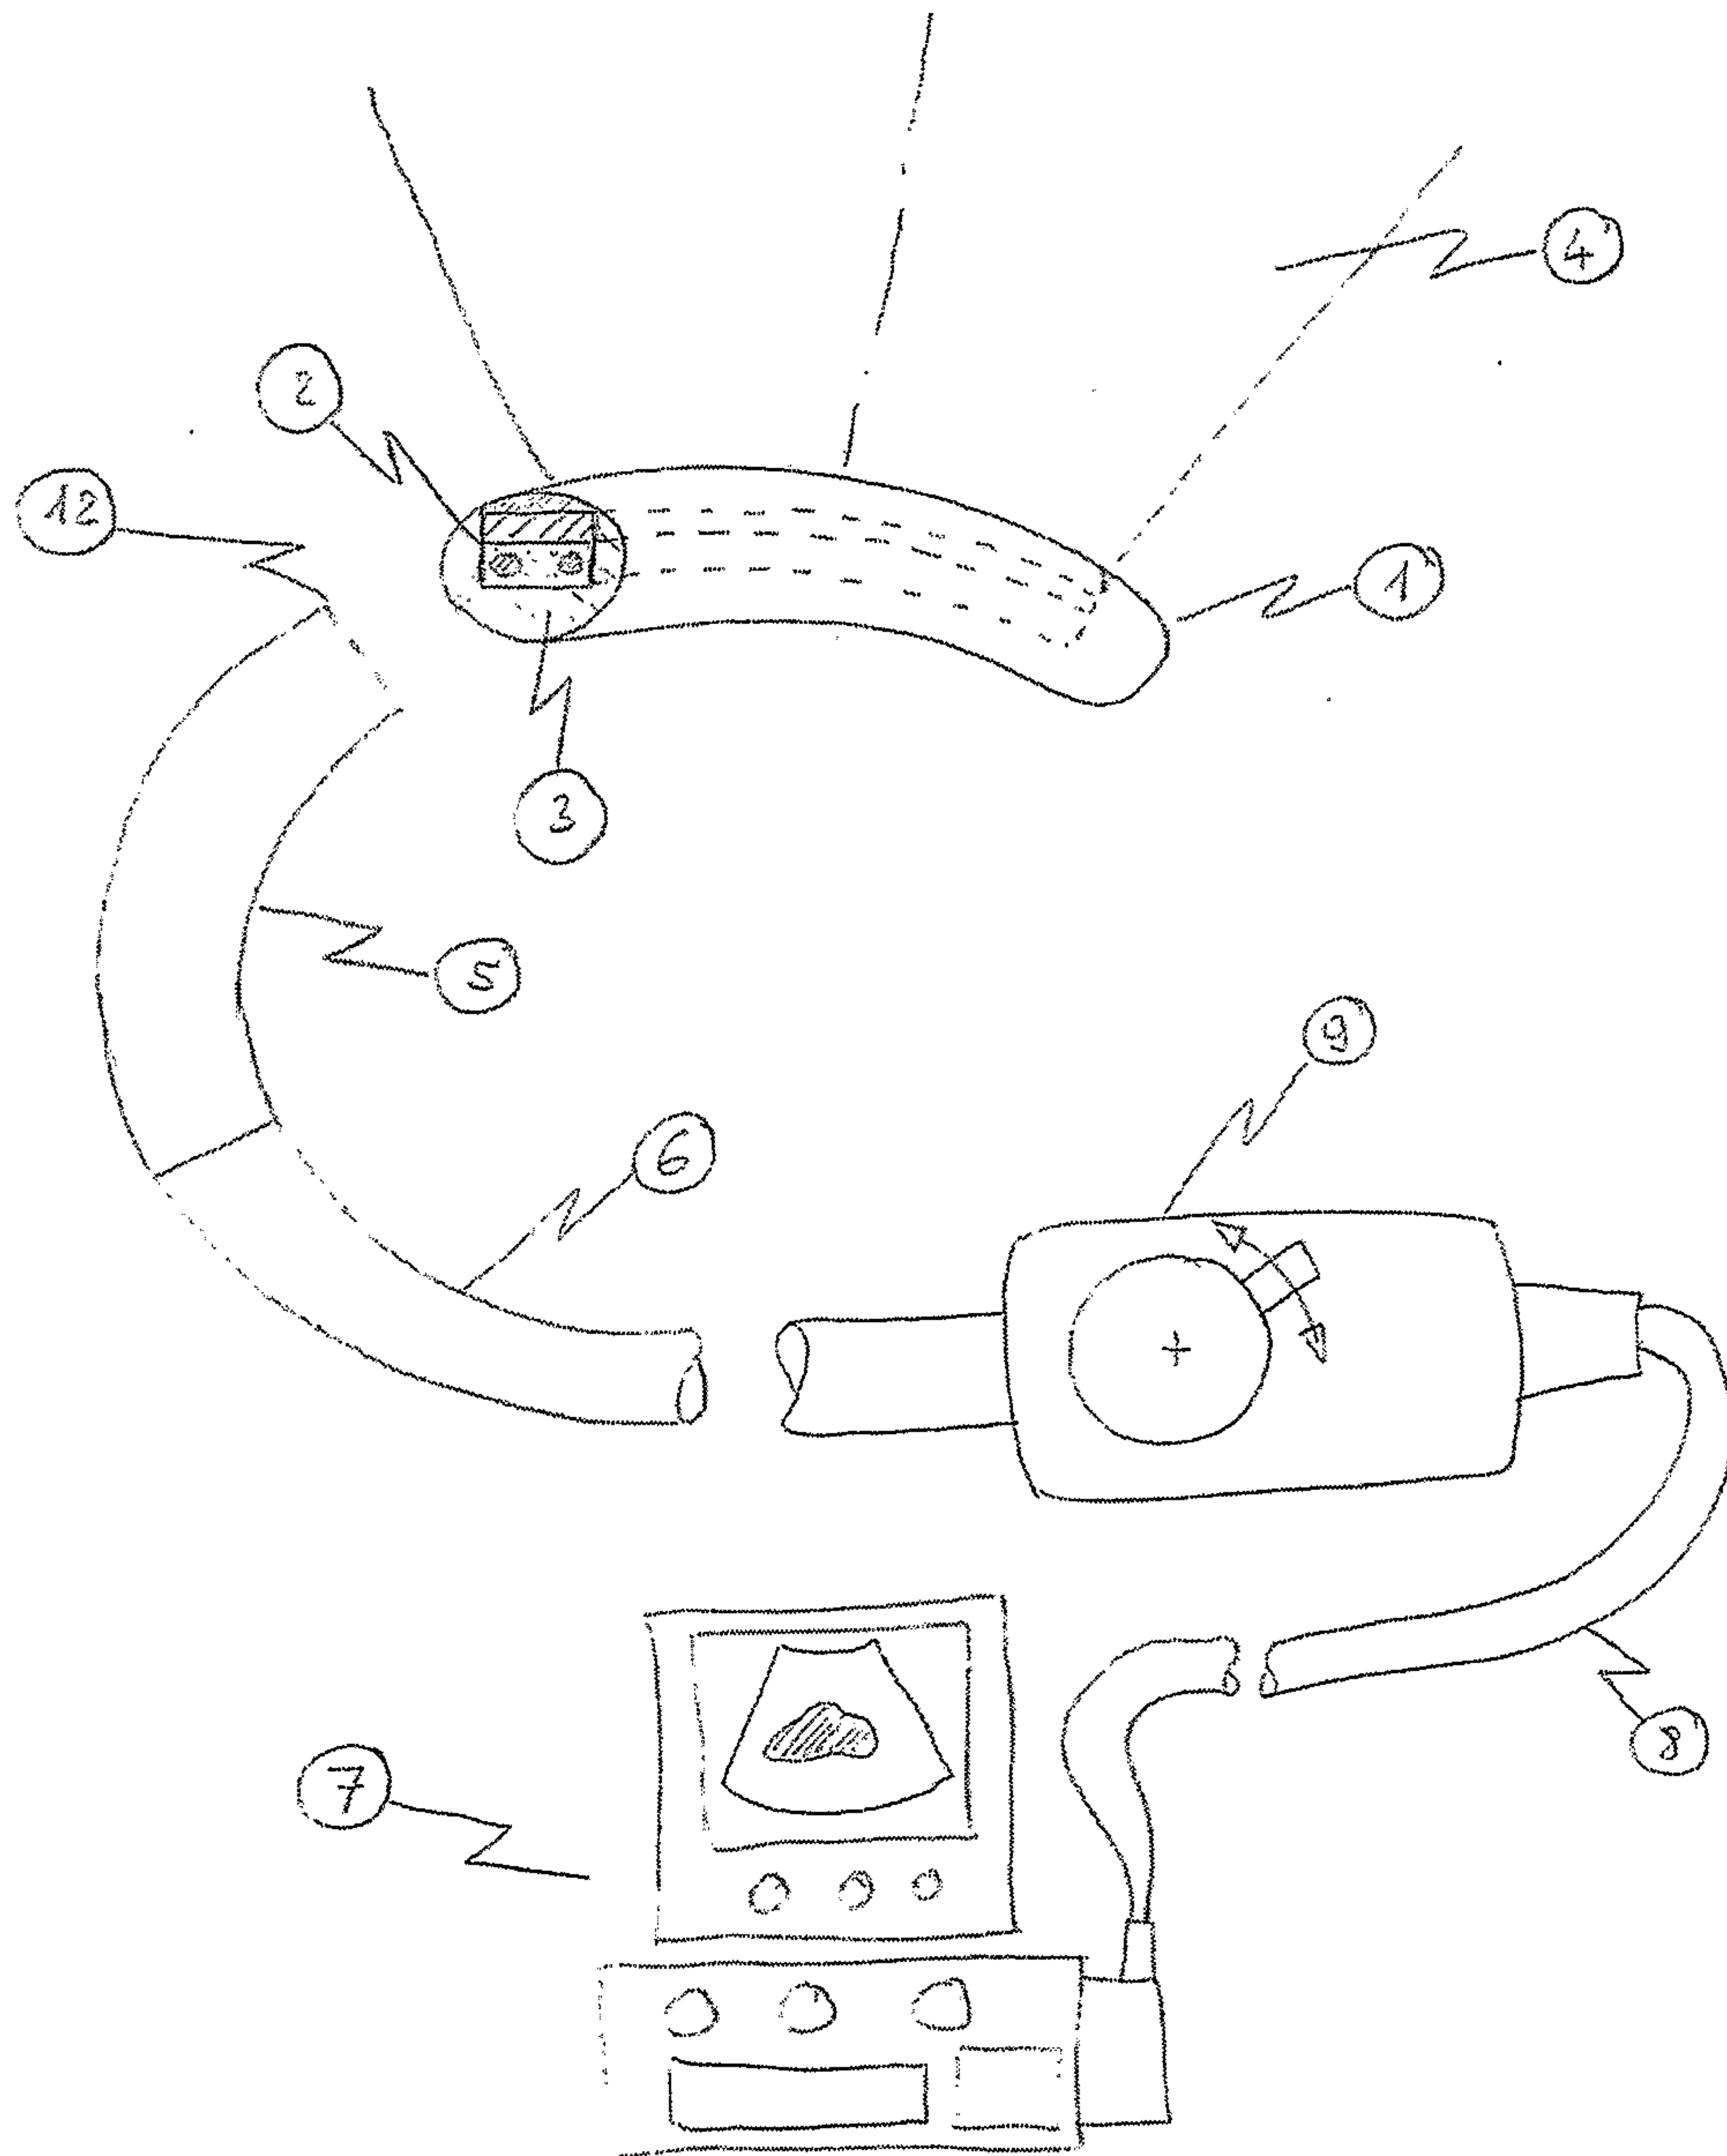
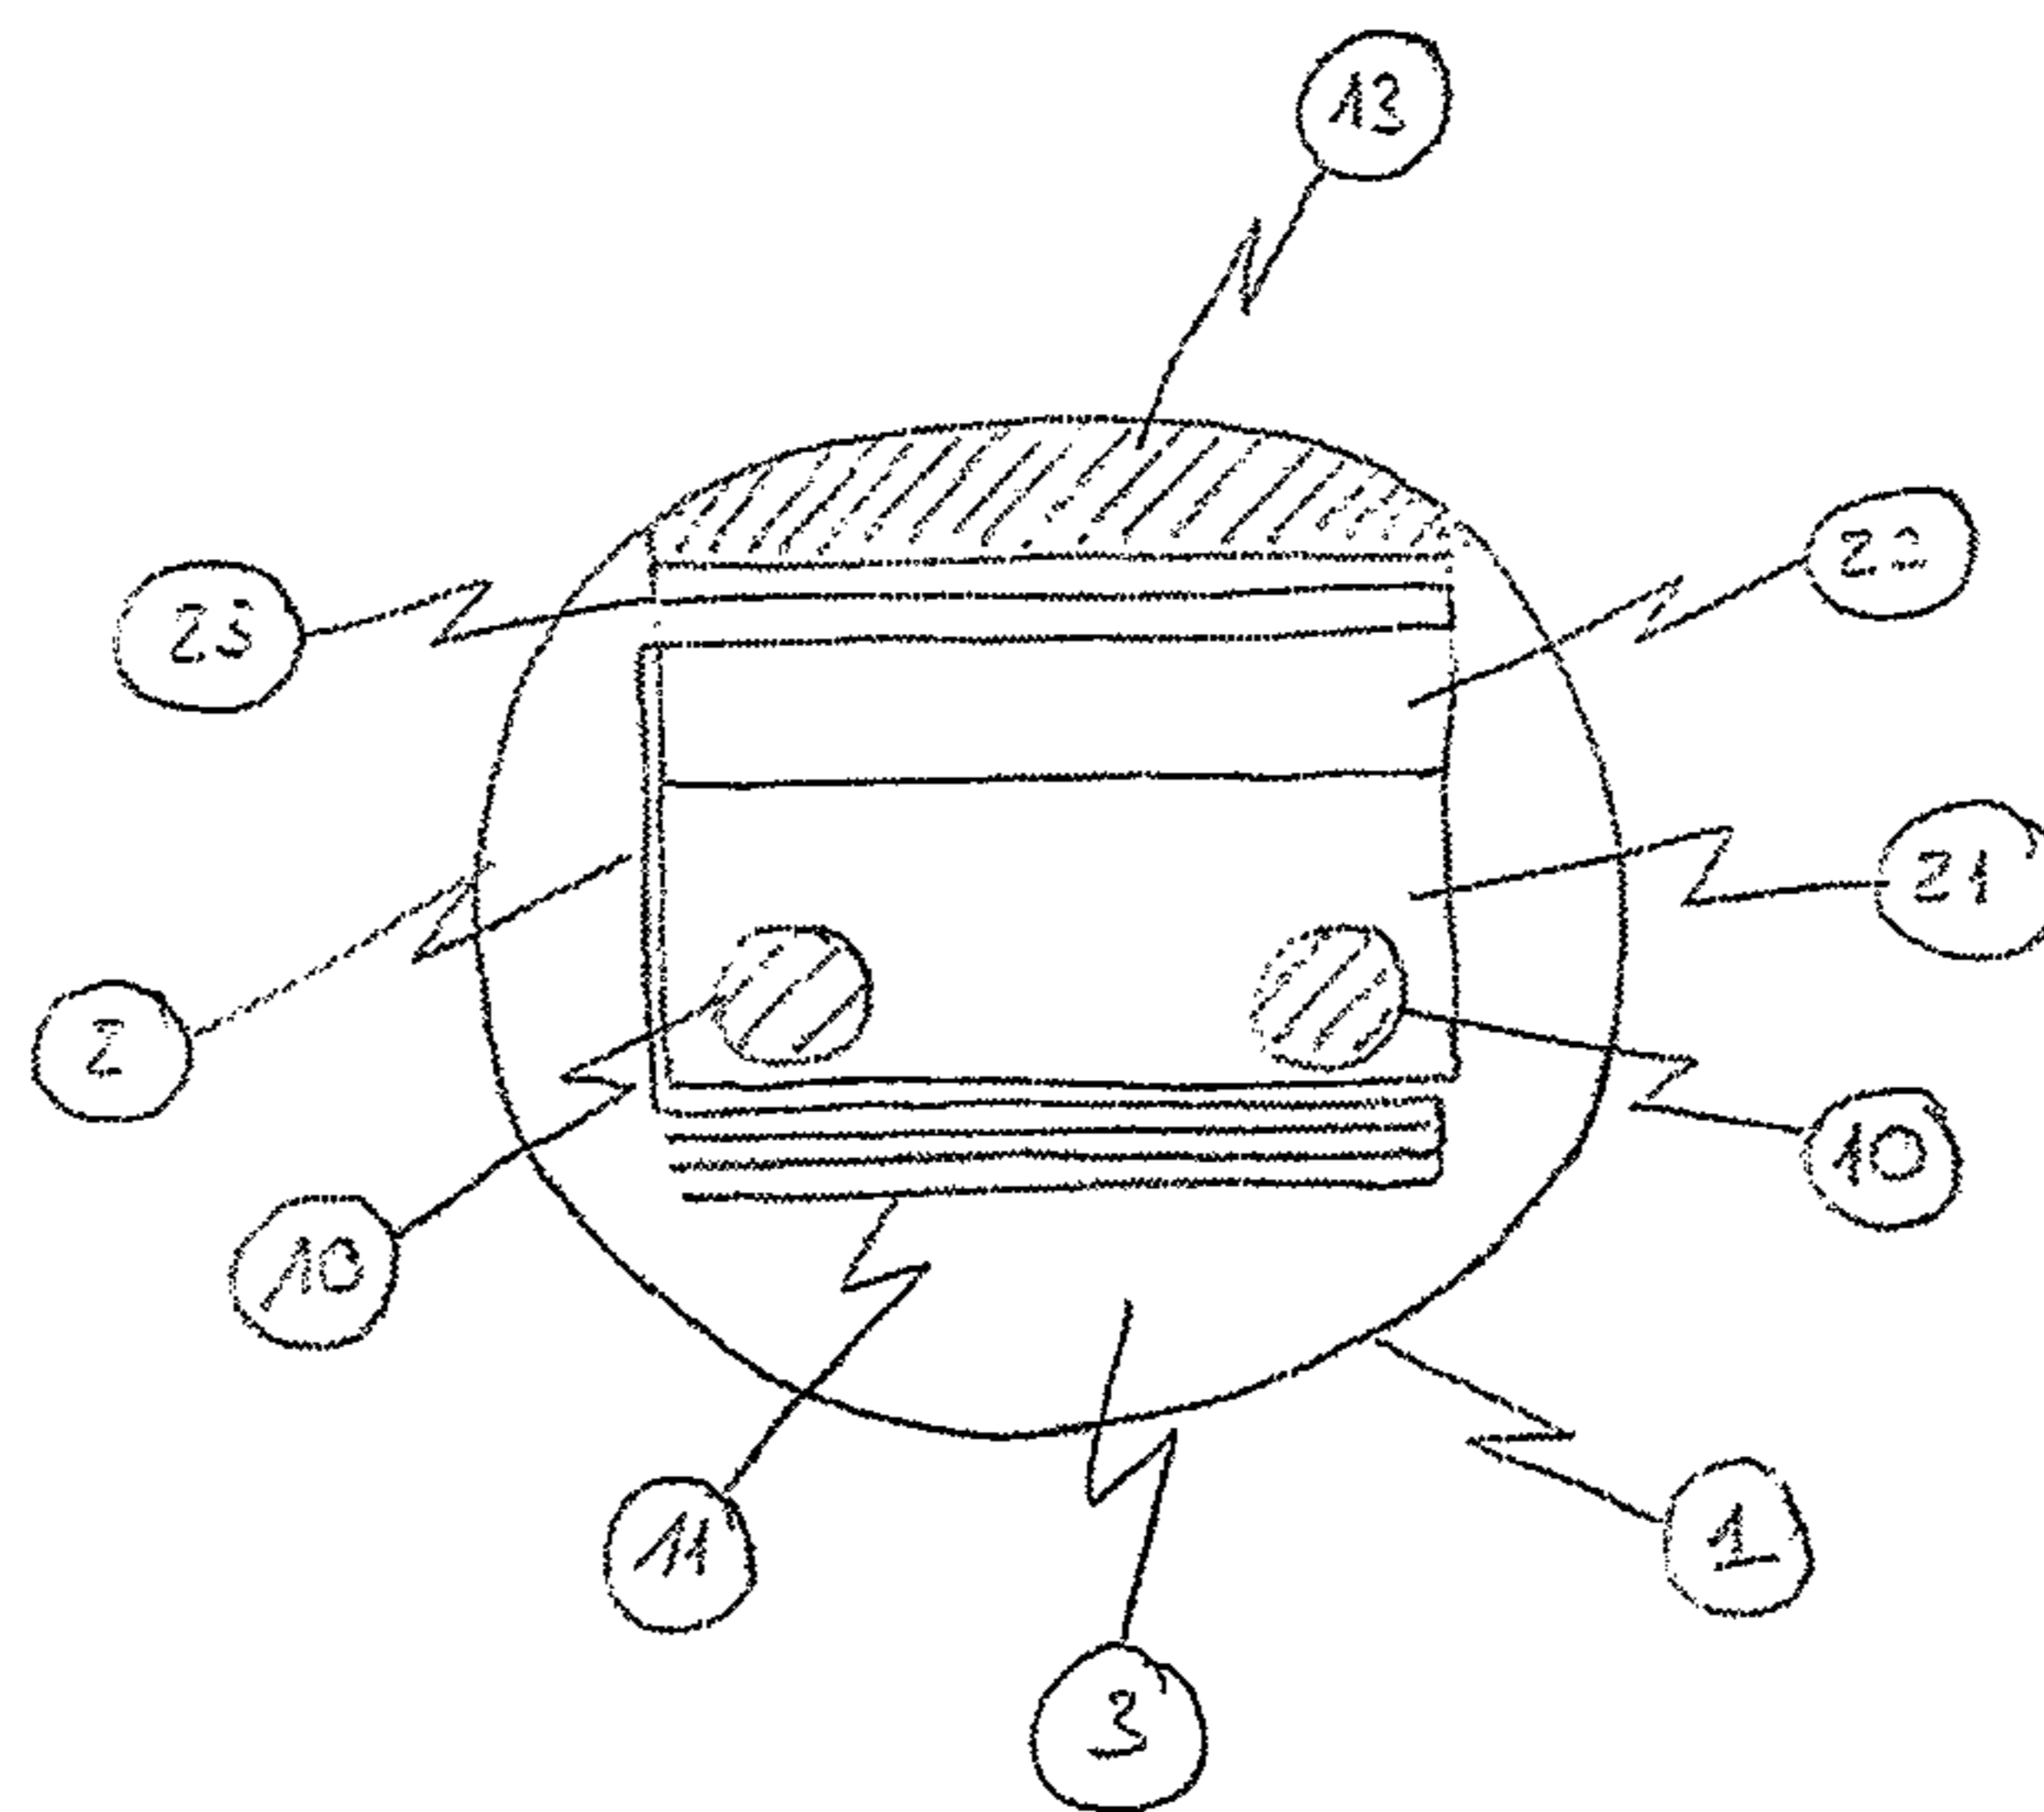
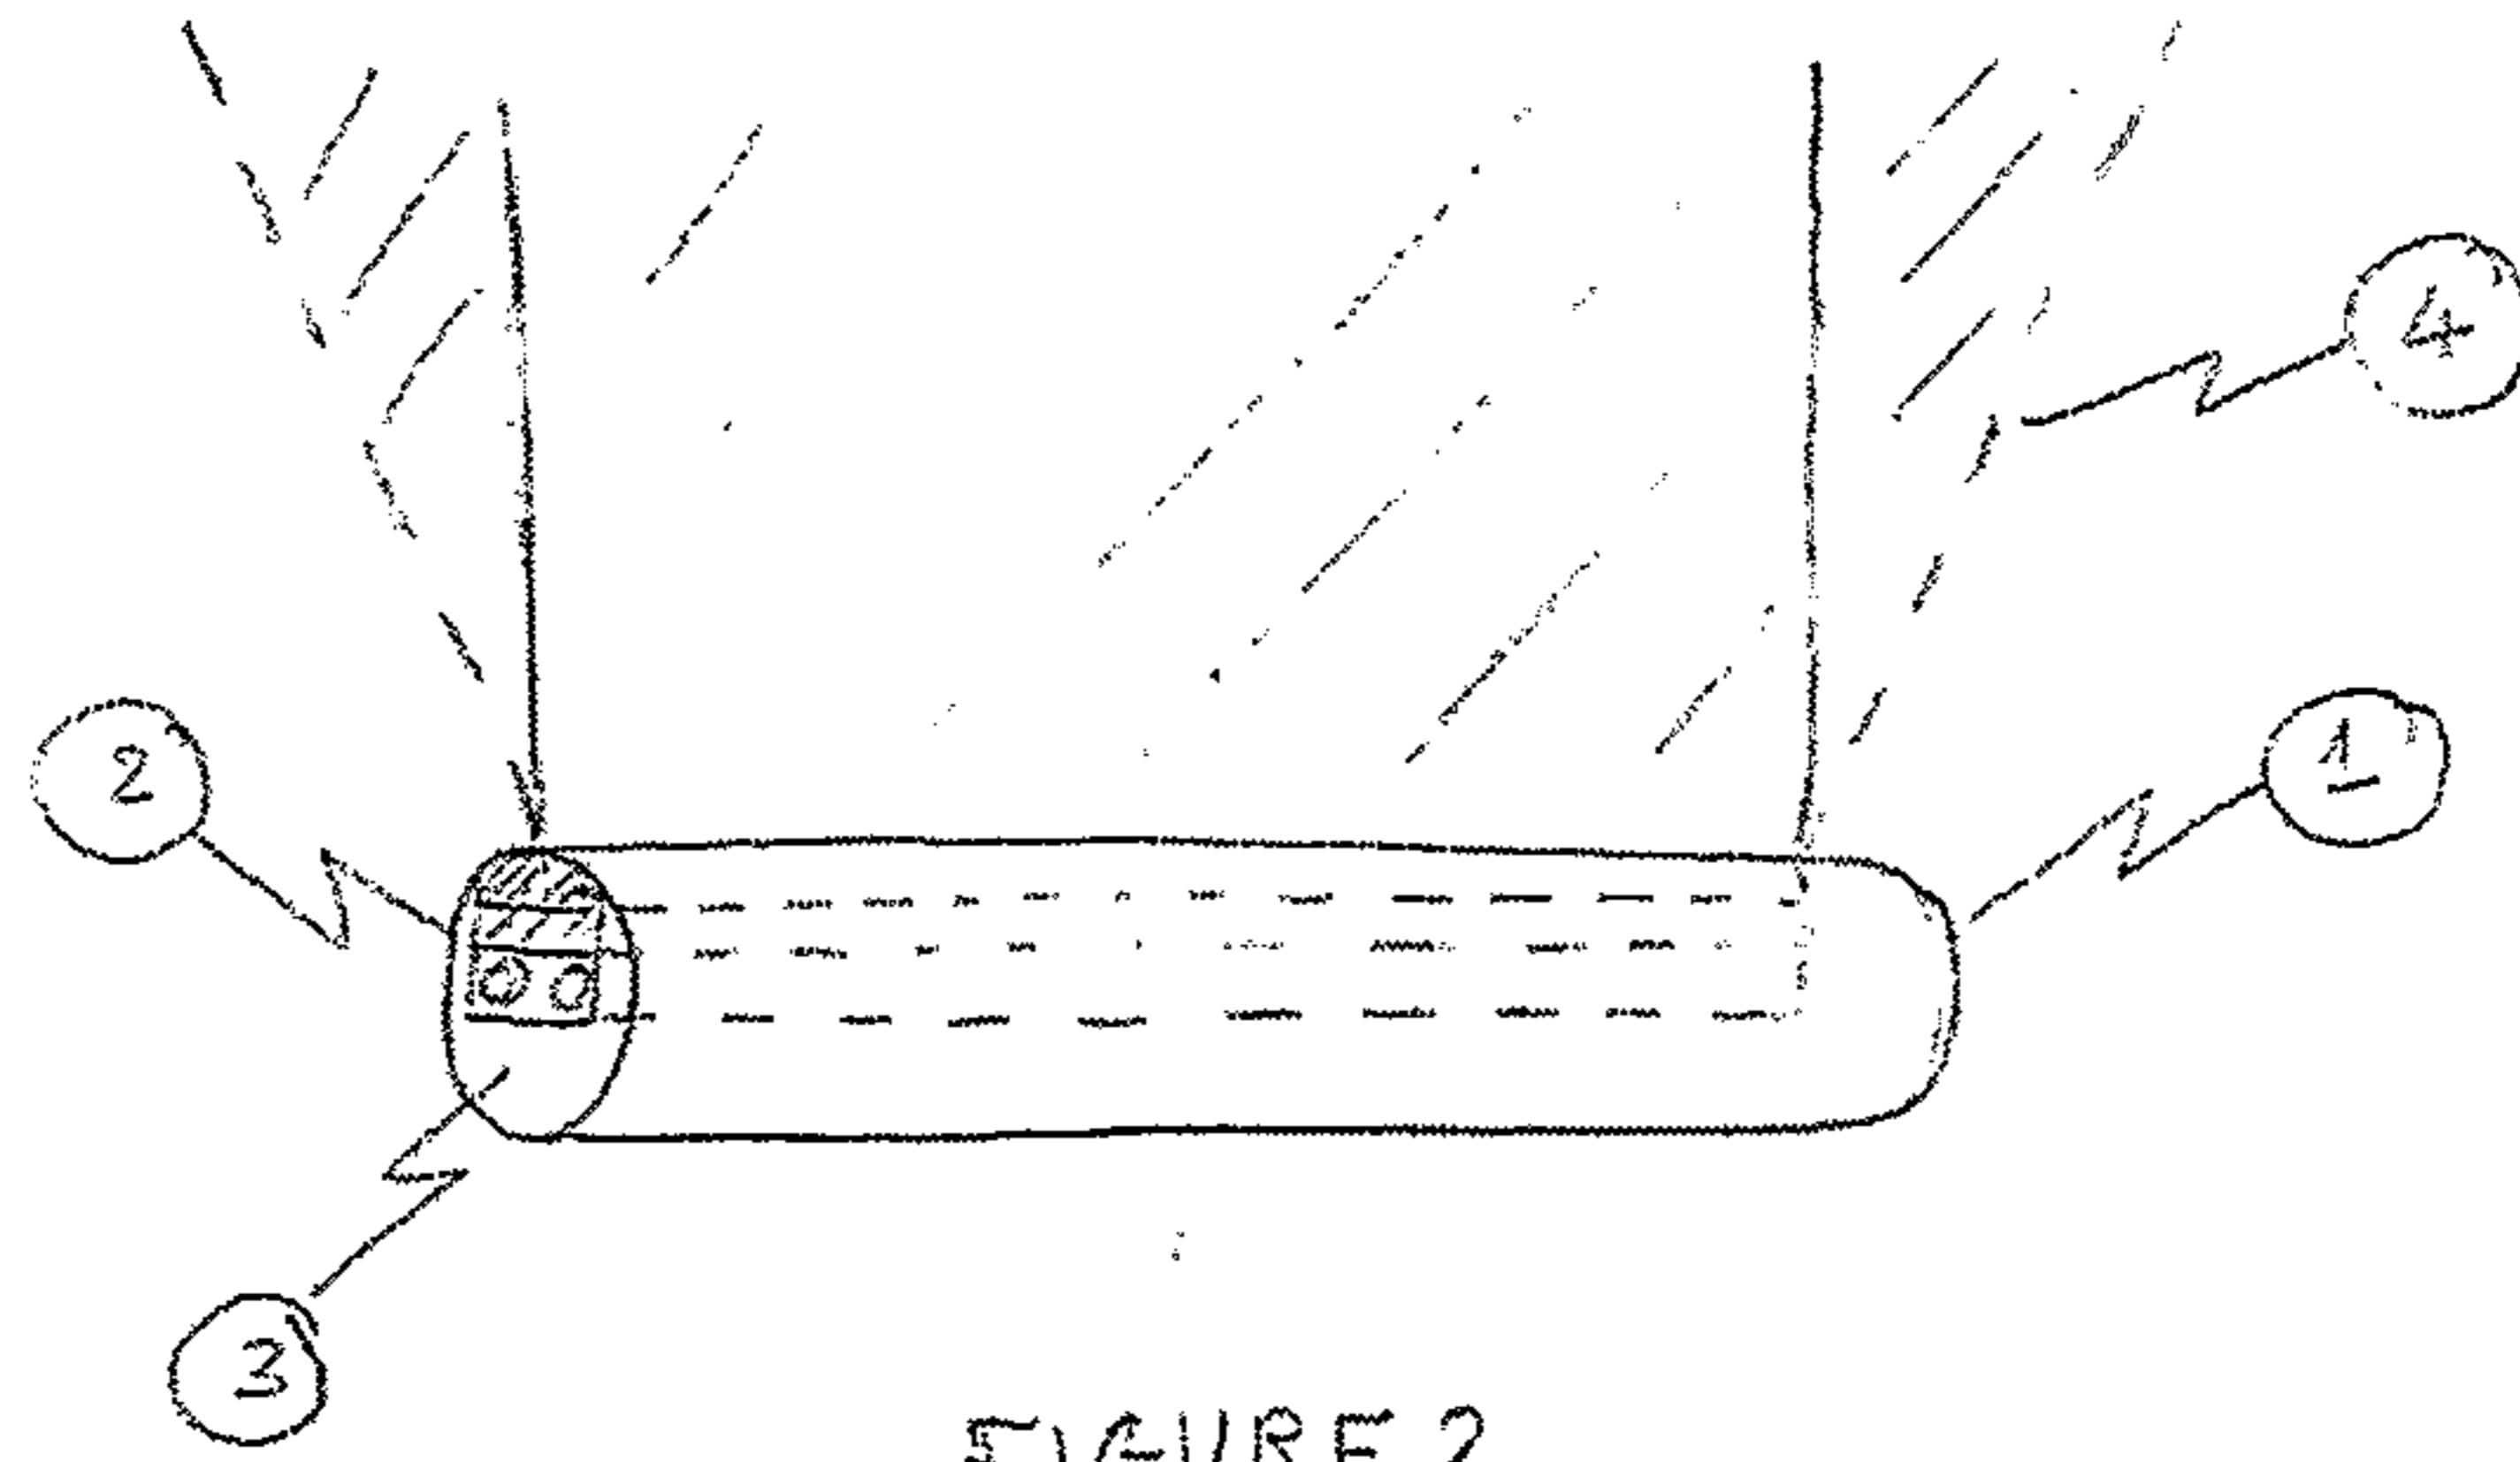


FIGURE 1



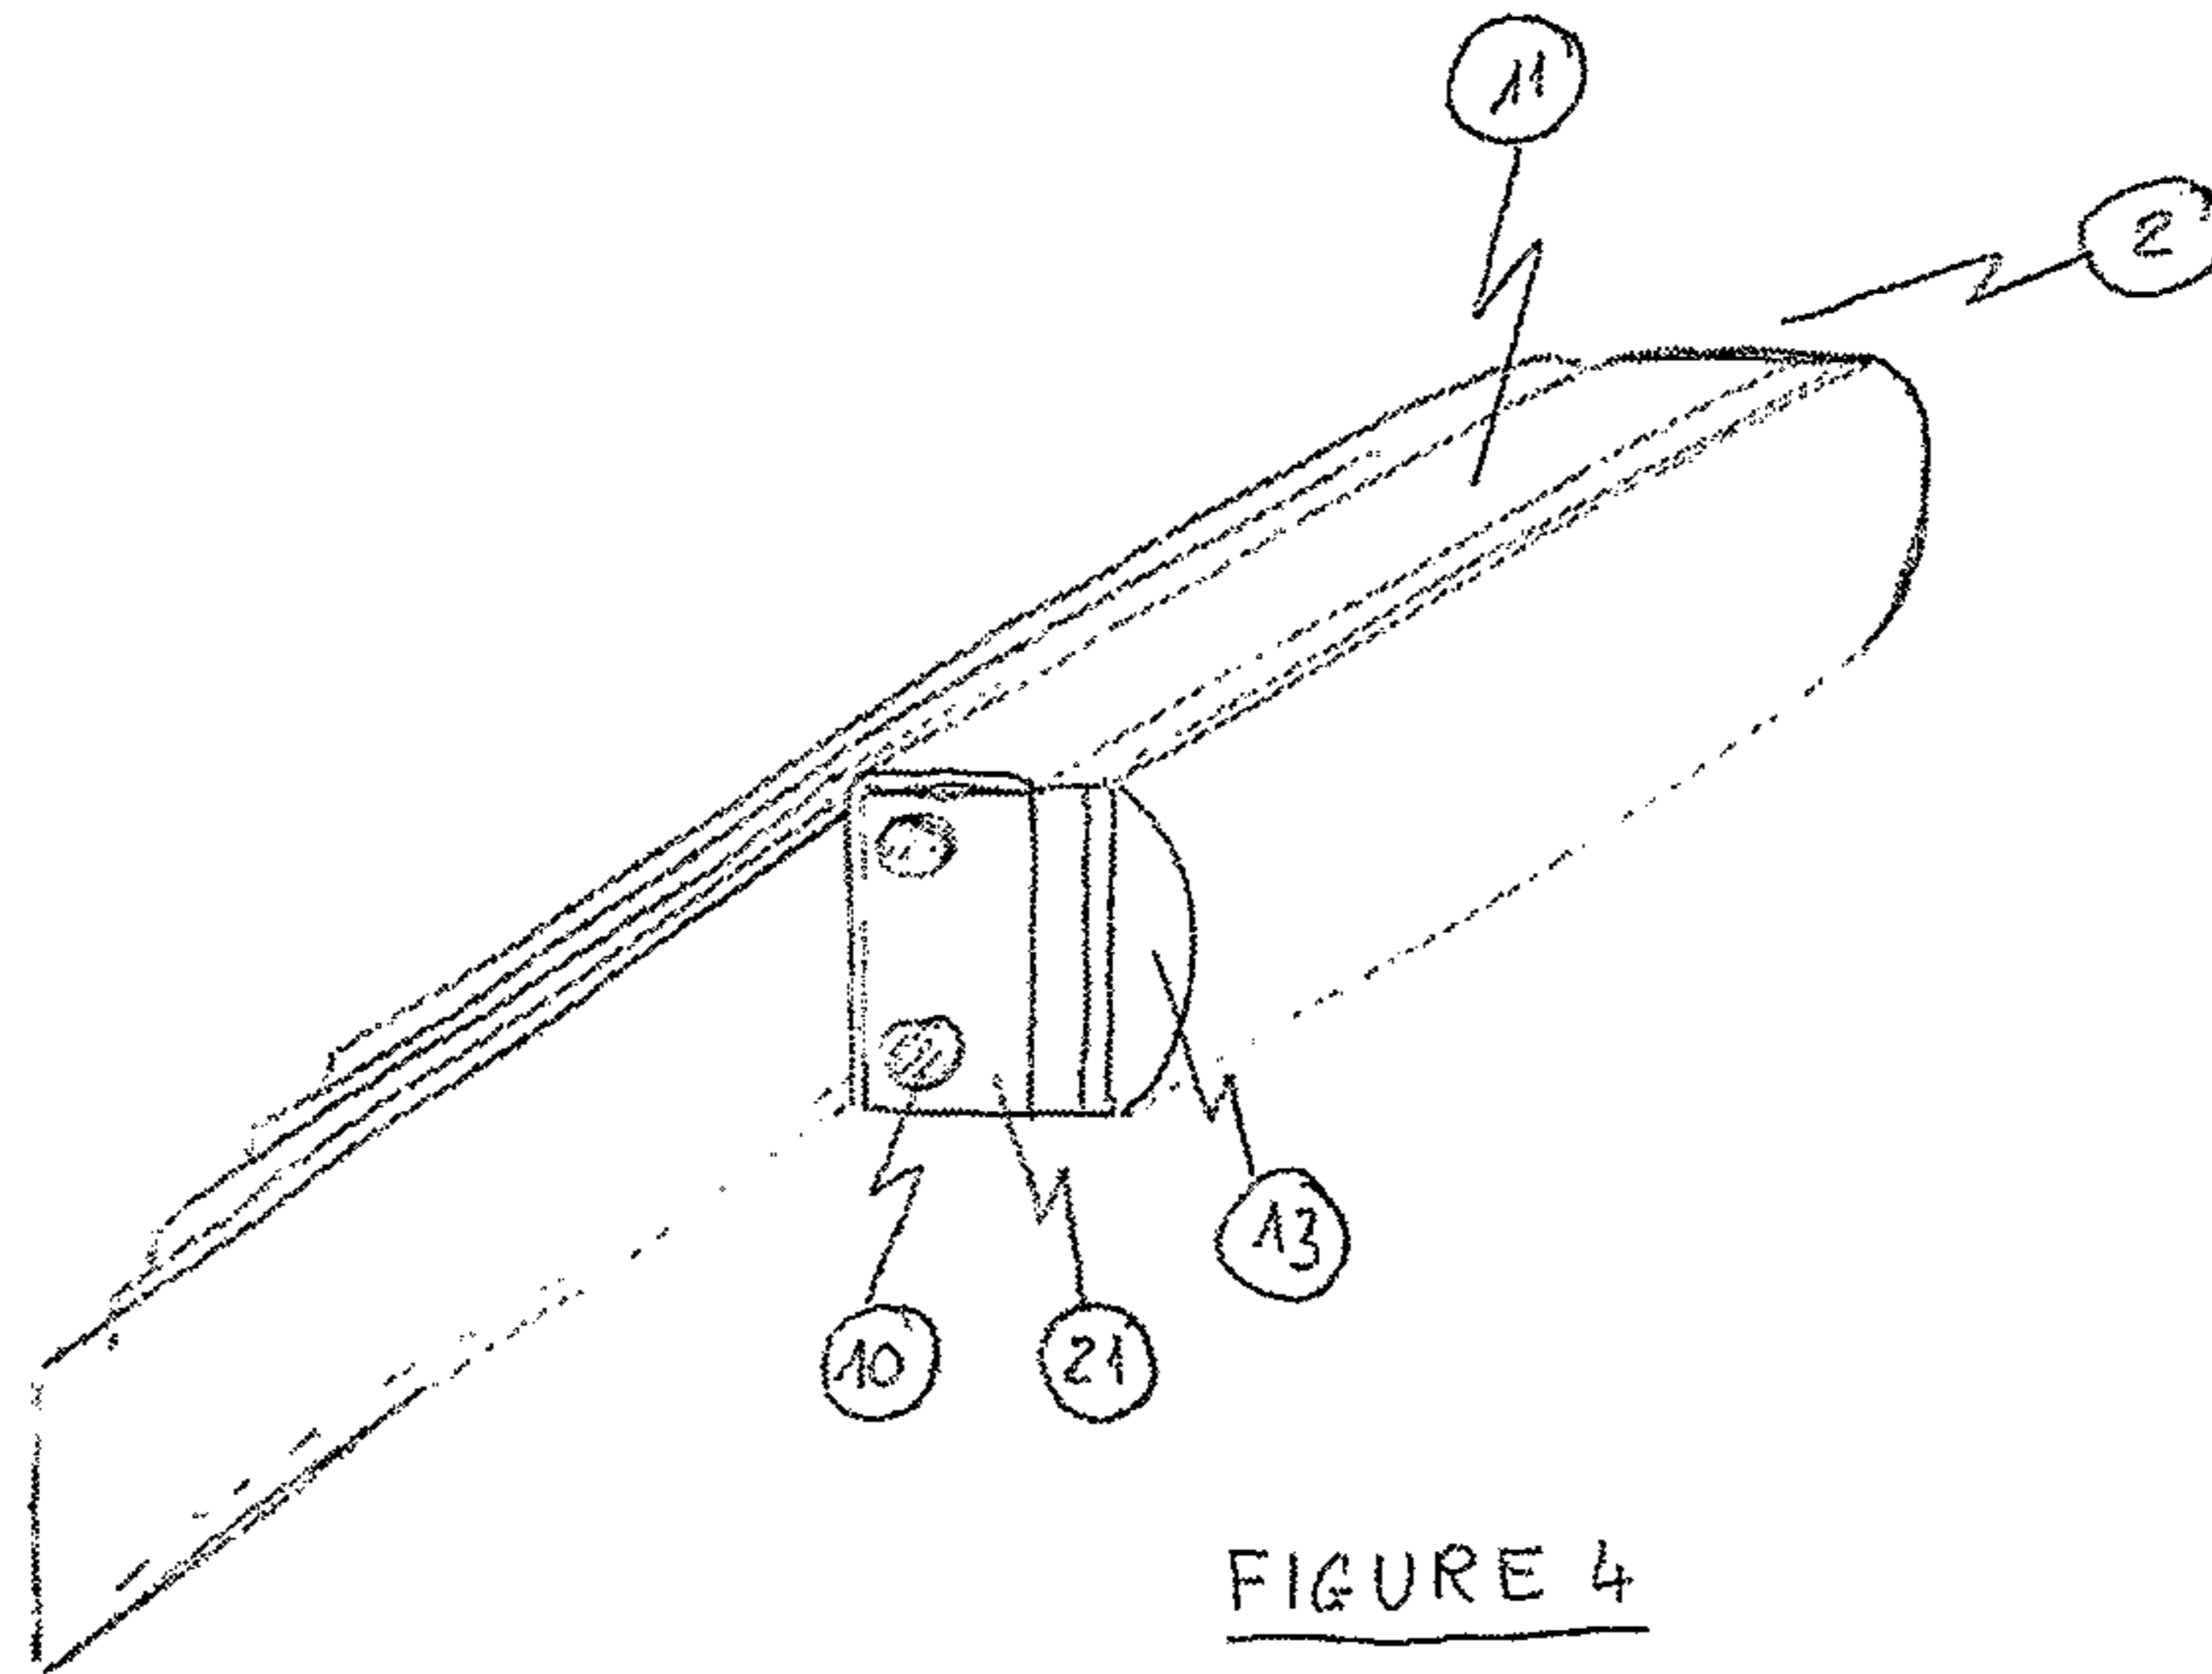


FIGURE 4

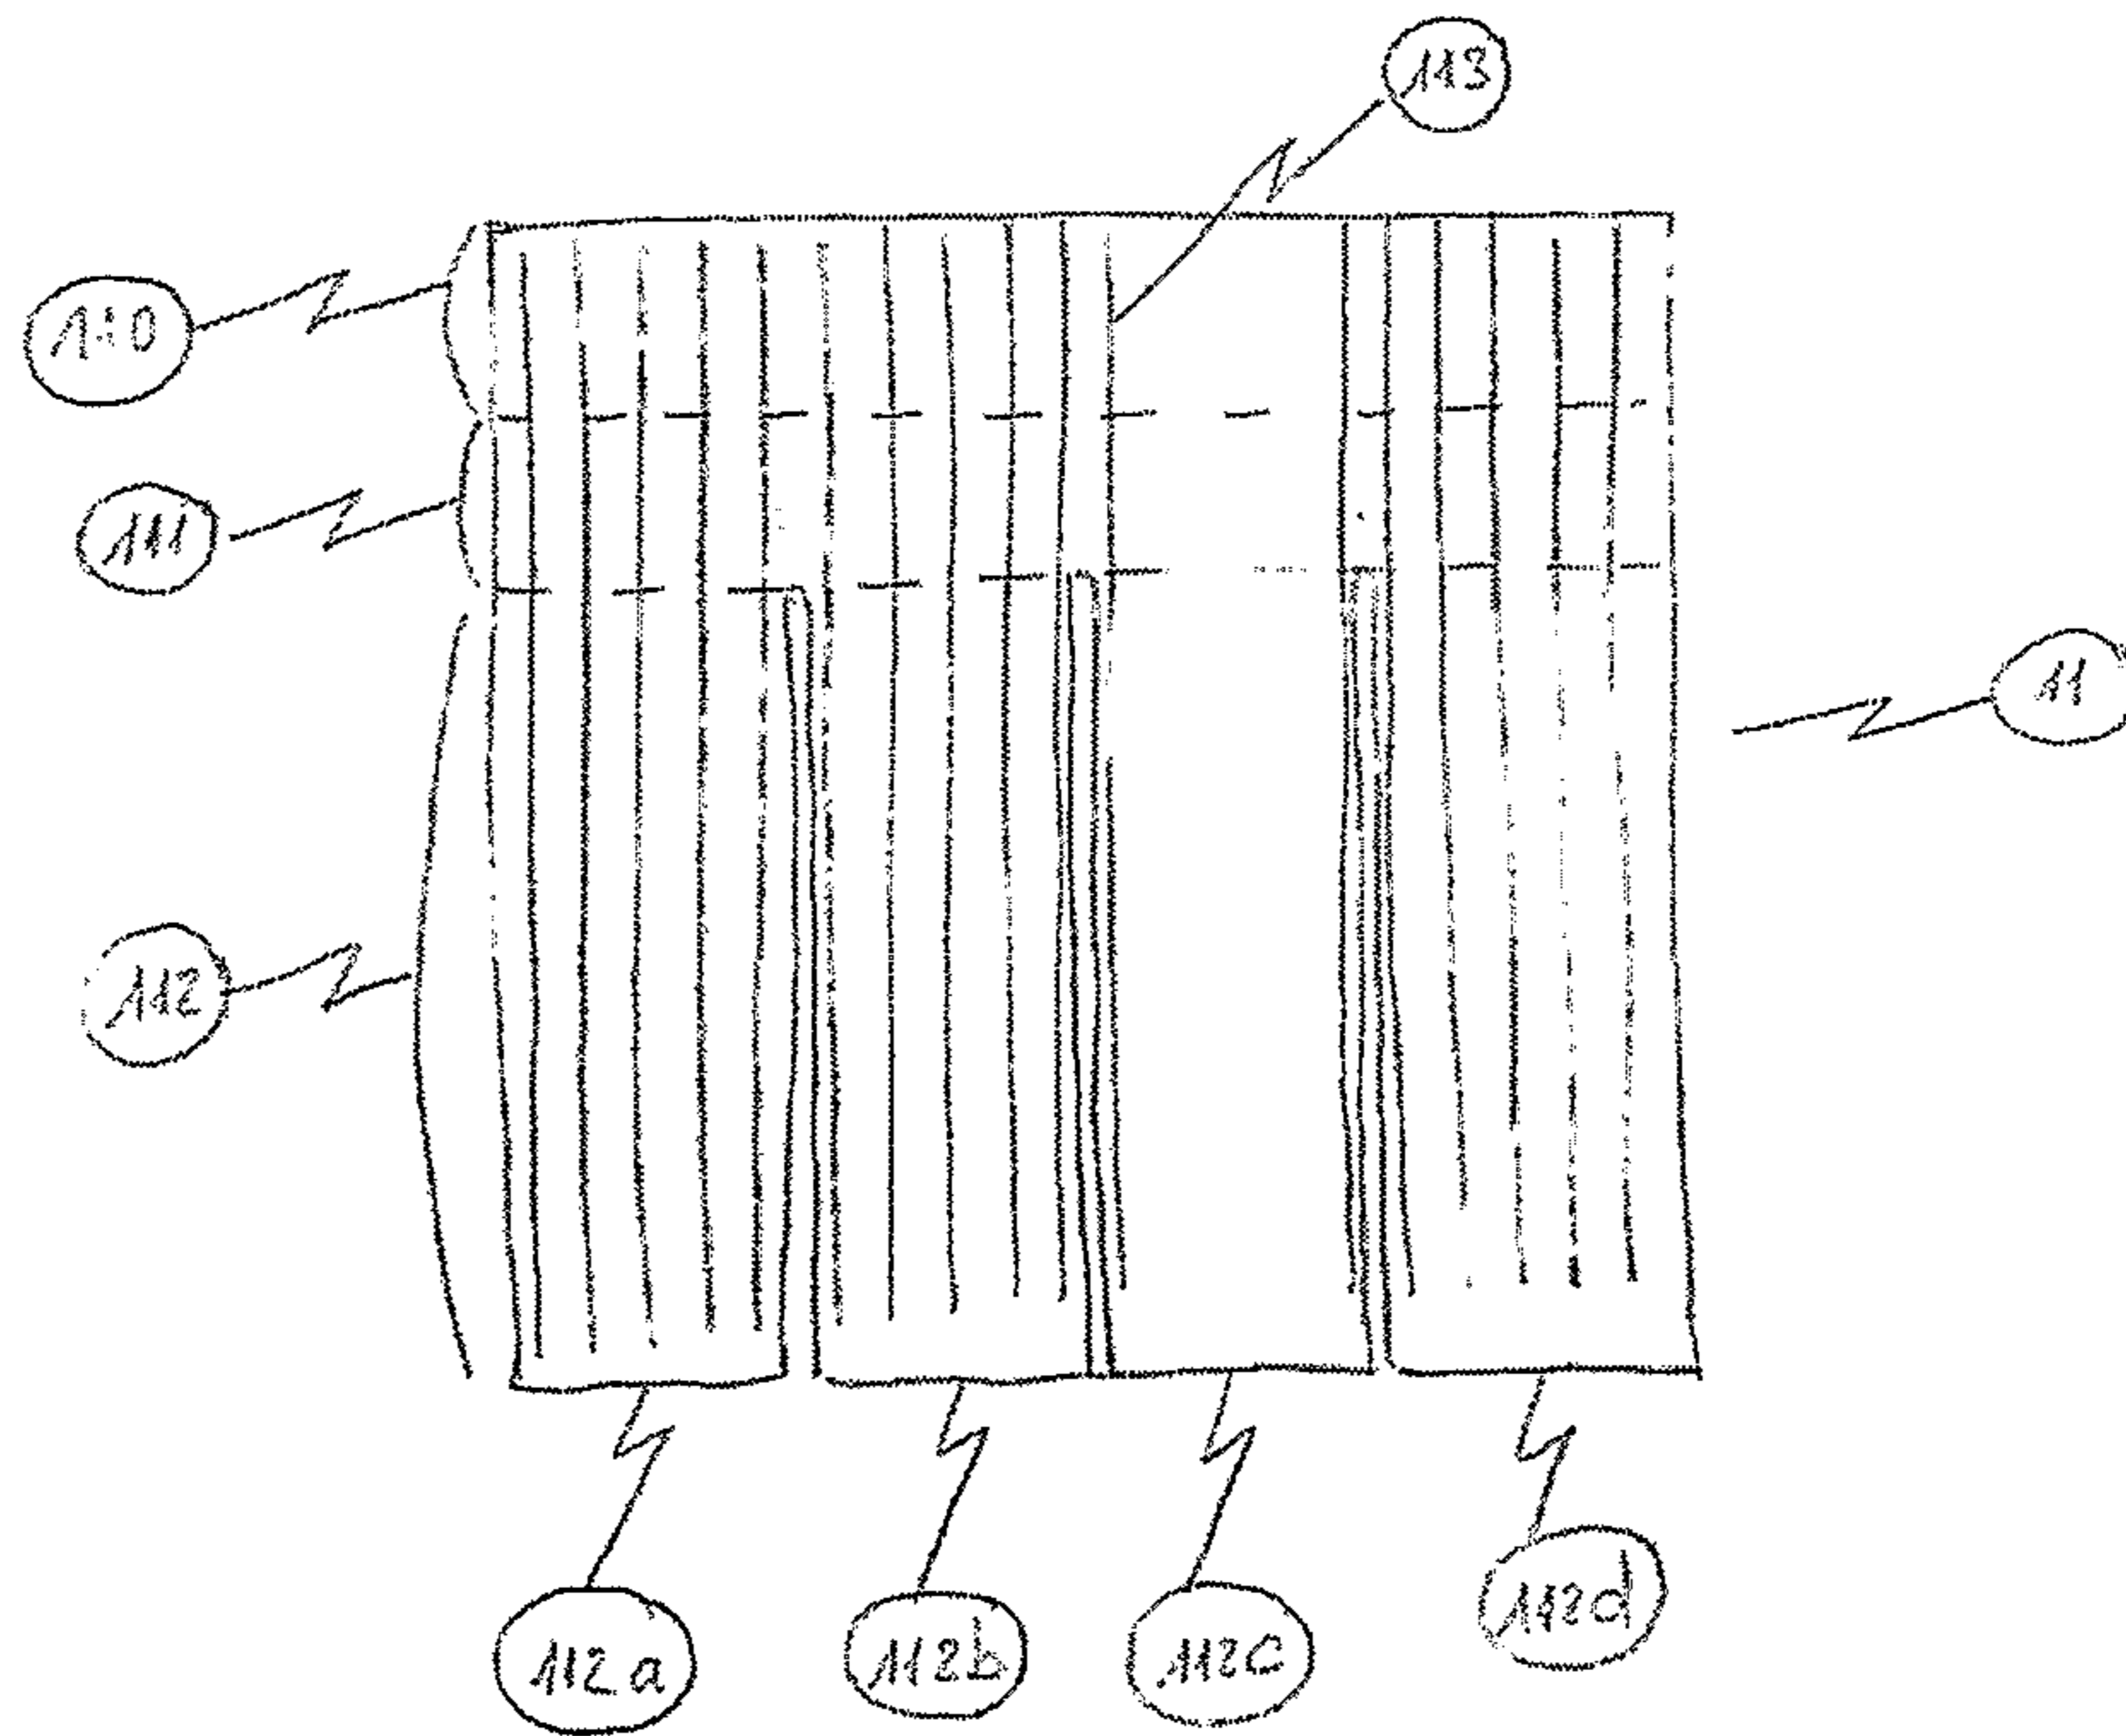


FIGURE 5

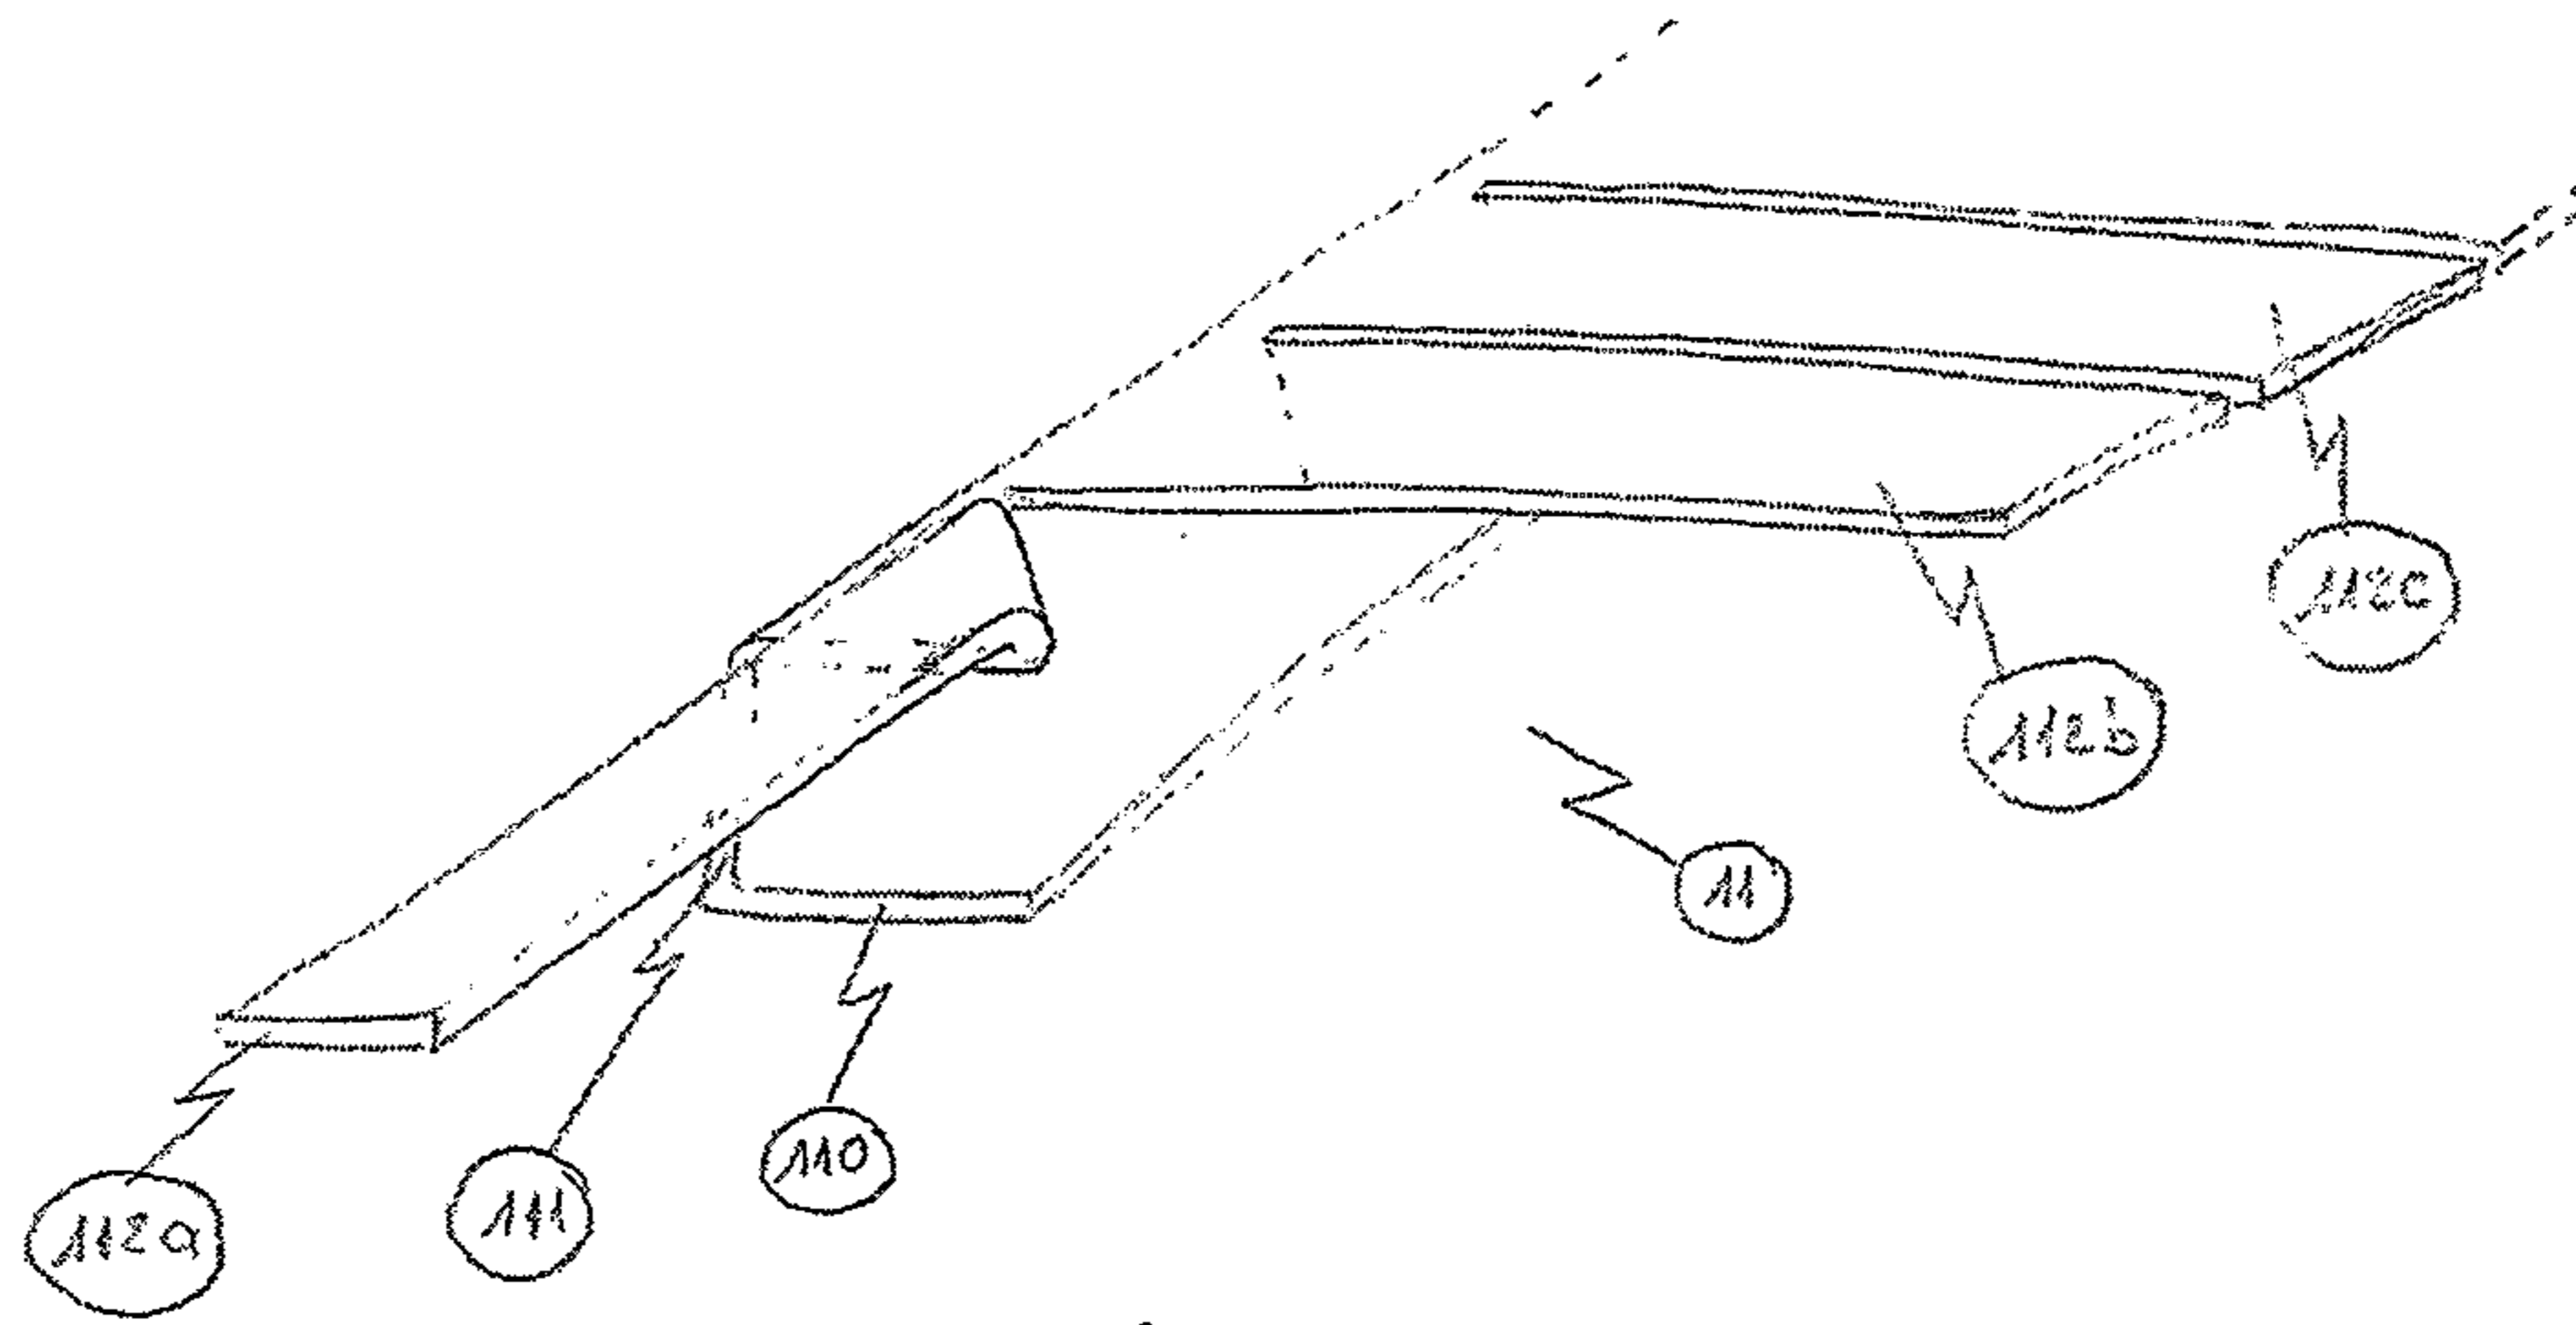


FIGURE 6

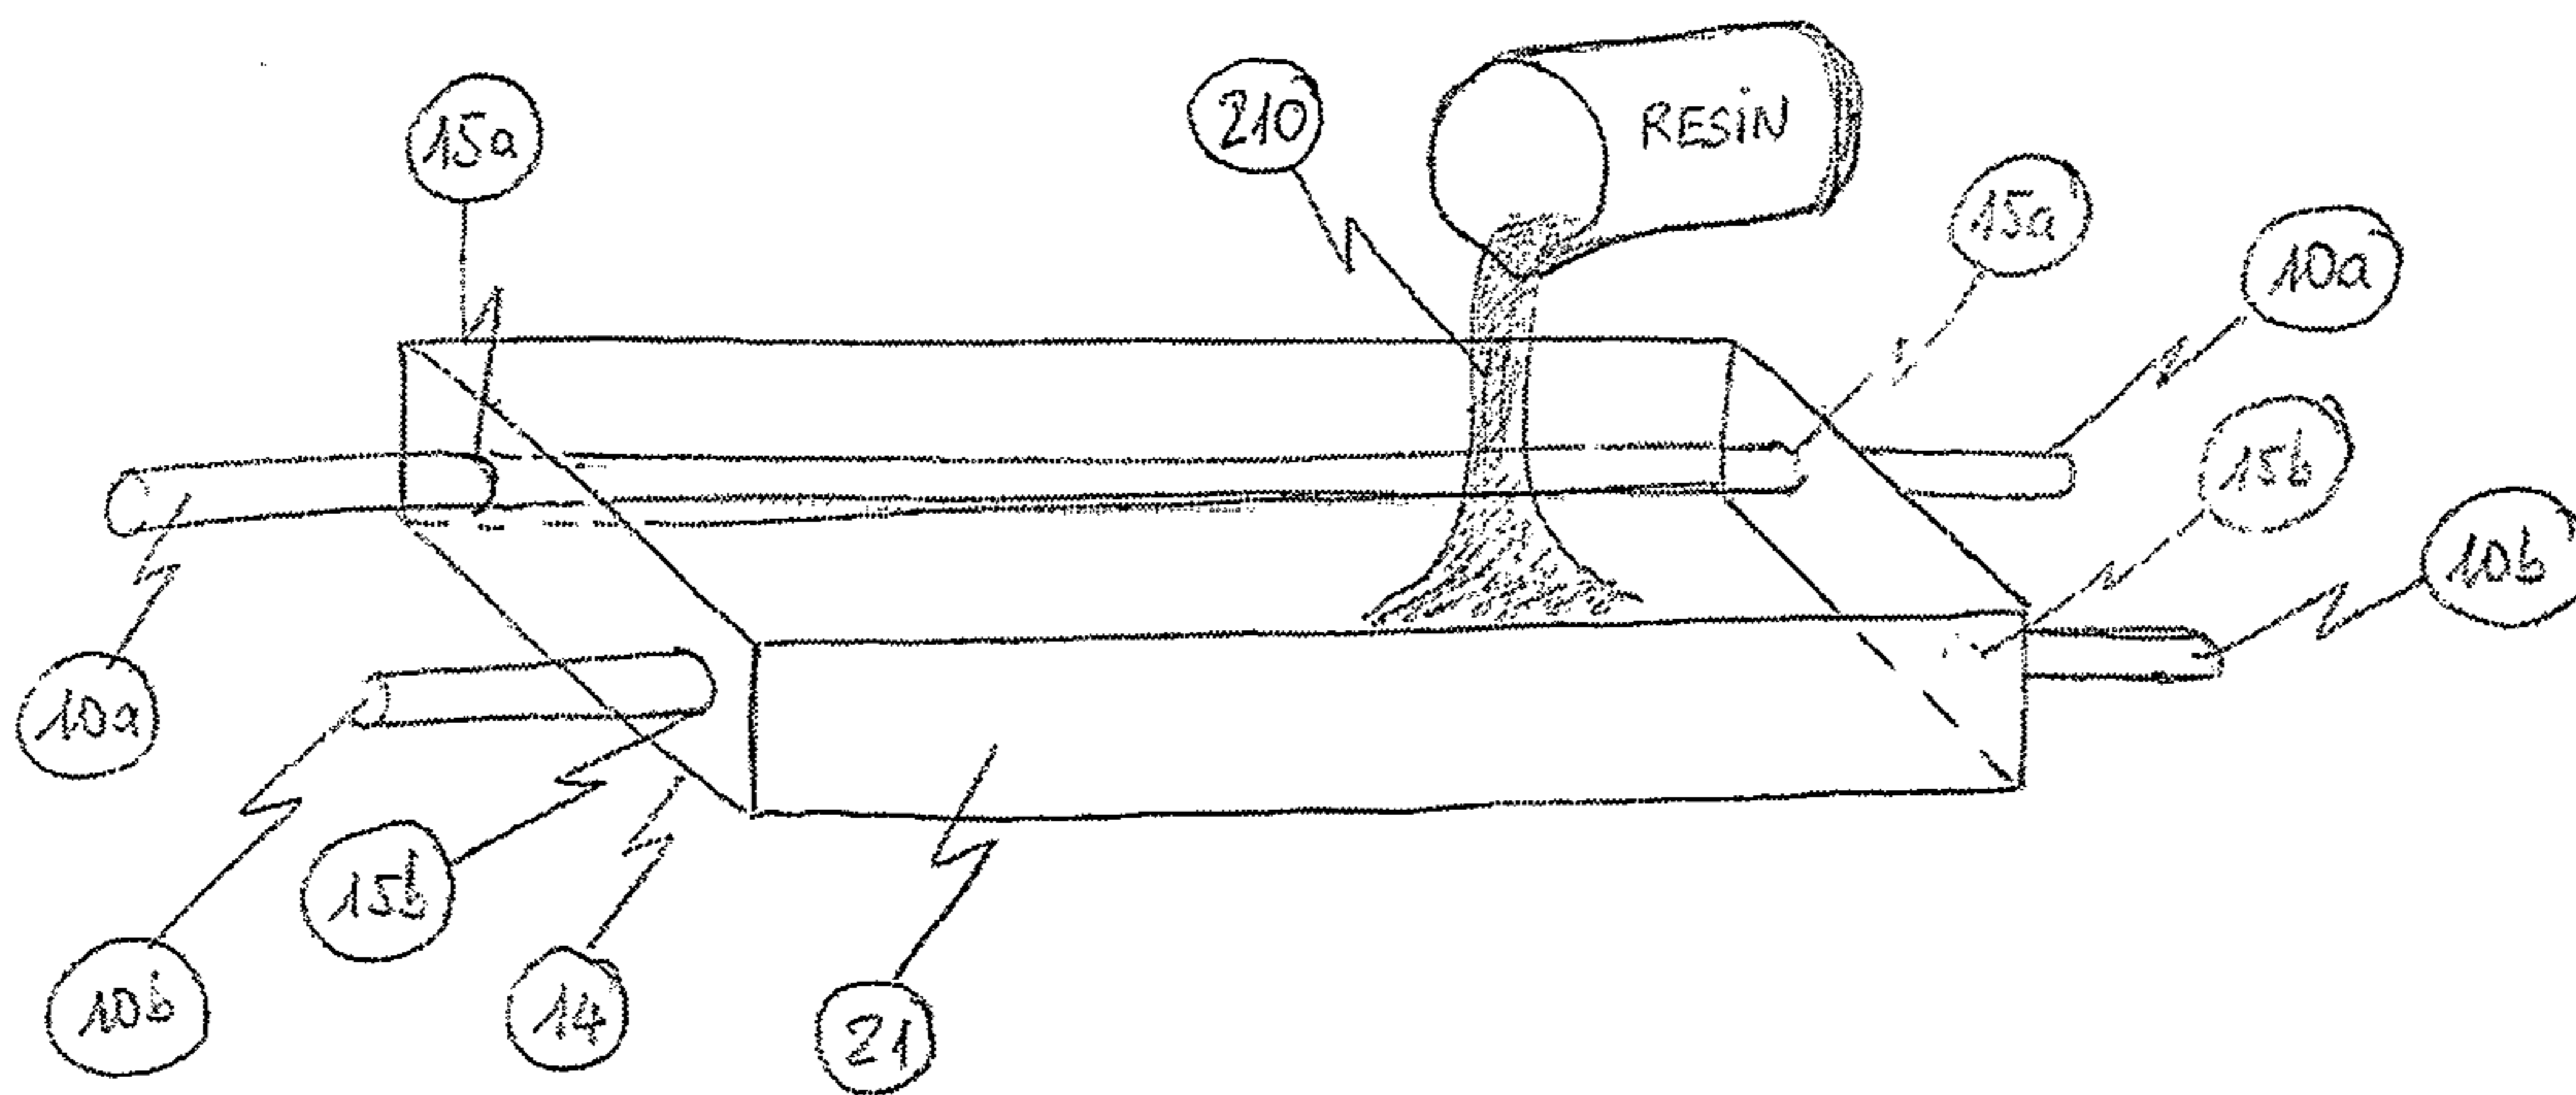


FIGURE 7

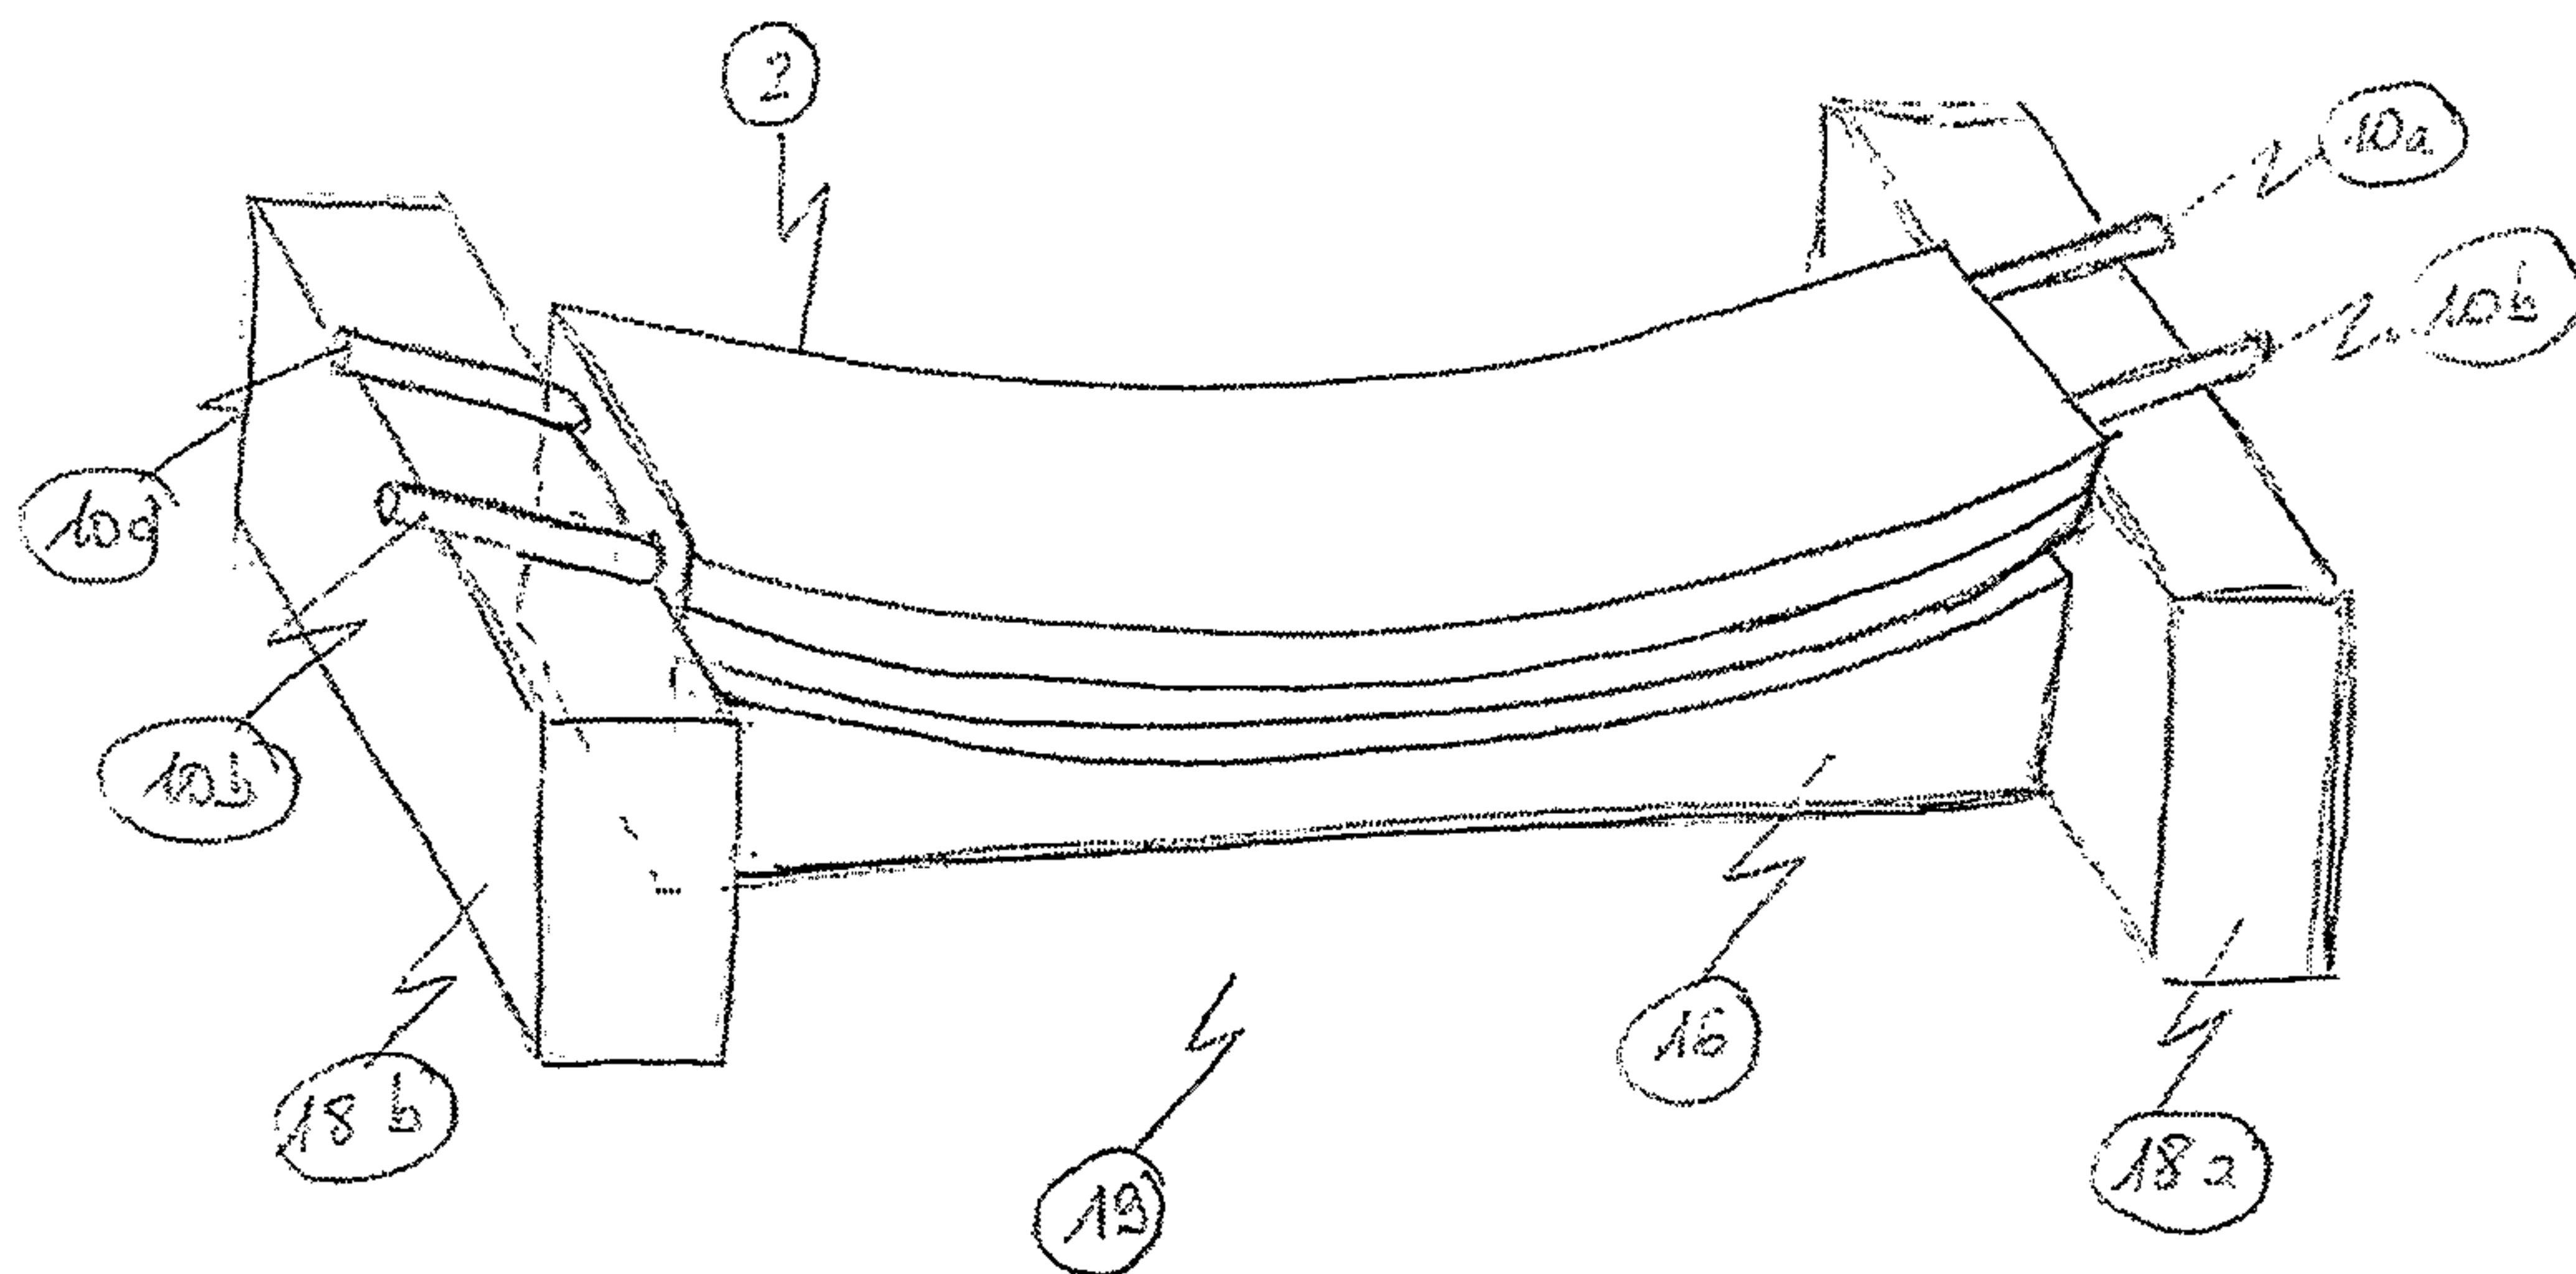


FIGURE 8

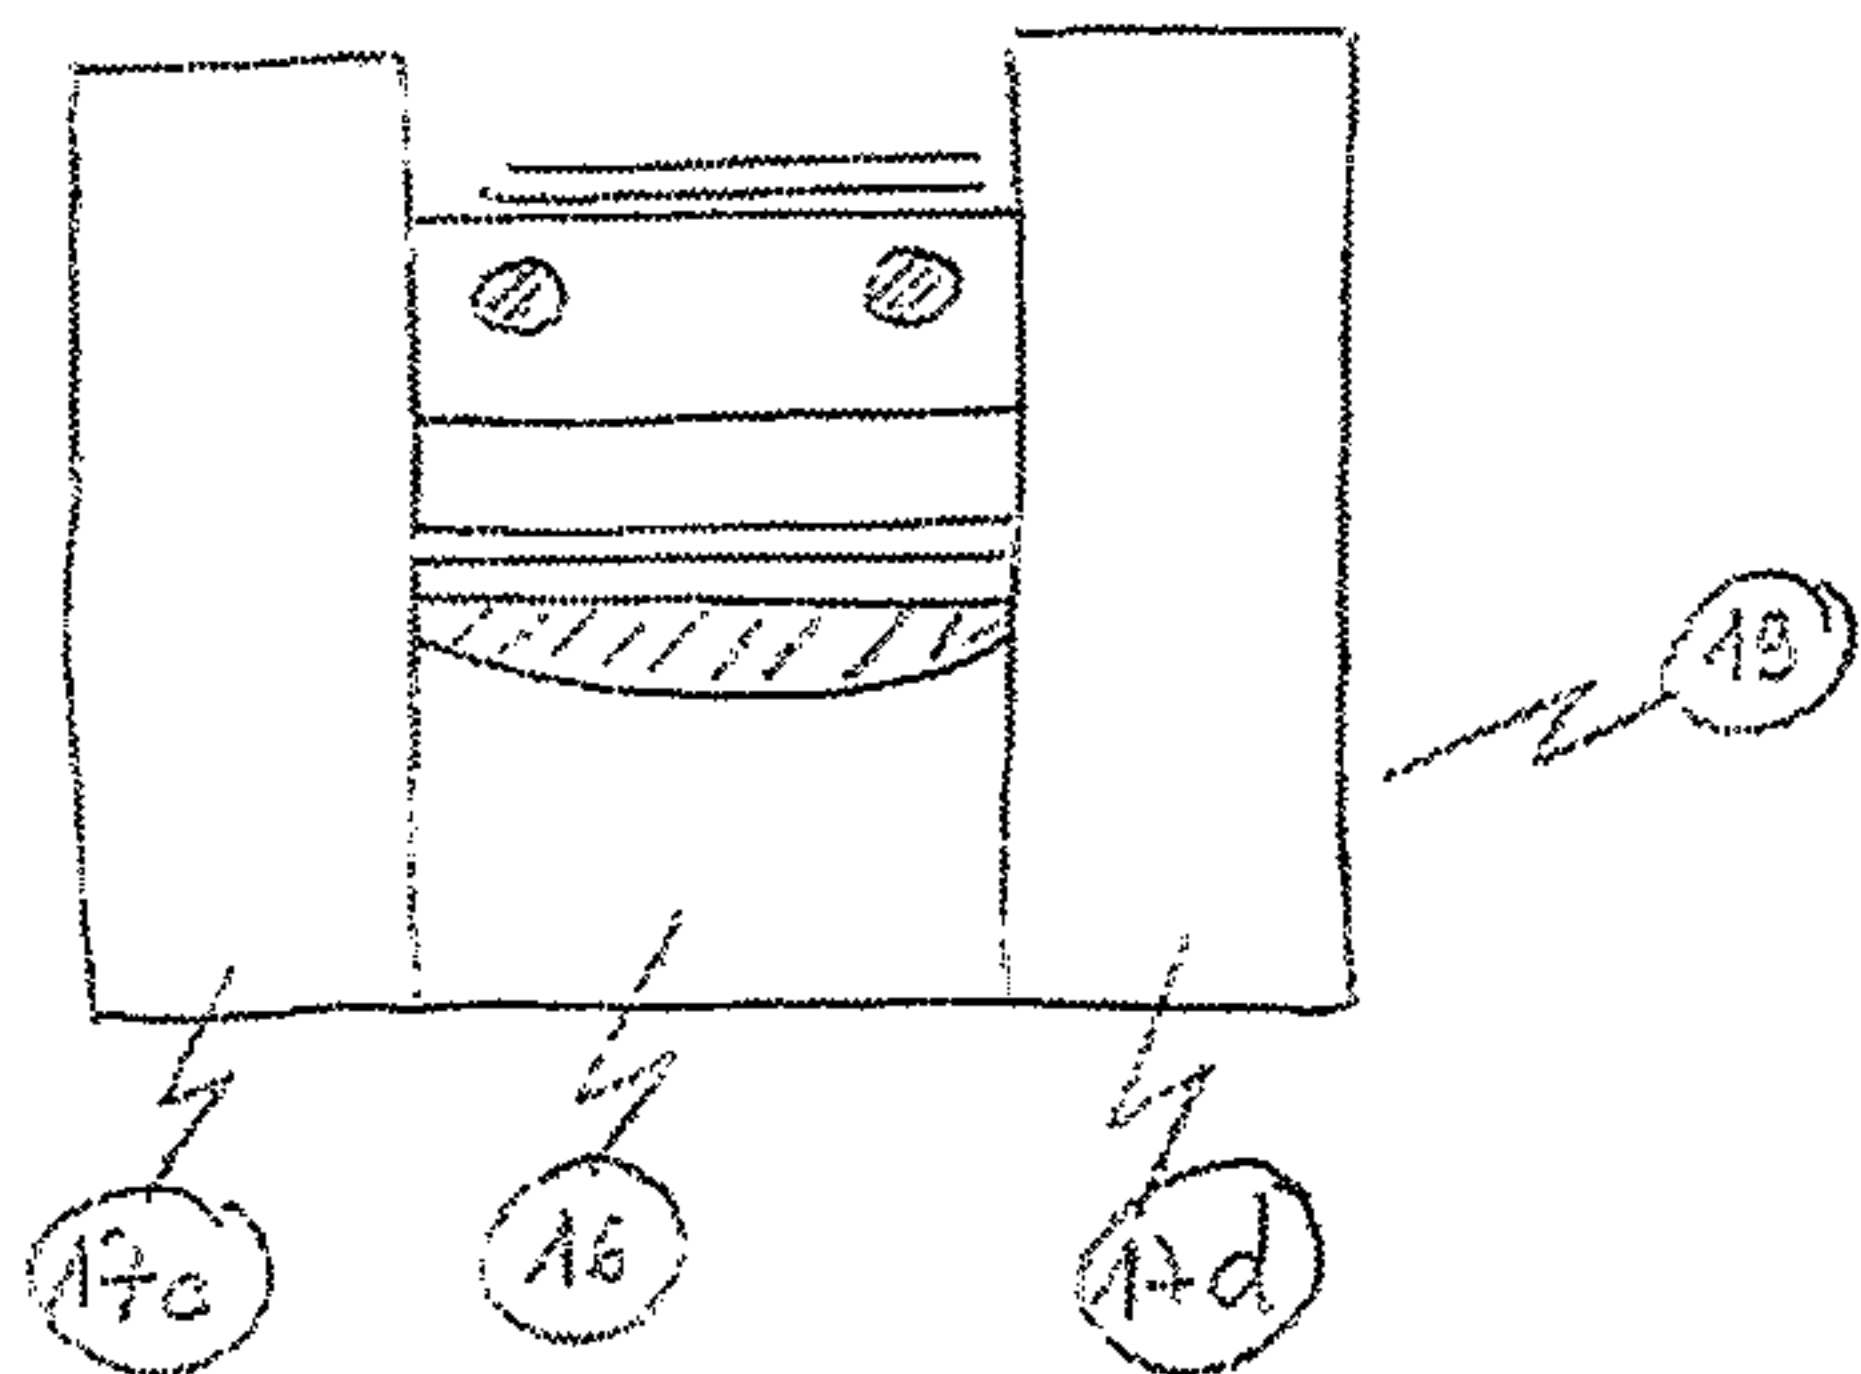


FIGURE 9

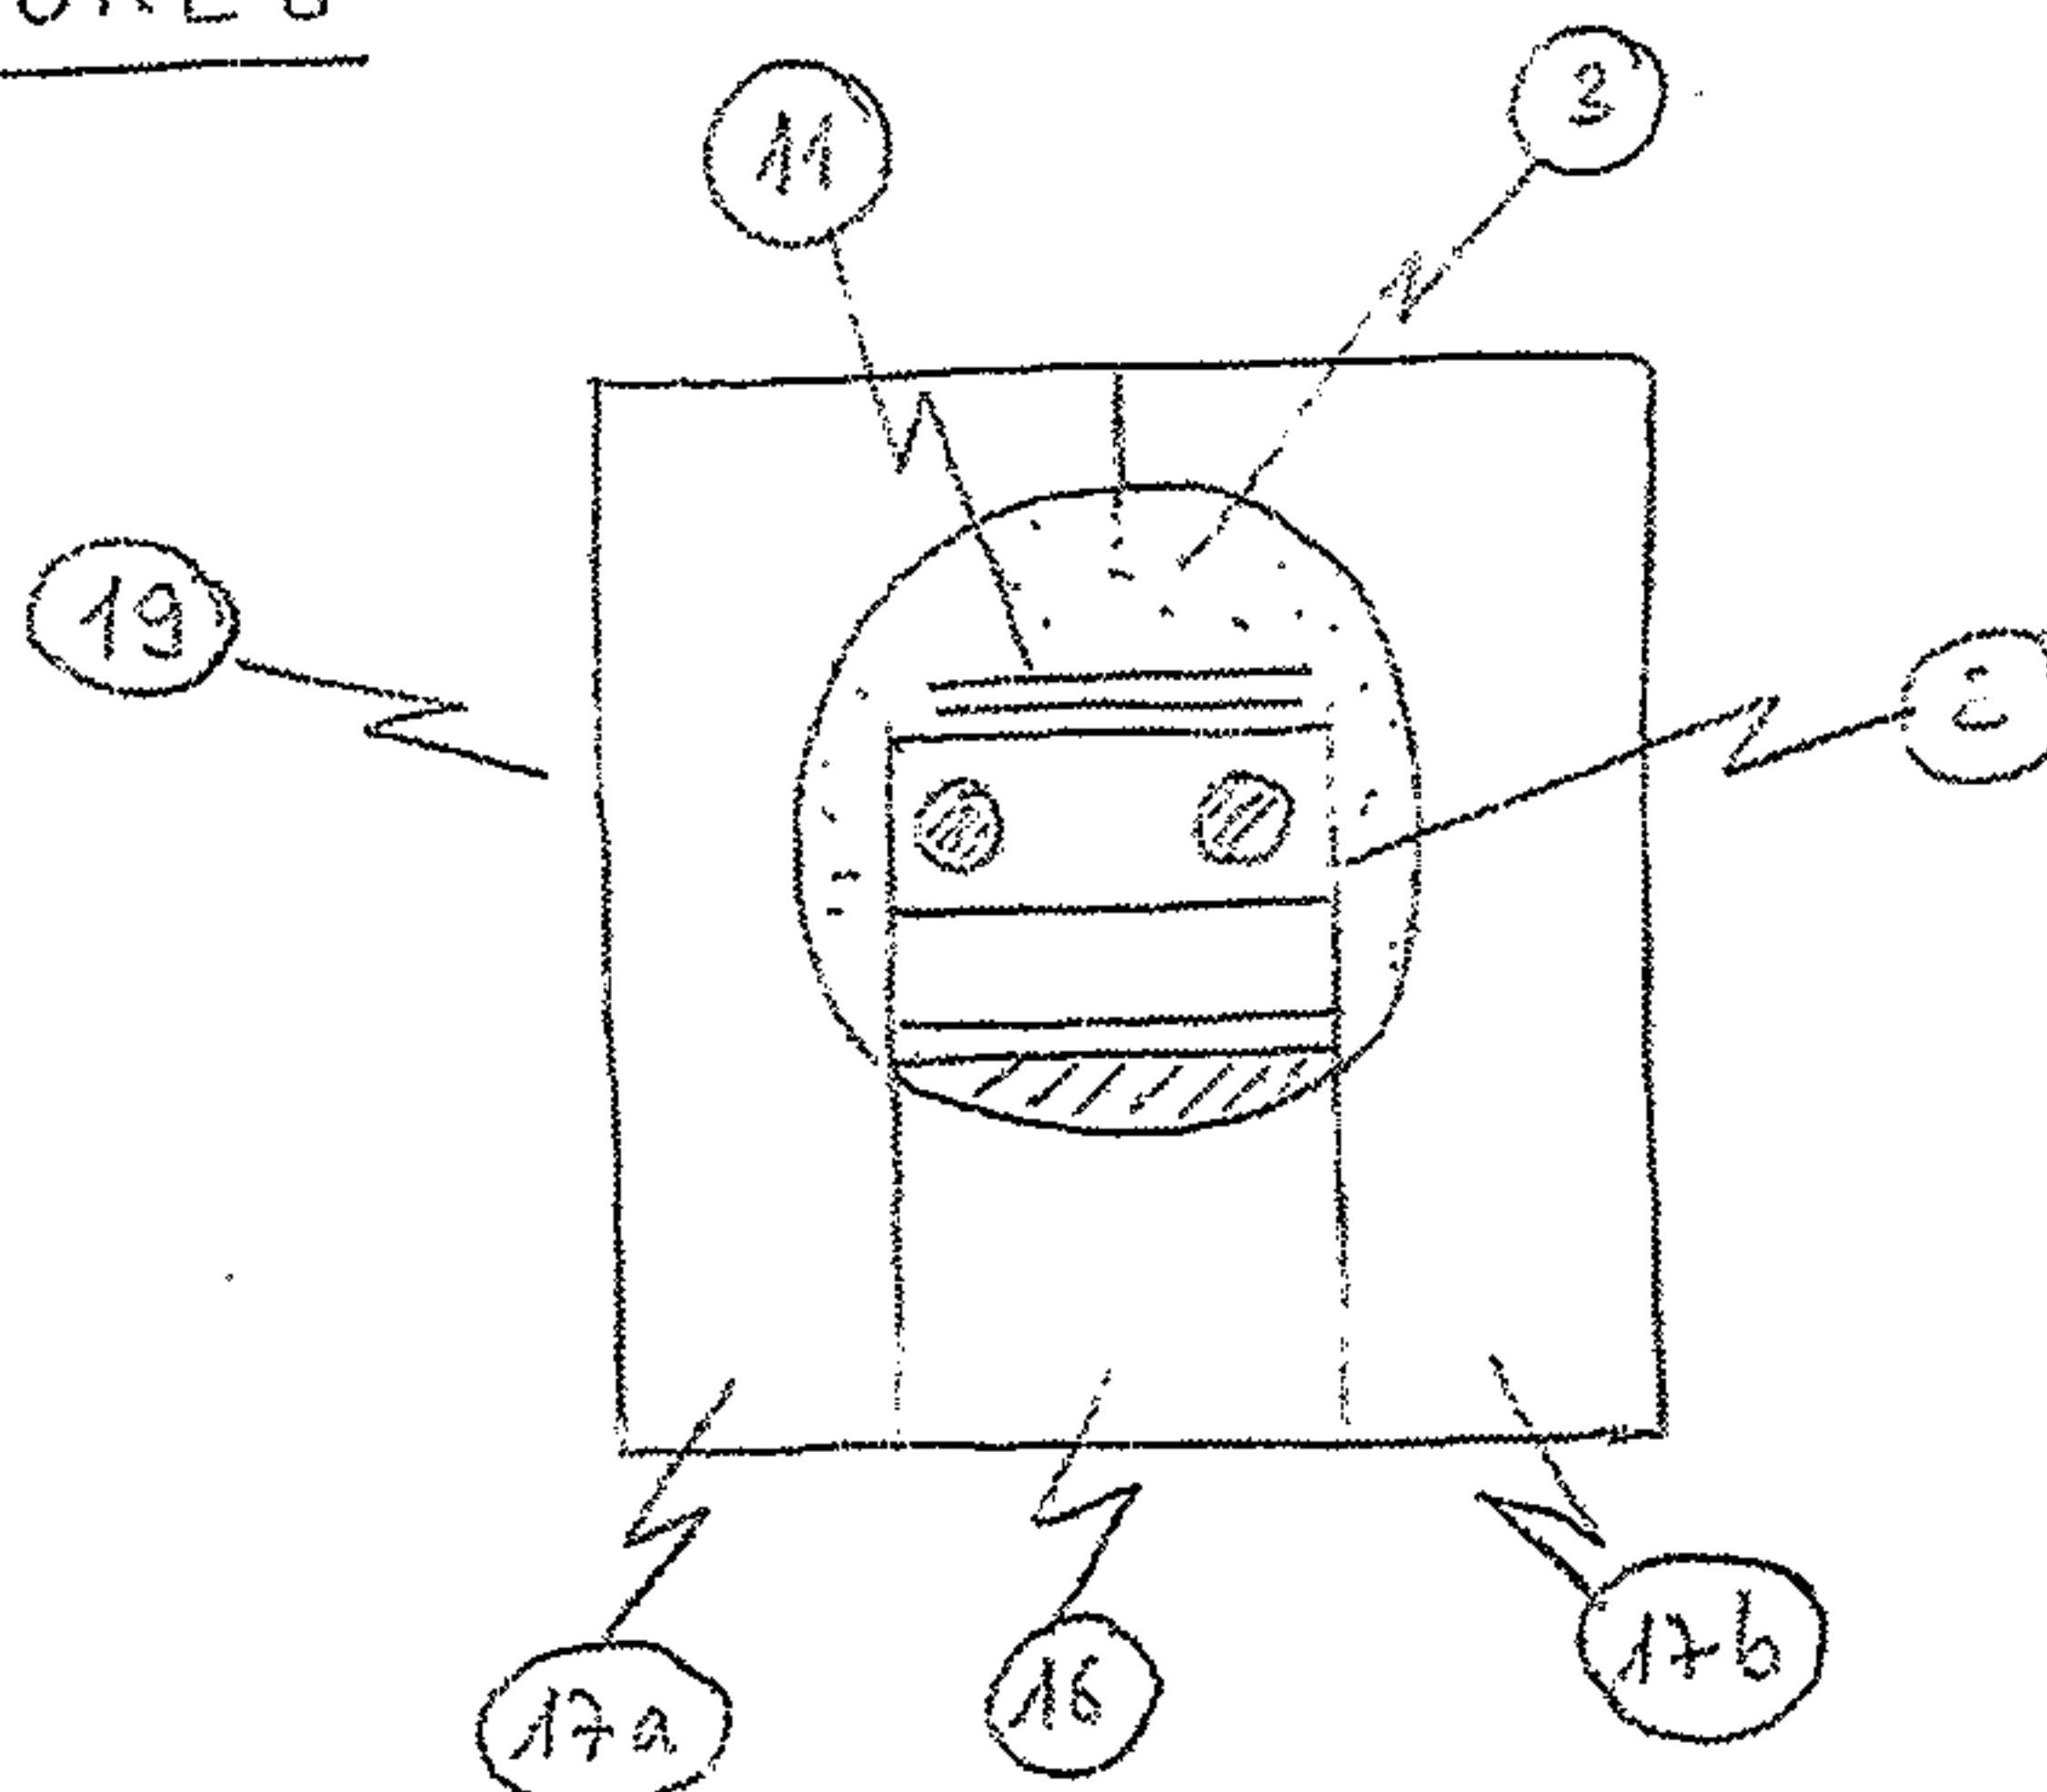


FIGURE 10

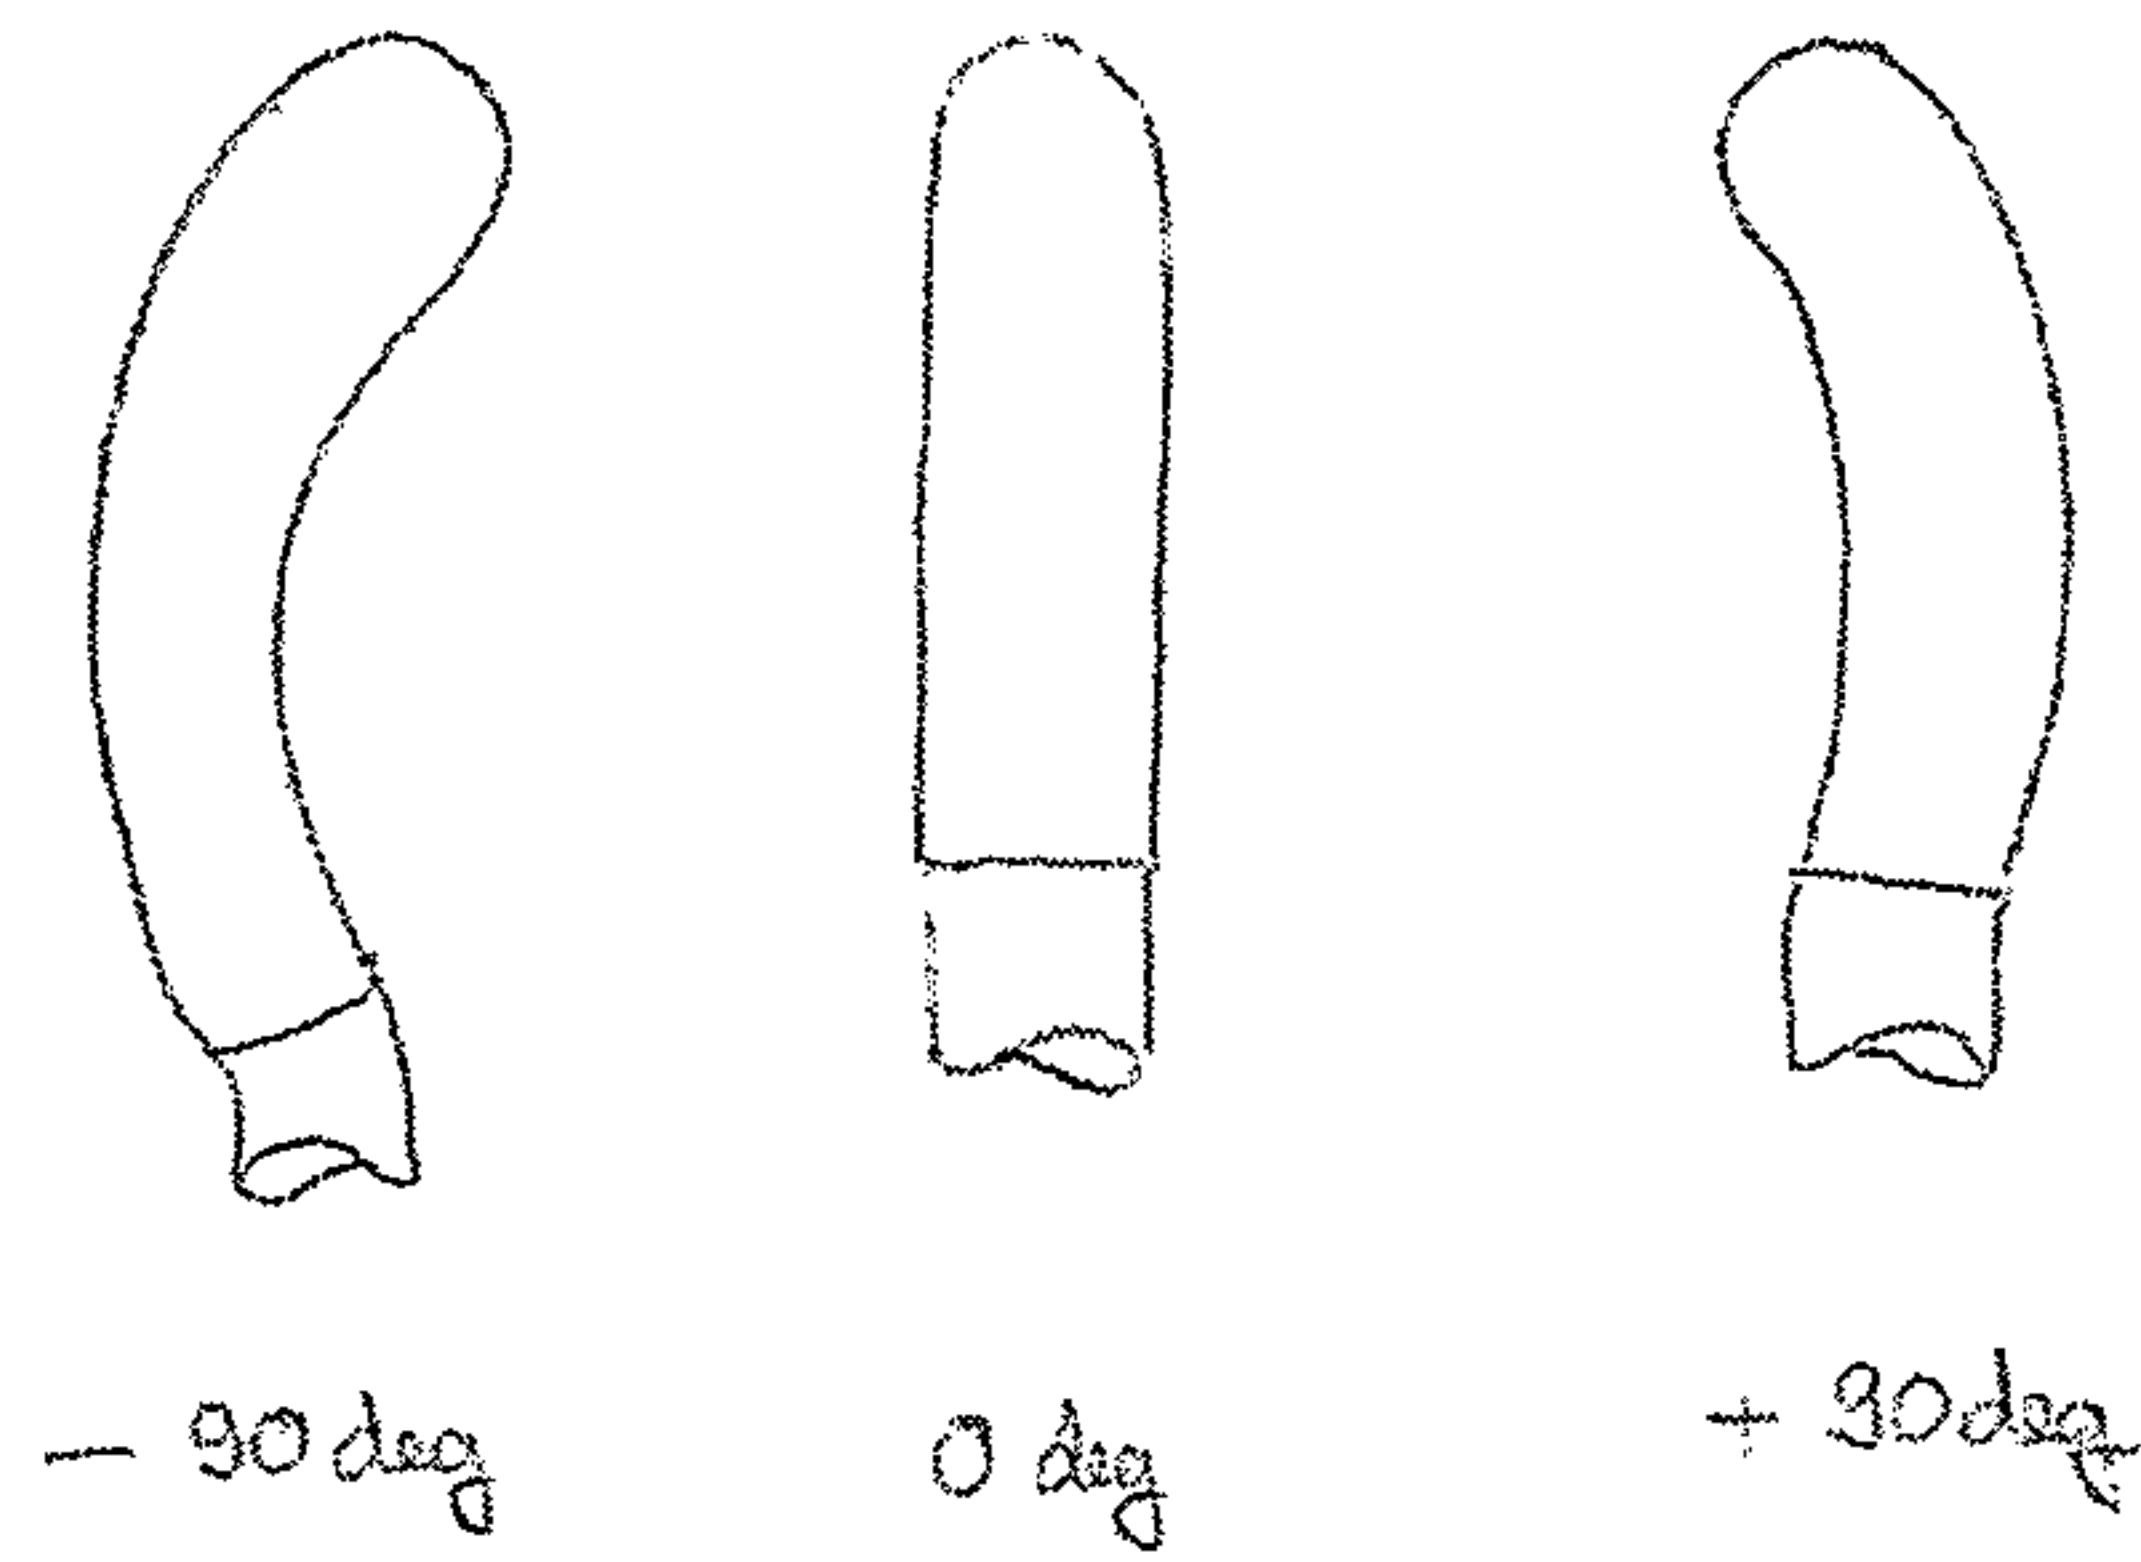


FIGURE 11

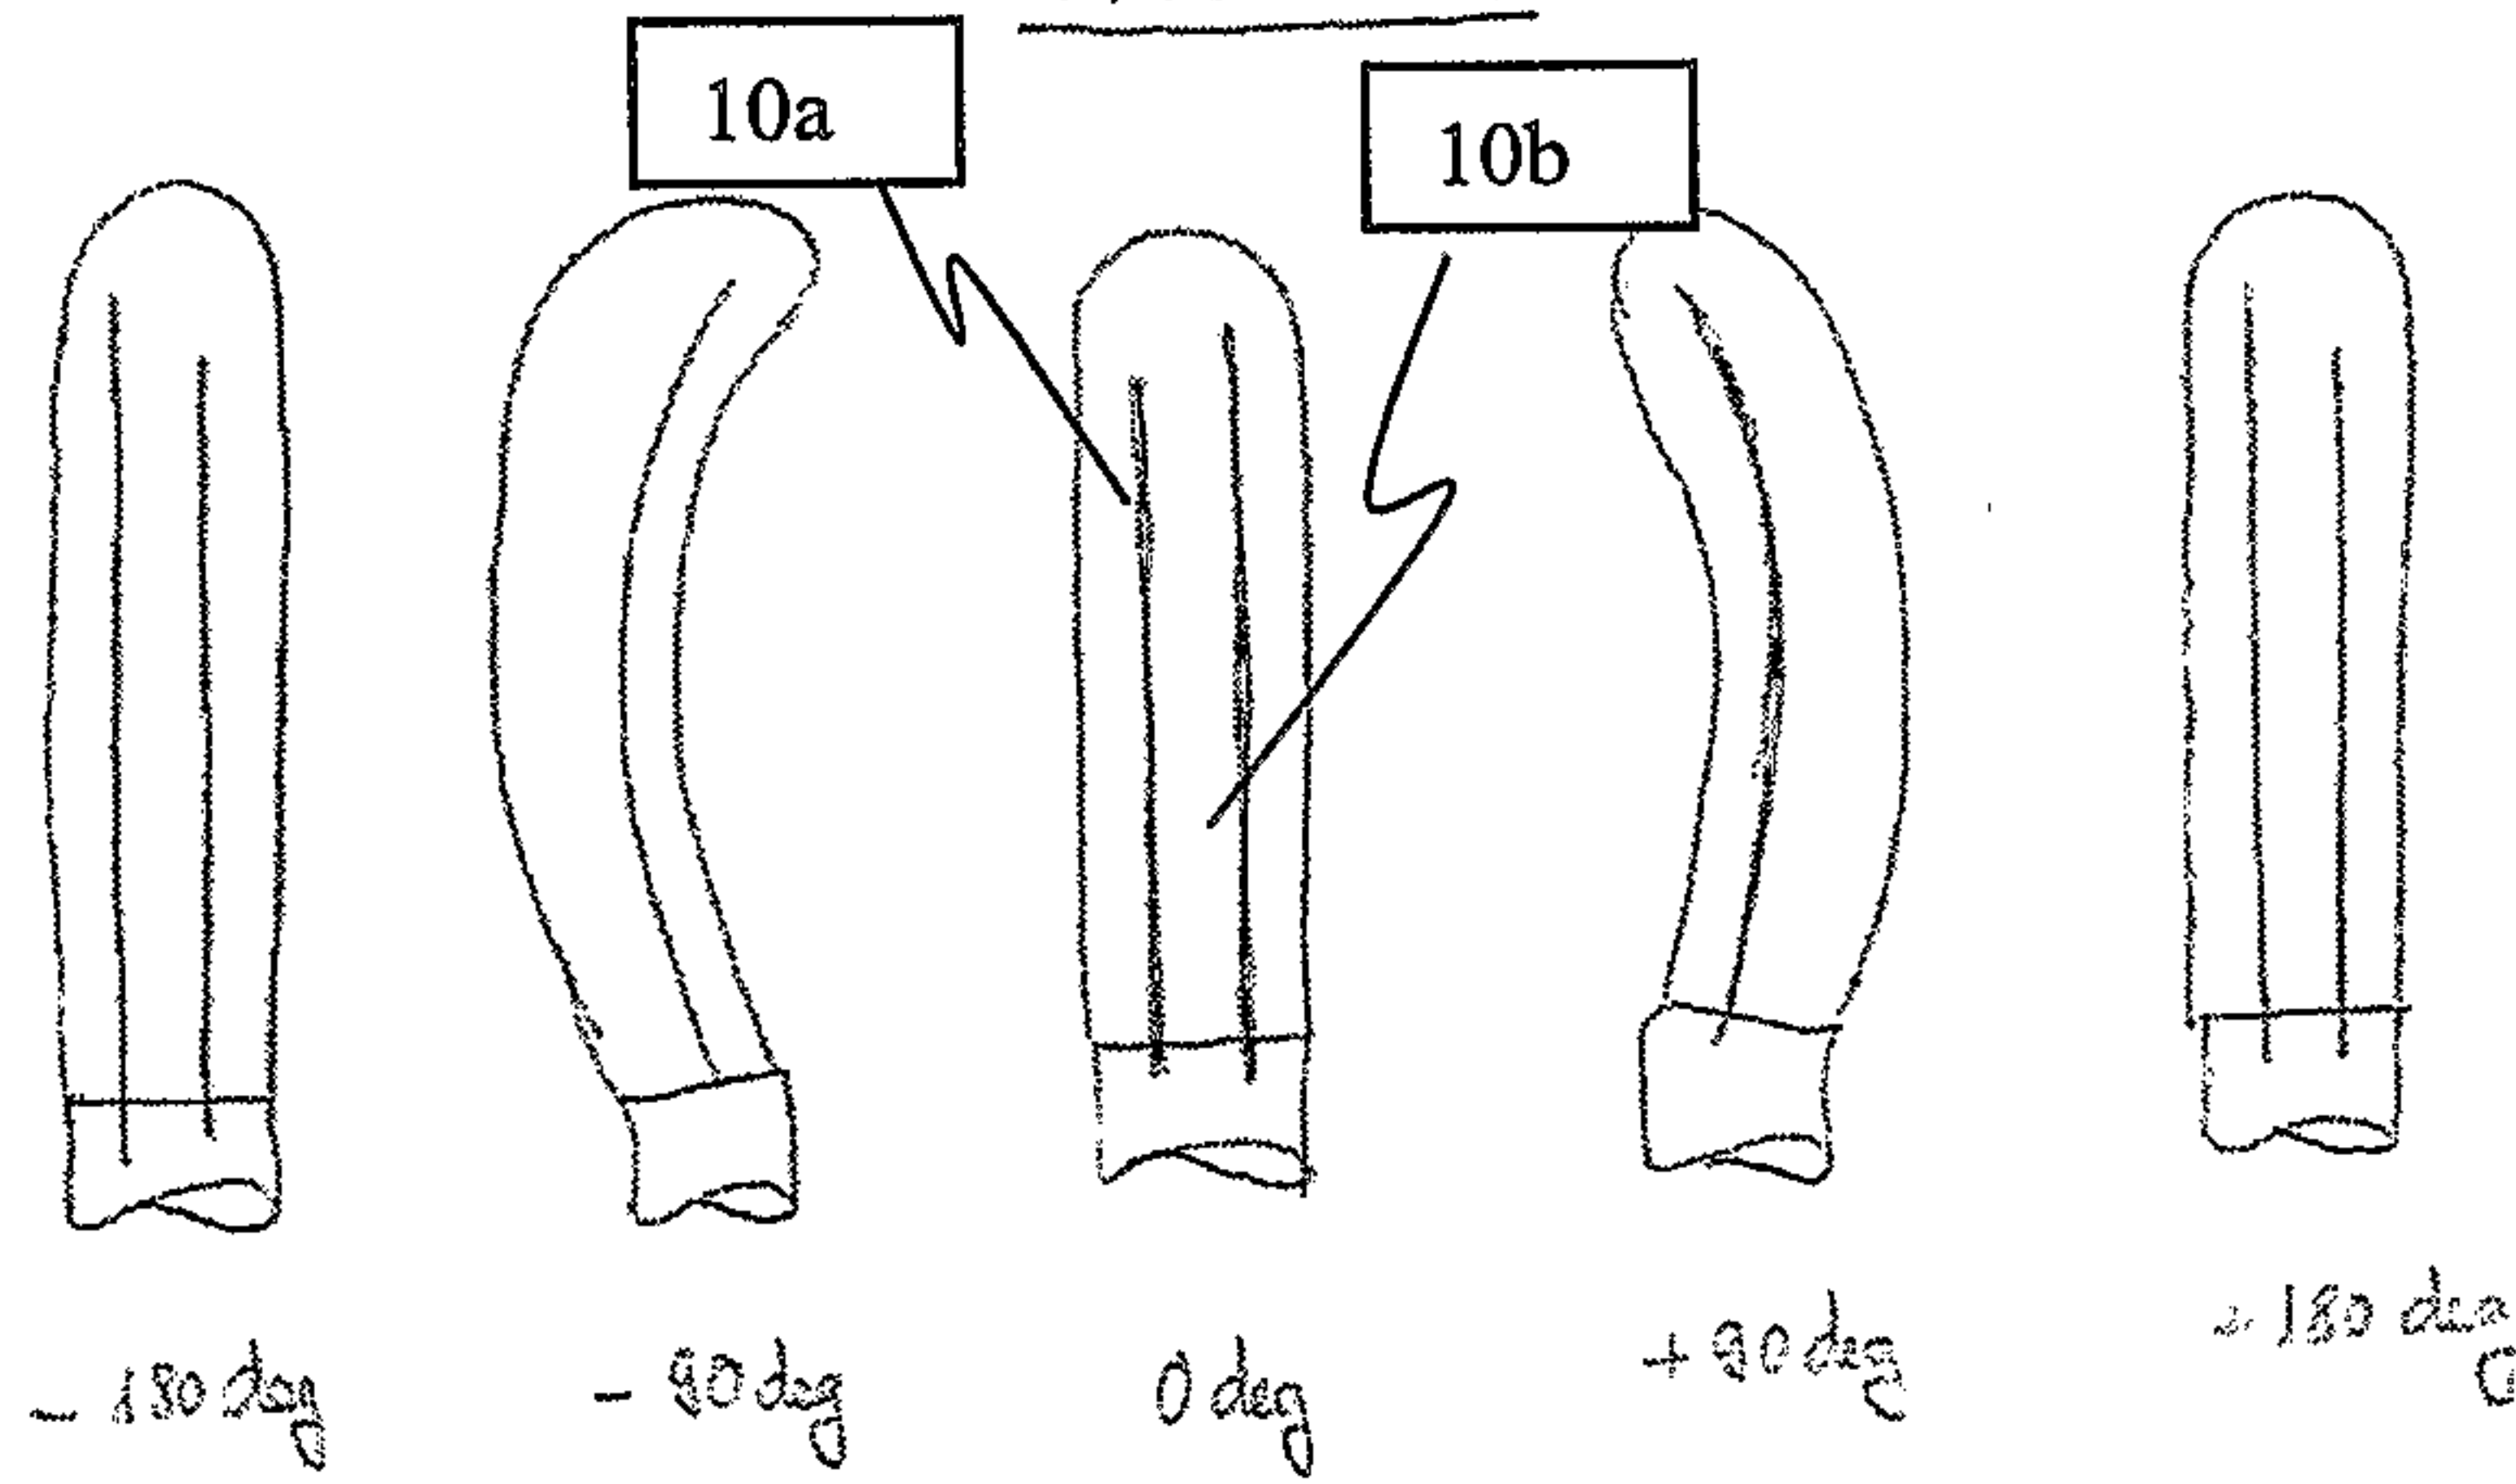


FIGURE 12

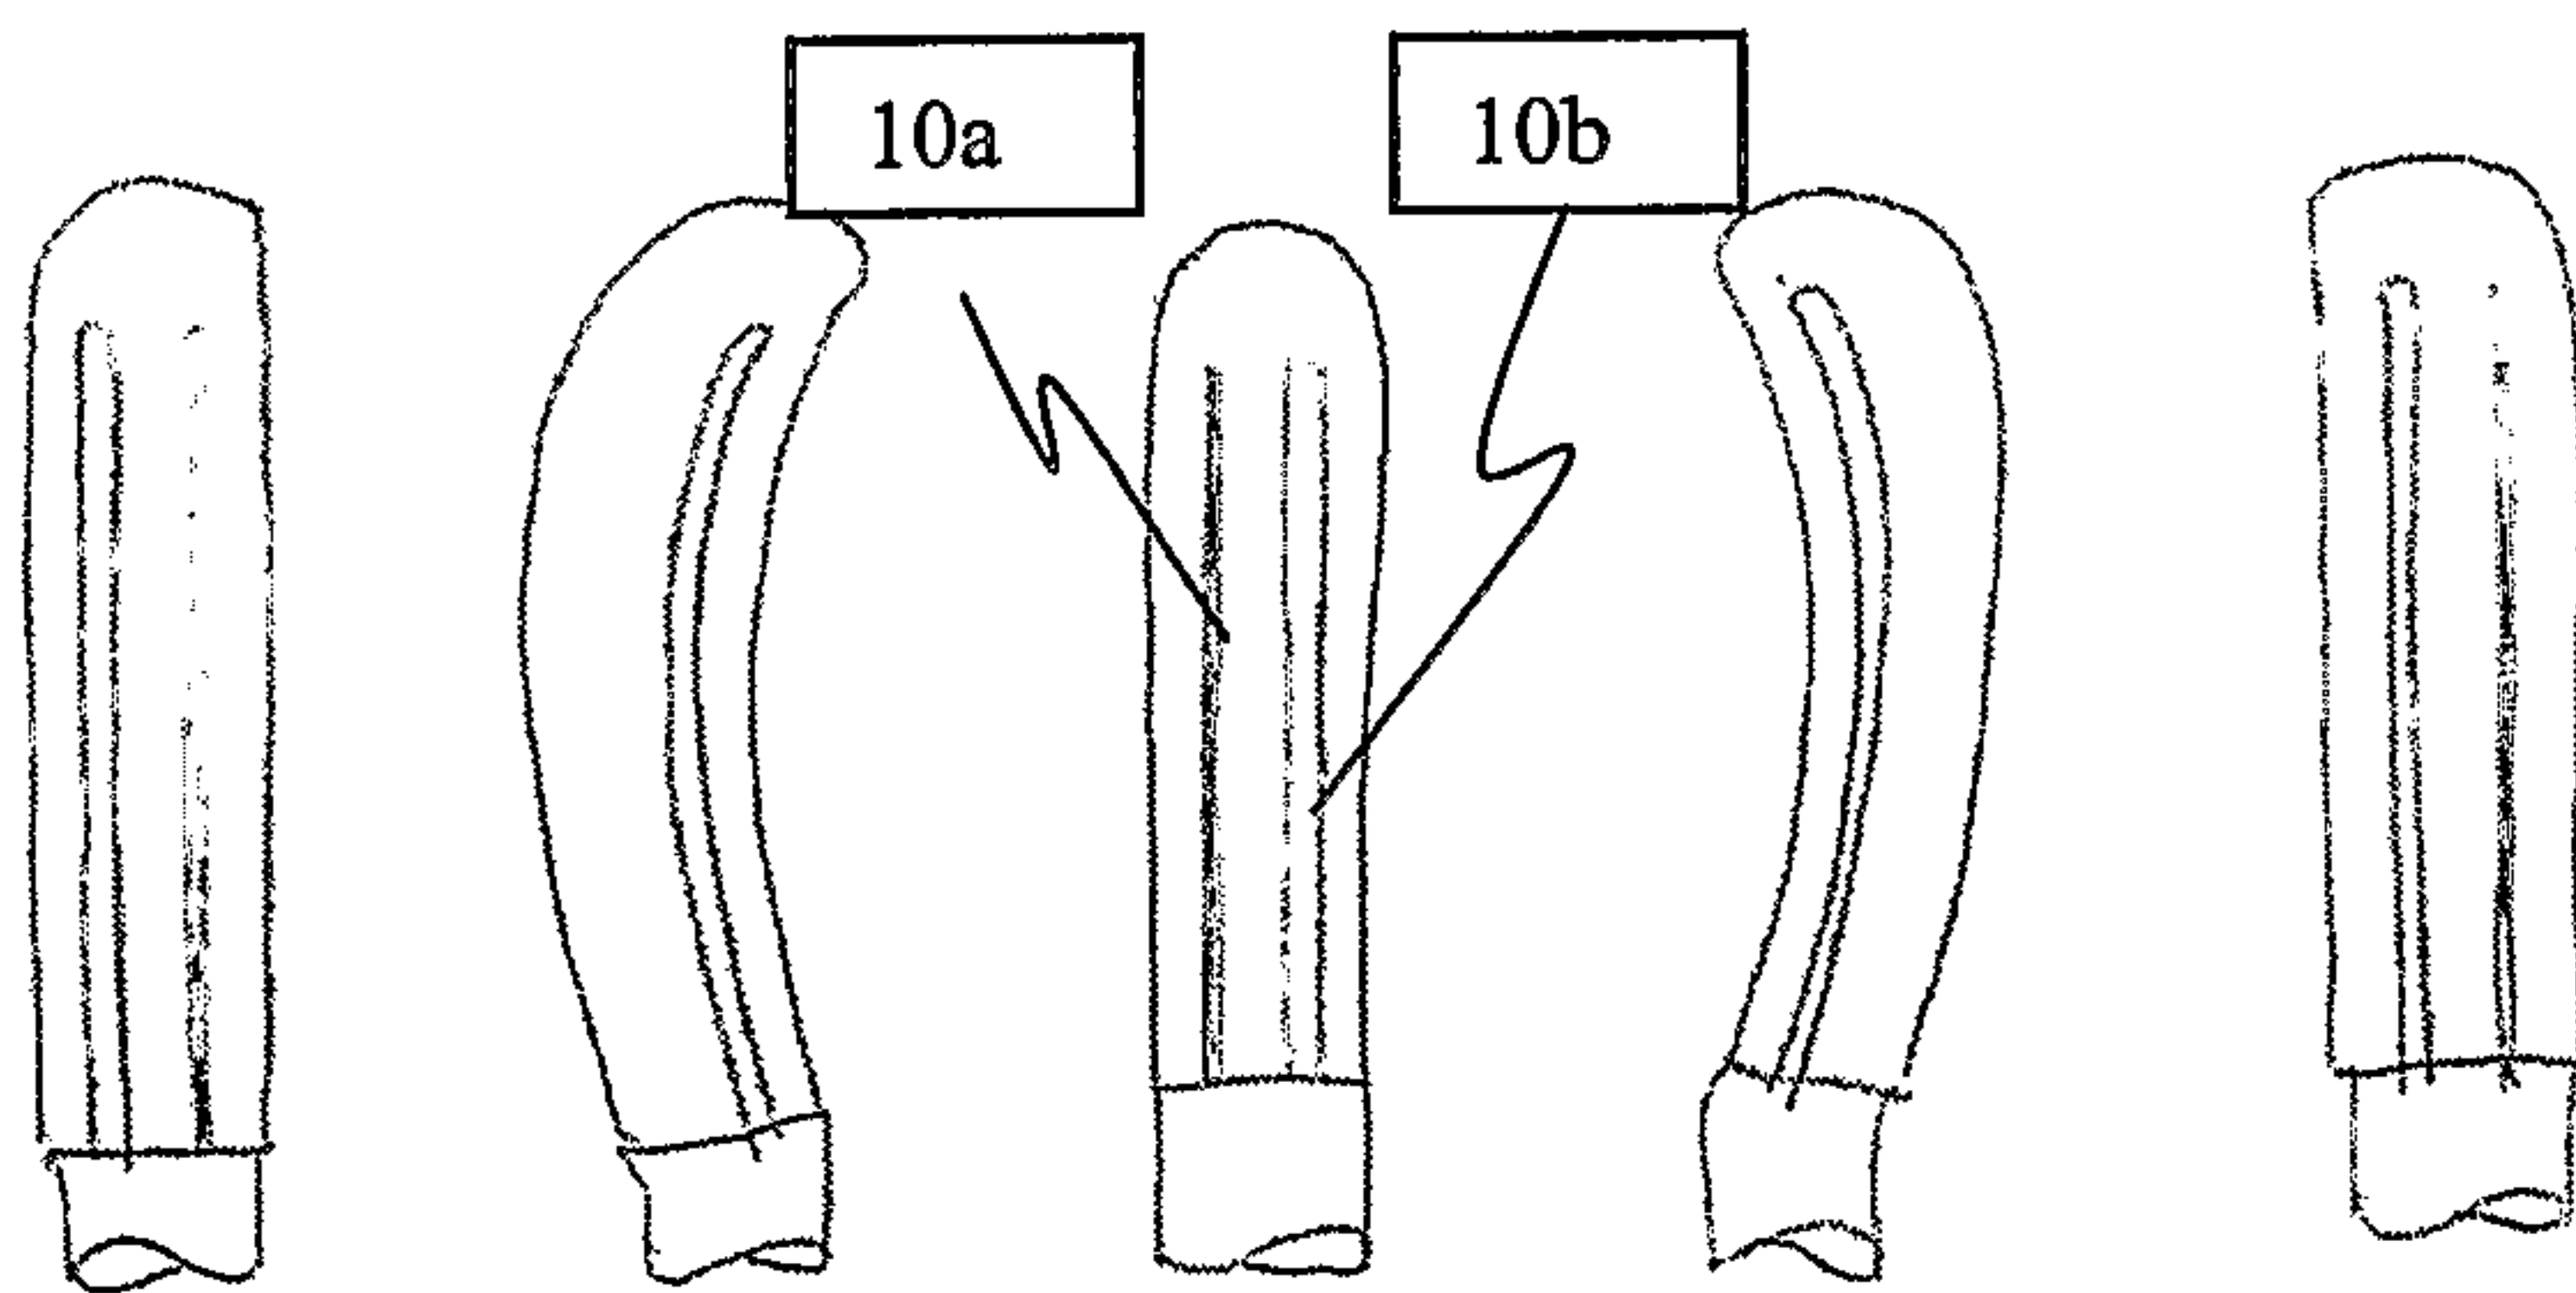
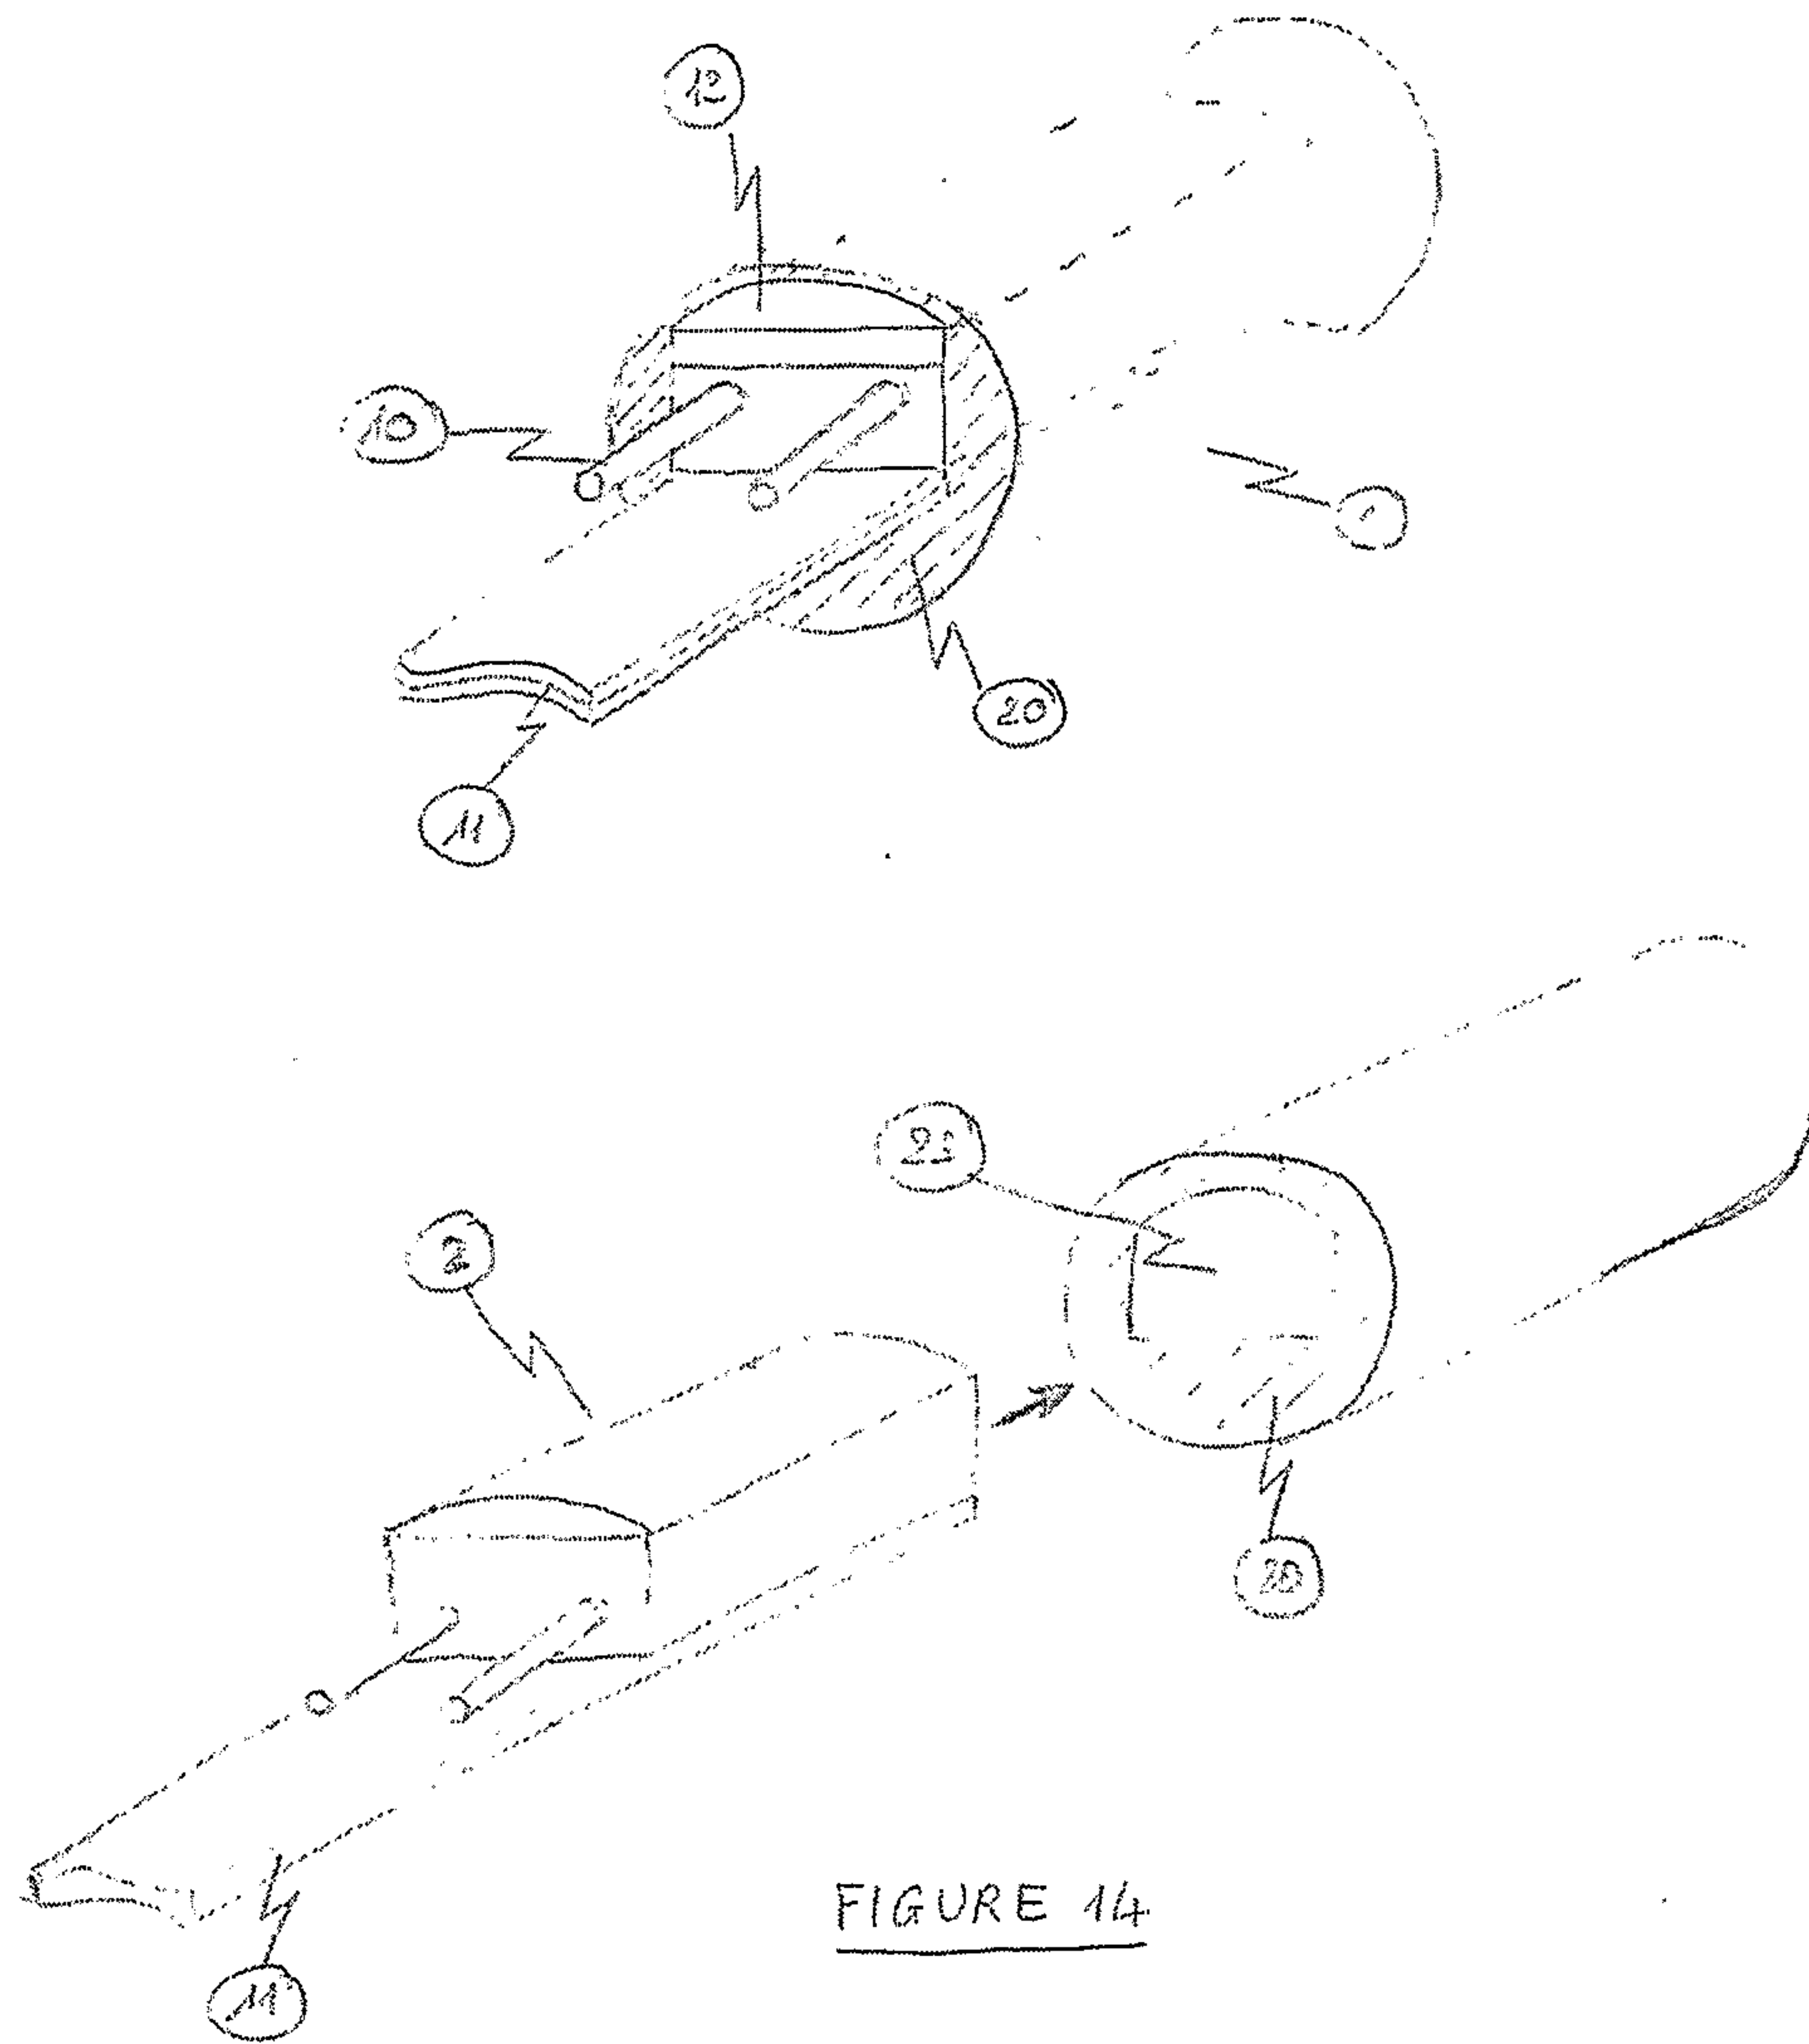


FIGURE 13



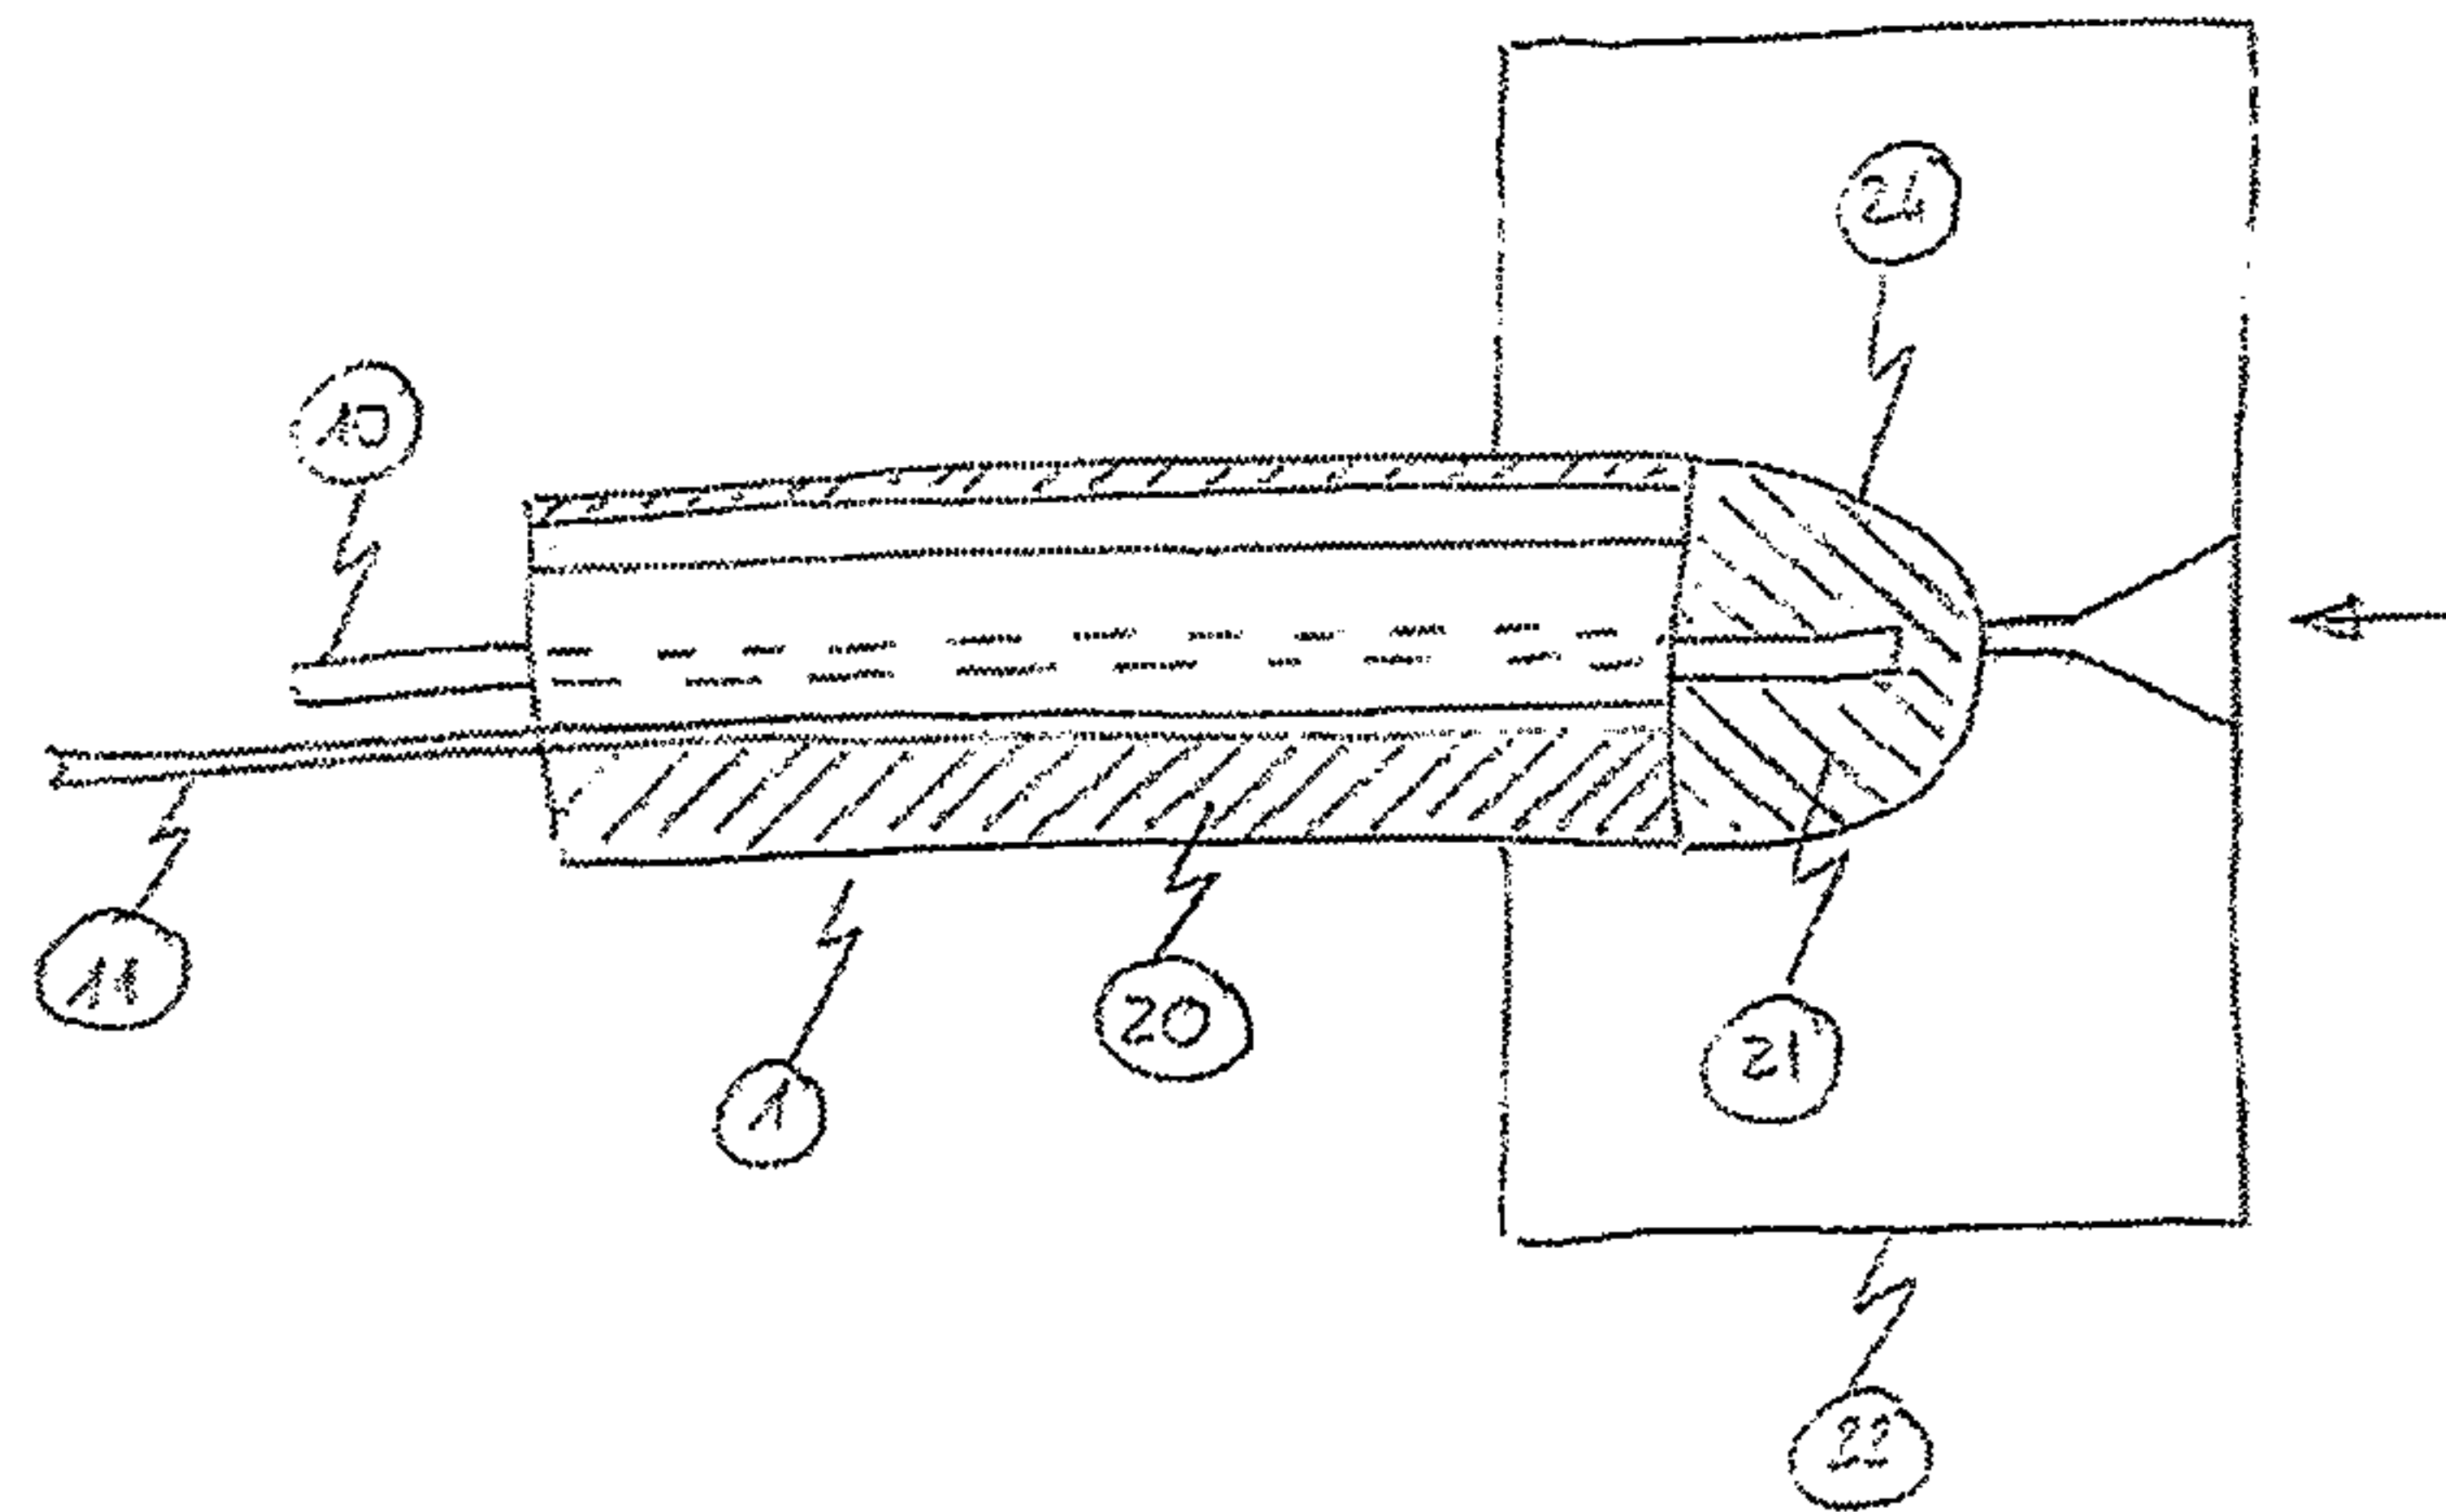


FIGURE 15

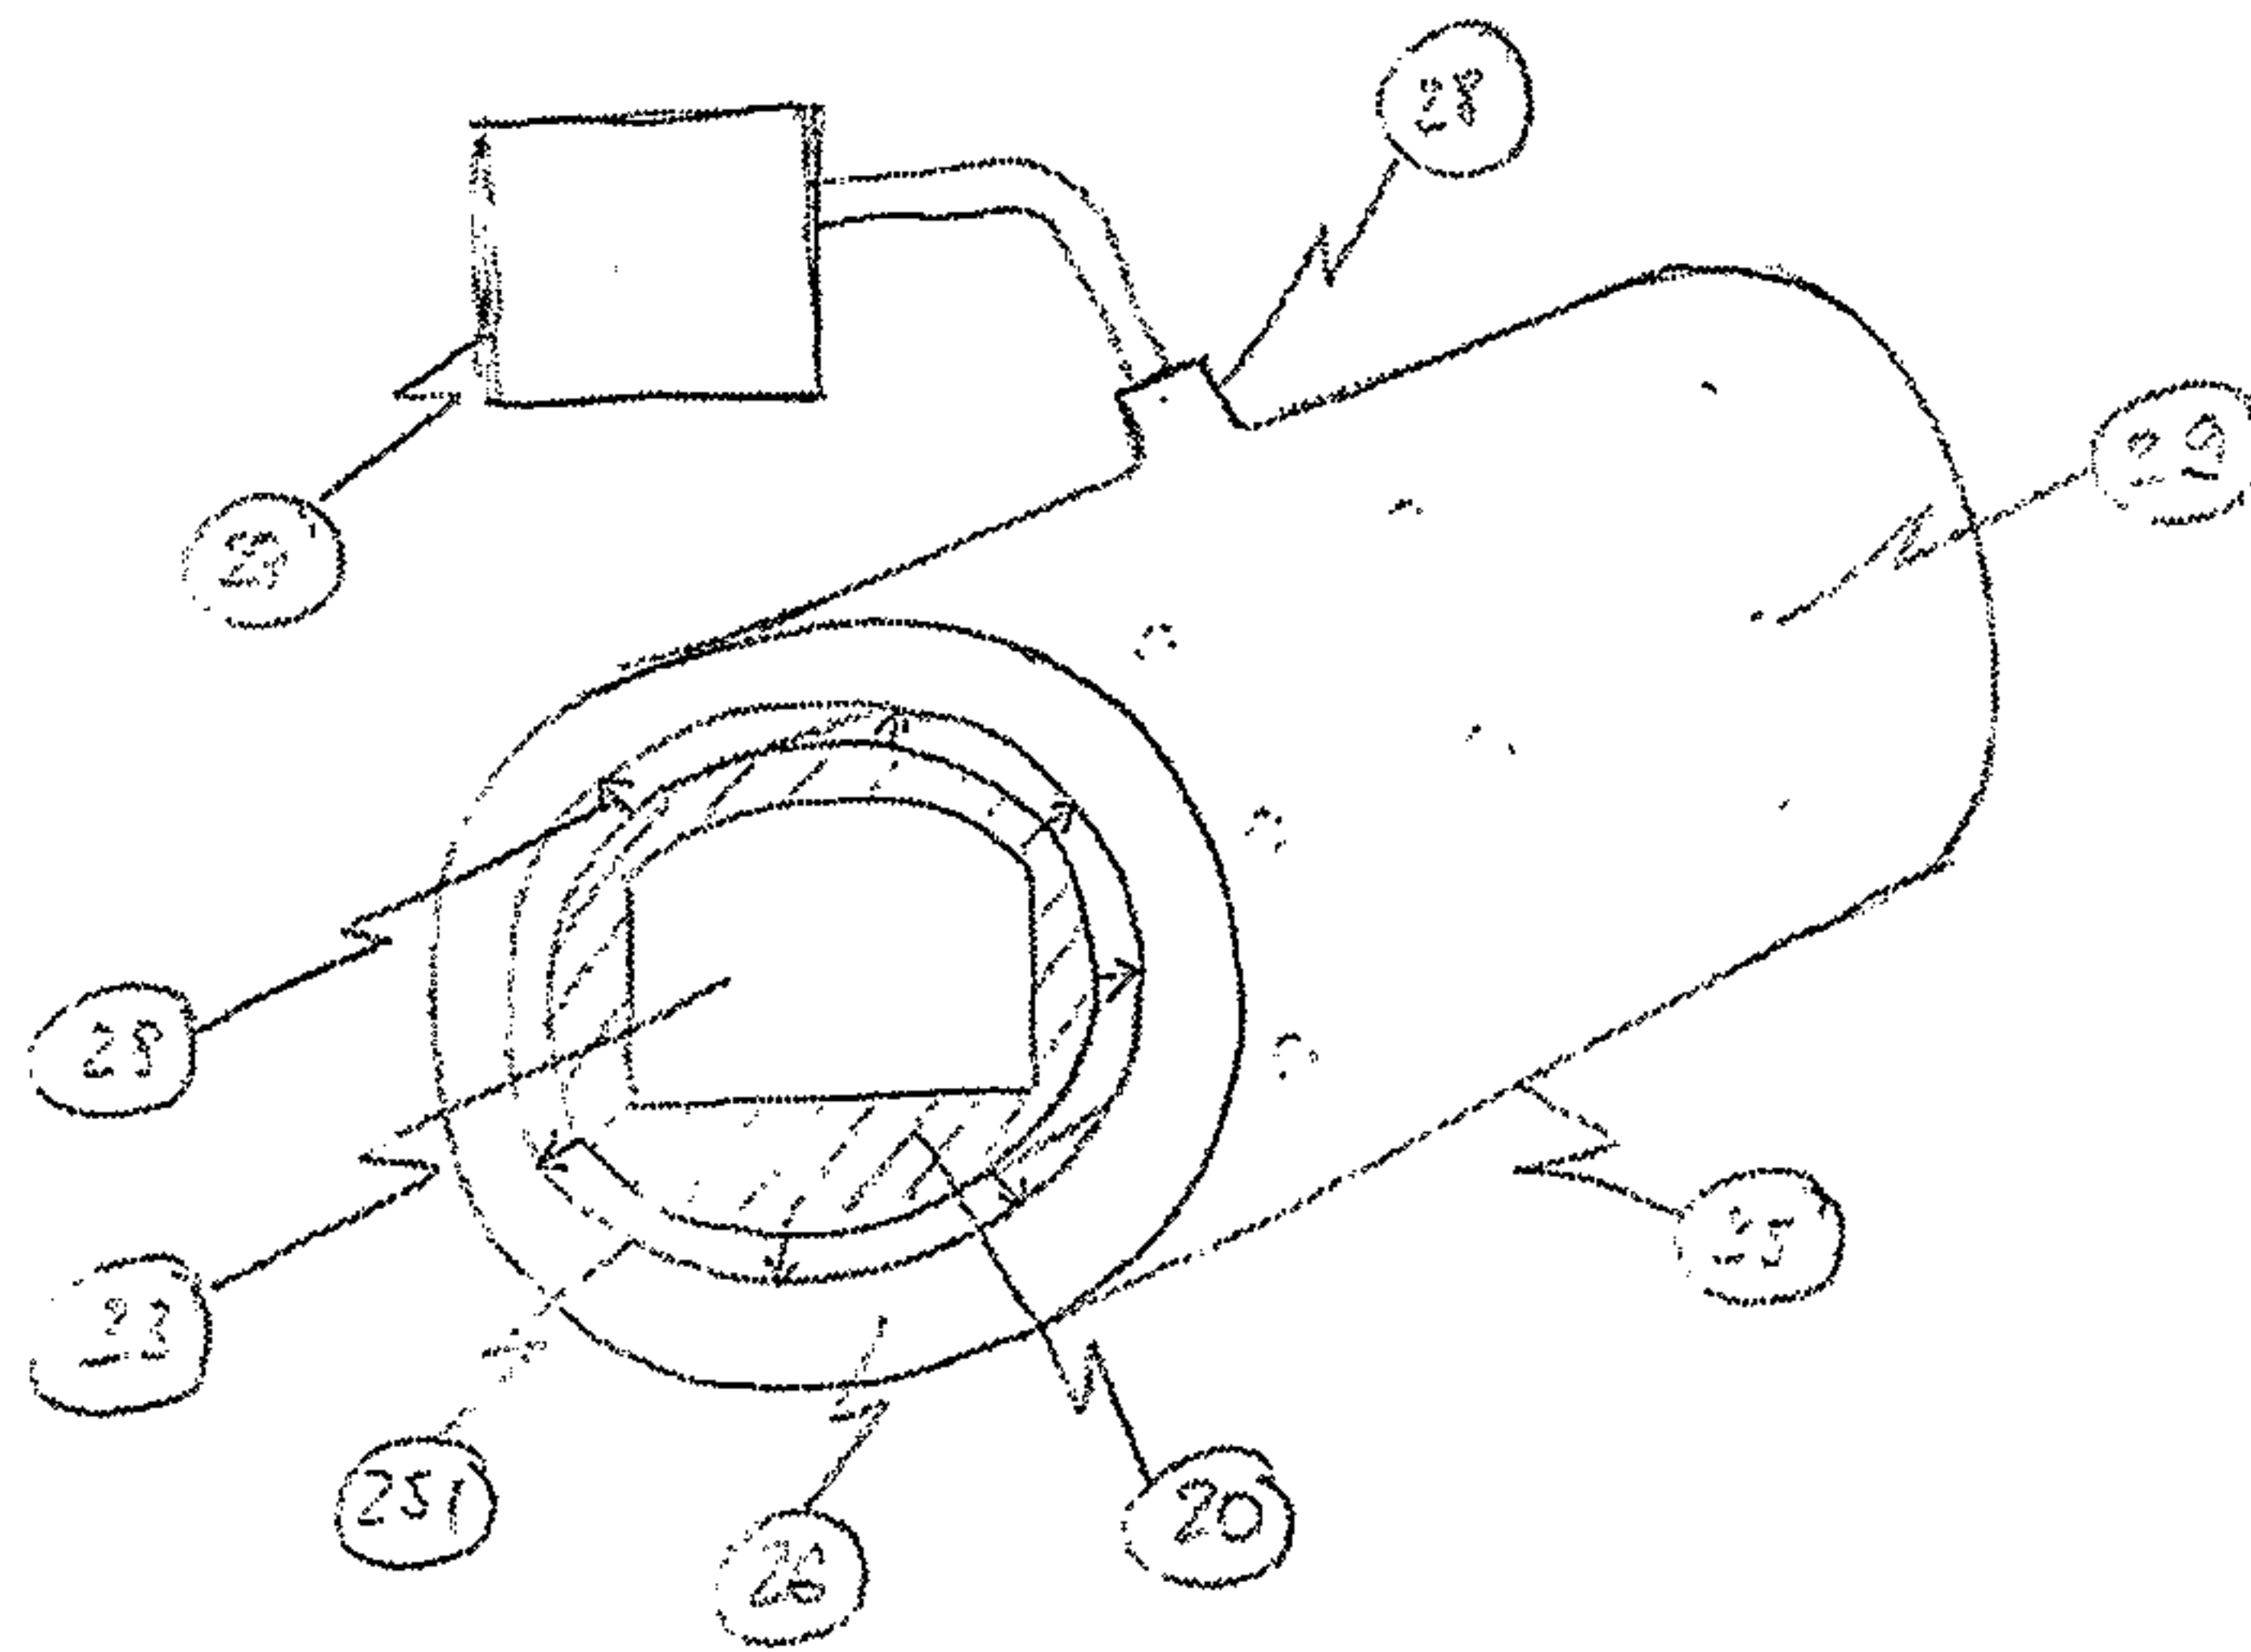


FIGURE 16

