



US0D1042851S

(12) **United States Design Patent** (10) **Patent No.:** **US D1,042,851 S**  
**Farkash et al.** (45) **Date of Patent:** **\*\* Sep. 17, 2024**

(54) **MEDICAL DIAGNOSTIC DEVICE**

FOREIGN PATENT DOCUMENTS

(71) Applicant: **Sanolla Ltd.**, Nesher (IL)  
(72) Inventors: **Asaf Farkash**, Tel Aviv (IL); **Stav Havazelet**, Tel Aviv (IL); **Ran Litvak**, Tel Aviv (IL)

CN 103479385 A 1/2014  
CN 103479386 A 1/2014

(Continued)

(73) Assignee: **SANOLLA LTD.**, Nesher (IL)

(\*\*) Term: **15 Years**

(21) Appl. No.: **29/794,958**

(22) Filed: **Jun. 16, 2021**

(51) **LOC (14) Cl.** ..... **24-02**

(52) **U.S. Cl.**

USPC ..... **D24/186**

(58) **Field of Classification Search**

USPC ..... D24/107, 108, 109, 111, 134, 137, 146,  
D24/158, 164, 165, 166, 167, 168, 169,  
D24/177, 185, 186, 187, 216, 223, 231,  
D24/232

CPC ..... A61B 5/00; A61B 5/0205; A61B 5/091;  
A61B 5/6824; A61B 5/0022; A61B  
5/0006; A61B 5/0008; A61B 5/02108;  
A61B 7/04; A61B 7/00; A61B 7/003;  
A61B 8/00; A61B 8/08; A61B 8/02-06;  
A61B 8/065; A61B 8/52; A61H 2230/04;  
H04R 1/46; B06B 1/00; G01H 3/00;  
G01H 3/12; G01H 9/00; G01N 29/265

See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

872,448 A 12/1907 Penhallow  
3,433,959 A 3/1969 Atwood et al.  
3,580,082 A 5/1971 Strack et al.  
4,792,145 A 12/1988 Eisenberg et al.  
5,031,637 A 7/1991 Parra  
5,301,679 A 4/1994 Taylor  
5,853,005 A 12/1998 Scanlon

(Continued)

OTHER PUBLICATIONS

JMSscience, Electronic Stethoscope, Downloaded on: Sep. 18, 2023, JMSscience.com, Retrieved from Internet: <https://jmscience.com/products/electronic-stethoscopemitorika> (Year: 2023).\*

(Continued)

*Primary Examiner* — John R Yeh

*Assistant Examiner* — Edward P Jones

(74) *Attorney, Agent, or Firm* — MEITAR PATENTS LTD.


(57) **CLAIM**

The ornamental design for a medical diagnostic device, as shown and described.

**DESCRIPTION**

FIG. 1 is a top, front, left-side perspective view of a medical diagnostic device showing our new design; FIG. 2 is bottom, front, left-side perspective view thereof; FIG. 3 a top plan view thereof; FIG. 4 is a left side elevation view thereof, the right side elevation view being identical thereto; FIG. 5 is a bottom plan view thereof; FIG. 6 is a from elevation view thereof; FIG. 7 is a rear elevation view thereof; and, FIG. 8 is a top, front, left-side perspective view thereof showing an alternative configuration of the device. The broken lines in the drawing views are included to illustrate portions of the medical diagnostic device and form no part of the claimed design.

**1 Claim, 7 Drawing Sheets**

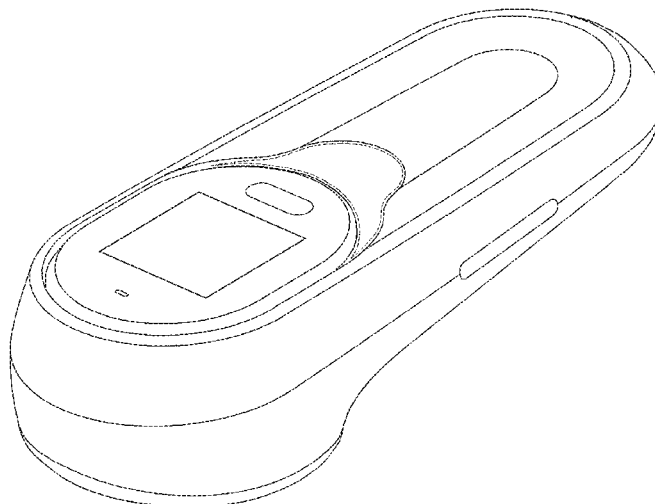

(56)

References Cited

U.S. PATENT DOCUMENTS

6,050,950 A 4/2000 Mohler  
 6,154,551 A 11/2000 Frenkel  
 6,520,924 B2 2/2003 Lee  
 6,699,204 B1 3/2004 Kehyayan et al.  
 6,778,673 B1 8/2004 Hobelsberger  
 6,788,417 B1 9/2004 Zumberge et al.  
 6,887,208 B2 5/2005 Kushnir et al.  
 D526,320 S \* 8/2006 Brandon D14/426  
 7,458,939 B2 12/2008 Munk  
 7,520,861 B2 4/2009 Murphy  
 7,976,480 B2 7/2011 Grajales et al.  
 8,015,878 B2 9/2011 Melikechi et al.  
 D659,840 S \* 5/2012 Cheng D24/186  
 D673,678 S \* 1/2013 Hong D24/146  
 8,419,652 B2 4/2013 Rajamani et al.  
 8,475,396 B2 7/2013 Jones et al.  
 D711,532 S \* 8/2014 Habboushe D24/134  
 8,920,343 B2 12/2014 Sabatino  
 9,101,274 B2 8/2015 Bakema et al.  
 9,138,257 B2 \* 9/2015 Revivo A46B 13/008  
 9,208,287 B2 12/2015 Waterson et al.  
 9,277,330 B2 3/2016 Aharoni et al.  
 9,345,432 B2 5/2016 Salisbury et al.  
 D767,770 S \* 9/2016 Purfey D24/186  
 9,445,779 B2 9/2016 Shams et al.  
 D794,201 S \* 8/2017 Newhouse D24/169  
 9,867,591 B2 1/2018 Shams et al.  
 10,092,269 B2 10/2018 Shams et al.  
 10,141,007 B1 11/2018 Kim et al.  
 D865,167 S 10/2019 Kirgizov  
 D880,710 S \* 4/2020 Amoyal D24/209  
 10,709,353 B1 7/2020 McLane  
 10,842,416 B2 11/2020 Joseph et al.  
 10,881,330 B2 1/2021 Joseph et al.  
 11,000,257 B2 5/2021 Adler et al.  
 D950,748 S \* 5/2022 Gong D24/214  
 D1,000,624 S \* 10/2023 Nichols D24/209  
 2001/0030077 A1 10/2001 Watson  
 2002/0071570 A1 6/2002 Cohen et al.  
 2002/0183642 A1 12/2002 Murphy  
 2003/0002685 A1 1/2003 Werblud  
 2004/0260193 A1 12/2004 LaSala  
 2005/0222515 A1 10/2005 Polyshchuk et al.  
 2005/0273015 A1 12/2005 Bauer et al.  
 2006/0070623 A1 4/2006 Wilkinson et al.  
 2007/0050715 A1 3/2007 Behar  
 2007/0058818 A1 3/2007 Yoshimine  
 2008/0013747 A1 1/2008 Tran  
 2009/0171231 A1 7/2009 Caro et al.  
 2009/0232322 A1 9/2009 Tseng  
 2009/0316925 A1 12/2009 Eisenfeld et al.  
 2010/0298740 A1 6/2010 Gelman et al.  
 2011/0137209 A1 6/2011 Lahiji et al.  
 2011/0222697 A1 9/2011 Dong et al.  
 2011/0224988 A1 9/2011 Mahajan et al.  
 2012/0143018 A1 6/2012 Skidmore et al.  
 2012/0209131 A1 8/2012 Jones et al.  
 2013/0041278 A1 2/2013 Bai et al.  
 2013/0060100 A1 3/2013 Wurm et al.  
 2014/0073864 A1 3/2014 Engelbrecht et al.  
 2014/0155762 A1 6/2014 Maskara et al.  
 2014/0290372 A1 10/2014 Lagaros et al.  
 2014/0327775 A1 11/2014 Cho  
 2015/0073306 A1 3/2015 Abeyratne et al.  
 2015/0119758 A1 4/2015 Rogers et al.  
 2015/0327775 A1 11/2015 Carter  
 2016/0007923 A1 1/2016 Yamamoto  
 2016/0050506 A1 2/2016 Kim  
 2016/0306940 A1 10/2016 Farhoud  
 2017/0079612 A1 3/2017 Park  
 2017/0156632 A1 6/2017 Swiston et al.  
 2017/0273580 A1 \* 9/2017 Lee A61B 5/332  
 2018/0115839 A1 4/2018 Eichfeld et al.  
 2018/0228468 A1 8/2018 Adler et al.  
 2019/0076129 A1 3/2019 Ward, III et al.

2019/0099156 A1 4/2019 Bocca et al.  
 2019/0125270 A1 5/2019 Deriso  
 2019/0298183 A1 10/2019 Burg et al.  
 2020/0060641 A1 2/2020 Shekhar et al.  
 2020/0253480 A1 8/2020 Hall et al.  
 2020/0368090 A1 11/2020 Waterson et al.  
 2021/0145398 A1 5/2021 Adler et al.  
 2021/0345939 A1 11/2021 Jumbe et al.  
 2022/0202310 A1 6/2022 Adler  
 2023/0142937 A1 \* 5/2023 Jha A61B 5/0022  
 600/586

FOREIGN PATENT DOCUMENTS

CN 203506748 U 4/2014  
 CN 107510473 A 12/2017  
 CN 306290265 \* 1/2021  
 CN 307317496 \* 5/2022  
 DE 202005006661 U1 8/2005  
 JP D1561413 \* 10/2016  
 JP D1717812 \* 6/2022  
 KR 20120040530 A 4/2012  
 WO 9325874 A1 12/1993  
 WO 0002486 A1 1/2000  
 WO 2002009586 A2 2/2002  
 WO 2006075263 A1 7/2006  
 WO 2011117862 A2 9/2011  
 WO 2014163443 A1 10/2014  
 WO 2015157458 A1 10/2015  
 WO 2016113562 A1 7/2016  
 WO 2017141165 A1 8/2017  
 WO 2019048960 A1 3/2019  
 WO 2019048961 A1 3/2019  
 WO 2022118105 A1 6/2022  
 WO 2022118106 A1 6/2022  
 WO 2022144614 A1 7/2022

OTHER PUBLICATIONS

Dr. Bertalan Mesko, PhD, Playback Heart Sounds: The eKuore Pro Digital Stethoscope Review, Published on: May 14, 2019, medicalfuturist.com, Retrieved from Internet: <https://medicalfuturist.com/ekuore-digital-stethoscopereview/> (Year: 2019).\*

PyXy.ai, PyXy + AI = new health surveillance system, Downloaded on: Sep. 18, 2023, Rudolf Riestter GmbH, Retrieved from Internet: <https://pyxy.ai/technology> (Year: 2023).\*

Cision PR Newswire, "Bat-Call's Revolutionary AI Based Infra-Sound Auscultation Technology to Fight Covid-19", pp. 1-4, Apr. 1, 2020, as downloaded from <https://www.prnewswire.com/news-releases/bat-calls-revolutionary-ai-based-infra-sound-auscultation-technology-to-fight-covid-19-301033267.html>.

International Application # PCT/IB2021/058755 Search Report dated Jan. 5, 2022.

International Application # PCT/IB2021/059711 Search Report dated Feb. 3, 2022.

International Application # PCT/IB2021/059710 Search Report dated Feb. 10, 2022.

U.S. Appl. No. 16/636,649 Office Action dated Feb. 17, 2023.

EP Application # 18855091.7 Office Action dated Mar. 15, 2023.

U.S. Appl. No. 17/138,986 Office Action dated Mar. 21, 2023.

Padmanabhan et al., "Accelerometer type cardiac transducer for detection of low-level heart sounds", IEEE Transactions on Bio-medical Engineering, vol. 40, No. 1, pp. 21-28, Jan. 1, 1993.

Bukhman et al., "Spectral analysis of acoustic vibrations on the surface of the human body," Acoustical Physics, vol. 41, Issue 1, pp. 1-10, year 1995.

Adler, U.S. Appl. No. 17/138,986, filed Dec. 31, 2020.

Bachner-Hinzenon et al., U.S. Appl. No. 63/119,677, filed Dec. 1, 2020.

Bat-Call, "CompuSteth", pp. 1-3, Mar. 23, 2019 downloaded from <https://bat-call.com/products/compuSteth/>.

Amazon, "Thinklabs One Digital Stethoscope", pp. 1-9, Jan. 6, 2019 downloaded from [www.amazon.com/Thinklabs-One-Digital-Stethoscope/dp/B07BRQRNW7](http://www.amazon.com/Thinklabs-One-Digital-Stethoscope/dp/B07BRQRNW7).

(56)

**References Cited**

OTHER PUBLICATIONS

EP Application # 18855091.7 Search Report dated Apr. 22, 2021.  
EP Application # 18853978.7 Search Report dated Apr. 22, 2021.  
Huang et al., "The Respiratory Sound Features of COVID-19 Patients Fill Gaps Between Clinical Data and Screening Methods," medRxiv, Preprint, pp. 1-12, Apr. 10, 2020, as downloaded from <https://www.medrxiv.org/content/10.1101/2020.04.07.20051060v1>.  
U.S. Appl. No. 17/138,986 Office Action dated Sep. 15, 2022.  
U.S. Appl. No. 16/636,649 Office Action dated Aug. 10, 2023.

\* cited by examiner

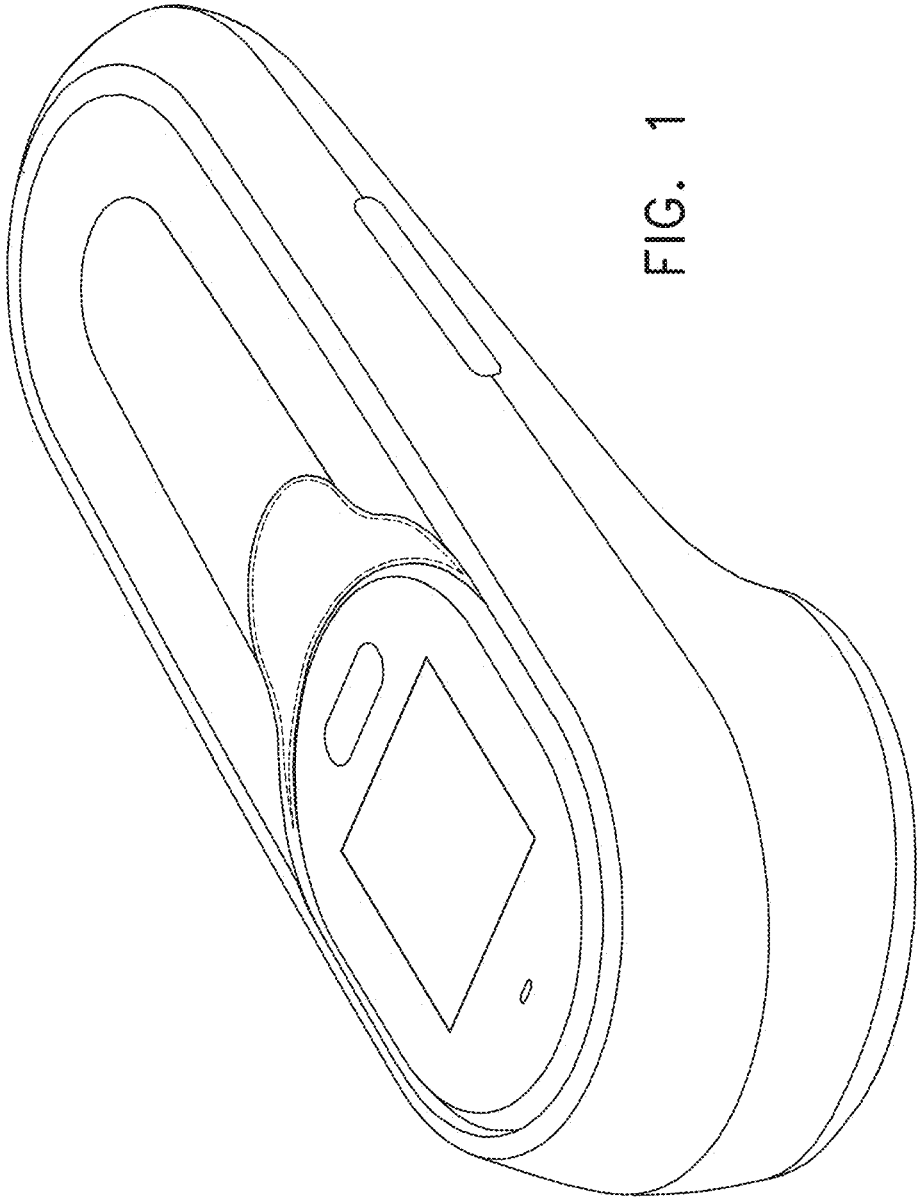


FIG. 1

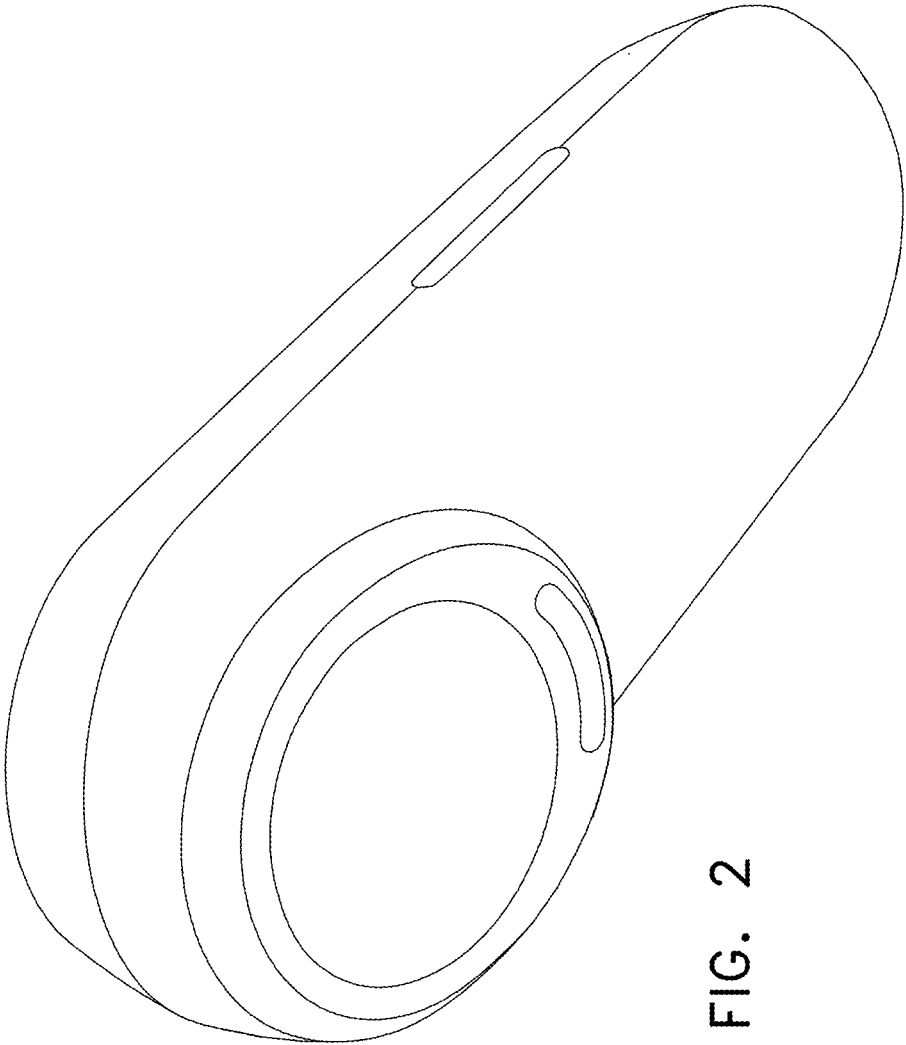


FIG. 2

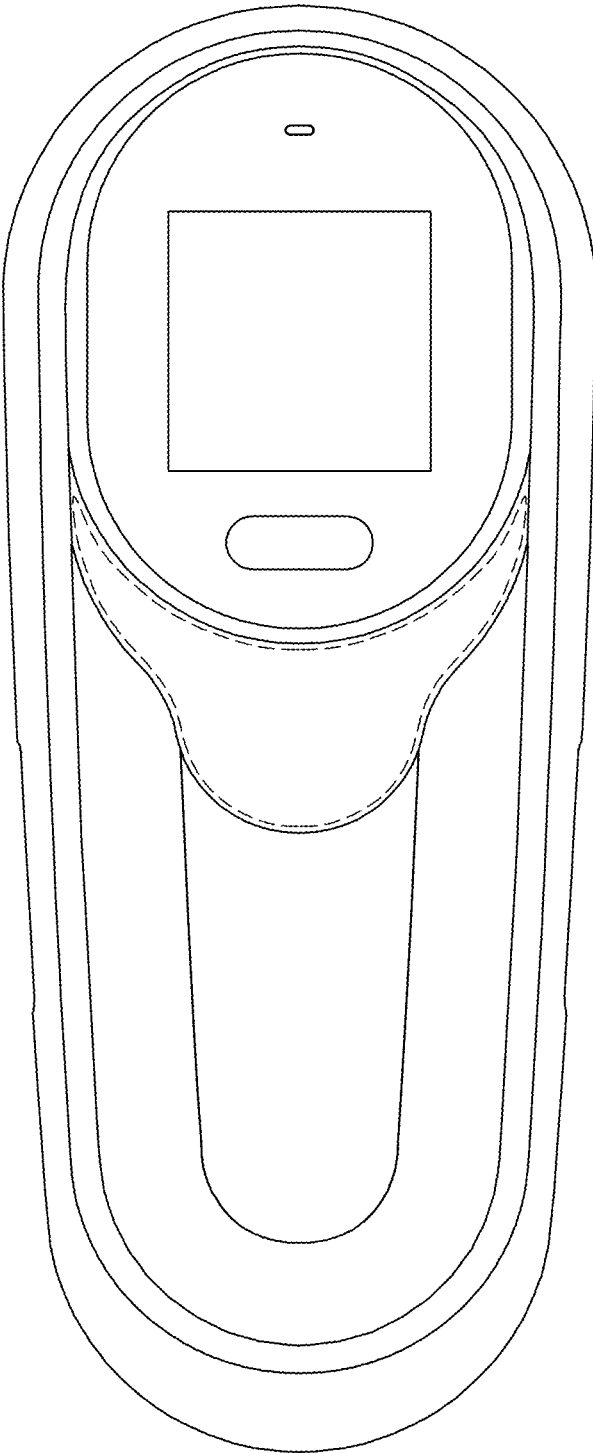


FIG. 3

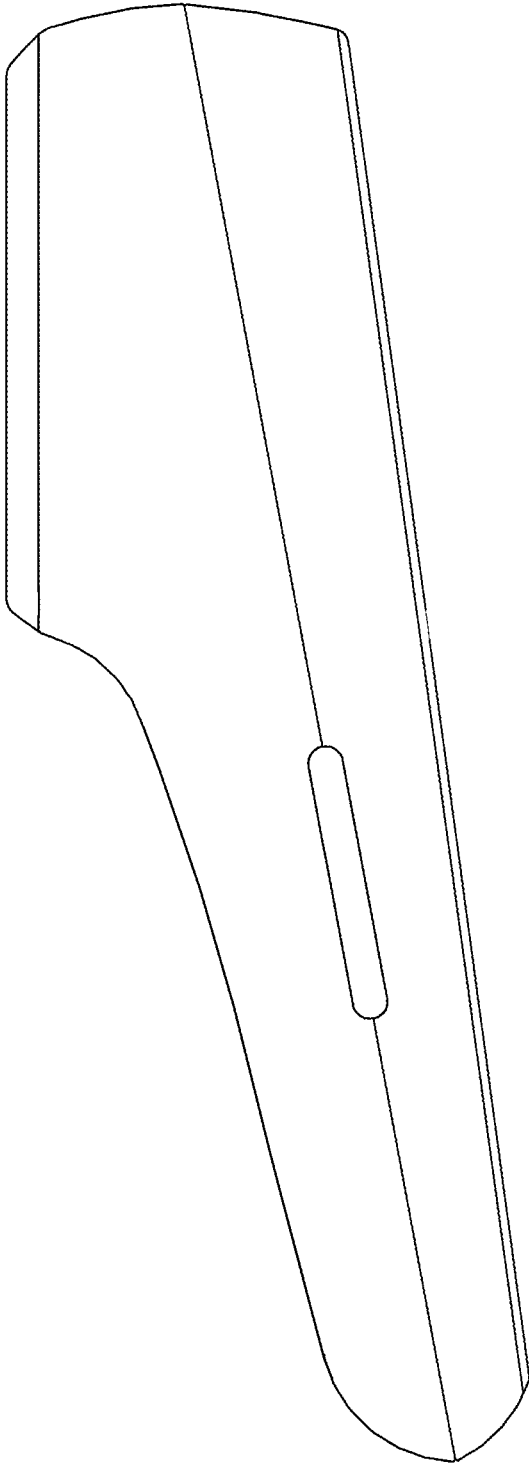


FIG. 4

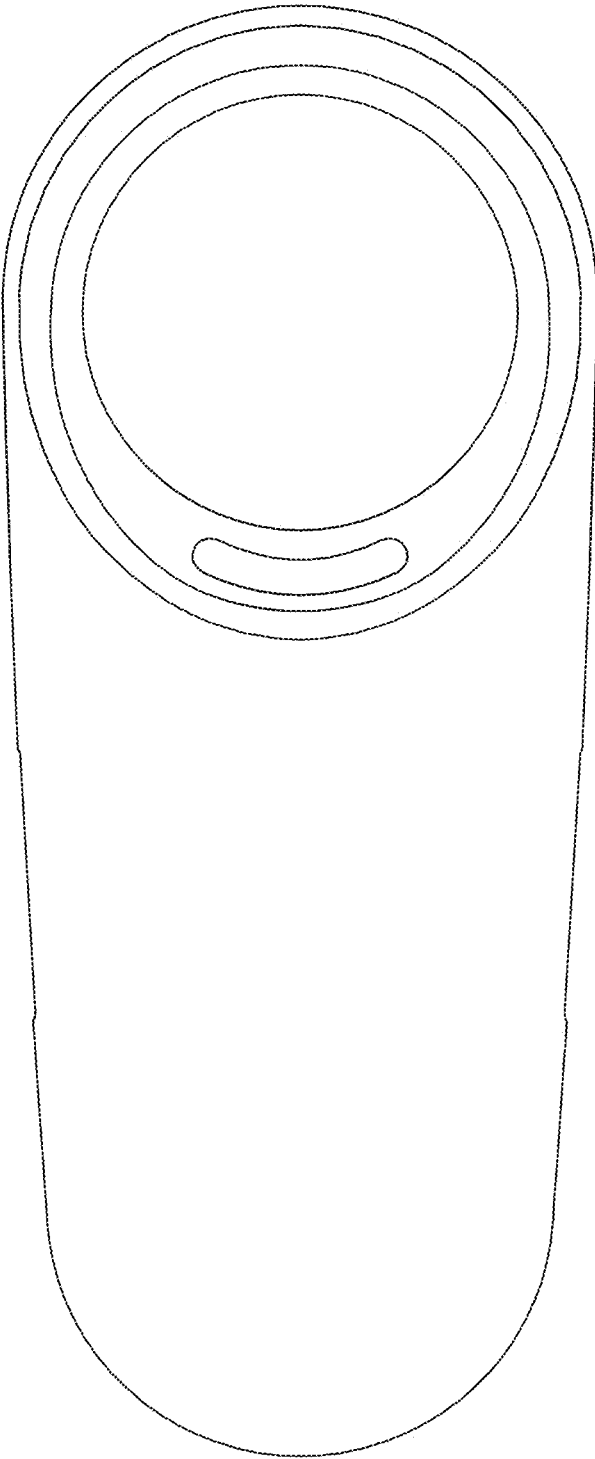


FIG. 5



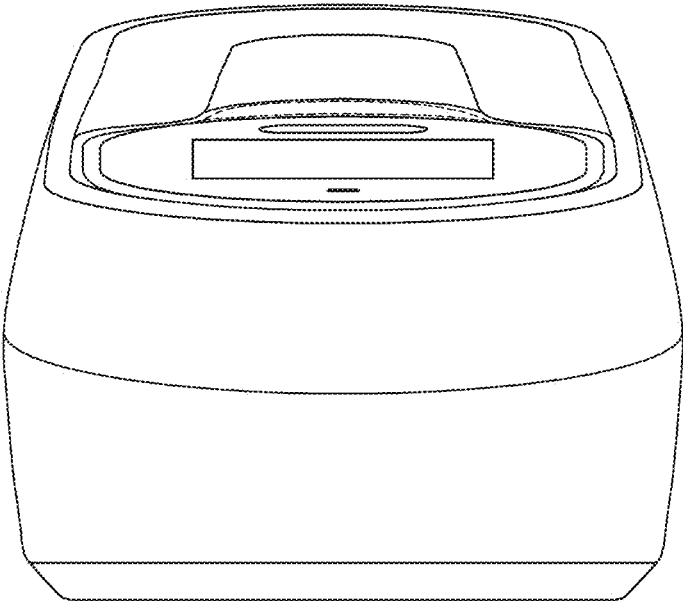


FIG. 6

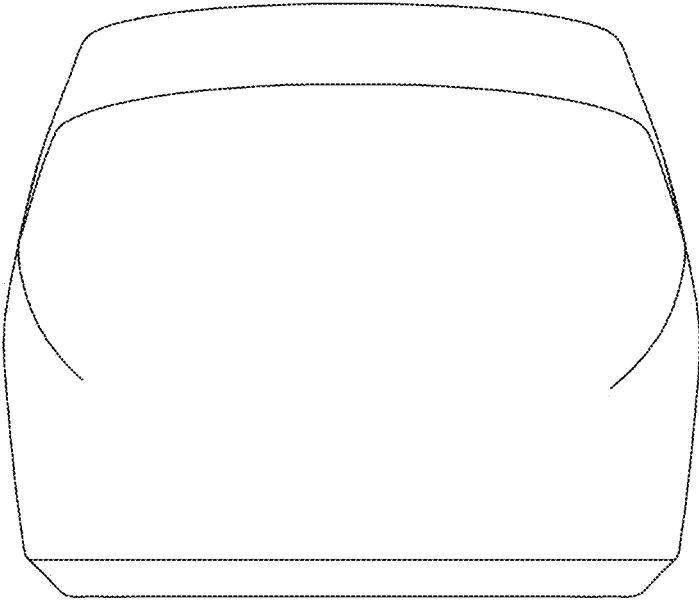


FIG. 7

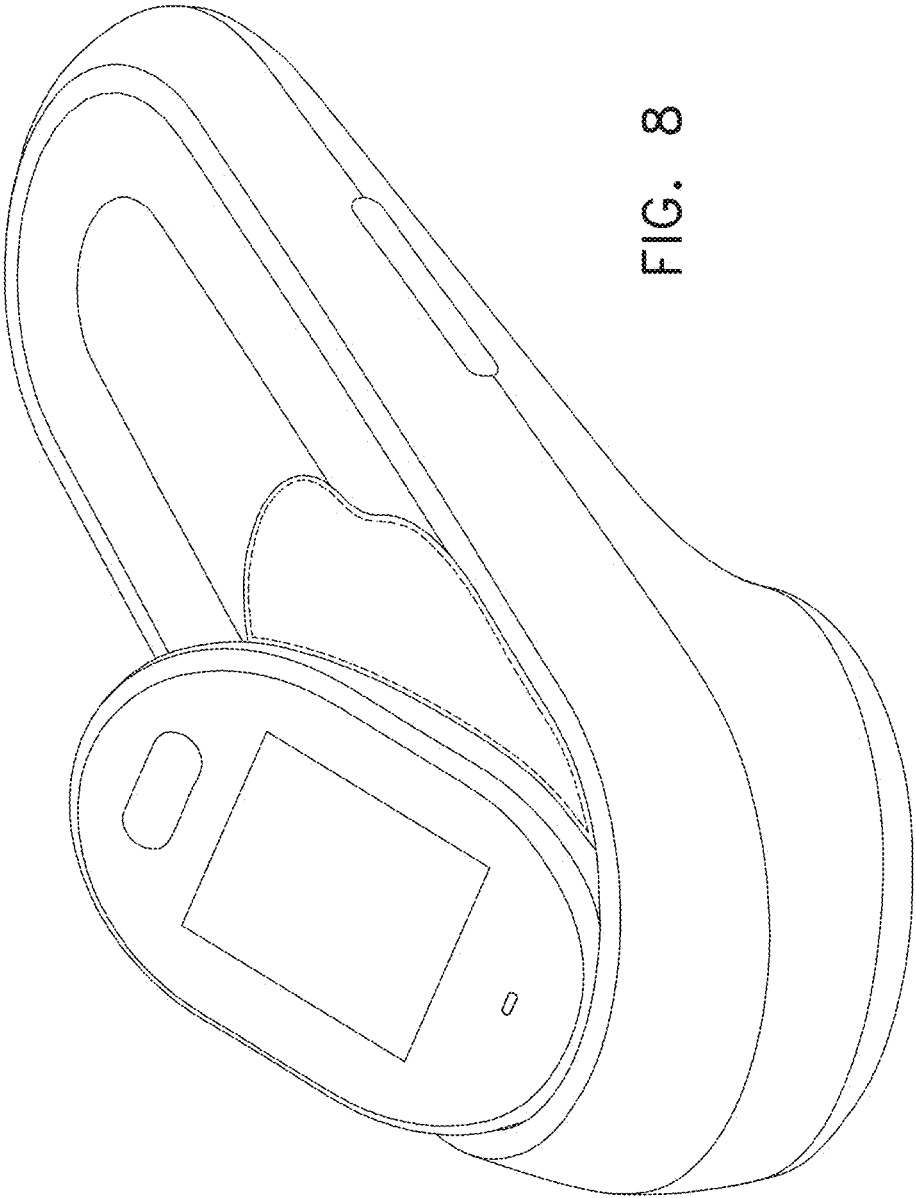


FIG. 8