

(19) World Intellectual Property Organization
International Bureau



(43) International Publication Date
15 June 2006 (15.06.2006)

PCT

(10) International Publication Number
WO 2006/063027 A1

- (51) International Patent Classification:
A61F 7/02 (2006.01)
- (21) International Application Number:
PCT/US2005/044214
- (22) International Filing Date:
6 December 2005 (06.12.2005)
- (25) Filing Language: English
- (26) Publication Language: English
- (30) Priority Data:
11/006,491 7 December 2004 (07.12.2004) US
- (71) Applicant (for all designated States except US):
ARIZANT HEALTHCARE INC [US/US]; 10393
West 70th Street, Eden Prairie, Minnesota 55344 (US).
- (72) Inventor; and
- (75) Inventor/Applicant (for US only): ANDERSON,
Thomas, P. [US/US]; 13289 Alabama Avenue South,
Savage, Minnesota 55378 (US).
- (74) Agent: MEADOR, Terrance, A.; INCAPLAW, 1050
Rosecrans Street, Suite K, San Diego, California 92106
(US).
- (81) Designated States (unless otherwise indicated, for every
kind of national protection available): AE, AG, AL, AM,

AT, AU, AZ, BA, BB, BG, BR, BW, BY, BZ, CA, CH, CN,
CO, CR, CU, CZ, DE, DK, DM, DZ, EC, EE, EG, ES, FI,
GB, GD, GE, GH, GM, HR, HU, ID, IL, IN, IS, JP, KE,
KG, KM, KN, KP, KR, KZ, LC, LK, LR, LS, LT, LU, LV,
LY, MA, MD, MG, MK, MN, MW, MX, MZ, NA, NG, NI,
NO, NZ, OM, PG, PH, PL, PT, RO, RU, SC, SD, SE, SG,
SK, SL, SM, SY, TJ, TM, TN, TR, TT, TZ, UA, UG, US,
UZ, VC, VN, YU, ZA, ZM, ZW.

(84) Designated States (unless otherwise indicated, for every
kind of regional protection available): ARIPO (BW, GH,
GM, KE, LS, MW, MZ, NA, SD, SL, SZ, TZ, UG, ZM,
ZW), Eurasian (AM, AZ, BY, KG, KZ, MD, RU, TJ, TM),
European (AT, BE, BG, CH, CY, CZ, DE, DK, EE, ES, FI,
FR, GB, GR, HU, IE, IS, IT, LT, LU, LV, MC, NL, PL, PT,
RO, SE, SI, SK, TR), OAPI (BF, BJ, CF, CG, CI, CM, GA,
GN, GQ, GW, ML, MR, NE, SN, TD, TG).

Declarations under Rule 4.17:


- as to applicant's entitlement to apply for and be granted a
patent (Rule 4.17(ii))
- as to the applicant's entitlement to claim the priority of the
earlier application (Rule 4.17(iii))

Published:

- with international search report

[Continued on next page]

(54) Title: WARMING DEVICE

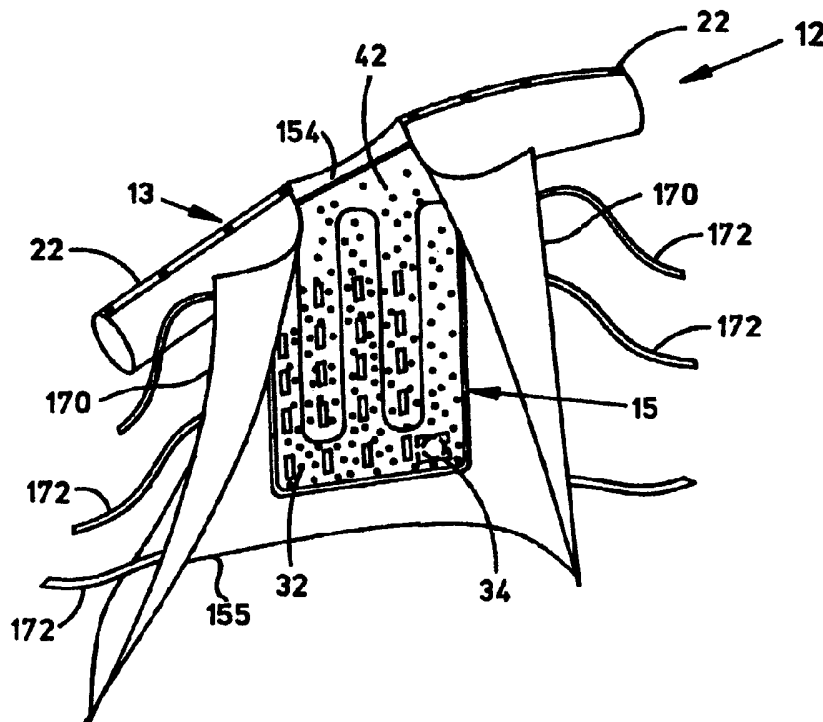

(57) Abstract: A warming device includes a clinical garment having an inside surface supporting a convective apparatus with separately inflatable sections, each adapted to enable a particular mode of warming.

WO 2006/063027 A1



-
- *before the expiration of the time limit for amending the claims and to be republished in the event of receipt of amendments* *For two-letter codes and other abbreviations, refer to the "Guidance Notes on Codes and Abbreviations" appearing at the beginning of each regular issue of the PCT Gazette.*

WARMING DEVICE

RELATED APPLICATIONS

5 This application contains subject matter related to the subject matter of the following patent applications, commonly owned herewith:

Patent Cooperation Treaty (PCT) Application No. PCT/US03/11128, filed April 10, 2003, entitled "Patient Comfort Apparatus and System", and published on October 23, 2003 under Publication No. WO 03/086500;

10 US Patent Application No. 10/411,431, filed April 10, 2003, entitled "Forced Air Warming Unit"; and

US Patent Application No. 11/005,883, filed December 7, 2004, for "Warming Device With Varied Permeability."

15 BACKGROUND OF THE INVENTION

A warming device that may be used perioperatively use includes a clinical garment and convective apparatus with multiple sections supported on the inside of the garment.

20 Convective devices that transfer heat to a human body are known. For example, there are devices that receive a stream of warmed pressurized air, inflate in response to the pressurized air, distribute it within a pneumatic structure, and emit the warmed air onto a body. These devices are typically called "convective thermal blankets" or "covers". Arizant Healthcare Inc., the assignee of this application, makes and sells such
25 thermal blankets under the BAIR HUGGER® brand. One such device is the Model 522 Upper Body Blanket.

Use of the term "convective" to denote the transfer of heat between a warming device and a body refers to the principal mode of heat transfer, it being understood that heat may at the same time be transferred between a convective warming device and a
30 body by conduction and radiation, although not to the degree of convection.

Convective warming has been used with increasing frequency to prevent or mitigate hypothermia during medical treatment. However, with the expansion of convective warming to treat core body cooling, it becomes apparent that it has manifold medical uses.

For example, a recent invention disclosed in the referenced PCT application adapts a clinical garment such as a robe or gown to receive a convective warming device in order to warm a person wearing the garment in a clinical setting for comfort and mobility of the person. Arizant Healthcare Inc., the assignee of this application, makes and sells such warming devices under the BAIR PAWS® brand. These devices are intended to warm patients prior to surgery, and there is a need to further adapt such a combination for use perioperatively.

The term "perioperative" is defined in the *PDR Medical Dictionary*, Second Edition, (Medical Economics Company, 2000), as "around the time of operation." The perioperative period is characterized by a sequence including the time preceding an operation when a patient is being prepared for surgery ("the preoperative period"), followed by the time spent in surgery ("the intraoperative period"), and by the time following an operation when the patient is closely monitored for complications while recovering from the effects of anesthesia ("the postoperative period").

According to Mahoney et al. (Maintaining intraoperative normothermia: A meta-analysis of outcomes with costs. *AANA Journal*. 4/99;67,2:155-164.), therapeutic warming is employed during at least the intraoperative period in order to prevent or mitigate a constellation of effects that result from hypothermia. In fact, it is increasingly manifest that maintenance of normothermia perioperatively enhances the prospects for a quick, successful recovery from surgery. The effectiveness of therapeutic warming depends upon delivery of enough heat to a patient's body to raise the patient's core body temperature to, or maintain it within, a narrow range, typically near 37°C. This range is called "normothermic" and a body with a core temperature in this range is at "normothermia." Hypothermia occurs when the core body temperature falls below 36°C; mild hypothermia occurs when core body temperature is in the range of 34°C to 36°C. Therefore, "perioperative therapeutic warming" is warming therapy capable of being delivered during one or more of the perioperative periods for the prevention or treatment of hypothermia.

Therapeutic warming is contrasted with "comfort warming" which is intended to maintain or enhance a patient's sense of "thermal comfort". Of course, therapeutic warming may also comfort a patient by alleviating shivering or a feeling of being cold, but this is a secondary or ancillary effect. And conversely, there may be a secondary or ancillary therapeutic effect derived from the application of thermal comfort treatments such as the relief of patient anxiety. Thermal comfort is a subjective notion; however, the

environmental conditions necessary to produce a sense of thermal comfort in a population of human beings are known and well tabulated. For example, Fanger (*Thermal Comfort: Analysis and Applications of Environmental Engineering*. Danish Technical press, Copenhagen, 1970) defines thermal comfort as "that condition of mind which expresses satisfaction with the thermal environment." Even when a patient is normothermic, less than ideal environmental conditions can result in acute feelings of discomfort. Under normothermic conditions, thermal comfort is largely determined with reference to skin temperature, not core body temperature. Comfort warming is warming applied to a patient to alleviate the patient's sense of thermal discomfort.

Therapeutic warming may be indicated during any one or more of the perioperative periods. For example, for a short operation in a surgery with no warming equipment available, a person may be warmed preoperatively in a preparation area to raise mean body temperature to a level higher than normal in order to store enough thermal energy to maintain normothermia, without heating, intraoperatively. After surgery, it may be necessary to apply therapeutic warming in a recovery area to raise the core temperature to normothermia and maintain it there for a period of time while anesthesia wears off. Alternatively, for a long surgery in an arena with heating equipment available, a person may be warmed for comfort before surgery and warmed therapeutically during and after surgery.

Thermal blankets are typically used for therapeutic heating. An example is found in U.S. Patent 6,524,332, "System and Method for Warming a Person to Prevent or Treat Hypothermia", commonly owned with this application. Thermal blanket designs have converged on a lightweight inflatable structure made of a flexible material which distributes warmed pressurized air over or against a permeable blanket surface that faces some portion of a patient's body and emits the distributed heated air through small apertures or interstices in the surface.

Thermal blanket design has been adapted for comfort warming by convective means such as those described in the referenced U.S. Patent Applications, and the referenced Publication No. WO 03/086500.

When delivered by convective devices, therapeutic warming is distinguished from comfort warming by intended effects and by the parameters of heat delivery that produce those effects. In this regard, a convective warming system typically includes a source of warmed pressurized air (also called a heater/blower unit, a forced air warming unit, a heater unit, etc.), a convective device such as a thermal blanket (which is, typically,

inflatable), and a flexible conduit or air hose connecting the heater/blower unit with the thermal blanket. Use of such a system for a particular type of warming requires delivery of warmed air through a convective device at parametric values that achieve a particular objective. The conditions by which a convective device produces thermal comfort in normothermic individuals at steady state are significantly different from those necessary to treat hypothermia. Typically the conditions for thermal comfort are met in a system with a relatively low capacity heater/blower unit, while those in a therapeutic warming system are achieved with a relatively high capacity heater/blower unit. The different capacities have led to use of air hoses with different capacities, with those delivering air flow for thermal comfort typically having smaller diameters than those serving a therapeutic warming requirement. The result is a divergence of designs leading to installation of different air delivery infrastructures for therapeutic and comfort warming.

Health care cost is an issue of national importance. The cost of warming perioperatively by convection is directly related to the number of perioperative periods in which a person is warmed; the cost increases when different convective warming apparatus are used in different periods to accomplish different goals. For example, when comfort and mobility are objectives of warming a person during the preoperative period and therapy is the objective of warming during one or more of the intraoperative and postoperative periods, it is presently necessary to use different convective warming configurations. Manifestly, if one convectively-operating warming device could be used or adapted to be used perioperatively, significant savings in thermal care could be realized.

SUMMARY

In one aspect, a warming device capable of being used perioperatively includes a clinical garment having an inside surface supporting a convective apparatus with multiple sections. At least one section is adapted for comfort warming and at least another section is adapted for therapeutic warming.

In another aspect, a warming device that may be used perioperatively includes a clinical garment and interleaved convective apparatus in an integrated structure attached to the inside of the garment.

10

BRIEF DESCRIPTION OF THE DRAWINGS

FIG. 1 is an illustration of a person wearing a warming device constituted of a clinical garment and a convective apparatus with multiple sections mounted to the inside
5 of the garment.

FIGS. 2A and 2B illustrate plan views of the warming device.

FIGS. 3A and 3B illustrate progressive stages of assembly of the warming device.

FIGS. 4A and 4B are magnified partial sectional drawings illustrating construction
10 of the convective apparatus.

FIGS. 5A-5C are plan views of alternate configurations for the convective apparatus with multiple sections.

SPECIFICATION

A warming device that may be used perioperatively is constituted of a clinical garment and a convective apparatus with multiple sections supported on an inside surface of the garment. In this regard, a "clinical garment" is a garment that is typically used to temporarily clothe a patient in a clinical setting. Such garments include hospital gowns, robes, bibs and other equivalents. The clinical setting may be a medical or dental office or clinic, a hospital, or any facility or institution that provides medical or dental treatment to patients. The convective apparatus has multiple sections, preferably two separate sections. Each section may receive and distribute at least one stream of warmed pressurized air in a pneumatic structure and emit the air through at least one permeable surface to thereby convectively warm a person wearing the clinical garment. One section is adapted for comfort warming by convection, the other for therapeutic warming by convection.

In one aspect, a warming device capable of perioperative use may be worn on a person where it receives a first stream of warmed pressurized air in one section of the convective apparatus, distributes the pressurized air within the one section, and emits the air through a permeable surface of the one section to convectively warm the person's body for comfort. In another aspect, a warming device capable of perioperative use may be worn on a person where it receives a second stream of warmed pressurized air in the other section of the convective apparatus, distributes the pressurized air within the other section, and emits the air through a permeable surface of the other section to convectively warm the person's body for therapy. Preferably, the permeable surfaces are respective sections or regions of the same surface. Further, although not necessary to the practice of this warming device, the permeable surfaces may have differing or varied permeabilities in order to optimize the effects produced by the sections of the convective apparatus.

In the warming device illustrated and discussed below, each of the sections of the convective apparatus is inflatable. That is, the structure of each section, flaccid when not in use, tautens when receiving a stream of pressurized air.

Refer now to FIG.1 in which a person 10 wearing a warming device 12 that may be used perioperatively is shown. The warming device 12 is constituted of a clinical garment 13 and a convective apparatus 15 with multiple sections that is supported on an inside surface of the clinical garment 13. The convective apparatus has for example two

separate sections, each of which has at least one inlet port through which the section may receive warmed pressurized air from a heater/blower unit (not seen). Each inlet port is accessible through an aperture in the clinical garment 13. For example one inlet port for one of the sections may be accessed through a flap 18 in the clinical garment. An inlet port of another section may be accessed by releasing and folding down a portion 20 of the clinical garment. This latter form of access is illustrated in FIG. 1 where an air hose 21 with a nozzle 23 is received in an inlet port of one section of the convective apparatus. In this case, the portion 20 of the clinical garment comprises a portion of the upper edge and left sleeve that may be held to an opposing portion of the clinical garment by opposing strips of hook-and-eye material. Of course, this other inlet port may also be accessed through a flap such as the flap 18 instead of a folded-down garment section. Yet another means of accessing the inlet port for the other section would be to provide perforations in the nearest sleeve.

Convective apparatus such as thermal blankets have been specifically designed for particular uses. For example, a full body thermal blanket is adapted to lie upon the person and to extend longitudinally along the body of the person in order to cover substantially the person's entire body, from near the ankles or feet up to the neck. A lower body thermal blanket is adapted to lie upon the person and to extend longitudinally along the body of a person in order to cover the person's lower body, from near the ankles or feet up to the waist or pelvis of the person. An upper body thermal blanket has a bow-tie shape that is adapted to lie upon and extend transversely across the upper body of a person in order to cover the person's chest and extended arms. When fed a stream of warmed pressurized air, each of these thermal blankets inflates and distributes the air within itself. The pressurized air flows through apertures on a permeable surface of the thermal blanket which faces the person. These thermal blankets may have one, two, or more inlet ports through which an air hose provides warmed pressurized air from a heater/blower unit. The construction of thermal blankets is well understood. Examples of specific constructions are given in US Patent 5,620,482, US Patent 5,443,488, US Patent 5,360,439, and US Patent 5,304,213.

Typically, convective warming products are designed to provide a single mode of warming. Each of the thermal blankets described above is designed for therapeutic warming. The devices described in publication WO 03/086500 are designed for comfort warming. In contrast, the warming device described in this specification may provide either therapeutic warming or comfort warming, depending on the need. One section of

the convective apparatus is constructed to receive air at low flow rates in order to provide comfort heating at steady state. Another section is constructed to receive air at higher flow rates in order to provide therapeutic heating at steady state.

A convective apparatus 15 with multiple sections is illustrated in FIGS. 2A and 2B. In FIG 2A the convective apparatus 15 is shown disposed inside the outline of the clinical garment 13; in FIG. 2B, the convective apparatus 15 is shown in plan view looking toward a permeable surface of the convective apparatus 15. The convective apparatus 15 has a "Tee" shape with a thick base 27 and an elongate top 28 which is perpendicular to the base 27. The elongate top 28 extends transversely across a longitudinal axis 21 of the clinical garment 13, between and at least partly into the sleeves 22 of the clinical garment 13. The base 27 is substantially centered on the longitudinal axis 21. The elongate top 28 has portions 29 on either side of the base 27. Each of the portions 29 protrudes at least part way into a respective sleeve 22 of the clinical garment 13.

The convective apparatus 15 has multiple sections. A "section" of the convective apparatus 15 is a portion or division of the convective apparatus 15 that may be inflated and operated separately from any other section of the convective apparatus 15. For example, the convective apparatus 15 has a section 32 and a section 42. The section 32 may be inflated and operated separately from the section 42, and the section 42 may be inflated and operated separately from the section 32. The section 32 has an inlet port 34, an elongate transverse part 36, and a plurality of elongate parts 37 that connect perpendicularly to the transverse part 36. Each of the two outermost elongate parts 37 transitions through an outward 90° bend to an sleeve portion 38. Each sleeve portion 38 is in a respective portion 29 of the convective apparatus 15. Although one inlet port 34 is illustrated in the section 32, one or more additional inlet ports may be provided for convenience. Unused inlet ports are sealed or closed by known means to prevent air escaping therethrough. Preferably the inlet port 34 is provided through the side of the convective apparatus 15 which is not visible in this figure; it may also be provided through an edge of the convective apparatus 15. The inlet port 34 may comprise a collar 34a of stiff material with an opening 34b to receive the nozzle of an air hose, or it may comprise a sleeve of material, or any other equivalent structure. The space in the transverse part 36 is in fluid communication with the spaces in the elongate parts 37 so that pressurized air flowing through an inlet port into the transverse part 36 flows also into the elongate parts 37, thereby inflating the section 32. The surface of the section 32

which is visible in FIG. 2, including the surfaces of the transverse part 36 and the elongate parts 37, is permeable, permitting pressurized air that is flowing into and inflating the section 32 to be expelled toward the interior of the clinical garment 13.

5 The section 42 has an inlet port 44, an elongate transverse part 46, and a plurality of elongate parts 47 that connect perpendicularly to the transverse part 46. The elongate transverse part 46 is parallel and adjacent to the sleeve portions 38 of the section 32. The end portions of the elongate part 46 are in respective portions 29 of the convective apparatus 15. The elongate parts 47 of the section 42 are interleaved with the elongate parts 37 of the section 32, thereby forming an integrated convective
10 apparatus 15 with dual sections. Although one inlet port 44 is illustrated in the section 42, one or more additional inlet ports may be provided for convenience. Unused inlet ports are sealed or closed by known means to prevent air escaping therethrough. Preferably the inlet port 44 is provided through the side of the convective apparatus 15 which is not visible in this figure; it may also be provided through an edge of the
15 convective apparatus 15. The inlet port 44 may comprise a collar 44a of stiff material with an opening 44b to receive the nozzle of an air hose, or it may comprise a sleeve of material, or any other equivalent structure. The space in the transverse part 46 is in fluid communication with the spaces in the elongate parts 47 so that pressurized air flowing through an inlet port into the transverse part 46 flows also into the elongate parts 47,
20 thereby inflating the section 42. The surface of the section 42 which is visible in FIG. 2, including the surfaces of the transverse part 46 and the elongate parts 47, is permeable, permitting pressurized air that is flowing into and inflating the section 42 to be expelled toward the interior of the clinical garment 13.

The inlet port 34 of the section 32 has a smaller opening 34b than the opening
25 44b through the inlet port 44 of the section 42. Consequently, the inlet port 34 accepts an air hose nozzle with a smaller diameter than the air hose nozzle diameter accepted by the inlet port 44. The smaller nozzle diameter signifies a comfort warming air supply with an air hose having a smaller diameter than the air hose of a therapeutic warming air supply. Further, the smaller air hose may be coupled to a heater blower unit with a
30 smaller capacity than that of the heater blower unit of the therapeutic warming air supply. The smaller-diameter, smaller-capacity comfort warming air supply ensures that the section 32 operates in response to a heater/blower unit designed for comfort warming while the larger-diameter, higher-capacity therapeutic air supply ensures that the section 42 operates in response to a heater/blower unit designed for therapeutic warming.

FIGS. 3A and 3B illustrate assembly of a perioperative warming device constituted of the clinical garment 13 and the convective apparatus 15 with multiple sections. The convective apparatus 15 is adapted to be attached to, received on, supported on or constructed on the inside surface 52 of the clinical garment 13. The clinical garment 13 has at least one flap 18 through which an inlet port of one section may be accessed. For example, the flap 18 provides access to the inlet port 34 for receiving and retaining the nozzle of an air hose through which warmed pressurized air may be provided at a temperature and a capacity (in ft³ per minute) to provide comfort warming for a person wearing the clinical garment 13.

Refer to FIGS. 2B, 3B, and 4 for an understanding of how the convective apparatus 15 may be constructed by joining two sheets of material, one permeable to permit warmed pressurized air to be emitted through the sheet, the other impermeable. With reference to FIGS. 2B and 3B, the impermeable sheet faces the clinical garment 13, while the permeable sheet faces the interior of the clinical garment 13. The convective apparatus 15 may be constructed as a separate piece and then attached to the inside surface 52 of the clinical garment 13 with the impermeable sheet against the inside surface 52, or it may be constructed integrally with the clinical garment by using a portion of the clinical garment itself as one of the sheets of the convective device. For example, with reference to FIGS. 2B and 4 two sheets 114 and 116 of flexible material are joined by a single substantially continuous seal 70 along the periphery of the convective apparatus 15, and also by a continuous seal 72 that separates the sections of the convective apparatus and defines the parts of each section. The seal 70 is interrupted at the ends of the transverse part 46 to provide vents 74 in the peripheral edge of the convective apparatus 15 through which warmed pressurized air can flow from the convective apparatus 15 into the sleeves 22 for warming the arms during therapeutic warming. Similarly, the seal 70 is interrupted at the ends of the arm portions 38 to provide vents 74 in the peripheral edge of the convective apparatus 15 through which warmed pressurized air can flow from the convective apparatus 15 into the sleeves 22 for warming the arms during comfort warming. The sheets may be further joined at multiple stake points within the periphery. Depending upon the materials selected, seals and stake points may be made for example by sewing, gluing, heating, or ultrasonically bonding the sheets along the seals, or by combinations thereof, or by any equivalent process.

Either or both of the sheets 114 and 116 may be a single sheet or may have a laminate structure. A laminate sheet structure may include a layer (114a, 116a) of extruded synthetic material lined with a layer (114b, 116b) of non-woven material. If the permeable sheet has a laminate structure, holes or apertures 132 are formed through both layers 114a, 114b of the sheet 114 to provide a permeable surface through which warmed pressurized air can be emitted toward the interior of the clinical garment 13. In Fig. 4A, the sheets 114 and 116 are oriented to have the extruded layers (114a and 116a) facing, and the seals 70, 72 are formed by a gluing process or by a heating or ultrasonic process acting through one of the layers of non-woven material. Once constructed, the convective apparatus 15 may be attached to the inside surface 52 of the clinical garment by mechanisms 150.

In Fig. 4B, the sheet 114 may be a laminate structure as described above. If the clinical garment 13 is a woven cloth, such as cotton, or a non-woven such as spunbond-meltblown-spunbond material (SMS), the seals 70, 72 between the portion of the garment's inside surface 52 and the extruded layer of the laminate sheet may be formed by a gluing, a heating, or an ultrasonic process acting between the inside surface and the sheet 114.

Another construction of the convective apparatus 15 may use a single sheet of permeable material in which the apertures are interstices in the material structure. For example with reference to either FIG. 4A or FIG. 4B, the impermeable layer 114a may be eliminated on the condition that the layer 114b be a permeable material capable of being sealed to the impermeable layer 116a or the woven cloth of the clinical garment.

Yet another alternative construction of the convective apparatus 15 is to construct the clinical garment 13 of a laminate sheet 116 and seal an apertured laminate sheet 114 or a single permeable layer 114b of woven or non-woven material thereto.

In yet another construction, the convective device may be constituted of an impermeable layer sealed around its periphery to the outside surface of the clinical garment so that the pneumatic structure is disposed on the outside of the clinical garment. In this case apertures are provided through the portion of the clinical garment beneath the impermeable layer.

Of course the sections of the convective device may be fabricated separately and placed on the inside surface 52 in the interleaved relationship shown in FIGS. 2A and 2B.

Examples of non-woven material include any one or more of polyester, cotton, rayon, polypropylene, and wood pulp. Examples of extruded synthetic material include polypropylene, polyesters, and polyurethanes. Polyolefin plastics, including polyethylene, may provide the best results in terms of manufacturability since both woven and extruded materials may be made from them. Examples of attachment materials and mechanisms 150 by which the convective apparatus 15 as presented in Fig. 4A can be attached to the inside surface 52 include two-sided adhesive, hook and loop, sewing, snaps, heat, ultrasonic, rivets, and any and all equivalents thereof.

As best seen in FIGS. 3A and 3B, the clinical garment 13 may be a standard gown, a modified gown or a special purpose gown. The gown may have a rear opening, a front opening or other suitable openings, such as a head opening in a poncho type gown. One type of gown shown in the figures has a rear opening. For example, in Figs. 3A and 3B the gown 13 has a slit 170 that extends from the neck portion 154 to a hemline 155. A fastening means is provided to provide for ease in securing the gown to the patient as well as allowing for ease in adjusting the size of the gown to accommodate various different-sized wearers. Fig. 3A shows one method using hook and eye buttons 171a, 171b positioned along opposing sides of the slit 170a, 170b that can be brought together and fastened to hold the gown to the patient. Another method attachment shown in FIG. 3B is a plurality of strings 172 positioned along opposing sides of the slit 170 that can be tied together for hold the gown to a patient. Other methods of attachments include hook and eye elements, double-sided adhesive, snaps, rivets, and any and all equivalents thereof.

The clinical garment 13 may include sleeves 22 that are sized and positioned for receiving a patient's arms. Two examples of such sleeves 22 are shown in the figures. In Figs. 3A-3B the sleeve portions 175 are slit the entire length on the shoulder or top 177. This allows access to the upper body of the patient and the inlet port 44 and allows for opening and closing of the slit sleeves 22 in an adjustable fashion using buttons, snaps, repositionable adhesive, hook and eye elements, double-sided adhesive, hook and loop, rivets, and any and all equivalents thereof. The design shown in Fig. 3A also facilitates the manufacturing of the clinical garment 13 in one piece.

As best seen in FIGS. 2A and 2B, to secure the convective apparatus to a patient, a strip 180 of double sided adhesive is adhered to the transverse part 42. During use of the perioperative warming device 12, a release liner may be removed from a

surface of the strip 180 facing the patient and adhered to the patient to prevent unintended movement of the convective apparatus 15 during warming.

Other configurations of the convective apparatus with multiple sections may be more useful for particular applications or may be more amenable to particular manufacturing architectures and/or processes than the configurations shown and discussed above; FIGS. 5A-5C illustrate three alternative configurations. Each of these figures is a schematic illustration of a convective apparatus with multiple sections presented against an outline of the clinical garment 12. The view in each case is into the clinical toward the inside surface. Accordingly, the permeable surfaces of the sections of the convective devices are visible in each drawing.

In FIG. 5A, the warming device 12 includes the clinical garment 13 and a Tee-shaped convective device 65 with multiple sections is illustrated. For example, the convective device has two sections, a section 67 and a section 68. The section 67 may be inflated and operated separately from the section 68, and the section 68 may be inflated and operated separately from the section 67. The section 67 has an elongate comb-shaped outline, with the teeth of the comb oriented generally transversely across the inside surface 52. The section 67 has an inlet port 69 (accessible through the front of the clinical garment 13). The section 68 has a comb-shaped lower part, with the teeth of the comb oriented generally transversely across the inside surface 52 and interleaved with the teeth of the section 67. The section 68 also has a transverse part that extends between and at least partially into sleeves 22 of the clinical garment 13. The section 68 has an inlet port 70 (accessible through the front of the clinical garment 13). Preferably, the section 67 may be used for comfort warming by convection, while the section 68 may be used for therapeutic warming by convection. In this latter regard the larger pneumatic structure and larger area of the permeable surface of the section 68 afford a higher capacity in ft^3 per minute for warming than the section 67.

In FIG. 5B, the warming device 12 includes the clinical garment 13 and a convective device 75 with multiple sections is illustrated. For example, the convective device has two sections, a section 77 and a section 78. The section 77 may be inflated and operated separately from the section 78, and the section 78 may be inflated and operated separately from the section 77. The section 77 has an elongate comb-shaped outline, with the teeth of the comb oriented generally transversely across the inside surface 52. The section 77 has an inlet port 79 (accessible through the front of the clinical garment 13). The section 78 has a comb-shaped lower part, with the teeth of the

comb oriented generally transversely across the inside surface 52 and interleaved with the teeth of the section 77. The section 78 also has a notched upper part that does not extend between the sleeves of the clinical garment 13. The section 78 has an inlet port 80 (accessible through the front of the clinical garment 13). Preferably, the section 77
5 may be used for comfort warming by convection, while the section 78 may be used for therapeutic warming by convection. In this latter regard the larger pneumatic structure and larger area of the permeable surface of the section 78 afford a higher capacity in ft³ per minute for warming than the section 77.

In FIG. 5C, the warming device 12 includes the clinical garment 13 and a
10 convective device 85 with multiple sections is illustrated. For example, the convective device has two sections, a section 87 and a section 88. The section 87 may be inflated and operated separately from the section 88, and the section 88 may be inflated and operated separately from the section 87. The section 87 has an upright comb-shaped outline, with the teeth of the comb oriented generally upwardly along the middle of the
15 inside surface 52. The section 87 has an inlet port 89 (accessible through the front of the clinical garment 13). The section 88 has a comb-shaped part, with the teeth of the comb oriented generally downwardly along the inside surface 52 and interleaved with the teeth of the section 87. The section 88 also has a notched upper part that does not extend between the sleeves of the clinical garment 13. The section 88 has an inlet port 90
20 (accessible through the front of the clinical garment 13). Preferably, the section 87 may be used for comfort warming by convection, while the section 88 may be used for therapeutic warming by convection. In this latter regard the larger pneumatic structure and larger area of the permeable surface of the section 88 afford a higher capacity in ft³ per minute for warming than the section 87.

In use, a person may be warmed perioperatively using a warming device
25 constituted of a clinical garment and a dual-section convective apparatus supported on an inside surface of the clinical garment by dressing a person with the clinical garment during the preoperative period, coupling a first section (the section 32 in FIG. 2B, for example) of the convective apparatus to a source of warmed pressurized air for comfort
30 warming, and convectively warming the person for comfort by way of the first section. To prepare for surgery, the first section is decoupled from the comfort warming source and the clinical garment is arranged to afford access to a surgical site. In preparation for surgery, the clinical garment may be left on the person, with its skirts rolled up to provide surgical access. Alternatively, the clinical garment may be removed to allow the

convective apparatus to be positioned on the person to provide surgical access. In this latter case, the skirts, sleeves and other loose parts of the clinical garment may be rolled or folded onto the convective device. In yet another alternative, if the convective device is releasably attached to the inside surface of the clinical garment, the garment may be
5 separated from the convective device during surgery and reattached later postoperatively. During surgery, the convective device may be secured to the person by means of the double sided adhesive and a second section of the convective apparatus (for example the section 42 in FIG. 2B) may be coupled to a source of warmed pressurized air for therapeutic warming, and the person may be convectively warmed for
10 therapy by way of the second section. Following surgery, the convective apparatus is detached from the person (but only if secured to the person for surgery), the convective apparatus is reattached to the clinical garment (but only if detached therefrom for surgery), the person is again dressed with the clinical garment and either warmed for comfort or warmed for therapy.

15 Manifestly, the descriptions and illustrations in this specification are presented for an understanding of how to make and use an exemplary warming device. The only limitations on the scope of protection afforded the inventive principles presented are in the following claims.

CLAIMS

1. A warming device, comprising:
a clinical garment with an inside surface; and
a convective apparatus supported on the inside surface;
the convective apparatus including a first section adapted to provide comfort warming by convection and a second section adapted to provide therapeutic warming by convection.
2. The warming device of claim 1, wherein the first and second sections are separately inflatable and each includes a permeable surface facing the interior of the clinical garment.
3. The warming device of claim 2, wherein the first section includes:
a transverse part;
a plurality of elongate parts extending from and in fluid communication with the transverse part; and
at least one inlet port.
4. The warming device of claim 3, wherein the second section includes:
a transverse part;
a plurality of elongate parts extending from and in fluid communication with the transverse part; and
at least one inlet port.
5. The warming device of claim 4 wherein the elongate parts of the first section are interleaved with the elongate parts of the second section.
6. The warming device of claim 4, wherein the elongate parts of the first section include respective elongate parts having oppositely-directed portions adjacent and parallel to the transverse part of the second section.

7. The warming device of claim 6, wherein the transverse part of the second section and the oppositely-directed portions extend between and at least partially into sleeves of the clinical garment.
8. The warming device of claim 7, wherein the transverse part of the second section and each oppositely-directed portions include ends, further including vents at ends of the transverse portion of the second section and vents at the ends of the oppositely-directed portions.
9. The warming device of claim 8, further including means for securing the convective apparatus to a person.
10. The warming device of claim 9, wherein the means include double-sided adhesive.
11. The warming device of claim 8, further including at least one inlet port in each of the first and second sections.
12. The warming device of claim 11, further including an aperture in the clinical garment to an inlet port of the first section.
13. The warming device of claim 11, further including a portion of at least one sleeve of the clinical garment separable from a corresponding portion of the sleeve to provide access to an inlet port of the second section.
14. The warming device of claim 1, further including a portion of at least one sleeve of the clinical garment separable from a corresponding portion of the sleeve and means for releasably joining the sleeve portions.

15. A warming device, comprising:
 - a clinical garment with an inside surface; and
 - a tee-shaped convective apparatus supported on the inside surface;
 - the convective apparatus including dual sections adapted to provide comfort warming and therapeutic warming by convection.

16. The warming device of claim 15, wherein the dual sections are separately inflatable and each includes a permeable surface facing the interior of the clinical garment.

17. The warming device of claim 16, wherein a first section includes:
 - a transverse part;
 - a plurality of elongate parts extending from and in fluid communication with the transverse part; and
 - at least one inlet port..

18. The warming device of claim 17, wherein a second section includes:
 - a transverse part;
 - a plurality of elongate parts extending from and in fluid communication with the transverse part; and
 - at least one inlet port.

19. The warming device of claim 18 wherein elongate parts of the first section are interleaved with elongate parts of the second section.

20. The warming device of claim 18, wherein the elongate parts of the first section include respective elongate parts having oppositely-directed portions adjacent and parallel to the transverse part of the second section.

21. The warming device of claim 6, wherein the transverse part of the second section and the oppositely-directed portions form a cross piece of the tee-shaped convective apparatus extending between and at least partially into sleeves of the clinical garment.

22. The warming device of claim 21, wherein the transverse part of the second section and each oppositely-directed portions include ends, further including means at ends of the transverse portion of the second section for emitting air from the second section into the sleeves and means at the ends of the oppositely-directed portions for emitting air from the first section into the sleeves.
23. The warming device of claim 22, further including means for securing the convective apparatus to a person.
24. The warming device of claim 23, wherein the means for securing include double-sided adhesive.
25. The warming device of claim 22, further including at least one inlet port in each of the first and second sections.
26. The warming device of claim 25, further including an aperture in the clinical garment to an inlet port of the first section.
27. The warming device of claim 25, further including a portion of at least one sleeve of the clinical garment separable from a corresponding portion of the sleeve to provide access to an inlet port of the second section.
28. The warming device of claim 15, further including a portion of at least one sleeve of the clinical garment separable from a corresponding portion of the sleeve and means for releasably joining the sleeve portions.

29. A warming device, comprising:
a clinical garment with an inside surface; and
a convective apparatus supported on the inside surface;
the convective apparatus including at least two separately inflatable sections.
30. The warming device of claim 29, wherein each inflatable includes a permeable surface facing the interior of the clinical garment.
31. The warming device of claim 30, wherein a first section includes:
a transverse part;
a plurality of elongate parts extending from and in fluid communication with the transverse part; and
at least one inlet port.
32. The warming device of claim 31, wherein a second section includes:
a transverse part;
a plurality of elongate parts extending from and in fluid communication with the transverse part; and
at least one inlet port.
33. The warming device of claim 32 wherein elongate parts of the first section are interleaved with elongate parts of the second section.

34. A method for warming a person using a warming device constituted of a clinical garment and a dual-section convective apparatus supported on an inside surface of the clinical garment, comprising:

- dressing a person with the clinical garment preoperatively;
- coupling a first section of the convective apparatus to a first source of warmed pressurized air; and
- convectively warming the person for comfort by way of the first section.

35. The method of claim 34, further including:

- decoupling the first section from the first source;
- coupling a second section of the convective apparatus to a second source of warmed pressurized air; and
- convectively warming the person for therapy by way of the second section.

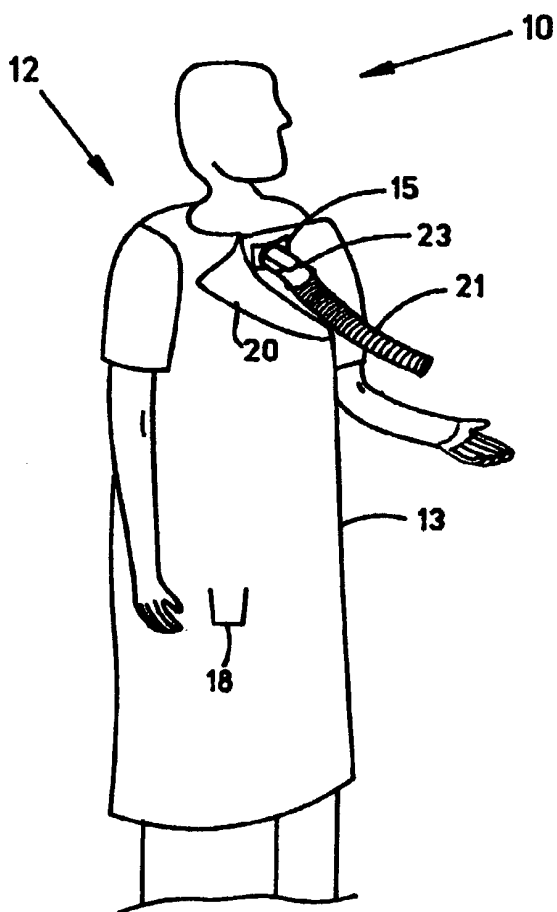


FIG. 1

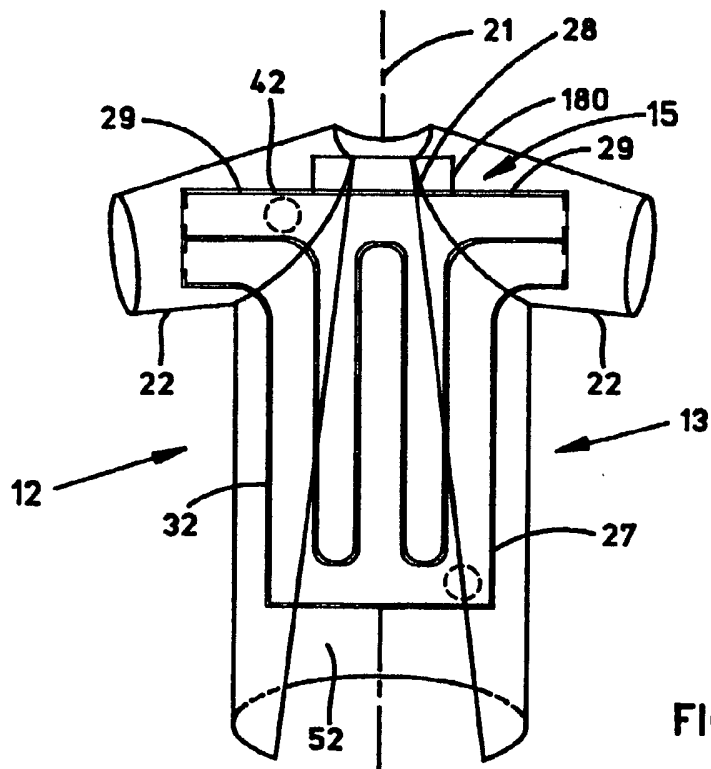


FIG. 2A

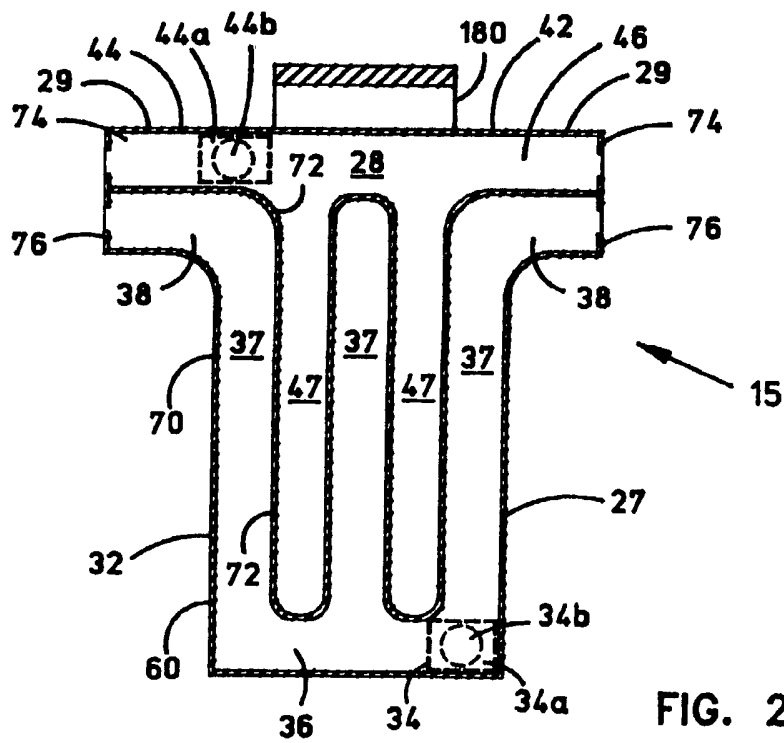
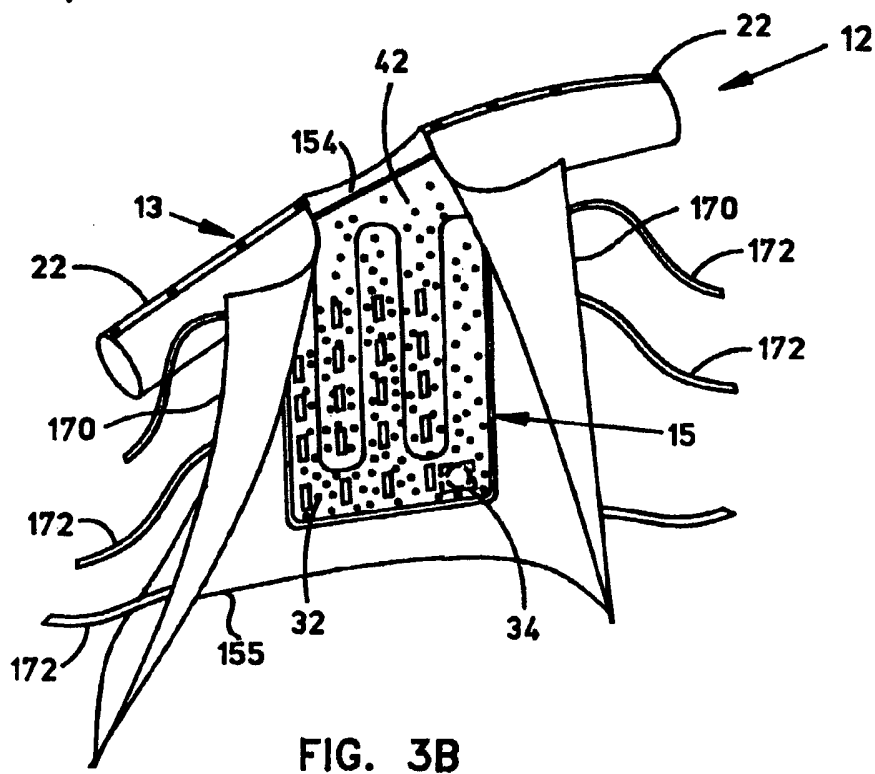
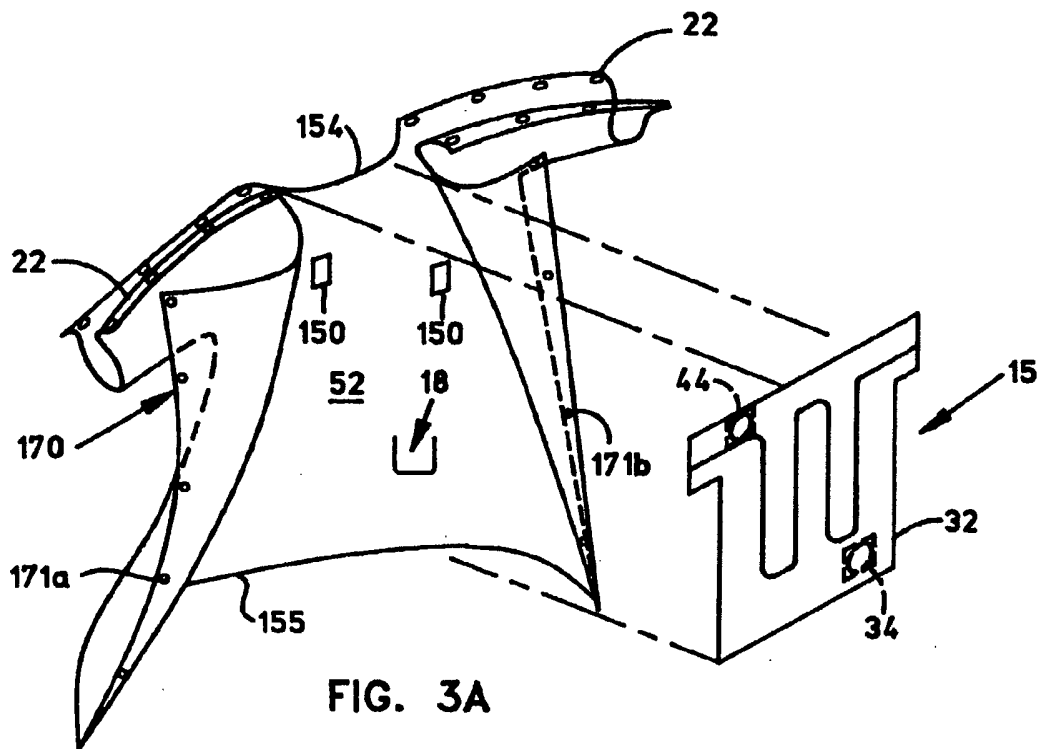
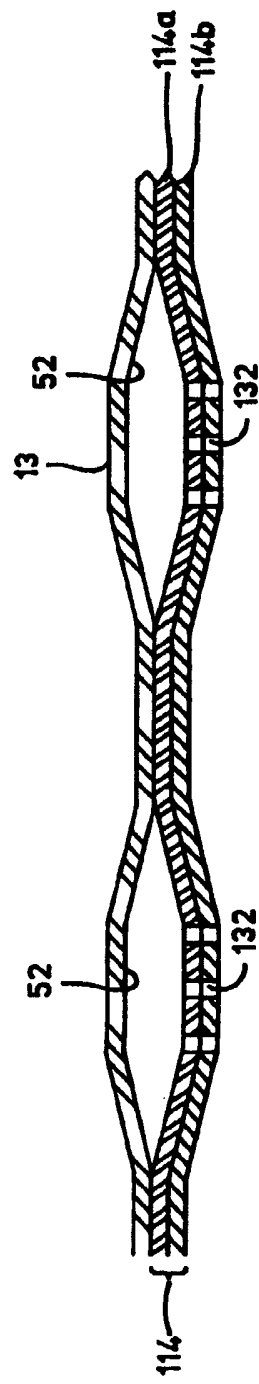
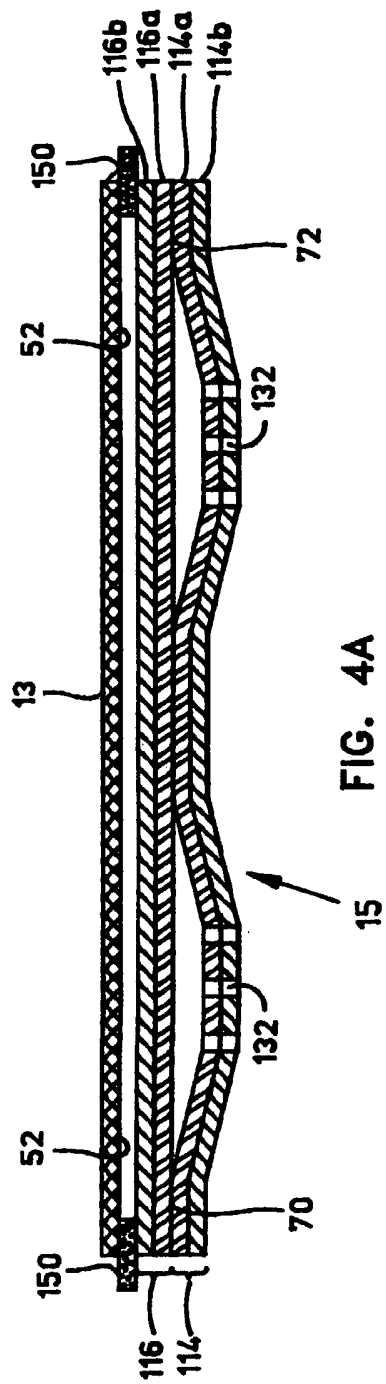


FIG. 2B





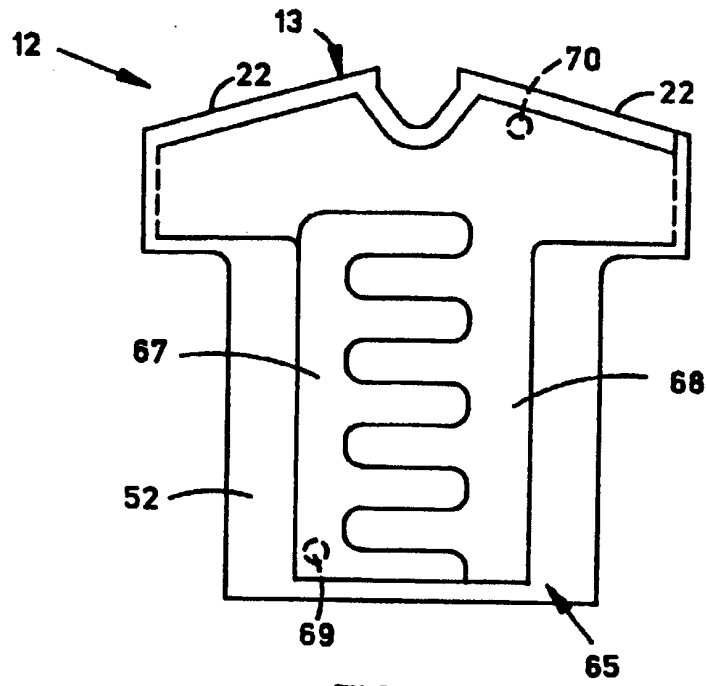


FIG. 5A

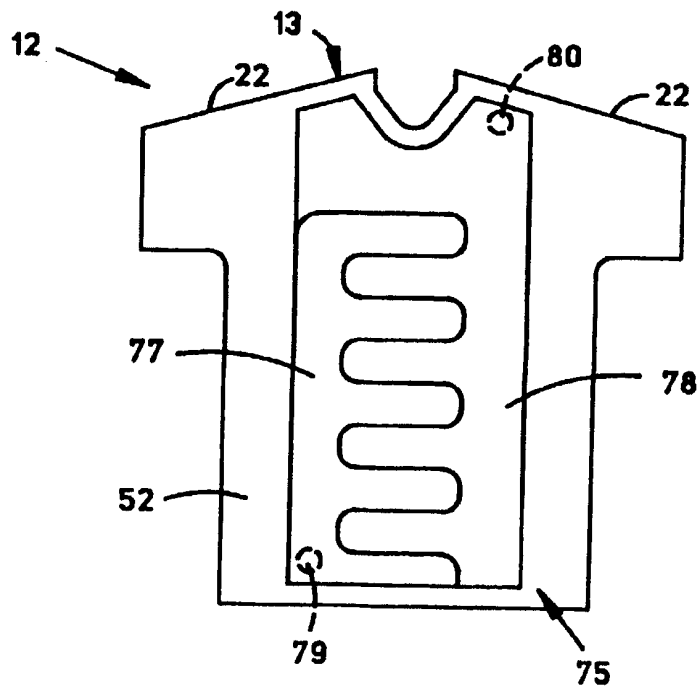


FIG. 5B

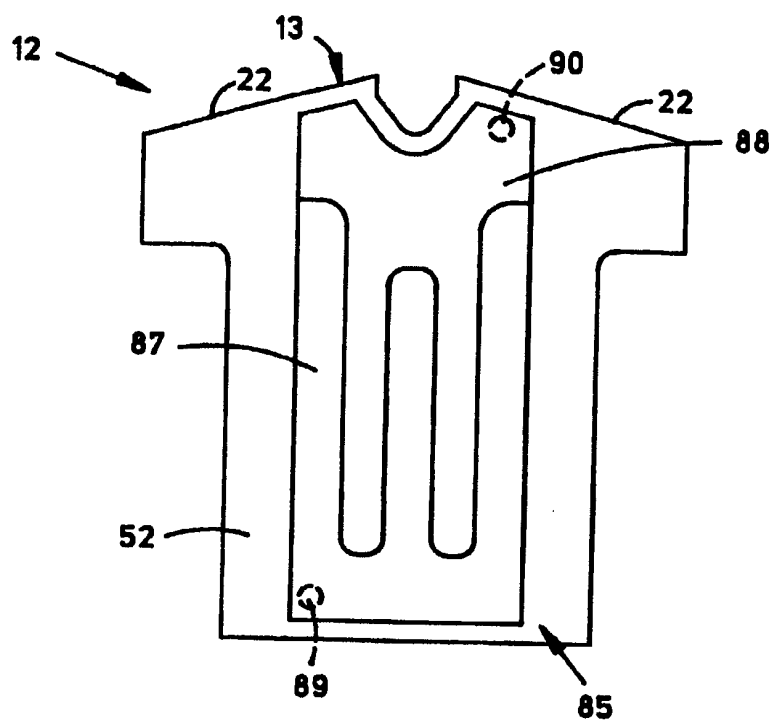


FIG. 5C

INTERNATIONAL SEARCH REPORT

International application No

PCT/US2005/044214

A. CLASSIFICATION OF SUBJECT MATTER

INV. A61F7/02

According to International Patent Classification (IPC) or to both national classification and IPC

B. FIELDS SEARCHED

Minimum documentation searched (classification system followed by classification symbols)

A61F

Documentation searched other than minimum documentation to the extent that such documents are included in the fields searched

Electronic data base consulted during the international search (name of data base and, where practical, search terms used)

EPO-Internal, WPI Data, PAJ

C. DOCUMENTS CONSIDERED TO BE RELEVANT

Category*	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
Y	WO 03/086500 A (ARIZANT HEALTHCARE INC; AUGUSTINE, SCOTT, D; ANDERSON, THOMAS, PETER;) 23 October 2003 (2003-10-23) cited in the application page 8, paragraph 3 - page 9, paragraph 1; figure 1a	1, 15
Y	WO 97/14381 A (MALLINCKRODT MEDICAL, INC) 24 April 1997 (1997-04-24) page 5, line 3 - line 17; figure 3	1, 15
A	US 6 524 332 B1 (AUGUSTINE SCOTT D ET AL) 25 February 2003 (2003-02-25) cited in the application abstract; figure 5	1, 15, 29
	----- -/--	

 Further documents are listed in the continuation of Box C. See patent family annex.

* Special categories of cited documents:

A document defining the general state of the art which is not considered to be of particular relevance

E earlier document but published on or after the international filing date

L document which may throw doubts on priority claim(s) or which is cited to establish the publication date of another citation or other special reason (as specified)

O document referring to an oral disclosure, use, exhibition or other means

P document published prior to the international filing date but later than the priority date claimed

T later document published after the international filing date or priority date and not in conflict with the application but cited to understand the principle or theory underlying the invention

X document of particular relevance; the claimed invention cannot be considered novel or cannot be considered to involve an inventive step when the document is taken alone

Y document of particular relevance; the claimed invention cannot be considered to involve an inventive step when the document is combined with one or more other such documents, such combination being obvious to a person skilled in the art.

Z document member of the same patent family

Date of the actual completion of the international search

10 April 2006

Date of mailing of the international search report

19/04/2006

Name and mailing address of the ISA/

European Patent Office, P.B. 5818 Patentlaan 2
NL - 2280 HV Rijswijk
Tel. (+31-70) 340-2040, Tx. 31 651 epo nl,
Fax: (+31-70) 340-3016

Authorized officer

Mayer-Martenson, E

INTERNATIONAL SEARCH REPORT

International application No
PCT/US2005/044214

C(Continuation). DOCUMENTS CONSIDERED TO BE RELEVANT

Category*	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
A	WO 2004/004500 A (MOELNLYCKE HEALTH CARE AB; MALMBERG, ANGELICA; RAUK BERGSTROEM, TINA;) 15 January 2004 (2004-01-15) abstract; figure 1 -----	1, 15, 29

INTERNATIONAL SEARCH REPORT

International application No.
PCT/US2005/044214

Box II Observations where certain claims were found unsearchable (Continuation of item 2 of first sheet)

This International Search Report has not been established in respect of certain claims under Article 17(2)(a) for the following reasons:

1. Claims Nos.: 34, 35
because they relate to subject matter not required to be searched by this Authority, namely:
Rule 39.1(iv) PCT - Method for treatment of the human or animal body by therapy
2. Claims Nos.:
because they relate to parts of the International Application that do not comply with the prescribed requirements to such an extent that no meaningful International Search can be carried out, specifically:
3. Claims Nos.:
because they are dependent claims and are not drafted in accordance with the second and third sentences of Rule 6.4(a).

Box III Observations where unity of invention is lacking (Continuation of item 3 of first sheet)

This International Searching Authority found multiple inventions in this international application, as follows:

1. As all required additional search fees were timely paid by the applicant, this International Search Report covers all searchable claims.
2. As all searchable claims could be searched without effort justifying an additional fee, this Authority did not invite payment of any additional fee.
3. As only some of the required additional search fees were timely paid by the applicant, this International Search Report covers only those claims for which fees were paid, specifically claims Nos.:
4. No required additional search fees were timely paid by the applicant. Consequently, this International Search Report is restricted to the invention first mentioned in the claims; it is covered by claims Nos.:

Remark on Protest

- The additional search fees were accompanied by the applicant's protest.
- No protest accompanied the payment of additional search fees.

INTERNATIONAL SEARCH REPORT

Information on patent family members

International application No

PCT/US2005/044214

Patent document cited in search report		Publication date	Patent family member(s)	Publication date
WO 03086500	A	23-10-2003	AU 2003223554 A1	27-10-2003
			CA 2480830 A1	23-10-2003
			EP 1494733 A2	12-01-2005
			JP 2005522591 T	28-07-2005
			MX PA04009700 A	11-01-2005

WO 9714381	A	24-04-1997	AT 247444 T	15-09-2003
			CA 2233669 A1	24-04-1997
			DE 69629577 D1	25-09-2003
			DE 69629577 T2	15-07-2004
			EP 0859579 A1	26-08-1998
			JP 11513279 T	16-11-1999

US 6524332	B1	25-02-2003	NONE	

WO 2004004500	A	15-01-2004	AU 2003243109 A1	23-01-2004
			BR 0312370 A	12-04-2005
			CA 2488098 A1	15-01-2004
			CN 1665413 A	07-09-2005
			EP 1524920 A1	27-04-2005
			MX PA04012027 A	07-03-2005
			SE 525415 C2	15-02-2005
			SE 0202079 A	04-01-2004
			US 2006047332 A1	02-03-2006
