

(12) STANDARD PATENT
(19) AUSTRALIAN PATENT OFFICE

(11) Application No. **AU 2013323538 B2**

- (54) Title
Medical device design, manufacture and testing systems
- (51) International Patent Classification(s)
G01N 33/50 (2006.01) **G01N 33/566** (2006.01)
- (21) Application No: **2013323538** (22) Date of Filing: **2013.09.26**
- (87) WIPO No: **WO14/052593**
- (30) Priority Data
- | | | |
|-------------------|-------------------|--------------|
| (31) Number | (32) Date | (33) Country |
| 61/705,650 | 2012.09.26 | US |
- (43) Publication Date: **2014.04.03**
(44) Accepted Journal Date: **2019.07.11**
- (71) Applicant(s)
Cook Biotech Incorporated;Muffin Incorporated
- (72) Inventor(s)
Ramachandran, Niraj;Fischer, Frank J.;Hiles, Michael C.;Fearnot, Neal E.
- (74) Agent / Attorney
Phillips Ormonde Fitzpatrick, L 16 333 Collins St, Melbourne, VIC, 3000, AU
- (56) Related Art
WO 2007076411 A1
US 20090253134 A1



- (51) International Patent Classification:
G01N 33/50 (2006.01) *G01N 33/566* (2006.01)
- (21) International Application Number:
PCT/US2013/061924
- (22) International Filing Date:
26 September 2013 (26.09.2013)
- (25) Filing Language: English
- (26) Publication Language: English
- (30) Priority Data:
61/705,650 26 September 2012 (26.09.2012) US
- (71) Applicants: **COOK BIOTECH INCORPORATED** [US/US]; 3055 Kent Avenue, West Lafayette, IN 47906 (US). **MUFFIN INCORPORATED** [US/US]; 1400 Cumberland Avenue, West Lafayette, IN 47906 (US).
- (72) Inventors: **RAMACHANDRAN, Niraj**; 354 Macbeth Drive, West Lafayette, IN 47906 (US). **FISCHER, Frank, J.**; 4901 South Old State Road 37, Bloomington, IN 47401 (US). **HILES, Michael, C.**; 3817 Cologne Court, Indianapolis, IN 46208 (US). **FEARNOT, Neal, E.**; 1311 E 500 N, West Lafayette, IN 47906 (US).
- (74) Agents: **GANDY, Kenneth, A.** et al.; Woodard, Emhardt, Moriarty, McNett & Henry LLP, 111 Monument Circle, Suite 3700, Indianapolis, IN 46204 (US).
- (81) Designated States (unless otherwise indicated, for every kind of national protection available): AE, AG, AL, AM,

AO, AT, AU, AZ, BA, BB, BG, BH, BN, BR, BW, BY, BZ, CA, CH, CL, CN, CO, CR, CU, CZ, DE, DK, DM, DO, DZ, EC, EE, EG, ES, FI, GB, GD, GE, GH, GM, GT, HN, HR, HU, ID, IL, IN, IS, JP, KE, KG, KN, KP, KR, KZ, LA, LC, LK, LR, LS, LT, LU, LY, MA, MD, ME, MG, MK, MN, MW, MX, MY, MZ, NA, NG, NI, NO, NZ, OM, PA, PE, PG, PH, PL, PT, QA, RO, RS, RU, RW, SA, SC, SD, SE, SG, SK, SL, SM, ST, SV, SY, TH, TJ, TM, TN, TR, TT, TZ, UA, UG, US, UZ, VC, VN, ZA, ZM, ZW.

- (84) Designated States (unless otherwise indicated, for every kind of regional protection available): ARIPO (BW, GH, GM, KE, LR, LS, MW, MZ, NA, RW, SD, SL, SZ, TZ, UG, ZM, ZW), Eurasian (AM, AZ, BY, KG, KZ, RU, TJ, TM), European (AL, AT, BE, BG, CH, CY, CZ, DE, DK, EE, ES, FI, FR, GB, GR, HR, HU, IE, IS, IT, LT, LU, LV, MC, MK, MT, NL, NO, PL, PT, RO, RS, SE, SI, SK, SM, TR), OAPI (BF, BJ, CF, CG, CI, CM, GA, GN, GQ, GW, KM, ML, MR, NE, SN, TD, TG).

Declarations under Rule 4.17:

- as to applicant's entitlement to apply for and be granted a patent (Rule 4.17(ii))
- as to the applicant's entitlement to claim the priority of the earlier application (Rule 4.17(iii))

Published:

- with international search report (Art. 21(3))

[Continued on next page]

(54) Title: MEDICAL DEVICE DESIGN, MANUFACTURE AND TESTING SYSTEMS

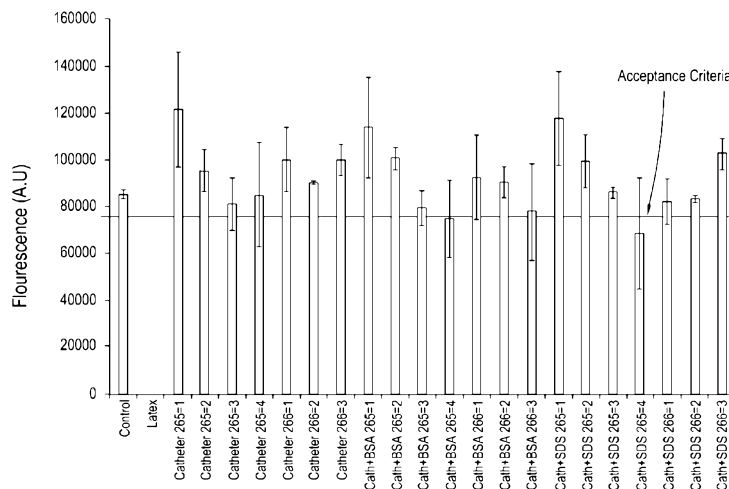


Fig. 6

(57) Abstract: Described are methods and systems for testing regions of medical devices, for example lumens of cannulated delivery components or assemblies thereof, that may be used to deliver cells to a patient or otherwise contact cells or cell preparations during use. Test cells are contacted with walls of the lumens or other device regions and/or liquids that contact walls of the lumens or other device regions, potentially over an incubation period. The test cells are then assessed for an effect of the wall contact, or the liquid contact, on at least one and preferably multiple characteristics of the test cells such as innate immune response, metabolic activity, viability, cytotoxic response, colony formation and/or motility. Methods and systems as described can be used in the development and/or manufacture of cannulated delivery devices or other medical device, for example providing specifications for design or process inputs or outputs, design or process validations, and/or device lot approvals. Also described are devices or products produced in accordance with such methods and systems.



- *before the expiration of the time limit for amending the claims and to be republished in the event of receipt of amendments (Rule 48.2(h))*

The discussion of the background to the invention included herein including reference to documents, acts, materials, devices, articles and the like is included to explain the context of the present invention. This is not to be taken as an admission or a suggestion that any of the material referred to was published,
5 known or part of the common general knowledge in Australia or in any other country as at the priority date of any of the claims.

BRIEF DESCRIPTION OF THE FIGURES

FIG. 1 provides a schematic diagram of one embodiment of a
10 manufacturing method of the invention.

FIG. 2 is a graph depicting activation/suppression of the NF-KB pathway through the TLR-2 receptor. HEK-293 cells transfected with TLR-2 receptors were cultured in the presence of negative (RPMI) and positive (PAM3CSK4) controls and in the presence of media that had been incubated in contact with
15 copper, polyvinylchloride (PVC) and the lumen of a Cook Advance 35LP balloon catheter, each shown as the average of four samples with three replicates each, taken from a first manufacturing lot identified herein as LOT 1, as described further in Example 1 below.

FIG. 3 is a graph depicting NF-KB activation/suppression levels in the
20 individual replicates from LOT 1 used to generate FIG. 2, as described further in Example 1 below.

FIG. 4 is a graph depicting activation/suppression of the NF-KB pathway through the TLR-2 receptor. HEK-293 cells transfected with TLR-2 receptors were cultured in the presence of negative (RPMI) and positive (PAM3CSK4)
25 controls and in the presence of media that had been incubated in contact with copper, polyvinylchloride (PVC) and the lumen of a Cook Advance 35LP balloon catheter, each shown as the average of four samples with three replicates each, taken from a second manufacturing lot identified herein as LOT 2, as described further in Example 1 below.

FIG. 5 is a graph depicting depicting NF-KB activation/suppression
30 levels in the individual replicates from LOT 2 used to generate FIG. 4, as described further in Example 1 below.

FIGs. 6 and 7 are graphs depicting the metabolic activity and total cytotoxic response of U937 cells after culture in the absence of applied condition (Control), in presence of media incubated in the presence of latex (used as a positive control), or in the presence of media incubated in the lumens of replicate 35 LP samples taken from LOT 1 and LOT 2 for purposes of metabolic activity and cytotoxicity testing (the replicate 35LP samples for this metabolic activity and cytotoxicity testing were new samples as opposed to re-used samples from TLR testing noted above; the incubated media from each 35LP replicate was split into separate aliquots and used for the separate assays).

SUMMARY

Embodiments of the invention relate to systems and methods by which medical devices are tested for their effect on viable cells, including for example for their effect on cellular characteristics related to the performance of the cells when introduced into a human or animal patient for a therapeutic purpose. The effect may in some embodiments relate to immune response, metabolic activity, viability (e.g. percent viable cells after an exposure), cytotoxic response, proliferation, activation down an undesirable pathway, capacity for colony formation, and/or migration. Sample test cells can be passed through a delivery passageway of a medical delivery device and collected, or otherwise caused to reside in the presence of and/or contact a surface of a medical device and collected. The collected cells can then be assayed to determine characteristics of the cells. The results from the collected cells can be compared to corresponding results from control cells, to determine a potential impact(s) of the medical delivery device or other medical device on the cells. These methods can be used as a part of a medical device or process design or validation, and/or as a part of device lot approval. In certain embodiments the cell-based testing can be conducted on a medical delivery device that is a component assembly including at least first and second delivery components associated with one another to form the cell delivery passageway. In this fashion, the entire delivery passageway to be used by the end user can be assessed for its affect on the cells, rather than or in addition to separately assessing the component passageways. This can be used to account for

potential differences in cellular effect that may occur between separate component exposure and entire passageway exposure. These differences may for example be due to contact with differing materials or surface features, connection regions between the components, or fluid stresses during flow through the entire delivery passageway.

Viewed from one aspect of the present invention, there is provided a method for testing a lumen of a medical device for a potential effect of the lumen on cells delivered through the lumen, the lumen being for delivery of cell-containing flowable materials, the method comprising the steps of: incubating a liquid medium in contact with a wall of the lumen during a residence time of the liquid medium within the lumen ; contacting at least one cell with the liquid medium; collecting the liquid medium from the lumen after said incubating; and assessing the effect of said contacting on expression of at least one toll-like receptor by the cell.

Viewed from another aspect of the present invention, there is provided a method for testing a lumen of a medical device for a potential effect of the lumen on cells delivered through the lumen, the method comprising the steps of: first assessing the lumen for an effect on innate immune response of a cell, the first assessing including incubating a liquid medium in contact with a wall of the lumen during a residence time of the liquid medium within the lumen, collecting the liquid medium from the lumen after said incubating, contacting the cell with the liquid medium, and assessing the effect of said contacting on an innate immune response of the cell; and second assessing lumen region for an effect on at least one other characteristic of a cell, said at least one other characteristic selected a group including from cytotoxicity, motility, viability, metabolic activity or any combination thereof, and said second assessing including incubating a liquid medium in contact with a wall of the lumen during a residence time of the liquid medium within the lumen, collecting the liquid medium from the lumen after said incubating, contacting the cell with the liquid medium, and assessing the effect of said contacting on said at least one other characteristic of the cell.

Viewed from another aspect of the present invention, there is provided a method for assessing a lumen of a medical device for a potential effect of the

lumen on cells delivered through the lumen, the method comprising the steps of:
contacting at least one cell with a liquid medium that has been incubated in contact
with a wall of the lumen during a residence time of the liquid medium within the
lumen; collecting the liquid medium from the lumen after said contacting; and
5 assessing the effect of said contacting on at least one characteristic of the at least
one cell.

Viewed from another aspect of the present invention, there is provided a
method for testing components of an assembly, the method comprising the steps
of: incubating a liquid medium in contact with a wall of a passageway of a sample
10 assembly during a residence time of the liquid medium within the passageway, the
sample assembly including a sample first component having a first lumen coupled
to a sample second component having a second lumen to form the passageway, the
passageway including the first lumen and the second lumen; contacting at least one
cell with the liquid medium; collecting the liquid medium from the passageway
15 after said incubating; and assessing the effect of said contacting on at least one
characteristic of the cell.

Viewed from another aspect of the present invention, there is provided a
kit manufacturing method, the method comprising the steps of: manufacturing a
first device lot including a plurality of units of a first delivery component each
20 having a first lumen for passage of cells; manufacturing a second device lot
including a plurality of units of a second delivery component each having a second
lumen for passage of cells, wherein the first delivery component is associable with
the second delivery component to provide a delivery assembly having a
passageway for passing cells, the passageway including the first lumen and second
25 lumen; sampling the first device lot to obtain first test sample units of the first
delivery component; sampling the second device lot to obtain second test sample
units of the second delivery component; associating one of said first test sample
units with one of said second sample units to provide a sample delivery assembly
having a passageway including the first lumen of the first test sample unit and the
30 second lumen of the second sample unit; assessing the passageway for an effect on
at least one characteristic of a cell, said assessing the passageway including placing
a liquid medium in contact with a wall of the passageway during a residence time

of the liquid medium within the passageway, contacting at least one cell with the liquid medium, collecting the liquid medium from the passageway after said placing, and assessing the effect of said contacting on at least one characteristic of the cell; and packaging first delivery components from the first device lot with
5 second delivery components from the second device lot.

Additional embodiments as well as features and advantages associated therewith will be apparent from the descriptions herein.

Where the terms "comprise", "comprises", "comprised" or "comprising" are used in this specification (including the claims) they are to be interpreted as
10 specifying the presence of the stated features, integers, steps or components, but not precluding the presence of one or more other features, integers, steps or components, or group thereof.

DETAILED DESCRIPTION

For the purpose of promoting an understanding of the principles of the invention, reference will now be made to embodiments, some of which are illustrated in the drawings, and specific language will be used to describe the same.

5 It will nevertheless be understood that no limitation of the scope of the invention is thereby intended. Any alterations and further modifications in the described embodiments, and any further applications of the principles of the invention as described herein are contemplated as would normally occur to one skilled in the art to which the invention relates.

10 As disclosed above, aspects of the present invention relate to methods and systems for testing delivery pathways of medical delivery devices (e.g. as individual components or assemblies) that may be used to deliver cells to a patient and/or for testing other regions or surfaces of a medical device to which cells will be exposed, for example by contact or residence in proximity. In certain

15 embodiments, test cells are contacted with walls of the lumens or other surfaces of a medical device and/or liquid mediums that have contacted walls of the lumens or other surfaces of a medical device, potentially over an incubation period. The test cells are then assessed for an effect of the wall or other surface contact, or the liquid medium contact, on at least one and preferably multiple characteristics of the

20 test cells. The effect may in some embodiments pertain to immune response, metabolic activity, viability, cytotoxic response, proliferation, and/or migration. Methods and systems as described can be used in the development, manufacture and/or distribution of cannulated delivery devices or other medical devices, for example providing specifications for product design or process inputs, product

25 design or process validations, and/or device lot release criteria. Also described are devices or products produced in accordance with such methods and systems, and methods for distributing the same.

Embodiments herein are useful for testing medical devices. In particular

30 embodiments, medical delivery devices defining lumens or other pathways for the delivery of flowable materials, and especially cell-containing flowable materials such as liquids, gels or pastes, can be tested. Such delivery devices or other medical devices to be tested can be a single piece or can be an assembly of

multiple pieces. The delivery device or devices may include one or more of a catheter having a lumen to be tested, a catheter hub having a lumen to be tested, a needle having a lumen to be tested, a needle hub having a lumen to be tested, and a syringe having a barrel to be tested. The catheter may have an expandable portion, for example as embodied in a balloon catheter. Some or all of these devices can be interconnectable with each other or with other devices, and can have adaptations for the same. Illustratively, these devices may be configured for threaded connection to one another, such as in a standard lure-lock mechanism, press-fit or other friction fit to one another, or any other suitable connection mechanism to form an assembly that provides an overall pathway for delivery of the flowable material or another device region that may contact, pass or hold a cell preparation. Still other medical devices that can be tested include, for example, devices for storing or otherwise holding cells such as bags or vials. For example, the interior regions of such devices configured to store or otherwise hold cells can be tested in accordance with the disclosures herein.

The medical delivery device or other medical device component(s) can be made to include any suitable material or combination of materials. Polymeric materials and metal materials are typically incorporated in such devices. Suitable polymeric materials include, for example, cellulose acetate, cellulose nitrate, silicone, cross-linked polyvinyl alcohol (PVA), polyurethane, polyamide, styrene isobutylene-styrene block copolymer (Kraton), polyethylene terephthalate, polyester, polyorthoester, polyanhydride, polyether sulfone, polycarbonate, polypropylene, high molecular weight polyethylene, polytetrafluoroethylene, polyesters, polylactic acid or polyglycolic acid or copolymers thereof, polyanhydride, polycaprolactone, polyhydroxybutyrate valerate, or other biodegradable polymer, or mixtures or copolymers of any of these identified polymers. Suitable metals include stainless steel, nitinol, MP35N, gold, tantalum, platinum or platinum iridium, niobium, tungsten, iconel, nickel, titanium, stainless steel/titanium composites, cobalt, chromium, cobalt/chromium alloys, magnesium, aluminum, or other biocompatible metals and/or composites or alloys thereof. The walls of the medical device lumen or other delivery pathway may include any one or combination of these, or other, suitable materials.

In accordance with aspects of the invention, a sample is prepared for testing by contacting the sample in some manner with a wall or walls of a medical device, for example a wall or walls defining a medical device delivery pathway or other medical device region expected to contact cells or a cellular preparation during use.

5 In some embodiments, the sample material will contain cells as it is contacted with the walls of the pathway or other medical device region. The contact of such a cellular preparation with the pathway or other medical device region may be for any suitable incubation time and in some aspects will be for an incubation time longer than that which is expected from a typical or worst case use of the delivery

10 pathway or other medical device region. This can assist in incorporating a safety factor in testing the pathway or other region. Incubation of the sample in contact with the walls of the pathway or other region may be done under static conditions, flow conditions, or both. Examples of static contact strategies may be found when testing for the sensitivity of the cells to a material of construction of the walls of

15 the pathway or other region, e.g. a polymeric material, and/or to any materials that may leach from such a material of construction. Examples in which a flowing contact of the cellular preparation with the pathway or other region include those noted immediately above as well as testing for the tendency of cells to adhere to the pathway walls or other walls under flow conditions, as might affect the number

20 or dose of cells finally delivered out of the pathway and into a patient or to otherwise remain unadhered to a device region. When flow conditions are used, worst case testing can be performed. This may include a worst case slow-flow testing, at a flow rate that is the lowest expected flow rate that would be employed clinically in use of the delivery pathway or other device region. For cells that may

25 tend to adhere to the pathway walls or other region walls, this may be incorporated into testing related to the released dose of cells from the pathway or other region of the medical device. Worst case high-flow testing may be conducted at a flow rate at or exceeding the maximum flow rate that would be expected to be applied during clinical use of the pathway or region. Because cells can be sensitive to

30 shear forces and other forces that may be generated during high rates of flow, this worst case testing may for example be used in testing for any impact of the

delivery pathway or other device region on the performance characteristics of the cells once released from the pathway or other region.

As noted above, the delivery pathway or other region that is tested may be defined from a single device, or a combination of devices provided in assembly
5 form. In such assemblies, lumens or passages or regions in each of the devices will typically fluidly couple to another to form an overall lumen or passageway or region. The physical parameters of such overall passageways or regions are determined not only by each individual passageway of the respective coupled devices, but also the regions for coupling and any gaps, ledges, changes in
10 diameter, or other physical variations that occur at the coupling regions of the devices. These potential irregularities at coupling regions may, for example, affect the tendency of cells to be retained within the pathway or other region even under anticipated deliver conditions e.g. by being trapped or adhered within irregularities in the pathway or region surface, and may also affect flow conditions to which the
15 cells are exposed. In certain embodiments, the pathway or other region is defined by an assembly that includes at least two of a syringe barrel, a catheter, and a needle, and potentially all three of these components. It will be understood that still other delivery devices or device components may be used either alone or in assemblies. Additionally, in certain embodiments the delivery pathway or other
20 region defined by the device or assembly of devices can be manipulated in a manner that would be expected during clinical use. This manipulation may for example include contact with another device, for example a guide wire, physically positioning the delivery pathway to an expected shape, e.g. a tortuous shape, expected during clinical use, or exposure of the pathway or other region to
25 materials or media expected during clinical use, for example exposure to blood or blood fractions in order to condition the delivery pathway with biological components as expected in use in a patient, prior to contact of the pathway or other region with the test cells.

The delivery pathway or other region testing will be conducted at a suitable
30 temperature for the test undertaken. The pathway or other region may be cooled, heated, or retained at room temperature (e.g. about 22-25°C) during the contact of the sample to be developed for testing with the pathway or other region. Where

cellular preparations are comprised in the sample, some tests will undertake the contacting step at about physiologic temperature (about 37°C) and/or for a suitable contact time, for example about 10 minutes to 5 hours, or about 30 minutes to about 3 hours. Any suitable arrangement for heating the delivery pathway or other region to such temperature may be used, including for example incubators or water
5 baths. For other sample contacts, e.g. in the absence of cells to develop the sample, temperatures lower than physiologic temperature, for example room temperature or cool temperatures, may sometimes be used.

In certain embodiments of the invention, a sample in the absence of cells is
10 contacted with the delivery pathway or other device region. This sample can be constituted of cell culture medium. As noted above, the conditions of sample contact may be under flow, static, or combined flow and static conditions. Advantageously, in developing samples for testing in the absence of cells, long residence times within the delivery pathway or other region can be utilized, e.g. to
15 provide ample safety factor in the testing regimen.

The sample residence time in the absence of cells can vary. In certain embodiments, the sample residence time will be at least about 30 minutes, at least about 1 hour, or at least about 2 hours, for example in the range of about 30 minutes to about 48 hours, or about 1 hour to about 24 hours, or about 1 hour to 5 hours. In
20 some aspects, the sample residence time in the absence of cells will exceed about 10 hours, for example in the range of about 10 hours to 48 hours. This incubation time can be sufficient to condition the sample with any impurities or other leach aids that may be released by the delivery pathway and the walls defining it, to which the cells may be sensitive. After the cell-free sample is conditioned in this manner, it can be
25 collected from the delivery pathway for subsequent use in testing in contact with test cells. In this regard, for such cell-free samples or for cell-containing samples are discussed above, the sample volume collected from the delivery pathway can in some aspects be sufficiently large that it can be split into multiple aliquots and used in multiple tests which are the same or of differing nature.

30 Samples developed as discussed above or suitably otherwise will be assayed to determine whether the delivery pathway may have an affect on cells. A wide variety of cellular characteristic may be tested, including for example metabolic

activity, viability, motility, proliferation, colony formation, or immune affects including for instance innate or adaptive immune affects. A variety of tests for these or other cell characteristics are known and can be used. The assays for affect on cells may be qualitative or quantitative in nature, and may for example assay for the
5 expression of proteins or transcription of DNA elements. Such expression or transcription assays may test for a selected one or group of proteins or DNA elements, or may in some instances involve an entire expression or transcription profile for the cells. Such assays may utilize intact cells (e.g. in florescence activated cell sorting), or may utilize cellular extracts such as those prepared in
10 expression or transcription testing. Additionally, in dose testing, cell counts or estimates can be provided before and after passing a cellular preparation through the delivery pathway, in order to determine any loss of cell count experienced during passage through the delivery pathway.

Each of these tests or other determinative tests can and typically will utilize
15 a suitable control, as is well known in the art. Controls may be positive controls, negative or null controls.

The test methods described herein may be used for a wide variety of device design, development or manufacturing purposes. Illustratively, in device design, one or more of the tests described herein may be used in the selection and testing
20 of physical and/or materials of construction parameters for an intended delivery device. In these respects, tests described herein may be used as design or validation inputs. As well, during device development, tests as described herein may be used as specifications for design inputs or validation for devices or manufacturing processes therefor. Still further, tests as described herein may be
25 used during manufacture of devices for commercial distribution. In one aspect, tests as described herein can be used as lot release criteria. In such embodiments, manufactured lots of devices can be isolated or quarantined until tests as described herein, designated as lot release criteria, are completed. Upon passage of the tests, the devices can be released for distribution and distributed to end users.

30 With reference now to Figure 1, disclosed is one embodiment of a kit manufacturing method of the invention. In the method a manufactured lot 16 of kits is to be produced. To do so, a first lot 12 of a first component of a delivery

assembly is made, along with lot 13 and lot 14 of second and third components of the delivery assembly, respectively, are manufactured. Sample components 12a–12c are taken from lot 12, sample components 13a–13c are taken from lot 13, and sample components 14a–14c are taken from lot 14. These samples are paired each
5 with one of the samples from the other lots to create sample delivery assemblies 121314a, 121314b, and 121314c. These respective sample assemblies are subjected respectively to test A, test B, and test C as shown. These tests may for example be part of a lot release requirement for manufactured kits in lot 16. Test A, test B and test C can include any one or combination of the cell-related tests as
10 described herein. Further, in addition to testing sample assemblies as disclosed, individual devices from lots 12, 13 and 14 may be tested singly. If the sample assemblies 121314a-c pass tests a, b and c respectively, as at determination step 15, then devices 12d-l from lot 12, devices 13d-l from lot 13, and devices 14d-l from lot 14 can be packaged as shown with packaging 17 and optionally terminally
15 sterilized. In an additional potential sampling step, samples of kits from kit lot 16 may be taken, opened and the respective components combined to make additional sample assemblies, which can be subjected to cell-related testing using any one or combination of those methods described herein. Thereafter, kits from lot 16 can be released for distribution to end users.

20 Any one or any combination of a wide variety of cell types can be used in samples for test methods of the invention and/or as the target cell type for delivery from the medical delivery device. For example, the cells can be skin cells, skeletal muscle cells, cardiac muscle cells, lung cells, mesentery cells, or adipose cells. The adipose cells may be from omental fat, properitoneal fat, perirenal fat,
25 pericardial fat, subcutaneous fat, breast fat, or epididymal fat. In certain embodiments, the cells comprise stromal cells, stem cells, or combinations thereof. As used herein, the term "stem cells" is used in a broad sense and includes traditional stem cells, adipose derived stem cells, progenitor cells, preprogenitor cells, reserve cells, and the like. Exemplary stem cells include embryonic stem
30 cells, adult stem cells, pluripotent stem cells, neural stem cells, liver stem cells, muscle stem cells, muscle precursor stem cells, endothelial progenitor cells, bone marrow stem cells, chondrogenic stem cells, lymphoid stem cells, mesenchymal

stem cells, hematopoietic stem cells, central nervous system stem cells, peripheral nervous system stem cells, and the like. Additional illustrative cells which can be used include hepatocytes, epithelial cells, Kupffer cells, fibroblasts, human embryonic kidney cells, neurons, cardiomyocytes, myocytes, chondrocytes, 5 pancreatic acinar cells, islets of Langerhans, osteocytes, myoblasts, satellite cells, endothelial cells, adipocytes, preadipocytes, biliary epithelial cells, and progenitor cells of any of these cell types.

Mixtures of any of the cells identified herein, or other mixtures, may also be utilized. In certain embodiments, naturally-occurring cellular mixtures, or 10 fractions thereof, are used. Examples of these embodiments include the use of peripheral blood or fractions thereof, bone marrow or fractions thereof, umbilical cord blood or fractions thereof, and the like.

In some embodiments, the cells are, or include, endothelial progenitor cells (EPCs). Preferred EPCs for use in the invention are endothelial colony forming 15 cells (ECFCs), especially ECFCs with high proliferative potential. Suitable such cells are described for example in U.S. Patent Application Publication No. 20050266556 published December 1, 2005, publishing U.S. Patent Application Serial No. 11/055,182 filed February 9, 2005, and U.S. Patent Application Publication No. 20080025956 published January 1, 2008, publishing U.S. Patent 20 Application No. 11/837,999, filed August 13, 2007, each of which is hereby incorporated by reference in its entirety. Such ECFC cells can be a clonal population, and/or can be obtained from umbilical cord blood of humans or other animals. Additionally or alternatively, the endothelial colony forming cells have the following characteristics: (a) express the cell surface antigens CD31, CD105, 25 CD146, and CD144; and/or (b) do not express CD45 and CD14; and/or (c) ingest acetylated LDL; and/or (d) replating into at least secondary colonies of at least 2000 cells when plated from a single cell; and/or (e) express high levels of telomerase, at least 34% of that expressed by HeLa cells; and/or (f) exhibit a nuclear to cytoplasmic ratio that is greater than 0.8; and/or (g) have cell diameters of less than 30 about 22 microns. Any combination of some or all of these features (a)-(g) may characterize ECFCs used in the present invention.

In other embodiments, the cells are, or include, muscle derived cells, including muscle derived myoblasts and/or muscle derived stem cells. Suitable such stem cells and methods for obtaining them are described, for example, in U.S. Patent No. 6,866,842 and U.S. Patent No. 7,155,417, each of which is hereby
5 incorporated herein by reference in its entirety. The muscle derived cells can express desmin, M-cadherin, MyoD, myogenin, CD34, and/or Bcl-2, and can lack expression of CD45 or c-Kit cell markers.

In still other embodiments, the cells are, or include, stem cells derived from adipose tissue. Suitable such cells and methods for obtaining them are described
10 for example in U.S. Patent No. 6,777,231 and U.S. Patent No. 7,595,043, each of which is hereby incorporated herein by reference in its entirety. The cellular population can include adipose-derived stem and regenerative cells, sometimes also referred to as stromal vascular fraction cells, which can be a mixed population including stem cells, endothelial progenitor cells, leukocytes, endothelial cells, and
15 vascular smooth muscle cells, which can be adult-derived. In certain forms, the cells can include adipose-derived cells that can differentiate into two or more of a bone cell, a cartilage cell, a nerve cell, or a muscle cell.

The cells to be used in testing can either be genetically unmodified or genetically modified cells. Genetically modified cells can include cells that have
20 been modified to contain expressible DNA that encodes a protein or other substance of interest. The cells can then be used in tests to determine whether the cell delivery passageway has any effect (including e.g. suppression or activation) on the expression of the protein or other substance of interest. Illustratively, cells can be genetically modified by transfection or otherwise to contain exogenous
25 DNA encoding proteins or other substances that are involved in immune response, for example toll-like receptors (TLRs), such as TLR-2, TLR-4, or TLR-7. These TLR-modified cells can then be used in testing as described herein to determine whether the delivery passageway has an effect on TLR expression by the cells.

In certain embodiments, a medical delivery device delivery pathway or
30 other medical device region, which can be a single component or an assembly as described herein, will be tested in the presence of multiple different cells types or preparations, e.g. any of those disclosed herein, for example two or more, or three

or more different cell types or preparations. In addition, as to each different cell type or cell preparation type, the affect of the medical delivery device delivery pathway or other medical device region on multiple characteristics (e.g. two or more, or three or more characteristics) of the cells, e.g. any of those disclosed
5 herein, can be tested.

For the purpose of promoting a further understanding of aspects of the present invention, the following Examples are provided. It will be understood that these Examples are illustrative, and not limiting, in nature.

10

Example 1

Innate Immune Response Assay

This Example describes cell based assays for assessment of catheter lumens for their effect on cellular innate immune response. Specifically herein,
15 genetically modified cells expressing TLR2 and TLR4 were used to assess catheter lumens for their potential to activate or suppress TLR2 or TLR4 expression in the cells.

Materials

20 Human Embryonic Kidney 293 (HEK-293) cells stably transfected with different TLR plasmids -2, -4, or -7 (TLR4 cells were also co-transfected with CD14 and MD-2) were obtained from InvivoGen (San Diego, California 92121)

Cook Advance 35 LP catheters were obtained from Cook Medical, Bloomington, Indiana.

25 Culture media for the HEK-293 cells was obtained from InvivoGen (San Diego, California 92121).

Other test materials used as positive controls were tubing's of Copper and PVC. The copper tubing used was a 1/8" thick, soft refrigeration tubing bought from Kleindorfer's Hardware Store in Bloomington IN (Manufacturer: Cambridge-
30 Lee Industries, Inc., Manufacturers Notice: Cleaned per ASTM B280 and NFPA 99). The PVC tubing was an 8.0 FR White manufactured by Cook Polymer Technology (Material Compound # 11011, Cook Polymer Project # D-4520, Year

Extruded: 2000). DMEM (negative control) was obtained from Invivogen, and PAM3CSK4 (positive control) was obtained from Imgenex.

Methods

5 Test Media: HEK-293 cell culture medium was incubated in contact with the 35 LP catheters and other test materials for 16 hours at room temperature (20-22 °C). For the 35 LP catheters, which were taken from a first device lot designated LOT 1, the guide wire lumen was filled completely with a volume of approximately 1mL of the culture medium for the incubation period. For the other
10 samples, the volume varied due to inner diameter and length of the copper (2 ml) and PVC (1.2 ml) tubes but the incubation times and temperature remained the same.(describe the incubation process). After the incubation period, the conditioned samples of culture media were collected in FACS tubes and were either for prompt use in the cellular assays.

15 Cell Culture: HEK-293, TLR-2 transfected cells were plated at a concentration of 40,000 cells/well while the TLR4 transfected cells were plated at a concentration of 10,000 cells/well in separate 96 well plates. Specific media supplements were added to each cell line as directed by the cell line vendor's literature. All cytotoxicity indicator cells were incubated for 24 hours in the cell
20 culture incubator (5% CO₂, 37° C). Following this incubation period, the cell culture media was removed and replaced with the device- exposed-media. Normal cell culture media was used as a negative control. Pam3CSK4 (10ng) and LPS (100ug) were used as a positive controls for TLR2 and TLR4 transfected cells respectively.

25 NFkb Activation/Suppression Assay: Following a 24-hour incubation period in the device or positive control modified cell culture media, a 15µL aliquot of the cell culture supernatants was added to a 96 well microtiter plate containing 185µL/well volume of Quick-Blue developer substrate. This substrate is used to
30 quantitate the levels of secreted embryonic alkaline phosphatase (SEAP) enzyme activity. TLR cell lines secrete an embryonic AP enzyme form at varying levels dependent upon the amount of TLR associated signal transduction occurring as a result of the interaction of the TLR receptor with contaminants leached from

devices. Activation of both the AP-1 and NF-kB proteins by the surface stimulation of the TLR type receptors leads to AP-1 and NF-kB binding to their specific binding sites on the promoter region controlling the transcription of the SEAP reporter gene. This leads to an increase in the production and export of the SEAP enzyme into the cell culture media.

AP substrate development reactions were allowed to proceed for 3 hours at 37° C in the CO₂ incubator. The presence of AP associated substrate color development was assessed using a Molecular Devices Spectra Max 250 colorimetric plate reader set to read absorbance at OD₆₅₅. After removing this initial 15µL of cell culture supernatant from the TLR cell cultures, the cell culture plates were placed back into the incubator for additional 24-hours to allow us to secure a 48-hour time point too. At this time, another 15 µL aliquot of cell culture supernatant was removed from the respective TLR cell cultures and added to another 96 well micro titer plate containing 185 µL/well of Quick-Blue AP developer substrate. This substrate reaction was subsequently incubated for 3 hours at 37° C in the CO₂ incubator. The Quick-Blue AP developer substrate was again read at OD₆₅₀ on the Molecular Devices Spectra Max 250 colorimetric plate reader to quantitate the relative levels of SEAP production. Again, the level of SEAP reporter enzyme secretion is correlated with the degree of TLR type receptor stimulation by leached device-tubing contaminants. The results are shown in Figs. 1-2 (TLR2 testing) and Figs. 3-4 (TLR4 testing). As shown in Figs. 1-2, which show averaged and individual replicate values, respectively, TLR2 was activated in the positive control (PAM3CSK4) relative to the negative control (RPMI). In the test articles, copper-, PVC- and 35LP-conditioned media samples all suppressed TLR2 relative to the negative control, with the 35LP-conditioned samples suppressing to a lower extent than copper and PVC.

The results for TLR4 shown in Figs. 3-4 were similar to those for TLR2. TLR4 was activated in the positive control (LPS) relative to the negative control (RPMI). In the test articles, copper-, PVC- and 35LP-conditioned media samples all suppressed TLR4 relative to the negative control, with the 35LP-conditioned samples suppressing to a lower extent than copper and PVC.

Example 2

Metabolic Activity and Cytotoxicity Assays

This Example describes cell based assays for assessment of catheter lumens
5 for their effect on the metabolic activity of cells or for potential cytotoxicity to
cells. Specifically herein, U937 cells were used for these purposes.

Materials

U937 cells were obtained from ATCC (ATCC CRL-1593.2).

10 Cook Advance 35 LP balloon catheters from two different device lots
(designated LOT 1 and LOT 2) were obtained from Cook Medical, Bloomington,
Indiana.

Culture media for the U937 cells was obtained from ATCC. ATCC
complete growth medium was prepared for culturing these cells by adding a total
15 concentration of 10% fetal bovine serum to ATCC formulated RPMI-1640
medium (Cat # 30-2001) and 100 units/mL penicillin and 100 µg/mL streptomycin.
The cells were cultured in 95% air, 5%CO₂ in a humidified atmosphere at 37°C.

Latex tubing (positive control) was commercially obtained.

20 Methods

Test Media: Approximately 1mL of theU937 cell culture medium was
incubated in contact with the 35 LP catheters and the latex (positive control) for
_48 hours at human physiologic temperature (37 °C). For the 35 LP catheters, the
guidewire lumen of each catheter was filled completely by injecting a volume of
25 about 1mL of the culture medium into the lumen, after which the lumen was
clamped off at each end with parafilm and the catheter incubated in a 37 °C
incubator for 48hours. After the incubation period, the conditioned samples of
culture media were collected in 15 ml conical tubes, for prompt use in the
metabolic activity and cytotoxicity assays.

30 Initial Cell Culture: U937 cells were cultured at passage 7 or 8 in T75 cell
culture flasks at approximately 5 X 10⁵ cells per mL. After aspirating the cells into
a 50 ml conical tube they were centrifuged at 300xg for 5 minutes at room

temperature. Following this the supernatant was removed and the pellet was resuspended in fresh media to give a cell concentration of 1×10^6 cells/mL. An aliquot that gave 1×10^6 cells was aspirated into a 12x75mm polystyrene tube with a cap and the tubes were centrifuged at 300xg for 5 minutes at room temperature.

5 The media was aspirated following centrifugation and tubes were racked to loosen the pellet. One mL of either the device exposed or latex tube exposed treatment media was added to the pellet in their respective tubes whereas untreated media was added to the control tubes and the tubes for staurosporine. The cells were then transferred to a 24 well plate for an incubation period of about 5 hours after which

10 the 2 different assays were performed.

Presto Blue Assay: The Presto Blue assay (metabolic activity) was set to be read at 5 hours after the staurosporine was added to its well. Using cells from the control wells a standard curve was made with cell culture media: media alone (blank); 31,300; 62,500; 125,000; 250,000 and 500,000 cells. 90 μ l of each

15 standard and treatment groups were placed in triplicate, in a 96 well plate followed by addition of 10 μ l of the Presto Blue reagent to every well. The plate was covered and placed into a 37°C incubator for 30 minutes. The plate was read on a fluorescence plate reader following this incubation.

Cell Viability/Cytotoxicity Assay: 200 μ l of cells from each treatment well

20 were pipetted into a 12x75mm polystyrene tube with a cap, in duplicate. FAM-FLICA an apoptosis detection probe was diluted with DMSO to a 150X stock concentrate solution. Prior to use a 1:7.5 dilution was prepared to obtain a 20X working solution. About 10 μ l of this working solution was added to each tube except the unstained cells following which the tubes were left to incubate at 37°C

25 for 45 minutes. 2 mL of a 1% BSA in PBS solution was added to each tube including unstained after the incubation period. The tubes were then centrifuged at 300xg for 5 minutes at room temperature. Aspiration of the media followed and the tubes were racked to loosen the pellet. The above steps were repeated for a second wash. Finally 200 micro liters of a 1% BSA in PBS solution was added to

30 each tube including unstained and set on ice prior to reading.

The results are shown in Figures 6 (metabolic activity) and 7 (cytotoxicity), which demonstrate that the assays conducted and modifications thereof will be

suitable for the assessment of catheter lumens for their effect on the metabolic activity of cells or for potential cytotoxicity to cells relative to selected acceptance criteria.

5 The uses of the terms "a" and "an" and "the" and similar references in the context of describing the invention (especially in the context of the following claims) are to be construed to cover both the singular and the plural, unless otherwise indicated herein or clearly contradicted by context. Recitation of ranges of values herein are merely intended to serve as a shorthand method of referring
10 individually to each separate value falling within the range, unless otherwise indicated herein, and each separate value is incorporated into the specification as if it were individually recited herein. All methods described herein can be performed in any suitable order unless otherwise indicated herein or otherwise clearly contradicted by context. The use of any and all examples, or exemplary language
15 (e.g., "such as") provided herein, is intended merely to better illuminate the invention and does not pose a limitation on the scope of the invention unless otherwise claimed. No language in the specification should be construed as indicating any non-claimed element as essential to the practice of the invention.

 While the invention has been illustrated and described in detail in the
20 drawings and foregoing description, the same is to be considered as illustrative and not restrictive in character, it being understood that only the preferred embodiment has been shown and described and that all changes and modifications that come within the spirit of the invention are desired to be protected. In addition, all references cited herein are indicative of the level of skill in the art and are hereby
25 incorporated by reference in their entirety.

The claims defining the invention are as follows:

1. A method for testing a lumen of a medical device for a potential effect of the lumen on cells delivered through the lumen, the lumen being for
5 delivery of cell-containing flowable materials, the method comprising the steps of:
incubating a liquid medium in contact with a wall of the lumen during a residence time of the liquid medium within the lumen;;
contacting at least one cell with the liquid medium;
collecting the liquid medium from the lumen after said incubating; and
10 assessing the effect of said contacting on expression of at least one toll-like receptor by the cell.
2. A method for testing a lumen of a medical device for a potential effect of the lumen on cells delivered through the lumen, the method comprising the steps of:
15 first assessing the lumen for an effect on innate immune response of a cell, the first assessing including incubating a liquid medium in contact with a wall of the lumen during a residence time of the liquid medium within the lumen, collecting the liquid medium from the lumen after said incubating, contacting the cell with the liquid medium, and assessing the effect of said contacting on an
20 innate immune response of the cell; and
second assessing the lumen for an effect on at least one other characteristic of a cell, said at least one other characteristic selected from a group including cytotoxicity, motility, viability, metabolic activity, or any combination thereof, and said second assessing including incubating a liquid medium in contact with a wall
25 of the lumen during a residence time of the liquid medium within the lumen, collecting the liquid medium from the lumen after said incubating, contacting the cell with the liquid medium, and assessing the effect of said contacting on said at least one other characteristic of the cell.
3. A method for assessing a lumen of a medical device for a potential
30 effect of the lumen on cells delivered through the lumen, the method comprising the steps of:

contacting at least one cell with a liquid medium that has been incubated in contact with a wall of the lumen during a residence time of the liquid medium within the lumen;

collecting the liquid medium from the lumen after said contacting; and
5 assessing the effect of said contacting on at least one characteristic of the at least one cell.

4. A method for testing components of an assembly, the method comprising the steps of:

incubating a liquid medium in contact with a wall of a passageway of a
10 sample assembly during a residence time of the liquid medium within the passageway, the sample assembly including a sample first component having a first lumen coupled to a sample second component having a second lumen to form the passageway, the passageway including the first lumen and the second lumen ;

contacting at least one cell with the liquid medium;
15 collecting the liquid medium from the passageway after said incubating;
and

assessing the effect of said contacting on at least one characteristic of the cell.

5. A kit manufacturing method, the method comprising the steps of:
20 manufacturing a first device lot including a plurality of units of a first delivery component each having a first lumen for passage of cells;

manufacturing a second device lot including a plurality of units of a second delivery component each having a second lumen for passage of cells, wherein the first delivery component is associable with the second delivery component to
25 provide a delivery assembly having a passageway for passing cells, the passageway including the first lumen and second lumen;

sampling the first device lot to obtain first test sample units of the first delivery component;

sampling the second device lot to obtain second test sample units of the
30 second delivery component;

associating one of said first test sample units with one of said second sample units to provide a sample delivery assembly having a passageway including

the first lumen of the first test sample unit and the second lumen of the second sample unit;

5 assessing the passageway for an effect on at least one characteristic of a cell, said assessing the passageway including placing a liquid medium in contact with a wall of the passageway during a residence time of the liquid medium within the passageway, contacting at least one cell with the liquid medium, collecting the liquid medium from the passageway after said placing, and assessing the effect of said contacting on at least one characteristic of the cell; and

10 packaging first delivery components from the first device lot with second delivery components from the second device lot.

6. The method of any one of claims 3 to 5, wherein said at least one characteristic is selected from a group including cytotoxicity, metabolic activity, innate immune response, migration, motility, viability, or any combination thereof.

15 7. The method of claim 1, wherein the at least one cell includes exogenous DNA encoding the at least one toll-like receptor.

8. The method of claim 1 or 7, wherein the liquid medium is an aqueous medium.

9. The method of any one of claims 1, 7 or 8, which comprises simultaneously conducting said incubating and said contacting within the lumen.

20 10. The method of any one of claims 1 or 7 to 9, wherein said incubating comprises incubating the liquid medium in contact with the wall of the lumen in the absence of said at least one cell.

25 11. The method of claim 2, wherein said second assessing includes assessing the effect of the lumen on both cytotoxicity of a cell and metabolic activity of a cell.

12. The method of claim 3, wherein the liquid medium has been incubated in contact with the lumen for a period of time greater than one hour.

13. The method of claim 3 or 12, wherein said least one cell is a population of cells.

30 14. The method of claim 4 or 6, wherein the assembly is a cell delivery assembly, the passageway is a cell delivery pathway, the sample first component is

a sample first delivery component, and the sample second component is a sample second delivery component.

15. The method of any one of claims 1, 4, 7 or 14, wherein the at least one cell is a human cell.

5 16. The method of any one of claims 1, 3, 4, 7, 8, 12, 13, 14, or 15, wherein the at least one cell is a population of cells.

17. The method of claim 16, wherein the population is a clonal population.

10 18. The method of claim 17, when appended to claim 1, wherein the clonal population is a clonal population of human embryonic kidney cells.

19. The method of claim 16, when appended to claim 3, wherein the population of cells is a heterogenous population of cells.

20. The method of claim 19, wherein the heterogenous population of cells is provided by bone marrow.

15 21. The method of claim 17, when appended to claim 4, wherein the clonal population is a clonal population of human embryonic kidney cells containing exogenous DNA encoding at least one toll-like receptor.

20 22. The method of any one of claims 1, 7, 8 or 21, wherein the at least one toll-like receptor includes one or both of toll-like receptor 2 and toll-like receptor 4.

23. The method of any one of claims 1, 3 or 4, 6, 7, 8, 12, 14 to 22, wherein said liquid medium is a cell growth medium.

25 24. The method of any one of claims 4, 6, 14 and 15 to 17 or 21 to 23 when appended to claim 4, which comprises simultaneously conducting said incubating and said contacting within the passageway.

25. The method of any one of claims 4, 6, 14 and 15 to 17 or 21 to 24 when appended to claim 4, wherein said incubating comprises incubating the liquid medium in contact with the wall of the passageway in the absence of said at least one cell, and wherein said collecting is prior to said contacting.

30 26. The method of any one of claims 4, 14 and 15 to 17 or 21 to 25 when appended to claim 4, wherein said incubating is for a period of at least about 30 minutes.

27. The method of claim 26, wherein said incubating is for a period of about 30 minutes to about 48 hours.

28. The method of claim 5, wherein said assessing comprises:
5 passing cells through the passageway;
recovering the cells after said passing; and
assessing the recovered cells for an effect of the passageway on at least one characteristic of the cells.

29. The method of claim 5 or claim 28, wherein said assessing comprises:
10 incubating a liquid medium in contact with a wall of the passageway, said wall including wall portions from the first lumen and wall portions from the second lumen, to form a treated medium; and
contacting cells with the treated medium.

30. The method of any one of claims 4, 28 or 29, also comprising, prior
15 to said packaging, determining that said sample delivery assembly meets at least one predetermined criterion related to said effect on at least one characteristic of a cell.

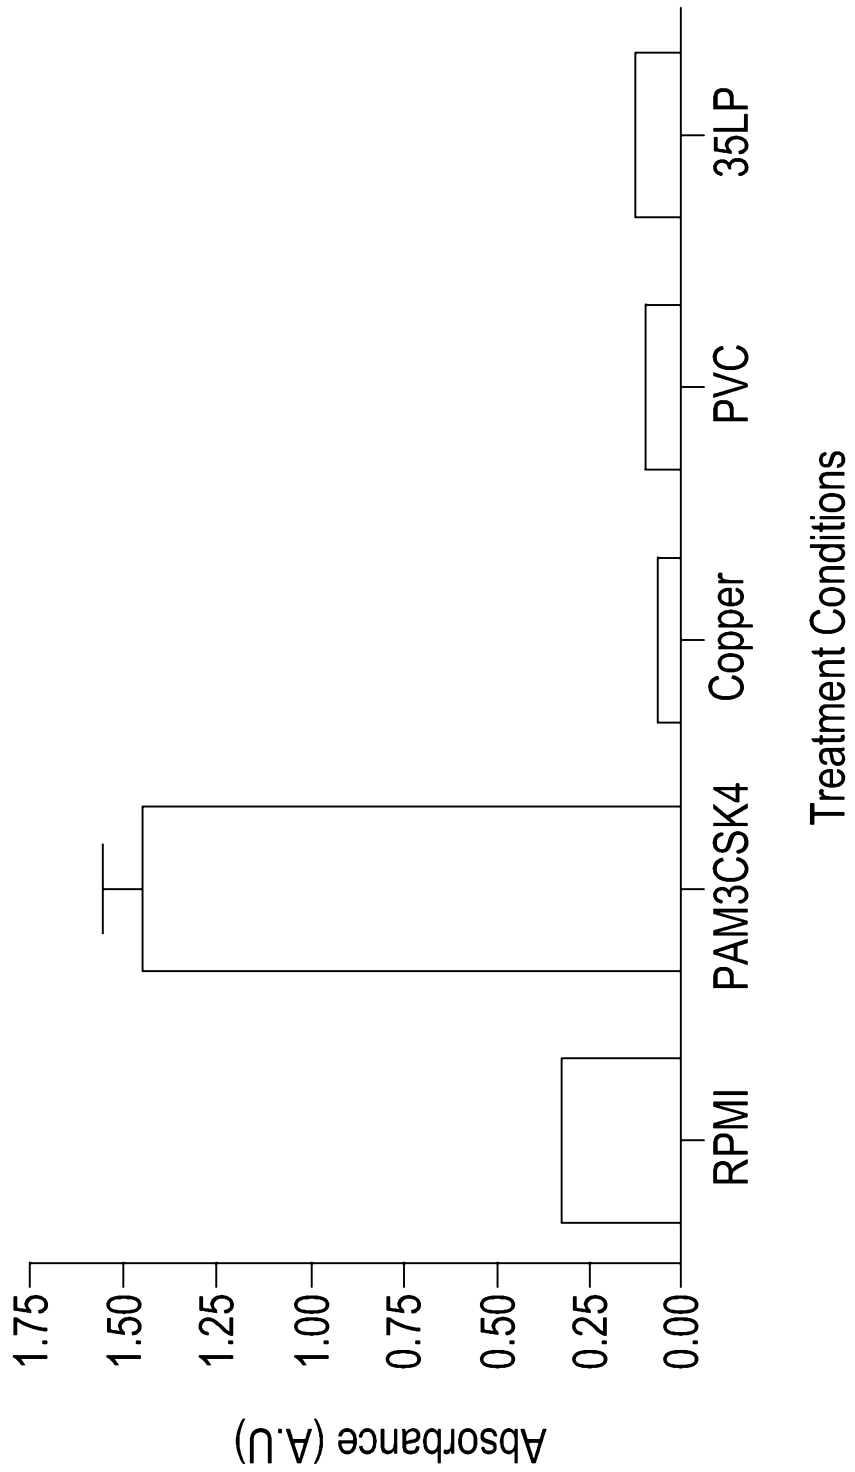


Fig. 2

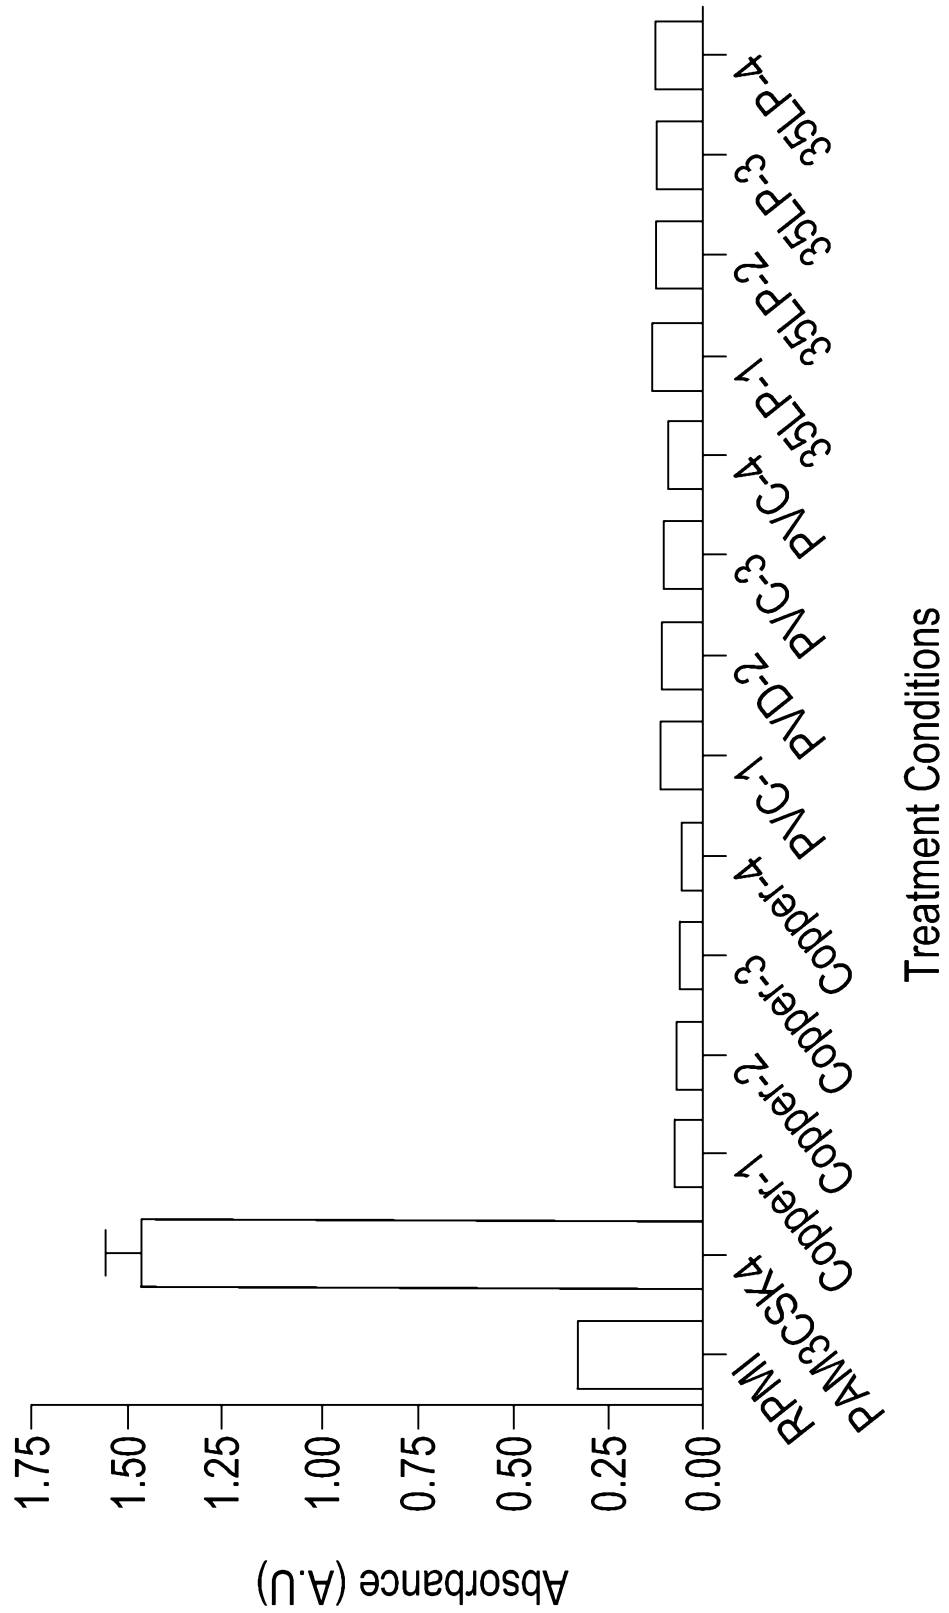


Fig. 3


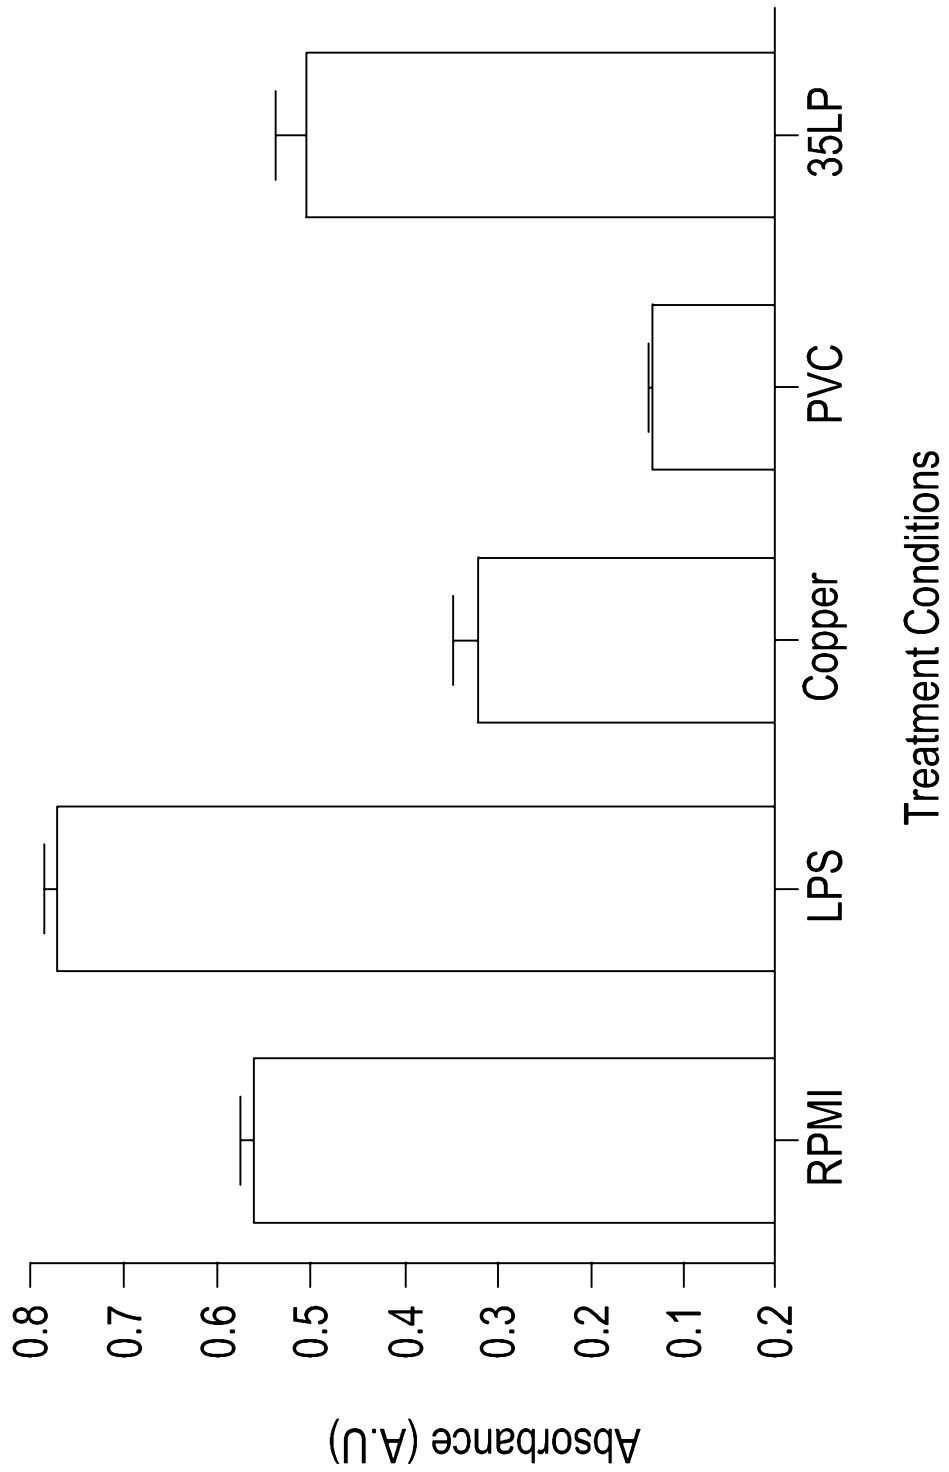


Fig. 4

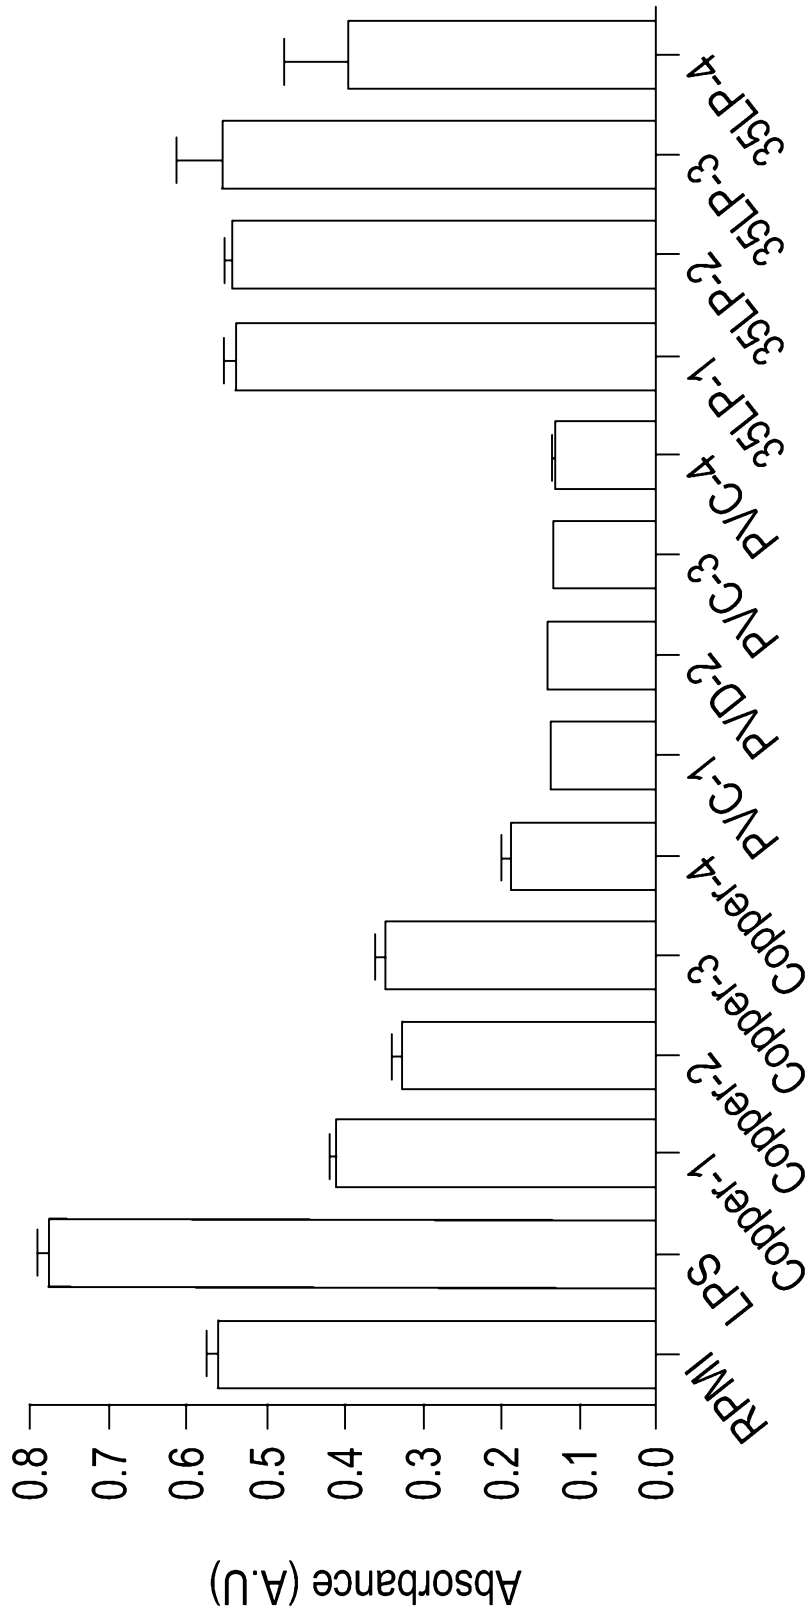

Treatment Conditions

Fig. 5

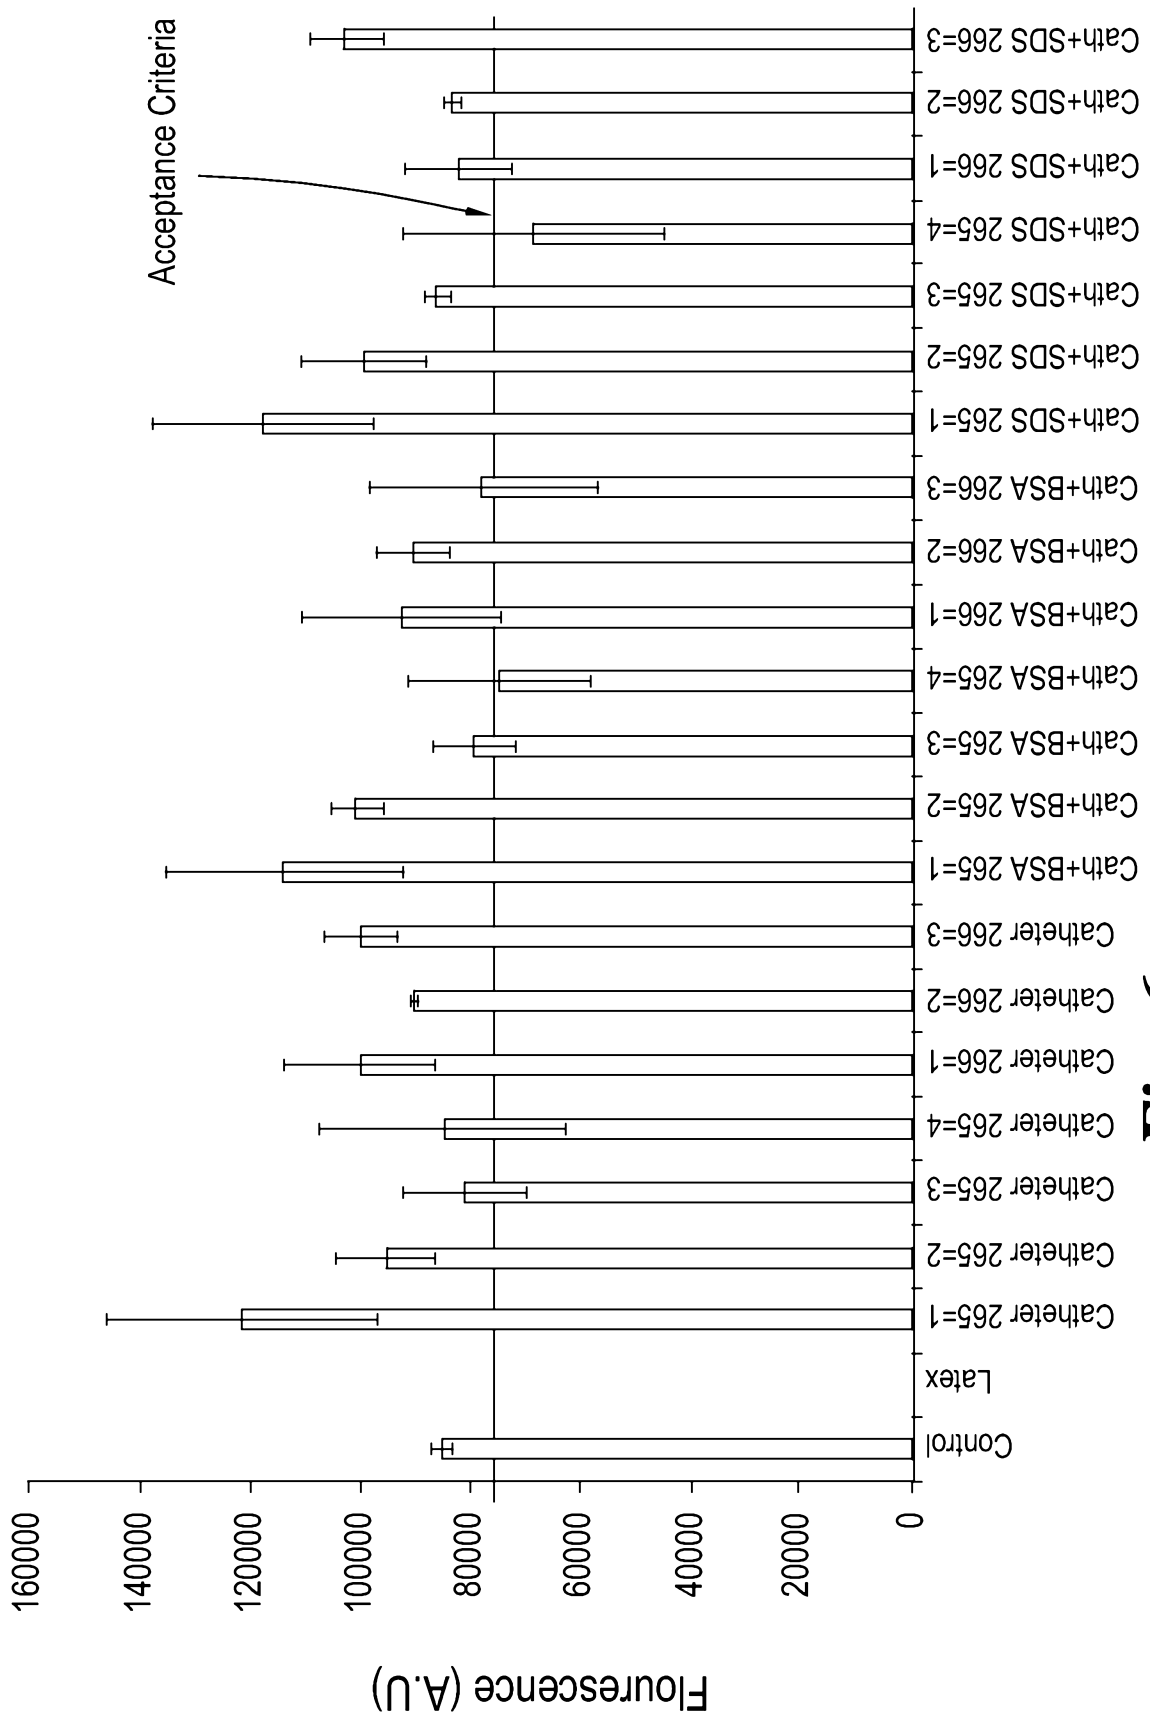


Fig. 6

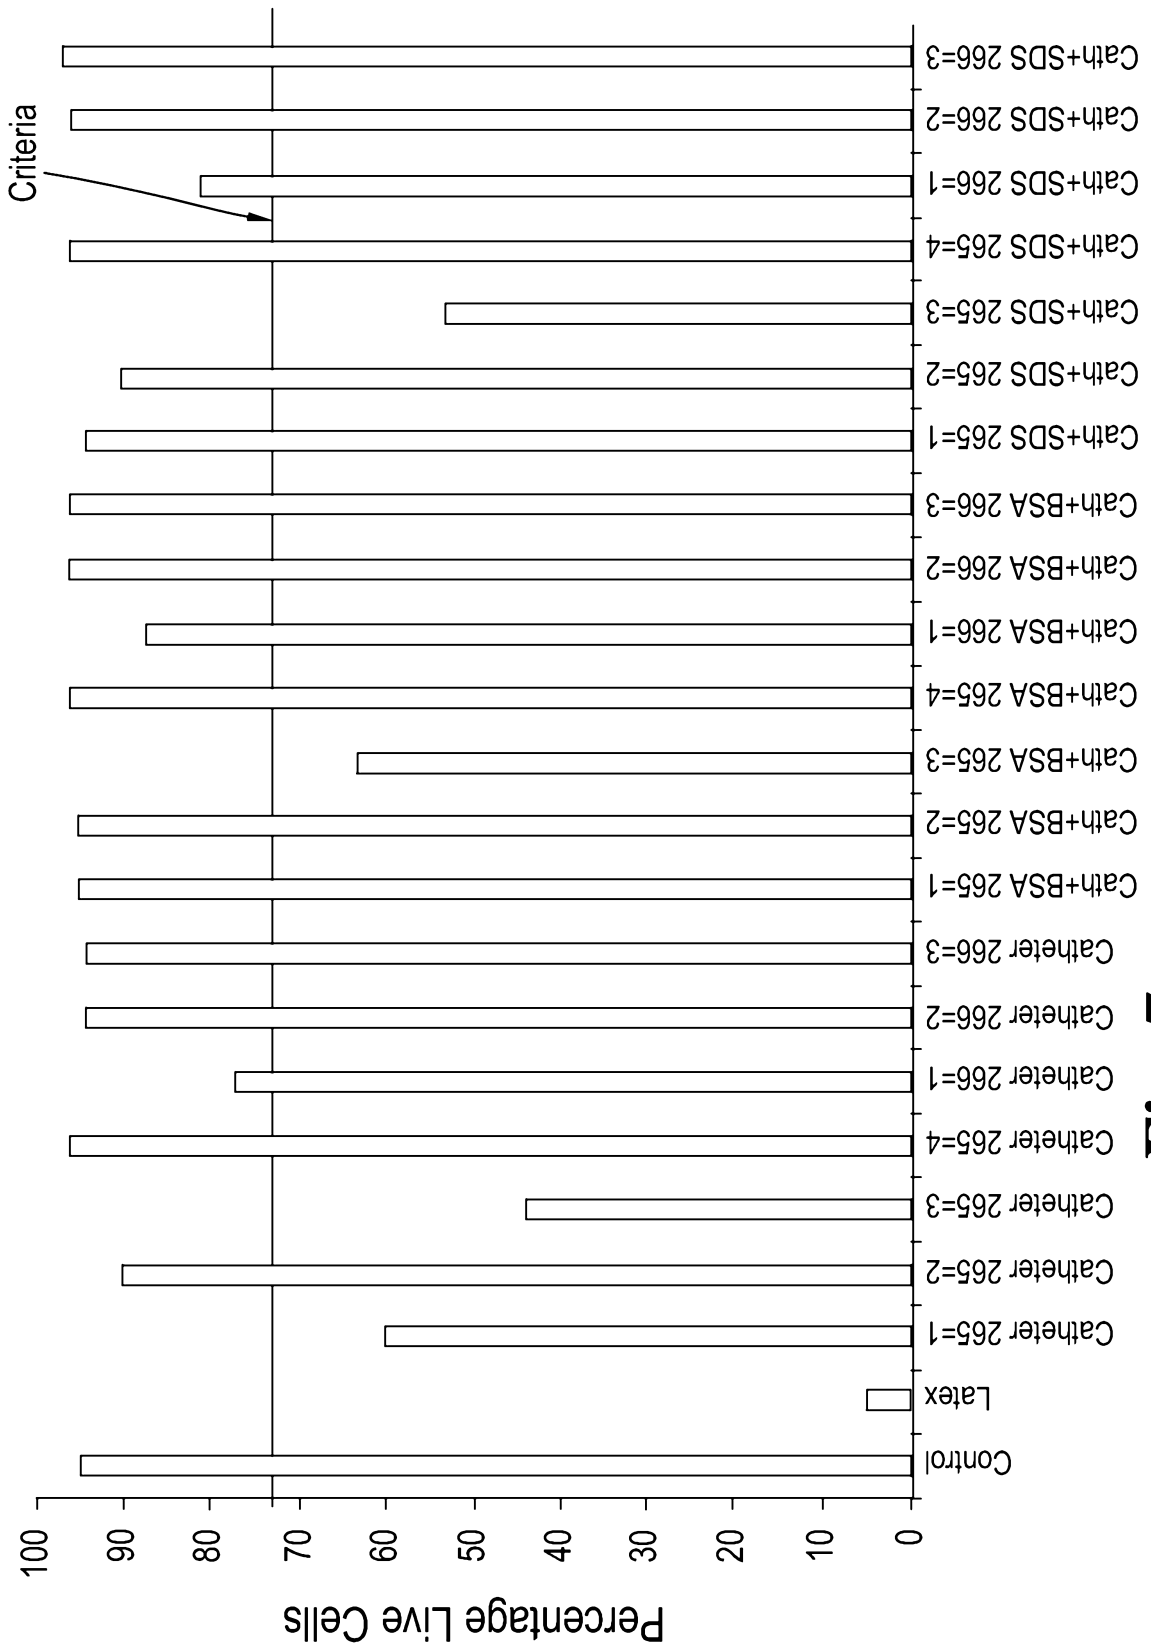


Fig. 7