

Abstract ORIGINAL**Injector Apparatus**

An injector apparatus comprises a housing (10¹, 10²) for a cartridge or syringe, a plunger (40) for cooperating in use with the cartridge or syringe to express successive doses, a dose setting arrangement (16, 20) to select a dose volume, and a drive mechanism (22, 24) releasable to advance said plunger in respective predetermined increments of magnitude to express said successive doses. The drive mechanism includes a drive spring (22) for imparting movement directly or indirectly to said plunger (40), and said dose setting arrangement comprises a dose setting element (16) moveable in a dose setting routine to define a magnitude of an increment of movement of said plunger for a given dose. The drive mechanism further includes a clutch arrangement (56) operable during said dose setting routine to inhibit forward movement of the plunger and/or to isolate said dose setting element from the force of said drive spring.

Figure 3 refers.

CLAIMS

1. An injector apparatus for use with a cartridge (12) or syringe to deliver a plurality of doses therefrom, the injector apparatus comprising:

a housing (10¹, 10²) for the cartridge or syringe;

a plunger (40) for cooperating in use with the cartridge or syringe to express successive doses;

a dose setting arrangement (16, 20) to select a dose volume;

a drive mechanism (22, 24) releasable to advance said plunger in respective predetermined increments of magnitude to express said successive doses;

characterised in that said drive mechanism includes a drive spring (22) for imparting movement directly or indirectly to said plunger (40), and said dose setting arrangement comprises a dose setting element (16) moveable in a dose setting routine to define a magnitude of an increment of movement of said plunger for a given dose, said drive mechanism further including a clutch arrangement (56) operable during said dose setting routine to inhibit forward movement of the plunger and/or to isolate said dose setting element from the force of said drive spring.

2. An injector apparatus according to Claim 1, wherein said dose setting element (16) is moveable angularly to define said increment of plunger movement.

3. An injector apparatus according to Claim 2, wherein said clutch arrangement includes a clutch element (56) moveable between disengaged and engaged positions.

4. An injector apparatus according to Claim 3, wherein said clutch element (56) is adapted to move axially with said dose setting element (16), whereby axial movement of said dose setting element from a first, rest, position to a second, dose-setting, position causes said clutch element (56) to engage to inhibit forward movement of the plunger.

5. An injector apparatus according to Claim 4, wherein said dose-setting element (16) and said housing (10¹, 10²) include complementary abutments (62,64) that engage to prevent relative rotation of said dose setting element relative to said housing when said dose setting element is in its rest position, but disengage to allow relative rotation therebetween when said dose setting element is in its setting position.

6. An injector apparatus according to Claim 5, wherein upon moving said dose setting element (16) from said rest position to said setting position, said clutch element (56) engages before disengagement of the abutments (62, 64) on said dose setting element and said housing.

7. An injector apparatus according to any of Claims 4 to 6, wherein the thrust of the drive spring (22) is reacted by said dose setting element (16) when said dose setting element is in its rest position.

8. An injector apparatus according to any of Claims 4 to 7, wherein returning said dose setting element (16) to said first position after having set a predetermined dose disengages the clutch element (56) to release the drive mechanism (22,24) to cause said plunger (40) to advance by a predetermined increment corresponding to said predetermined set dose.

9. An injector apparatus according to any of Claims 3 to 8, wherein moving said clutch element to its disengaged position moves said plunger against the force of said spring to relieve residual load between said plunger and said cartridge or syringe.

10. An injector apparatus according to any of the preceding Claims, wherein said plunger (40) is threadedly engaged with an associated control element (24), whereby linear movement of said plunger is accompanied by rotation of one of the plunger and the control element, and the magnitude of the increment of movement is controlled by limiting said rotation.

11. An injector apparatus according to Claim 10, wherein a stop surface (54) associated with said dose setting element (16), is adjustable on movement of said dose setting element to define an angular increment of movement for the relative rotation between the plunger (40) and the control element (24) upon release of said drive mechanism.

12. An injector apparatus according to Claim 11, wherein an intermediate shuttle member (20) is threadedly engaged with said dose setting element (16) and is constrained to rotate with the rotatable one of the plunger (40) and the control element (24), with the extent of relative angular movement of the shuttle member (20) and the dose setting element being set by the relative position of the stop surface associated with the dose setting element.

13. An injector apparatus according to any of the preceding Claims, wherein said drive spring (22) is a torsion spring.

14. An injector apparatus according to any of the preceding Claims, wherein said drive spring (22) is a compression spring.

15. An injector apparatus for use with a cartridge (12) or syringe to deliver a plurality of doses therefrom, the injector apparatus comprising:

a housing (10¹, 10²) for the cartridge or syringe;

a plunger (40) for cooperating in use with the cartridge or syringe to express successive doses;

a dose setting arrangement (16, 20) to select a dose volume;

a drive mechanism (22, 24) releasable to advance said plunger in respective predetermined increments of magnitude to express said successive doses;

characterised in that said drive mechanism includes a rotary stored energy element (22) with a preload sufficient to deliver at least a plurality of said successive doses.

16. An injector apparatus according to Claim 15, wherein said rotary stored energy element (22) has a preload selected to deliver substantially the entire usable contents of the syringe or cartridge over a succession of doses.

17. An injector apparatus according to Claim 16, which includes means for re-energising said rotary stored energy element.

18. An injector apparatus for use with a cartridge (12) or syringe to deliver a plurality of doses therefrom, the injector apparatus comprising:

a housing (10¹, 10²) for the cartridge or syringe;

a plunger (40) for cooperating in use with the cartridge or syringe to express successive doses;

a dose setting arrangement (16, 20) to select a dose volume;

a drive mechanism (22, 24) releasable to advance said plunger in respective predetermined increments of magnitude to express said successive doses and in which advance of said plunger 40 is controlled by a control member (24) that moves angularly in response to advance of said plunger;

characterised in that said dose setting arrangement includes first and second complementary dose setting elements (16,20) threadedly engaged for relative threaded movement away from a first limit position, with said first dose setting element (16) being moveable relative to said housing (10¹, 10²) in a setting routine from a rest position to a variable angular position that sets the dose volume, and said second dose setting element (20) being constrained to rotate with said control element (24) ,

whereby on release of said drive mechanism said control member (24) and said second member (20) rotate until the second member returns to said first limit position with respect to the first member and prevents further rotation of the control member (24).

19. An injector apparatus for use with a cartridge (12) or syringe to deliver a plurality of doses therefrom, the injector apparatus comprising:

a housing (10¹, 10²) for the cartridge or syringe;

a plunger (40) for cooperating with the cartridge or syringe to express successive doses;

a drive mechanism (22, 24) energised by a drive spring (22), and releasable to advance said plunger in predetermined increments as determined by adjustment of a dose setting element (16), and

a re-energising element (70) for re-energising said spring (24) independently of movement of said dose setting element (16).

20. An injection apparatus according to Claim 19, wherein said drive spring is a torsion spring and said re-energising element is a rotary element.

21. An injection apparatus according to Claim 20, wherein said rotary re-energising element is mounted for rotary movement in one direction on said housing by a ratchet arrangement.

22. An injection apparatus for use with a cartridge (12) or syringe to deliver a plurality of doses therefrom, the injector apparatus comprising:

a housing (10¹, 10²) for the cartridge or syringe;


a plunger (40) for cooperating in use with the cartridge or syringe to express successive doses;

a dose setting element (16) movable to select a dose volume;

a drive mechanism (22) releasable to advance said plunger in respective predetermined increments of magnitude to express said selected dose volumes, said drive mechanism including a drive spring (24) for providing motive force directly or indirectly to said plunger to advance said plunger, and

the apparatus being configurable between a first position in which the motive force of the drive spring (24) is transmitted via the dose setting element (16) to the housing (10) to be reacted thereby, and a second position in which a clutch element (56) is moved into a position in which motive force of the drive spring (24) is transmitted via the clutch element (56) to the housing (10) to be reacted thereby.

Dated this 10th day of April 2012


**of Anand and Anand Advocates
 Agents for the Applicant**

ORIGINAL 1/5

3078 DEPT 12

10 APR 2012

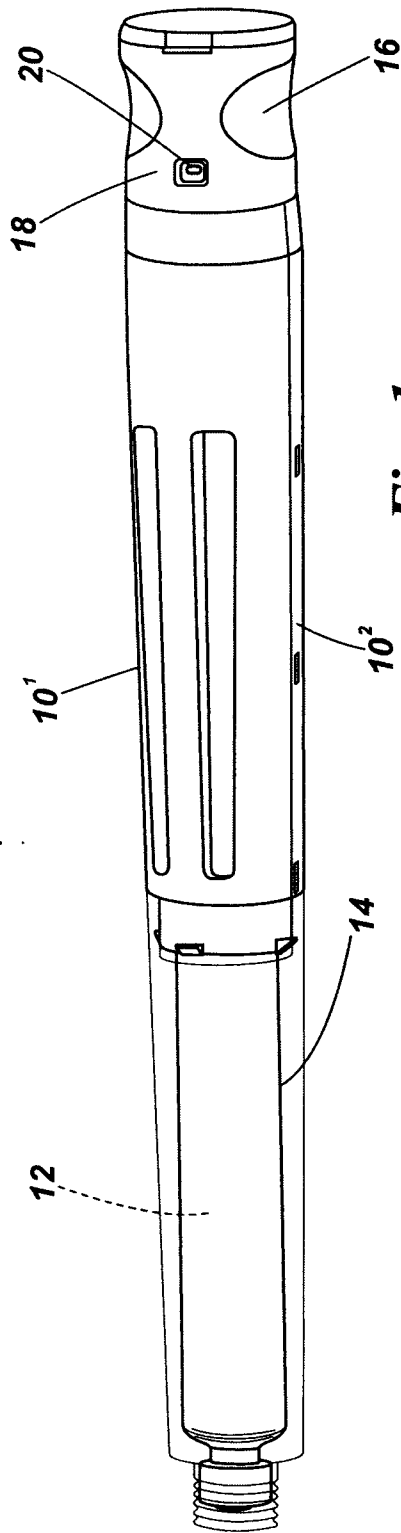


Fig. 1

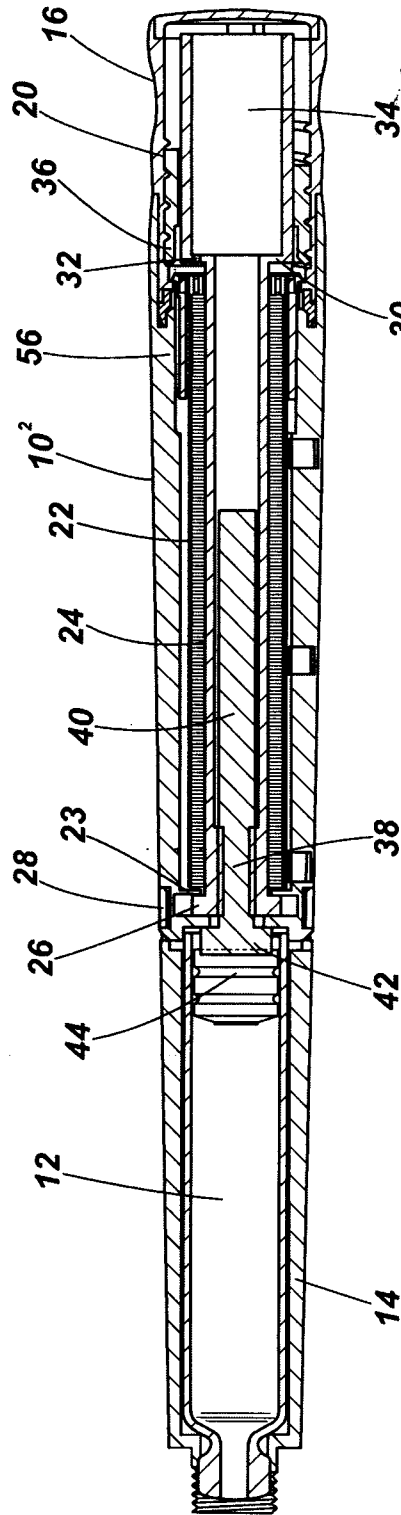


Fig. 2

Shanker
Archana Shanker
of Anand and Anand Advocates
Agent for the Applicant

ORIGINAL

2/5

3078 DELIP T2

10 APR 2012

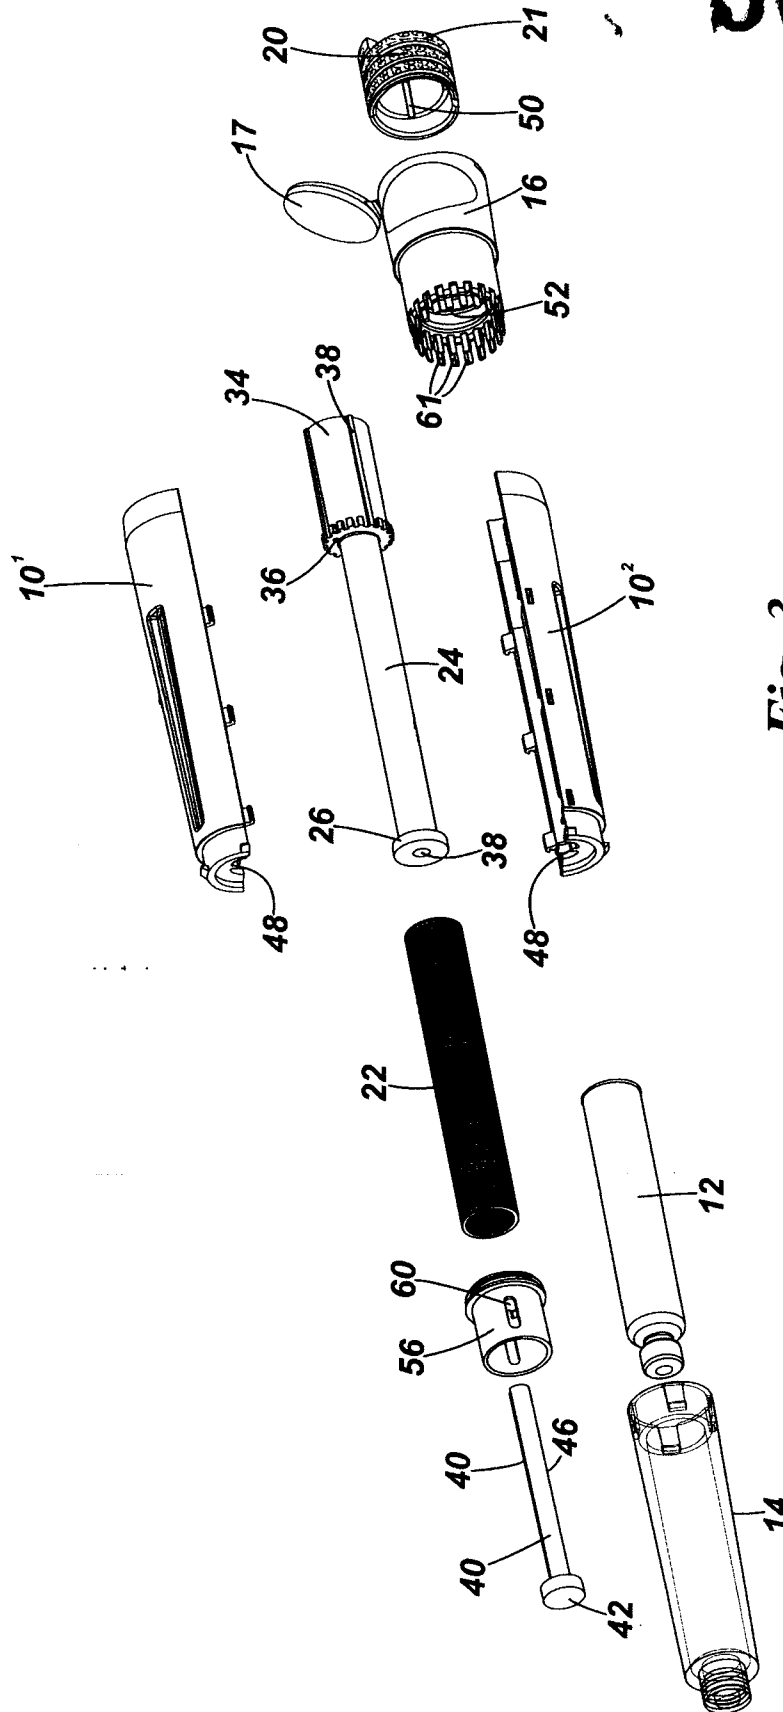


Fig. 3

Shanker
Archana Shanker
of Anand and Anand Advocates
Agent for the Applicant

ORIGINAL

3/5

3078 DELP 12

10 APR 2012

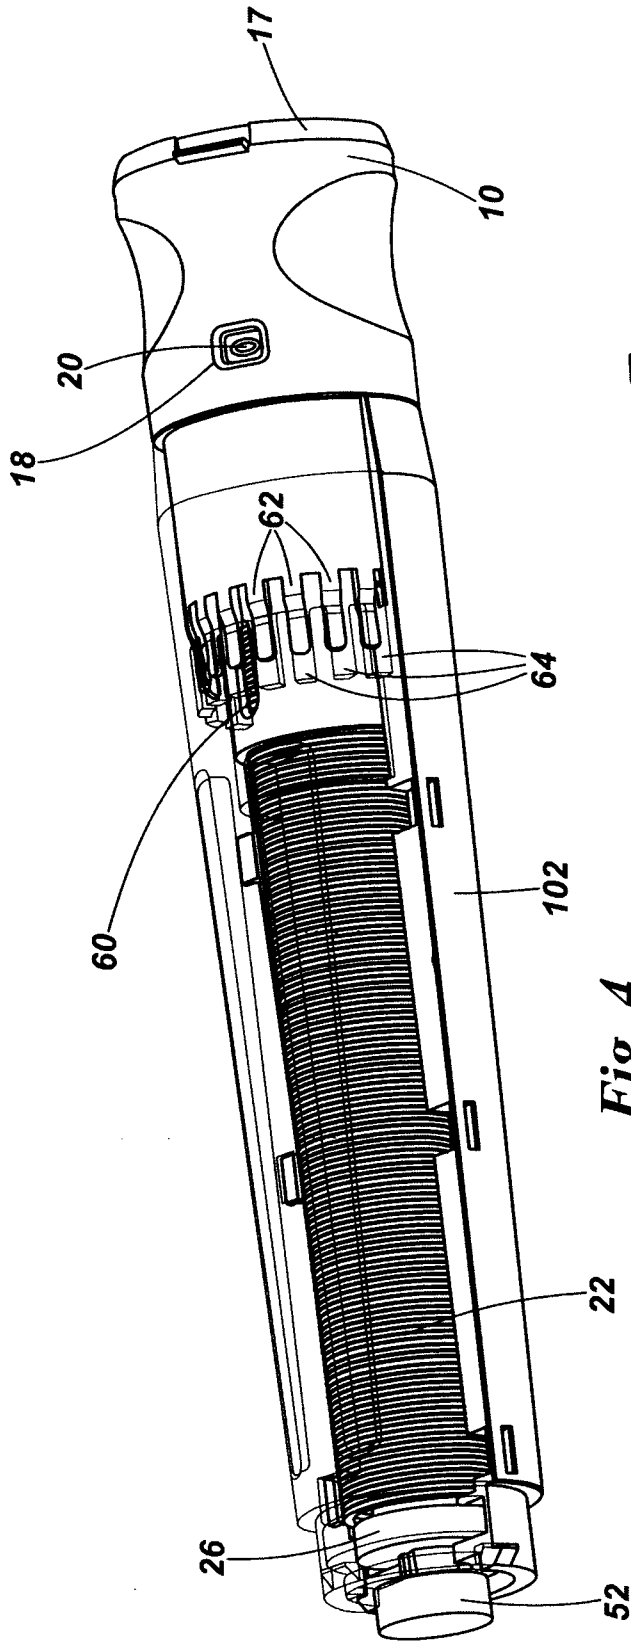


Fig. 4

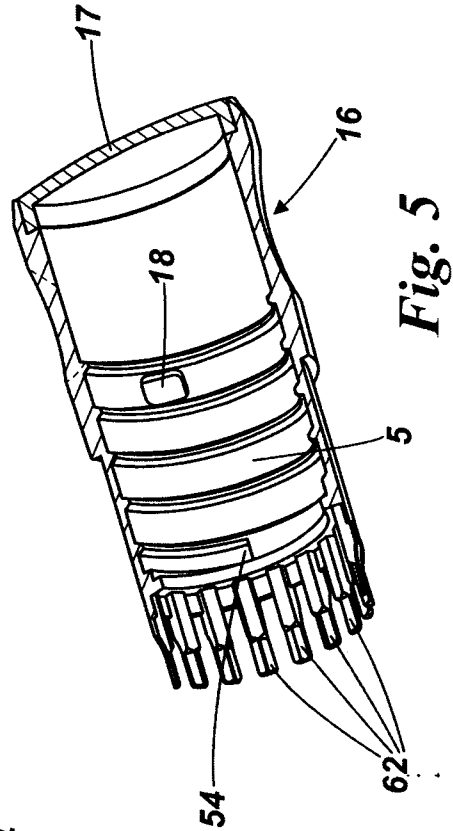


Fig. 5

Shanker

Archana Shanker
of Anand and Anand Advocates
Agent for the Applicant

ORIGINAL

4/5

3078 DELIN T2

10 APR 2012

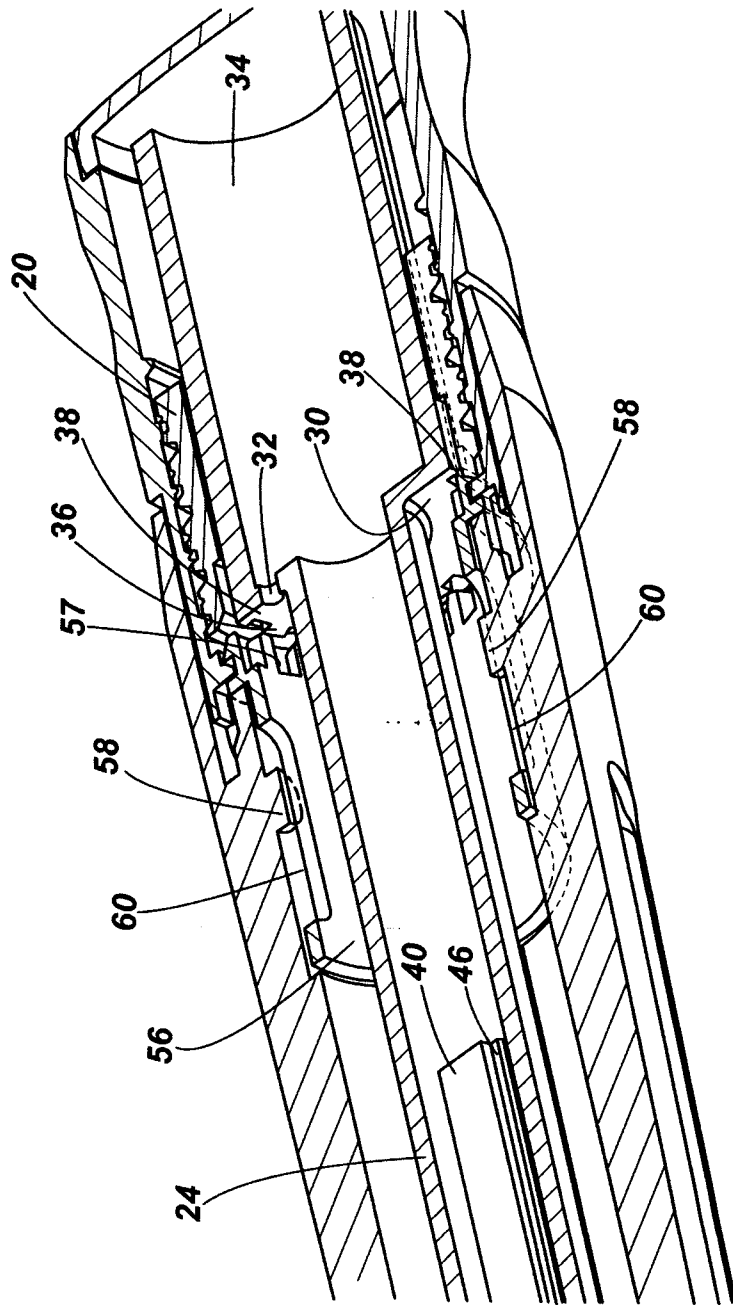


Fig. 6

Shanker

Archana Shanker
of Anand and Anand Advocates
Agent for the Applicant

ORIGINAL

5/5

3078 DELIMP 12

10 APR 2012

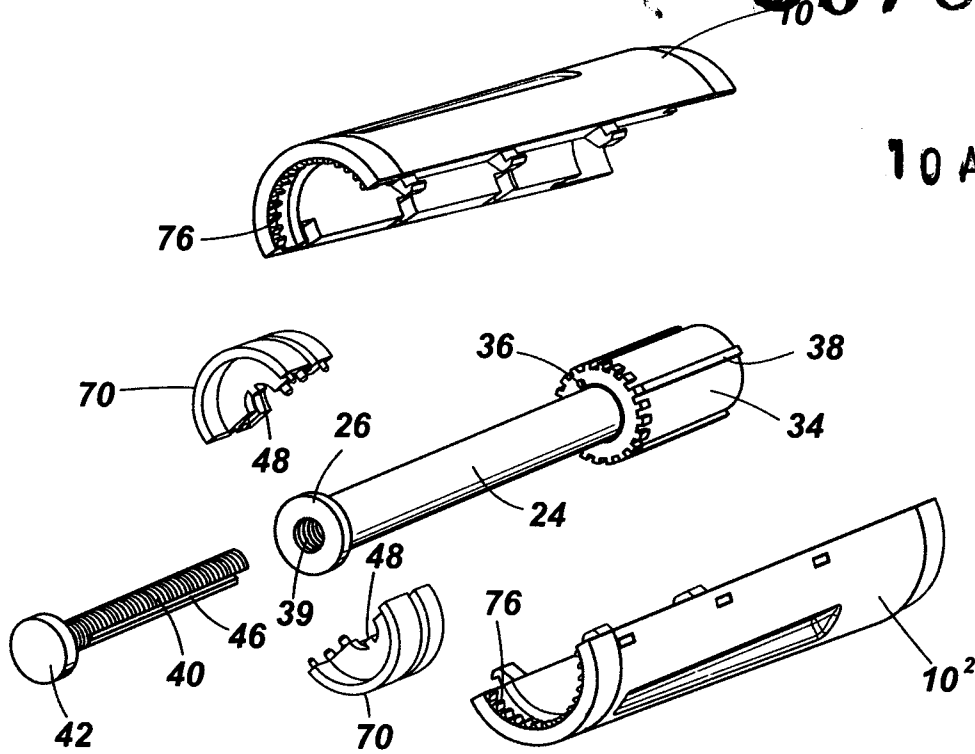


Fig. 7

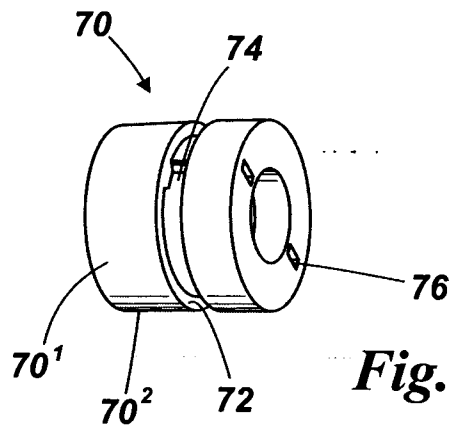


Fig. 8

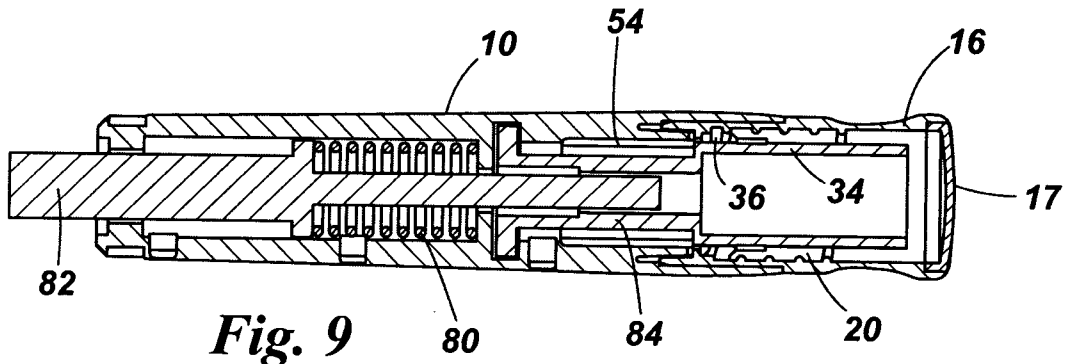


Fig. 9

Archer

Archana Shanker
of Anand and Anand Advocates
Agent for the Applicant

Injector Apparatus

This invention relates to injector apparatus and in particular, but not exclusively, to such apparatus used for injecting multiple doses of variable magnitude, for example of insulin.

In our earlier Autopen[®] device, a rotatable dose setting knob attached to the rear end of the pen injector is connected to a hollow drive sleeve that carries an annular ratchet surface at its front end which engages a corresponding ratchet surface on a threaded drive collar. The threaded drive collar is threadedly engaged with the stem of a plunger so that rotary movement of the drive collar is converted into a linear advance of the plunger. A trigger can be moved to release the drive collar for rotary movement. During a dose setting routine, with the drive collar held against rotation by the trigger, a dose is dialled in by rotating the dose setting knob and the drive sleeve against a spring bias provided by a main drive spring. The dose setting movement is unidirectional only due to the ratchet action between the drive sleeve and the drive collar. Upon release of the trigger, the drive collar rotates by an angular amount equivalent to the angular amount initially dialled in, and the plunger is advanced by the corresponding amount to deliver the dose of the required number of units.

This device performs extremely well and enjoys considerable success but we have identified a number of improvement opportunities. In the above device, in setting a dose the user winds up the spring to provide the motive force that is needed for the next dose. This means that it can be awkward for those of limited dexterity to exert sufficient grip to rotate the dose setting knob against the bias of

the drive spring. Also in this design, because the action of dose setting winds up the drive spring, a ratchet action is required so that when the user releases their grip on the dose setting knob, the knob stays in that position and does not immediately return to the zero position under the influence of the drive spring. To allow dose setting reversal in case of setting overshoot, a bi-directional ratchet mechanism is then needed, or otherwise a disconnection mechanism is required, either of which complicate the device.

We have therefore designed an injector apparatus in which a clutch arrangement is provided to isolate the dose setting element from the force of the drive spring during the dose setting routine.

Accordingly, in one aspect, this invention provides an injector apparatus for use with a cartridge or syringe to deliver a plurality of doses therefrom, the injector apparatus comprising:

a housing for the cartridge or syringe;

a plunger for cooperating in use with the cartridge or syringe to express successive doses;

a dose setting arrangement to select a dose volume;

a drive mechanism releasable to advance said plunger in respective predetermined increments of magnitude to express said successive selected doses;

characterised in that said drive mechanism includes a drive spring for applying expulsion drive movement directly or indirectly to said plunger, and said dose setting arrangement comprises a dose setting element moveable in a dose setting routine to set a magnitude of an increment of movement of said plunger

for a given dose, said drive mechanism further including a clutch arrangement operable during said dose setting routine to isolate said dose setting element from the force of said drive spring and optionally to inhibit directly or indirectly forward movement of the plunger.

In an arrangement where the dose setting element is isolated from the force of the drive spring during the dose setting routine, the dose setting element can be rotated easily, and also preferably can be moved in the reverse sense if the user moves the dose setting element past a required dose. Isolating the dose setting element means that the dose-setting movement of said dose setting element is not resisted by said spring.

It follows from the above that if the dose setting action does not energise the drive spring, the drive spring needs to be energised in some fashion. Conveniently, the drive spring is preloaded to an extent sufficient to deliver substantially the entire useable contents of the syringe or cartridge in a succession of doses. Where the dose setting element is isolated from the force of the drive spring during the dose setting routine, a more powerful spring may be used than would be appropriate for the conventional user-wound device. Instead of providing a fully preloaded drive spring, the drive spring could be partially preloaded or with no preload but with suitable separate means for energising the spring. It will also be appreciated that in such arrangements the drive mechanism will usually already be under load from the drive spring prior to dose setting, in contrast to prior art devices where the drive mechanism is under load only once the dose has been dialled in.

Preferably, the dose setting element is moveable angularly to set said increment of plunger movement.

The clutch arrangement preferably includes a clutch element moveable between disengaged and engaged positions. Thus the clutch element may be adapted to move axially with said dose setting element, whereby axial movement of said dose setting element from a first, rest, position to a second, dose setting position causes said clutch element to engage to inhibit movement of said plunger. It is also convenient for the dose setting element and the housing to include complementary abutments that engage to prevent relative rotation of said dose setting element relative to said housing when the dose setting element is in its rest position, but which disengage to allow dose setting rotation of the dose setting element when it is in its setting position. In this manner, the dose setting element may be moved axially from its rest position to its dose setting position, then turned to dial in a required dosage volume, and then returned axially to its rest position to lock it against rotation.

Preferably, upon moving the dose setting element from its rest position to its setting position, the clutch engages to inhibit movement of the drive plunger a predetermined distance before the abutments on the dose setting element and the housing disengage to release the dose setting element for dose setting movement.

In a preferred arrangement, when the dose setting element is in its rest position, it receives and reacts the thrust of the drive spring so that the dose setting element thereby inhibits movement of the drive plunger. In this manner, when the dose setting element is in its rest position the thrust of the drive spring

is reacted by the dose setting element and thence to the housing, but when the dose setting element is in its setting position, the thrust of the drive spring is reacted by the clutch member having engaged with the housing.

Preferably, having set a dose, returning the dose setting element axially to its first position disengages the clutch element to release the drive mechanism to cause the plunger to advance by a predetermined increment corresponding to the predetermined set dose.

Preferably, said plunger is threadedly engaged with an associated drive or control element whereby advance of said plunger is accompanied by rotation of the plunger or the drive or control element, with the magnitude of the incremental advance being set by constraining said rotation.

Preferably a stop member is associated with the dose setting element and is adjustable by moving the dose setting element, thereby to define an angular increment for the relative rotation between the plunger and the drive or control element upon release of the drive mechanism.

The stop member could simply be an abutment surface provided on the dose setting element. This would allow the maximum useable extent of angular movement of the dose setting element to be just short of 360°. This would mean that the indicia needed to be fairly closely packed in some instances. Accordingly it is preferred for there to be an intermediate dial or shuttle member threadedly engaged with the dose setting element and constrained to rotate with the rotatable one of the plunger and the control member, with the extent of relative angular movement of the dial or shuttle member and the dose setting element being set by the relative position of the stop member associated with

the dose setting element. The provision of a threaded dial or shuttle member means that it is now possible to set a dose of several turns. This has advantages both in terms of the available size for the indicia, and also allows greater flexibility over the choice of the pitch of the thread between the plunger and the control member. In a particularly preferred arrangement, the dosage indicia may be provided as a helical strip on one of said complementary dose setting elements, and read off via a marker or window on the other dose setting element.

The drive spring in the various arrangements described above may be either a torsion spring that imparts a rotary movement when released, or a compression spring that imparts a linear movement.

In many applications it may be desirable to provide a multiple dose injector device that is supplied preloaded so that it is not necessary to re-energise the drive between each dose, for example if the device is intended to be disposable.

Accordingly, in another aspect, this invention provides an injector apparatus for use with a cartridge or syringe to deliver a plurality of doses therefrom, the injector apparatus comprising:

- a housing for the cartridge or syringe;

- a plunger for cooperating in use with the cartridge or syringe to express successive doses;

- a dose setting arrangement to select a dose volume;

- a drive mechanism releasable to advance said plunger in respective predetermined increments of magnitude to express said successive doses;

characterised in that said drive mechanism includes a rotary stored energy element with a preload sufficient to deliver at least a plurality of said successive doses.

In the above arrangement, the injector apparatus may for example be provided with a fully preloaded spring so that the user is not required to input the mechanical energy required to express the doses. This renders the device particularly suitable for those with limited dexterity or poor grip.

As noted above, conventional Autopen[®] and similar devices have an angular range of dose setting movement that is limited to 360°, and this places constraints on the marking indicia, the pitch of the drive thread, and the properties of the drive spring. We have therefore designed an arrangement in which the dose setting arrangement includes threadedly engaged first and second complementary dose setting elements which enables the dose setting movement to be several turns if required.

Accordingly, in another aspect of this invention, there is provided an injector apparatus for use with a cartridge or syringe to deliver a plurality of doses therefrom, the injector apparatus comprising:

a housing for the cartridge or syringe;

a plunger for cooperating in use with the cartridge or syringe to express successive doses;

a dose setting arrangement to select a dose volume;

a drive mechanism releasable to advance said plunger in respective predetermined increments of magnitude to express said successive doses and

in which advance of said plunger is controlled by a control member that moves angularly in response to advance of said plunger;

characterised in that said dose setting arrangement includes first and second complementary dose setting elements threadedly engaged for relative threaded movement away from a limit position, with said first dose setting element being moveable relative to said housing in a setting routine from a rest position to a variable angular position that sets the dose volume, and said second dose setting element being constrained to rotate with said control member,

whereby on release of said drive mechanism said control member and said second dose-setting element rotate until the second element returns to said first limit position with respect to the first element, thereby preventing further rotation of the control member.

According to another aspect, the invention provides an injector apparatus for use with a cartridge or syringe to deliver a plurality of doses therefrom, the injector apparatus comprising:

a housing for the cartridge or syringe;

a plunger for cooperating with the cartridge or syringe to express successive doses;

a drive mechanism energised by a drive spring, and releasable to advance said plunger in predetermined increments as determined by adjustment of a dose setting element, and

a re-energising element for re-energising said spring independently of movement of said dose setting element.

Preferably said drive spring is a torsion spring and said re-energising element is a rotary element, for example a manually rotatable element.

According to another aspect, this invention provides an injection apparatus for use with a cartridge or syringe to deliver a plurality of doses therefrom, the injector apparatus comprising:

a housing for the cartridge or syringe;

a plunger for cooperating in use with the cartridge or syringe to express successive doses;

a dose setting element movable to select a dose volume;

a drive mechanism releasable to advance said plunger in respective predetermined increments of magnitude to express said selected dose volumes, said drive mechanism including a drive spring for providing motive force directly or indirectly to said plunger to advance said plunger, and

the apparatus being configurable between a first position in which the motive force of the drive spring is transmitted via the dose setting element to the housing to be reacted thereby, and a second position in which a clutch element is moved into a position in which motive force of the drive spring is transmitted via the clutch element to the housing to be reacted thereby, so that dose setting movement of the dose setting element is not resisted by the drive spring.

Whilst the invention has been described above, it extends to any inventive combination of the features set out above or in the following description of claims.

The invention may be performed in various ways, and an embodiment thereof will now be described by way of example only, reference being made to the accompanying drawings in which:

Figure 1 is a side view of a first embodiment of pen injector in accordance with this invention:

Figure 2 is a side section view of the pen injector of Figure 1;

Figure 3 is an exploded view of the pen injector of Figures 1 and 2;

Figure 4 is an enlarged view of the main body of the pen injector of Figures 1 to 3, containing the drive mechanism, with one body half shown transparent;

Figure 5 is a perspective section view of the dose setting knob showing the thread on the inside of the dose setting knob;

Figure 6 is a perspective section view on the rear part of the drive mechanism showing the clutch and dose setting knob and dose dial;

Figure 7 is an exploded view of a second embodiment of pen injector in accordance with the invention having a rewind facility;

Figure 8 is a detailed view of the rewind knob, and

Figure 9 is a side section view of a third embodiment of pen injector driven by a compression spring.

The embodiment of pen injector illustrated in Figures 1 to 6 is designed to be a disposable automatic pen type injector capable of expelling a succession of doses of variable preset magnitude from a cartridge. The injector comprises a body made up of symmetric body halves 10¹ and 10² which may be snap-fitted or glued together. A cartridge or syringe 12 is received in a transparent forward cartridge housing 14 which is a snap-fit on the forward end of the body halves

10¹, 10². On the rear end of the body is mounted a dose setting knob 16 having a window 18 through which a dose dial 20 is visible. As to be described below, the device contains a preloaded torsion spring which in this particular embodiment supplies the entire force required to express all the useable dosage volume in the cartridge. Doses are set by pulling the dose setting knob 16 rearwardly, rotating it until the required dosage unit is visible on the dose dial and then pushing the dose dial back in to release the drive mechanism to expel the required dose.

Referring now more particularly to Figures 2, 3 and 4 the body 10¹, 10² defines an internal cylindrical space in which a torsion spring 22 is located in an energised state, with the forward end of the spring being anchored on an inner part 23 of the body. A hollow tubular drive shaft 24 is disposed concentrically within the spring having a radial flange 26 which is rotatably held within an annular recess 28 on the forward part of the body to allow rotation of the drive shaft but to prevent axial movement thereof. Towards its rear end, the diameter of the shaft increases at a shoulder 30 in which is provided an anchorage hole 32 for the rear end of the drive spring. When assembled and prior to first use, the torsion spring 22 is fully energised and acts on the drive shaft to rotate it in the dispensing direction. The enlarged portion 34 at the rear end of the drive shaft is provided with upstanding splines 36 adjacent the shoulder 30, with four of the splines 38 at 90° extending the full length of the enlarged portion 34.

At the front end the drive shaft has an internally threaded bore 38 into which is threaded the lead screw of a plunger 40. The plunger has an enlarged head 42 which engages the bung 44 of the cartridge 12. Immediately behind the

enlarged head 42 the drive shaft has two diametrically opposed keyways 46 which cooperate with respective keys 48 on the front end of the body halves 10¹ and 10², to allow axial movement of the plunger, but prevent rotation thereof, as the drive shaft 24 rotates to advance the plunger.

The dose dial 20 is slideably mounted on the enlarged portion 34 of the drive shaft 24 but prevented from rotation thereof by means of four, internal, equispaced, keyways 50 that engage the longer splines 38 on the enlarged portion. The forward end of the dose dial has an enlarged internal diameter so as to be clear of the shorter splines 36. The external surface of the dose dial 20 carries a coarse helical thread 21 which threadedly engages a corresponding internal threaded portion 52 on the inner surface of the dose setting knob 16. The threaded portion 52 on the inside of the dose setting knob 16 has a forward limit position set by termination of the thread (see blind end 54 in Figure 5). A rear limit position stop may optionally be provided, for example, on the inner part of a hinged cap portion 17 of the dose setting knob.

The dose setting knob 16 is connected at its forward end to a clutch collar 56 by means of a snap-fit which allows the clutch and the dose setting knob to rotate relative to each other but secures them against relative axial movement (see Figure 6). The clutch collar 56 is mounted for axial sliding movement in the body 10 but prevented from rotation with respect thereto by means of two lugs 58 in the body engaging opposed respective slots 60 in the cylindrical wall of the clutch collar 56. At its rear end, the clutch collar 56 has an internal splined arrangement 57 designed to slide into splined engagement with the splines 36 on the enlarged portion 34 of the drive shaft so as to lock the drive shaft against

movement under the influence of the spring by reacting the thrust into the body by via the lugs 58. Referring now more particularly to Figures 4 to 6, the forward end of the dose setting knob 16 has a series of axially extending fingers 62 which are an axial sliding fit with a series of pockets 64 provided in the body.

The axial lengths of the fingers 62 and of the pockets 64 are carefully selected having regard to the axial spacing between the internal splines 57 on the clutch collar 56 and the external splines 36 on the drive shaft 24 such that, on pulling the dose setting knob 16 out axially, the splines 57 on the clutch collar 56 engage the splines 36 on the drive shaft 24 some distance before the fingers 62 of the dose setting knob 16 are withdrawn axially from the pockets 64 on the body. The reason for this is that, in the position shown in Figure 2, as indicated above, the thrust of the drive spring is transmitted via the drive shaft splines 38 to the dose dial 20 and thence to the dose setting knob 16 (by virtue of the dose dial being at its forward limit position relative to the dose setting knob). It is therefore important to ensure that the clutch 56 has engaged the drive shaft 24 to react the load of the torsion spring 22 through the clutch 56 and the lugs 58 to the housing before the dose setting knob has withdrawn enough to rotate.

Once the dose setting knob has been withdrawn far enough to disengage the fingers 58 from the pockets 64, it is in a setting position in which it may be rotated to set a dose against a light detent action provided by the fingers 62, which provide a audible/tactile click to enable the user to count the number of units dialled in. It will be appreciated that during dose setting, the body 10, drive shaft 24, clutch 56 all remain stationary, both axially and rotationally. The dose dial is fixed against rotation due to its splined engagement with the large portion

34 of the drive shaft but is capable of moving axially. Thus in this condition, with the dose setting knob 16 axially in its setting position, rotation of the dose setting knob in the appropriate direction moves the dose dial 20 axially in a lead screw fashion. The dose dial numbers are visible through the window 18. The threaded arrangement allows multiple turns of the dose setting knob. Also at this point there is no loading between the dose dial and the cap and so there is little resistance to rotary movement of the dose setting knob apart from that provided by the detent.

Once the required dose has been dialled in on the helical scale, the device is ready for firing. In this arrangement this is achieved by pushing the dose setting knob 16 back in. As the dose setting knob is pushed back in, the fingers 62 re-engage the pockets and thereafter the clutch 56 is shifted forwardly off the enlarged portion of the drive shaft to disengage it so that the drive shaft is now free to rotate. The drive shaft rotates by the angular amount dialled in.

In the above arrangement, as the setting of the dose is independent of the drive spring, the operating stroke length and force can be reduced to design a device in which a large dose is delivered with a small movement and force. This contrasts with existing devices in which the user has to apply a large user movement to set a dose and/or expel the set dose.

There is a potential issue in existing multi-dose devices in which after expulsion of a dose the plunger remains in contact with the bung. Due to the friction between the bung and the cartridge wall and its resilience, at the end of an injection the bung will be under residual compression. Vibrations transmitted

to the bung either via the plunger or the wall of the cartridge can cause the bung to expand slightly and expel a drip which can affect dose accuracy. As a modification of the above embodiment the clutch arrangement can be designed so that, as it is pulled to disengage, it backs off the plunger 40 from the bung 44 a fraction, so that the bung 44 is unloaded.

This unloading effect may be achieved for example by putting a slight form on the splines 57 of the clutch collar 56 and on the splines 36 of the drive shaft 24 so that, as the dose setting knob is pulled out to engage the clutch collar 56 on the drive shaft, the drive shaft is rotated a few degrees against the spring bias to unload the bung.

Whilst in this embodiment the body is formed in two separate halves it may instead be formed in a clamshell type arrangement where the two halves are hinged by a live hinge.

In order to ease manufacture, the torsion spring in the illustrated embodiment may be formed with a wave or compression portion at its forward end to apply a light axial load to the cartridge in order to hold the cartridge firmly in a forward position. This allows variations in length due to production variances to be accommodated. Furthermore although the wire that is coiled to make the spring may be circular in section in some applications it is preferred for it to be non-circular, such as of square or rectangular section.

Referring now to Figures 7 and 8, a second embodiment provides an arrangement for rewinding the plunger 40 and simultaneously energising the drive spring 22 (see Figures 3 and 4) of the first embodiment. In the second embodiment most of the components are similar to those of the first embodiment

and will not be described again and will be given like reference numerals. Referring to Figure 7, the forward part of the housing which defines the keys 48 that engage the keyways 46 on the lead screw of the plunger is formed as a separate rewind knob 70 which is uni-directionally rotatable about the longitudinal axis of the housing. The knob 70 is formed in two halves 70¹, 70² and defines a central aperture with the diametrically opposed keys 48. The knob 70 has an outer circumferential groove 72 in the base of which are two diametrically opposed sprung ratchet teeth 74, as seen in Figure 8. The knob 70 is rotatably received in the forward end of the housing by means of an inwardly directed toothed annular rib 76 locating in the groove 72 and cooperating with the ratchet teeth 74 to allow rotation in one direction only. The rear end of the rewind knob 70 is provided with two slots 76 into one of which the front end of the torsion drive spring 22 (not shown) is anchored. Engagement of the keys 48 on the knob 70 with the keyways 46 on the lead screw of plunger 40 ensures that the plunger 40 rotates with the knob in one direction only but is capable of axial sliding movement. The knob and the plunger may therefore be rotated in the direction permitted by the ratchet to wind up the drive spring 22 and to retract the plunger back into the driveshaft 24 by virtue of the threaded engagement between the lead screw of the plunger 40 and the driveshaft.

The rewind knob will normally be accessible only when the cartridge housing (see first embodiment) has been removed from the body.

In the above arrangements, a torsion spring provides the motive force for expelling the useable contents of the cartridge. It would of course be possible to use other suitable drive configurations. For example, as shown in Figure 9, the

torsion spring could be replaced by a compression spring 80 which acts on the plunger 82 to apply a thrust in the longitudinal direction. In this case, instead of the drive shaft there is a drive control shaft 84 that is used to modulate forward movement of the plunger 82 under the influence of the compression spring 80.

The rear end of the plunger 82 is formed with a threaded portion which threadedly engages an internal bore on the drive control shaft 84 so that as the plunger 82 is urged forwardly by the compression spring the drive control shaft rotates. The drive control shaft 84 is formed at its rear end with an enlarged portion 34 provided with upstanding splines 36 similar to those of the drive shaft 24 of the first embodiment, and fulfilling a similar function in conjunction with a clutch collar 56, the dose setting knob 16 and the dose dial 20 of the first embodiment. The construction and operation of these elements will not be described in detail again. As previously, the drive control shaft 84 is alternately held and released by the clutch collar 56 and the dose setting knob 16.

ORIGINAL 1/5

3078 DEPT 12

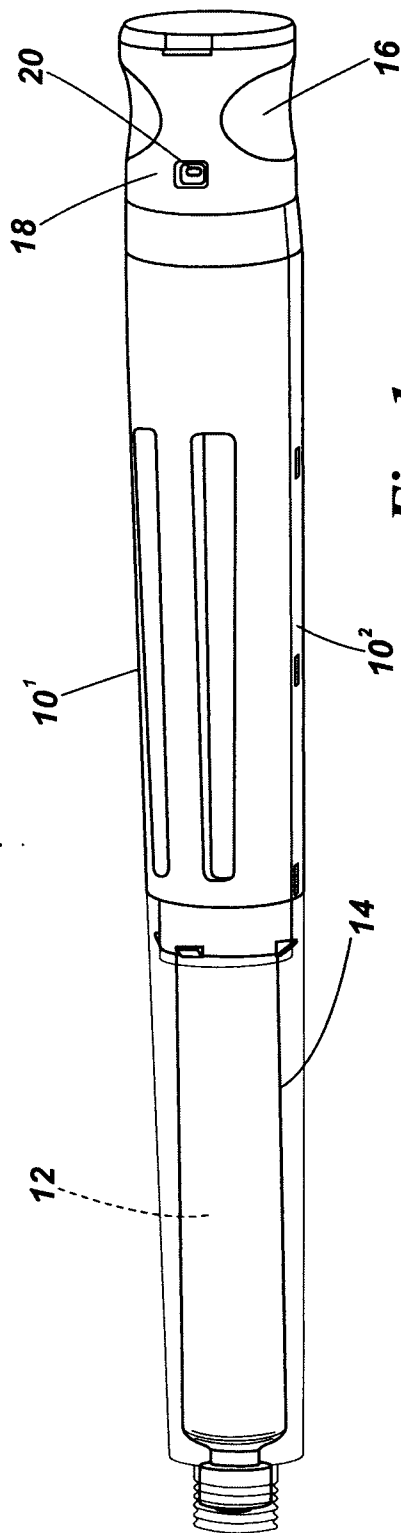


Fig. 1

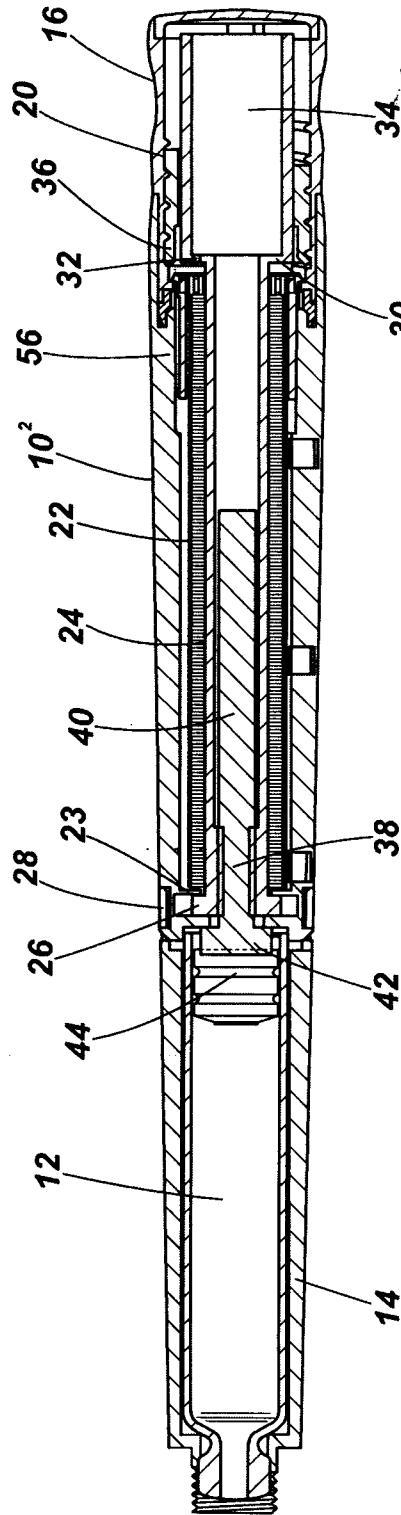


Fig. 2

10 APR 2012

Shanker
Archana Shanker
of Anand and Anand Advocates
Agent for the Applicant

ORIGINAL

2/5

3078 DELIP T2

10 APR 2012

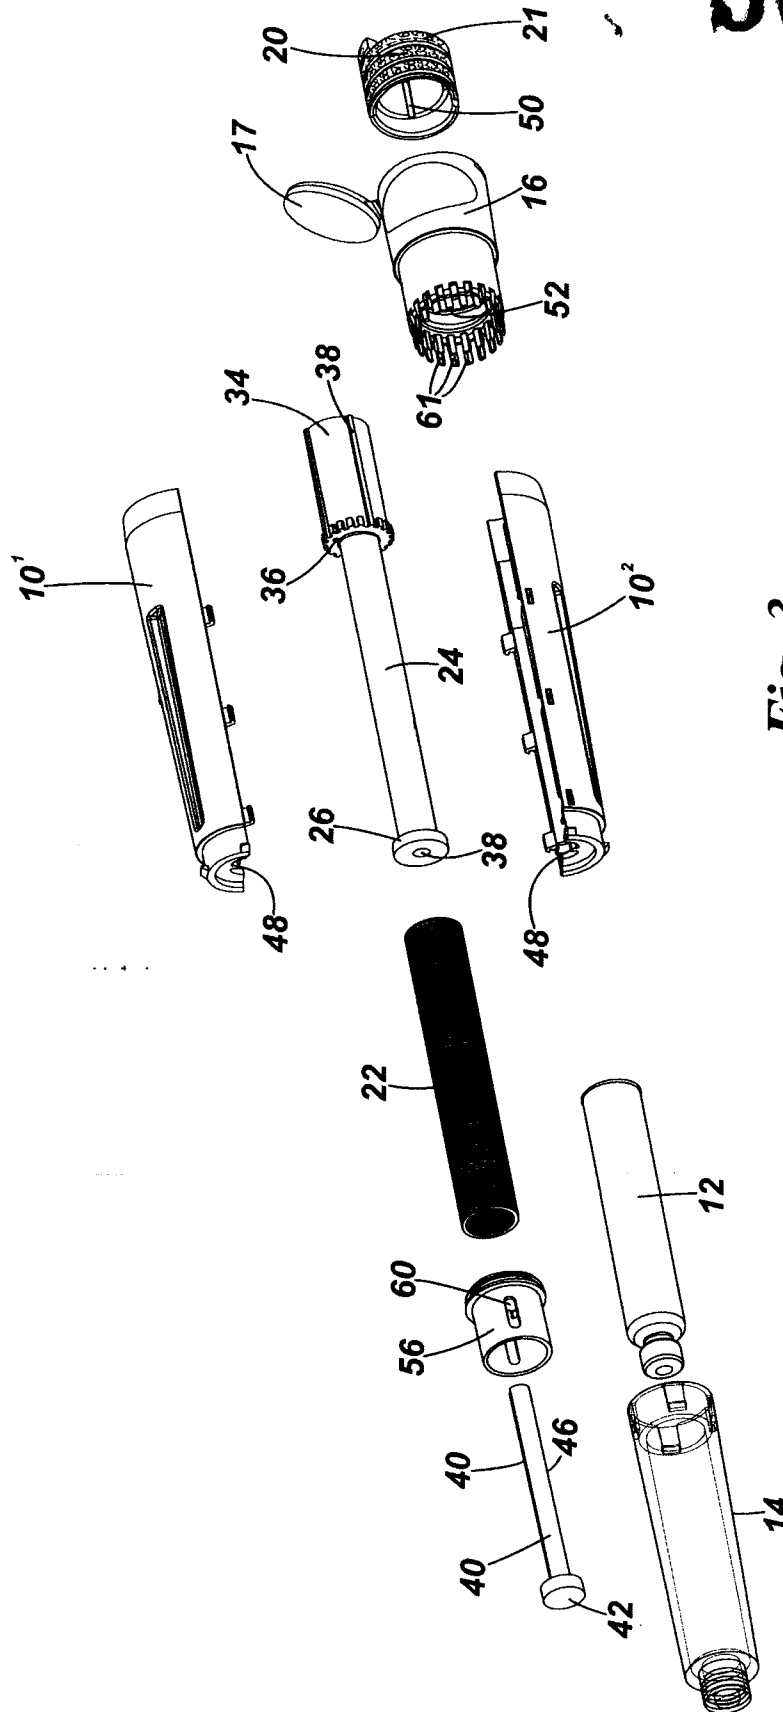


Fig. 3

Shanker
Archana Shanker
of Anand and Anand Advocates
Agent for the Applicant

ORIGINAL

3/5

3078 DELP 12

10 APR 2012

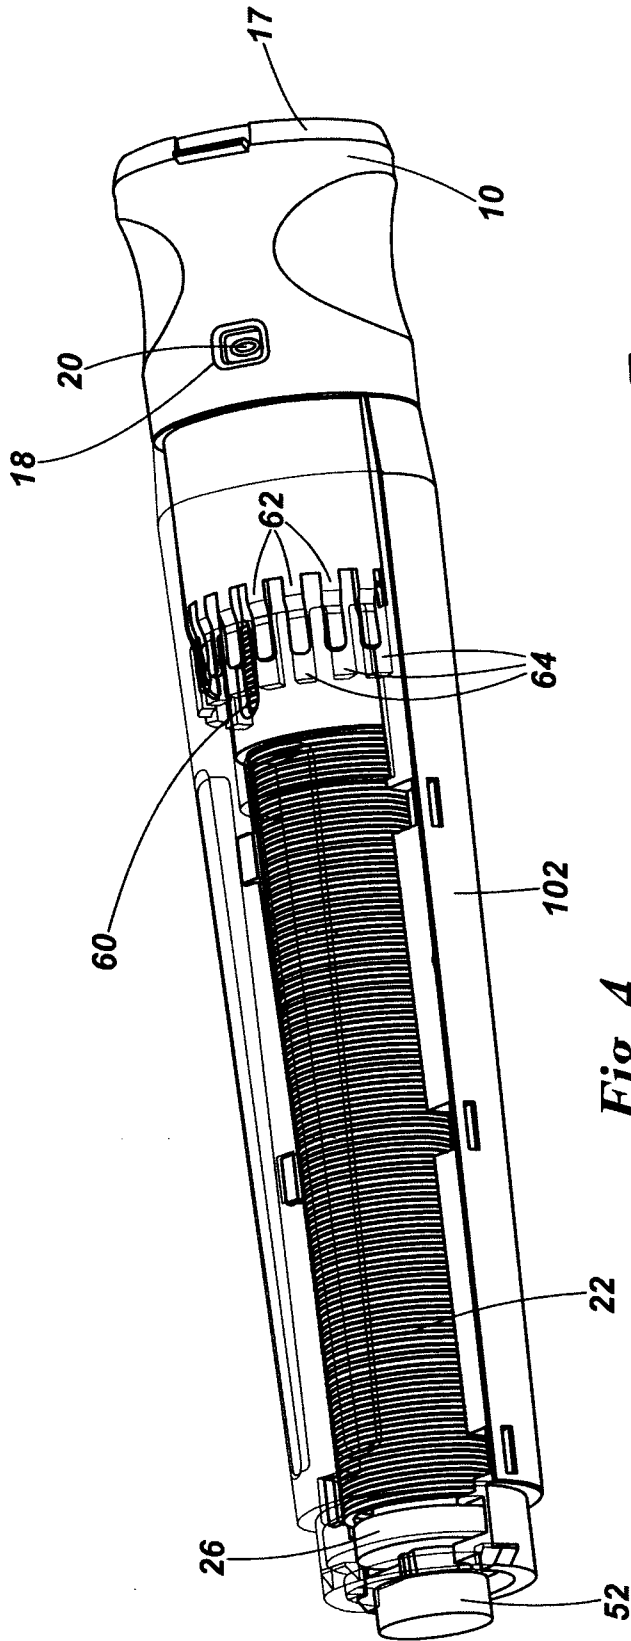


Fig. 4

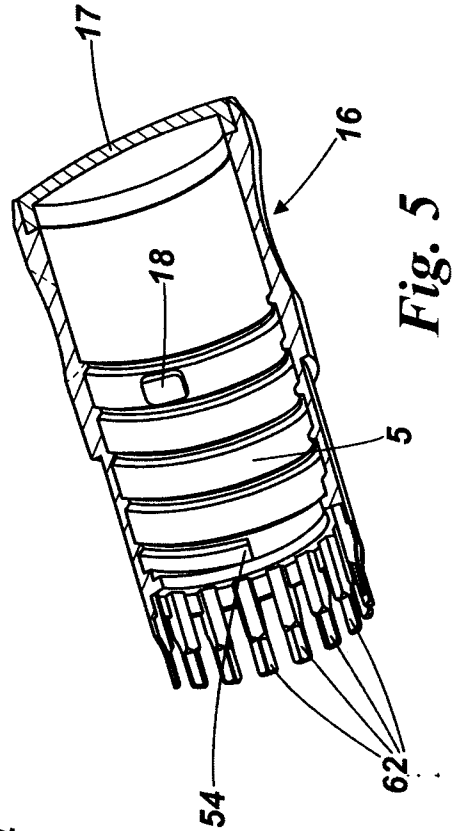


Fig. 5

Shanker

Archana Shanker
of Anand and Anand Advocates
Agent for the Applicant

ORIGINAL

4/5

3078 DELIN T2

10 APR 2012

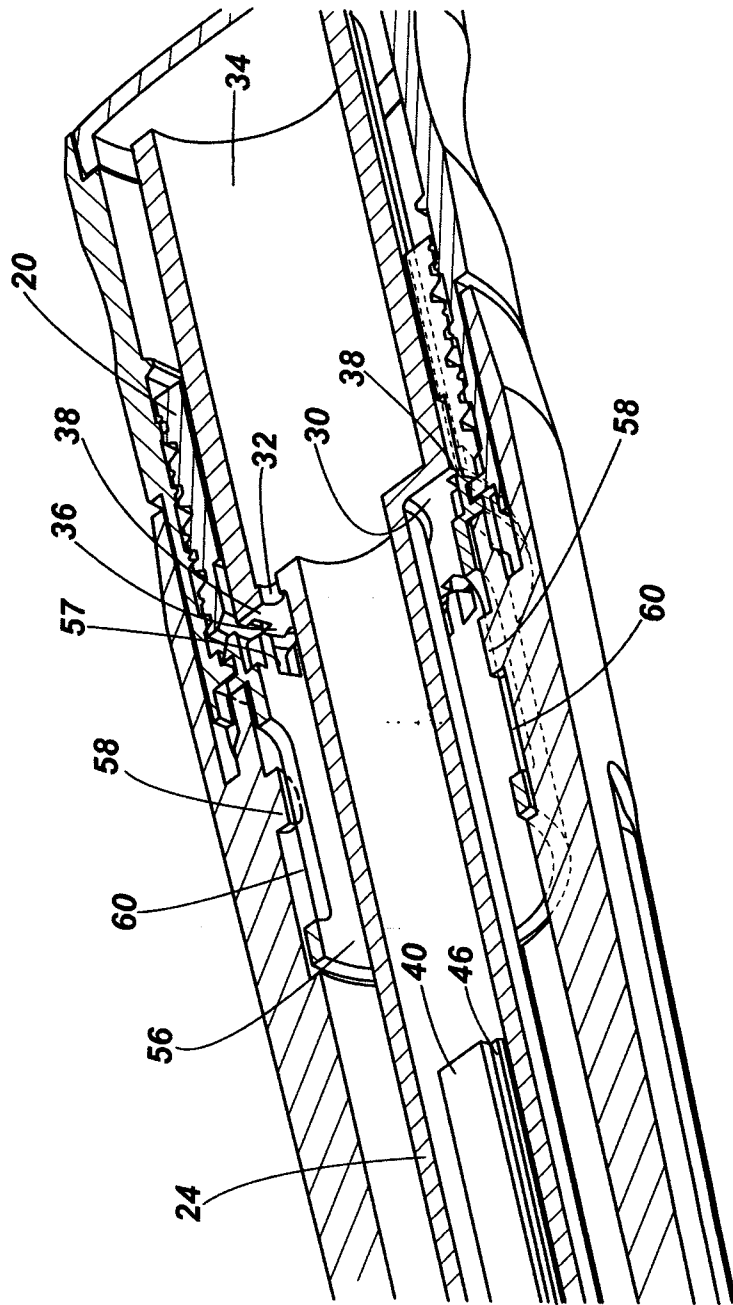


Fig. 6

Shanker

Archana Shanker
of Anand and Anand Advocates
Agent for the Applicant

ORIGINAL

5/5

3078 DELIMP 12

10 APR 2012

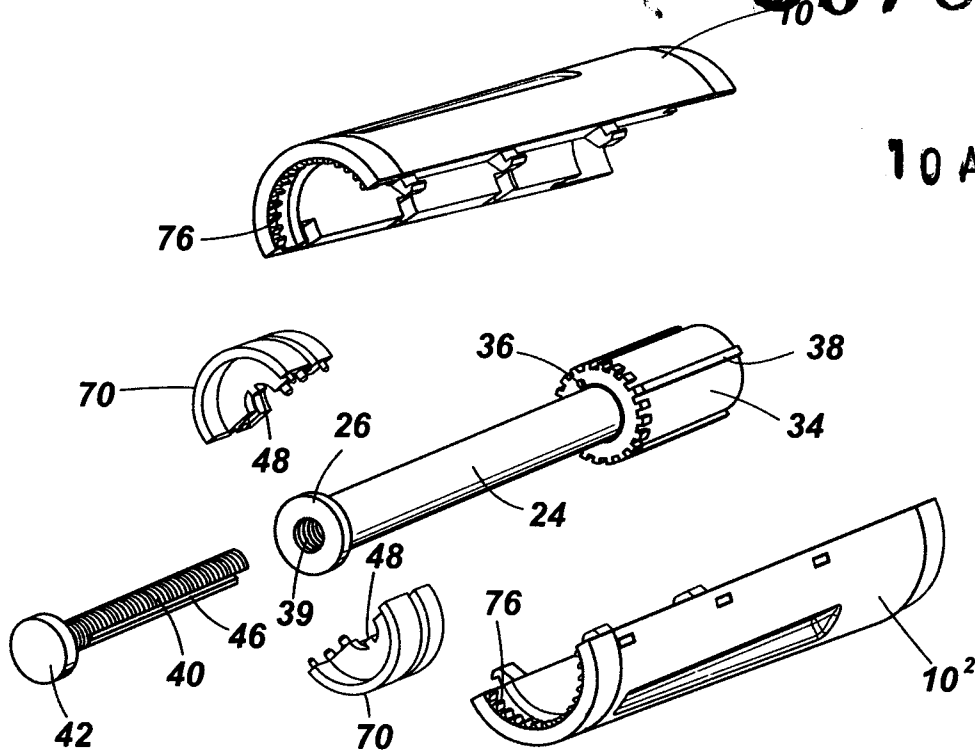


Fig. 7

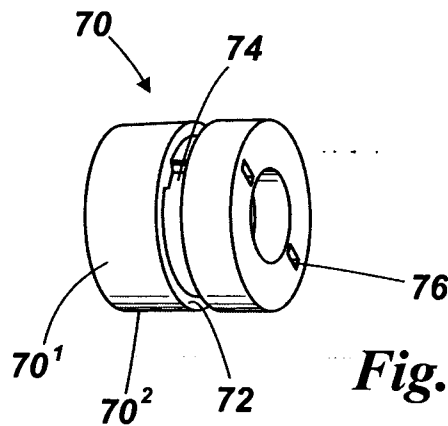


Fig. 8

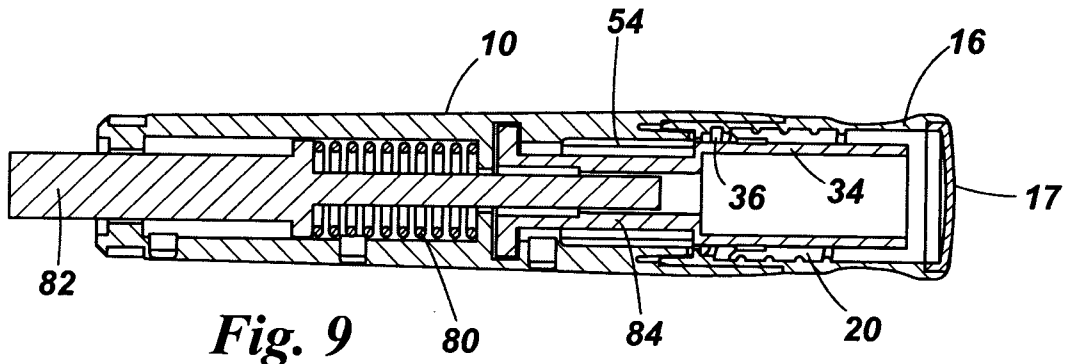


Fig. 9

Archer

Archana Shanker
of Anand and Anand Advocates
Agent for the Applicant