



US007604721B2

(12) **United States Patent**
Groll et al.

(10) **Patent No.:** **US 7,604,721 B2**
(45) **Date of Patent:** **Oct. 20, 2009**

(54) **SYSTEM AND METHOD FOR CODING INFORMATION ON A BIOSENSOR TEST STRIP**

3,770,607 A 11/1973 Williams
3,776,832 A 12/1973 Oswin et al.
3,838,033 A 9/1974 Mindt et al.
3,902,970 A 9/1975 Levin
3,919,627 A 11/1975 Allen
3,925,183 A 12/1975 Oswin et al.
3,937,615 A 2/1976 Clack et al.
3,980,437 A 9/1976 Kishimoto et al.

(75) Inventors: **Henning Groll**, Indianapolis, IN (US);
Michael J. Celentano, Fishers, IN (US)

(73) Assignees: **Roche Diagnostics Operations, Inc.**,
Indianapolis, IN (US); **Roche Operations, Ltd.**, Hamilton (BM)

(*) Notice: Subject to any disclaimer, the term of this patent is extended or adjusted under 35 U.S.C. 154(b) by 785 days.

(Continued)

FOREIGN PATENT DOCUMENTS

(21) Appl. No.: **10/871,489**

AU 737 787 8/2001

(22) Filed: **Jun. 18, 2004**

(65) **Prior Publication Data**

US 2005/0161345 A1 Jul. 28, 2005

(Continued)

Related U.S. Application Data

OTHER PUBLICATIONS

(60) Provisional application No. 60/480,199, filed on Jun. 20, 2003.

Skladal, "Compensation of Temperature Variations Disturbing Performance of an Amperometric Biosensor for Continuous Monitoring," *Sensors and Actuators B*, Elsevier Sequoia S.A., Lausanne, CH, vol. 28, No. 1, Jul. 1, 1995, pp. 59-62, XP004004390, ISSN: 0925-4005.

(51) **Int. Cl.**
C25B 11/00 (2006.01)
G01N 27/26 (2006.01)

(Continued)

(52) **U.S. Cl.** **204/403.01**; 204/403.03;
205/775

Primary Examiner—Alex Noguerola
Assistant Examiner—J. Christopher Ball
(74) *Attorney, Agent, or Firm*—Woodard, Emhardt, Moriarty, McNett & Henry LLP

(58) **Field of Classification Search** 205/775;
204/403.02, 403.01, 403.06, 403.14, 403.15
See application file for complete search history.

(56) **References Cited**


(57) **ABSTRACT**

U.S. PATENT DOCUMENTS

3,526,480 A 9/1970 Findl et al.
3,551,295 A 12/1970 Dyer
3,621,381 A 11/1971 Eckfeldt
3,715,192 A 2/1973 Wenz et al.
3,720,093 A 3/1973 Gill
3,763,422 A 10/1973 MacPhee et al.

The present invention provides a test strip for measuring a concentration of an analyte of interest in a biological fluid, wherein the test strip may be encoded with information that can be read by a test meter into which the test strip is inserted.

12 Claims, 13 Drawing Sheets

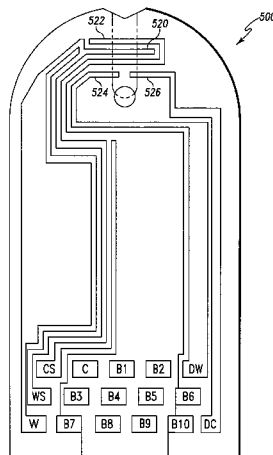

U.S. PATENT DOCUMENTS					
4,005,002 A	1/1977	Racine et al.	4,810,203 A	3/1989	Komatsu
4,008,448 A	2/1977	Muggli	4,816,224 A	3/1989	Vogel et al.
4,040,908 A	8/1977	Clark, Jr.	4,820,399 A	4/1989	Senda et al.
4,053,381 A	10/1977	Hamblen et al.	4,820,636 A	4/1989	Hill et al.
4,065,263 A	12/1977	Woodbridge, III	4,832,814 A	5/1989	Root
4,086,631 A	4/1978	Vick	4,834,234 A	5/1989	Sacherer et al.
4,123,701 A	10/1978	Josefsen et al.	4,849,330 A	7/1989	Humphries et al.
4,127,448 A	11/1978	Schick et al.	4,865,873 A	9/1989	Cole, Jr. et al.
4,184,936 A	1/1980	Paul et al.	4,877,580 A	10/1989	Aronowitz et al.
4,214,968 A	7/1980	Battaglia et al.	4,897,162 A	1/1990	Lewandowski et al.
4,217,196 A	8/1980	Huch	4,897,173 A	1/1990	Nankai et al.
4,224,125 A	9/1980	Nakamura et al.	4,919,770 A	4/1990	Preidel et al.
4,225,410 A	9/1980	Pace	4,927,516 A	5/1990	Yamaguchi et al.
4,230,537 A	10/1980	Delente et al.	4,935,105 A	6/1990	Churchouse
4,233,029 A	11/1980	Columbus	4,935,106 A	6/1990	Liston et al.
4,260,680 A	4/1981	Muramatsu et al.	4,935,346 A	6/1990	Phillips et al.
4,263,343 A	4/1981	Kim	4,938,860 A	7/1990	Wogoman
4,265,250 A	5/1981	Parker	4,940,945 A	7/1990	Littlejohn et al.
4,273,134 A	6/1981	Ricciardelli	4,954,087 A	9/1990	Lauks et al.
4,273,639 A	6/1981	Gottermeier	4,956,275 A	9/1990	Zuk et al.
4,297,569 A	10/1981	Flies	4,963,814 A	10/1990	Parks
4,301,412 A	11/1981	Hill et al.	4,970,145 A	11/1990	Bennetto et al.
4,303,887 A	12/1981	Hill et al.	4,975,647 A	12/1990	Downer et al.
4,323,536 A	4/1982	Columbus	4,976,724 A	12/1990	Nieto et al.
4,329,642 A	5/1982	Luthi et al.	4,999,582 A	3/1991	Parks et al.
4,366,033 A	12/1982	Richter et al.	4,999,632 A	3/1991	Parks
4,407,290 A	10/1983	Wilber	5,018,164 A	5/1991	Brewer et al.
4,407,959 A	10/1983	Tsuji et al.	5,019,974 A	5/1991	Beckers
4,413,407 A	11/1983	Columbus	5,035,862 A	7/1991	Dietze et al.
4,413,628 A	11/1983	Tamulis	5,039,618 A	8/1991	Stone
4,420,564 A	12/1983	Tsuji et al.	5,049,487 A	9/1991	Phillips et al.
4,431,004 A	2/1984	Bessman et al.	5,053,199 A	10/1991	Keiser et al.
4,436,094 A	3/1984	Cerami	5,059,394 A	10/1991	Phillips et al.
4,440,175 A	4/1984	Wilkins	5,066,372 A	11/1991	Weetall
4,476,149 A	10/1984	Poppe et al.	5,075,077 A	12/1991	Durley, III et al.
4,477,314 A	10/1984	Richter et al.	5,096,669 A	3/1992	Lauks et al.
4,477,575 A	10/1984	Vogel et al.	5,108,564 A	4/1992	Szuminsky et al.
4,499,423 A	2/1985	Matthiessen	5,112,455 A	5/1992	Cozzette et al.
4,510,383 A	4/1985	Ruppender	5,112,758 A	5/1992	Fellman et al.
4,517,291 A	5/1985	Seago	5,118,183 A	6/1992	Cargill et al.
4,545,382 A	10/1985	Higgins et al.	5,120,420 A	6/1992	Nankai et al.
4,547,735 A	10/1985	Kiesewetter et al.	5,122,244 A	6/1992	Hoenes et al.
4,552,458 A	11/1985	Lowne	5,126,952 A	6/1992	Kildal-Brandt et al.
4,571,292 A	2/1986	Liu et al.	5,128,015 A	7/1992	Szuminsky et al.
4,578,716 A	3/1986	van Rijckevorsel et al.	5,141,850 A	8/1992	Cole et al.
4,592,893 A	6/1986	Poppe et al.	5,141,868 A	8/1992	Shanks et al.
4,628,193 A	12/1986	Blum	5,143,694 A	9/1992	Schafer et al.
4,642,295 A	2/1987	Baker	5,179,005 A	1/1993	Phillips et al.
4,648,665 A	3/1987	Davis et al.	5,179,288 A	1/1993	Miffitt et al.
4,652,830 A	3/1987	Brown	5,182,707 A	1/1993	Cooper et al.
4,654,197 A	3/1987	Lilja et al.	5,187,100 A	2/1993	Matzinger et al.
4,671,288 A	6/1987	Gough	5,192,415 A	3/1993	Yoshioka et al.
4,676,653 A	6/1987	Strohmeier et al.	5,220,920 A	6/1993	Gharib
4,679,562 A	7/1987	Luksha	5,232,516 A	8/1993	Hed
4,682,602 A	7/1987	Prohaska	5,232,668 A	8/1993	Grant et al.
4,686,479 A	8/1987	Young et al.	5,234,813 A	8/1993	McGeehan et al.
4,703,017 A	10/1987	Campbell et al.	5,243,516 A	9/1993	White
4,703,756 A	11/1987	Gough et al.	5,246,858 A	9/1993	Arbuckle et al.
4,711,245 A	12/1987	Higgins et al.	5,250,439 A	10/1993	Musho et al.
4,713,347 A	12/1987	Mitchell et al.	5,264,103 A	11/1993	Yoshioka et al.
4,714,874 A	12/1987	Morris et al.	5,266,179 A	11/1993	Nankai et al. 204/401
4,731,726 A	3/1988	Allen, III	5,269,891 A	12/1993	Colin
4,734,184 A	3/1988	Burleigh et al.	5,279,294 A	1/1994	Anderson et al.
4,750,496 A	6/1988	Reinhart et al.	5,281,395 A	1/1994	Markart et al.
4,759,828 A	7/1988	Young et al.	5,284,770 A	2/1994	Adrian et al.
4,789,804 A	12/1988	Karube et al.	5,286,362 A	2/1994	Hoenes et al.
4,795,542 A	1/1989	Ross et al.	5,288,636 A	2/1994	Pollmann et al.
4,797,256 A	1/1989	Wattlington, IV	5,296,192 A	3/1994	Carroll et al.
4,805,624 A	2/1989	Yao et al.	5,304,468 A	4/1994	Phillips et al.
4,806,311 A	2/1989	Greenquist	5,306,623 A	4/1994	Kiser
4,806,312 A	2/1989	Greenquist	5,311,426 A	5/1994	Donohue et al.
			5,312,762 A	5/1994	Guisseppi-Elie
			5,344,754 A	9/1994	Zweig

US 7,604,721 B2

5,352,351 A	10/1994	White et al.	5,654,178 A	8/1997	Fitzpatrick et al.
5,353,351 A	10/1994	Bartoli et al.	5,656,142 A *	8/1997	Park et al. 204/403.1
5,366,609 A	11/1994	White et al.	5,656,502 A	8/1997	MacKay et al.
5,371,687 A	12/1994	Holmes, II et al.	5,658,443 A	8/1997	Yamamoto et al.
5,376,254 A	12/1994	Fisher	5,658,802 A	8/1997	Hayes et al.
5,379,214 A	1/1995	Arbuckle et al.	5,665,215 A	9/1997	Bussmann et al.
5,385,846 A	1/1995	Kuhn et al.	5,670,031 A	9/1997	Hintsche et al.
5,389,215 A	2/1995	Horiuchi et al.	5,682,884 A	11/1997	Hill et al.
5,395,504 A	3/1995	Saurer et al.	5,686,659 A	11/1997	Neel et al.
5,405,511 A	4/1995	White et al.	5,691,486 A	11/1997	Behringer et al.
5,411,647 A	5/1995	Johnson et al.	5,691,633 A	11/1997	Liu et al.
5,413,690 A	5/1995	Kost et al.	5,695,623 A	12/1997	Michel et al.
5,413,764 A	5/1995	Haar	5,698,083 A	12/1997	Glass
5,418,142 A	5/1995	Kiser et al.	5,700,695 A	12/1997	Yassinzadeh et al.
5,421,189 A	6/1995	Dussault	5,708,247 A	1/1998	McAleer et al.
5,424,035 A	6/1995	Hones et al.	5,710,622 A	1/1998	Neel et al.
5,426,032 A	6/1995	Phillips et al.	5,719,667 A	2/1998	Miers
5,437,772 A	8/1995	De Castro et al.	5,720,862 A	2/1998	Hamamoto et al.
5,437,999 A	8/1995	Diebold et al.	5,723,284 A	3/1998	Ye
5,438,271 A	8/1995	White et al.	5,727,548 A	3/1998	Hill et al.
5,439,826 A	8/1995	Kontorovich	5,728,074 A	3/1998	Castellano et al.
5,445,967 A	8/1995	Deuter	5,745,308 A	4/1998	Spangenberg
5,447,837 A	9/1995	Urnovitz	5,757,666 A	5/1998	Schreiber et al.
5,453,360 A	9/1995	Yu	5,759,794 A	6/1998	Levine et al.
5,469,846 A	11/1995	Khan	5,762,770 A	6/1998	Pritchard et al.
5,470,533 A	11/1995	Shindo et al.	5,776,710 A	7/1998	Levine et al.
5,477,326 A	12/1995	Dosmann	5,780,304 A	7/1998	Matzinger et al.
5,489,414 A	2/1996	Schreiber et al.	5,786,584 A	7/1998	Button et al.
5,494,638 A	2/1996	Gullick	5,788,833 A	8/1998	Lewis et al.
5,500,350 A	3/1996	Baker et al.	5,789,255 A	8/1998	Yu
5,504,011 A	4/1996	Gavin et al.	5,792,668 A	8/1998	Deamer et al.
5,508,171 A	4/1996	Walling et al.	5,798,031 A	8/1998	Charlton et al.
5,508,200 A	4/1996	Tiffany et al.	5,801,057 A	9/1998	Smart et al.
5,508,203 A	4/1996	Fuller et al.	5,820,551 A	10/1998	Hill et al.
5,509,410 A	4/1996	Hill et al.	5,820,622 A	10/1998	Gross et al.
5,515,170 A	5/1996	Matzinger	5,832,921 A	11/1998	Lennert et al.
5,515,847 A	5/1996	Braig et al.	5,834,217 A	11/1998	Levine et al.
5,526,111 A	6/1996	Collins et al.	5,837,546 A	11/1998	Allen et al.
5,526,120 A	6/1996	Jina et al.	5,843,691 A	12/1998	Douglas et al.
5,526,808 A	6/1996	Kaminsky	5,843,692 A	12/1998	Phillips et al.
5,532,128 A	7/1996	Eggers et al.	5,846,744 A	12/1998	Athey et al.
5,552,116 A	9/1996	Yokota et al.	5,849,174 A	12/1998	Sanghera et al.
5,554,531 A	9/1996	Zweig	5,856,195 A	1/1999	Charlton et al.
5,556,789 A	9/1996	Goerlach-Graw et al.	5,873,990 A	2/1999	Wojciechowski et al.
5,563,031 A	10/1996	Yu	5,883,378 A	3/1999	Irish et al.
5,563,042 A	10/1996	Phillips et al.	5,885,839 A	3/1999	Lingane et al.
5,569,591 A	10/1996	Kell et al.	5,890,489 A	4/1999	Elden
5,569,608 A	10/1996	Sommer	5,904,898 A	5/1999	Markart
5,572,159 A	11/1996	McFarland	5,911,872 A	6/1999	Lewis et al.
5,575,895 A	11/1996	Ikeda et al.	5,916,156 A	6/1999	Hildenbrand et al.
5,576,073 A	11/1996	Kickelhain	5,921,925 A	7/1999	Cartmell et al.
5,580,794 A	12/1996	Allen	5,922,530 A	7/1999	Yu
5,582,697 A	12/1996	Ikeda et al.	5,922,591 A	7/1999	Anderson et al.
5,593,390 A	1/1997	Castellano et al.	5,925,021 A	7/1999	Castellano et al.
5,593,739 A	1/1997	Kickelhain	5,945,341 A	8/1999	Howard, III
5,594,906 A	1/1997	Holmes, II et al.	5,948,289 A	9/1999	Noda et al.
5,597,532 A	1/1997	Connolly	5,951,836 A	9/1999	McAleer et al.
5,604,110 A	2/1997	Baker et al.	5,965,380 A	10/1999	Heller
5,605,662 A	2/1997	Heller et al.	5,968,760 A	10/1999	Phillips et al.
5,605,837 A	2/1997	Karimi et al.	5,971,923 A	10/1999	Finger
5,611,900 A	3/1997	Worden et al.	5,989,917 A	11/1999	McAleer et al.
5,620,579 A	4/1997	Genshaw et al.	5,997,817 A	12/1999	Crismore et al.
5,620,863 A	4/1997	Tomasco et al.	6,004,441 A	12/1999	Fujiwara et al.
5,628,890 A	5/1997	Carter et al.	6,013,170 A	1/2000	Meade
5,630,986 A	5/1997	Charlton et al.	6,042,714 A	3/2000	Lin et al.
5,635,362 A	6/1997	Levine et al.	6,044,285 A	3/2000	Chaiken et al.
5,635,364 A	6/1997	Clark et al.	6,045,567 A	4/2000	Taylor et al.
5,639,671 A	6/1997	Bogart et al.	6,061,128 A	5/2000	Zweig et al.
5,642,734 A	7/1997	Ruben et al.	6,071,391 A	6/2000	Gotoh et al.
5,645,798 A	7/1997	Schreiber et al.	6,087,182 A	7/2000	Jeng et al.
5,650,061 A	7/1997	Kuhr et al.	6,091,975 A	7/2000	Daddona et al.
5,650,062 A	7/1997	Ikeda et al.	6,102,872 A	8/2000	Doneen et al.
5,653,863 A	8/1997	Genshaw et al.	6,103,033 A	8/2000	Say et al.

6,120,676 A	9/2000	Heller et al.	6,338,790 B1	1/2002	Feldman et al.
6,121,009 A	9/2000	Heller et al.	6,340,428 B1	1/2002	Ikeda et al.
6,121,050 A	9/2000	Han	6,342,364 B1	1/2002	Watanabe et al.
6,126,609 A	10/2000	Keith et al.	6,349,230 B1	2/2002	Kawanaka
6,128,519 A	10/2000	Say	6,358,752 B1	3/2002	Durst et al.
6,129,823 A	10/2000	Hughes et al.	6,377,894 B1	4/2002	Deweese et al.
6,134,461 A	10/2000	Say et al.	6,377,896 B1	4/2002	Sato et al.
6,136,549 A	10/2000	Feistel	6,379,513 B1	4/2002	Chambers et al.
6,136,610 A	10/2000	Polito et al.	6,389,891 B1	5/2002	D'Angelico et al.
6,143,164 A	11/2000	Heller et al.	6,391,558 B1	5/2002	Henkens et al.
6,143,247 A	11/2000	Sheppard, Jr. et al.	6,391,645 B1	5/2002	Huang et al.
6,144,869 A	11/2000	Berner et al.	6,394,952 B1	5/2002	Anderson et al.
6,150,124 A	11/2000	Riedel	6,395,227 B1	5/2002	Kiser et al.
6,153,069 A	11/2000	Pottgen et al.	6,399,258 B2	6/2002	O'Brien et al.
RE36,991 E	12/2000	Yamamoto et al.	6,401,532 B2	6/2002	Lubbers
6,156,051 A	12/2000	Schraga	6,413,213 B1	7/2002	Essenpreis et al.
6,156,173 A	12/2000	Gotoh et al.	6,413,395 B1	7/2002	Bhullar et al.
6,159,745 A	12/2000	Roberts et al.	6,413,410 B1	7/2002	Hodges et al.
6,162,611 A	12/2000	Heller et al.	6,420,128 B1	7/2002	Ouyang et al.
6,162,639 A	12/2000	Douglas	6,444,115 B1	9/2002	Hodges et al.
6,168,563 B1	1/2001	Brown	6,447,657 B1	9/2002	Bhullar et al.
6,168,957 B1	1/2001	Matzinger et al.	6,447,659 B1 *	9/2002	Peng 204/424
6,170,318 B1	1/2001	Lewis	6,454,921 B1	9/2002	Hodges et al.
6,174,420 B1	1/2001	Hodges et al.	6,461,496 B1	10/2002	Feldman et al.
6,175,752 B1	1/2001	Say et al.	6,475,360 B1	11/2002	Hodges et al.
6,176,988 B1	1/2001	Kessler	6,475,372 B1	11/2002	Ohara et al.
6,179,979 B1	1/2001	Hodges et al.	6,484,046 B1	11/2002	Say et al.
6,180,062 B1	1/2001	Naka et al.	6,485,923 B1	11/2002	Yani et al.
6,180,416 B1	1/2001	Kurnik et al.	6,488,827 B1	12/2002	Shartle
6,193,873 B1	2/2001	Ohara et al.	6,489,133 B2	12/2002	Phillips et al.
6,197,040 B1	3/2001	LeVaughn et al.	6,491,803 B1	12/2002	Shen et al.
6,200,773 B1	3/2001	Ouyang et al.	6,491,870 B2	12/2002	Patel et al.
6,201,607 B1	3/2001	Roth et al.	6,501,976 B1	12/2002	Sohrab
6,203,952 B1	3/2001	O'Brien et al.	6,503,381 B1	1/2003	Gotoh et al.
6,206,282 B1	3/2001	Hayes, Sr. et al.	6,512,986 B1	1/2003	Harmon
6,206,292 B1	3/2001	Robertz et al.	6,514,718 B2	2/2003	Heller et al.
6,218,571 B1	4/2001	Zheng et al.	6,514,769 B2	2/2003	Lee
6,225,078 B1	5/2001	Ikeda et al.	6,521,110 B1	2/2003	Hodges et al.
6,226,081 B1	5/2001	Fantone et al.	6,521,182 B1	2/2003	Shartle et al.
6,241,862 B1	6/2001	McAleer et al.	6,525,330 B2	2/2003	Paolini et al.
6,246,330 B1	6/2001	Nielsen	6,525,549 B1	2/2003	Poellmann
6,246,966 B1	6/2001	Perry	6,526,298 B1	2/2003	Khalil et al.
6,251,260 B1	6/2001	Heller et al.	6,531,239 B2	3/2003	Heller
6,258,229 B1	7/2001	Winarta et al.	6,531,322 B1	3/2003	Jurik et al.
6,258,254 B1	7/2001	Miyamoto et al.	6,538,735 B1	3/2003	Duebendorfer et al.
6,259,937 B1	7/2001	Schulman et al.	6,540,890 B1	4/2003	Bhullar et al.
6,261,519 B1	7/2001	Harding et al.	6,540,891 B1	4/2003	Stewart et al.
6,262,749 B1	7/2001	Finger et al.	6,541,266 B2	4/2003	Modzelewski et al.
6,268,162 B1	7/2001	Phillips et al.	6,544,474 B2	4/2003	Douglas
6,270,637 B1	8/2001	Crismore et al.	6,549,796 B2	4/2003	Sohrab
6,271,044 B1	8/2001	Ballerstadt et al.	6,551,494 B1	4/2003	Heller et al.
6,272,364 B1	8/2001	Kurnik	6,555,061 B1	4/2003	Leong et al.
6,277,641 B1	8/2001	Yager	6,558,528 B1	5/2003	Matzinger
6,281,006 B1	8/2001	Heller et al.	6,560,471 B1	5/2003	Heller et al.
6,284,125 B1	9/2001	Hodges et al.	6,562,625 B2	5/2003	Modzelewski et al.
6,284,550 B1	9/2001	Carroll et al.	6,565,509 B1	5/2003	Say et al.
6,287,451 B1	9/2001	Winarta et al.	6,565,738 B1	5/2003	Henning et al.
6,287,595 B1	9/2001	Loewy et al.	6,570,390 B2	5/2003	Hirayama et al.
6,287,875 B1	9/2001	Geisberg	6,571,651 B1	6/2003	Hodges
6,294,281 B1	9/2001	Heller	6,572,822 B2	6/2003	Jurik et al.
6,295,506 B1	9/2001	Heinonen et al.	6,574,425 B1	6/2003	Weiss et al.
6,299,757 B1	10/2001	Feldman et al.	6,576,101 B1	6/2003	Heller et al.
6,300,123 B1	10/2001	Vadgama et al.	6,576,117 B1	6/2003	Iketaki et al.
6,300,142 B1	10/2001	Andrewes et al.	6,576,416 B2	6/2003	Haviland et al.
6,300,961 B1	10/2001	Finger et al.	6,576,461 B2	6/2003	Heller et al.
6,309,526 B1	10/2001	Fujiwara et al.	6,579,690 B1	6/2003	Bonnecaze et al.
6,315,951 B1	11/2001	Markart	6,591,125 B1	7/2003	Buse et al.
6,316,264 B1	11/2001	Corey et al.	6,592,744 B1	7/2003	Hodges et al.
6,325,917 B1	12/2001	Maxwell et al.	6,592,745 B1	7/2003	Feldman et al.
6,326,160 B1	12/2001	Dunn et al.	6,594,514 B2	7/2003	Berner et al.
6,329,161 B1	12/2001	Heller et al.	6,599,406 B1	7/2003	Kawanaka et al.
6,330,464 B1	12/2001	Colvin, Jr. et al.	6,600,997 B2	7/2003	Deweese et al.
6,335,203 B1	1/2002	Patel et al.	6,605,200 B1	8/2003	Mao et al.

6,605,201 B1	8/2003	Mao et al.	2002/0175075 A1	11/2002	Deng et al.
6,607,658 B1	8/2003	Heller et al.	2002/0175087 A1	11/2002	Hodges et al.
6,616,819 B1	9/2003	Liamos et al.	2002/0177788 A1	11/2002	Hodges et al.
6,618,934 B1	9/2003	Feldman et al.	2002/0179440 A1	12/2002	Tokunaga et al.
6,623,501 B2	9/2003	Heller et al.	2002/0179441 A1	12/2002	Yamanishi et al.
6,627,057 B1	9/2003	Bhullar et al.	2002/0179442 A1	12/2002	Miyazaki et al.
6,632,349 B1	10/2003	Hodges et al.	2002/0185385 A1	12/2002	Charlton
6,638,415 B1	10/2003	Hodges et al.	2002/0189941 A1	12/2002	Katsuki et al.
6,638,716 B2	10/2003	Heller et al.	2003/0000834 A1	1/2003	Yoshioka et al.
6,645,359 B1	11/2003	Bhullar et al.	2003/0024811 A1	2/2003	Davies et al.
6,654,625 B1	11/2003	Say et al.	2003/0032875 A1	2/2003	Taniike et al.
6,656,702 B1	12/2003	Yugawa et al.	2003/0036202 A1	2/2003	Teodorczyk et al.
6,676,995 B2	1/2004	Dick et al.	2003/0042137 A1	3/2003	Mao et al.
6,689,411 B2	2/2004	Dick et al.	2003/0042150 A1	3/2003	Ryu et al.
6,814,844 B2	11/2004	Bhullar et al.	2003/0054427 A1	3/2003	Phillips et al.
6,875,327 B1	4/2005	Miyazaki et al.	2003/0064525 A1	4/2003	Liess
7,041,206 B2	5/2006	Gephart et al.	2003/0073151 A1	4/2003	Phillips et al.
2001/0006149 A1	7/2001	Taniike et al.	2003/0073152 A1	4/2003	Phillips et al.
2001/0006150 A1	7/2001	Taniike et al.	2003/0073153 A1	4/2003	Phillips et al.
2001/0017269 A1	8/2001	Heller et al.	2003/0079987 A1	5/2003	Hodges et al.
2001/0019831 A1	9/2001	Phillips et al.	2003/0080001 A1	5/2003	Hodges et al.
2001/0034068 A1	10/2001	Spivey et al.	2003/0088166 A1	5/2003	Say et al.
2001/0039057 A1	11/2001	Douglas et al.	2003/0094383 A1	5/2003	Kermani
2001/0041830 A1	11/2001	Varalli et al.	2003/0098233 A1	5/2003	Kermani et al.
2001/0042683 A1	11/2001	Musho et al.	2003/0098234 A1	5/2003	Hasegawa et al.
2001/0052470 A1	12/2001	Hodges et al.	2003/0100030 A1	5/2003	Nadaoka et al.
2001/0053535 A1	12/2001	Ladisch et al.	2003/0100040 A1	5/2003	Bonnecaze et al.
2001/0054319 A1	12/2001	Heller et al.	2003/0100821 A1	5/2003	Heller et al.
2001/0055784 A1	12/2001	Noda et al.	2003/0102213 A1	6/2003	Gotoh et al.
2002/0003087 A1	1/2002	Chih-hui	2003/0106809 A1	6/2003	Kermani et al.
2002/0004196 A1	1/2002	Whitson	2003/0108976 A1	6/2003	Braig et al.
2002/0008038 A1	1/2002	Heller et al.	2003/0109798 A1	6/2003	Kermani
2002/0019707 A1	2/2002	Cohen et al.	2003/0132110 A1	7/2003	Hasegawa et al.
2002/0023489 A1	2/2002	Reimelt et al.	2003/0134347 A1	7/2003	Heller et al.
2002/0025469 A1	2/2002	Heller	2003/0143113 A2	7/2003	Yuzhakov et al.
2002/0029058 A1	3/2002	LeVaughn et al.	2003/0143116 A1	7/2003	Zheng et al.
2002/0033345 A1	3/2002	Meade	2003/0146110 A1	8/2003	Karinka et al.
2002/0040850 A1	4/2002	Liu et al.	2003/0150724 A1	8/2003	Kawanaka et al.
2002/0042090 A1	4/2002	Heller et al.	2003/0152823 A1	8/2003	Heller
2002/0043471 A1	4/2002	Ikeda et al.	2003/0155237 A1	8/2003	SurrIDGE et al.
2002/0044890 A1	4/2002	Black	2003/0155538 A1	8/2003	Siepmann
2002/0053523 A1	5/2002	Liamos et al.	2003/0159944 A1	8/2003	Pottgen et al.
2002/0081588 A1	6/2002	De Lumley-woodyear et al.	2003/0159945 A1	8/2003	Miyazaki et al.
2002/0082797 A1	6/2002	Deweese et al.	2003/0164293 A1	9/2003	Hodges et al.
2002/0084184 A1	7/2002	Chambers et al.	2003/0167862 A1	9/2003	Hodges
2002/0084196 A1	7/2002	Liamos et al.	2003/0168338 A1	9/2003	Gao et al.
2002/0092612 A1	7/2002	Davies et al.	2003/0175841 A1	9/2003	Watanabe et al.
2002/0100685 A1	8/2002	Huang et al.	2003/0175946 A1	9/2003	Tokunaga et al.
2002/0102739 A1	8/2002	Nomura et al.	2003/0176183 A1	9/2003	Drucker et al.
2002/0112969 A1	8/2002	Hodges et al.	2003/0178322 A1	9/2003	Iyengar et al.
2002/0117404 A1	8/2002	Maxwell et al.	2003/0179914 A1	9/2003	Tokunaga
2002/0117639 A1	8/2002	Paolini et al.	2003/0180183 A1	9/2003	Fukuoka et al.
2002/0125145 A1	9/2002	Ohara et al.	2003/0187338 A1	10/2003	Say et al.
2002/0130042 A1	9/2002	Moerman et al.	2003/0188427 A1	10/2003	Say et al.
2002/0130043 A1	9/2002	Hodges et al.	2003/0190069 A1	10/2003	Nikitin et al.
2002/0133064 A1	9/2002	Ueno et al.	2003/0199744 A1	10/2003	Buse et al.
2002/0137200 A1	9/2002	Takahashi et al.	2003/0199893 A1	10/2003	Boecker et al.
2002/0137230 A1	9/2002	Nadaoka et al.	2003/0201194 A1	10/2003	Heller et al.
2002/0138275 A1	9/2002	Amano et al.	2003/0203498 A1	10/2003	Neel et al.
2002/0138356 A1	9/2002	Dutta et al.	2003/0203503 A1	10/2003	Fukuoka et al.
2002/0139692 A1	10/2002	Tokunaga et al.	2003/0217918 A1	11/2003	Davies et al.
2002/0146835 A1	10/2002	Modzelewski et al.	2004/0005721 A1	1/2004	Tanike et al.
2002/0148726 A1	10/2002	Yamamoto et al.	2004/0016642 A1	1/2004	Miyazaki et al.
2002/0148739 A2	10/2002	Liamos et al.	2004/0020777 A1	2/2004	Miyamoto et al.
2002/0150930 A1	10/2002	Nadaoka et al.	2004/0106941 A1	6/2004	Roe et al.
2002/0152793 A1	10/2002	Sato et al.	2004/0134779 A1	7/2004	Hsu et al.
2002/0155030 A1	10/2002	Matsuda et al.	2004/0216516 A1*	11/2004	Sato 73/64.56
2002/0155615 A1	10/2002	Novikov et al.	2006/0070878 A1*	4/2006	Wu et al. 204/403.01
2002/0157948 A2	10/2002	Liamos et al.			
2002/0160517 A1	10/2002	Modzelewski et al.			
2002/0164822 A1	11/2002	Takahashi et al.			
2002/0168290 A1	11/2002	Yuzhakov et al.			
2002/0168298 A1	11/2002	Huhn et al.			
			DE	40 11 428 A1	11/1990
			EP	0 010 456	4/1980
			FOREIGN PATENT DOCUMENTS		

US 7,604,721 B2

EP	0 034 049	8/1981	EP	1 413 879	4/2004
EP	0 057 110	8/1982	EP	1 431 758 A1	6/2004
EP	0 164 180	12/1985	GB	2 295 676	6/1996
EP	0 171 148	2/1986	GB	2 365 123	2/2002
EP	0 171 239	2/1986	JP	91-59644	6/1997
EP	0 186 286	7/1986	JP	10 332626	12/1998
EP	0 241 309 A2	10/1987	JP	2000 019147	1/2000
EP	0 287 883	10/1988	JP	2001-021526	* 1/2001
EP	0 359 831	3/1990	WO	WO 81/01794	7/1981
EP	0 206 218 B1	6/1991	WO	WO 83/00926	3/1983
EP	0 471 986 A2	2/1992	WO	WO 89/08713	9/1989
EP	0 471 986 A3	4/1992	WO	WO 90/05293	5/1990
EP	0 255 291 B1	6/1992	WO	WO 92/01928	2/1992
EP	0 546 536	6/1993	WO	WO 92/07655	5/1992
EP	0 537 761 A3	2/1994	WO	WO 92/15859	9/1992
EP	0 417 796 B1	11/1994	WO	WO 92/15861	9/1992
EP	0 213 343 B2	2/1995	WO	WO 92/15950	9/1992
EP	0 636 880 A2	2/1995	WO	WO 92/22669	12/1992
EP	0 640 832 A	3/1995	WO	WO 93/09433	5/1993
EP	0 651 250 A2	5/1995	WO	WO 94/12950	6/1994
EP	0 471 986 B1	10/1995	WO	WO 94/16095	7/1994
EP	0 127 958 B2	4/1996	WO	WO 94/23295	10/1994
EP	0 732 406 A1	9/1996	WO	WO 94/28414	12/1994
EP	0 732 590 A2	9/1996	WO	WO 94/29705	12/1994
EP	0 383 322 B1	2/1997	WO	WO 95/03542	2/1995
EP	0 537 761 B1	8/1997	WO	WO 95/06919	3/1995
EP	0 840 122 A2	5/1998	WO	WO 95/07050	3/1995
EP	0 851 224	7/1998	WO	WO 95/22597	8/1995
EP	0 859 230	8/1998	WO	WO 96/04398	2/1996
EP	0 837 320 A3	12/1998	WO	WO 96/07908	3/1996
EP	0 887 421 A1	12/1998	WO	WO 96/13707	5/1996
EP	0 894 509 A2	2/1999	WO	WO 96/15454	5/1996
EP	0 470 649 B1	6/1999	WO	WO 96/33403	10/1996
EP	0 942 278 A2	9/1999	WO	WO 97/00441	1/1997
EP	0 964 059	12/1999	WO	WO 97/02487	1/1997
EP	0 987 544	3/2000	WO	WO 97/08544	3/1997
EP	1 024 358 A1	8/2000	WO	WO 97/16726	5/1997
EP	1024358 A1 *	8/2000	WO	WO 97/18465	5/1997
EP	1 035 216 A1	9/2000	WO	WO 97/29366	8/1997
EP	0 230 472 B2	12/2000	WO	WO 97/29847	8/1997
EP	1 067 384 A2	1/2001	WO	WO 97/30344	8/1997
EP	1 074 832 A1	2/2001	WO	WO 97/39341	10/1997
EP	1 081 490 A1	3/2001	WO	WO 97/39343	10/1997
EP	1 130 390 A1	9/2001	WO	WO 97/42882	11/1997
EP	0 741 186 B1	10/2001	WO	WO 97/42888	11/1997
EP	1 143 245	10/2001	WO	WO 98/05424	2/1998
EP	1 147 739 A2	10/2001	WO	WO 98/19153	5/1998
EP	1 152 239 A1	11/2001	WO	WO 98/19159	5/1998
EP	1 156 324	11/2001	WO	WO 98/35225	8/1998
EP	1 225 448	7/2002	WO	WO 98/55853	12/1998
EP	1 235 069 A1	8/2002	WO	WO 98/57159	12/1998
EP	0 958 495	11/2002	WO	WO 99/05966	2/1999
EP	1 102 991 B1	11/2002	WO	WO 99/09404	2/1999
EP	1 256 798	11/2002	WO	WO 99/12008	3/1999
EP	1 275 732	1/2003	WO	WO 99/12021	3/1999
EP	1 281 955	2/2003	WO	WO 99/13099	3/1999
EP	1 009 850 B1	3/2003	WO	WO 99/13100	3/1999
EP	1 288 653 A1	3/2003	WO	WO 99/05516	4/1999
EP	1 312 919 A2	5/2003	WO	WO 99/22236	5/1999
EP	1 316 367	6/2003	WO	WO 99/23479	5/1999
EP	1 318 396 A1	6/2003	WO	WO 99/29230	6/1999
EP	0 876 506	7/2003	WO	WO 99/30152	6/1999
EP	1 129 211 B1	7/2003	WO	WO 99/32881	7/1999
EP	1 308 720 A1	7/2003	WO	WO 99/39627	8/1999
EP	1 324 025 A2	7/2003	WO	WO 99/41596	8/1999
EP	1 324 038	7/2003	WO	WO 99/57317	11/1999
EP	1 327 881	7/2003	WO	WO 99/58709	11/1999
EP	1 352 611 A1	10/2003	WO	WO 99/59464	11/1999
EP	1 352 969	10/2003	WO	WO 99/60383	11/1999
EP	1 369 684	12/2003	WO	WO 99/64620	12/1999
EP	1 369 687	12/2003	WO	WO 00/09996	2/2000
EP	1 119 637	3/2004	WO	WO 00/10007	2/2000
EP	1394535	3/2004	WO	WO 00/20626	4/2000

WO	WO 00/26638	5/2000
WO	WO 00/28068	5/2000
WO	WO 00/33072	6/2000
WO	WO 00/33074	6/2000
WO	WO 00/42422	7/2000
WO	WO 00/45160	8/2000
WO	WO 00/54047	9/2000
WO	WO 00/57177	9/2000
WO	WO 00/60340	10/2000
WO	WO 00/73778	12/2000
WO	WO 00/73785 A2	12/2000
WO	WO 00/78917 A1	12/2000
WO	WO 00/078992	12/2000
WO	WO 01/02093 A2	1/2001
WO	WO 01/25775	4/2001
WO	WO 01/28423	4/2001
WO	WO 01/30915	5/2001
WO	WO 01/33216 A1	5/2001
WO	WO 01/36430	5/2001
WO	WO 01/36660	5/2001
WO	WO 01/46457 A2	6/2001
WO	WO 01/57238	8/2001
WO	WO 01/57239	8/2001
WO	WO 01/57510	8/2001
WO	WO 01/64105	9/2001
WO	WO 01/67099 A1	9/2001
WO	WO 01/71328 A1	9/2001
WO	WO 01/71329	9/2001
WO	WO 01/72220	10/2001
WO	WO 01/73109	10/2001
WO	WO 01/73114	10/2001
WO	WO 01/73124	10/2001
WO	WO 01/73395	10/2001
WO	WO 01/74242	10/2001
WO	WO 01/75433	10/2001
WO	WO 01/75438 A2	10/2001
WO	WO 01/84142	11/2001
WO	WO 01/88524	11/2001
WO	WO 01/92857	12/2001
WO	WO 01/95806	12/2001
WO	WO 01/96596	12/2001
WO	WO 02/00112 A2	1/2002
WO	WO 02/06822	1/2002
WO	WO 02/08750	1/2002
WO	WO 02/08753 A2	1/2002
WO	WO 02/10728	2/2002
WO	WO 02/13966	2/2002
WO	WO 02/13970	2/2002
WO	WO 02/14535	2/2002
WO	WO 02/18053 A1	3/2002
WO	WO 02/22855	3/2002
WO	WO 02/32559	4/2002
WO	WO 02/48707	6/2002
WO	WO 02/49507	6/2002
WO	WO 02/50609	6/2002
WO	WO 02/054055 A1	7/2002
WO	WO 02/057781	7/2002
WO	WO 02/058537	8/2002
WO	WO 02/062212	8/2002
WO	WO 02/067768	9/2002
WO	WO 02/070734 A1	9/2002
WO	WO 02/071044	9/2002
WO	WO 02/078512 A2	10/2002
WO	WO 02/078533	10/2002
WO	WO 02/093152	11/2002
WO	WO 02/095355	11/2002
WO	WO 03/005015	1/2003
WO	WO 03/012422	2/2003
WO	WO 03/015627	2/2003
WO	WO 03/015629	2/2003
WO	WO 03/025257	3/2003
WO	WO 03/032411	4/2003
WO	WO 2003/029804 A1	4/2003

WO	WO 03/039483 A2	5/2003
WO	WO 03/060154 A2	7/2003
WO	WO 03/067252	8/2003
WO	WO 03/069304 A2	8/2003
WO	WO 03/083469	10/2003
WO	WO 03/085372	10/2003
WO	WO 03/091717	11/2003

OTHER PUBLICATIONS

Aoki et al., "Quantitative Analysis of Reversible Diffusion Controlled Currents of Redox Soluble Species At Interdigitated Array Electrodes Under Steady-State Conditions", *J. Electroanal. Chem.* 256 (1988) 269-282.

Aoki et al., "Time-Dependence of Diffusion-Controlled Currents of A Soluble Redox Couple At Interdigitated Microarray Electrodes". *J. Electroanal. Chem.* 266 (1989) 11-20.

Bartlett, P.N. and Whitaker, R.G., "Electrochemical Immobilisation of Enzymes: Part I. Theory", *J. Electroanal. Chem.*, 224 (1987) 27-35.

Bartlett, P.N. and Whitaker, R.G., "Electrochemical Immobilisation of Enzymes: Part II. Glucose Oxidase Immobilised in Poly-N-Methylpyrrole", *J. Electroanal. Chem.*, 224 (1987) 37-48.

Beyer et al., "Development and Application of a New Enzyme Sensor Type Based on the EIS-Capacitance Structure for Bioprocess Control," *Biosensors & Bioelectronics*, vol. 9, pp. 17-21 (1994).

Bradley et al., "Kinetic Analysis of Enzyme Electrode Response," *Anal. Chem.*, vol. 56, pp. 664-667 (1984).

Burke, et al., Improved-Accuracy Biosensor Strip For AccuChek™ Advantage ®, Presented Orally At ACS Boston Meeting (~1993-1994).

Cardosi et al., The Realization of Electron Transfer from Biological Molecules to Electrodes, *Biosensors Fundamentals and Applications*, chapt. 15 (Turner et al. eds., Oxford University Press. 1987).

Cass et al., "Ferrocene-Mediated Enzyme Electrode for Amperometric Determination of Glucose," *Anal. Chem.*, vol. 56, pp. 667-671 (1984).

Chiba, K.; Ohsaka, T.; Ohnuki, Y.; and Oyama, N., "Electrochemical Preparation of A Ladder Polymer Containing Phenazine Rings." *J. Electroanal. Chemo.*, 219 (1987) 117-124.

Gebhardt, et al., "Electrocatalytic Glucose Sensor," *Siemens Forschung, Entwickl.-Ber. Bd.*, vol. 12, pp. 91-95 (1983).

Gregg, et al., "Cross-Lined Redox Gels Containing Glucose Oxidase For Amperometric Biosensor Applications", *Anal. Chem.* 1990, 62, 258-263.

Hintsche, R. et al., "Chip Biosensors On Thin-Film Metal Electrodes", *Sensors and Actuators B.* 4 (1991) 287-291.

Ho et al., "Electrochemical Sensor for Measurement of Urea and Creatinine in Serum Based on AC Impedance Measurement of Enzyme-Catalyzed Polymer Transformation." *Analytical Chemistry*, vol. 71, No. 10, May 15, 1999.

Jin et al., "Application Of The Finite Analytic Numerical Method. Part 1. Diffusion Problems On Coplanar an dElevated Interdigitated Microarray Band Electrodes" *J. Electroanal. Chem.* 441 (1996) 29-36.

Kasapbasioglu et al., "An Impedance Based Ultra-Thin Platinum Island Film Glucose Sensor," *Sensor and Actuators B.* vol. 13-14, pp. 749-451 (1993).

Koichi, "Measurements of Current-Potential Curves, 6, Cottrell Equation and its Analogs. What Can We Known from Chronoamperometry?" *Denki Kagaku ovopi Kogyo Butsuri Kagaku*, vol. 54, No. 6, pp. 471-5 (1986).

Lambda Physik Brochure For LPX® Series.

Lee, et al., "A New Glucose Sensor Using Microporous Enzyme Membrane", *Sensors and Actuators B*, 3 (1991) 215-219.

Lifescan Guide Entitled "Quick Start" For The Onetouch® Ultra™ Blood Glucose Monitoring System.

Lifescan Owner's Booklet Entitled "The Comfort of Control".

Lifescan Product Brochure For Onetouch® Ultra™ Blood Glucose Monitoring System.

Lifescan Product Brochure For Onetouch® Ultra™ Test Strip.

- Malitesta, et al., "Glucose Fast-Response Amperometric Sensor Based On Glucose Oxidase Immobilized In An Electropolymerized Poly (O-Phenylenediamine) Film", *Anal. Chem.* 1990, 62, 2735-2740.
- Meier, et al., "Sensor and Sensor Elements Manufacturing: Laser Direct Patterning (LDP) for Reel to Reel Processing to generate High Throughput", LPKF Laser & Electronics AG, pp. 1-6.
- Mell, et al., "A Model for the Amperometric Enzyme Electrode Obtained Through Digital Simulation and Applied to the immobilized Glucose Oxidase System," *Analytical Chemistry*, vol. 47, pp. 299-307 (Feb. 1975).
- Mell et al., "Amperometric Response Enhancement of the Immobilized Glucose Oxidase Enzyme Electrode", *Analytical Chemistry*, vol. 48, pp. 1597-1601 (Sep. 1976).
- Miao et al., "Amperometric Glucose Biosensor Based On Immobilization of Glucose Oxidase In Chitosan dMatrix Cross-Linked With Glutaraldehyde", *Electroanalysis* 2001, 13, No. 4, 347-349.
- Mohri, et al., "Characteristic Response of Electrochemical Nonlinearity to Taste Compounds with a Gold Electrode Modified with 4-Aminobenzenethiol," *Bull. Chem. Soc. Jpn.*, vol. 66, pp. 1328-1332 (1993).
- Morris, et al., "An Electrochemical Capillary Fill Device for the Analysis of Glucose Incorporating Glucose Oxidase and Ruthenium (III) Hexamine as Mediator," *Electroanalysis*, vol. 4, pp. 1-9 (1992).
- Muller et al., "Influence of Hematocrit and Platelet Count on Impedance and Reactivity of Whole Blood for Electrical Aggregometry," *Journal of Pharmacological and Toxicological Methods*, vol. 34, pp. 17-22 (1995).
- Myland et al., "Membrane-Covered Oxygen Sensors: An Exact Treatment of the Switch-on Transient," *Journal of the Electrochemical Society*, vol. 131, pp. 1815-1823 (Aug. 1984).
- Nishihara et al., "Interdigitated Array Electrode Diffusion Measurements in Donor/Acceptor Solutions in Polyether Electrolyte Solvents", *Anal. Chem.* 1991, 63, 2955-2960.
- Niwa et al., "Electrochemical Behavior Of Reversible Redox Species At Interdigitated Array Electrodes With Different Geometries: Consideration Of Redox Cycling and Collection Efficiency" *Anal. Chem.* 62 (1990) 447-452.
- Paeschke et al., "Properties of Interdigital Electrode Arrays With Different Geometries", *Analytica Chimica Acta* 305 (1995) 126-136.
- Preidel et al. "Glucose Measurements by Electrocatalytic Sensor in the Extracorporeal Blood Circulation of a Sheep," *Sensors and Actuators B*, vol. 2, pp. 257-263 (1990).
- Preidel et al. "In Vitro Measurements with Electrocatalytic Glucose Sensor in Blood," *Biomed. Biochim. Acta*, vol. 48, pp. 897-903 (1989).
- Saeger et al., "Influence of Urea on the Glucose Measurement by Electrocatalytic Sensor in the Extracorporeal Blood Circulation of a Sheep," *Biomed. Biochim. Acta*, vol. 50, pp. 885-891 (1991).
- Talbott, et al., "A New Microchemical Approach to Amperometric Analysis," *Microchemical Journal*, vol. 37, pp. 5-12 (1988).
- Tender et al., "Electrochemical Patterning of Self-Assembled Monolayers onto Microscopic Arrays of Gold Electrodes Fabricated by Laser Ablation," *American Chemical Society, Langmuir*, vol. 12, No. 23, pp. 5515-5518, (1996).
- Vorburger et al., "In the Rough," *National Institute of Standards and Technology, and Ndubuisi Orji, University of North Carolina, Spie's oe magazine*, pp. 31-34, (2002).
- Williams et al., "Electrochemical-Enzymatic Analysis of Blood Glucose and Lactate," *Analytical Chemistry*, vol. 42, No. 1, pp. 118-121 (Jan. 1970).
- Wollenberger et al., "Interdigitated Array Microelectrodes For The Determination Of Enzyme Activities", *Analyst*, Jun. 1994, 1245-1249.
- Zhao, "Contributions of Suspending Medium to Electrical Impedance of Blood," *Biochimica et Biophysica Acta*, vol. 1201, pp. 179-185 (1994).
- Zhao, "Electrical Impedance and Haematocrit of Human Blood with Various Anticoagulants," *Physiol. Meas.*, vol. 14, pp. 299-307 (1993).
- <http://216.239.41.104/search?q=cache:oNNpSzoOXvgJ:www.future-fab.com,+Introduction>, Future Fab International, Montgomery Research, Inc., pp. 1-10, (Jan. 2004).
- <http://216.239.41.104/search?q=cache:bEmigi1MhtUJ:www.coe.uncc.edu,+LER>, Ndubuisi George Orji, pp. 1-3 (Jan. 2004).
- <http://www.circuitree.com>, Vaucher et al., "Laser Direct Imaging and Structuring: An Update", posted on Aug. 2002, pp. 1-6 (Nov. 2003).
- <http://www.ifm.liu.se/Applphys/ftir/sams.html>, "Self-Assembled Monolayers", pp. 1-5 (Jan. 2004).
- <http://www.tamsci.com/library/news-05-DECEMBER-2002.html>, "Patterning Thin Film Circuits at the Speed of Light", Press Release, pp. 1-2 (Nov. 2003).
- <http://www.zurich.ibm.com/~bmi/samtech.html>, "Technological Application of Self-Assembled Monolayers", pp. 1-2 (Jan. 2004).
- US 6,517,703, 02/2003, Beaty et al. (withdrawn)
- * cited by examiner

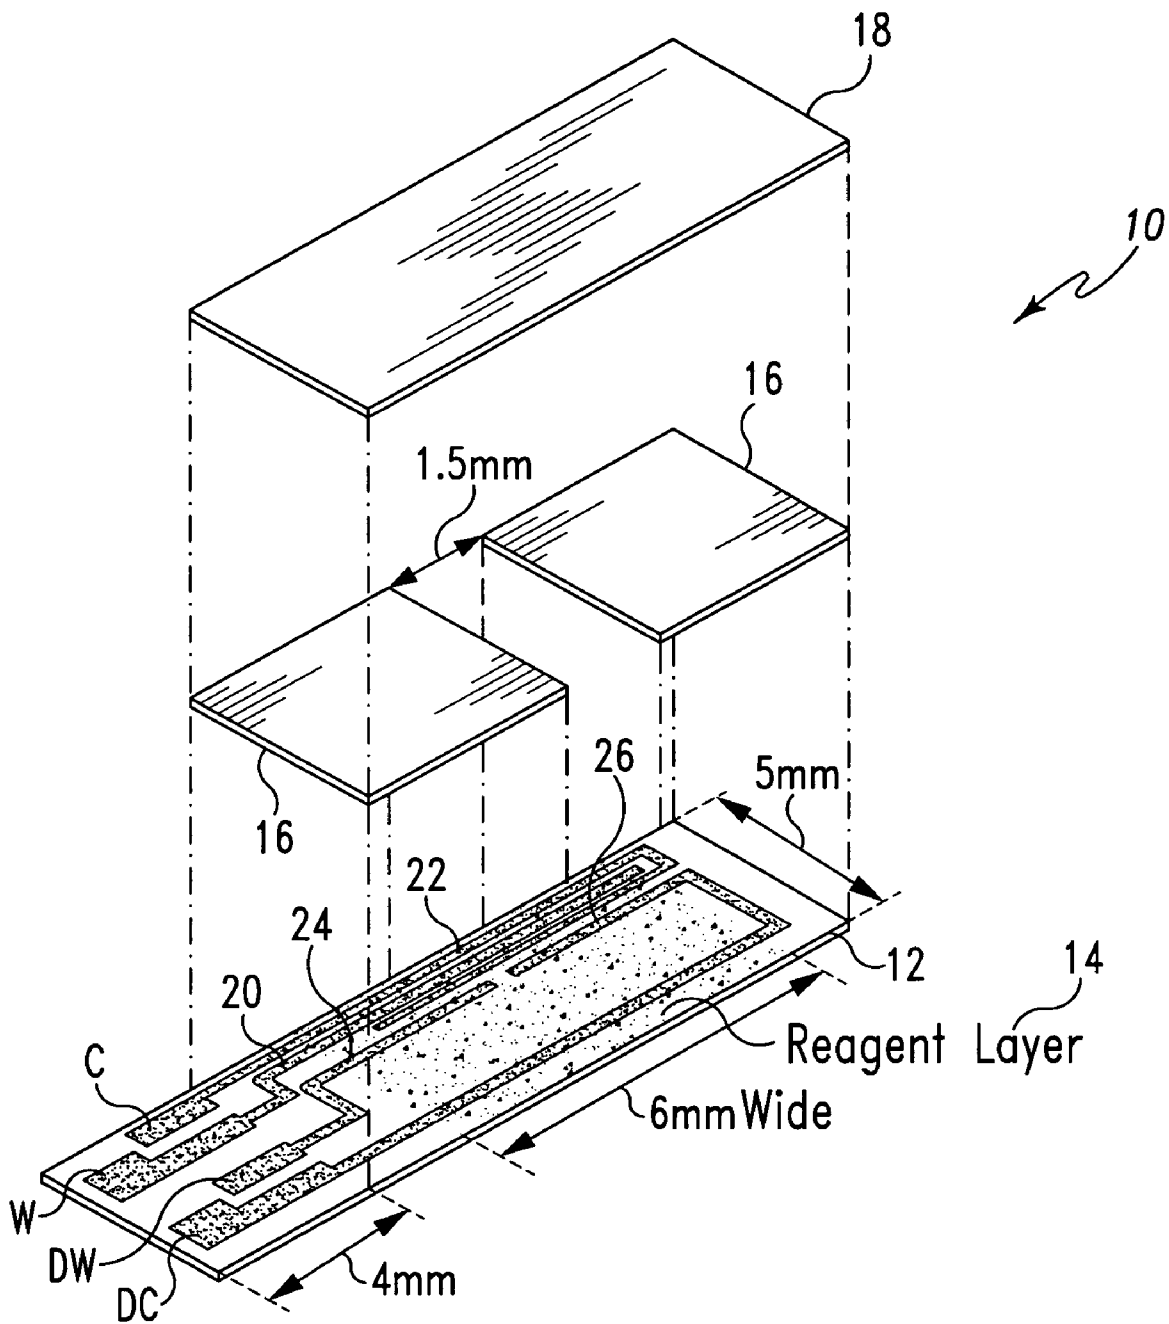


Fig. 1

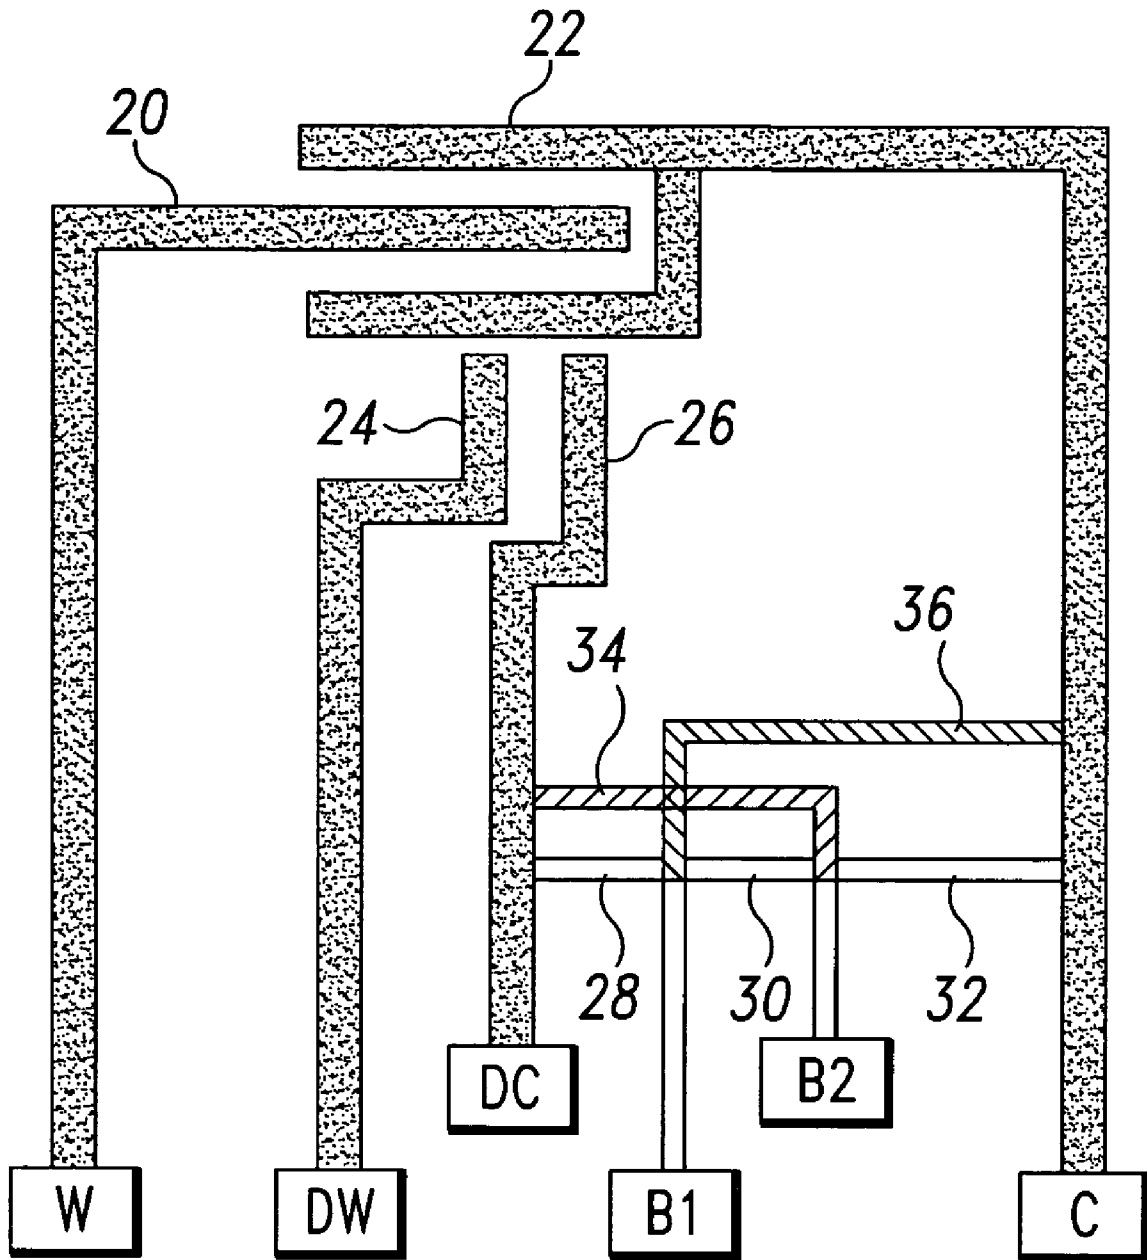


Fig. 2

#	C1	C2	C3	C4	C5	B1	B2
0	0	0	0	0	0	-	-
1	0	0	0	1	0	-	DC
2	0	0	1	0	0	-	C
3	0	1	0	1	0	DC/B2	DC/B1
4	0	1	1	0	0	C/B2	C/B1
5	1	0	0	0	0	DC	-
6	1	0	1	0	0	DC	C
7	0	0	0	0	1	C	-
8	0	1	0	0	0	B2	B1

Fig. 3

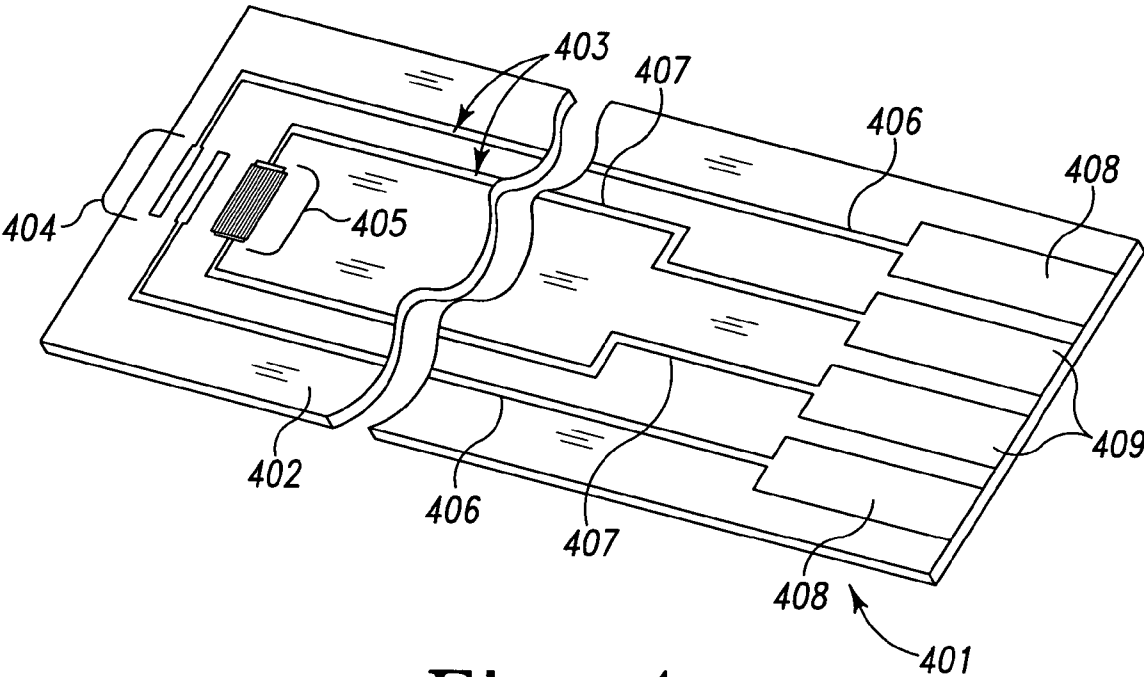


Fig. 4

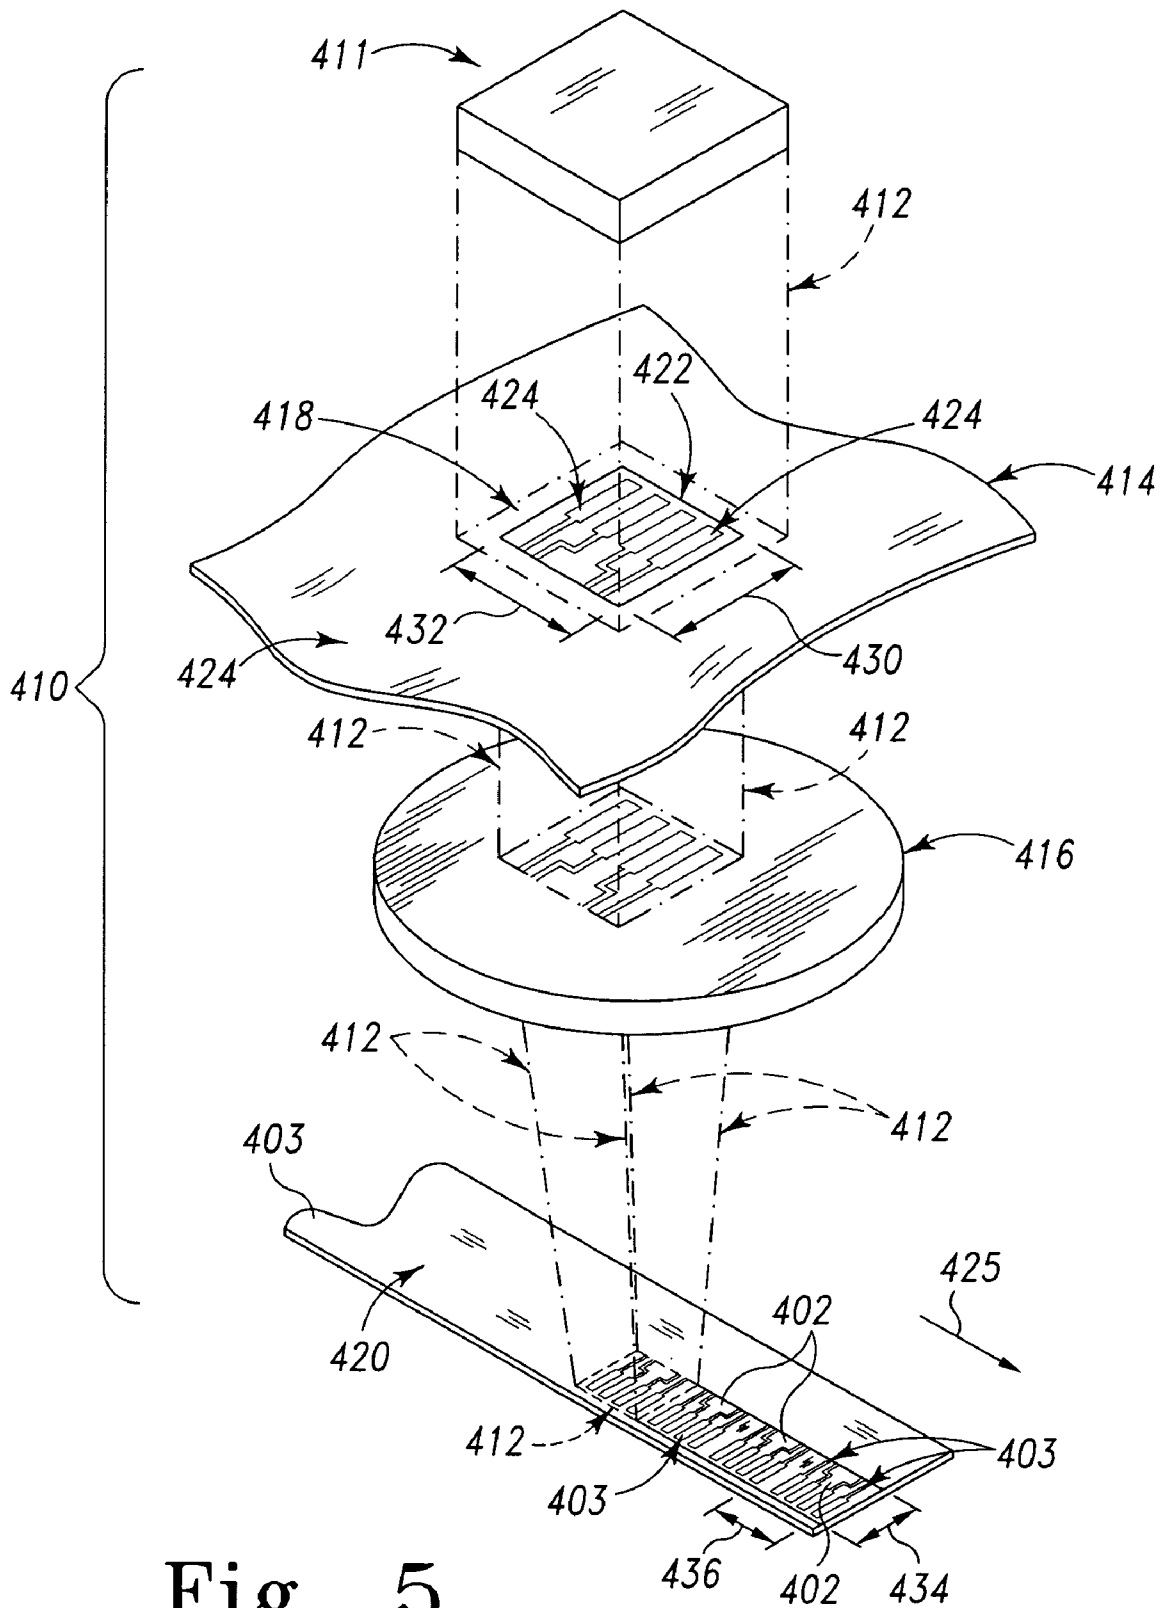


Fig. 5

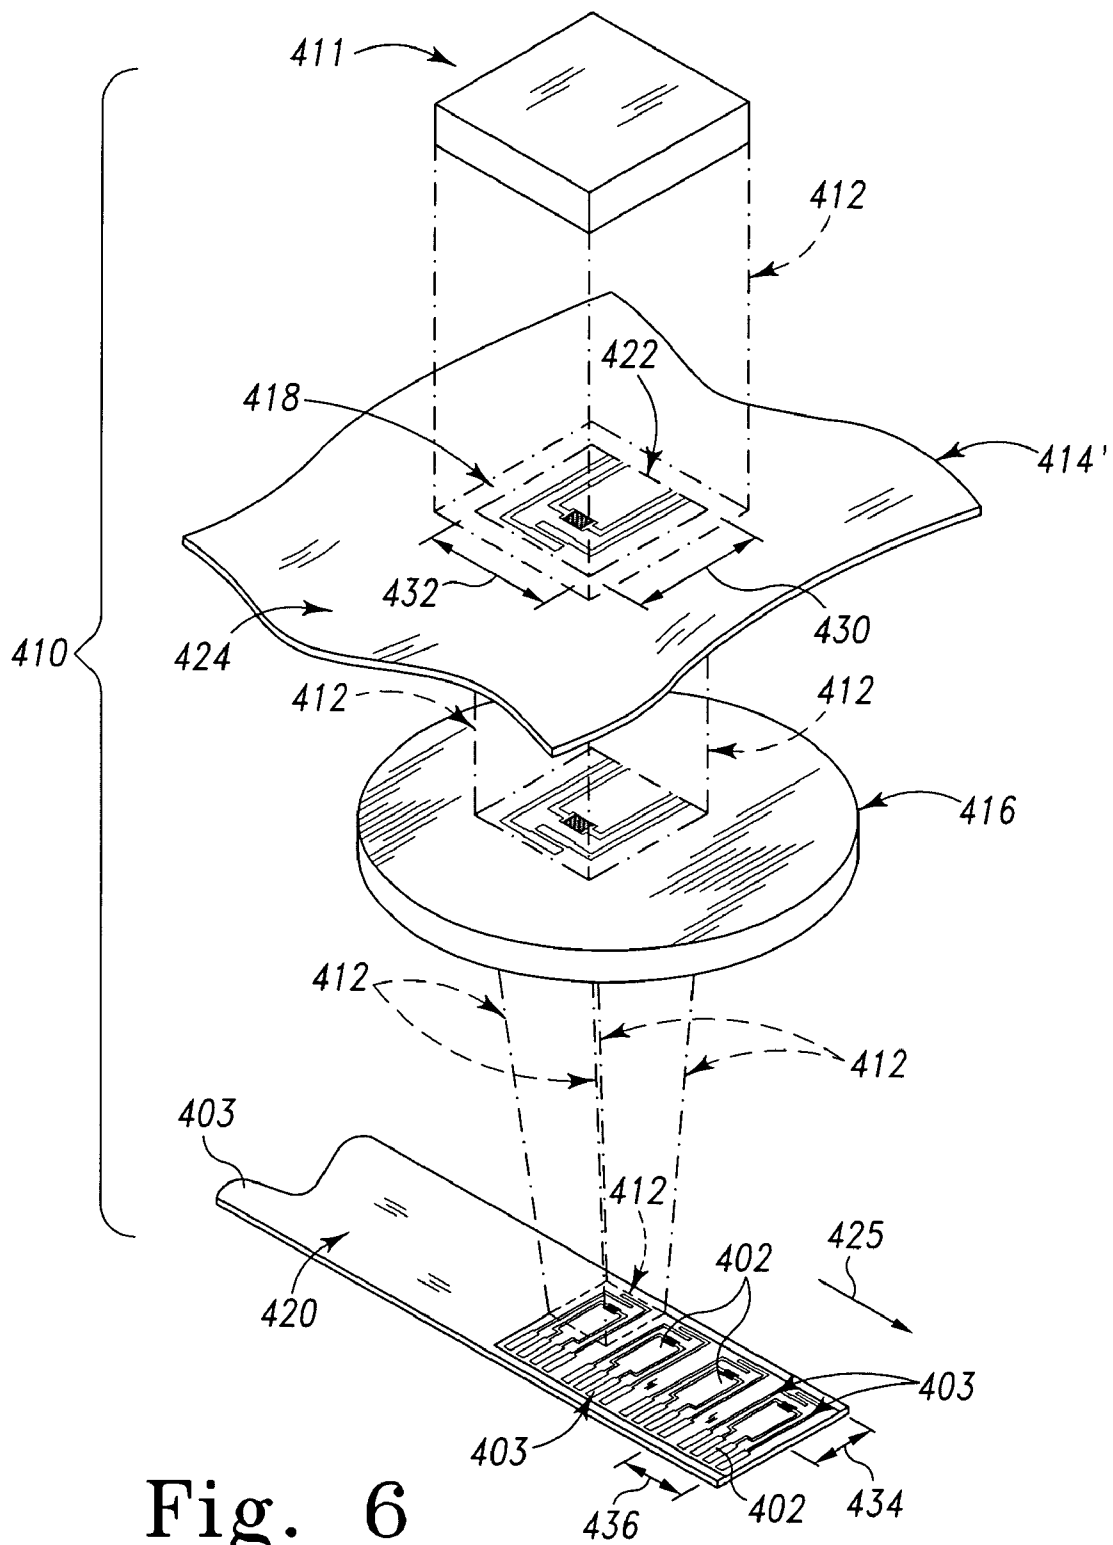


Fig. 6

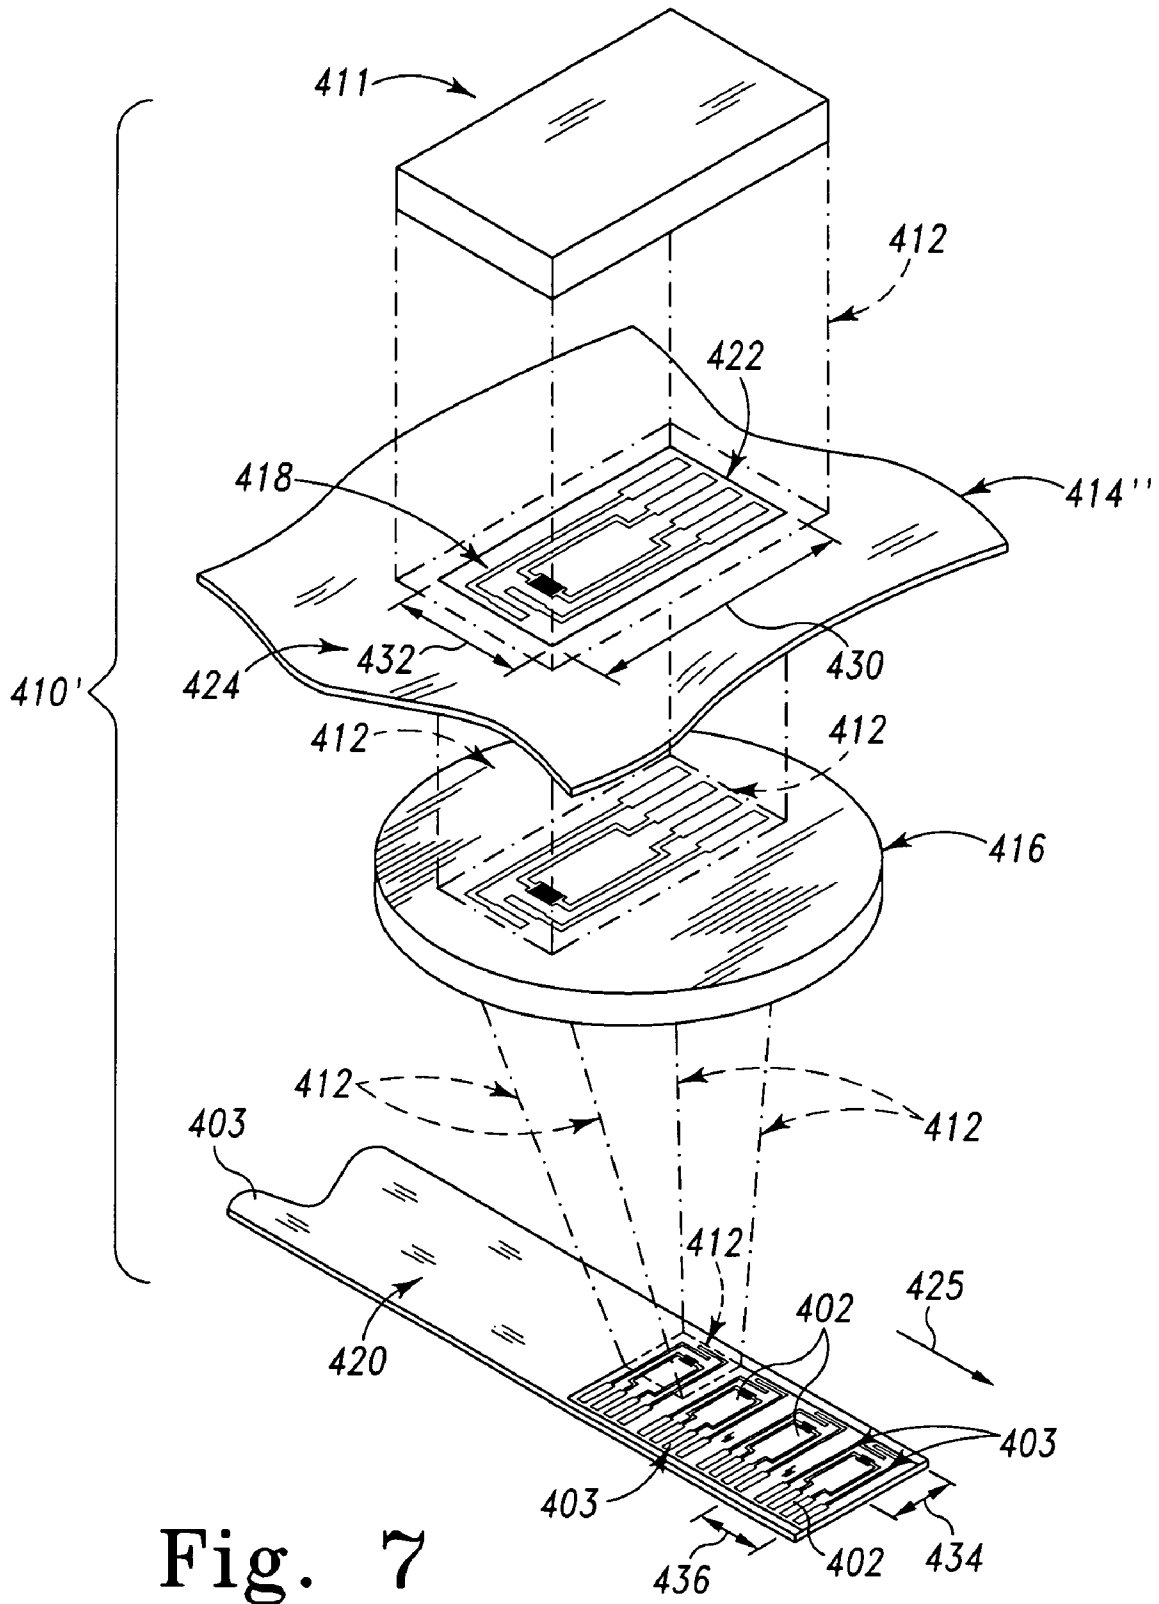


Fig. 7

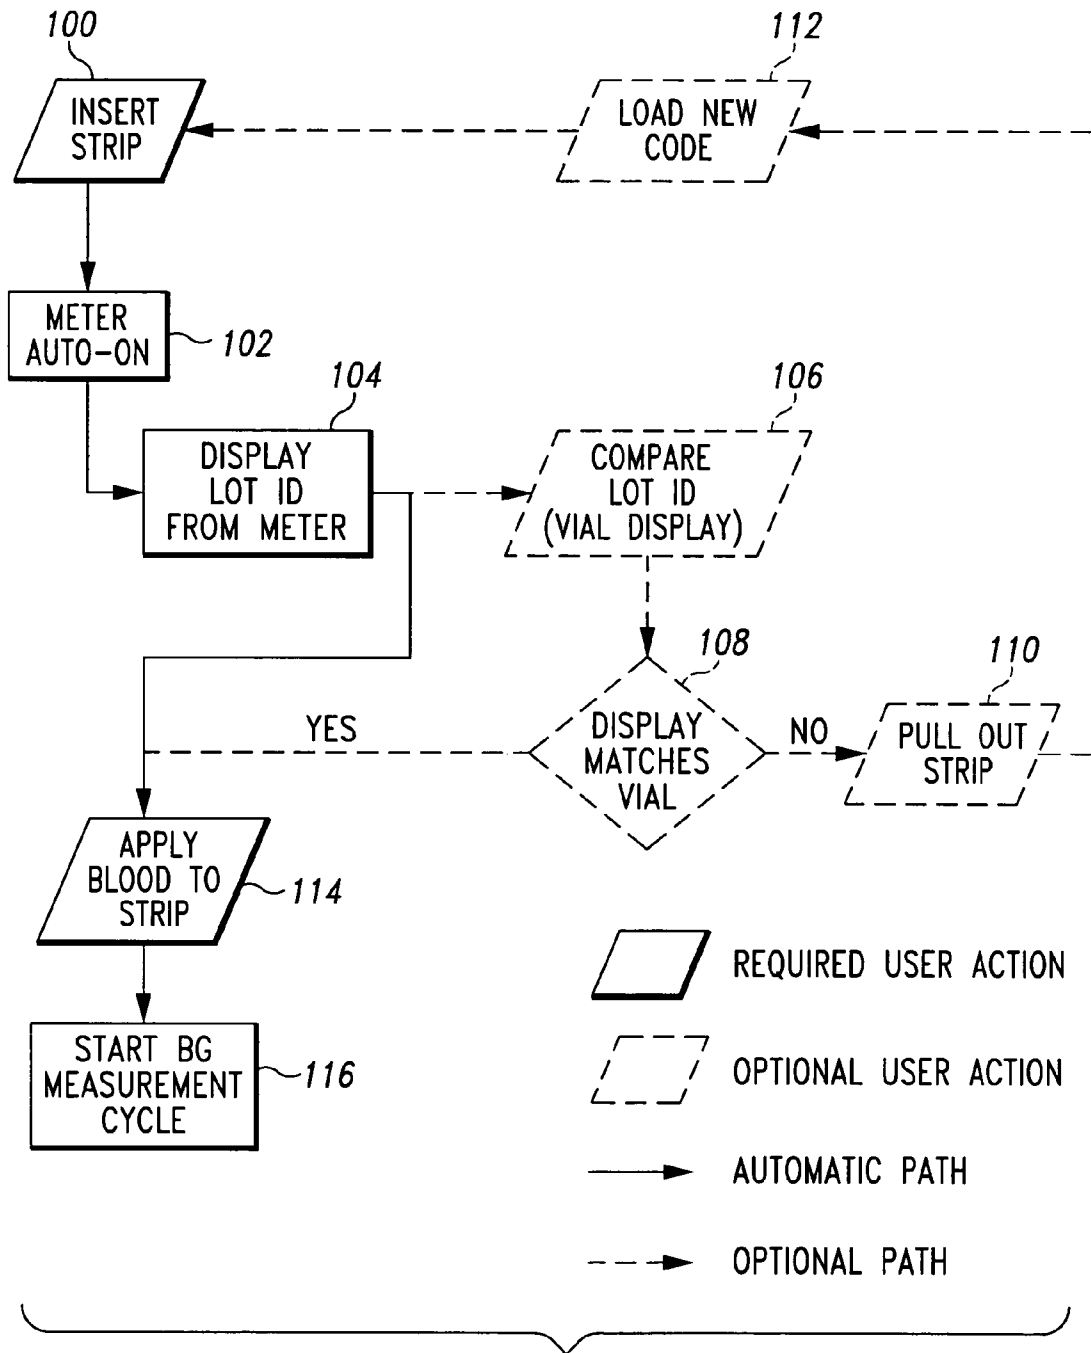


Fig. 8
(Prior Art)

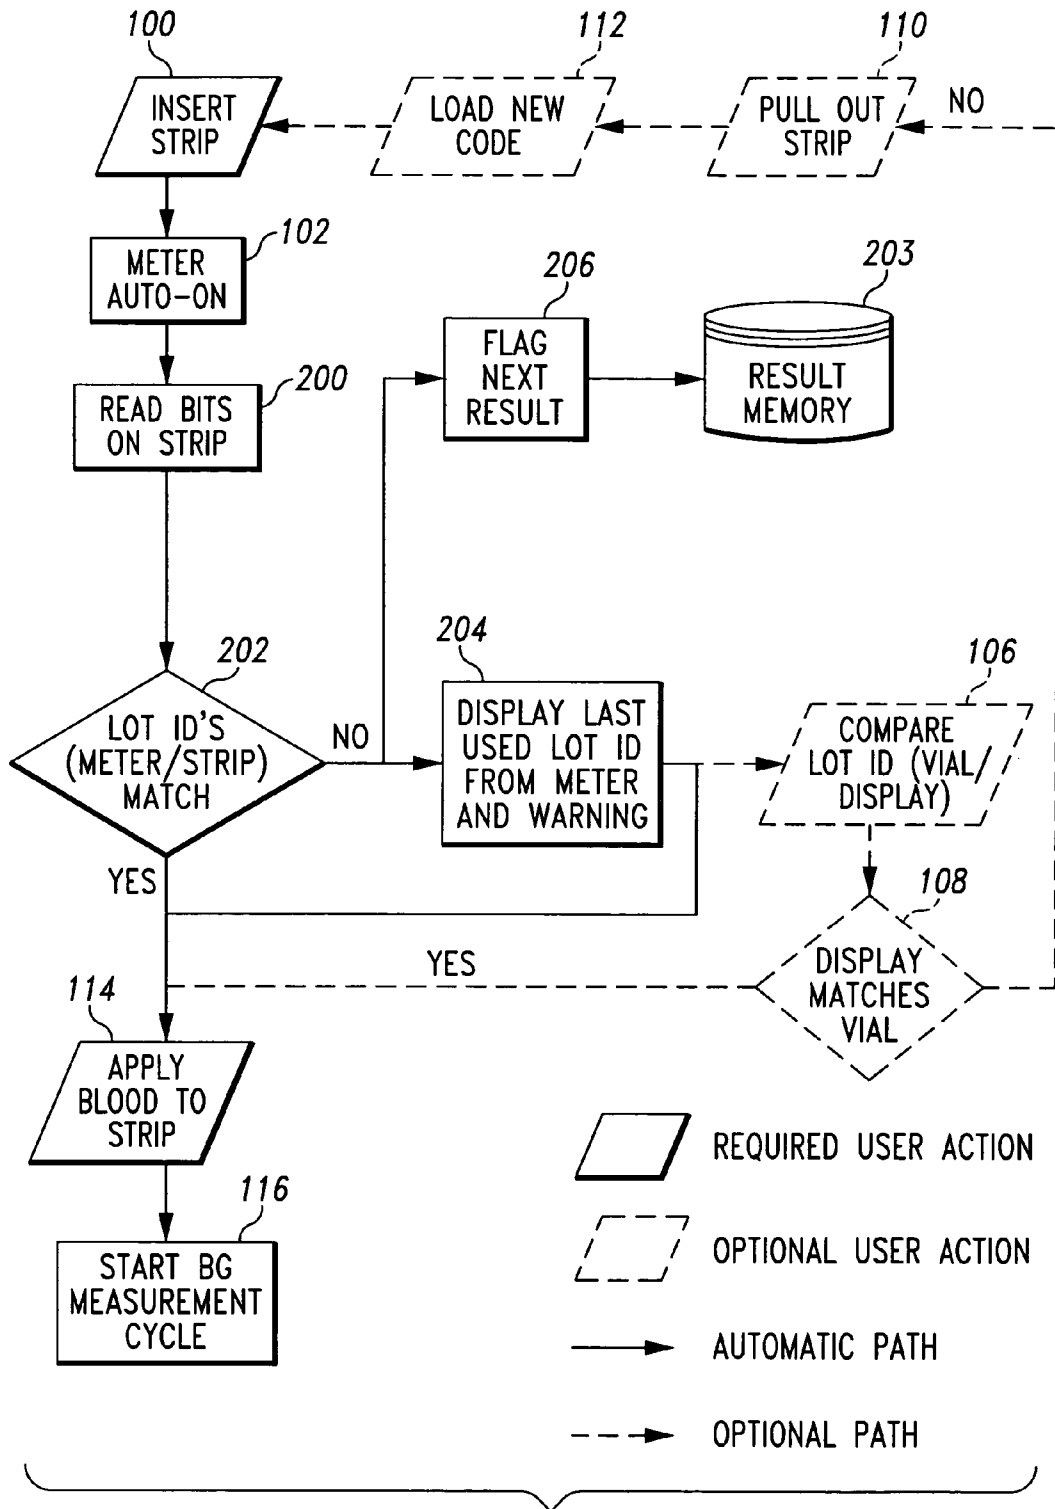


Fig. 9

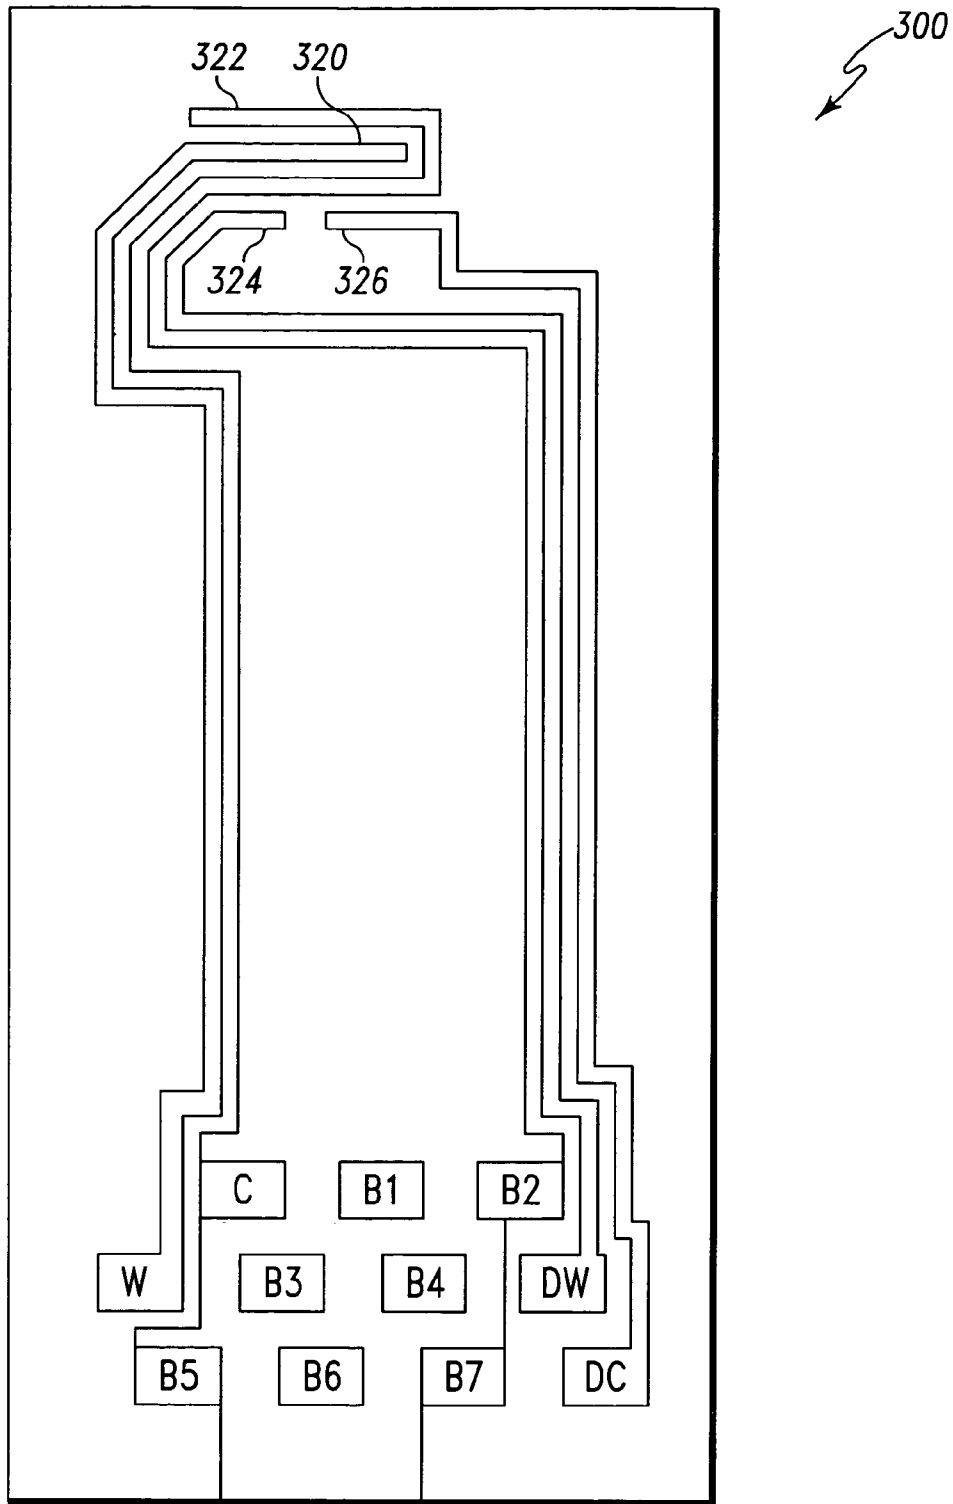


Fig. 10

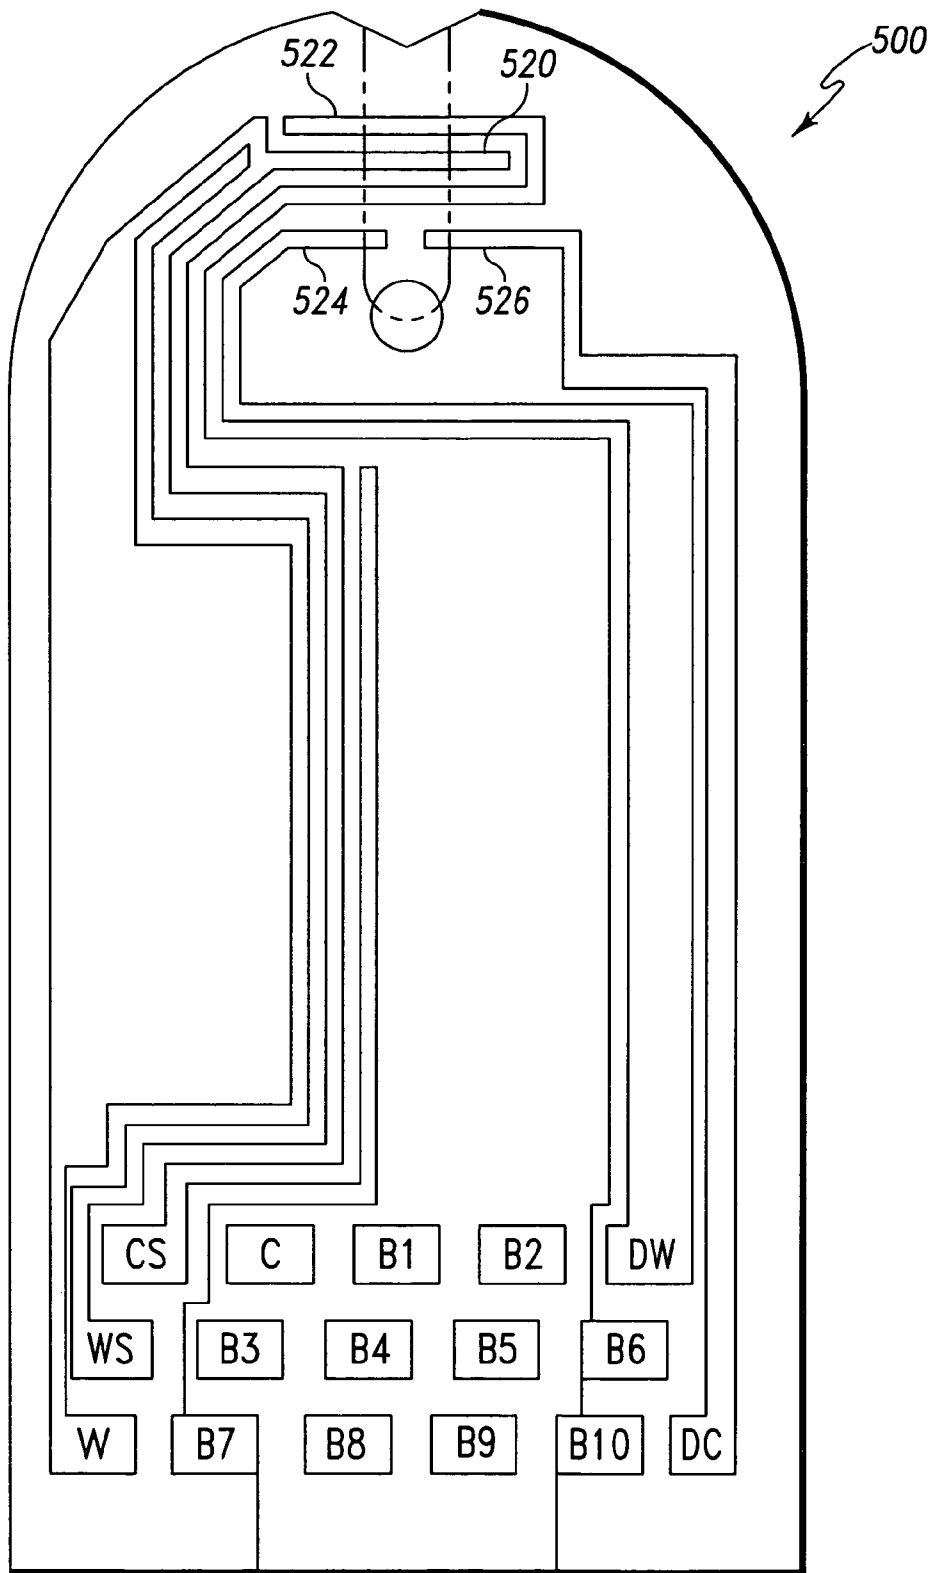


Fig. 11

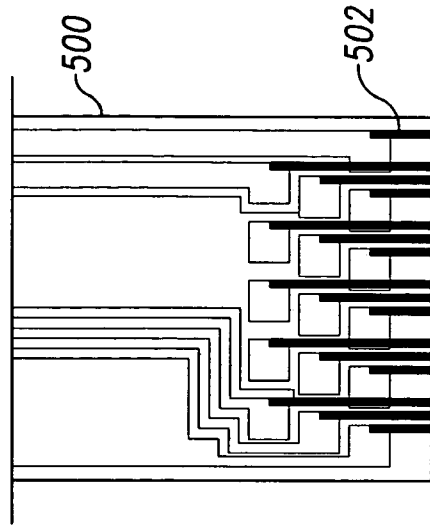


Fig. 12

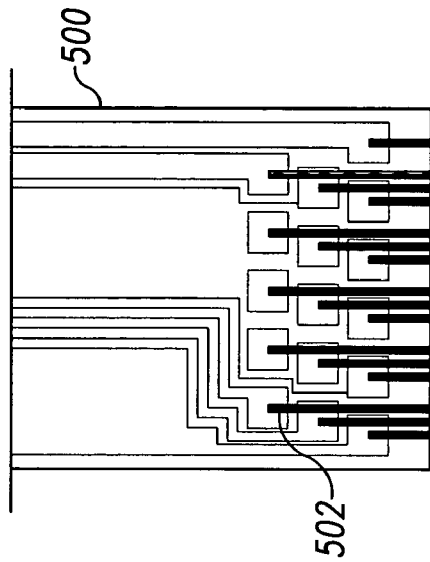


Fig. 13

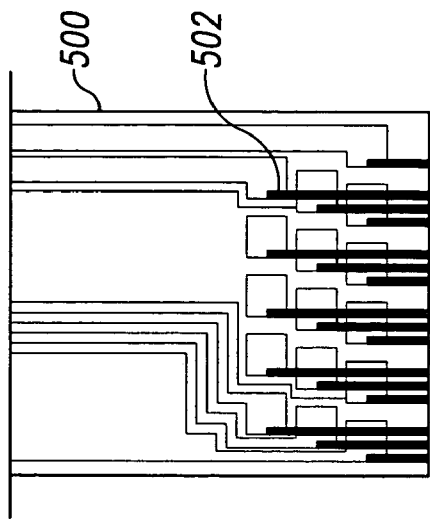


Fig. 14

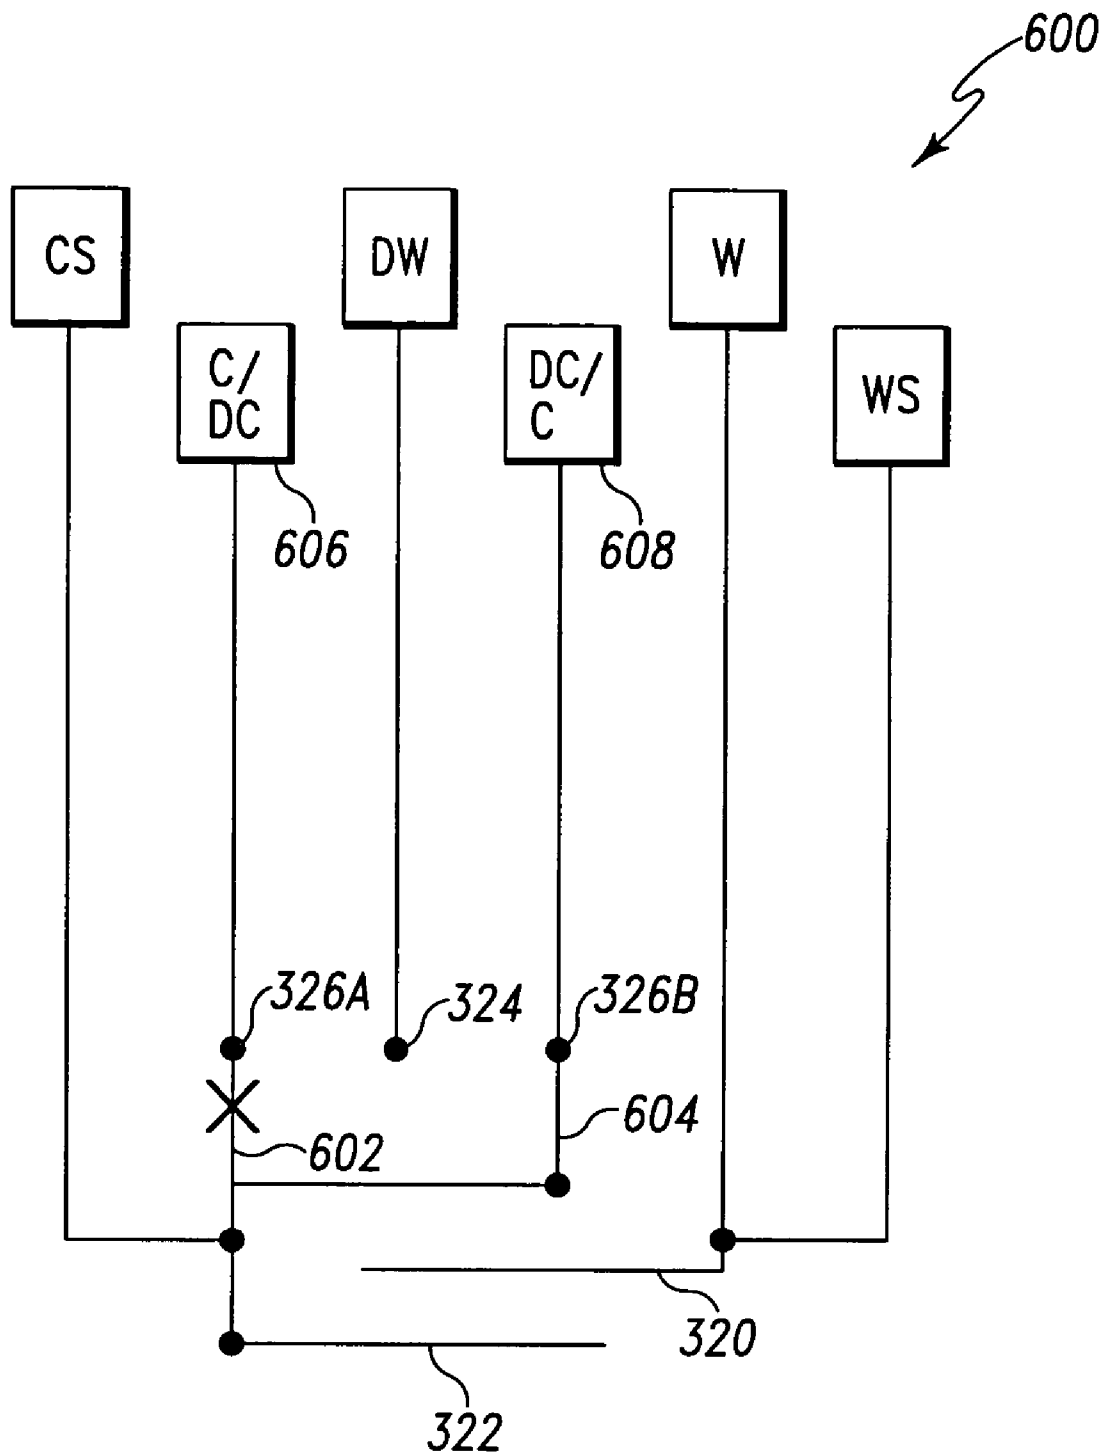


Fig. 15

SYSTEM AND METHOD FOR CODING INFORMATION ON A BIOSENSOR TEST STRIP

REFERENCE TO RELATED APPLICATIONS

This application is related to an application titled BIOSENSOR AND METHODS OF MAKING (U.S. patent application Ser. No. 10/871,937, filed Jun. 18, 2004) which is incorporated herein by reference in its entirety. This application claims the benefit of U.S. Provisional Application No. 60/480,199, filed Jun. 20, 2003, the contents of which are hereby incorporated by reference herein.

TECHNICAL FIELD OF THE INVENTION

The present invention relates to an apparatus for use in measuring concentrations of an analyte in a biological fluid. The invention relates more particularly to a system and method for coding information on a biosensor test strip.

BACKGROUND OF THE INVENTION

Measuring the concentration of substances in biological fluids is an important tool for the diagnosis and treatment of many medical conditions. For example, the measurement of glucose in body fluids, such as blood, is crucial to the effective treatment of diabetes.

Diabetic therapy typically involves two types of insulin treatment: basal, and meal-time. Basal insulin refers to continuous, e.g. time-released insulin, often taken before bed. Meal-time insulin treatment provides additional doses of faster acting insulin to regulate fluctuations in blood glucose caused by a variety of factors, including the metabolization of sugars and carbohydrates. Proper regulation of blood glucose fluctuations requires accurate measurement of the concentration of glucose in the blood. Failure to do so can produce extreme complications, including blindness and loss of circulation in the extremities, which can ultimately deprive the diabetic of use of his or her fingers, hands, feet, etc.

Multiple methods are known for determining the concentration of analytes in a blood sample, such as, for example, glucose. Such methods typically fall into one of two categories: optical methods and electrochemical methods. Optical methods generally involve spectroscopy to observe the spectrum shift in the fluid caused by concentration of the analyte, typically in conjunction with a reagent that produces a known color when combined with the analyte. Electrochemical methods generally rely upon the correlation between a current (Amperometry), a potential (Potentiometry) or accumulated charge (Coulometry) and the concentration of the analyte, typically in conjunction with a reagent that produces charge-carriers when combined with the analyte. See, for example, U.S. Pat. Nos. 4,233,029 to Columbus, 4,225,410 to Pace, 4,323,536 to Columbus, 4,008,448 to Muggli, 4,654,197 to Lilja et al., 5,108,564 to Szuminsky et al., 5,120,420 to Nankai et al., 5,128,015 to Szuminsky et al., 5,243,516 to White, 5,437,999 to Diebold et al., 5,288,636 to Pollmann et al., 5,628,890 to Carter et al., 5,682,884 to Hill et al., 5,727,548 to Hill et al., 5,997,817 to Crismore et al., 6,004,441 to Fujiwara et al., 4,919,770 to Priedel, et al., and 6,054,039 to Shieh, which are hereby incorporated in their entireties. The biosensor for conducting the tests is typically a disposable test strip having a reagent thereon that chemically reacts with the analyte of interest in the biological fluid. The test strip is mated to a nondisposable test meter such that the test meter

can measure the reaction between the analyte and the reagent in order to determine and display the concentration of the analyte to the user.

It is common practice in such test meter/test strip systems to ensure proper identification of the test strip in order to ensure proper test results. For example, a single test meter may be able to analyze several different types of test strips, wherein each type of test strip is designed to test for the presence of a different analyte in the biological fluid. In order to properly conduct the test, the test meter must know which type of test is to be performed for the test strip currently in use.

Also, lot-to-lot variations in the test strips normally require calibration information to be loaded into the test meter in order to ensure accurate test results. A common practice for downloading such calibration information into the test meter is the use of an electronic read-only memory key (ROM key) that is inserted into a socket of the test meter. Because this calibration data may only be accurate for a particular production lot of test strips, the user is usually asked to confirm that the lot number of the test strip currently in use matches the lot number for which the ROM key was programmed.

Many other instances in which it is desirable to have information relating to the test strip are known to those having skill in the art. Prior art attempts to code information onto the test strip for reading by the test meter have suffered from many problems, including a severely limited amount of information that can be coded and the use of relatively large amounts of test strip surface area for the information coding function.

Thus, a system and method are needed that will allow information to be coded onto a biosensor for reading of the information by the test meter. The present invention is directed toward meeting this need.

SUMMARY OF THE INVENTION

The present invention provides a test strip for measuring a concentration of an analyte of interest in a biological fluid, wherein the test strip may be encoded with information that can be read by a test meter into which the test strip is inserted.

In one form of the invention, a method for forming a test strip for measuring a concentration of an analyte of interest in a biological fluid is disclosed, the method comprising the steps of: providing a basic test strip design comprising: a substrate having a surface and at least one measurement electrode formed thereon; a plurality of conductive contact pads formed upon the substrate surface, including at least one information contact pad and at least one measurement contact pad; and a plurality of potential conductive links conductively coupling various ones of the plurality of contact pads; wherein the at least one information contact pad is not coupled to any of the at least one measurement electrodes except by one or more of the plurality of potential conductive links, and the at least one measurement contact pad is coupled to one of the at least one measurement electrodes by a path other than one or more of the plurality of potential conductive links; defining a set of valid test strip designs; wherein each one of the set of valid test strip designs incorporates none, one or more than one of the plurality of potential conductive links; and wherein at least one of the plurality of potential conductive links couples a first one of the information contact pads to a first one of the measurement contact pads in a first valid test strip design, and at least one of the plurality of potential conductive links couples the first one of the information contact pads to a second one of the measurement contact pads in a second valid test strip design; selecting one design from the set of valid test strip designs; and forming a test strip per said selected one design.

In another form of the invention, a plurality of test strips for measuring a concentration of an analyte of interest in a biological fluid is disclosed, each of the plurality of test strips being substantially identical to one another except for a presence or absence of a plurality of potential conductive links, at least one of the test strips comprising: a substrate having a surface and at least one measurement electrode formed thereon; a plurality of conductive contact pads formed upon the substrate surface, including at least one information contact pad and at least one measurement contact pad; and a plurality of conductive links selected from the plurality of potential conductive links, wherein the plurality of conductive links conductively couple at least three contact pads together; wherein the at least one information contact pad is not coupled to any of the at least one measurement electrodes except by one or more of the plurality of potential conductive links, and the at least one measurement contact pad is coupled to one of the at least one measurement electrodes by a path other than one or more of the plurality of potential conductive links.

In another form of the invention, a method for forming a test strip for measuring a concentration of an analyte of interest in a biological fluid is disclosed, the method comprising the steps of: providing a basic test strip design comprising: a substrate having a surface and at least one measurement electrode formed thereon; a plurality of conductive contact pads formed upon the substrate surface, including at least one information contact pad and at least one measurement contact pad; and a plurality of potential conductive links conductively coupling various ones of the plurality of contact pads; wherein the at least one information contact pad is not coupled to any of the at least one measurement electrodes except by one or more of the plurality of potential conductive links, and the at least one measurement contact pad is coupled to one of the at least one measurement electrodes by a path other than one or more of the plurality of potential conductive links; defining a set of valid test strip designs; wherein each one of the set of valid test strip designs incorporates none, one or more than one of the plurality of potential conductive links; and wherein at least one of the set of valid test strip designs includes conductive links that conductively couple at least three contact pads together; selecting one design from the set of valid test strip designs; and forming a test strip per said selected one design.

In another form of the invention, a test strip for measuring a concentration of an analyte of interest in a biological fluid is disclosed, the test strip comprising: a substrate having a surface and at least one measurement electrode formed thereon; a plurality of conductive contact pads formed upon the substrate surface, including at least one information contact pad and at least one measurement contact pad; and at least one conductive link conductively coupling at least three of the contact pads; wherein the at least one information contact pad is not coupled to any of the at least one measurement electrodes except by one or more of the at least one conductive links, and the at least one measurement contact pad is coupled to one of the at least one measurement electrodes by a path other than one or more of the at least one conductive links.

In another form of the invention, a test strip for measuring a concentration of an analyte of interest in a biological fluid is disclosed, the test strip comprising: a substrate having a surface and at least one measurement electrode formed thereon; a plurality of conductive contact pads formed upon the substrate surface, including at least one information contact pad and at least one measurement contact pad; and at least one conductive link conductively coupling at least three of the contact pads; wherein the at least one information contact pad

is not coupled to any of the at least one measurement electrodes except by one or more of the at least one conductive links, and the at least one measurement contact pad is coupled to one of the at least one measurement electrodes by a path other than one or more of the at least one conductive links.

In another form of the invention, a test strip for measuring a concentration of an analyte of interest in a biological fluid is disclosed, the test strip adapted to be inserted into a test meter having at least one connector contact that touches the inserted test strip, the test strip comprising: a substrate having a top surface; a conductive layer formed on at least a portion of the substrate top surface; and at least one predetermined contact pad position defined upon the substrate top surface; wherein each of the at least one contact pad positions is touched by a respective one of the at least one connector contacts when the at least one connector contacts touch the test strip; wherein a presence of the conductive layer in a respective one of the contact pad positions is operative to indicate a first state of a binary bit to the test meter; and wherein an absence of the conductive layer in a respective one of the contact pad positions is operative to indicate a second state of a binary bit to the test meter.

In another form of the invention, a method for measuring a concentration of an analyte of interest in a biological fluid, comprising the steps of: providing a test meter having at least one connector contact that touches an inserted test strip, providing a test strip adapted to be inserted into the test meter, the test strip comprising: a substrate having a top surface; a conductive layer formed on at least a portion of the substrate top surface; and at least one predetermined contact pad position defined upon the substrate top surface; touching each of the at least one predetermined contact pad positions with a respective one of the at least one connector contacts; indicating a first state of a binary bit within the test meter in response to a presence of the conductive layer in a respective one of the contact pad positions; and indicating a second state of a binary bit within the test meter in response to an absence of the conductive layer in a respective one of the contact pad positions.

In another form of the invention, a test strip for measuring a concentration of an analyte of interest in a biological fluid is disclosed, the test strip comprising a substrate having a surface; a first measurement electrode formed on the surface; a second measurement electrode formed on the surface; a third potential electrode formed on the surface; a fourth potential electrode formed on the surface; a first contact pad formed on the surface and conductively coupled to the first measurement electrode; a second contact pad formed on the surface and conductively coupled to the second measurement electrode; a third contact pad formed on the surface and conductively coupled to the third potential electrode; a fourth contact pad formed on the surface and conductively coupled to the fourth potential electrode; and a conductive link coupling one of the third and fourth potential electrodes to the first measurement electrode, whereby another one of the third and fourth potential electrodes becomes an actual electrode.

In another form of the invention, a method of using a test meter and associated test strip for measuring a concentration of an analyte of interest in a biological fluid is disclosed, comprising the steps of a) providing a test strip comprising a substrate having at least a first, second and third contact pad formed thereon; b) providing a test meter comprising a connector configured to make conductive contact with the first, second and third contact pads when the test strip is inserted into the test meter; c) operating the test meter to determine if conductivity exists between the first and second contact pads; d) operating the test meter to determine if conductivity exists

5

between the first and third contact pads; e) designating the second contact pad to have a first function and the third contact pad to have a second function if the test meter determines that conductivity exists between the first and second contact pads and that conductivity does not exist between the first and third contact pads; and f) designating the second contact pad to have the second function and the third contact pad to have the first function if the test meter determines that conductivity does not exist between the first and second contact pads and that conductivity exists between the first and third contact pads.

In another form of the invention, a method of using a test meter and associated test strip for measuring a concentration of an analyte of interest in a biological fluid is disclosed, comprising the steps of a) providing a test strip comprising a substrate having at least a first, second and third contact pad formed thereon; b) providing a test meter comprising a connector configured to make conductive contact with the first, second and third contact pads when the test strip is inserted into the test meter; c) operating the test meter to determine if conductivity exists between the first and second contact pads; d) designating the second contact pad to have a first function and the third contact pad to have a second function if the test meter determines that conductivity exists between the first and second contact pads; and e) designating the second contact pad to have the second function and the third contact pad to have the first function if the test meter determines that conductivity does not exist between the first and second contact pads.

In another form of the invention, a method of using a test meter adapted to measure a concentration of an analyte of interest in a biological fluid placed on a test strip is disclosed, the method comprising the steps of a) inserting the test strip into the test meter such that the test meter makes electrical contact with the test strip; b) operating the meter to read information encoded onto the test strip; and c) choosing a language in which the test meter displays user operating instructions based upon the information read from the test strip.

In another form of the invention, a method of using a test meter adapted to measure a concentration of an analyte of interest in a biological fluid placed on a test strip is disclosed, the method comprising the steps of a) inserting the test strip into the test meter such that the test meter makes electrical contact with the test strip; b) operating the meter to read information encoded onto the test strip; and c) determining if the test meter and the test strip were sold in the same geographic market based upon the information read from the test strip.

In another form of the invention, a method of using a test meter adapted to measure a concentration of an analyte of interest in a biological fluid placed on a test strip is disclosed, wherein the test meter is not intended for use with subscription test strips sold on a subscription basis, the method comprising the steps of a) inserting the test strip into the test meter such that the test meter makes electrical contact with the test strip; b) operating the meter to read information encoded onto the test strip; c) determining if the test strip is a subscription test strip based upon the information read from the test strip; and d) preventing use of the test strip by the meter if the test strip is a subscription test strip.

In another form of the invention, a method of using a test meter adapted to measure a concentration of an analyte of interest in a biological fluid placed on a test strip is disclosed, the method comprising the steps of a) inserting the test strip into the test meter such that the test meter makes electrical contact with the test strip; b) operating the meter to read

6

information encoded onto the test strip; and c) activating a latent feature of the test meter based upon the information read from the test strip.

In another form of the invention, a method of using a test meter adapted to measure a concentration of an analyte of interest in a biological fluid placed on a test strip is disclosed, the method comprising the steps of a) inserting the test strip into the test meter such that the test meter makes electrical contact with the test strip; b) operating the meter to read information encoded onto the test strip; and c) changing the user operating instructions displayed to the user based upon the information read from the test strip.

In another form of the invention, a test system for measuring a concentration of an analyte of interest in a biological fluid is disclosed, the test system comprising a test meter comprising a connector having at least ten contacts; and a test strip adapted to be inserted into the test meter connector, the test strip comprising: a substrate having a surface; at least ten contact pads formed on the surface; wherein the at least ten contacts make contact with the respective at least ten contact pads when the test strip is inserted into the test meter connector.

BRIEF DESCRIPTION OF THE DRAWINGS

The invention will be further described, by way of example only, with reference to the accompanying drawings, in which:

FIG. 1 is an exploded perspective view of a first typical test strip for use in measuring the concentration of an analyte of interest in a biological fluid.

FIG. 2 is a schematic plan view of a first embodiment test strip electrode and contact pad arrangement according to the present invention.

FIG. 3 is a table showing a first embodiment coding sequence for the test strip of FIG. 2.

FIG. 4 is a perspective view of a second typical test strip for use in measuring the concentration of an analyte of interest in a biological fluid.

FIG. 5 illustrates a view of an ablation apparatus suitable for use with the present invention.

FIG. 6 is a view of the laser ablation apparatus of FIG. 5 showing a second mask.

FIG. 7 is a view of an ablation apparatus suitable for use with the present invention.

FIG. 8 is a schematic process flow diagram of a prior art process for verifying the applicability of the calibration data in the test meter to the test strip currently inserted into the test meter.

FIG. 9 is a schematic process flow diagram of a first embodiment process of the present invention for verifying the applicability of the calibration data in the test meter to the test strip currently inserted into the test meter.

FIG. 10 is a schematic plan view of a second embodiment test strip electrode and contact pad arrangement according to the present invention.

FIG. 11 is a schematic plan view of a third embodiment test strip electrode and contact pad arrangement according to the present invention.

FIG. 12 is a schematic plan view of an electrical connector-to-test strip contact pad interface illustrating worst case left tolerance stack-ups.

FIG. 13 is a schematic plan view of the electrical connector-to-test strip contact pad interface of FIG. 12 illustrating normal case tolerance stack-ups.

FIG. 14 is a schematic plan view of the electrical connector-to-test strip contact pad interface of FIG. 12 illustrating worst case right tolerance stack-ups.

FIG. 15 is a schematic plan view of a fourth embodiment test strip electrode and contact pad arrangement according to the present invention.

DETAILED DESCRIPTION OF THE PREFERRED EMBODIMENTS

For the purposes of promoting an understanding of the principles of the invention, reference will now be made to the embodiment illustrated in the drawings, and specific language will be used to describe that embodiment. It will nevertheless be understood that no limitation of the scope of the invention is intended. Alterations and modifications in the illustrated device, and further applications of the principles of the invention as illustrated therein, as would normally occur to one skilled in the art to which the invention relates are contemplated, are desired to be protected. In particular, although the invention is discussed in terms of a blood glucose meter, it is contemplated that the invention can be used with devices for measuring other analytes and other sample types. Such alternative embodiments require certain adaptations to the embodiments discussed herein that would be obvious to those skilled in the art.

Although the system and method of the present invention may be used with test strips having a wide variety of designs and made with a wide variety of construction techniques and processes, a typical electrochemical test strip is illustrated in FIG. 1, and indicated generally at 10. Referring to FIG. 1, the test strip 10 comprises a bottom substrate 12 formed from an opaque piece of 350 μm thick polyester (such as Melinex 329 available from DuPont) coated on its top surface with a 50 nm conductive (gold) layer (by sputtering or vapor deposition, for example). Electrodes, connecting traces and contact pads therefore are then patterned in the conductive layer by a laser ablation process. The laser ablation process is performed by means of an excimer laser which passes through a chrome-on-quartz mask. The mask pattern causes parts of the laser field to be reflected while allowing other parts of the field to pass through, creating a pattern on the gold which is ablated where contacted by the laser light. The laser ablation process is described in greater detail hereinbelow. For example, working 20, counter 22, dose sufficiency working 24, and dose sufficiency counter 26 electrodes may be formed as shown and coupled, respectively, to measurement contact pads W, C, DW and DC. These contact pads provide a conductive area upon the test strip 10 to be contacted by a connector contact of the test meter once the test strip 10 is inserted into the test meter.

The bottom substrate 12 is then coated in the area extending over the electrodes with a reagent layer 14 as a continuous, extremely thin reagent film. The reagent layer 14 is a stripe of approximately 6 millimeters width across the substrate 12 in the region labeled "Reagent Layer" on FIG. 1. For example, this region may be coated at a wet-coat weight of 50 grams per square meter of coated surface area. The reagent strip is dried conventionally with an in-line drying system where the nominal air temperature is at 110° C. The rate of processing is nominally 30-38 meters per minute and depends upon the rheology of the reagent.

The materials are processed in continuous reels such that the electrode pattern is orthogonal to the length of the reel, in the case of the substrate 12. Once the substrate 12 has been coated with reagent, the spacers 16 are slit and placed in a reel-to-reel process onto the substrate 12. Two spacers 16 formed from 100 μm polyester (for example, Melinex 329 available from DuPont) coated with 25 μm PSA (hydrophobic adhesive) on both the dorsal and ventral surfaces are applied

to the bottom substrate 12, such that the spacers 16 are separated by 1.5 mm and the working, counter and dose sufficiency electrodes are centered in this gap. A top foil layer 18 formed from 100 μm polyester coated with a hydrophilic film on its ventral surface (using the process described in U.S. Pat. No. 5,997,817) is placed over the spacers 16. The hydrophilic film is coated with a mixture of Vitel and Rhodapex surfactant at a nominal thickness of 10 microns. The top foil layer 18 is laminated using a reel-to-reel process. The test strips can then be produced from the resulting reels of material by means of slitting and cutting.

Although the basic test strip 10 illustrated in FIG. 1 can provide accurate measurements of blood glucose in a whole blood sample, it does not provide any means for the test meter into which it is inserted to identify anything about the test strip. The present invention presents several systems by which information relating to the test strip can be coded directly onto the test strip itself, such that this information can be conveyed to a test meter into which the test strip is inserted.

In a first embodiment of the present invention, information about the test strip can be coded directly onto the test strip by the addition of two or more contact pads dedicated to reading such coded information. As illustrated in FIG. 2, a pair of additional information contact pads B1 and B2 are added to the proximal end of the test strip. Additionally, potential conductive links between the information contact pads B1 and B2 and between them and measurement contact pads connected to test strip measurement electrodes are identified at 28, 30, 32, 34 and 36. These links are denominated as potential conductive links because they may either be present or absent in the finished test strip, depending upon the information that is to be coded onto the test strip. Therefore, a "potential conductive link" indicates a conductive link that is found on some, but not all, of a group of otherwise substantially identical test strips. As used herein, the phrase "information contact pad" is defined as a contact pad on the test strip that is either not conductively coupled to a measurement electrode of the test strip at all, or is so coupled only by a potential conductive link. As used herein, the phrase "measurement contact pad" is defined as a contact pad on the test strip that is always conductively coupled to a measurement electrode of the test strip, regardless of the presence or absence of the potential conductive links.

Specifically, potential conductive link 28 couples the DC contact pad and the B1 contact pad. Potential conductive link 30 couples the B1 contact-pad and the B2 contact pad. Potential conductive link 32 couples the B2 contact pad and the C contact pad. Potential conductive link 34 couples the DC contact pad and the B2 contact pad. Potential conductive link 36 couples the B1 contact pad and the C contact pad. It should be noted that the first embodiment of the present invention illustrates potential conductive links between the information contact pads B1 and B2 and the measurement contact pads DC and C by way of example only, and that the information contact pads may be conductively linked to any desired measurement contact pad(s) on the test strip.

FIG. 3 illustrates a table showing the possible combinations for the potential conductive links 28-36 formed on any one test strip of the first embodiment. The first five columns of the table represent each of the potential conductive links 28-36, which are labeled C1-C5, respectively. Each of the nine rows of the table numbered 0-8 represent a different number that can be encoded using the potential conductive links 28-36. A "0" in a table position indicates that the potential conductive link is not formed when encoding the number of that row, while a "1" in a table position indicates that the potential conductive link is formed when encoding the num-

ber of that row. Note that there are some combinations of potential conductive links that are not allowed because the DC contact pad and the C contact pad cannot be conductively linked without harming the measurement functionality of the test strip measurement electrodes. For example, potential conductive links **34** and **36** may not be used at the same time, as they cross one another and therefore would conductively connect the DC contact pad to the C contact pad. Similarly, potential conductive links **28**, **30** and **32** may not be used at the same time.

The last two columns of the table of FIG. **3** are labeled **B1** and **B2**, respectively, and indicate to which of the other contact pads the labeled contact pad is coupled when the number of that row is encoded onto the test strip. For example, when the number six (6) is encoded onto the test strip (i.e. potential conductive links **28** and **32** are formed on the test strip) the **B1** contact pad is conductively coupled to the DC contact pad, and the **B2** contact pad is conductively coupled to the C contact pad, but **B1** and **B2** are not conductively coupled to any other contact pads (including to each other). Therefore, a measurement by the test meter of the resistance (either directly or indirectly) between each of the contact pads DC, **B1**, **B2** and C will indicate which of the eight (8) possible numbers has been encoded onto the test strip. The present invention also comprehend other methods for determining the presence or absence of potential conductive links on the test strip other than by measurement of resistance or conductivity. By way of non-limiting example, the potential conductive links can also be sensed in a non-contact fashion by inducing and sensing eddy currents using an electromagnetic field, by capacitive means, by optical scanning techniques, or by other methods that would be apparent to one having ordinary skill in the art.

Note that the absence of all of the potential conductive links **28-36** is preferably not considered to be a valid state as this could be caused by a localized defect obliterating the region of the test strip containing the potential conductive links **28-36**, but this state could be considered a valid state in other, non-preferred, embodiments. It should also be noted that a reading of conduction between combinations of contact pads not indicated as a valid combination in the table of FIG. **3** will be interpreted by the test meter as a defective strip with an unintended short.

It will be appreciated that the use of measurement contact pads in combination with dedicated information contact pads in the present invention, and the opportunity to potentially couple each information contact pad to more than one measurement contact pad significantly increases the amount of numbers that may be encoded onto the test strip. By way of comparison, the two (2) information contact pads of the first embodiment of the present invention conservatively allow the coding of eight (8) numbers. The design disclosed in JP 2000352034 would only allow two (2) possible states with two information contact pads, while the design disclosed in EP 1152239A1 would only allow four (4) possible states with two information contact pads.

One method of preparing a test strip encoded with information as described herein is by the use of laser ablation techniques. Examples of the use of these techniques in preparing electrodes for biosensors are described in U.S. patent application Ser. No. 09/866,030, "Biosensors with Laser Ablation Electrodes with a Continuous Coverlay Channel" filed May 25, 2001, and in U.S. patent application Ser. No. 09/411,940, entitled "Laser Defined Features for Patterned Laminates and Electrode," filed Oct. 4, 1999, both disclosures incorporated herein by reference.

It is desirable in the present invention to provide for the accurate placement of the electrical components relative to one another and to the overall biosensor. In a preferred embodiment, the relative placement of components is achieved, at least in part, by the use of broad field laser ablation that is performed through a mask or other device that has a precise pattern for the electrical components. This allows accurate positioning of adjacent edges, which is further enhanced by the close tolerances for the smoothness of the edges.

FIG. **4** illustrates a simple biosensor **401** useful for illustrating the laser ablation process of the present invention, including a substrate **402** having formed thereon conductive material **403** defining electrode systems comprising a first electrode set **404** and a second electrode set **405**, and corresponding traces **406**, **407** and contact pads **408**, **409**, respectively. The conductive material **403** may contain pure metals or alloys, or other materials, which are metallic conductors. Preferably, the conductive material is absorptive at the wavelength of the laser used to form the electrodes and of a thickness amenable to rapid and precise processing. Non-limiting examples include aluminum, carbon, copper, chromium, gold, indium tin oxide (ITO), palladium, platinum, silver, tin oxide/gold, titanium, mixtures thereof, and alloys or metallic compounds of these elements. Preferably, the conductive material includes noble metals or alloys or their oxides. Most preferably, the conductive material includes gold, palladium, aluminum, titanium, platinum, ITO and chromium. The conductive material ranges in thickness from about 10 nm to 80 nm, more preferably, 30 nm to 70 nm, and most preferably 50 nm. It is appreciated that the thickness of the conductive material depends upon the transmissive property of the material and other factors relating to use of the biosensor.

While not illustrated, it is appreciated that the resulting patterned conductive material can be coated or plated with additional metal layers. For example, the conductive material may be copper, which is then ablated with a laser into an electrode pattern; subsequently, the copper may be plated with a titanium/tungsten layer, and then a gold layer, to form the desired electrodes. Preferably, a single layer of conductive material is used, which lies on the base **402**. Although not generally necessary, it is possible to enhance adhesion of the conductive material to the base, as is well known in the art, by using seed or ancillary layers such as chromium nickel or titanium. In preferred embodiments, biosensor **401** has a single layer of gold, palladium, platinum or ITO.

Biosensor **401** is illustratively manufactured using two apparatuses **410**, **410'**, shown in FIGS. **5**, **6** and **7**, respectively. It is appreciated that unless otherwise described, the apparatuses **410**, **410'** operate in a similar manner. Referring first to FIG. **5**, biosensor **401** is manufactured by feeding a roll of ribbon **420** having an 80 nm gold laminate, which is about 40 mm in width, into a custom fit broad field laser ablation apparatus **410**. The apparatus **410** comprises a laser source **411** producing a beam of laser light **412**, a chromium-plated quartz mask **414**, and optics **416**. It is appreciated that while the illustrated optics **416** is a single lens, optics **416** is preferably a variety of lenses that cooperate to make the light **412** in a pre-determined shape.

A non-limiting example of a suitable ablation apparatus **410** (FIGS. **5-6**) is a customized MicrolinerLaser 200-4 laser system commercially available from LPKF Laser Electronic GmbH, of Garbsen, Germany, which incorporates an LPX-400, LPX-300 or LPX-200 laser system commercially available from Lambda Physik AG, Göttingen, Germany and a chromium-plated quartz mask commercially available from International Phototool Company, Colorado Springs, Colo.

For the MicrolineLaser 200-4 laser system (FIGS. 5-6), the laser source **411** is a LPX-200 KrF-UV-laser. It is appreciated, however, that higher wavelength UV lasers can be used in accordance with this disclosure. The laser source **411** works at 248 nm, with a pulse energy of 600 mJ, and a pulse repeat frequency of 50 Hz. The intensity of the laser beam **412** can be infinitely adjusted between 3% and 92% by a dielectric beam attenuator (not shown). The beam profile is 27×15 mm² (0.62 sq. inch) and the pulse duration 25 ns. The layout on the mask **414** is homogeneously projected by an optical elements beam expander, homogenizer, and field lens (not shown). The performance of the homogenizer has been determined by measuring the energy profile. The imaging optics **416** transfer the structures of the mask **414** onto the ribbon **420**. The imaging ratio is 2:1 to allow a large area to be removed on the one hand, but to keep the energy density below the ablation point of the applied chromium mask on the other hand. While an imaging of 2:1 is illustrated, it is appreciated that the any number of alternative ratios are possible in accordance with this disclosure depending upon the desired design requirements. The ribbon **420** moves as shown by arrow **425** to allow a number of layout segments to be ablated in succession.

The positioning of the mask **414**, movement of the ribbon **420**, and laser energy are computer controlled. As shown in FIG. 5, the laser beam **412** is projected onto the ribbon **420** to be ablated. Light **412** passing through the clear areas or windows **418** of the mask **414** ablates the metal from the ribbon **420**. Chromium coated areas **424** of the mask **414** blocks the laser light **412** and prevent ablation in those areas, resulting in a metallized structure on the ribbon **420** surface. Referring now to FIG. 6, a complete structure of electrical components may require additional ablation steps through a second mask **414'**. It is appreciated that depending upon the optics and the size of the electrical component to be ablated, that only a single ablation step or greater than two ablation steps may be necessary in accordance with this disclosure. Further, it is appreciated that instead of multiple masks, that multiple fields may be formed on the same mask in accordance with this disclosure.

Specifically, a second non-limiting example of a suitable ablation apparatus **410'** (FIG. 7) is a customized laser system commercially available from LPKF Laser Electronic GmbH, of Garbsen, Germany, which incorporates a Lambda STEEL (Stable energy excimer laser) laser system commercially available from Lambda Physik AG, Göttingen, Germany and a chromium-plated quartz mask commercially available from International Phototool Company, Colorado Springs, Colo. The laser system features up to 1000 mJ pulse energy at a wavelength of 308 nm. Further, the laser system has a frequency of 100 Hz. The apparatus **410'** may be formed to produce biosensors with two passes as shown in FIGS. 5 and 6, but preferably its optics permit the formation of a 10×40 mm pattern in a 25 ns single pass.

While not wishing to be bound to a specific theory, it is believed that the laser pulse or beam **412** that passes through the mask **414**, **414'**, **414''** is absorbed within less than 1 μm of the surface **402** on the ribbon **420**. The photons of the beam **412** have an energy sufficient to cause photo-dissociation and the rapid breaking of chemical bonds at the metal/polymer interface. It is believed that this rapid chemical bond breaking causes a sudden pressure increase within the absorption region and forces material (metal film **403**) to be ejected from the polymer base surface. Since typical pulse durations are around 20-25 nanoseconds, the interaction with the material occurs very rapidly and thermal damage to edges of the conductive material **403** and surrounding structures is mini-

mized. The resulting edges of the electrical components have high edge quality and accurate placement as contemplated by the present invention.

Fluence energies used to remove or ablate metals from the ribbon **420** are dependent upon the material from which the ribbon **420** is formed, adhesion of the metal film to the base material, the thickness of the metal film, and possibly the process used to place the film on the base material, i.e. supporting and vapor deposition. Fluence levels for gold on KALADDEX® range from about 50 to about 90 mJ/cm², on polyimide about 100 to about 120 mJ/cm², and on MELINEX® about 60 to about 120 mJ/cm². It is understood that fluence levels less than or greater than the above mentioned can be appropriate for other base materials in accordance with the disclosure.

Patterning of areas of the ribbon **420** is achieved by using the masks **414**, **414'**. Each mask **414**, **414'** illustratively includes a mask field **422** containing a precise two-dimensional illustration of a pre-determined portion of the electrode component patterns to be formed. FIG. 5 illustrates the mask field **422** including contact pads and a portion of traces. As shown in FIG. 6, the second mask **414'** contains a second corresponding portion of the traces and the electrode patterns containing fingers. As previously described, it is appreciated that depending upon the size of the area to be ablated, the mask **414** can contain a complete illustration of the electrode patterns (FIG. 7), or portions of patterns different from those illustrated in FIGS. 5 and 6 in accordance with this disclosure. Preferably, it is contemplated that in one aspect of the present invention, the entire pattern of the electrical components on the test strip are laser ablated at one time, i.e., the broad field encompasses the entire size of the test strip (FIG. 7). In the alternative, and as illustrated in FIGS. 5 and 6, portions of the entire biosensor are done successively.

While mask **414** will be discussed hereafter, it is appreciated that unless indicated otherwise, the discussion will apply to masks **414'**, **414''** as well. Referring to FIG. 5, areas **424** of the mask field **422** protected by the chrome will block the projection of the laser beam **412** to the ribbon **420**. Clear areas or windows **418** in the mask field **422** allow the laser beam **412** to pass through the mask **414** and to impact predetermined areas of the ribbon **420**. As shown in FIG. 5, the clear area **418** of the mask field **422** corresponds to the areas of the ribbon **420** from which the conductive material **403** is to be removed.

Further, the mask field **422** has a length shown by line **430** and a width as shown by line **432**. Given the imaging ratio of 2:1 of the LPX-200, it is appreciated that the length **30** of the mask is two times the length of a length **434** of the resulting pattern and the width **432** of the mask is two times the width of a width **436** of the resulting pattern on ribbon **420**. The optics **416** reduces the size of laser beam **412** that strikes the ribbon **420**. It is appreciated that the relative dimensions of the mask field **422** and the resulting pattern can vary in accordance with this disclosure. Mask **414'** (FIG. 6) is used to complete the two-dimensional illustration of the electrical components.

Continuing to refer to FIG. 5, in the laser ablation apparatus **410** the excimer laser source **411** emits beam **412**, which passes through the chrome-on-quartz mask **414**. The mask field **422** causes parts of the laser beam **412** to be reflected while allowing other parts of the beam to pass through, creating a pattern on the gold film where impacted by the laser beam **412**. It is appreciated that ribbon **420** can be stationary relative to apparatus **410** or move continuously on a roll through apparatus **410**. Accordingly, non-limiting rates of movement of the ribbon **420** can be from about 0 ml/min to

about 100 m/min, more preferably about 30 m/min to about 60 m/min. It is appreciated that the rate of movement of the ribbon 420 is limited only by the apparatus 410 selected and may well exceed 100 m/min depending upon the pulse duration of the laser source 411 in accordance with the present disclosure.

Once the pattern of the mask 414 is created on the ribbon 420, the ribbon is rewound and fed through the apparatus 410 again, with mask 414' (FIG. 6). It is appreciated, that alternatively, laser apparatus 410 could be positioned in series in accordance with this disclosure. Thus, by using masks 414, 414', large areas of the ribbon 420 can be patterned using step-and-repeat processes involving multiple mask fields 422 in the same mask area to enable the economical creation of intricate electrode patterns and other electrical components on a substrate of the base, the precise edges of the electrode components, and the removal of greater amounts of the metallic film from the base material.

The ability to code information directly onto the test strip can dramatically increase the capabilities of the test strip and enhance its interaction with the test meter. For example, it is well known in the art to supply the test meter with calibration data applicable to any given manufacturing lot of test strips. Typically, this is done by supplying a read-only memory key (ROM key) with each vial of test strips, where the ROM key has encoded thereon the calibration data applicable to the test strips in the vial. Before using the test strips from the vial, the user inserts the ROM key into a port in the test meter so that the test meter may have access to this data while performing tests using the test strip. The quality of the measurement result can be verified by allowing the meter to electronically assess the applicability of the ROM key data to the test strip currently inserted into the meter, without the need for an optical reader to read bar code information on the test strip as has been taught in the prior art.

Current commercially-available products require the user to be involved in verifying the correct ROM key has been inserted into the test meter for the test strip currently being used. For example, FIG. 8 illustrates a typical prior art process for verifying the match between the ROM key data and the test strip lot identification (ID) number. Prior to executing this process, the ROM key has been inserted into the test meter, the ROM data has been loaded into the test meter, and the test meter is turned off. The process begins by inserting a test strip (step 100) into the test meter, which causes the test meter to automatically turn on (step 102). The test meter displays the lot ID of the currently loaded calibration data (step 104) in order to give the user the chance to verify that this lot ID matches the lot ID printed on the vial/package (for example) containing a plurality of test strips from the same production lot as the test strip currently inserted into the test meter.

Because the process relies upon the user to perform this check, there is no way to guarantee that it is done or if it is, that it is done accurately. The process of FIG. 8 therefore indicates an optional step for the user to compare the lot ID on the test meter display to the lot ID on the test strip vial (step 106) and to determine (step 108) if there is a match. If the two lot IDs do not match, then the user should remove the test strip (step 110) and insert the ROM key that matches the test strip vial into the test meter (step 112) so that the proper calibration code can be loaded into the test meter. The process would then start over at step 100 with the insertion of the test strip. Once it has been determined that the test meter's calibration code lot ID matches the lot ID of the test strip (step 108), then the measurement sequence can continue by applying blood to the test strip (step 114) and beginning the blood glucose measurement cycle (step 116).

It will be appreciated that responsibility for verification of the accuracy of the measurement calibration data has been placed completely in the hands of the user in the prior art process of FIG. 8. It is sometimes encountered that users ignore stated use instructions provided with the test strips. One such example is the removal of test strips from a first vial that were manufactured in lot X and consolidating these test strips into a second vial containing test strips manufactured in lot Y. Therefore, it is desirable to bring lot specific calibration information to the individual test strip level instead of to the vial level as is done in the prior art.

In order to remove the possibility of human error or neglect from the process, and to thereby improve the quality of the measurement, the information contact pads of the present invention allow the test meter itself to perform checks as to the applicability of the currently loaded calibration data to the currently inserted test strip. A first embodiment process of the present invention to allow the test meter to actively participate in such verification is illustrated in FIG. 9. The steps of the process of FIG. 9 that are identical to the corresponding steps in FIG. 8 are numbered with the same reference designators.

Prior to executing this process, the ROM key has been inserted into the test meter, the ROM data has been loaded into the test meter, and the test meter is turned off. The process begins by inserting a test strip (step 100) into the test meter, which causes the test meter to automatically turn on (step 102). The test meter then measures the conductivity between the various information and measurement contact pads on the test strip that have been designated for encoding information onto the test strip in order to ascertain the lot or family ID of the test strip (step 200). Depending upon the quantity of information that may be encoded onto the test strip, it may or may not be possible to code a unique production lot number onto the test strip. If there is not sufficient space for unique production lot IDs to be encoded, it is still possible to encode calibration family information onto the test strip. For example, the test strips usable in the test meter may be of two or more families where significant differences exist between the family test strip designs. For example, two families may use a different reagent on the test strip. In such situations, the test meter can still verify that the loaded calibration data matches the test strip family encoded onto the test strip, even if it is not possible to verify the precise production lot of the test strip. Therefore, as used herein, the phrase "lot ID" is intended to encompass any information that identifies a group to which the test strip or calibration data belongs, even if that group is not as small as a production lot of the test strip.

Returning to the process of FIG. 9, the test meter compares (step 202) the lot ID of the calibration data stored within the ROM key currently inserted into the meter (or calibration data previously-loaded into the test meter internal memory) to the lot ID read from the test strip. If they do not match, the test meter displays the lot ID of the currently loaded calibration data (step 204) and a warning in order to give the user the chance to insert a correct test strip or to insert a different ROM key into the test meter. Alternatively, the test meter may simply display an error message to the user. The fact that the lot IDs do not match is flagged (step 206) in the test meter's result memory 203 so that there is a record in the memory 203 that the measurement result obtained is suspect in view of the discrepancy in the lot IDs. Alternatively, the user may be prohibited from running a test and the process may be aborted.

Because in some embodiments it is desired that the test meter not be completely disabled if the lot IDs do not match, the process of FIG. 9 indicates an optional step for the user to compare the lot ID on the test meter display to the lot ID on the

15

test strip vial (step 106) and to determine (step 108) if there is a match. If the two lot IDs do not match, then the user should remove the test strip (step 110) and insert the ROM key that matches the test strip vial into the test meter (step 112) so that the proper calibration code can be loaded into the test meter. The process would then start over at step 100 with the insertion of the test strip.

Also optionally, if the test meter has the capacity to store more than one calibration dataset within the meter's internal memory, then the meter may determine the multiple lot IDs of calibration data that may be stored within the test meter and automatically choose the calibration dataset that matches the test strip currently inserted into the meter. The meter can then return to step 114.

Once it has been determined that the test meter's calibration code lot ID matches the lot ID of the test strip (step 108), then the measurement sequence can continue by applying blood to the test strip (step 114) and beginning the blood glucose measurement cycle (step 116). It will be appreciated that the process of FIG. 9 represents an improvement over the prior art process of FIG. 8 in that the user is automatically warned when the lot ID of the test strip does not match the lot ID of the currently-selected calibration dataset. Furthermore, if a test is conducted with this mismatched combination, then the result memory within the test meter is flagged to indicate that the result may not be as accurate as would be the case if the correct calibration dataset were used.

As a further example of the usefulness of encoding information directly onto the test strip, the present invention allows the test strip to activate or deactivate certain features programmed into the test meter. For example, a single test meter may be designed to be used in several different geographic markets, where a different language is spoken in each market. By encoding the test strips with information indicating in which market the test strips were sold, the encoded information can cause the test meter to display user instructions and data in a language that is appropriate for that market. Also, a meter may be designed for sale in a certain geographic market and it is desired that the meter not be used with test strips obtained in a different geographic market (for example when governmental regulations require the test strips sold in one geographic market to have different features than those sold in other geographic markets). In this situation, information coded onto the test strip may be used by the test meter to determine that the test strip did not originate in the designated geographic market and therefore may not provide the features required by regulation, in which case the test may be aborted or flagged.

Further, a business model (subscription business model) may be applied for the distribution of test strips where proliferation of the test strips into other sales channels is not desired. For example, users may enroll into a subscription program in which they are provided with a test meter designed for use by subscription participants, and the subscription participants may be provided with subscription test strips on a regular basis (for example by mail or any other convenient form of delivery). Using the techniques of the present invention, the "subscription test strips" may be encoded to indicate that they were supplied to a subscription participant. For a variety of reasons, the manufacturer of the subscription test strips may not want the subscription test strips to be sold in other channels of trade. One way to prevent this is to design test meters provided to users who are not subscription participants that will not work with subscription test strips. Therefore, the present invention may be used to provide test meters to subscription participants in the subscription business model that are programmed to accept sub-

16

scription test strips encoded to indicate that they are delivered to a user on the basis of a subscription, while other test meters are programmed not to accept subscription test strips so encoded.

As a further example, the test meter can have certain functionalities (software- and/or hardware-implemented) designed into the meter that are not active when the test meter is first sold. The performance of the test meter can then be upgraded at a later date by including information encoded on the test strips sold at that later time that will be recognized by the meter as an instruction to activate these latent features. As used herein, the phrase "activating a latent feature of the test meter" comprehends turning on a test meter functionality that previously was not active, such that the test meter functionality thereafter remains activated indefinitely (i.e. after the current test with the present test strip is finished).

Another example of information that can be encoded onto the test strip using the present invention is an indication of whether the test strip was sold to the hospital market or to the consumer market. Having this information may allow the test meter to take action accordingly, such as displaying user instructions in less detail for the hospital professional. It will be appreciated by those skilled in the art that a variety of types of communication between the test strip and the test meter may be facilitated by the information encoding provided by the present invention.

A second embodiment test strip configuration that allows information to be encoded directly onto the test strip is illustrated in FIG. 10 and indicated generally at 300. The test strip 300 may preferably be formed generally as described above with respect to the test strips 10 and 401, with working 320, counter 322, dose sufficiency working 324, and dose sufficiency counter 326 electrodes may be formed as shown and coupled, respectively, to measurement contact pads W, C, DW and DC. These contact pads provide a conductive area upon the test strip 300 to be contacted by an electrical connector contact of the test meter once the test strip 300 is inserted into the test meter. The test strip may be formed with a sample inlet in the distal end of the test strip (as shown in FIG. 10), or with a sample inlet on the side of the test strip as shown in FIG. 1. The functionality of the information encoding portion thereof is not affected by the positioning of the measurement electrodes in either position.

It will be noted from an examination of FIG. 10 that the area surrounding the counter electrode contact pad C is formed to provide a relatively large expanse of conductive layer, which is divided into information contact pad positions B1-B7. In the second embodiment of the present invention, the conductive layer may be formed during manufacture of the test strip such that the conductive layer is either present or absent within each of the contact pad positions B1-B7, depending upon what number is to be encoded onto the test strip 300. It should be noted that the counter electrode contact pad C is always formed with the conductive layer present in this area, as this contact pad is always necessary for the making of measurements.

Each of the contact pads C, W, DC and DW, as well as each of the contact pad positions B1-B7 are contacted by individual contacts of a multi-pin electrical connector located within the test meter when the test strip 300 is inserted into the test meter. The multi-pin electrical connector allows electrical signals to be applied from the test meter to the test strip and vice versa. The test meter is programmed (by means well-known in the art), to measure the conductivity between the counter electrode contact pad C and each of the contact pad positions B1-B7. The contact pad C can therefore be selectively conductively coupled to each of the contact pad posi-

tions B1-B7 depending upon whether the conductive layer is formed, respectively, in each of the contact pad positions B1-B7. By measuring the conductivity between the contact pad C and each of the contact pad positions B1-B7, the test meter is able to determine the presence or absence of the conductive layer in each of the contact pad positions B1-B7. By assigning, for example, a digital value of "1" when the conductive layer is present in a particular contact pad position and a digital value of "0" when the conductive layer is absent in a particular contact pad position, a digital word may be encoded onto the test strip 300.

It will be appreciated that all of the desirable benefits discussed hereinabove with respect to the first embodiment of the present invention may also be achieved using the second embodiment of the present invention. The second embodiment has the added advantage that, because the contact pad positions B1-B7 can never be conductively coupled to more than one measurement electrode, there are no "forbidden" states and each of the contact pad positions B1-B7 may be coded as a "0" or "1" in any possible seven digit digital word to be encoded onto the test strip. This provides 2^7 or 128 possible unique words that can be encoded onto the test strip using the contact pad positions B1-B7. The number of contact pad positions that can be designated for such information encoding is only limited by the available space on the test strip surface, the resolution of the process used to define the conductive features on the test strip, the electrical connector contact spacing, and the tolerance stack-ups relevant to placing the connector contact on the contact pad position once the test strip is inserted into the test meter.

Furthermore, the number of possible states in the second embodiment of the present invention can be further increased by severing the conductive path between individual pairs of the contact pad positions B1-B7. Therefore, a connector contacting contact pad B1 (for example) can check for electrical continuity not only with contact pad C (as described hereinabove), but also for electrical continuity with any of the other contact pads B2-B7.

The laser ablation process described hereinabove allows for resolution of test strip conductive features not previously achievable using prior art techniques such as screen printing and photolithography. Because of this, relatively large quantities of data can be coded onto the test strip when the conductive features are formed using the laser ablation process. For example, a third embodiment of the present invention is illustrated in FIG. 11 and indicated generally at 500. The test strip 500 is similar to the test strip 300 of FIG. 10, except that the resolution of the laser ablation process allows for an even greater number of contact pads to be formed on the test strip. Equivalent structures in FIG. 11 are given the same reference designators as used in FIG. 10. A total of sixteen contact pads are formed on the test strip 500, with B1-B10 being designated as information contact pads in addition to the measurement contact pads W, WS, C, CS, DW and DC coupled to working 520, counter 522, dose sufficiency working 524, and dose sufficiency counter 526 electrodes. These contact pads provide a conductive area upon the test strip 500 to be contacted by an electrical connector contact of the test meter once the test strip 500 is inserted into the test meter. The test strip may be formed with a sample inlet in the distal end of the test strip (as shown in FIG. 11), or with a sample inlet on the side of the test strip as shown in FIG. 1. The functionality of the information encoding portion thereof is not affected by the positioning of the measurement electrodes in either position.

As with the second embodiment of FIG. 10, it will be noted from an examination of FIG. 11 that the area surrounding the counter electrode contact pad C is formed to provide a rela-

tively large expanse of conductive layer, which is divided into information contact pad positions B1-B10. In the third embodiment of the present invention, the conductive layer may be formed during manufacture of the test strip such that the conductive layer is either present or absent within each of the contact pad positions B1-B10, depending upon what number is to be encoded onto the test strip 500. As noted hereinabove, the counter electrode contact pad C is always formed with the conductive layer present in this area, as this contact pad is always necessary for the making of measurements.

Each of the contact pads C, CS, W, WS, DC and DW, as well as each of the contact pad positions B1-B10 are contacted by individual contacts of a multi-pin electrical connector located within the test meter when the test strip 500 is inserted into the test meter. The multi-pin electrical connector allows electrical signals to be applied from the test meter to the test strip and vice versa. The test meter is programmed to measure the conductivity between the counter electrode contact pad C and each of the contact pad positions B1-B10. The contact pad C can therefore be selectively conductively coupled to each of the contact pad positions B1-B10 depending upon whether the conductive layer is formed, respectively, in each of the contact pad positions B1-B10. By measuring the conductivity between the contact pad C and each of the contact pad positions B1-B10, the test meter is able to determine the presence or absence of the conductive layer in each of the contact pad positions B1-B10. By assigning, for example, a digital value of "1" when the conductive layer is present in a particular contact pad position and a digital value of "0" when the conductive layer is absent in a particular contact pad position, a digital word may be encoded onto the test strip 500.

It will be appreciated that, as with the second embodiment, all of the desirable benefits discussed hereinabove with respect to the first embodiment of the present invention may also be achieved using the third embodiment of the present invention. Like the second embodiment, the third embodiment has the added advantage that, because the contact pad positions B1-B10 can never be conductively coupled to more than one measurement electrode, there are no "forbidden" states and each of the contact pad positions B1-B10 may be coded as a "0" or "1" in any possible ten digit digital string to be encoded onto the test strip. This provides 2^{10} or 1,024 possible unique strings that can be encoded onto the test strip using the contact pad positions B1-B10.

Furthermore, as with the second embodiment test strip 300, the number of possible states in the third embodiment test strip 500 of the present invention can be further increased by severing the conductive path between individual pairs of the contact pad positions B1-B10. Therefore, a connector contacting contact pad B1 (for example) can check for electrical continuity not only with contact pad C (as described hereinabove), but also for electrical continuity with any of the other contact pads B2-B10. This greatly increases the number of unique digital words that can be encoded onto the test strip 500.

It should be noted that the contact pad densities achieved in the present invention through the use of the laser ablation process represent a significant advancement over the prior art. For example, published European patent application EP 1 024 358 A1 discloses a system which uses up to 35 contact pads on a single test strip; however, the density of features is so low that the inventors are forced to contact only five of those contact pads at any one time. Not only does this require much more test strip surface area than the present invention to form the same number of contact pads, but it is impossible for the test meter to make conductivity checks between each of the

contact pads because the test meter is never in contact with more than five of the contact pads at any one time. The tight control of feature dimensions enabled by the laser ablation process of the present invention allows for the use of contact pad density never before achieved in the art. For example, the embodiment of FIG. 10 allows eleven contact pads to be contacted simultaneously by the test meter connector. Even greater density is achieved in the embodiment of FIG. 11, where sixteen contact pads may be contacted simultaneously by the test meter connector. Some embodiments of the present invention therefore preferably include at least ten test strip contact pads coupled to at least ten test meter connector contacts; more preferably include at least eleven test strip contact pads coupled to at least eleven test meter connector contacts; and most preferably includes at least fifteen test strip contact pads coupled to at least fifteen test meter connector contacts.

FIGS. 12-14 illustrate a preferred embodiment multiple-pin electrical connector mating with the third embodiment test strip 500 of FIG. 11. The electrical connector is housed in the test meter (not shown) and includes multiple contacts that produce contact traces 502 when mated with respective contact pads on the test strip 500 when the test strip 500 is inserted into the test meter electrical connector. FIG. 13 illustrates the nominal case in which each electrical connector contact is positioned approximately at the center of the respective test strip 500 contact pad when the test strip 500 is mated to the test meter. In the preferred embodiment, the tolerances of the placement of the conductive features on the test strip 500, as well as the tolerances of the placement of the electrical connector contacts with respect to the test strip mating port of the test meter are controlled such that the worst case tolerance stack-ups will still result in reliable contact between each connector contact and the respective contact pad. As can be seen in FIG. 12, when all of the tolerances are at their maximum so as to move the connector contacts left with respect to their respective contact pads, the electrical contacts are still positioned to make reliable electrical contact with the respective contact pad, and all of the contact pads B1-B10 are still electrically connected to the contact pad C (if their respective metallization is present) even if the mechanical interaction of the connector contacts with the test strip during insertion completely removes the metallization in the areas of contact traces 502. Similarly, as can be seen in FIG. 14, when all of the tolerances are at their maximum so as to move the connector contacts right with respect to their respective contact pads, the electrical contacts are still positioned to make reliable electrical contact with the respective contact pad, and all of the contact pads B1-B10 are still electrically connected to the contact pad C (if their respective metallization is present) even if the mechanical interaction of the connector contacts with the test strip during insertion completely removes the metallization in the areas of contact traces 502.

A fourth embodiment test strip of the present invention is schematically illustrated in FIG. 15 and designated as 600. The test strip 600 is similar to the test strip 300 of FIG. 10, except that the fourth embodiment uses only six contact pads on the test strip. Embodiments using fewer or more contact pads are contemplated by the present invention. Equivalent structures in FIG. 15 are given the same reference designators as used in FIG. 10. The test strip includes a working electrode 320, a counter electrode 322, a dose sufficiency working electrode 324, and two potential dose sufficiency counter electrodes 326A and 326B. Each of the electrodes is coupled to at least one contact pad formed on the test strip 600.

The working electrode 320 is coupled to both a W and a WS contact pad. The counter electrode 322 is coupled to a C

contact pad and a CS contact pad, although which contact pad is designated as C is optional as explained hereinbelow. The dose sufficiency working electrode 324 is coupled to a DW contact pad. The dose sufficiency counter electrode 326A/326B is coupled to a DC contact pad, although which contact pad is designated as DC is optional as explained hereinbelow.

The test strip 600 allows a single binary bit to be encoded onto the test strip 600, depending on which of the two potential conductive links 602 and 604 are formed on the test strip 600. At least one of the potential conductive links 602/604 is preferably formed on the test strip 600, and both potential conductive links 602/604 may not be formed at the same time without losing the second separate dose sufficiency electrode functionality.

If the potential conductive link 602 is formed on the test strip 600 and the potential conductive link 604 is not formed, then the contact pad 606 becomes the C contact pad (since it is coupled to the counter electrode 322 by the potential conductive link 602). Without the presence of the potential conductive link 604, electrode 326B functions as the actual dose sufficiency counter electrode and contact pad 608 becomes the DC contact pad.

Similarly, if the potential conductive link 604 is formed on the test strip 600 and the potential conductive link 602 is not formed, then the contact pad 608 becomes the C contact pad (since it is coupled to the counter electrode 322 by the potential conductive link 604). Without the presence of the potential conductive link 602, electrode 326A functions as the actual dose sufficiency counter electrode and contact pad 606 becomes the DC contact pad.

Once the test strip 600 is inserted into the test meter, the test meter can easily determine if the potential conductive link 602 is present by checking the conductivity between the CS contact pad and the contact pad 606. Conductivity between these two contact pads indicates the presence of the potential conductive link 602. Similarly, the test meter can determine if the potential conductive link 604 is present by checking the conductivity between the CS contact pad and the contact pad 608. Conductivity between these two contact pads indicates the presence of the potential conductive link 604. Once the test meter has determined which potential conductive link 602/604 is present, it thereafter knows which contact pad to treat as the C contact pad and which to treat as the DC contact pad. In one embodiment, the test meter only checks for the presence or absence of one of the potential conductive links 602/604 and assumes that the other potential conductive link 602/604 is absent or present, respectively. In another embodiment, the test meter confirms the presence or absence of both potential conductive links 602/604, which is a more robust methodology as it is more likely to detect a damaged test strip.

In another embodiment, the code key inserted into the test meter tells the test meter which of the two possible configurations to expect. The test meter then checks to see if the expected contact pad 606/608 is coupled to the CS contact pad. If the expected connection is not present, then the meter checks to see if the other contact pad 606/608 is coupled to the CS contact pad. If the wrong contact pad 606/608 is coupled to the CS contact pad, then the meter indicates a code key error (i.e. a code key has been inserted into the test meter that does not match the test strip inserted into the test meter). If neither contact pad 606/608 is coupled to the CS contact pad, then the test meter indicates a strip error (i.e. the test strip is defective and cannot be used).

More importantly than assigning contact pad functionalities, by determining which potential conductive link 602/604 is present, the test meter has been supplied with one bit of information from the test strip 600. This single bit of infor-

21

mation can convey important information to the test meter, such as whether the test strip is designed to test for a first analyte or a second analyte, where the test meter should look for calibration information relating to the test strip, etc. Therefore, supplying a single bit of information by simply reassigning the functions of some of the contact pads on the test strip can easily provide important information to the test meter about the test strip that has been inserted therein.

All publications, prior applications, and other documents cited herein are hereby incorporated by reference in their entirety as if each had been individually incorporated by reference and fully set forth.

While the invention has been illustrated and described in detail in the drawings and foregoing description, the description is to be considered as illustrative and not restrictive in character. Only the preferred embodiment, and certain other embodiments deemed helpful in further explaining how to make or use the preferred embodiment, have been shown. All changes and modifications that come within the spirit of the invention are desired to be protected.

What is claimed is

1. A test strip for measuring a concentration of an analyte of interest in a biological fluid, the test strip comprising:

- a substrate having a surface;
- a first measurement electrode formed on the surface;
- a second measurement electrode formed on the surface;
- a first latent electrode formed on the surface;
- a second latent electrode formed on the surface;
- a first contact pad formed on the surface and conductively coupled to the first measurement electrode;
- a second contact pad formed on the surface and conductively coupled to the second measurement electrode;
- a third contact pad formed on the surface and conductively coupled to the first latent electrode;
- a fourth contact pad formed on the surface and conductively coupled to the second latent electrode; and
- a conductive link formed when manufacturing the test strip, said conductive link coupling one of the first and second latent electrodes to the first measurement electrode, whereby the one of the first and second latent electrodes coupled to the first measurement electrode is not used as an electrode and the one of the first and second latent electrodes not coupled to the first measurement electrode becomes an active electrode.

2. The test strip of claim 1, wherein the active electrode is a dose sufficiency electrode.

3. A method of using a test meter and associated test strip for measuring a concentration of an analyte of interest in a biological fluid, comprising the steps of:

- providing a test strip comprising:
 - a substrate having at least a first, second and third contact pad formed thereon; and
 - a conductive connection, formed during manufacture of the test strip, coupling either the first and second contact pads or the first and third contact pads;
- providing a test meter comprising a connector configured to make conductive contact with the first, second and third contact pads when the test strip is inserted into the test meter;
- operating the test meter to determine if conductivity exists between the first and second contact pads;
- operating the test meter to determine if conductivity exists between the first and third contact pads;
- designating the second contact pad to have a first function and the third contact pad to have a second function if the test meter determines that conductivity exists between

22

the first and second contact pads and that conductivity does not exist between the first and third contact pads; and

designating the second contact pad to have the second function and the third contact pad to have the first function if the test meter determines that conductivity does not exist between the first and second contact pads and that conductivity exists between the first and third contact pads.

4. A method of using a test meter and associated test strip for measuring a concentration of an analyte of interest in a biological fluid, comprising the steps of:

- providing a test strip comprising:
 - a substrate having at least a first, second and third contact pad formed thereon; and
 - a conductive connection, formed during manufacture of the test strip, coupling either the first and second contact pads or the first and third contact pads;
- providing a test meter comprising a connector configured to make conductive contact with the first, second and third contact pads when the test strip is inserted into the test meter;

operating the test meter to determine if conductivity exists between the first and second contact pads;

designating the second contact pad to have a first function and the third contact pad to have a second function if the test meter determines that conductivity exists between the first and second contact pads; and

designating the second contact pad to have the second function and the third contact pad to have the first function if the test meter determines that conductivity does not exist between the first and second contact pads.

5. A test strip for measuring a concentration of an analyte of interest in a biological fluid, the test strip comprising:

- a substrate having a surface;
- a first measurement electrode formed on the surface;
- a second measurement electrode formed on the surface;
- a first latent electrode formed on the surface;
- a second latent electrode formed on the surface;
- a first contact pad formed on the surface and conductively coupled to the first measurement electrode;
- a second contact pad formed on the surface and conductively coupled to the second measurement electrode;
- a third contact pad formed on the surface and conductively coupled to the first latent electrode;
- a fourth contact pad formed on the surface and conductively coupled to the second latent electrode; and
- a conductive link coupling one of the first and second latent electrodes to the first measurement electrode prior to said biological fluid being applied to the test strip, whereby the one of the first and second latent electrodes coupled to the first measurement electrode is not used as an electrode and the one of the first and second latent electrodes not coupled to the first measurement electrode becomes an active electrode.

6. The test strip of claim 5, wherein the active electrode is a dose sufficiency electrode.

7. A method of using a test meter and associated test strip for measuring a concentration of an analyte of interest in a biological fluid, comprising the steps of:

- providing a test strip comprising a substrate having at least a first, second and third contact pad formed thereon;
- providing a test meter comprising a connector configured to make conductive contact with the first, second and third contact pads when the test strip is inserted into the test meter;

23

operating the test meter prior to application of the biological fluid to the test strip to determine if conductivity exists between the first and second contact pads;
operating the test meter prior to application of the biological fluid to the test strip to determine if conductivity exists between the first and third contact pads;
designating the second contact pad to have a first function and the third contact pad to have a second function if the test meter determines that conductivity exists between the first and second contact pads and that conductivity does not exist between the first and third contact pads;
and
designating the second contact pad to have the second function and the third contact pad to have the first function if the test meter determines that conductivity does not exist between the first and second contact pads and that conductivity exists between the first and third contact pads.

8. A method of using a test meter and associated test strip for measuring a concentration of an analyte of interest in a biological fluid, comprising the steps of:
providing a test strip comprising a substrate having at least a first, second and third contact pad formed thereon;
providing a test meter comprising a connector configured to make conductive contact with the first, second and third contact pads when the test strip is inserted into the test meter;
operating the test meter prior to application of the biological fluid to the test strip to determine if conductivity exists between the first and second contact pads;
designating the second contact pad to have a first function and the third contact pad to have a second function if the test meter determines that conductivity exists between the first and second contact pads; and
designating the second contact pad to have the second function and the third contact pad to have the first function if the test meter determines that conductivity does not exist between the first and second contact pads.

9. A test strip for measuring a concentration of an analyte of interest in a biological fluid, the test strip comprising:
a substrate having a surface;
a first measurement electrode formed on the surface;
a second measurement electrode formed on the surface;
a first latent electrode formed on the surface;
a second latent electrode formed on the surface;
a first contact pad formed on the surface and conductively coupled to the first measurement electrode;
a second contact pad formed on the surface and conductively coupled to the second measurement electrode;
a third contact pad formed on the surface and conductively coupled to the first latent electrode;
a fourth contact pad formed on the surface and conductively coupled to the second latent electrode; and
a conductive link coupling one of the first and second latent electrodes to the first measurement electrode independent of said biological fluid, whereby the one of the first

24

and second latent electrodes coupled to the first measurement electrode is not used as an electrode and the one of the first and second latent electrodes not coupled to the first measurement electrode becomes an active electrode.

10. The test strip of claim 9, wherein the active electrode is a dose sufficiency electrode.

11. A method of using a test meter and associated test strip for measuring a concentration of an analyte of interest in a biological fluid, comprising the steps of:
providing a test strip comprising a substrate having at least a first, second and third contact pad formed thereon;
providing a test meter comprising a connector configured to make conductive contact with the first, second and third contact pads when the test strip is inserted into the test meter;
operating the test meter to determine if conductivity exists between the first and second contact pads independent of said biological fluid;
operating the test meter to determine if conductivity exists between the first and third contact pads independent of said biological fluid;
designating the second contact pad to have a first function and the third contact pad to have a second function if the test meter determines that conductivity exists between the first and second contact pads and that conductivity does not exist between the first and third contact pads; and
designating the second contact pad to have the second function and the third contact pad to have the first function if the test meter determines that conductivity does not exist between the first and second contact pads and that conductivity exists between the first and third contact pads.

12. A method of using a test meter and associated test strip for measuring a concentration of an analyte of interest in a biological fluid, comprising the steps of:
providing a test strip comprising a substrate having at least a first, second and third contact pad formed thereon;
providing a test meter comprising a connector configured to make conductive contact with the first, second and third contact pads when the test strip is inserted into the test meter;
operating the test meter to determine if conductivity exists between the first and second contact pads independent of said biological fluid;
designating the second contact pad to have a first function and the third contact pad to have a second function if the test meter determines that conductivity exists between the first and second contact pads; and
designating the second contact pad to have the second function and the third contact pad to have the first function if the test meter determines that conductivity does not exist between the first and second contact pads.

* * * * *

UNITED STATES PATENT AND TRADEMARK OFFICE
CERTIFICATE OF CORRECTION

PATENT NO. : 7,604,721 B2
APPLICATION NO. : 10/871489
DATED : October 20, 2009
INVENTOR(S) : Groll et al.

Page 1 of 1

It is certified that error appears in the above-identified patent and that said Letters Patent is hereby corrected as shown below:


On the Title Page:

The first or sole Notice should read --

Subject to any disclaimer, the term of this patent is extended or adjusted under 35 U.S.C. 154(b) by 1127 days.

Signed and Sealed this

Fifth Day of October, 2010

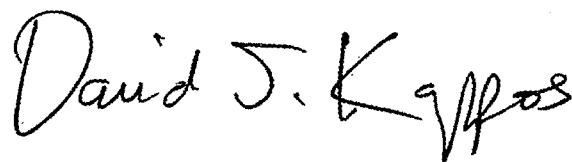A handwritten signature in black ink that reads "David J. Kappos". The signature is written in a cursive, flowing style.

David J. Kappos
Director of the United States Patent and Trademark Office