

(19) World Intellectual Property Organization  
International Bureau



(43) International Publication Date  
31 May 2007 (31.05.2007)

PCT

(10) International Publication Number  
**WO 2007/062306 A2**

(51) International Patent Classification:  
A61L 33/00 (2006.01) B05D 3/00 (2006.01)

(21) International Application Number:  
PCT/US2006/060929

(22) International Filing Date:  
15 November 2006 (15.11.2006)

(25) Filing Language: English

(26) Publication Language: English

(30) Priority Data:  
60/738,198 18 November 2005 (18.11.2005) US

(71) Applicant (for all designated States except US): **THE BOARD OF REGENTS OF THE UNIVERSITY OF TEXAS SYSTEM** [US/US]; 201 W. 7th St., Austin, TX 78701 (US).

(72) Inventor; and

(75) Inventor/Applicant (for US only): **RAAD, Issam** [US/US]; 4207 Clearwater Court, Missouri City, TX 77459 (US).

(74) Agent: **DE LA PAZ, Monica, A.**; FULBRIGHT & JAWORSKI L.L.P., 600 Congress Avenue, Suite 2400, Austin, TX 78701 (US).

(81) Designated States (unless otherwise indicated, for every kind of national protection available): AE, AG, AL, AM, AT, AU, AZ, BA, BB, BG, BR, BW, BY, BZ, CA, CH, CN, CO, CR, CU, CZ, DE, DK, DM, DZ, EC, EE, EG, ES, FI, GB, GD, GE, GH, GM, GT, HN, HR, HU, ID, IL, IN, IS, JP, KE, KG, KM, KN, KP, KR, KZ, LA, LC, LK, LR, LS, LT, LU, LV, LY, MA, MD, MG, MK, MN, MW, MX, MY, MZ, NA, NG, NI, NO, NZ, OM, PG, PH, PL, PT, RO, RS, RU, SC, SD, SE, SG, SK, SL, SM, SV, SY, TJ, TM, TN, TR, TT, TZ, UA, UG, US, UZ, VC, VN, ZA, ZM, ZW.

(84) Designated States (unless otherwise indicated, for every kind of regional protection available): ARIPO (BW, GH, GM, KE, LS, MW, MZ, NA, SD, SL, SZ, TZ, UG, ZM, ZW), Eurasian (AM, AZ, BY, KG, KZ, MD, RU, TJ, TM), European (AT, BE, BG, CH, CY, CZ, DE, DK, EE, ES, FI, FR, GB, GR, HU, IE, IS, IT, LT, LU, LV, MC, NL, PL, PT, RO, SE, SI, SK, TR), OAPI (BF, BJ, CF, CG, CI, CM, GA, GN, GQ, GW, ML, MR, NE, SN, TD, TG).

**Published:**

— without international search report and to be republished upon receipt of that report

For two-letter codes and other abbreviations, refer to the "Guidance Notes on Codes and Abbreviations" appearing at the beginning of each regular issue of the PCT Gazette.

(54) Title: METHODS FOR COATING SURFACES WITH ANTIMICROBIAL AGENTS

(57) Abstract: Disclosed are methods for coating or impregnating a surface with an antimicrobial agent that involve contacting the surface with a composition that includes an antimicrobial agent and a solvent, and curing the surface by applying heat. Also disclosed are methods for reducing the risk of development or progression of an infection in a subject in need of a medical device, that involve coating or impregnating a surface of the medical device with an antimicrobial agent and then curing the surface by applying heat, wherein the risk of development or progression of an infection is reduced.



WO 2007/062306 A2

## DESCRIPTION

### METHODS FOR COATING SURFACES WITH ANTIMICROBIAL AGENTS

#### BACKGROUND OF THE INVENTION

[0001] The present application is related to U.S. Provisional Patent Application 60/738,198,  
5 filed on November 18, 2005, which is hereby incorporated by reference in its entirety.

#### **1. Field of the Invention**

[0002] The present invention relates generally to the fields of infectious disease control and medical devices. More particularly, the invention provides methods for coating antiseptic and antimicrobial compositions onto a surface, such as the surface of a medical device.

#### **10 2. Description of Related Art**

[0003] Medical devices, such as urinary catheters, endotracheal tubes and central venous catheters (CVC), are the driving and leading cause of hospital-acquired infections in high-risk patients. These high-risk patients include critically ill patients admitted to the Intensive Care Unit (ICU), cancer patients, or patients with chronic diseases requiring long-term care, such  
15 as those patients on total parenteral nutrition (TPN). Anti-infective devices coated with antimicrobial agents have been shown to significantly decrease the risk of device-related and hospital-acquired infection.

[0004] Most nosocomial (hospital-acquired) infections are caused by the contamination of medical devices. One class of nosocomial infection is nosocomial pneumonia. Nosocomial  
20 pneumonias are associated with a very high attributable mortality and morbidity. Recent data have shown that at least 300,000 episodes of nosocomial pneumonia occur annually in the United States (Official Statement, American Thoracic Society). The attributable mortality of nosocomial pneumonia is 33%-50%, hence, around 100,000 patients die annually because of nosocomial pneumonia (CDC, 1993; Leu *et al.*, 1989). The risk of nosocomial pneumonia  
25 increases 6- to 20-fold from the use of mechanical ventilation (Official Statement, American Thoracic Society).

[0005] The endotracheal tube is considered a common vehicle for colonization/contamination leading to nosocomial pneumonia. The endotracheal tube connects the oropharyngeal environment with the sterile bronchoalveolar space, significantly increasing the risk of

nosocomial pneumonia. Endotracheal tubes are typically constructed of polyvinylchloride, which is known to be very difficult to impregnate with antiseptic or antimicrobial agents. Thus, there are no endotracheal tubes that are impregnated with antibiotics or antiseptics currently in use.

5 [0006] Another class of nosocomial infections includes bloodstream infections. The primary contributors to nosocomial bloodstream infections are vascular catheters. It is estimated that around 400,000 vascular catheter-related bloodstream infections (CRBSI) occur annually in the United States (Raad, 1998). The attributable mortality of these infections in the intensive care unit (ICU) was estimated in JAMA in 1994 to be 25% (Reiselman *et al.*, 1994). Hence,  
10 these infections are a major cause of morbidity and mortality in hospitalized patients. Vascular catheters are mostly polyurethane short-term catheters used in the ICU and long-term silicone catheters used in cancer/AIDS patients.

[0007] The most common class of nosocomial infection are urinary tract infections (UTI), contributing to 34% of all nosocomial infections (Klempner *et al.*, 1998). Nosocomial UTI  
15 are usually associated with contamination of urinary catheters. In addition, nosocomial surgical wound infections are common complications of surgical procedures, particularly in cancer and immunocompromised patients with devitalized tissue and decreased immunity. Surgical wound infections contribute to 17% of all nosocomial infections (Platt and Bucknall, 1988). Many surgical wound infections are associated with the contamination of sutures.

20 [0008] Antibiotics and antiseptics have been used to impregnate vascular catheters. The concern with the use of antibiotics has been that resistance might develop to antibiotics, preventing their use therapeutically and systemically in hospitalized patients. Furthermore, the durability of the existing antiseptics has been limited. For example, the use of chlorhexidine/silver sulfadiazine on polyurethane surfaces has had limited effectiveness.  
25 Moreover, chlorhexidine/silver sulfadiazine impregnating the surface of vascular catheters resulted in limited activity against gram-negative bacilli, such as *Pseudomonas* (Raad *et al.* 1996).

[0009] U.S. Patent App. Pub. No. 20050197634 and 20030078242 describe certain antiseptic coatings on medical devices. These applications have shown that antiseptics consisting of  
30 antiseptic dyes (such as Gentian violet) and quadinium compounds (such as chlorhexidine) are highly effective as a combination in coating various medical devices and preventing the

adherence of diverse resistant bacteria and fungi (including gram-positive and gram-negative bacteria as well as *Candida* spp.) U.S. Patent 5,624,704 discloses methods for impregnating a non-metallic medical implant with an antimicrobial agent.

5 [00010] Although highly effective from an antimicrobial perspective, the drawback of antiseptic dyes is their high level of leaching into body fluids (such as urine, serum or bronchoalveolar lavage) as well as their staining potential. The leaching into body fluids might lead to systemic toxicity clinically. The staining could lead to a cosmetic problem, thus making these devices unmarketable. Thus, there thus exists a need for improved methods for coating medical devices with antiseptics that reduces the risk of nosocomial infections.

### 10 SUMMARY OF THE INVENTION

[00011] The present invention provides for novel methods of coating or impregnating a surface with an antimicrobial agent. For example, the inventors have found that their method of coating or impregnating a surface with an antimicrobial agent can be applied in coating or impregnating a medical device with an antimicrobial agent such that there is a decrease in staining potential of the medical device, decrease in leaching of the antimicrobial into tissue, and prolonged antimicrobial efficacy.

20 [00012] The present invention generally pertains to methods for coating or impregnating a surface with an antimicrobial agent, that involve (1) contacting the non-organic surface with an composition that includes an antimicrobial agent and a solvent; and (2) curing the surface at a temperature that is at least about 40°C, wherein at least some of the solvent that was contacted with the surface is removed, and wherein the antimicrobial agent coats or impregnates the surface. An “antimicrobial agent” as used herein refers to an agent that can prevent or reduce the growth or reproduction of a microorganism or kill a microorganism. A “microorganism” is defined herein to refer to a bacterium, a fungus, a protozoan, or a virus.

25 In particular embodiments, the surface is a non-organic surface. A “non-organic surface” as used herein refers to a superficial or external aspect of any object other than a living organism. By way of example, the surface may be the surface of medical device.

[00013] A “medical device” is defined herein to refer to an instrument, apparatus, implement, machine, contrivance, implant, or other similar or related article, including a component part, or accessory which is intended for use in the diagnosis, treatment, or prevention of disease or other health-related conditions in a subject. The subject can be any vertebrate, such as a

mammal. In particular embodiments, the subject is a human. Non-limiting examples of medical devices include a stent, a tube, a catheter, or a valve. A “stent” as used herein refers to a thread, rod, or catheter inserted into a tubular structure, such as a blood vessel, to provide support during or after anastomosis. A “catheter” is defined herein to refer to a hollow tube  
5 (which may or may not be flexible) for insertion into a body cavity, duct, or vessel to allow the passage of fluids or distend a passageway. Particular non-limiting examples of medical devices include an endotracheal tube, tracheotomy tube, ureteral stent, biliary stent, ventriculostomy catheters, chest tube, a vascular catheter, an urinary catheter, a gastric tube, an intestinal tube, a nephrostomy tube, a biliary stent, a peritoneal catheter, an epidural catheter, a  
10 central nervous system catheter, an orthopedic device, a prosthetic valve, orthopedic devices, pacemakers, infusion pumps, infusion ports, dialysis catheters, neurotransmitters, drug-delivery implant, and gloves. Non-limiting examples of vascular catheters include of a central venous catheter, an arterial line, a pulmonary artery catheter, a stent, and a peripheral venous catheter.

[00014] Other medical devices that can benefit from the present invention include blood  
15 exchanging devices, vascular access ports, cardiovascular catheters, extracorporeal circuits, stents, implantable prostheses, vascular grafts, pumps, heart valves, and cardiovascular sutures, to name a few. Regardless of detailed embodiments, applicability of the invention should not be considered limited with respect to the type of medical device, implant location or materials of construction of the device.

[00015] Other examples of non-organic surfaces contemplated by the present invention  
20 include surfaces of medical supplies and medical equipment. Non-limiting examples of medical supplies and equipment include gloves (such as disposable gloves), gowns, pads, wheelchairs, stretchers, tables, swabs, sponges, sutures (such as silk sutures), bags, surgical supplies, and packaging materials for the packaging of sterile medical or hospital supplies.  
25 Further examples of non-organic surfaces include the surfaces of a sponge, wipe, pad, or mop.

[00016] Further examples of non-organic surfaces include floors, countertops, the surface of  
30 a container (such as for food storage), and the surfaces of food processing supplies and equipment, mopping equipment or sponges. Still further examples of non-organic surfaces include the surface of personal care products such as gloves, condoms, diaphragms, sanitary napkins.

[00017] The antimicrobial agent can be any antimicrobial agent known to those of ordinary skill in the art. For example, the antimicrobial agent may be an antibiotic, an antiseptic, an antiviral agent, an antifungal agent, or a disinfectant. An "antibiotic" is defined herein to refer to a compound or agent that can prevent or reduce the growth and reproduction of a bacterium or kill a bacterium. Some antibiotics kill bacteria, whereas others prevent or inhibit their growth. Antibiotics are applied in the treatment of subjects with infections, such as bloodstream infections. They are administered via any of a variety of routes, such as through oral, intravenous, subcutaneous, or intramuscular routes. Examples of antibiotics include penicillin, cephalosporins, vancomycin, minocycline, and rifampin. In certain embodiments, the antibiotic is a tetracycline or a macrocyclic antibiotic or a combination thereof. The tetracycline can be any tetracycline known to those of ordinary skill in the art, such as minocycline. Non-limiting examples of macrocyclic antibiotics include rifampin, rifampicin, or a combination thereof. Additional examples of antibiotics are discussed in the specification below.

[00018] As used herein, the term "antifungal agent" is defined as a compound having either a fungicidal or fungistatic effect upon fungi contacted by the compound. As used herein, the term "fungicidal" is defined to mean having a destructive killing action upon fungi. As used herein, the term "fungistatic" is defined to mean having an inhibiting action upon the growth of fungi. As used herein, the term "antiviral agent" is defined as a compound that can either kill viral agents or one that stops the replication of viruses upon contact by the compound.

[00019] The antimicrobial agent may also be an antiseptic. An "antiseptic" is defined herein to refer to an agent that can prevent or reduce the growth and reproduction of any microorganism (such as bacteria, fungi, protozoa, and viruses) or kill any microorganism but which is generally not applied in the treatment of a systemic infection in a subject usually because of limitations related to absorption, penetration, or systemic toxicity. These agents can generally be used on the skin and external mucosal surfaces. Examples include chlorhexidine and povidone iodine. "Disinfectants" operate only on nonliving objects, but are otherwise similar to antiseptics.

[00020] In particular embodiments of the present invention, the composition that is contacted with the non-organic surface includes a basic reagent, a dye, or a basic reagent in combination with a dye. The composition may include a single dye or a combination of dyes. The composition may include a single basic reagent, or a combination of basic reagents. In

particular embodiments, the dye and/or basic reagent has antimicrobial activity. In some  
embodiments, the dye is bonded to the basic reagent to form a compound that has  
antimicrobial activity. Non-limiting examples of basic reagents contemplated by the present  
invention include a guanidium compound, a biguanide, a bipyridine, a phenoxide antiseptic,  
5 an alkyl oxide, an aryl oxide, a thiol, a halide, an aliphatic amine, or an aromatic amine. In  
particular embodiments, the basic reagent is a guanidium compound. For example, the  
guanidium compound may be chlorhexidine, alexidine, or hexamidine. In other  
embodiments, the basic reagent is a bipyridine. For example, the bipyridine may be  
octenidine. In further embodiments, the basic reagent is a phenoxide antiseptic. For example,  
10 the phenoxide antiseptic may be clofoctol, chloroxylonol, or triclosan. One of ordinary skill in  
the art would be familiar with basic reagents that can be included in the context of the present  
invention.

[00021] The dye can be any dye known to those of ordinary skill in the art. Non-limiting  
examples of dyes include a triarylmethane dye, a monoazo dye, a diazo dye, an indigoid dye, a  
15 xanthene dye, an anthraquinone dye, a quinoline dye, an FD&C dye, a D&C dye, or brilliant  
green. For example, the triarylmethane dye may be a dye selected from the group consisting  
of gentian violet, crystal violet, and ethyl violet. Non-limiting examples of FD&C dyes  
include Blue No. 1 and Green No. 3. Non-limiting examples of monoazo dyes include FD&C  
Yellow No. 5 or FD&C Yellow No. 6. A non-limiting example of a diazo dye is D&C Red  
20 No. 17. A non-limiting example of an indigoid dye is FD&C Blue No. 2. A non-limiting  
example of a xanthene dye is FD&C Red No. 3. A non-limiting example of an anthraquinone  
dye is D&C Green No. 6. A non-limiting example of a quinoline dye is D&C Yellow No. 1.

[00022] The basic reagent may be bonded to the dye. The basic reagent and the dye may be  
bonded ionically to form the antiseptic compound. In other embodiments, the basic reagent  
25 and the dye are bonded covalently to form the antiseptic compound. The basic reagent and  
the dye can be combined in any amount to obtain the antiseptic composition of the invention,  
however, in a particular embodiment, an equimolar amount of the basic reagent is added to  
the dye solution. The inventors also contemplate that the antiseptic composition of the  
invention can be made by combining other amounts of the dye and basic reagent for example,  
30 one may combine, in molar ratios, 1:1, 1:2, 1:3, 1:4, 1:5, 1:6, 1:7, 1:8, 1:9, 1:10, 1:15, 1:20,  
1:25, 1:30, 1:35, 1:40, 1:45, 1:50, 1:55, 1:60, 1:65, 1:70, 1:75, 1:80, 1.85, 1:90, 1:95, to 1:99  
of either dye : basic reagent or basic reagent : dye. This includes all the intermediate ranges  
as well, for example it includes molar ratios such as, 1.1:1, 1.2:1, 1.3:1, 1.4:1, 1.5:1, 1.6:1,

1.7:1, 1.8:1, 1.9:1 and the like for other values listed. It also includes the ranges in between these values such as 1.11:1, 1.12:1 and so on. The skilled artisan will therefore recognize that the dye and basic reagent can be combined in different molar ratio amounts to obtain the antiseptic composition disclosed and that the invention is therefore not limited to any particular molar ratio of dye : basic reagent or basic reagent : dye.

[00023] A "solvent" as used herein refers to a compound or molecule that exists as a liquid at a temperature of about 20°C to about 60°C. In some embodiments, the solvent has a boiling point of over 35°C. Non-limiting examples of solvent as used herein may be an aqueous solvent or a nonaqueous solvent. In particular embodiments, the solvent is inert in that it has no ability to alter or modify the chemical structure of the antimicrobial agent. Nonlimiting examples of solvents include water, methylene chloride, alcohols (such as methanol and ethanol), ketones (such as acetone, methylethylketone), esters (such as tetrahydrofuran), aldehydes (such as formaldehyde), acetonitrile, acetic acid, methylene chloride, chloroform, butyl acetate, or a combination thereof. In some embodiments, the solvent is a dipolar aprotic solvent, such as dimethylsulfoxide or N,N-dimethylformamide. The solvent may also be a protic solvent or an aprotic solvent. Additional examples of solvents are set forth in the specification below.

[00024] The surface may be a smooth surface or an irregular surface. In some particular embodiments, the surface comprises one or more pores. The pores can be of any size. For example, the pore may be a micropore (a pore with a diameter of about 100 nm to about 100 μm) or a nanopore (a pore with a diameter in the range of from about 1 nm to about 100 nm in a membrane or solid media).

[00025] The surface can be composed of any material known to those of ordinary skill in the art. For example, the surface may be composed of a polymer, silicone, or a mixture thereof. Any polymer known to those of ordinary skill in the art is contemplated by the present invention. Examples include polyvinyl chloride, polyurethane, polyethylene, silastic elastomers, polytetrafluoroethylene, dacron, collodion, carboethane and nylon.

[00026] "Curing" in the context of the present invention is defined herein to refer to heating the surface such that some or all of the solvent that was contacted with the surface is removed from the surface. "Heating" as used herein refers to an increase in temperature of the surface due to application of a heat source compared to temperature of the surface in the absence of



the heat source. Heating can be by any method known to those of ordinary skill in the art. Heat sources that may be used with the methods set forth herein include but are not limited to a heat lamp, heating incubator, heat from an electrical source, infrared radiation, visible light, ultraviolet radiation, inductive heating, laser illumination, high-frequency ultrasound or combinations thereof.

[00027] Curing can comprising heating the surface to a temperature that is at least about 30°C, 36°C, 37°C, 38°C, 39°C, 40°C, 41°C, 42°C, 43°C, 44°C, 45°C, 46°C, 47°C, 48°C, 49°C, 50°C, 51°C, 52°C, 53°C, 54°C, 55°C, 56°C, 57°C, 58°C, 59°C, 60°C, 61°C, 62°C, 63°C, 64°C, 65°C, 66°C, 67°C, 68°C, 69°C, 70°C, 71°C, 72°C, 73°C, 74°C, 75°C, 76°C, 77°C, 78°C, 79°C, 80°C, 81°C, 82°C, 83°C, 84°C, 85°C, 86°C, 87°C, 88°C, 89°C, 90°C, 91°C, 92°C, 93°C, 94°C, 95°C, 96°C, 97°C, 98°C, 99°C, 100°C, 105°C, 110°C, 115°C, 120°C, or greater, or to at least any intermediate temperature between one of the specifically recited temperatures, or within any range of temperature. For example, the surface may be heated to about 40 to about 100°C. In further embodiments, curing involves heating the surface to a temperature that is about 40°C to about 80°C. In still further embodiments, curing involves heating the surface to a temperature that is about 40°C to about 60°C.

[00028] In certain particular embodiments, curing occurs at a temperature of from about 30°C to about 220°C, at a temperature of from about 40°C to about 100°C, at a temperature of from about 45°C to about 100°C, at a temperature of from about 45°C to about 90°C, at a temperature of from about 45°C to about 80°C, 45°C to about 70°C, or at a temperature of from about 50°C to about 60°C.

[00029] The heating may occur before, after or during the time that the medical device is contacted with an antibiotic or an antiseptic. The heating may result in the fixation of the antiseptic agent or the antibiotic to the medical device. In certain embodiments, the heating may affect nanopores or micropores which exist on the medical device (*e.g.*, the heating may enlarge and/or improve the ability of the micropore or nanopore to contain or adhere an antiseptic or antibiotic). The heating may occur once or more than once. In certain embodiments the medical device may be heated 1, 2, 3, 4, 5 or more times.

[00030] The surface can be heated for any duration of time. For example, the surface may be heated to remove some but not all of the solvent that was contacted with the surface.

Alternatively the surface can be heated until the surface is dry. For example, the surface may be heated for at least 5 minutes, 10 minutes, 15 minutes, 20 minutes 25 minutes 30 minutes 35 minutes 40 minutes 45 minutes, 50 minutes, 55 minutes, 1 hour, 1.25 hour, 1.5 hour, 1.75 hour, 2.0 hours 2.25 hours, 2.5 hours, 2.75 hours, 3.0 hours, 3.25 hours, 3.5 hours, 3.75 hours, 5 4.0 hours, 4.5 hours, 5.0 hours, 5.5 hours, 6.0 hours, 6.5 hours, 7.0 hours, 7.5 hours. 8.0 hours, 8.5 hours, 9.0 hours, 9.5 hours, 10.0 hours. 15 hours, 24 hours, 36 hours, 48 hours, 60 hours, 72 hours, 84 hours, 2 weeks, 2.5 weeks, 3 weeks, 1 month, or longer, or for at least any duration in between one of the specifically recited durations, or within any range of durations set forth herein. In further embodiments, the surface is further heated after the surface is dry. 10 In some embodiments, the surface is heated for about 1 hour to about 3 weeks. In further embodiments, the surface is heated for about 12 hours to about 96 hours. In still further embodiments, the surface is heated for about 24 hours to about 72 hours.

[00031] In particular embodiments set forth herein, the surface is washed after it is cured. Washing is defined herein to refer to application of a liquid for the purpose of removing a 15 substance. For example, washing may be further defined as contacting the surface with a composition comprising a detergent and water. The contacting may result in removal of antimicrobial agent not bound to the surface of the medical device. Any method known to those of ordinary skill in the art can be applied in washing the medical device. Washing can, for example, include rinsing, dipping, or immersing the device in a wash solution using any 20 method known to those of ordinary skill in the art.

[00032] In further embodiments, the method further involves curing the surface at a temperature of at least 40°C after washing the surface. The surface may be cured as discussed above. For example, the surface may be cured for at least 1 hour to at least 96 hours or for at least 24 hours to at least 72 hours.

25 [00033] When the surface is the surface of a medical device, the method may further involve packing the medical device in a container. The container can be any container known to those of ordinary skill in the art that can be applied in packing the device for shipping to a site where the device will be used. In some embodiments, the method further involves sterilizing the medical device. Any method known to those of ordinary skill in the art can be used to 30 sterilize the medical device. For example, the medical device may be sterilized after it is heated using any method known to those of ordinary skill in the art. Examples of such

methods of sterilization include heat sterilization, radiation sterilization, including gamma irradiation, chemical sterilization, or gas sterilization.

[00034] In a particular embodiments, the method is a method for coating or impregnating a medical device with an antimicrobial composition, involving the steps of: (1) contacting the medical device with a composition comprising an antimicrobial agent and a solvent; (2) curing the medical device at a temperature of about 40°C to about 80°C for about 12 hours to about 72 hours, wherein the medical device is dried; (3) washing the medical device with an aqueous composition; and (4) repeating step (2), wherein the medical device becomes coated or impregnated with an antimicrobial composition.

[00035] Additional information regarding contacting an antimicrobial agent with a medical device can be found in U.S. Patent 5,624,704, herein specifically incorporated by reference in its entirety. Additional information regarding antiseptic compositions for coating medical devices can be found in U.S. Patent App. Pub. Nos. 20050197634 and 20030078242, herein specifically incorporated by reference in their entirety.

[00036] The present invention is also generally directed to a medical device, personal product, or health care product coated with an antimicrobial agent using any of the methods set forth above. The medical device, personal product, food processing supply, or health care product can be any of those items set forth above. The antimicrobial agent can be any of those agents set forth above and elsewhere in this specification.

[00037] The present invention also generally pertains to a method for reducing the risk of development or progression of an infection in a subject in need of a medical device, involving coating or impregnating a surface of the medical device with an antimicrobial agent in accordance with the method of claim 1 prior to contacting the medical device with the subject, wherein the risk of development or progression of an infection is reduced. The subject can be any subject, such as a vertebrate. For example, the subject may be a mammal. In particular embodiments, the mammal is a human. For example, the human may be a subject in need of a medical device.

[00038] The antimicrobial agent can be any of those agents discussed above and elsewhere in this specification. As discussed above, the antimicrobial agent may be an antibiotic, an antiseptic, an antiviral agent, an antifungal agent, or a disinfectant. In particular embodiments, the antibiotic is a tetracycline, a macrocyclic antibiotic compound, or a

combination thereof. For example, the tetracycline may be minocycline. The macrocyclic antibiotic may be a macrocyclic antibiotic such as rifampim, rifampicin, or a combination thereof.

5 [00039] The infection can be any type of infection. Non-limiting examples of types of infection include pneumonia, bacteremia, fungimia, candidemia, a urinary tract infection, a catheter-exit site infection, or a surgical wound infection. In particular embodiments, the infection is a nosocomial infection. For example, the infection may be an infection caused by methicillin-resistant staphylococci, vancomycin-resistant enterococci, resistant *Pseudomonas aeruginosa*, or a combination thereof. In some embodiments, the infection is a fungal  
10 infection. For example, the fungal infection may be an infection secondary to a *Candida species*.

[00040] In some embodiments, the medical device has been contacted with a composition comprising a basic reagent and a dye. The basic reagent can be any of those reagents discussed above and elsewhere in this specification. The dye can be any of those reagents  
15 discussed above and elsewhere in this specification. In particular embodiments, the dye is gentian violet, and the basic reagent is chlorhexidine, clofoctol, chloroxylenol, or triclosan. Throughout this application, the term “gendine” refers to a composition comprising chlorhexidine and gentian violet, the term “genlosan” refers to a composition comprising gentian violet and triclosan, the term “genfoctol” refers to a composition comprising gentian  
20 violet and clofoctol, and the term “genlenol” refers to a composition comprising gentian violet and chloroxylenol.

[00041] The medical device can be any medical device known to those of ordinary skill in the art, including any of those examples discussed above. Non-limiting examples include an endotracheal tube, a vascular catheter, an urinary catheter, a nephrostomy tube, a biliary stent, a  
25 peritoneal catheter, an epidural catheter, a central nervous system catheter, an orthopedic device, a prosthetic valve, a silk suture, or a medical implant. In particular embodiments, the medical device is a vascular catheter further defined as a central venous catheter, an arterial line, an pulmonary artery catheter, or a peripheral venous catheter. In further embodiments, the medical device is a central nervous system catheter, such as an intraventricular shunt.

30 [00042] An aspect of the present invention relates to a method for coating a medical device with an antimicrobial composition comprising: contacting said medical device with a solvent

comprising the antimicrobial composition, drying the medical device and heating the medical device, wherein if the antimicrobial composition does not comprise a basic reagent and a dye, then the medical device is heated for at least about 12 hours. The antimicrobial composition may be minocycline or rifampin.

5 [00043] In certain embodiments, the antimicrobial composition is an antiseptic composition. The antiseptic may comprise a basic reagent and a dye. The solvent may comprise water, methylene chloride, alcohols (such as methanol and ethanol), ketones (such as acetone, methylethylketone), esters (such as tetrahydrofuran), aldehydes (such as formaldehyde),  
10 acetonitrile, acetic acid, methylene chloride, chloroform, butyl acetate, or a combination thereof. The medical device may be heated before, after or during contacting the medical device with the solvent. In certain embodiments, the medical device comprises a micropore or a nanopore. In certain embodiments, the medical device is heated both before and after contacting the medical device with the solvent.

[00044] The composition may include additional agents, such as penetrating agents (i.e. agents used to promote impregnation of the antimicrobial agent through the surface. Examples include esters (e.g., ethyl acetate, propyl acetate, butyl acetate, amyl acetate, and combinations therefore), ketones, methylene chloride, and chloroform. The composition may also include one or more alkalizing agents (such as an organic or inorganic base such as sodium hydroxide, potassium hydroxide, ammonia, diethylamine, triethylamine), and one or  
15 more high ionic strength salts, such as sodium chloride, potassium chloride, or ammonium acetate.  
20

[00045] The medical device may be heated to from about 40°C to about 100°C, more preferably from about 50°C to about 80°C. In certain embodiments, the medical device is heated to about 60°C. The medical device is heated for a period of at least 30 minutes. In  
25 certain embodiments, the medical device is heated for a period of time from about 12 hours to about 96 hours, more preferably from about 24 hours to about 96 hours.

[00046] In certain embodiments, the method further comprises washing the medical device. The washing may be used to remove excessive antiseptic composition. In certain embodiments, the medical device is washed with a mild detergent and de-ionized water.

30 [00047] As used herein the specification and claim(s), the words "a" or "an" when used in conjunction with the word "comprising" may mean one or more.

[00048] Throughout this application, the term "about" is used to indicate that a value includes the inherent variation of error for the device, the method being employed to determine the value, or the variation that exists among the study subjects.

[00049] The use of the term "or" in the claims is used to mean "and/or " unless explicitly indicated to refer to alternatives only or the alternatives are mutually exclusive, although the disclosure supports a definition that refers to only alternatives and "and/or."

[00050] As used herein the specification and claim(s), the words "ionic bonding" or "ionically bound" refers to the electrostatic interactions among ions which can be formed by the transfer of one or more electrons from one atom or group of atoms to another, to create an ionic bond between the basic reagent and the dye comprising an antiseptic compound.

[00051] As used herein the specification and claim(s), the words "covalent bonding" or "covalently bound" refers to the chemical bond formed by the sharing of one or more pairs of electrons between the basic reagent and the dye comprising an antiseptic compound.

[00052] Other objects, features and advantages of the present invention will become apparent from the following detailed description. It should be understood, however, that the detailed description and the specific examples, while indicating preferred embodiments of the invention, are given by way of illustration only, since various changes and modifications within the spirit and scope of the invention will become apparent to those skilled in the art from this detailed description.

#### **BRIEF DESCRIPTION OF THE DRAWINGS**

[00053] The following drawings form part of the present specification and are included to further demonstrate certain aspects of the present invention. The invention may be better understood by reference to one or more of these drawings in combination with the detailed description of specific embodiments presented herein.

[00054] **FIG. 1:** Heating reduces Gendine leaching.

[00055] **FIG. 2:** Heating reduces bacteria (*Pseudomonas aeruginosa*) adherence.

[00056] **FIG. 3:** Zones of inhibitions formed by Gendine coated PVC endotracheal tubes in methicillin resistant *Staphylococcus aureus*.

- [00057] FIG. 4: Effects of heating on the leaching of Gendine from coated polyurethane CVC.
- [00058] FIG. 5: Adherence of bacteria to polyurethane CVC surfaces.
- [00059] FIG. 6: Zones of inhibitions formed by Gendine coated cook polyurethane catheters  
5 in methicillin resistant *Staphylococcus aureus*.
- [00060] FIG. 7: Zones of inhibitions formed by Gendine coated cook polyurethane catheters  
in *Pseudomonas aeruginosa*.
- [00061] FIG. 8: Zones of inhibitions formed by Gendine coated cook polyurethane catheters  
*Candida parapsilosis*.
- 10 [00062] FIG. 9: Effects of heating on the leaching of Gendine from coated cook silicone  
urinary catheters.
- [00063] FIG. 10: Adherence of bacteria to silicone urinary catheter surfaces.
- [00064] FIG. 11: Zones of inhibitions formed by Gendine coated cook silicone urinary  
catheters in vancomycin resistant *Enterococcus* (VRE).
- 15 [00065] FIG. 12: Zones of inhibitions formed by Gendine coated cook silicone urinary  
catheters in *E. coli*.
- [00066] FIG. 13: Zones of inhibitions formed by Gendine coated cook silicone urinary  
catheters in *Candida parapsilosis*.
- [00067] FIG. 14. Durability of Spectrum (unheated Mino-Rifampin catheters) compared to  
20 heated mino-rifampin catheters over 12 weeks – tested against MRSA 4798.
- [00068] FIG. 15. Durability of Spectrum compared to heated Mino-Rifampin catheters over  
12 weeks – tested against *S. malto* 5075.
- [00069] FIG. 16. Durability of Spectrum compared to heated Mino-Rifampin catheters over  
12 weeks – tested against *S. malto* 4807.
- 25 [00070] FIG. 17. Durability of Spectrum compared to heated Mino-Rifampin catheters over  
12 weeks – tested against *S. malto* 4709.

[00071] FIG. 18. Adherent of biofilm to coated polymers.

### DESCRIPTION OF ILLUSTRATIVE EMBODIMENTS

[00072] The present invention provides for novel methods of coating or impregnating a surface with an antimicrobial agent. By way of example, the inventors have found that coating a medical device with a composition that includes an antimicrobial agent and a solvent following by curing the medical device at a temperature of greater than 40°C results in a decrease in staining potential of the medical device, decrease in leaching of the antimicrobial into tissue, and prolonged antimicrobial efficacy. Medical devices, such as indwelling catheters, are used routinely in hospitals on a diverse group of patients. A common cause of failure of these medical devices is infection. Pathogens often attach to and proliferate in such devices and eventually invade the patient leading to nosocomial infections. Microorganisms usually migrate along the surfaces of devices to invade sterile environments, such as the bronchoalveolar space leading to pneumonia, the bloodstream leading to bacteremia, or the urinary bladder leading to urinary tract infections.

[00073] For example, in certain embodiments, the present invention relates to the use of antiseptic compositions with broad-spectrum activity against various nosocomial microorganisms, including resistant bacteria and fungi. For example, the antiseptic compositions are effective against resistant staphylococci, vancomycin-resistant enterococci, resistant *Pseudomonas aeruginosa* and *Candida* species. These antiseptics also have unique properties that enable penetration/impregnation of various polymers, such as polyvinyl chloride, polyethylene, silastic elastomers, polytetrafluoroethylene, dacron, collodion, carboethane, nylon, polymers used in the formation of endotracheal tubes, silicone and polyurethane polymers used in the formation of vascular catheters and surgical silk sutures. Thus, they are suitable for coating a wide range of device surfaces.

[00074] The present invention provides safe antimicrobial-treated surfaces wherein the coated or impregnated surface has a durability that may last through the life-span of the device. For example, with regard to medical devices, this significantly decreases patient mortality and morbidity associated with the various nosocomial infections such as nosocomial pneumonias, nosocomial bacteremias, nosocomial urinary tract infections and nosocomial surgical wound infections.



## A. Antimicrobial Agents

[00075] For the purposes of this disclosure, the phrase “effective amount” or “therapeutically effective amount” is defined as a dosage sufficient to induce a microbicidal or microbistatic effect upon the microbes contacted by the composition on a surface.

5 [00076] In some embodiments of the invention, the antimicrobial agent is an antibacterial agent. While any antibacterial agent may be used in the preparation of the instant antimicrobial solutions, some non-limiting exemplary antibacterial agent(s) include those classified as aminoglycosides, beta lactams, quinolones or fluoroquinolones, macrolides, sulfonamides, sulfamethoxozoles, tetracyclines, streptogramins, oxazolidinones (such as  
10 linezolid), clindamycins, lincomycins, rifamycins, glycopeptides, polymyxins, lipo-peptide antibiotics, as well as pharmacologically acceptable sodium salts, pharmacologically acceptable calcium salts, pharmacologically acceptable potassium salts, lipid formulations, derivatives and/or analogs of the above.

[00077] Each of these classes of antibacterial agents have different mechanisms of action and  
15 are represented by several antibiotics a discussion of which is presented below. However, the skilled artisan will recognize that the invention is in no way limited to the agents set forth here and that these agents are described merely as examples.

[00078] The aminoglycosides are bactericidal antibiotics that bind to the 30S ribosome and inhibit bacterial protein synthesis. They are typically active against aerobic gram-negative  
20 bacilli and staphylococci. Exemplary aminoglycosides that may be used in some specific aspects of the invention include amikacin, kanamycin, gentamicin, tobramycin, or netilmicin.

[00079] Beta lactams are a class of antibacterials that inhibit bacterial cell wall synthesis. A majority of the clinically useful beta-lactams belong to either the penicillin group (penam) or cephalosporin (cephem) groups. The beta-lactams also include the carbapenems (*e.g.*,  
25 imipenem), and monobactams (*e.g.*, aztreonam). Inhibitors of beta-lactamase such as clavulanic acid and its derivatives are also included in this category.

[00080] Non-limiting examples of the penicillin group of antibiotics that may be used in the solutions of the present invention include amoxicillin, ampicillin, benzathine penicillin G, carbenicillin, cloxacillin, dicloxacillin, piperacillin, or ticarcillin, *etc.* Examples of  
30 cephalosporins include ceftiofur, ceftiofur sodium, cefazolin, cefaclor, ceftibuten,

ceftizoxime, cefoperazone, cefuroxime, cefprozil, ceftazidime, cefotaxime, cefadroxil, cephalixin, cefamandole, cefepime, cefdinir, ceftriaxone, cefixime, cefpodoximeproxetil, cephapirin, cefoxitin, cefotetan *etc.* Other examples of beta lactams include mipenem or meropenem which are extremely active parenteral antibiotics with a spectrum against almost  
5 all gram-positive and gram-negative organisms, both aerobic and anaerobic and to which *Enterococci*, *B. fragilis*, and *P. aeruginosa* are particularly susceptible.

[00081] Examples of beta lactamase inhibitors include clavulanate, sulbactam, or tazobactam. In some aspects of the present invention, the antibacterial solutions may comprise a combination of at least one beta lactam and at least one beta lactamase inhibitor.

10 [00082] Macrolide antibiotics are another class of bacteriostatic agents that bind to the 50S subunit of ribosomes and inhibit bacterial protein synthesis. These drugs are active against aerobic and anaerobic gram-positive cocci, with the exception of enterococci, and against gram-negative anaerobes. Exemplary macrolides include erythromycin, azithromycin, clarithromycin.

15 [00083] Quinolones and fluoroquinolones typically function by their ability to inhibit the activity of DNA gyrase. Examples include nalidixic acid, cinoxacin, trovafloxacin, ofloxacin, levofloxacin, grepafloxacin, trovafloxacin, sparfloxacin, norfloxacin, ciprofloxacin, moxifloxacin and gatifloxacin.

20 [00084] Sulphonamides are synthetic bacteriostatic antibiotics with a wide spectrum against most gram-positive and many gram-negative organisms. These drugs inhibit multiplication of bacteria by acting as competitive inhibitors of *p*-aminobenzoic acid in the folic acid metabolism cycle. Examples include mafenide, sulfisoxazole, sulfamethoxazole, and sulfadiazine.

25 [00085] The tetracycline group of antibiotics include tetracycline derivatives such as tigecycline which is an investigational new drug (IND), minocycline, doxycycline or demeclocycline and analogs such as anhydrotetracycline, chlorotetracycline, or epioxycycline. The present inventors have previously shown that minocycline has a higher penetration of the microbial biofilm layer than vancomycin and that EDTA is unique in effectively preventing and dissolving polysaccharide-rich microbial glycocalyx (U.S. Patent  
30 5,362,754).

[00086] The streptogramin class of antibacterial agents is exemplified by quinupristin, dalfopristin or the combination of two streptogramins.

[00087] Drugs of the rifamycin class typically inhibit DNA-dependent RNA polymerase, leading to suppression of RNA synthesis and have a very broad spectrum of activity against most gram-positive and gram-negative bacteria including *Pseudomonas aeruginosa* and *Mycobacterium* species. An exemplary rifamycin is rifampicin.

[00088] Other antibacterial drugs are glycopeptides such as vancomycin, teicoplanin and derivatives thereof. Yet other antibacterial drugs are the polymyxins which are exemplified by colistin.

[00089] In addition to these several other antibacterial agents such as prestinomycin, chloramphenicol, trimethoprim, fusidic acid, metronidazole, bacitracin, spectinomycin, nitrofurantoin, daptomycin or other leptoepptides, oritavancin, dalbavancin, ramoplanin, ketolide *etc.* may be used in preparing the compositions described herein. Of these, metronidazole is active only against protozoa, such as *Giardia lamblia*, *Entamoeba histolytica* and *Trichomonas vaginalis*, and strictly anaerobic bacteria. Spectinomycin, is a bacteriostatic antibiotic that binds to the 30S subunit of the ribosome, thus inhibiting bacterial protein synthesis and nitrofurantoin is used orally for the treatment or prophylaxis of UTI as it is active against *Escherichia coli*, *Klebsiella-Enterobacter* species, staphylococci, and enterococci.

[00090] In other embodiments, the antimicrobial agent is an antifungal agent. Some exemplary classes of antifungal agents include imidazoles or triazoles such as clotrimazole, miconazole, ketoconazole, econazole, butoconazole, omoconazole, oxiconazole, terconazole, itraconazole, fluconazole, voriconazole (UK 109,496), posaconazole, ravuconazole or flutrimazole; the polyene antifungals such as amphotericin B, liposomal amphoterecin B, natamycin, nystatin and nystatin lipid formulations; the cell wall active cyclic lipopeptide antifungals, including the echinocandins such as caspofungin, micafungin, anidulfungin, cilofungin; LY121019; LY303366; the allylamine group of antifungals such as terbinafine. Yet other non-limiting examples of antifungal agents include naftifine, tolnaftate, mediocidin, candicidin, trichomycin, hamycin, aurefungin, ascosin, ayfattin, azacolutin, trichomycin, levorin, heptamycin, candimycin, griseofulvin, BF-796, MTCH 24, BTG-137586, pradimicins (MNS 18184), benanomycin; ambisome; nikkomycin Z; flucytosine, or perimycin.

[00091] In still other embodiments of the invention, the antimicrobial agent is an antiviral agent. Non-limiting examples of antiviral agents include cidofovir, amantadine, rimantadine, acyclovir, gancyclovir, pencyclovir, famciclovir, foscarnet, ribavirin, or valcyclovir. In some  
 5 embodiments the antimicrobial agent is an innate immune peptide or proteins. Some exemplary classes of innate peptides or proteins are transferrins, lactoferrins, defensins, phospholipases, lysozyme, cathelicidins, serprocidins, bacteriocidal permeability increasing proteins, amphipathic alpha helical peptides, and other synthetic antimicrobial proteins.

[00092] In other embodiments of the invention, the antimicrobial agent is an antiseptic agent. Several antiseptic agents are known in the art and these include a taurinamide derivative, a  
 10 phenol, a quaternary ammonium surfactant, a chlorine-containing agent, a quinaldinium, a lactone, a dye, a thiosemicarbazone, a quinone, a carbamate, urea, salicylamide, carbanilide, a guanide, an amidine, an imidazoline biocide, acetic acid, benzoic acid, sorbic acid, propionic acid, boric acid, dehydroacetic acid, sulfurous acid, vanillic acid, esters of p-hydroxybenzoic acid, isopropanol, propylene glycol, benzyl alcohol, chlorobutanol, phenylethyl alcohol, 2-  
 15 bromo-2-nitropropan-1,3-diol, formaldehyde, glutaraldehyde, calcium hypochlorite, potassium hypochlorite, sodium hypochlorite, iodine (in various solvents), povidone-iodine, hexamethylenetetramine, noxythiolin, 1-(3-chloroallyl)-3,5,7-triazo 1-azoniaadamantane chloride, taurolidine, taurultam, N(5-nitro-2-furfurylidene)-1-amino-hydantoin, 5-nitro-2-furaldehyde semicarbazone, 3,4,4'-trichlorocarbanilide, 3,4',5-tribromosalicylanilide, 3-  
 20 trifluoromethyl-4,4'-dichlorocarbanilide, 8-hydroxyquinoline, 1-cyclopropyl-6-fluoro-1,4-dihydro-4-oxo-7-(1-piperaziny)-3-quinolinecarboxylic acid, 1,4-dihydro-1-ethyl-6-fluoro-4-oxo-7-(1-piperaziny)-3-quinolinecarboxylic acid, hydrogen peroxide, peracetic acid, phenol, sodium oxychlorosene, parachlorometaxylenol, 2,4,4'-trichloro-2'-hydroxydiphenol, thymol, chlorhexidine, benzalkonium chloride, cetylpyridinium chloride, silver sulfadiazine, or silver  
 25 nitrate.

## B. Solvents

[00093] Non-limiting examples of solvents are set forth in Table 1.

**Table 1. Examples of Solvents**

Name	Structure
water	H-OH
methanol	CH <sub>3</sub> -OH

Name	Structure
ethanol	$\text{CH}_3\text{CH}_2\text{-OH}$
1-propanol	$\text{CH}_3\text{CH}_2\text{CH}_2\text{-OH}$
1-butanol	$\text{CH}_3\text{CH}_2\text{CH}_2\text{CH}_2\text{-OH}$
formic acid	
acetic acid	
formamide	
....	....
acetone	
tetrahydrofuran (THF)	
methyl ethyl ketone	
ethyl acetate	
acetonitrile	$\text{H}_3\text{C-C}\equiv\text{N}$
N,N-dimethylformamide (DMF)	
diethyl sulfoxide (DMSO)	
....	....
hexane	$\text{CH}_3(\text{CH}_2)_4\text{CH}_3$
benzene	
diethyl ether	$\text{CH}_3\text{CH}_2\text{OCH}_2\text{CH}_3$
methylene chloride	$\text{CH}_2\text{Cl}_2$
carbon tetrachloride	$\text{CCl}_4$

### C. Dyes

[00094] In some embodiments of the present invention, the surface is contacted with a composition that includes a dye. A "dye" is defined herein to refer to an agent that is used to impart color. The dye may or may not have antimicrobial activity. In some embodiments, the composition includes a dye and a basic reagent. The dye may or may not be bonded to the basic reagent. The dye may be ionically or covalently bonded to the basic reagent. The dye bonded to the basic reagent may or may not have antimicrobial activity

[00095] The dye may be obtained from any source known to those of ordinary skill in the art. The dye may be obtained, for example, from natural sources, from commercial sources, or may be chemically synthesized.

[00096] The dyes that may be used to synthesize certain antiseptic compounds of the invention include but are not limited to, gentian, or crystal violet, ethyl violet, brilliant green, *etc.*, and the FD&C dyes such as Blue No. 1 and Green No. 3. In addition, other dyes include the following FD&C and D&C colors: (1) monoazo dyes such as, but not limited to, FD&C Yellow No. 5, FD&C Yellow No. 6, (2) diazo dyes such as, but not limited to, D&C Red No. 17, (3) indigoid dyes such as, but not limited to, FD&C Blue No. 2, (4) xanthene (Fluorescein) dyes such as, but not limited to, FD&C Red No. 3, (5) anthraquinone dyes such as, but not limited to, D&C Green No. 6, (6) quinoline dyes such as, but not limited to, D&C Yellow No. 1. An extensive list of dyes and stains that may be employed is also provided in Table 1.

**Table 1.** The Color Index (C.I.) Number and/or Chemical Abstracts Service Registry (CAS) Number for Selected Dyes and Stains:

No.	C.I. #	CAS #	No.	C.I. #	CAS #
1	15670	2092-55-9	51	65005	1328-24-1
2	26370	3071-73-6	52	62055	6408-78-2
3	20460	5850-35-1	53	62125	6424-85-7
4	62130	2666-17-3	54	63010	2861-02-1
5	61585	4474-24-2	55	13390	3861-73-2
6	26360	3351-05-1	56	26400	3529-01-9
7	62058	6397-02-0	57	15706	12392-64-2
8	42685	3244-88-0	58	61570	4403-90-1
9	61580	6408-57-7	59	62560	4430-16-4
10	15575	5850-86-2	60	26550	8003-88-1
11	22870	15792-50-4	61	18745	10127-27-2
12	18050	3734-67-6	62	14710	5858-39-9
13	14900	4787-93-3	63	17045	6360-07-2
14	18070	12167-45-2	64	15620	1658-56-6
15	22890	10169-02-5	65	18110	6844-74-2
16	23635	6459-94-5	66	26900	6406-56-0

No.	C.I. #	CAS #	No.	C.I. #	CAS #
17	18800	6408-31-7	67	18125	10130-48-0
18	18055	4321-69-1	68	42650	4129-84-4
19	18965	6359-98-4	69	18835	6359-85-9
20	18900	6359-91-7	70	18890	6359-90-6
21	25135	13390-47-1	71	18950	6372-96-9
22	22910	6375-5-9	72	14170	6408-90-8
23	18850	6359-88-2	73	13900	10343-58-5
24	46005:1	494-38-2	74	46025	135-49-9
25		8048-52-0	75	12840	61968-76-1
26	58000	72-48-0	76	63615	1324-21-6
27		3952-78-1	77	58005	130-22-3
28	61710	6408-63-5	78	14025	584-42-9
29	42750	30586-13-1	79	42080	3486-30-4
30		569-58-4	80	16185	915-67-3
31		52417-22-8	81	42780	
32		520-10-5	82		1668-00-4
33	48035	3056-93-7	83	41000	2465-27-2
34		4431-00-9	84	43810	13186-45-3
35	50090	25360-72-9	85	52005	531-53-3
36	52010	531-55-5	86	51004	33203-82-6
37	61111	12217-43-5	87	11075	94233-04-2
38	42500	569-61-9	88	42510	632-99-5
39	11460	42373-04-6	89	48055	4208-80-4
40	23500	992-59-6	90	26905	4196-99-0
41		298-95-3	91		2315-97-1
42	21010	5421-66-9	92	21000	10114-58-6
43		1871-22-3	93	16180	5858-33-3
44	28440	2519-30-4	94	42655	6104-58-1
45	42660	6104-59-2	95		81029-05-2
46	27290	5413-75-2	96	42040	633-03-4
47	24890	3051-11-4	97		102185-52-4
48		76-60-8	98		62625-32-5
49		115-40-2	99		62625-30-3
50		115-39-9	100		62625-28-9
101		14337-53-2	152		16574-43-9
102		76-59-5	153		34722-90-2
103		40070-59-5	154		617-19-6
104		3147-14-6	155	51050	1562-90-9
105	24410	2610-05-1	156		4430-20-0
106	43825	1667-99-8	157	14720	3567-69-9
107	16575	548-80-1	158	16570	4197-07-3
108	43820	3564-18-9	159	11270	532-82-1
109	24895	2870-32-8	160	18105	17681-50-4
110	18972	50662-99-2	161	22120	573-58-0
111		596-27-0	162		2411-89-4
112		2303-01-7	163		62625-31-4
113		1733-12-6	164		62625-29-0
114		10510-54-0	165		41830-80-2
115	15970	1934-20-9	166	42555	548-62-9
116		15391-59-0	167	45370:1	596-03-2
117		76-54-0	168		620-45-1
118		4727-50-8	169	45425:1	31395-16-1
119		54-88-6	170		73688-85-4
120		6473-13-8	171	34140	4399-55-7
121	23655	6420-03-7	172	29160	3441-14-3
122	25380	2829-43-8	173	28160	2610-11-9
123	27905	5489-77-0	174	13920	10130-29-7

No.	C.I. #	CAS #	No.	C.I. #	CAS #
124	13950	10190-68-8	175	19556	6537-66-2
125	29025	3214-47-9	176	36900	6409-90-1
126	64500	2475-45-8	177	61505	2475-46-9
127	61500	2475-44-7	178	11080	2581-69-3
128	1005	730-40-5	179	26080	6253-10-7
129		31482-56-1	180	11110	2872-52-8
130	11115	3180-81-2	181	11130	2734-52-3
131	11855	2832-40-8	182	12790	6439-53-8
132	26090	6300-37-4	183		518-82-1
133	45400	548-24-3	184		56360-46-4
134	45380	548-26-5	185	45380:2	15086-94-9
135		15086-94-9	186	14645	1787-61-7
136	14640	3564-14-5	187	18760	3618-63-1
137	42090	3844-45-9	188	45430	568-63-8
138	45430:2	15905-32-5	189		1239-45-8
139	45386	6359-05-3	190		62758-12-7
140		76058-33-8	191	42600	2390-59-2
141	23860	314-13-6	192	37190	64071-86-9
142	11160	97-56-3	193	42053	2353-45-9
143	13015	2706-28-7	194	12010	6535-42-8
144	11285	6416-57-5	195	18820	6359-82-6
145	45350:1	2321-07-5	196	45350	518-47-8
146		596-09-8	197		3326-32-7
147		3326-34-9	198		51649-83-3
148	51030	1562-85-2	199	42085	4680-78-8
149		1634-82-8	200	75290	517-28-2
150		3737-95-9	201		90-33-5
151		165660-27-5	202	73000	482-89-3
203	73015	860-22-0	254		3599-32-4
204	12210	4569-88-4	255		146-68-9
205	11050	2869-83-2	256	42095	5141-20-8
206	44090	3087-16-9	257	42000:1	510-13-4
207	42000	2437-29-8	258		129-16-8
208	13065	587-98-4	259	52015	61-73-4
209	52041	2516-05-4	260	50206	4569-86-2
210	45385	23391-49-3	261	42590	7114-03-6
211	13025	547-58-0	262	13020	493-52-7
212		32469-43-5	263	11020	60-11-7
213	14855	3624-68-8	264	20110	3564-15-6
214	11335	6247-27-4	265	11875	6247-28-5
215	11880	6370-46-3	266	13250	3618-62-0
216	11300	6232-53-7	267	14030	2243-76-7
217	26520	3564-27-0	268	26560	6406-37-7
218	18735	1934-24-3	269		6408-91-9
219	14010	6054-99-5	270	14045	6470-98-0
220	44530	5715-76-4	271	20470	1064-48-8
221	11350	131-22-6	272	50040	553-24-2
222	16255	2611-82-7	273	42520	3248-91-7
223	52030	6586-05-6	274	51180	3625-57-8
224		7385-67-3	275	14890	5423-07-4
225		74-39-5	276		56431-61-9
226	60760	6409-77-4	277	61555	2646-15-3
227	26120	4477-79-6	278	26125	1320-06-5
228	16230	1936-15-8	279	15510	633-96-5
229	15705	2538-85-4	280	15711	5610-64-0
230	19010	10127-05-6	281	12070	6410-10-2
231	42045	129-17-9	282		143-74-8



No.	C.I. #	CAS #	No.	C.I. #	CAS #
232		34487-61-1	283	11000	60-09-3
233		101-75-7	284		16201-96-0
234	11800	1689-82-3	285		975-17-7
235	45410	18472-87-2	286		2768-90-3
236	16680	1058-92-0	287	27195	6226-79-5
237	27190	6226-78-4	288		67627-18-3
238	49000	30113-37-2	289	58205 (75410)	81-54-9
239		16593-81-0	290		115-41-3
240		85531-30-2	291	45010	2150-48-3
241	45005	92-32-0	292		117-92-0
242	58500	81-61-8	293	58050	81-64-1
243	47000	8003-22-3	294	47005	8004-92-0
244	20505	17095-24-8	295	61211	12236-82-7
245	61205	13324-20-4	296	17757	12225-82-1
246	17908	25489-36-5	297	61200	2580-78-1
247		635-78-9	298		123333-76-6
248	45170	81-88-9	299	45170:1	509-34-2
249	45160	989-38-8	300		13161-28-9
250	45440	632-69-9	301	43800	603-45-2
251	50240	477-73-6	302	61554	17354-14-2
252	61552	6994-46-3	303	61565	128-80-3
253		7423-31-6	304	12055	842-07-9
305	12140	3118-97-6	328	26100	85-86-9
306	26105	85-83-6	329	26150	4197-25-5
307	11920	2051-85-6	330	26050	6368-72-5
308		123359-42-2	331		68504-35-8
309		23647-14-5	332		123333-78-8
310	45100	3520-42-1	333	45220	5873-16-5
311	19140	1934-21-0	334		4430-25-5
312		108321-10-4	335		1301-20-8
313		62637-91-6	336		123333-63-1
314		6262-21-1	337		386-17-4
315		632-73-5	338		4430-24-4
316		42798-98-1	339		1719-71-7
317	19540	1829-00-1	340	49005	2390-54-7
318	52000	78338-22-4	341		76-61-9
319		81012-93-3	342		125-20-2
320		123359-43-3	343	52040	92-31-9
321	12120	2425-85-6	344	14270	547-57-9
322	23850	72-57-1	345		14541-90-3
323	44045	2580-56-5	346	44040	2185-86-6
324	42595	2390-60-5	347	45190	6252-76-2
325		125-31-5	348		63721-83-5
326	16150	3761-53-3	349		14936-97-1
327		135-52-4	350		

#### D. Basic Reagents

[00097] Some embodiments of the present invention involve contacting a surface, such as a medical device, with a composition that includes a basic reagent. Any basic reagent known to those of ordinary skill in the art is contemplated. For example, the basic reagents can be alkyl and aryl oxides, thiols, sulfides, phosphorous, aliphatic and aromatic amines, guanidines and halides such as F<sup>-</sup>, Br<sup>-</sup> and I<sup>-</sup>. Some examples of the basic reagents that can be used include phenoxide antiseptics (such as clofoctol, chloroxylenol, triclosan) or guanidium compounds (such as chlorhexidine, alexidine, hexamidine) or bipyridines (such as octenidines).

[00098] Other examples include a guanidium compound, a biguanide, a bipyridine, a phenoxide antiseptic, an alkyl oxide, an aryl oxide, a thiol, a halide, an aliphatic amine, or an aromatic amine. Non-limiting examples of guanidium compounds include chlorhexidine, alexidine, hexamidine. In other specific embodiments, the basic reagent is a bipyridine. One example of a bipyridine is octenidine. In yet other aspects, the basic reagent is a phenoxide antiseptic.

#### E. Antiseptics

[00099] In some embodiments set forth herein, the antimicrobial is an antiseptic. The composition that includes an antiseptic agent may be applied to the surface by any method known to those of ordinary skill in the art. For example, if the surface is a surface of a medical device, the device may be immersed in the composition, or the composition may be painted or sprayed onto the device. The composition may include a dye, as set forth above. The self-impregnating property of the dyes such as for example, the triarylmethane dyes, removes the need for another binding agent. This is another feature of the composition provided by this invention which is a considerable improvement over certain other known compositions. Certain previously known compositions require other impregnating/coating agents and/or must typically be extruded into the device as it is made. Both these methods are time consuming and involve additional steps and techniques.

[00100] For example, one method of coating devices first requires application or absorption of a layer of surfactant, such as tridodecylmethyl ammonium chloride (TDMAC) followed by the antibiotic coating layer, to the surface of the medical device. Another method used to coat surfaces of medical devices with antibiotics involves first coating the selected surfaces with benzalkonium chloride followed by ionic bonding of the antibiotic composition (Solomon and

Sherertz, 1987; U.S. Patent 4,442,133). Other methods of coating surfaces of medical devices with antibiotics are taught in U.S. Patent 4,895,566 (a medical device substrate carrying a negatively charged group having a pH of less than 6 and a cationic antibiotic bound to the negatively charged group); U.S. Patent 4,917,686 (antibiotics are dissolved in a swelling agent which is absorbed into the matrix of the surface material of the medical device); U.S. Patent 4,107,121 (constructing the medical device with ionogenic hydrogels, which thereafter absorb or ionically bind antibiotics); U.S. Patent 5,013,306 (laminating an antibiotic to a polymeric surface layer of a medical device); and U.S. Patent 4,952,419 (applying a film of silicone oil to the surface of an implant and then contacting the silicone film bearing surface with antibiotic powders). Furthermore, most of the methods previously employed to coat the surfaces of medical devices use antibiotics such as tetracyclines, penicillins, cephalosporins and the beta-lactam antibiotics. The main drawback with antibiotics is the emergence of resistant strains.

[000101] In certain embodiments, antiseptic derivative compounds with broad-spectrum antiseptic activity against bacteria and fungi including nosocomial and multidrug-resistant varieties may be used to impregnate, bind, coat, adhere and/or attach to various device surfaces without the assistance of impregnating vehicles such as tridodecylmethylammonium chloride (TDMAC). Furthermore, antiseptic compounds of the invention also have an extended antimicrobial efficacy that can cover the life of the device.

[000102] One example of the a broad-spectrum antiseptic is a composition that includes a combination of gentian violet and chlorhexidine ("Gendine"). Gentian violet, on its own, is a good impregnating triarylmethane dye. Bhatnager *et al.*, 1993 have shown in an *in vitro* study that gentian violet alone can be used to impregnate the surface of CSF silicone shunts and prevent the colonization of *S. epidermis* on these surfaces. However, after impregnating the surfaces of various polymers, including polyvinylchloride, gentian violet on its own has no activity against *Pseudomonas aeruginosa*, which is the second most common cause of nosocomial pneumonia and the third most common cause of nosocomial urinary tract infections. Antiseptics such as chlorhexidine cannot attach on their own onto the surfaces of polyvinylchloride tubes or silicone catheters and silk sutures. They require an impregnating vehicle. Furthermore, on their own they are not highly active against *Pseudomonas aeruginosa*. On the other hand, upon the binding of gentian violet with chlorhexidine, the new antiseptic agent synthesized, is a potent and effective broad-spectrum antiseptic and has the additional ability to coat/impregnate various device surfaces. Gendine is unique in its

ability to impregnate various device polymers, such as polyvinylchloride used in the formation of endotracheal tubes, silicone and polyurethane polymers used in the formation of vascular, as well as peritoneal, epidural, urinary and intraventricular catheters. In addition, gendine is able to impregnate the silk sutures used in surgical wounds.

- 5 [000103] Compositions with antiseptic properties that are specifically contemplated for use in the invention include, but are not limited to Gendine, Genlenol and Genfoctol.

#### F. Microorganisms

[000104] In some embodiments, the methods set forth herein pertain to methods of reducing the risk of development or progression of an infection in a subject. For example, the subject  
10 may be a subject in need of a medical device. The infection to be prevented may be, for example bacteremia, pneumonia, meningitis, osteomyelitis, endocarditis, sinusitis, arthritis, urinary tract infections, tetanus, gangrene, colitis, acute gastroenteritis, bronchitis, an abscess, an opportunistic infection, or a nosocomial infection. Examples of bacterial pathogens include Gram-positive cocci such as *Staphylococcus aureus*, coagulase negative staphylococci  
15 such as *Staphylococcus epidermis*, *Streptococcus pyogenes* (group A), *Streptococcus spp.* (viridans group), *Streptococcus agalactiae* (group B), *S. bovis*, *Streptococcus* (anaerobic species), *Streptococcus pneumoniae*, and *Enterococcus spp.*; Gram-negative cocci such as *Neisseria gonorrhoeae*, *Neisseria meningitidis*, and *Branhamella catarrhalis*; Gram-positive bacilli such as *Bacillus anthracis*, *Corynebacterium diphtheriae* and *Corynebacterium species*  
20 which are diphtheroids (aerobic and anerobic), *Listeria monocytogenes*, *Clostridium tetani*, *Clostridium difficile*, *Escherichia coli*, *Enterobacter species*, *Proteus mirablis* and other spp., *Pseudomonas aeruginosa*, *Klebsiella pneumoniae*, *Salmonella*, *Shigella*, *Serratia*, and *Campylobacterjejuni*. The antibiotic resistant bacteria that can be killed by the antiseptic coated devices of the present invention include *Staphylococci* (methicillin-resistant strains),  
25 vancomycin-resistant enterococci (*Enterococcus faecium*), and resistant *Pseudomonas aeruginosa*.

[000105] Fungal infections may have cutaneous, subcutaneous, or systemic manifestations. Superficial mycoses include tinea capitis, tinea corporis, tinea pedis, onychomycosis, perionychomycosis, pityriasis versicolor, oral thrush, and other candidoses such as vaginal,  
30 respiratory tract, biliary, eosophageal, and urinary tract candidoses. Systemic mycoses include systemic and mucocutaneous candidosis, cryptococcosis, aspergillosis, mucormycosis

(phycomycosis), paracoccidioidomycosis, North American blastomycosis, histoplasmosis, coccidioidomycosis, and sporotrichosis. Fungal infections include opportunistic fungal infections, particularly in immunocompromised patients such as those with AIDS. Fungal infections contribute to meningitis and pulmonary or respiratory tract diseases.

5 [000106] Other pathogenic organisms include dermatophytes (*Microsporum canis* and other *M. spp.*; and *Trichophyton spp.* such as *T. rubrum*, and *T. mentagrophytes*), yeasts (e.g., *Candida albicans*, *C. Parapsilosis*, *C. glabrata*, *C. Tropicalis*, or other *Candida* species including drug resistant *Candida* species), *Torulopsis glabrata*, *Epidermophyton floccosum*, *Malassezia fuurfur* (*Pityrosporon orbiculare*, or *P. ovale*), *Cryptococcus neoformans*,  
10 *Aspergillus fumigatus*, and other *Aspergillus spp.*, *Zygomycetes* (*Rhizopus*, *Mucor*), *hyalohyphomycosis* (*Fusarium Spp.*), *Paracoccidioides brasiliensis*, *Blastomyces dermatitides*, *Histoplasma capsulatum*, *Coccidioides immitis*, and *Sporothrix schenckii*. Other examples include *Cladosporium cucumerinum*, *Epidermophyton floccosum*, and *Microsporum ypseum*.

## 15 G. Medical Devices

[000107] Non-limiting examples of medical devices are set forth herein. These include vascular devices such as grafts (e.g., abdominal aortic aneurysm grafts, etc.), stents, catheters (including arterial, intravenous, blood pressure, stent graft, etc.), valves (e.g., polymeric or carbon mechanical valves), embolic protection filters (including distal protection devices),  
20 vena cava filters, aneurysm exclusion devices, artificial hearts, cardiac jackets, and heart assist devices (including left ventricle assist devices), implantable defibrillators, electro-stimulation devices and leads (including pacemakers, lead adapters and lead connectors), implanted medical device power supplies, peripheral cardiovascular devices, atrial septal defect closures, left atrial appendage filters, valve annuloplasty devices, mitral valve repair  
25 devices, vascular intervention devices, ventricular assist pumps, and vascular access devices (including parenteral feeding catheters, vascular access ports, central venous access catheters); surgical devices such as sutures of all types, anastomosis devices (including anastomotic closures), suture anchors, hemostatic barriers, screws, plates, clips, vascular implants, tissue scaffolds, cerebro-spinal fluid shunts, shunts for hydrocephalus, drainage  
30 tubes, catheters including thoracic cavity suction drainage catheters, abscess drainage catheters, biliary drainage products, and implantable pumps; orthopedic devices such as joint implants, acetabular cups, patellar buttons, bone repair/augmentation devices, spinal devices

(*e.g.*, vertebral disks and the like), bone pins, cartilage repair devices, and artificial tendons; dental devices such as dental implants and dental fracture repair devices; drug delivery devices such as drug delivery pumps, implanted drug infusion tubes, drug infusion catheters, and intravitreal drug delivery devices; ophthalmic devices such as scleral buckles and sponges, glaucoma drain shunts and intraocular lenses; urological devices such as penile devices (*e.g.*, impotence implants), sphincter, urethral, prostate, and bladder devices (*e.g.*, incontinence devices, benign prostate hyperplasia management devices, prostate cancer implants, etc.), urinary catheters including indwelling ("Foley") and non-indwelling urinary catheters, and renal devices; synthetic prostheses such as breast prostheses and artificial organs (*e.g.*, pancreas, liver, lungs, heart, etc.); respiratory devices including lung catheters; neurological devices such as neurostimulators, neurological catheters, neurovascular balloon catheters, neuro-aneurysm treatment coils, and neuropatches, splints, nasal tampons, ear wicks, ear drainage tubes, tympanostomy vent tubes, otological strips, laryngectomy tubes, esophageal tubes, esophageal stents, laryngeal stents, salivary bypass tubes, and tracheostomy tubes; oncological implants; and pain management implants.

[000108] Classes of suitable non-implantable devices can include dialysis devices and associated tubing, catheters, membranes, and grafts; autotransfusion devices; vascular and surgical devices including atherectomy catheters, angiographic catheters, intraaortic balloon pumps, intracardiac suction devices, blood pumps, blood oxygenator devices (including tubing and membranes), blood filters, blood temperature monitors, hemoperfusion units, plasmapheresis units, transition sheaths, dialators, intrauterine pressure devices, clot extraction catheters, percutaneous transluminal angioplasty catheters, electrophysiology catheters, breathing circuit connectors, stylets (vascular and non-vascular), coronary guide wires, peripheral guide wires; dialators (*e.g.*, urinary, etc.); surgical instruments (*e.g.* scalpels and the like); endoscopic devices (such as endoscopic surgical tissue extractors, esophageal stethoscopes); and general medical and medically related devices including blood storage bags, umbilical tape, membranes, gloves, surgical drapes, wound dressings, wound management devices, needles, percutaneous closure devices, transducer protectors, pessary, uterine bleeding patches, PAP brushes, clamps (including bulldog clamps), cannulae, cell culture devices, materials for in vitro diagnostics, chromatographic support materials, infection control devices, colostomy bag attachment devices, birth control devices; disposable temperature probes; and pledgets.

## H. Examples

[000109] The following examples are included to demonstrate preferred embodiments of the invention. It should be appreciated by those of skill in the art that the techniques disclosed in the examples which follow represent techniques discovered by the inventor to function well in the practice of the invention, and thus can be considered to constitute preferred modes for its practice. However, those of skill in the art should, in light of the present disclosure, appreciate that many changes can be made in the specific embodiments which are disclosed and still obtain a like or similar result without departing from the spirit and scope of the invention.

### EXAMPLE 1

#### **Method of Coating Medical Device Results in Superior Properties**

##### Materials and Methods

[000110] Preparation of pieces. Gendine was prepared as described in U.S. Patent App. Pub. No. 20030078242. One-centimeter segments of endotracheal tube (ETT) made of polyvinylchloride (PVC-ETT) and urinary catheter (UC) made of silicone (SilUC) and central venous catheter (CVC) made of polyurethane (CVC-PU) were dipped into the Gendine solution, so that both internal and external surfaces were coated. The pieces were left to dry overnight, at 60°C. The pieces were then washed using mild detergent and de-ionized water to remove any possible loosely attached antiseptic off the surface of the coated segments. Some of the pieces were then left to dry for an additional 48 hours at a temperature of 60°C.

[000111] Absorbance and Quantitation of Leaching. To determine leaching of the dye, sets of standards with known concentrations of Gentian violet were made in each biological fluid (bronchoalveolar lavage, plasma, and artificial urine). Absorbances were read for each of the standards and a standard curve was plotted. Absorbances were also read from 200 µL biological fluids of each coated segments. Quantitation of leaching (in µg/L) was derived from the regression line in the standard curve. Unknown absorbances were read at 550 nm and then figured into the standard curve equation to determine amount of leaching in µg/L.

[000112] Adherence testing. The inventors evaluated bacterial adherence to the surface of Gendine-coated and control uncoated segments, as well as that of silver hydrogel urinary catheter and other antiinfective approved CVC, such as the antibiotic-coated CVC (Spectrum, Cook Critical Care, Bloomington, IN - coated with minocycline and rifampin), CVC coated with chlorhexidine/silver sulfadiazine (Arrow Guard Plus, Arrow, Reading, PA) and silver/platinum CVC (Edwards, Edwards Life Sciences, Irvine, CA). Six segments of each device were tested per organism. A modification of a previously published method for testing adherence and biofilm formation on silicone disks was used (Chaiban *et al.*, 2005).

[000113] The sterile device segments were placed into sterile 5 mL snap top tubes containing 1 mL of plasma. The tubes were then placed into the incubator for 24 hours at 37°C. The plasma was then removed from the tubes, leaving the pieces inside the tubes, and was replaced with 1mL of Mueller Hinton Broth (MHB), that was inoculated with bacteria. The inoculum was prepared as follows: Five colonies of freshly subbed bacteria were placed in 50 mLs of MHB (0.5 McFarland, approximately  $1.3 \times 10^8$  CFU/mL), and used immediately. The tubes were then placed in the incubator for 24 hours at 37°C. The MHB was then removed and replaced with 1 mL of 0.9% saline solution and the tube was placed in the 37°C incubator for 30 minutes as a washing step. The catheter segments were then removed from the washing saline, and placed into sterile 15 mL tubes containing 5 mLs of 0.9% sterile saline solution and sonicated for 15 minutes. After sonication, the tubes containing the catheters were vortexed for 60 seconds. A 100  $\mu$ L volume of the sample was pipetted and spread onto a trypticase soy agar plate with 5% sheep blood (this was the 1:50 dilution). The plates were placed in the incubator for 24 hours, and then the colonies were counted. A value of 100 CFU was used for any plate that had at least 100 counted colonies.

[000114] Zones of inhibition and antimicrobial durability. Using a modified Kirby-Bauer method, baseline antimicrobial activity was assessed by measuring the zones of inhibition created by duplicates of impregnated segments that were vertically embedded in Mueller Hinton agar plates coated with one of the following organisms: Methicillin-resistant staphylococcus aureus (MRSA), *C. albicans*, *C. parapsilosis*, Vancomycin-resistant *Enterococci* (VRE), *P. aeruginosa*, and *E. coli*. The zones of inhibition were measured and recorded as the diameter (mm) across the center of the embedded segments.

[000115] The antimicrobial durability of Gendine-coated ETT (GND-ETT), Gendine-coated UC (GND-UC) and Gendine-coated CVC (GND-CVC) segments was assessed over time by



testing zones of inhibitions of segments soaked in body fluids. The antimicrobial durability of that GND-CVC was compared with other anti-infective CVC described above (Arrow Guard Plus, Edwards and Spectrum). The segments were placed in sterile 50 mL polystyrene tubes (Falcon), containing 10 mL sterile bronchoalveolar lavage (ETT) or urine (UC), or serum (CVC), respectively, and were incubated at 37°C. The 10 mL volume was used to ensure the complete immersion of all of the pieces contained in the tube. Segments were tested in duplicates at weekly intervals, as the soaking fluids were replaced with fresh fluids. Zones of inhibition were determined using the modified Kirby-Bauer method against the same organisms mentioned above.

**[000116] Abbreviations.** MRSA (bacteria) = multidrug-resistant *Staphylococcus aureus*. PS (bacteria) = *Pseudomonas aeruginosa*. EC (bacteria) = *Escherichia coli*. VRE (bacteria) = vancomycin-resistant *Enterococcus*. CA (fungi) = *Candida albicans*.

## Results

**[000117] Endotracheal Tubes (ETT).** As shown in FIG. 1, heating of the Gendine-coated ETT decreased leaching of the antiseptic dye (Gendine) progressively and substantially ( $P < 0.01$ ). More than three-fold decrease in leaching of Gendine was quantitatively noted after three days of heating (Gendine H3) and by more than two-fold after one day of heating (Gendine H1). Furthermore, heating of the Gendine-coated ETT improved anti-infective anti-adherence effect of the Gendine-coated ETT against multidrug-resistant *Pseudomonas aeruginosa* as shown in FIG. 2. This improvement was significant ( $P < 0.001$ ) after one day of heating (Gendine H1) and three days of heating (Gendine H3). Heating did not compromise the antimicrobial durability of the Gendine-coated ETT against MRSA through the series of zones of inhibitions performed. This high level of antimicrobial durability was hence maintained as shown in FIG. 3.

**[000118] Central Venous Catheters (CVC).** As shown in FIG. 4 below, heating progressively decreased the leaching of Gendine-coated CVC into the serum ( $P < 0.05$ ). Heating of Gendine-coated CVC for one day (Gendine H1) resulted in almost 1.6-fold decrease in leaching whereas three days of heating (Gendine H3) was associated with 3.5-fold decrease leaching into the serum when compared to unheated Gendine-coated CVC. Furthermore, as shown in FIG. 5, three-day heating of Gendine-coated CVC (Gendine H3) maintained a significantly improved anti-adherence effect of multidrug-resistant bacteria,

such as *Pseudomonas aeruginosa* and MRSA when compared with uncoated CVC or other antimicrobial CVC, such as the spectrum coated with antibiotics (minocycline and rifampin) or Arrow Guard (coated with chlorhexidine and silver sulfadiazine) or the Edwards catheter (with electric silver and platinum ions) ( $p < 0.04$ ). Three day heating (Gendine H3) also  
5 maintained a significantly superior anti-adherence effect compared to uncoated CVC with the Spectrum and the Edwards catheter against fungi, ( $p < 0.02$ ) such as *Candida albicans* and *Candida parapsilosis*, which are known to be associated with catheter-related candidemia (FIG. 5). In addition, the heating of Gendine-coated CVC (Gendine H1 and Gendine H3) continued to maintain a superior antimicrobial durability against MRSA, multidrug-resistant  
10 *Pseudomonas aeruginosa* and *Candida parapsilosis* when compared to other antimicrobial catheters, such as the Spectrum, Arrow Guard and Edwards, as shown in FIG. 6, FIG. 7 and FIG. 8.

[000119] Urinary Catheters (UC). FIG. 9 shows that heating of Gendine-coated UC (Gendine H1 and Gendine H3) progressively and substantially decreased leaching ( $P < 0.001$ ).  
15 The one-day heating (Gendine H1) decreased the leaching of silicone UC by 1.6-fold, whereas the three-day heating (Gendine H3) decreased the leaching into urine of the Gendine by 2.5-fold. Furthermore, as shown below, heating of Gendine-coated UC (Gendine H3-UC) maintained a significantly ( $P \leq 0.025$ ) improved anti-adherence effect, compared to uncoated to uncoated urinary catheters or silver-coated UC against two isolates of multidrug-resistant  
20 *Pseudomonas* and two isolates of *E. coli* (FIG. 10). It should be noted that the silver-coated UC has been shown effective in decreasing bacteruria clinically. In addition, as shown in FIG. 11, FIG.12 and FIG.13, heating of Gendine-coated silicone UC maintained a high level of antimicrobial durability over a 56-day period against vancomycin-resistant Enterococci (VRE), resistant *E. coli* and *Candida parapsilosis* tested through zones of inhibition and urine.

25 [000120] Heating of Gendine-coated ETT was associated with a significant decrease in leaching into bronchoalveolar lavage ( $p < 0.05$ ) and a significant improvement in the anti-adherence/antimicrobial activity of Gendine-coated ETT against multidrug-resistant *Pseudomonas aeruginosa* ( $p < 0.001$ ). The high level of antimicrobial durability of Gendine-coated ETT against methicillin resistant staphylococcus aureus (MRSA) was maintained  
30 through heating.

[000121] Heating of Gendine-coated CVC was progressively and substantially associated with decreased leaching of this antiseptic dye into serum while maintaining a significant anti-

adherence activity against resistant bacteria and fungi compared to other antimicrobial catheters on the market. Furthermore, the antimicrobial durability of the heated Gendine-coated CVC was maintained in a superior fashion to other antimicrobial catheters placed in serum.

5 [000122] The heating of silicone UC coated with Gendine was associated with a progressive and substantial decrease of this antiseptic dye into urine while maintaining a significantly superior anti-adherence/antimicrobial activity against Multidrug-resistant gram-negative bacteria, such as *Pseudomonas aeruginosa* and *E. coli* compared to the only available anti-infective urinary catheter on the market, which is the silver hydrogel-coated Bard UC.  
10 Furthermore the high level of antimicrobial durability of Gendine-coated UC was maintained through heating for up to 56 days against fungi, such AS *Candida parapsilosis*, multidrug-resistant organisms, such as VRE and *E. coli*.

[000123] All medical devices coated with antiseptic dyes or antiseptic/antimicrobial agents including.

15

## EXAMPLE 2

### Studies Demonstrating that Heating Enhances the Durability of Antimicrobial Efficacy and Adherence of Biofilm to Minocycline/Rifampin-Coated and Heated Silicone and CVCs

#### **Materials and Method**

20

[000124] Antimicrobial coating procedure. Constantly stirring, 450 mg of NaOH was dissolved in a beaker containing 45 mL of methanol heated to 45°C. Once completely dissolved, 4.5 g of minocycline was added to the solution in small aliquots over 15 minutes and stirred until completely dissolved. Then, 9 g of rifampin were added to the solution in  
25 small aliquots over 15 minutes. Solution was stirred at 45°C until completely clear. Finally 255 mL of prewarmed (45°C) butyl acetate was added to the solution and stirred until thoroughly mixed.

[000125] Whole catheters (Cook silicone CVC) were coated for 1 hour at 45°C. Catheters were removed and allowed to dry for 1 day as described below.

[000126] 1 day heating - Dried at 60°C overnight (14-24 hours). Washed twice (ddH<sub>2</sub>O, ddH<sub>2</sub>O + detergent for 1 minute then dried for an additional 4 hours at 60°C. After drying, the catheters were cut into 0.5 cm segments for *in vitro* durability and adherence testing. Uncoated catheters and commercially available Spectrum catheters (coated catheters which were not heated) were also tested for comparison.

[000127] Efficacy and Durability of antiseptic activity in Coated CVCs. Using the modified Kirby-Bauer method, coated catheter segments were vertically inserted in agar plates inoculated with a 0.5 McFarland dilution of microorganisms. Organisms to be tested against included:

1. methicillin resistant *Staphylococcus aureus* (MRSA 4978) – clinical isolate
2. *Stenotrophomonas maltophilia* (5075, 4709, 4807) – catheter site isolate

[000128] Plates were incubated overnight then zones of inhibition (ZOI) were measured in millimeters (mm). Remaining coated segments were incubated in donor calf serum. Weekly segments were removed for durability testing and the donor calf serum was replaced with fresh.

[000129] Adherence of biofilm to coated CVCs. Following a modified Kuhn's method, coated catheter segments were incubated for 24 hours in plasma. The plasma was then replaced with  $5.0 \times 10^5$  cells in Muller Hinton Broth of either methicillin resistant *Staphylococcus aureus* (MRSA 4798) or *Stenotrophomonas maltophilia* (5075, 4709, 4807) and incubated for an additional 24 hours. After incubation, the bacterial inoculum was discarded and segments were washed shaking for 30 minutes in 1 mL of 0.9% sterile saline. The segments were then removed with sterile sticks placed in 5 mL of 0.9% sterile saline and sonicated for 15 minutes. After sonication, 100  $\mu$ L of liquid from each segment was spread onto trypticase soy agar with 5 % sheep blood and incubated at 37°C inverted for 24 hours. Plates were then counted for colony growth.

[000130] Statistical Methods. For each bacterium strain, the numbers of viable organisms adhering to the catheter segments indicated by CFU were compared by Kruskal-Wallis test ( $P < 0.05$  was regarded statistically significant). If a significant result was detected for the test, a Wilcoxon rank sum tests for the following pairwise comparisons was made: comparing PU-Mino/Rifam (H1=heated) with PU-Spectrum (not heated) and comparing each of them with control, respectively; comparing Silicone -Mino/Rifam (H1=heated) with Silicone-

Spectrum(not heated) and comparing each of them with control, respectively. The  $\alpha$  levels of the post-hoc pairwise comparisons were adjusted using a sequential Bonferroni adjustment to control type I error.

**Results**

5

[000131] Table 2 demonstrates results of studies evaluating the efficacy and durability of antiseptic activity in coated CVCs. Spectrum catheters are those coated with minocycline and rifampin without any heating to determine the antimicrobial durability of catheters coated with minocycline and rifampin. Segments of spectrum silicone catheters coated with minocycline and rifampin (without heating) and other silicone catheters coated with minocycline and rifampin that were heated were immersed in serum. Catheter segments were removed at weekly intervals and we determined zones of inhibition (ZOI) against resistant bacteria such as methicillin resistant *staphylococci* (MRSA) and *strenotrophomas maltophilia* (*S. malta*) strains. A ZOI of  $\geq 10$  mm is predictive of *in vivo* and clinical efficacy. It was found that heating of the catheters treated with Mino/Rifampin increased the efficacy (ZOI  $\geq 10$ ) of coating against MRSA from 28 days to 70 days (Table 2). It was also found that heating of the catheters treated with Mino/Rifampin increased the efficacy (ZOI  $\geq 10$ ) of coating against *Stenotrophomonas maltophilia* by 1 week.

10

15

**Table 2.** Efficacy and Durability of antiseptic activity in Coated CVCs as determined by zones of inhibition:

20

Silicone - Spectrum		MRSA 4798		S. malto 5075		S. malto 4807		S. malto 4709	
21-Feb-2006	Baseline (Day 0)	27	27	18	18	20	19	18	18
28-Feb-2006	Day 7	21	21	0	0	12	12	12	12
7-Mar-2006	Day 14	18	16	0	0	0	0	0	0
14-Mar-2006	Day 21	15	14	0	0	0	0	0	0
21-Mar-2006	Day 28	13	13	0	0	0	0	0	0
28-Mar-2006	Day 35	8	8	0	0	0	0	0	0
4-Apr-2006	Day 42	8	7	0	0	0	0	0	0
11-Apr-2006	Day 49	7	7	0	0	0	0	0	0
18-Apr-2006	Day 56	5	5	0	0				
25-Apr-2006	Day 63	0	0	0	0				
2-May-2006	Day 70	0	0	0	0				
9-May-2006	Day 77	0	0	0	0				
	Day 84								
<b>Silicone - Mino/Rifampin 1 day heat</b>									
21-Feb-2006	Baseline (Day 0)	32	30	20	20	22	21	21	20
28-Feb-2006	Day 7	25	24	8	7	16	15	15	12

7-Mar-2006	Day 14	22	21	0	0	12	12	8	7
14-Mar-2006	Day 21	21	21	0	0	0	0	0	0
21-Mar-2006	Day 28	20	19	0	0	0	0	0	0
28-Mar-2006	Day 35	14	14	0	0	0	0	0	0
4-Apr-2006	Day 42	10	10	0	0	0	0	0	0
11-Apr-2006	Day 49	10	10	0	0	0	0	0	0
18-Apr-2006	Day 56	10	10	0	0				
25-Apr-2006	Day 63	10	10	0	0				
2-May-2006	Day 70	10	10	0	0				
9-May-2006	Day 77	7	7	0	0				
	Day 84								

[000132] Table 3 demonstrates results of studies pertaining to an evaluation of the adherence of biofilm forming bacteria biofilm to coated CVCs.

5 [000133] Adherence of biofilm to coated CVC's:

[000134] Following a modified Kuhn's method coated silicone catheter segments were incubated for 24 hours in plasma. The plasma was then replaced with  $5.0 \times 10^5$  cells in Muller Hinton Broth of either methicillin resistant *Staphylococcus aureus* (MRSA 4798) or *Stenotrophomonas maltophilia* (5075, 4709, 4807) and incubated for an additional 24 hours.

10 After incubation, the bacterial inoculum was discarded and segments were washed by shaking for 30 minutes in 1 mL of 0.9% sterile saline. The segments were then removed with sterile sticks placed in 5 mL of 0.9% sterile saline and sonicated for 15 minutes. After sonication, 100  $\mu$ L of liquid from each segment was spread onto trypticase soy agar with 5% sheep blood and incubated at 37C° inverted for 24 hours. Plates were then counted for colony growth.

15

[000135] It was found that heating of polyurethane and silicone CVCs increased the inhibition of biofilm forming bacteria when tested against MRSA and *S.malto*. When tested against MRSA Sil Mino/Rifampin-1 (heated at 60°C for one day) significantly decreased adherence ( $p=0.0047$ ) when compared to CVCs coated with minocycline and rifampin without heating. All coated catheters showed significant decrease of adherence of biofilm forming bacteria ( $p<0.0001$ ) when compared to uncoated control catheters.

20

**Table 3. - Adherence of biofilm forming bacteria to coated CVCs:**

Tested against adherence of methicillin resistant Staph aureus (MRSA 4798)												
	Control		Control		PU Mino/Rifampin		Control		Control		Sil-Mino/Rifampin	
	PU-Uncoated		PU Spectrum		1 day heat		Silicone-Uncoated		Sil-Spectrum		1 day heat	
	Plate count	Dilution	Plate count	Dilution	Plate count	Dilution	Plate count	Dilution	Plate count	Dilution	Plate count	Dilution
1	100	5000	0	0	0	0	100	5000	1	50	0	0
2	100	5000	4	200	1	50	100	5000	1	50	0	0
3	100	5000	5	250	4	200	100	5000	4	200	1	50
4	100	5000	13	650	10	500	100	5000	4	200	4	200
5	100	5000	45	2250	27	1350	100	5000	5	250	0	0
6	100	5000	6	300	46	2300	100	5000	5	250	0	0
7	100	5000	73	3650	14	700	100	5000	6	300	4	200
8	100	5000	49	2450	0	0	100	5000	11	550	4	200
9	100	5000	92	4600	2	100	100	5000	3	150	0	0
10	100	5000	47	2350	5	250	100	5000	31	1550	0	0
Average		5000		1670		545		5000		355		65
St Dev		0.00		1626.04		745.15		0.00		443.13		94.43
Tested against adherence of Stenotrophomas Maltophilia (PS 4807 & 4709)												
	Control		Control		PU Mino/Rifampin		Control		Control		Sil-Mino/Rifampin	
	PU-Uncoated		PU Spectrum		1 day heat		Silicone-Uncoated		Sil-Spectrum		1 day heat	
	Plate count	Dilution	Plate count	Dilution	Plate count	Dilution	Plate count	Dilution	Plate count	Dilution	Plate count	Dilution
1	100	5000	0	0	3	150	100	5000	0	0	0	0
2	100	5000	0	0	4	200	100	5000	0	0	0	0
3	100	5000	2	100	22	1100	100	5000	0	0	0	0
4	100	5000	15	750	42	2100	100	5000	1	50	2	100
5	100	5000	100	5000	14	700	100	5000	100	5000	0	0
6	100	5000	67	3350	3	150	100	5000	100	5000	0	0
7	100	5000	100	5000	6	300	100	5000	100	5000	6	300
8	100	5000	100	5000	2	100	100	5000	100	5000	11	550
9	100	5000	100	5000	6	300	100	5000	100	5000	4	200
10	100	5000	3	150	9	450	100	5000	100	5000	7	350
Average		5000		2435		555		5000		3005		150
St Dev		0.00		2415.81		624.26		0.00		2575.57		194.37

1) Results pertaining to adherence of *S. maltophilia* (PS 4807):

5 [000136] The Kruskal-Wallis test detected a significant difference for PS4807 CFU among the 3 types of CVCs ( $\chi^2_{(3)} = 43.97, p < .0001$ ).

[000137] According to the Wilcoxon rank sum tests, there was no significant difference in CFU between PU Mino/Rifam (H1=heated) and PU-Spectrum (not heated) ( $p=0.45$ ), but both catheters significantly reduced CFU compared to the control ( $p < .0001$  for PU Mino/Rifam (H1=heated) vs control;  $p= 0.0059$  for PU-Spectrum (not heated) vs control). The CFU of Si-Mino/Rifam (H1=heated) was significantly less than that of Si-Spectrum (not heated) ( $p=0.022$ ), which in turn was less than that of the control ( $p < .0001$ ).

10

**Table 4.** *S. maltophilia* 4807 biofilm CFU among different catheters

Catheter	Mean	Median	(Min - Max)	N
PU - Uncoated	5000	5000	(5000 - 5000)	10
PU - Spectrum	2435	2050	(0 - 5000)	10
PU - Mino/Rifam (H1)	555	300	(100 - 2100)	10
Silicone - Uncoated	5000	5000	(5000 - 5000)	10
Silicone - Spectrum	240	125	(0 - 1250)	10
Silicone - Mino/Rifam (H1)	30	0	(0 - 150)	10

**Kruskal-Wallis test: Chi-square statistic with 5 d.f. =43.97, p < .0001**

- PU= Cool Polyurethane
- Spectrum = CVC coated with minocycline & rifampin without heating.
- Mino/Rifam (H1)=CVC coated with minocycline & rifampin with 1 day heating at 60 °C

Comparisons: (PS4807)

Catheters:	p-value
1. PU-Mino/Rifam (H1) vs Pu-Spectrum	0.45
2. PU-Mino/Rifam (H1) vs PU-Uncoated	< .0001
3. PU-Spectrum vs PU-Uncoated	0.0059
1. Si -Mino/Rifam (H1) vs Si -Spectrum	0.022
2. Si -Mino/Rifam (H1) vs Si -Uncoated	< .0001
3. Si-Spectrum vs Si-Uncoated	< .0001

2) Results pertaining to adherence of *S. maltophilia* (PS 4709):

[000138] The Kruskal-Wallis test detected a significant difference for PS4709 CFU among the 3 types of CVCs ( $\chi^2_{(3)} = 34.36, p < .0001$ ).

[000139] According to the Wilcoxon rank sum tests, there was no significant difference in CFU between PU Mino/Rifam (H1=heated) and PU-Spectrum (not heated) ( $p= 0.85$ ), and between a trend towards reducing adherence when we compared Silicone-Mino/Rifam (H1=heated) and to Silicone- Spectrum (coated with minocycline and rifampin but not heated)( $p=0.081$ ), respectively. However all the Mino/Rifam coated catheters significantly reduced CFU than their corresponding controls, respectively (Table 4).



**Table 5.** *S. maltophilia* 4709, Biofilm CFU among different catheters

Catheter	Mean	Median	(Min - Max)	N
PU - Uncoated	5000	5000	(5000 - 5000)	10
PU - Spectrum	650	525	(0 - 2900)	10
PU - Mino/Rifam (H1)	1600	600	(0 - 5000)	10
1. Silicone - Uncoated	5000	5000	(5000 - 5000)	10
2. Silicone - Spectrum	3005	5000	(0 - 5000)	10
3. Silicone - Mino/Rifam (H1)	150	50	(0 - 550)	10

**Kruskal-Wallis test: Chi-square statistic with 5 d.f. =34.36, p < .0001**

Comparisons: (PS4709)

Catheters:	<i>p</i> -value
1. PU-Mino/Rifam (H1) vs Pu-Spectrum	0.85
2. PU-Mino/Rifam (H1) vs PU-Uncoated	0.0007
3. PU-Spectrum vs PU-Uncoated	< .0001
1. Si -Mino/Rifam (H1) vs Si -Spectrum	0.081
2. Si -Mino/Rifam (H1) vs Si -Uncoated	< .0001
3. Si-Spectrum vs Si-Uncoated	0.034

5

3) Results pertaining to MRSA 4798

[000140] The Kruskal-Wallis test detected a significant difference for MRSA 4798 CFU among the 6 CVCs ( $\chi^2_{(5)} = 47.86, p < .0001$ ). According to the Wilcoxon rank sum tests (see Table 6), there was no significant difference in CFU between PU Mino/Rifam (H1=heated) and PU-Spectrum (not heated) ( $p=0.088$ ), but both catheters significantly reduced CFU compared to the control ( $p < .0001$ , respectively). The CFU of Si-Mino/Rifam (H1=heated) was significantly less than that of Si-Spectrum (not heated) ( $p=0.0047$ ), which in turn was less than that of the control ( $p < .0001$ ).

10

**Table 6.** MRSA 4798 Biofilm CFU among different catheters

Catheter	Mean	Median	(Min - Max)	N
PU - Uncoated	5000	5000	(5000 - 5000)	10
PU - Spectrum	1670	1450	(0 - 4600)	10
PU - Mino/Rifam (H1)	545	225	(0 - 2300)	10
Silicone - Uncoated	5000	5000	(5000 - 5000)	10
Silicone - Spectrum	355	225	(50 - 1550)	10
Silicone - Mino/Rifam (H1)	65	0	(0 - 200)	10

**Kruskal-Wallis test: Chi-square statistic with 5 d.f. =47.86, p < .0001**

15

Comparisons: (MRSA 4798)

Catheters:	<i>p</i> -value
1. PU-Mino/Rifam (H1) vs Pu-Spectrum	0.088
2. PU-Mino/Rifam (H1) vs PU-Uncoated	< .0001
3. PU-Spectrum vs PU-Uncoated	< .0001
4. Si -Mino/Rifam (H1) vs Si -Spectrum	0.0047
5. Si -Mino/Rifam (H1) vs Si -Uncoated	< .0001
6. Si-Spectrum vs Si-Uncoated	< .0001

\* \* \* \* \*

[000141] All of the methods disclosed and claimed herein can be executed without undue experimentation in light of the present disclosure. While the of this invention have been described in terms of preferred embodiments, it will be apparent to those of skill in the art that variations may be applied to the methods or in the sequence of steps of the method described herein without departing from the concept, spirit and scope of the invention. More specifically, it will be apparent that certain agents which are both chemically and physiologically related may be substituted for the agents described herein while the same or similar results would be achieved. All such similar substitutes and modifications apparent to those skilled in the art are deemed to be within the spirit, scope and concept of the invention as defined by the appended claims.

### REFERENCES

The following references, to the extent that they provide exemplary procedural or other details supplementary to those set forth herein, are specifically incorporated herein by reference.

- 5 U.S. Patent 4,107,121  
U.S. Patent 4,442,133  
U.S. Patent 4,895,566  
U.S. Patent 4,917,686  
U.S. Patent 4,952,419  
10 U.S. Patent 5,013,306  
U.S. Patent 5,362,754  
U.S. Patent 5,624,704  
U.S. Patent Application 2003/0078242  
U.S. Patent Application 2005/0197634  
15  
American Thoracic Society. Official Statement. *Respir. Crit. Care Med.*, 153:1711-1725, 1996.  
Centers for Disease Control and Prevention, Morbidity and Mortality Weekly Report CDC Surveillance, 46:891, 1993.  
20 Chaiban *et al.*, *Journal of Antimicrobial Chemotherapy* 55:51-56, 2005.  
Klempner *et al.*, In: *Infectious diseases: medical knowledge self-assessment program*, 2<sup>nd</sup> Ed., American College of Physicians, Philadelphia, PA, 210, 1998.  
Leu *et al.*, *Am. J. Epidemiol.*, 129:1258-1267, 1989.  
Platt and Bucknall, *J. Hosp. Infect.*, 11:396-397, 1988.  
25 Raad, *Lancet*, 351:893-898, 1998.  
Raad *et al.*, *J Infect Dis* 173:418-24, 1996.  
Reiselman *et al.*, *JAMA*, 272:1578-1601, 1994.  
Solomon and Sherertz, *Controlled Release*, 6:343-352, 1987.  
UK Appln. 109,496  
30

### CLAIMS

1. A method for coating or impregnating a non-organic surface with an antimicrobial agent, comprising:
  - 5 a) contacting the non-organic surface with an composition comprising an antimicrobial agent and a solvent; and
  - b) curing the non-organic surface at a temperature that is at least about 40°C, wherein at least some of the solvent that was contacted with the surface is removed, and wherein the antimicrobial agent coats or impregnates the surface.
- 10 2. The method of claim 1, further defined as a method for coating or impregnating a medical device with an antimicrobial agent, wherein the non-organic surface is the surface of a medical device.
- 15 3. The method of claim 2, wherein the medical device is an endotracheal tube, a tracheotomy tube, chest tube, a vascular catheter, an urinary catheter, a nephrostomy tube, a biliary stent, a peritoneal catheter, an epidural catheter, a central nervous system catheter, an orthopedic device, a prosthetic valve, a gastric tube, an intestinal tube, or drug-delivery implant.
- 20 4. The method of claim 3, wherein the medical device is a vascular catheter selected from the group consisting of a central venous catheter, an arterial line, a pulmonary artery catheter, a stent, and a peripheral venous catheter, an infusion port, or a dialysis catheter.
- 25 5. The method of claim 3, wherein the medical device is a central nervous system catheter further defined as an intraventricular shunt.
6. The method of claim 1, wherein the non-organic surface is a surface of a glove, a condom, a gown, hospital equipment, a table, a container, a countertop, a floor, a bag, a  
30 suture, a device used in food-processing, a sponge, or a mop.
7. The method of claim 1, wherein the antimicrobial agent is further defined as an antibiotic, an antiseptic, an antiviral agent, an antifungal agent, or a disinfectant.

8. The method of claim 7, wherein the antimicrobial agent is an antibiotic.
9. The method of claim 8, wherein the antibiotic is a tetracycline, a macrocyclic antibiotic compound, or a combination thereof.
- 5
10. The method of claim 9, wherein the tetracycline is minocycline.
11. The method of claim 9, wherein the macrocyclic antibiotic is rifampin, rifampicin, or a combination thereof.
- 10
12. The method of claim 8, wherein the composition comprises tetracycline and minocycline.
13. The method of claim 7, wherein the antimicrobial agent is an antiseptic.
- 15
14. The method of claim 7, wherein the antimicrobial agent is a disinfectant.
15. The method of claim 1, wherein the antimicrobial agent comprises a dye, a basic reagent, or a combination thereof.
- 20
16. The method of claim 15, wherein the composition comprises a basic reagent and a dye.
17. The method of claim 16, wherein the basic reagent is a guanidium compound, a biguanide, a bipyridine, a phenoxide antiseptic, an alkyl oxide, an aryl oxide, a thiol, a halide, an aliphatic amine, or an aromatic amine.
- 25
18. The method of claim 17, wherein the basic reagent is a guanidium compound.
19. The method of claim 18, wherein the guanidium compound is chlorhexidine, alexidine, or hexamidine.
- 30
20. The method of claim 17, wherein the basic reagent is a bipyridine.
21. The method of claim 20, wherein the bipyridine is octenidine.

22. The method of claim 17, wherein the basic reagent is a phenoxide antiseptic.
23. The method of claim 22, wherein the phenoxide antiseptic is clofocetol, chloroxylenol,  
5 or triclosan.
24. The method of claim 16, wherein the dye is a triarylmethane dye, a monoazo dye, a  
diaz dye, an indigoid dye, a xanthene dye, an anthraquinone dye, a quinoline dye, an  
FD&C dye, a D&C dye, or brilliant green.
- 10 25. The method of claim 24, wherein the dye is a triarylmethane dye selected from the  
group consisting of gentian violet, crystal violet, and ethyl violet.
26. The method of claim 25, wherein the FD&C dye is Blue No. 1 or Green No. 3.
- 15 27. The method of claim 24, wherein the monoazo dye is FD&C Yellow No. 5 or FD&C  
Yellow No. 6.
28. The method of claim 24, wherein the diazo dye is D&C Red No. 17.
- 20 29. The method of claim 24, wherein the indigoid dye is FD&C Blue No. 2.
30. The method of claim 24, wherein the xanthene dye is FD&C Red No. 3.
- 25 31. The method of claim 24, wherein the anthraquinone dye is D&C Green No. 6.
32. The method of claim 24, wherein the quinoline dye is D&C Yellow No. 1.
33. The method of claim 1, wherein the surface comprises a micropore or a nanopore.
- 30 34. The method of claim 1, wherein curing comprises heating the surface to a temperature  
that is about 40°C to about 100°C.

35. The method of claim 24, wherein curing comprises heating the surface to a temperature that is about 40°C to about 80°C.
36. The method of claim 35, wherein curing comprises heating the surface to a temperature that is about 40°C to about 60°C.
37. The method of claim 36, wherein the surface is heated for about 1 hour to about 3 weeks.
38. The method of claim 37, wherein the surface is heated for about 12 hours to about 96 hours.
39. The method of claim 38, wherein the surface is heated for about 24 hours to about 72 hours.
40. The method of claim 1, wherein curing is further defined as drying the surface.
41. The method of claim 1, further comprises washing the surface after curing the surface.
42. The method of claim 41, wherein washing is further defined as contacting the surface with a composition comprising a detergent and water.
43. The method of claim 41, further comprising curing the surface at a temperature of at least 40°C after washing the surface.
44. The method of claim 43, wherein the surface is cured for at least 1 hour to at least 96 hours.
45. The method of claim 44, wherein the surface is cured for at least 24 hours to at least 72 hours.
46. The method of claim 1, wherein the surface is composed of a polymer or silicone.

47. The method of claim 46, wherein the polymer is polyvinyl chloride, polyurethane, polyethylene, silastic elastomers, polytetrafluoroethylene, dacron, collodion, carboethane or nylon.
- 5 48. The method of claim 2, further comprising packaging the medical device in a container.
49. The method of claim 2, further comprising sterilizing the medical device.
- 10 50. A method for coating or impregnating a medical device with an antimicrobial composition, comprising the steps of:
- a) contacting the medical device with a composition comprising an antimicrobial agent and a solvent;
  - 15 b) curing the medical device at a temperature of about 40°C to about 80°C for about 12 hours to about 72 hours, wherein the medical device is dried;
  - c) washing the medical device with an aqueous composition; and
  - 20 d) repeating step b),
- wherein the medical device becomes coated or impregnated with an antimicrobial composition.
- 25 51. A method for reducing the risk of development or progression of an infection in a subject in need of a medical device, comprising coating or impregnating a surface of the medical device with an antimicrobial agent in accordance with the method of claim 1 prior to contacting the medical device with the subject, wherein the risk of development or progression of an infection is reduced.
- 30 52. The method of claim 51, wherein the subject is a human.
53. The method of claim 51, wherein the antimicrobial agent is further defined as an antibiotic, an antiseptic, an antiviral agent, an antifungal agent, or a disinfectant.




54. The method of claim 53, wherein the antimicrobial agent is an antibiotic.
55. The method of claim 54, wherein the antibiotic is a tetracycline, a macrocyclic antibiotic compound, or a combination thereof.
56. The method of claim 55, wherein the tetracycline is minocycline.
57. The method of claim 55, wherein the macrocyclic antibiotic is rifampim, rifampicin, or a combination thereof.
58. The method of claim 51, wherein the infection is pneumonia, bacteremia, fungemia, candidemia, a urinary tract infection, a catheter-exit site infection, or a surgical wound infection.
59. The method of claim 51, wherein the infection is a nosocomial infection.
60. The method of claim 59, wherein the infection is caused by methicillin-resistant staphylococci, vancomycin-resistant enterococci, resistant *Pseudomonas aeruginosa*, or a combination thereof.
61. The method of claim 59, wherein the infection is a fungal infection secondary to *Candida species*.
62. The method of claim 51, wherein the antimicrobial agent is an antibacterial agent, an antiviral agent, or an antifungal agent.
63. The method of claim 62, wherein the antibacterial agent is minocycline or rifampin.
64. The method of claim 51, wherein the composition comprises a basic reagent and a dye.
65. The method of claim 51, wherein the medical device is an endotracheal tube, a vascular catheter, an urinary catheter, a nephrostomy tube, a biliary stent, a peritoneal catheter, an

epidural catheter, a central nervous system catheter, an orthopedic device, a prosthetic valve, a silk suture, or a medical implant.


5 66. The method of claim 65, wherein the medical device is a vascular catheter further defined as a central venous catheter, an arterial line, an pulmonary artery catheter, or a peripheral venous catheter.

67. The method of claim 65, wherein said central nervous system catheter is an intraventricular shunt.

10

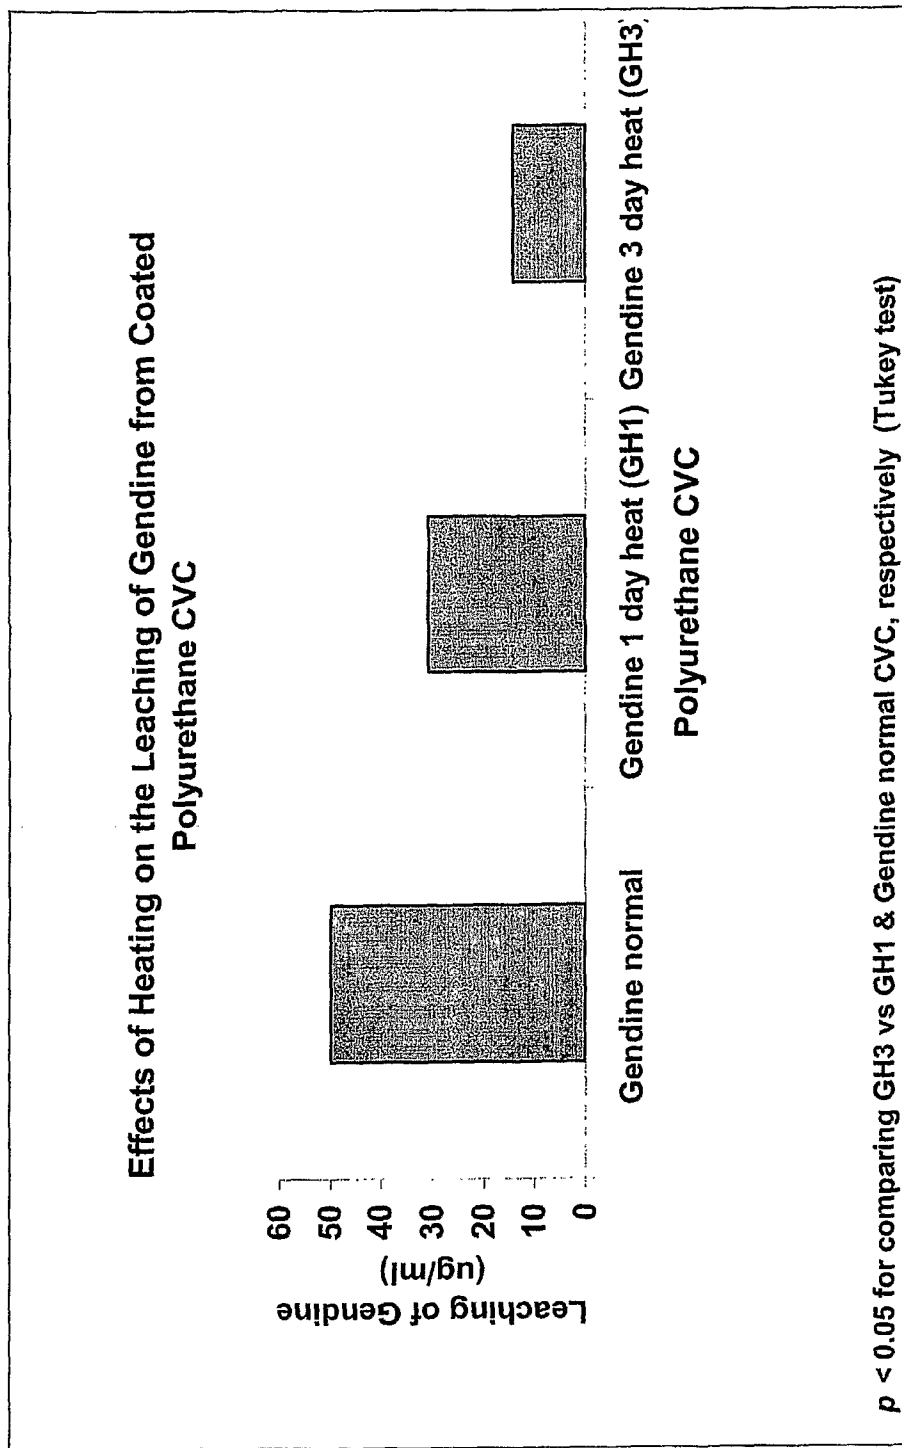

**FIG. 1**

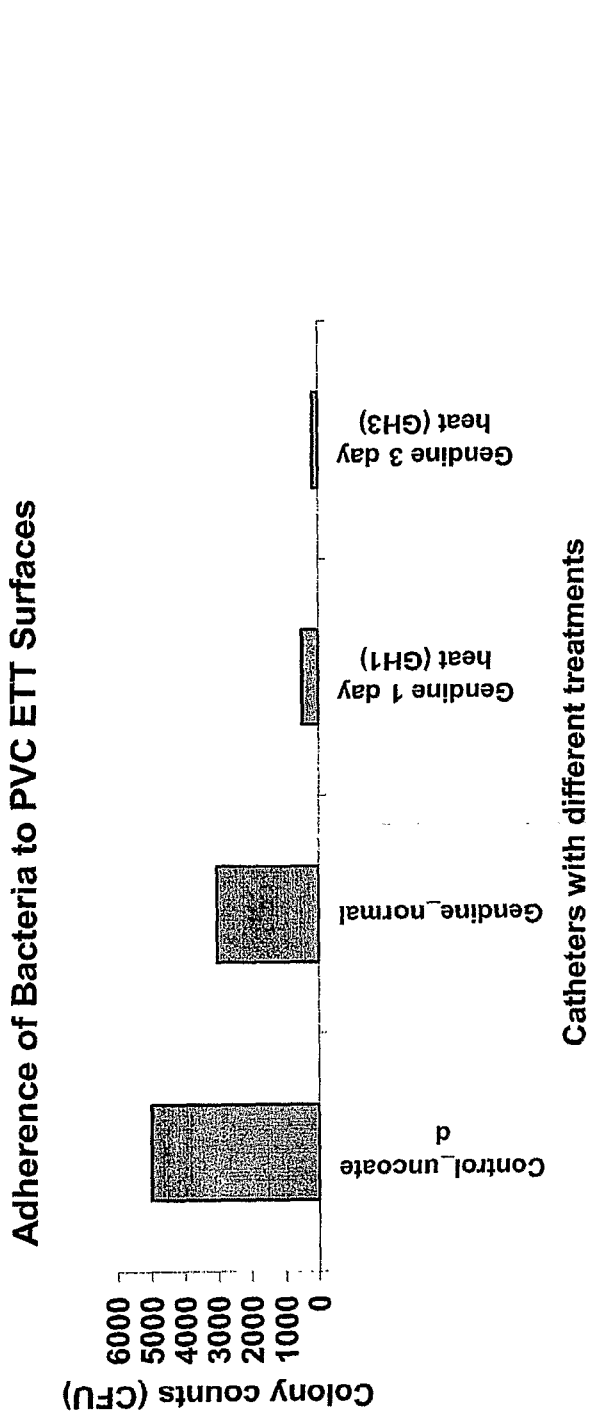

*P* < 0.0001 for comparing GH1, GH3 vs Control uncoated PVC ETT, respectively (Wilcoxon rank sum test)  
*P* < 0.001 for comparing GH1, GH3 vs Gendine normal PVC ETT, respectively (Wilcoxon rank sum test)

**FIG. 2**



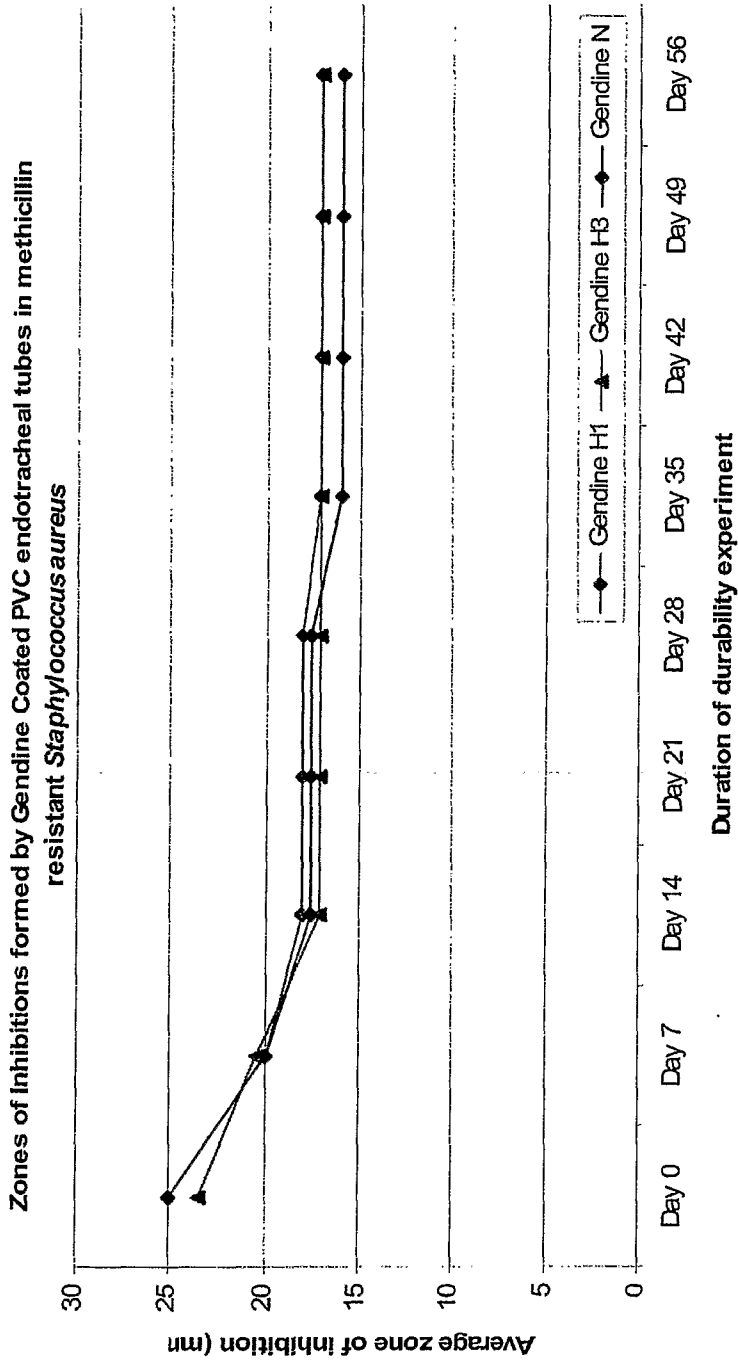


FIG. 3

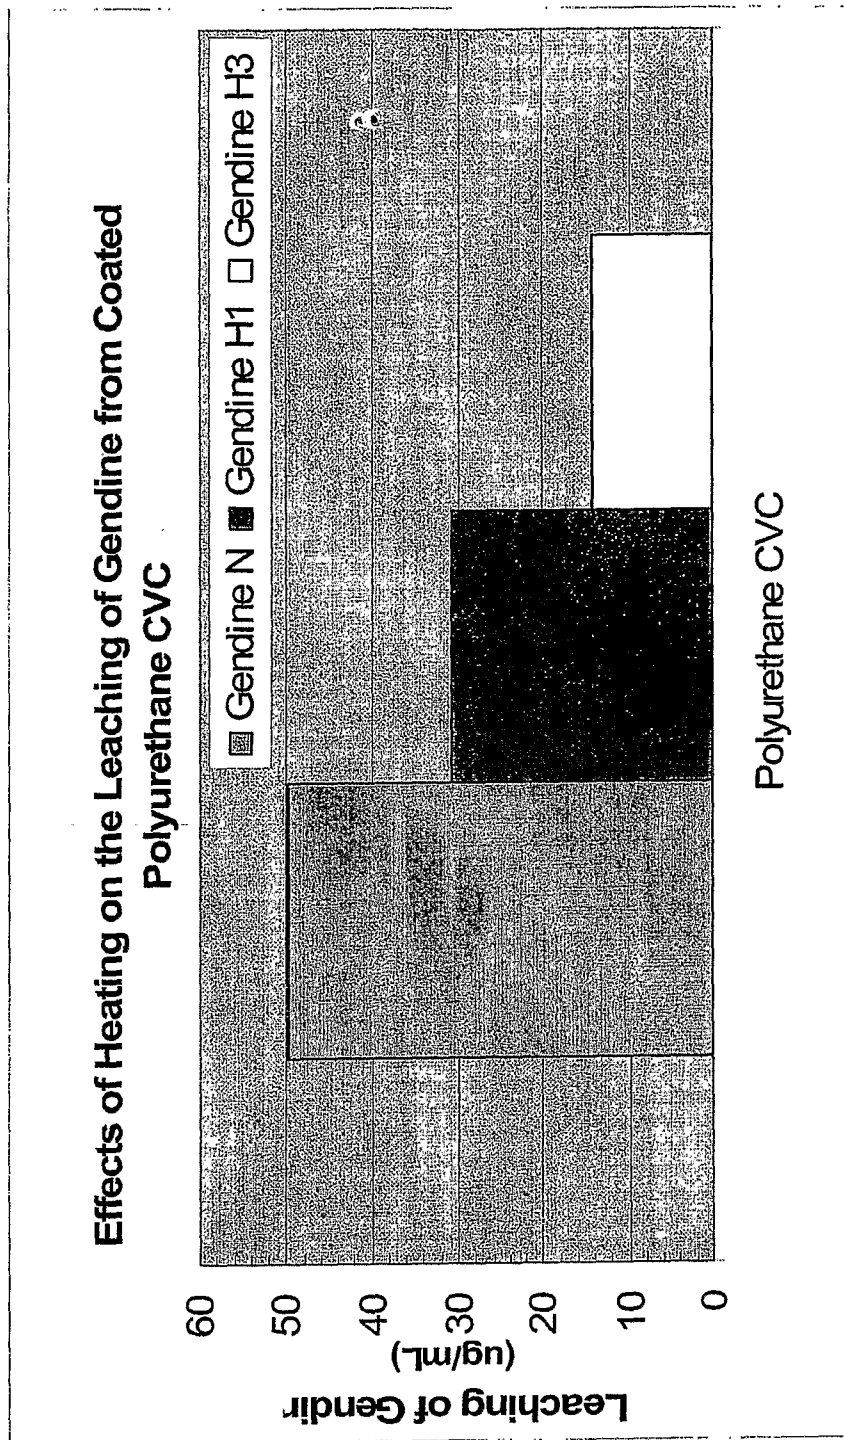

**FIG. 4**

Adherence of Bacteria to Polyurethane CVC Surfaces

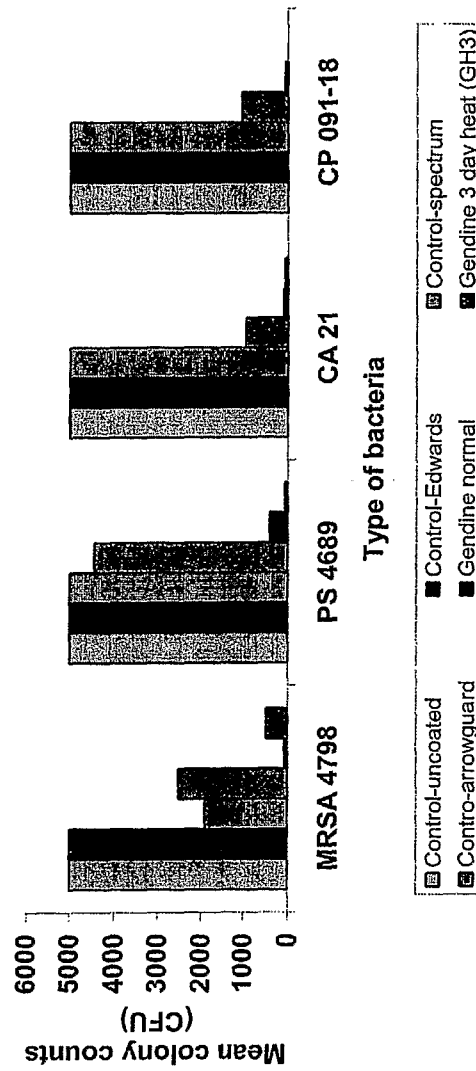

$P < 0.04$  for comparing GH3 vs all control CVC for MRSA & PS (Wilcoxon rank sum test)  
 $P < 0.02$  for comparing GH3 vs Control uncoated, Spectrum & Edwards CVC for *C. albicans* and *C. parapsilosis* Wilcoxon rank sum test)

FIG. 5

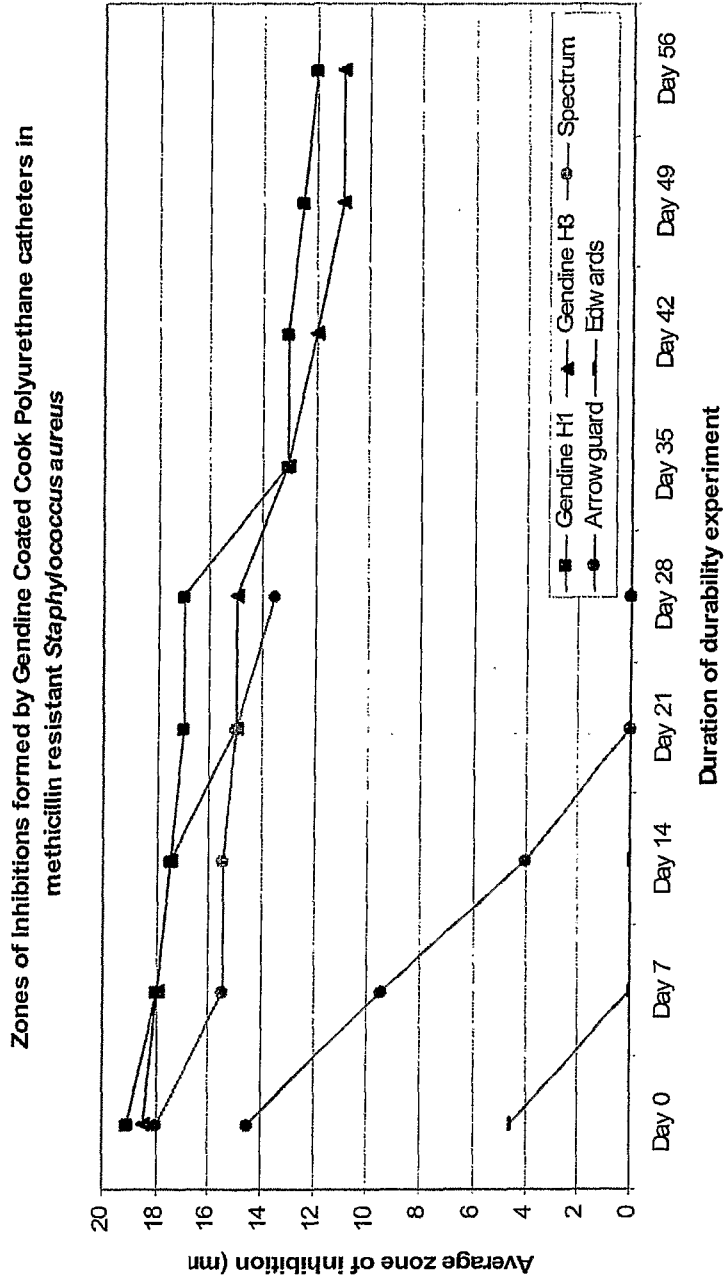


FIG. 6



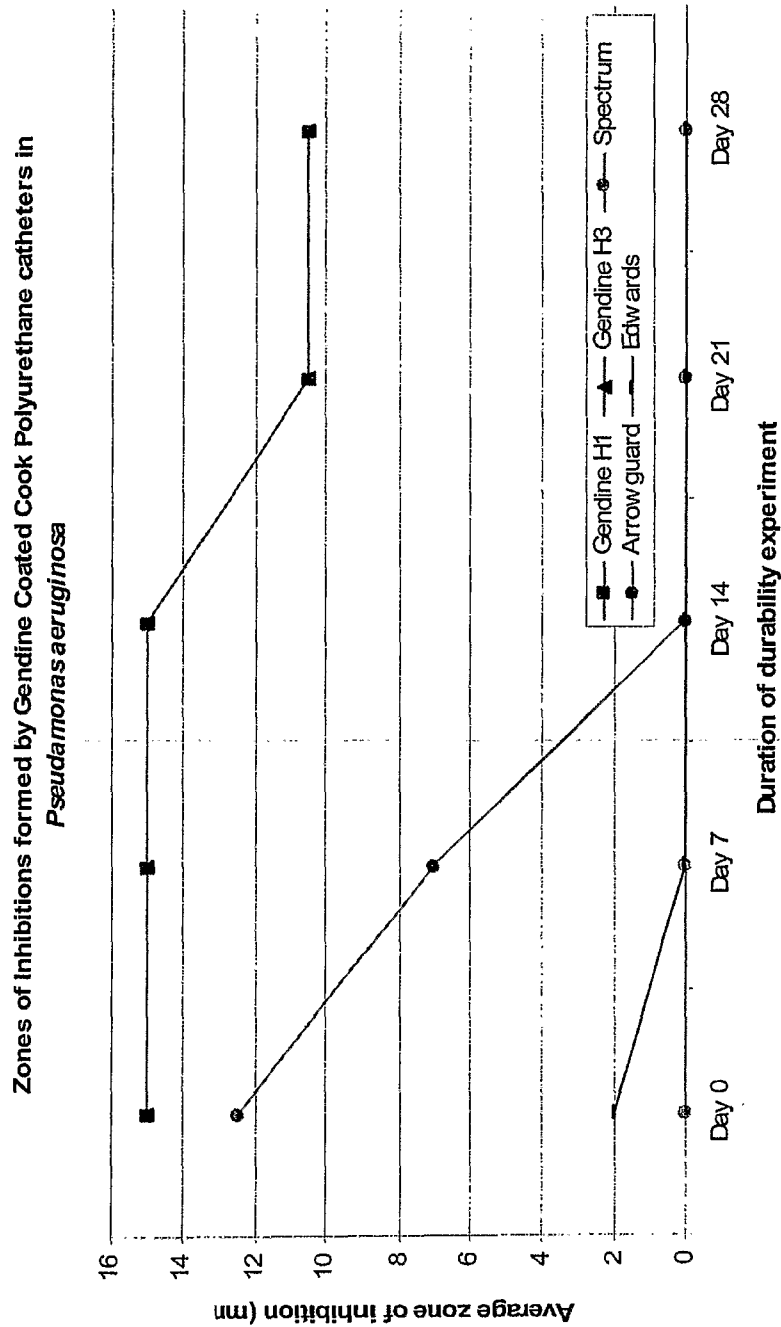


FIG. 7

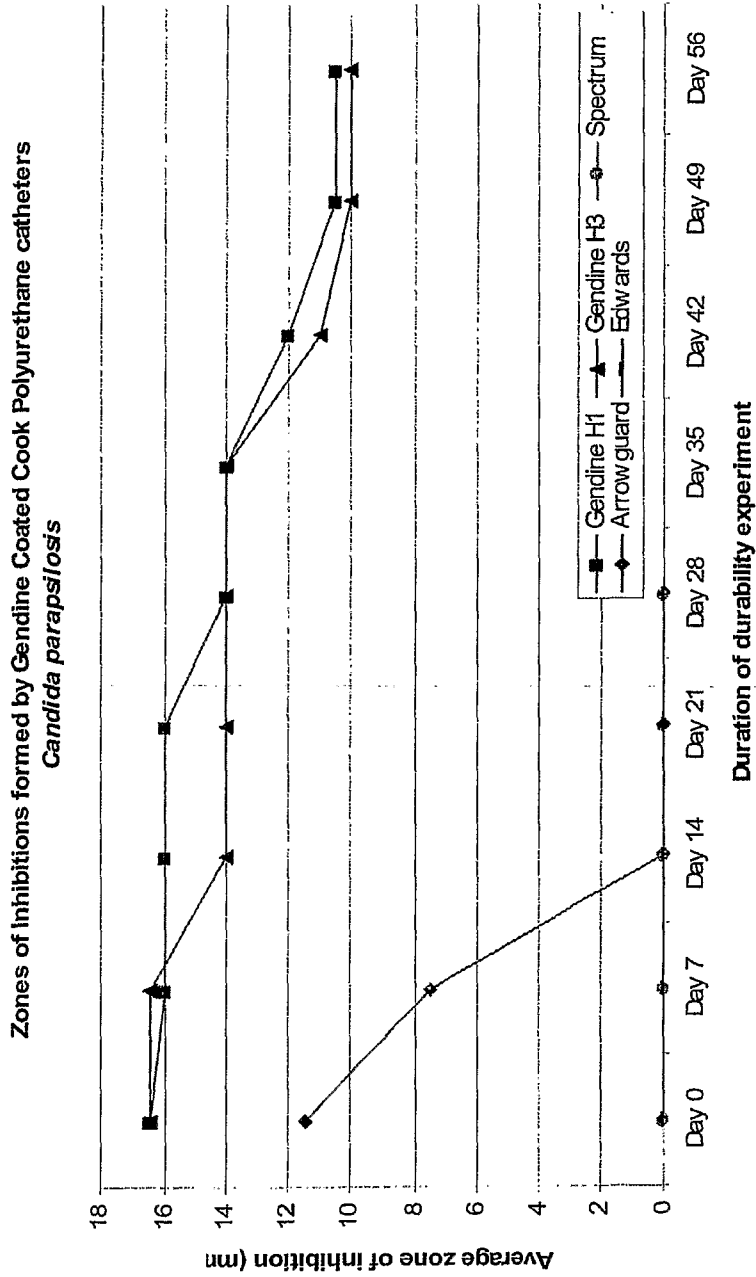


FIG. 8


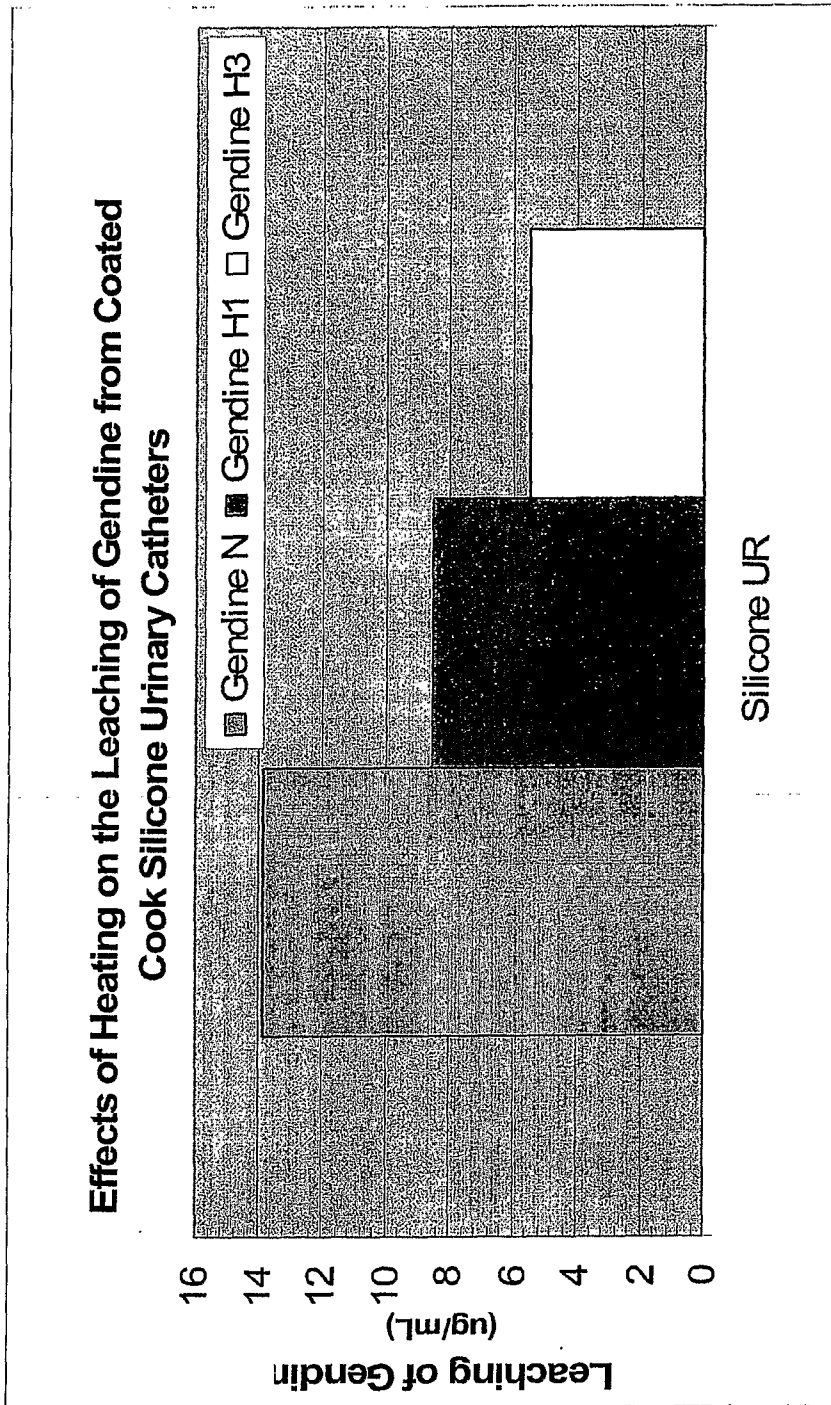


FIG. 9

**Adherence of Bacteria to Silicone Urinary Catheter Surfaces**

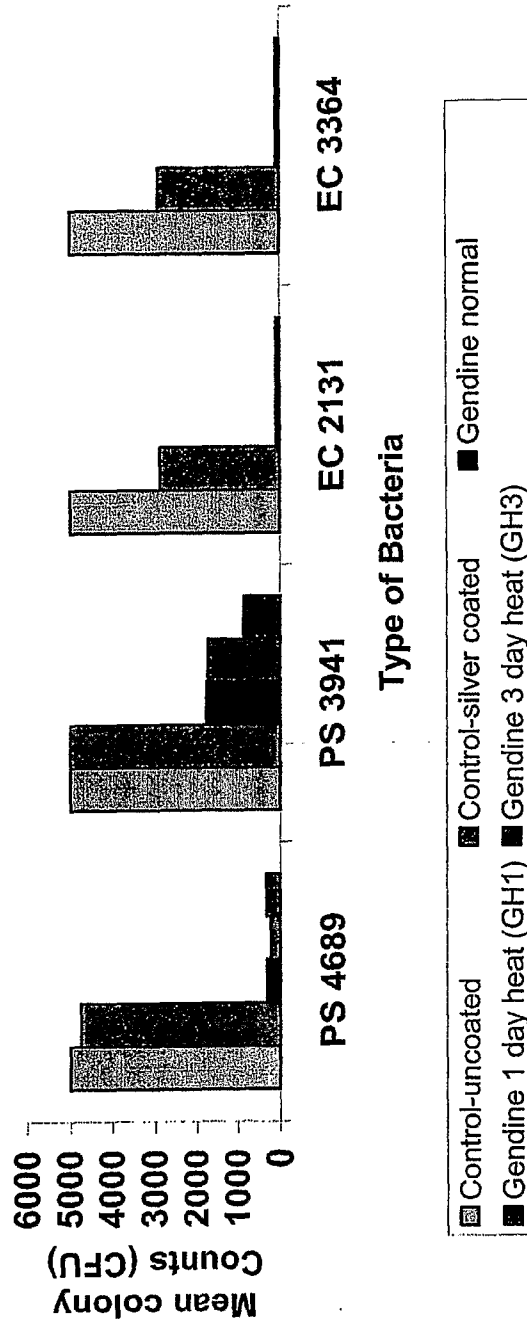

**P < 0.03 for comparing GH3 vs Control uncoated & silver coated UC, respectively (Wilcoxon rank sum test)**

**FIG. 10**

Zones of Inhibitions formed by Gendine Coated Cook Silicone Urinary Catheters  
in vancomycin resistant *Enterococcus* (VRE)

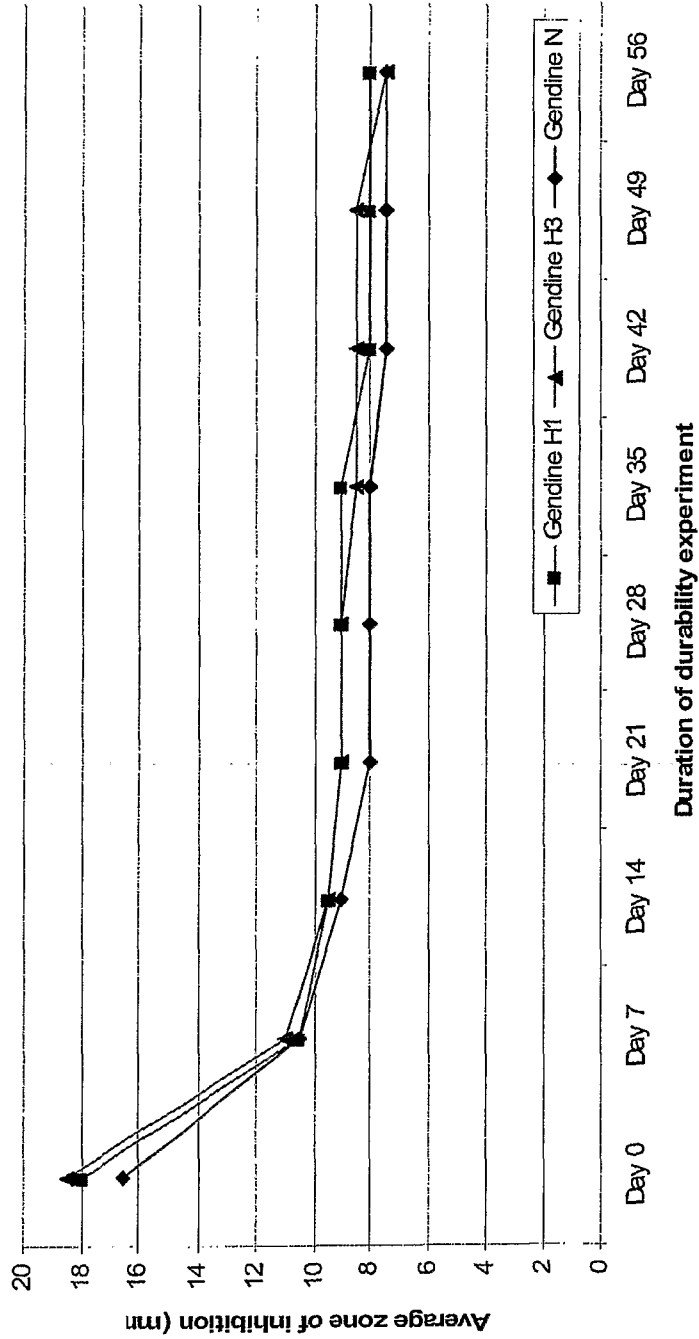


FIG. 11

Zones of Inhibitions formed by Gendine Coated Cook Silicone Urinary Catheters  
in *E. coli*

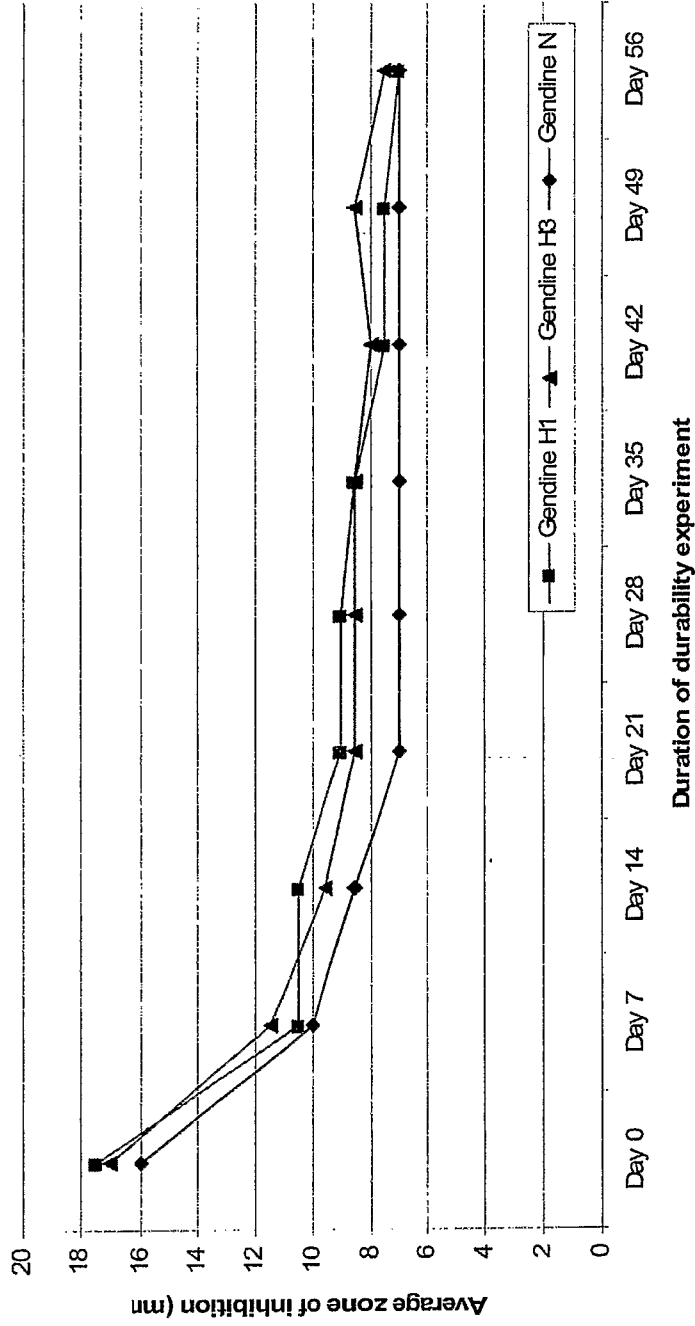


FIG. 12



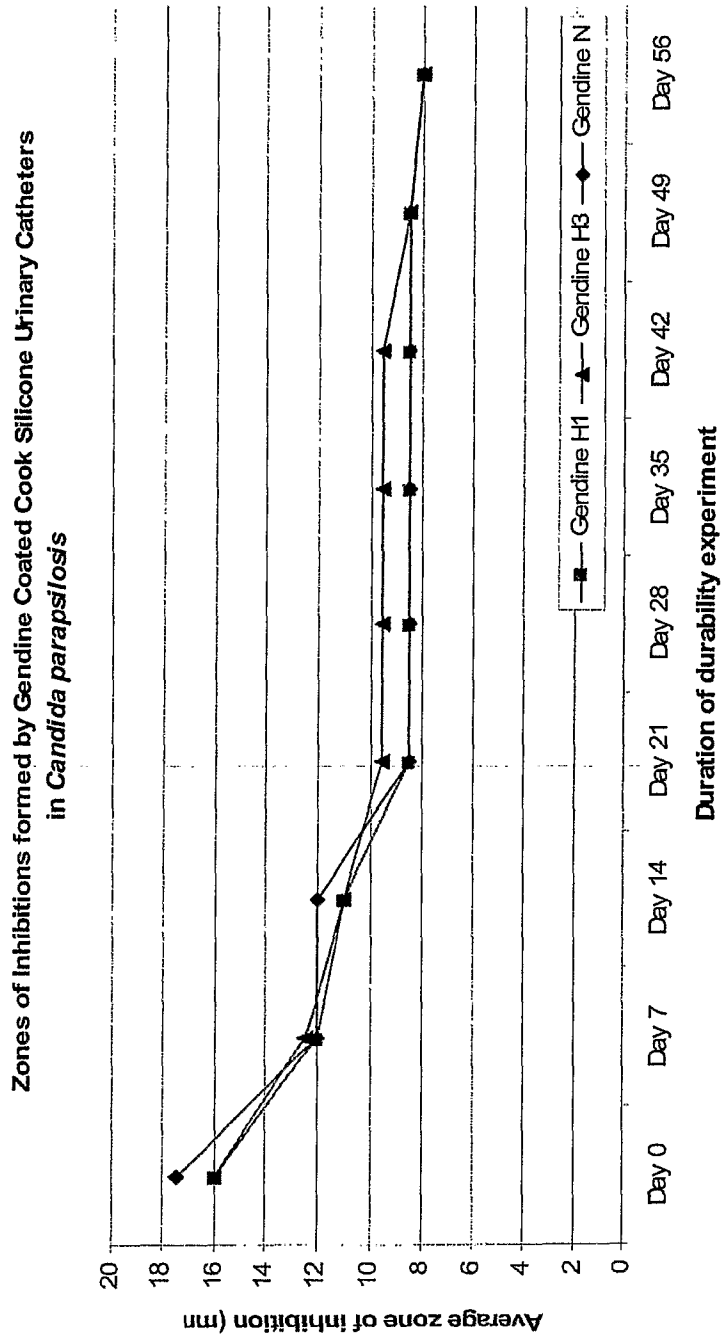


FIG. 13




**FIG. 14**

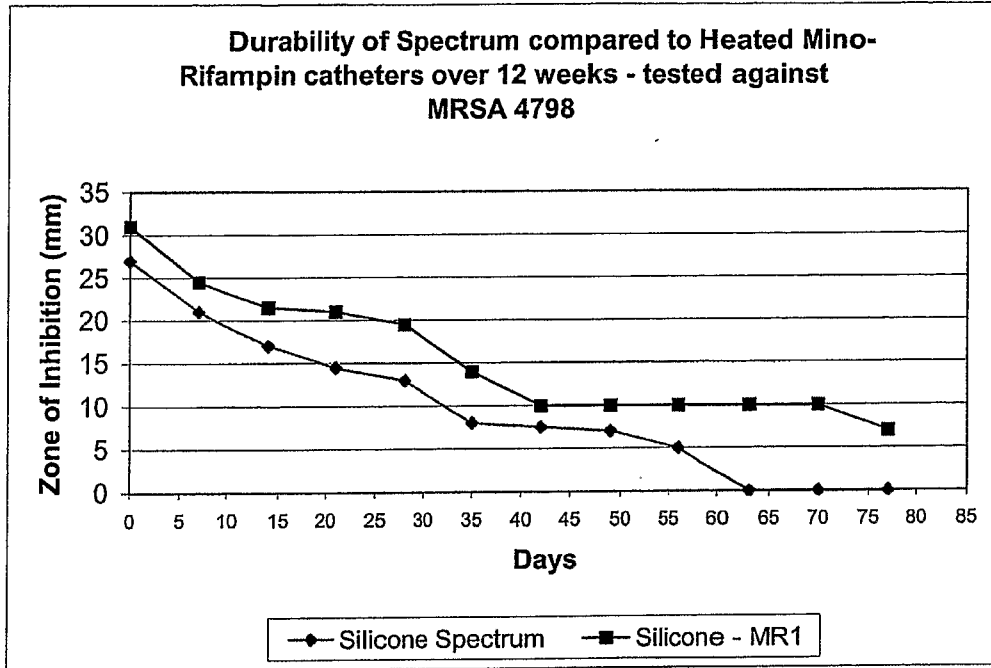


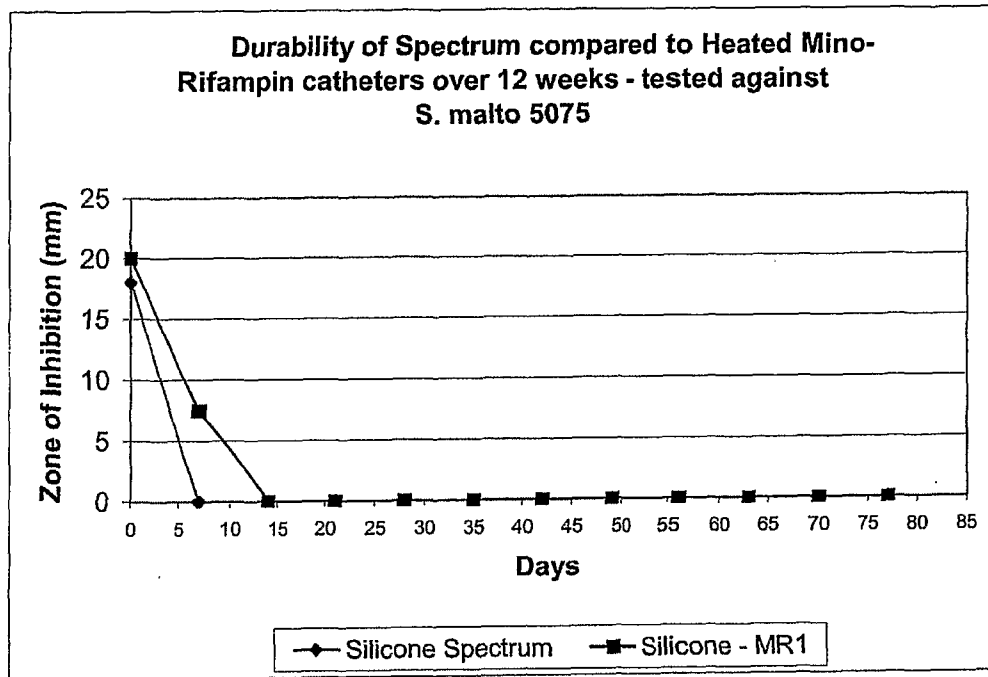

**FIG. 15**

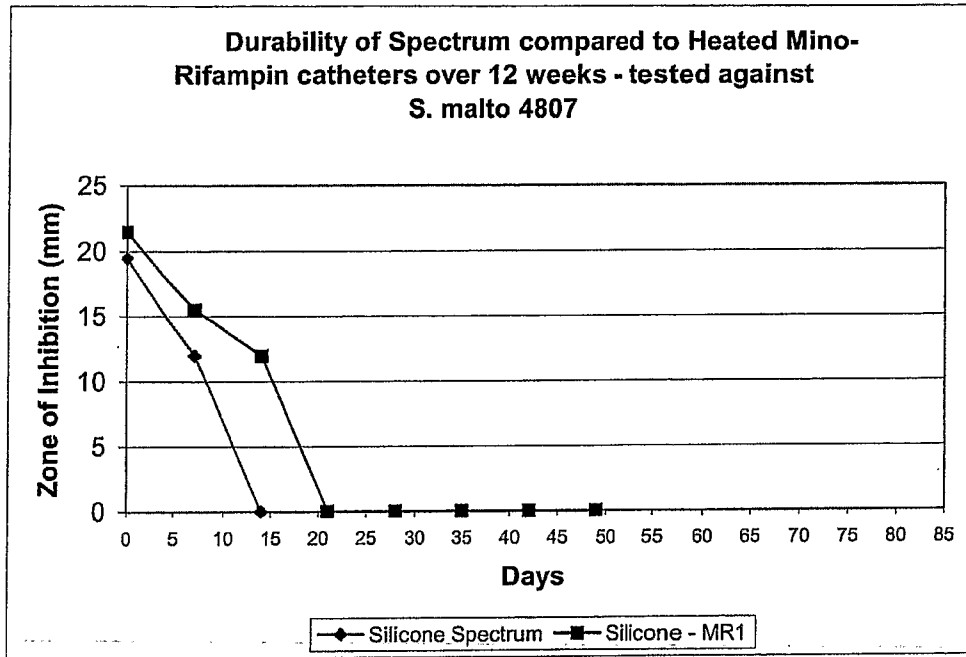

**FIG. 16**

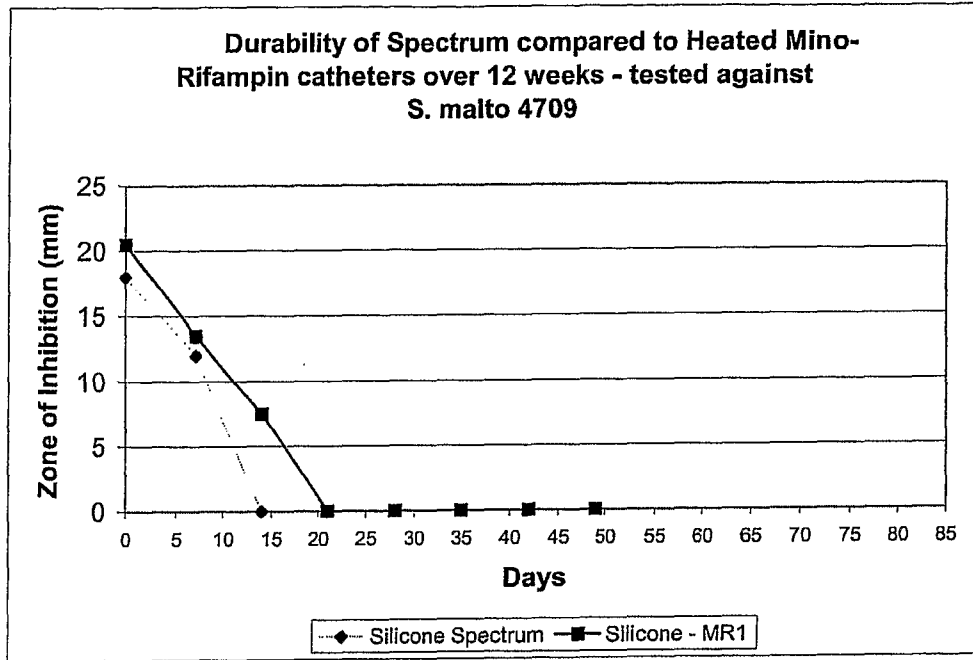

**FIG. 17**

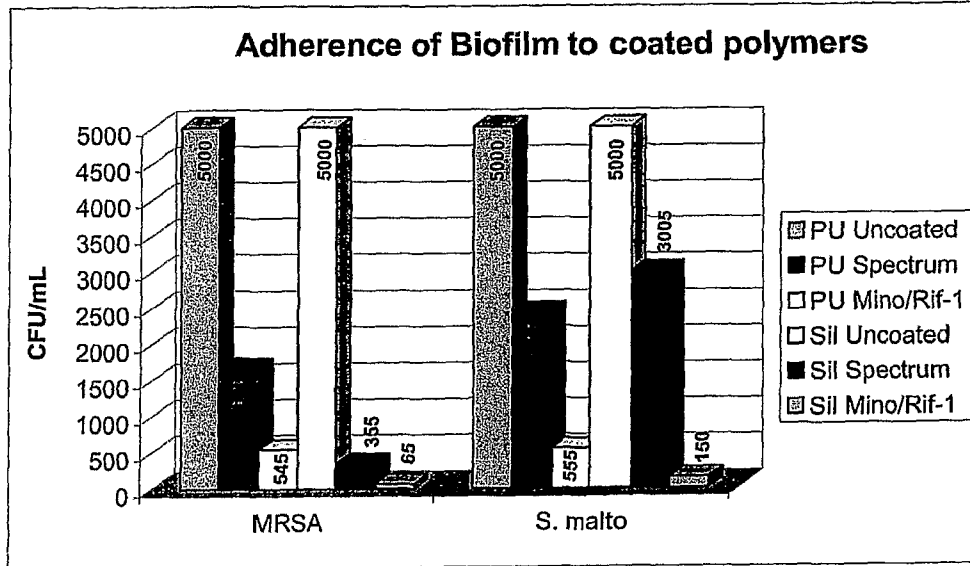


FIG. 18