



US00D586466S

(12) **United States Design Patent**
Smith et al.

(10) **Patent No.:** **US D586,466 S**

(45) **Date of Patent:** **** Feb. 10, 2009**

(54) **BLOOD GLUCOSE METER**

(75) Inventors: **Robert J. Smith**, Louisville, CO (US);
Thomas Aidan Stamp, Ashburton (AU);
Daniel D. Bouricius, Boulder, CO (US);
Eric Lancaster, Longmont, CO (US)

(73) Assignee: **Lifescan, Inc.**, Milpitas, CA (US)

(**) Term: **14 Years**

(21) Appl. No.: **29/319,326**

(22) Filed: **Jun. 6, 2008**

(51) **LOC (9) Cl.** **24-01**

(52) **U.S. Cl.** **D24/186**

(58) **Field of Classification Search** D10/78,
D10/81; D24/169, 183-187, 216-234; 422/68.1,
422/63, 65, 99, 56, 58, 61, 67, 102, 104;
436/180, 43, 46, 50, 55; 600/309, 318, 322,
600/368, 583; 204/403.03, 406, 407
See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

D406,895 S * 3/1999 Byrd et al. D24/169
D428,654 S * 7/2000 Schlesinger et al. D24/169
D484,600 S * 12/2003 Kaar et al. D24/169

D495,800 S * 9/2004 Kaar et al. D24/169
D499,805 S * 12/2004 D'Agostino D24/169
D546,456 S * 7/2007 May D24/186
D546,457 S * 7/2007 Hannant et al. D24/186
D546,458 S * 7/2007 Hannant D24/186
D557,422 S * 12/2007 Arbogast et al. D24/186

* cited by examiner

Primary Examiner—Robert A. Delehanty
Assistant Examiner—Mark Cavanna


(57) **CLAIM**

The ornamental design for a blood glucose meter, as shown and described.

DESCRIPTION

FIG. 1 is a perspective view, as seen from the top, front and left side of the blood glucose meter, showing our new design; FIG. 2 is a top plain view thereof; FIG. 3 is a rear elevational view thereof; FIG. 4 is a front elevational view thereof; FIG. 5 is a bottom plain view thereof. FIG. 6 is a right side elevational view thereof; and, FIG. 7 is a left side elevational view thereof.

1 Claim, 4 Drawing Sheets

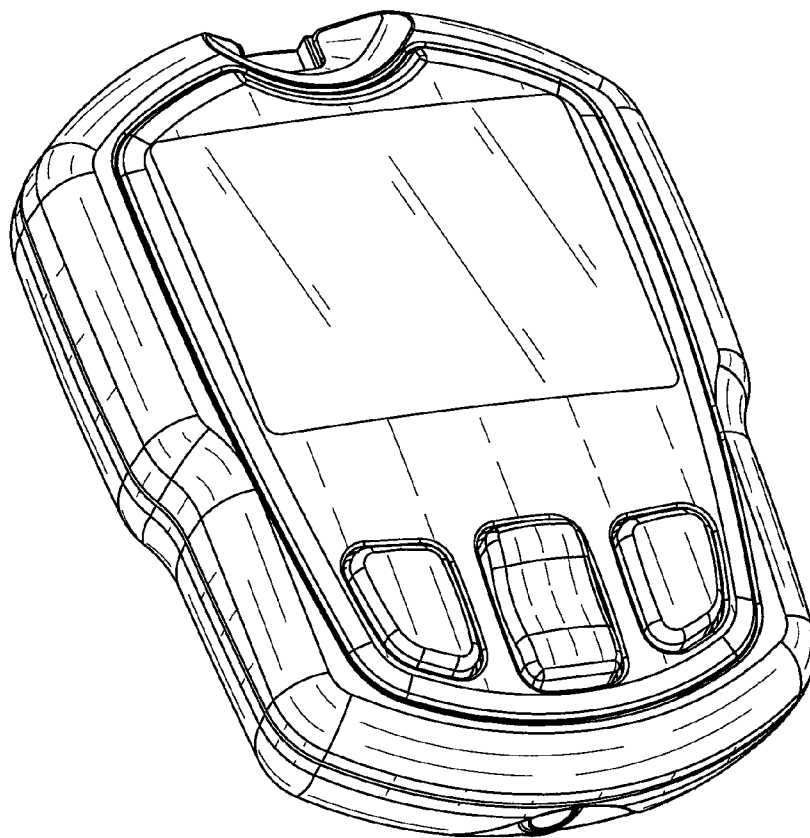

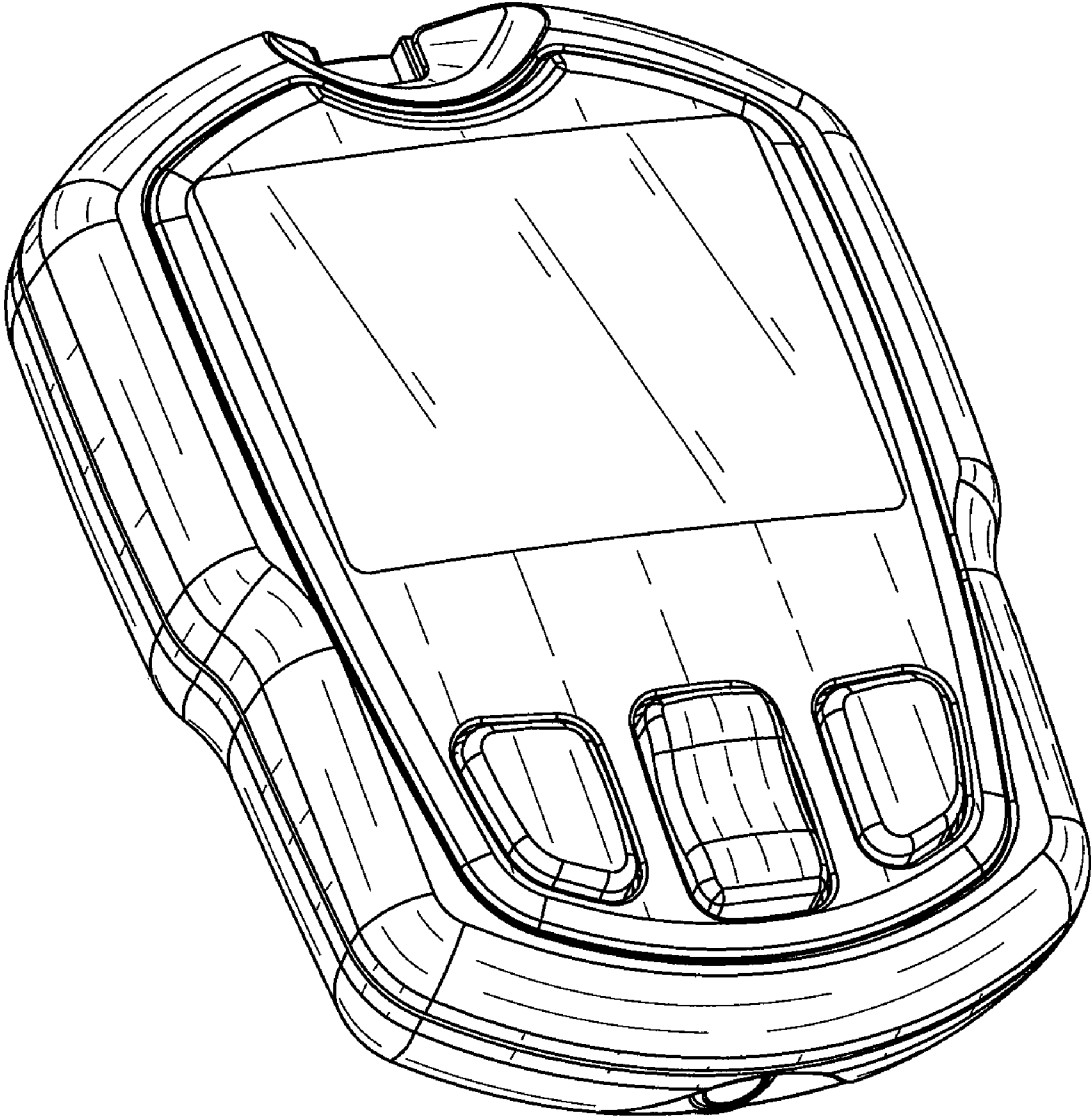


FIG. 1

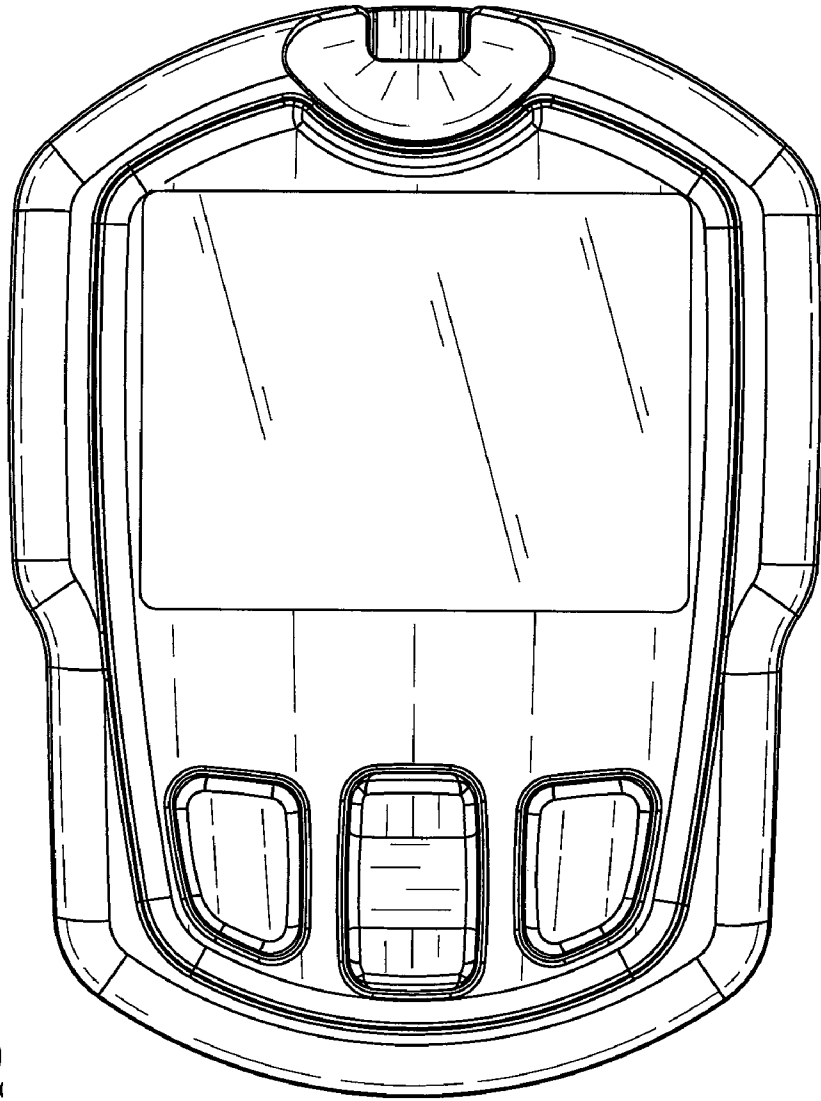


FIG. 2

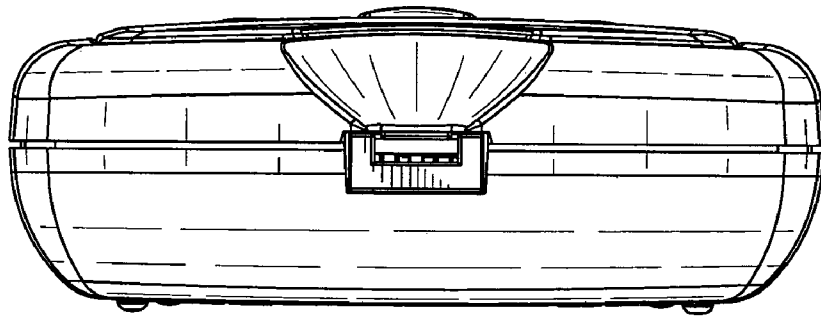


FIG. 3

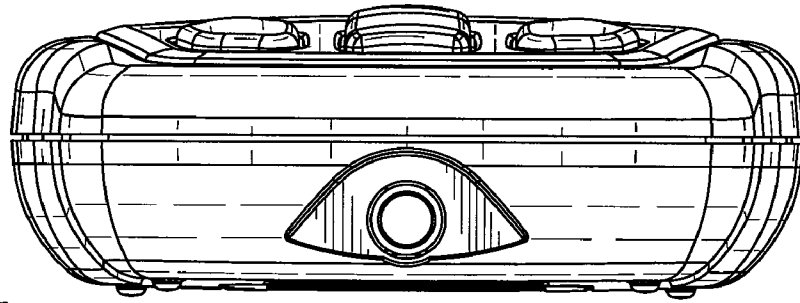


FIG. 4

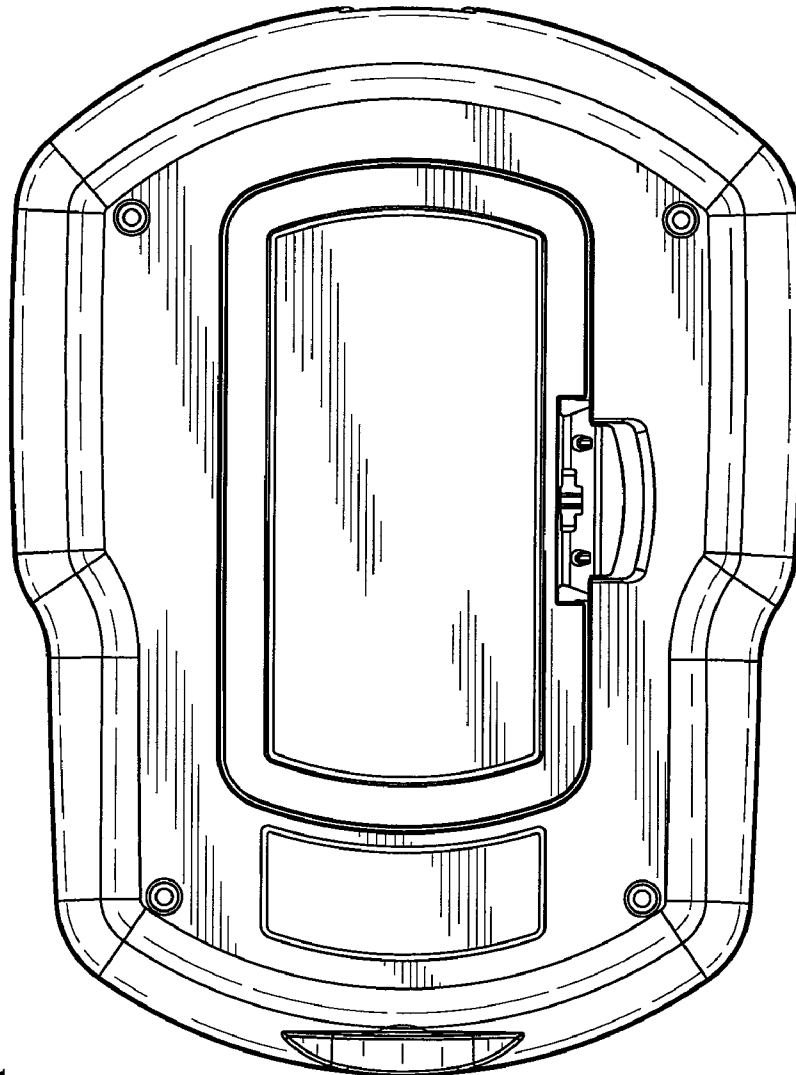


FIG. 5

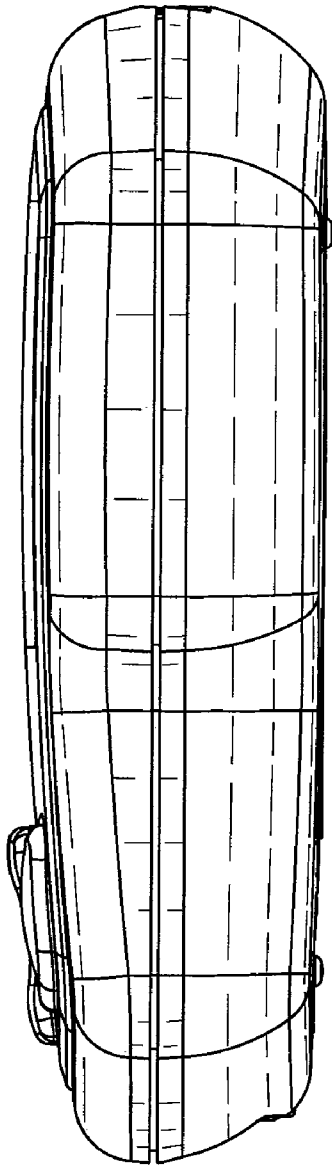


FIG. 6

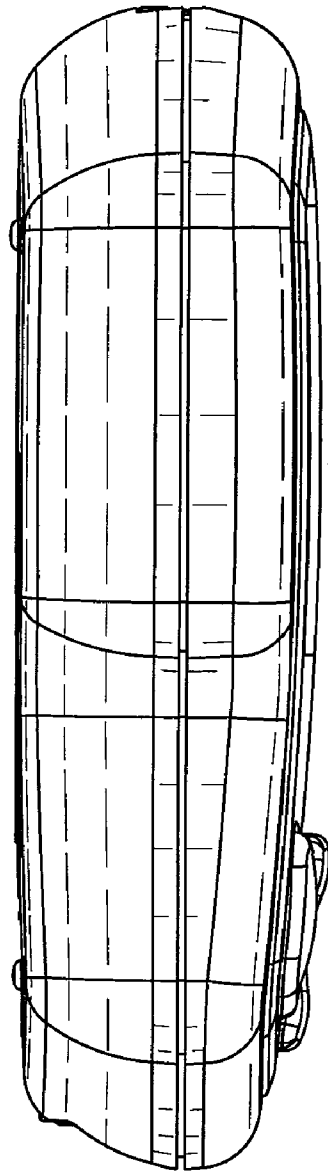


FIG. 7